

Data Path : Z:\HPCHEM1\BNA E\DATA\BE013118\
 Data File : BE095343.D
 Acq On : 1 Feb 2018 6:42
 Operator : SJ/JU
 Sample : J1245-12
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 F6B73

Quant Time: Feb 01 08:04:12 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Feb 01 06:27:03 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.44	152	2236	0.40	ng/ul	0.00
2) Naphthalene-d8	11.26	136	7014	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.02	164	4590	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.71
16) Chrysene-d12	21.80	240	9065	0.40	ng/ul	0.00
20) Perylene-d12	24.27	264	528238	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	3939	0.34	ng/ul	0.00
14) Fluoranthene-d10	19.70	212	10144	0.00	ng/ul	0.00
Target Compounds						
17) Pyrene	20.05	202	1645	0.054	ng/ul#	Ovalue 1




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE013118\
Data File : BE095343.D
Acq On : 1 Feb 2018 6:42
Operator : SJ/JU
Sample : J1245-12
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F6B73

Quant Time: Feb 01 08:04:12 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 01 06:27:03 2018
Response via : Initial Calibration

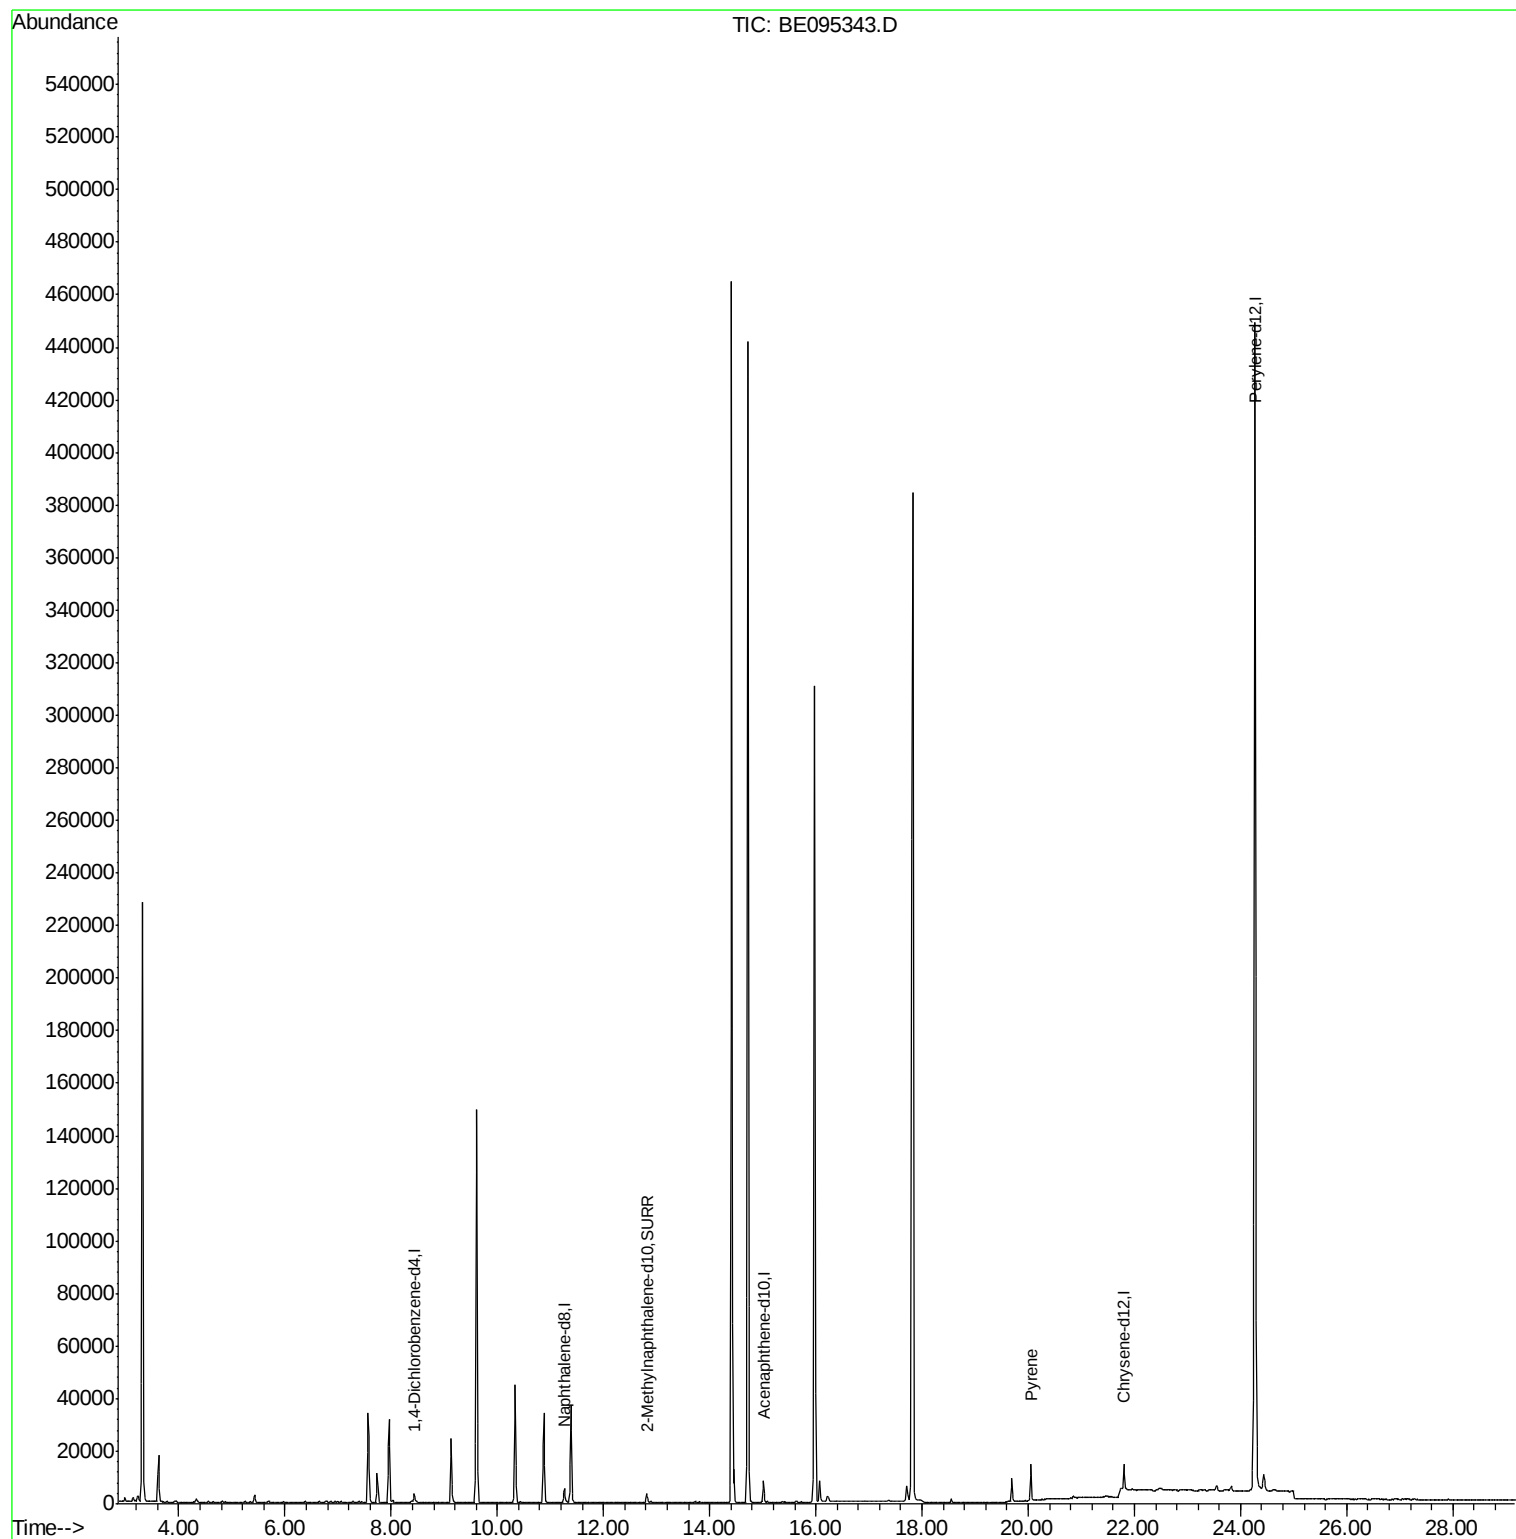

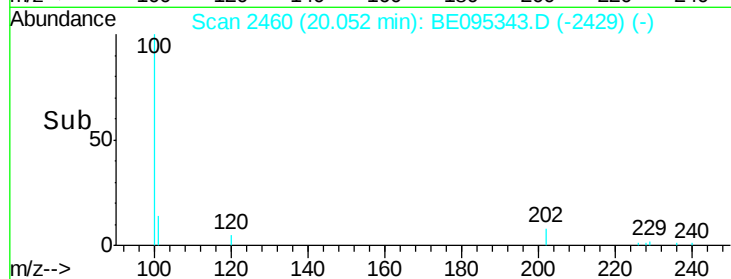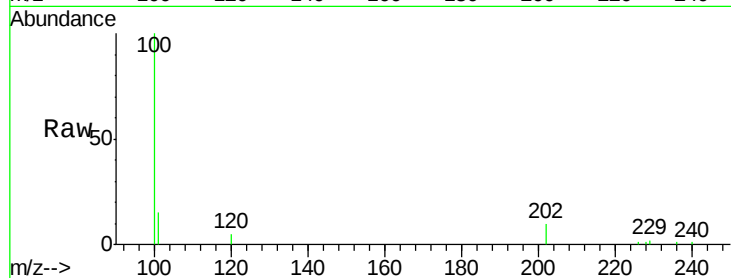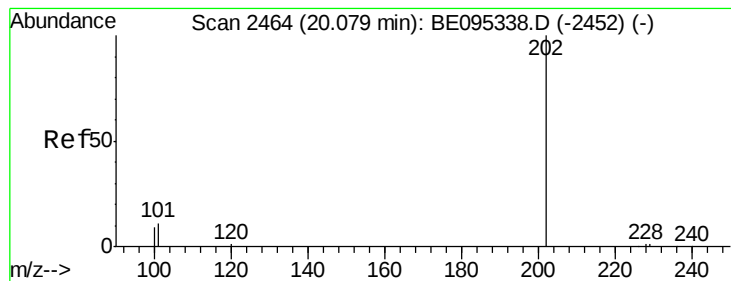

#17

Pvrene

Concen: 0.054 ng/ul

RT: 20.05 min Scan# 2460

Delta R.T. -0.03 min

Lab File: BE095343.D

Acq: 1 Feb 2018 6:42

Instrument :

BNA_E

ClientSampleId :

F6B73

Tot Ion:202 Resp: 1645

Ion Ratio Lower Upper

202 100

101 152.0 18.2 27.4#

100 1041.6 15.6 23.4#

