

Data Path : Z:\HPCHEM1\BNA E\DATA\BE013118\

Data File : BE095323.D

Acq On : 31 Jan 2018 18:45

Operator : SJ/JU

Sample : J1233-07DL 5X

Misc :

ALS Vial : 3 Sample Multiplier: 1

Quant Time: Feb 01 04:06:00 2018

Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Thu Feb 01 04:05:22 2018

Response via : Initial Calibration

Instrument :

BNA_E

ClientSampleId :




F6B11DL

Manual Integrations

APPROVED

Sohil

2/1/2018 5:58:22 PM

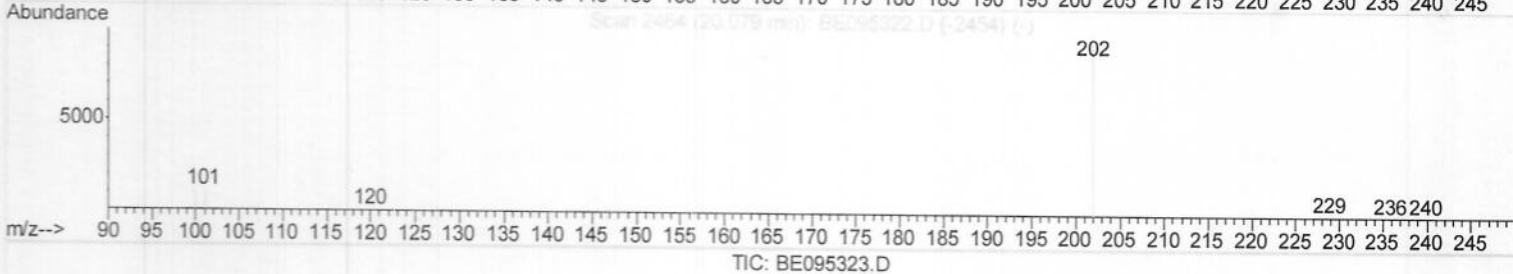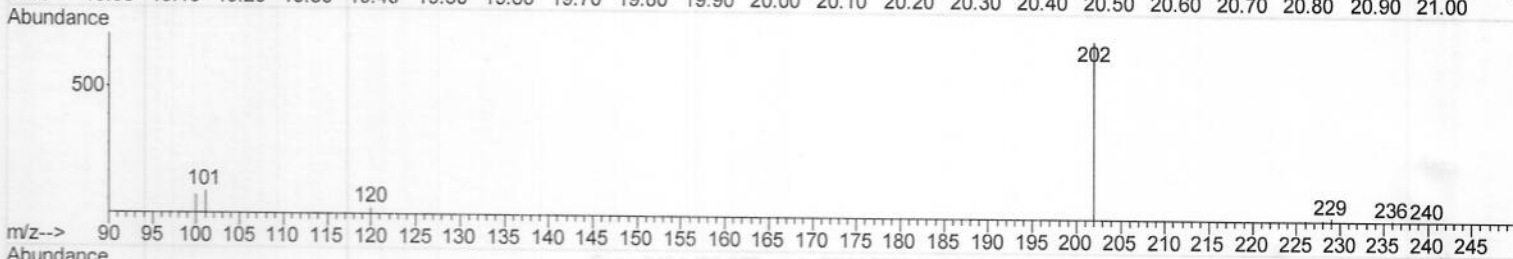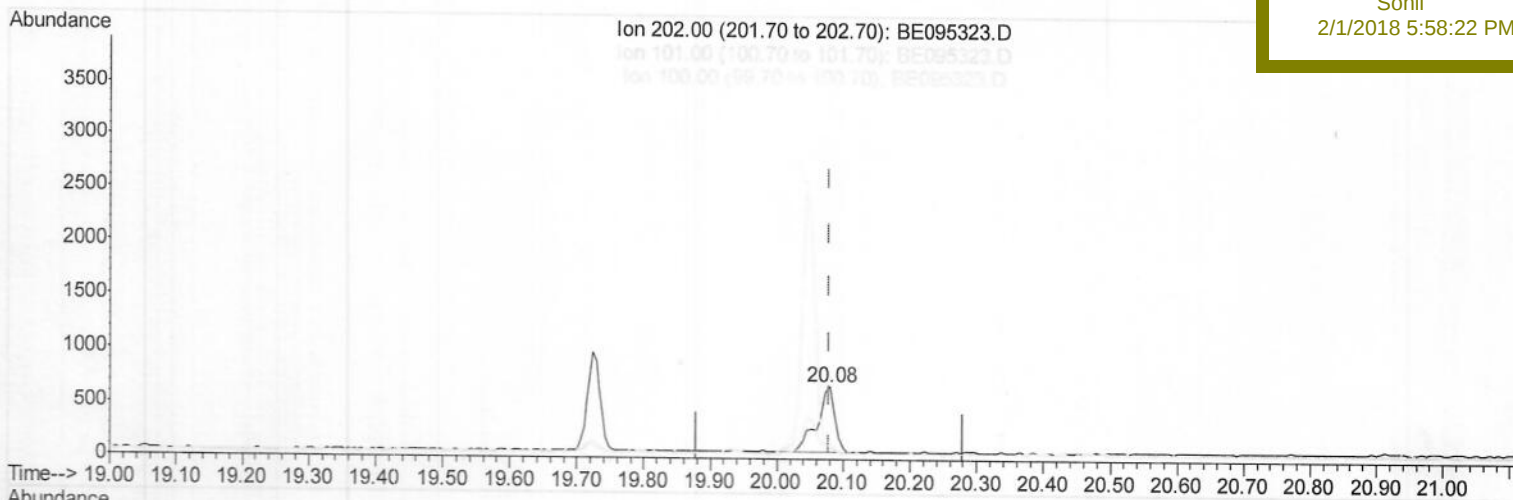

(17) Pyrene

20.079min (-0.000) 0.05ng/ul

response 1393

Ion	Exp%	Act%
202.00	100	100
101.00	22.80	19.27
100.00	19.50	17.08
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE013118\

Data File : BE095323.D

Acq On : 31 Jan 2018 18:45

Operator : SJ/JU

Sample : J1233-07DL 5X

Misc :

ALS Vial : 3 Sample Multiplier: 1

Quant Time: Feb 01 04:06:00 2018

Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Thu Feb 01 04:05:22 2018

Response via : Initial Calibration

Instrument :

BNA_E




ClientSampleId :

F6B11DL

Manual Integrations
APPROVED

Sohil

2/1/2018 5:58:22 PM

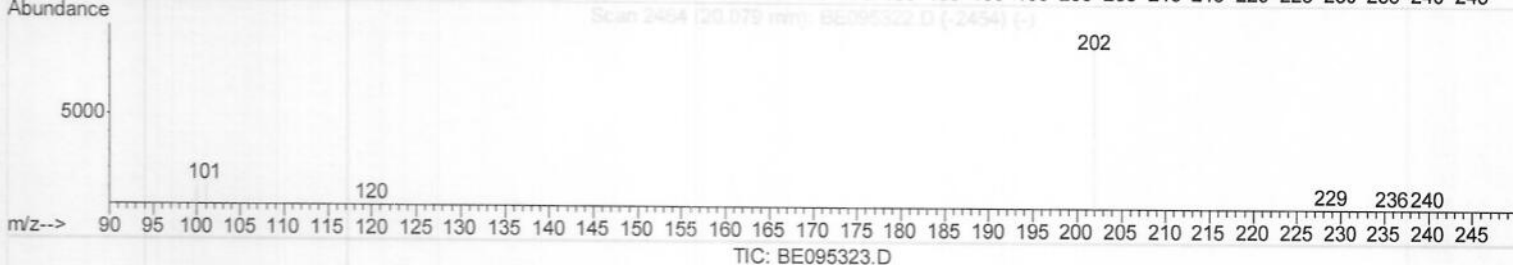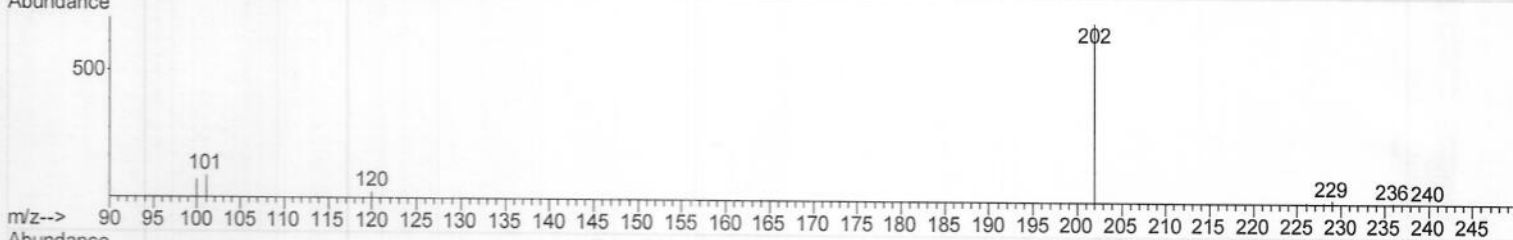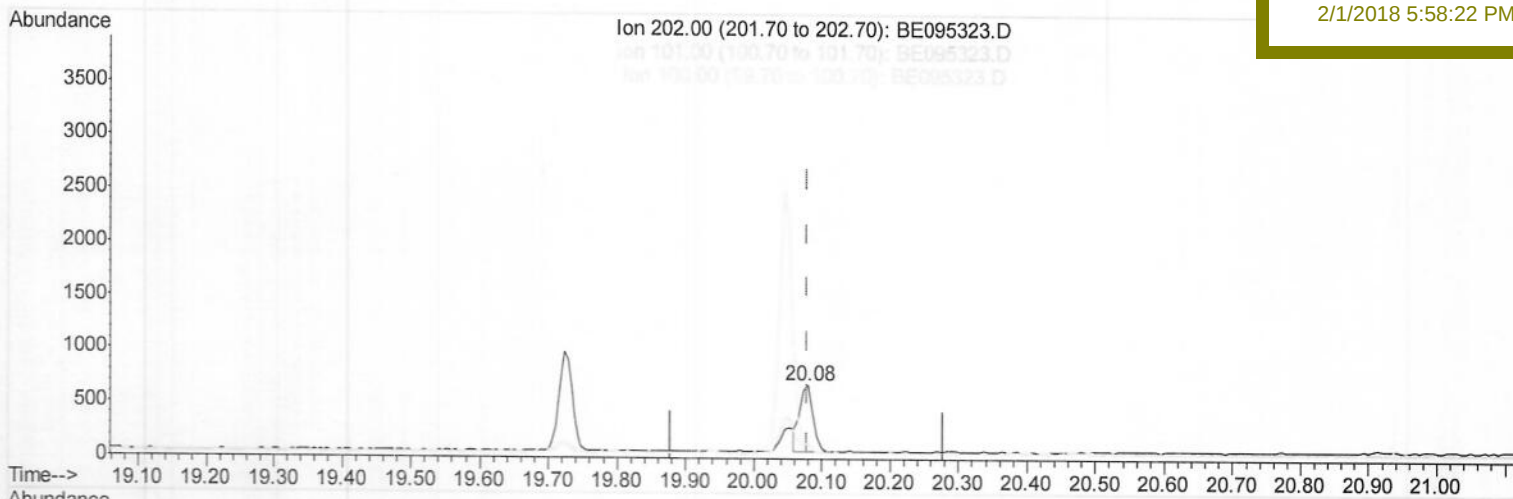

(17) Pyrene

20.079min (-0.000) 0.03ng/ul m >Jy 02/08/18

response 833

Ion	Exp%	Act%
202.00	100	100
101.00	22.80	19.27
100.00	19.50	17.08
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE013118\

Data File : BE095323.D

Acq On : 31 Jan 2018 18:45

Operator : SJ/JU

Sample : J1233-07DL 5X

Misc :

ALS Vial : 3 Sample Multiplier: 1

Quant Time: Feb 01 04:10:15 2018

Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Thu Feb 01 04:05:22 2018

Response via : Initial Calibration

Instrument :

BNA_E

ClientSampleId :

F6B11DL

Manual Integrations

APPROVED

Sohil

2/1/2018 5:58:22 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.44	152	2209	0.40	ng/ul	0.00
2) Naphthalene-d8	11.26	136	6775	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.01	164	4097	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	8250	0.40	ng/ul	0.00
16) Chrysene-d12	21.80	240	8875	0.40	ng/ul	0.00
20) Perylene-d12	24.44	264	9054	0.40	ng/ul	0.00

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	12.81	152	1305	0.12	ng/ul	0.00
14) Fluoranthene-d10	19.70	212	3192	0.10	ng/ul	0.00

Target Compounds

	R.T.	QIon	Response	Conc	Units	Ovalue
3) Naphthalene	11.31	128	4915	0.259	ng/ul#	90
5) 2-Methylnaphthalene	12.89	142	6549	0.517	ng/ul	100
8) Acenaphthene	15.07	153	912	0.060	ng/ul#	90
9) Fluorene	16.02	166	540	0.034	ng/ul#	74
11) Pentachlorophenol	17.36	266	3241	2.028	ng/ul	97
12) Phenanthrene	17.75	178	1811	0.065	ng/ul#	91
15) Fluoranthene	19.72	202	1201	0.033	ng/ul	85
17) Pyrene	20.08	202	833m)	0.028	ng/ul	

) 2402/08/18

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE013118\
Data File : BE095323.D
Acq On : 31 Jan 2018 18:45
Operator : SJ/JU
Sample : J1233-07DL 5X
Misc :
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Feb 01 04:10:15 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 01 04:05:22 2018
Response via : Initial Calibration

Instrument :
BNA_E
ClientSampleId :
F6B11DL

Manual Integrations
APPROVED

Sohil
2/1/2018 5:58:22 PM

