

Data Path : Z:\HPCHEM1\BNA E\DATA\BE013118\
Data File : BE095325.D
Acq On : 31 Jan 2018 19:57
Operator : SJ/JU
Sample : PB106079BL
Misc :
ALS Vial : 5 Sample Multiplier: 1




Instrument :
BNA_E
ClientSampleId :
SBLK79

Manual Integrations
APPROVED

Quant Time: Feb 01 04:06:16 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 01 04:05:22 2018
Response via : Initial Calibration

Sohil

2/1/2018 5:58:27 PM

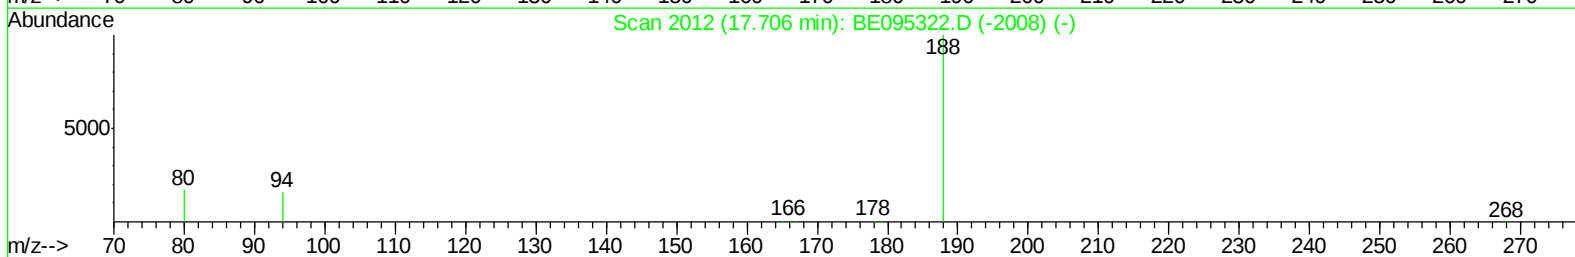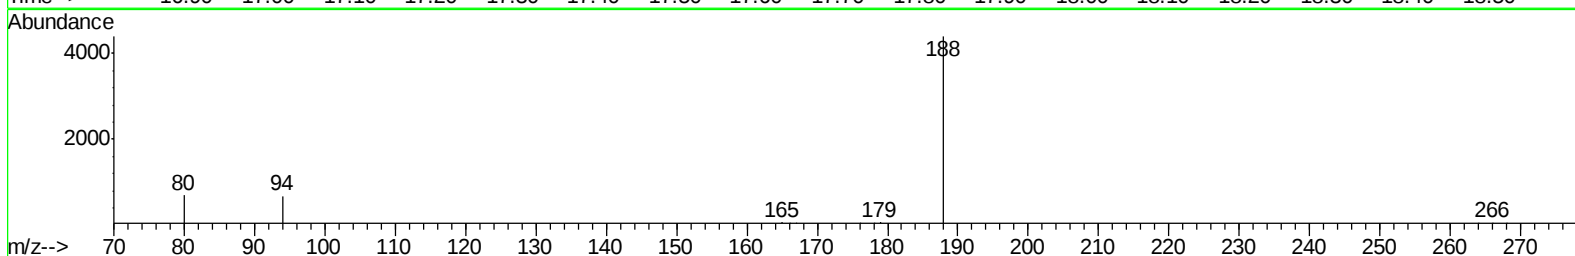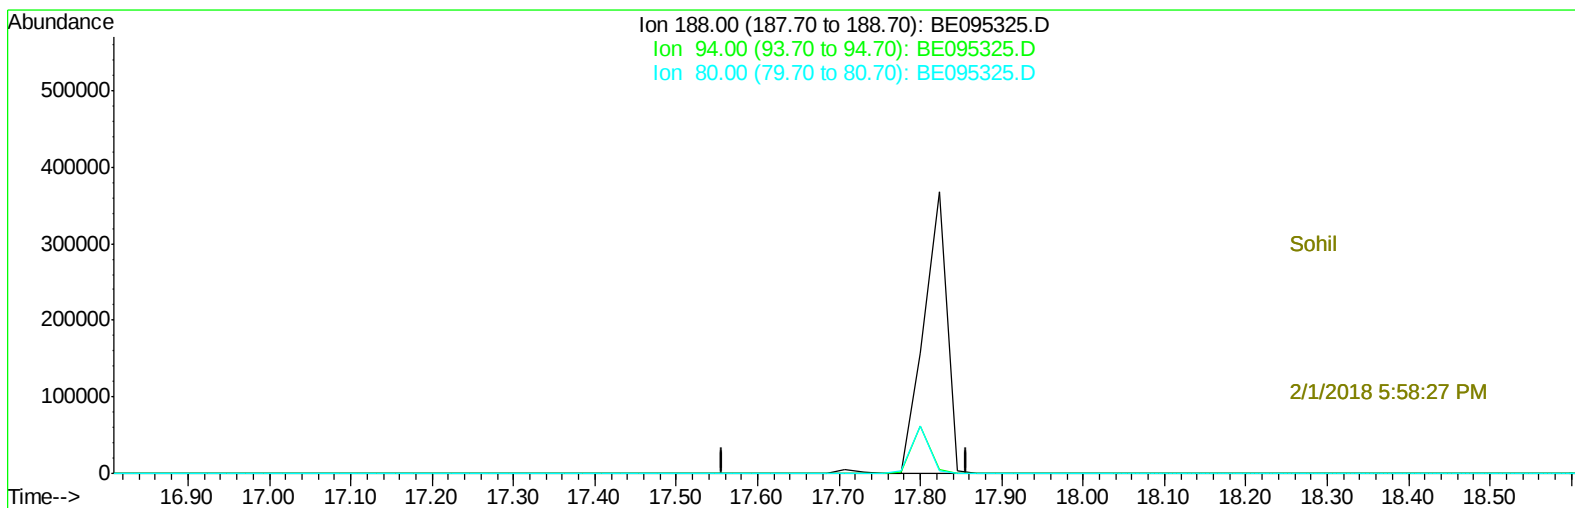

TIC: BE095325.D

(10) Phenanthrene-d10 (I)

17.706min (-17.706) 0.00ng/ul

response 0




Ion	Exp%	Act%
188.00	100	0.00
94.00	11.00	0.00#
80.00	11.80	0.00#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE013118\
Data File : BE095325.D
Acq On : 31 Jan 2018 19:57
Operator : SJ/JU
Sample : PB106079BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK79

Manual Integrations
APPROVED

Quant Time: Feb 01 04:06:16 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 01 04:05:22 2018
Response via : Initial Calibration

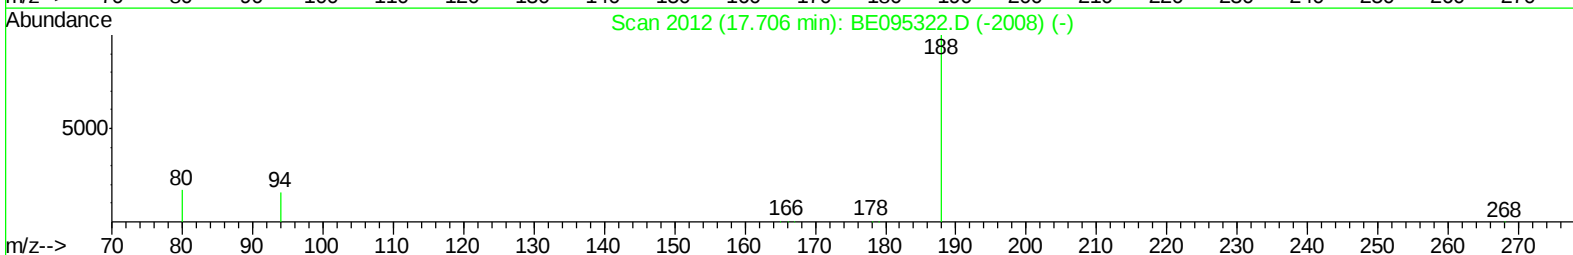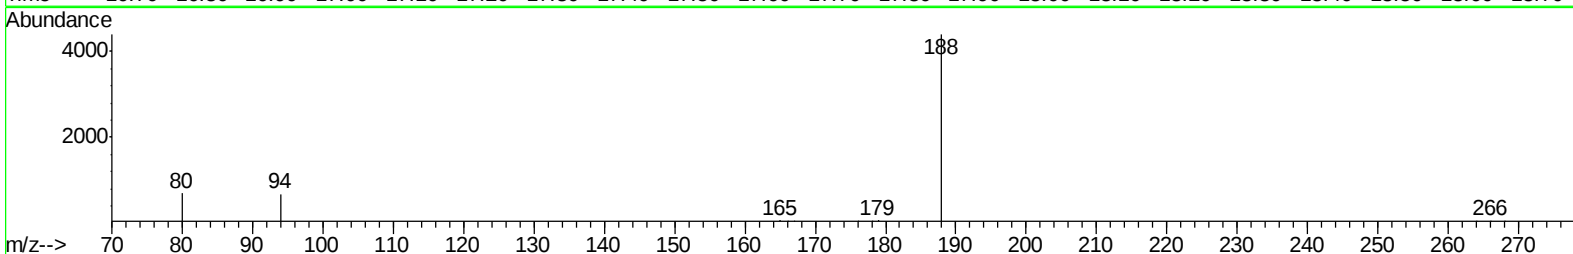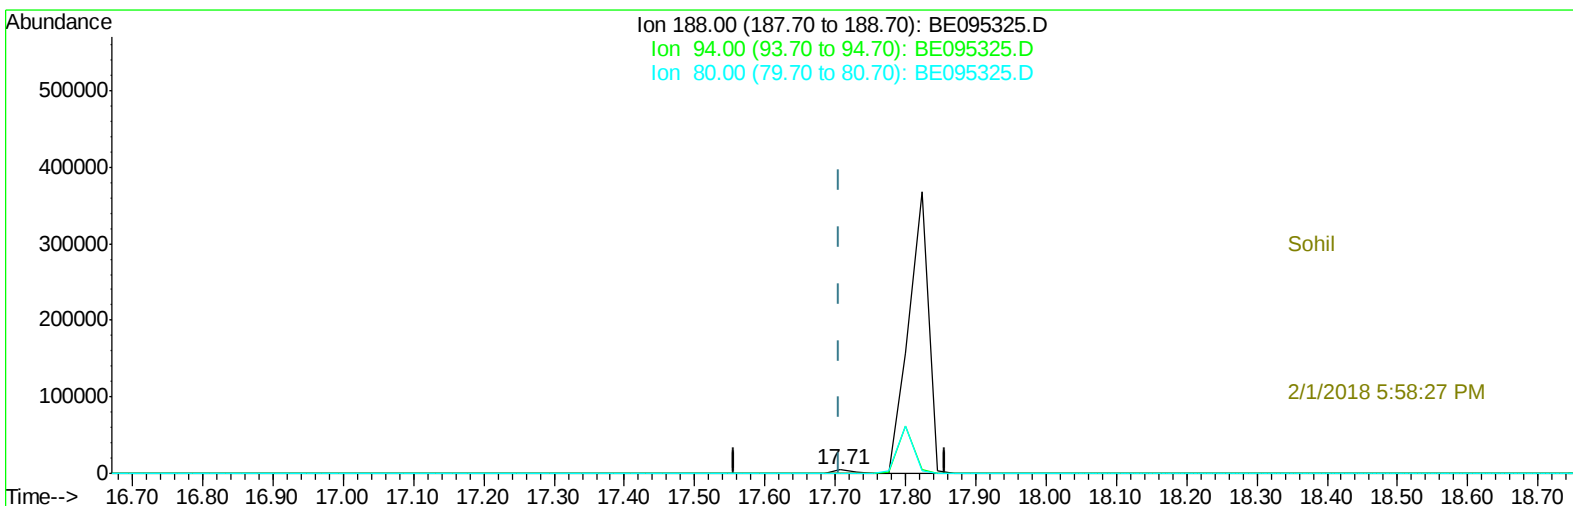

TIC: BE095325.D

(10) Phenanthrene-d10 (I)

17.708min (+0.001) 0.40ng/ul m

response 8813




Ion	Exp%	Act%
188.00	100	100
94.00	11.00	15.29#
80.00	11.80	15.95#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE013118\
Data File : BE095325.D
Acq On : 31 Jan 2018 19:57
Operator : SJ/JU
Sample : PB106079BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampled :
SBLK79

Manual Integrations
APPROVED

Quant Time: Feb 01 04:21:08 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 01 04:05:22 2018
Response via : Initial Calibration

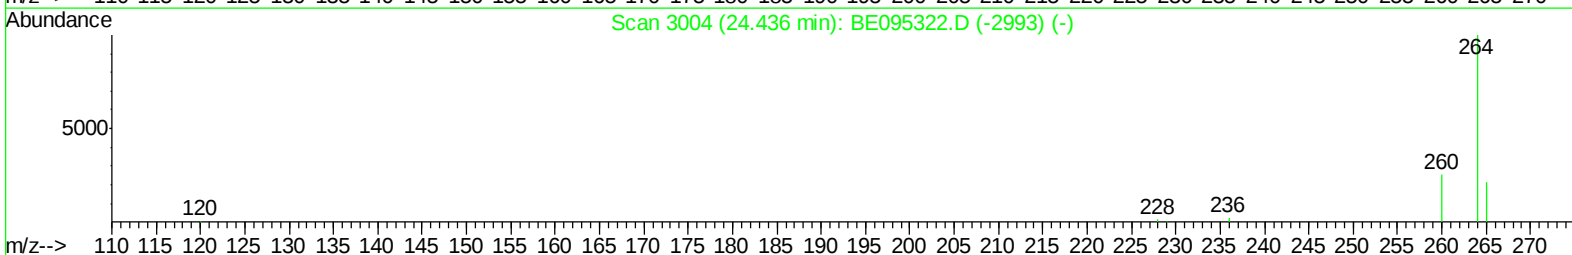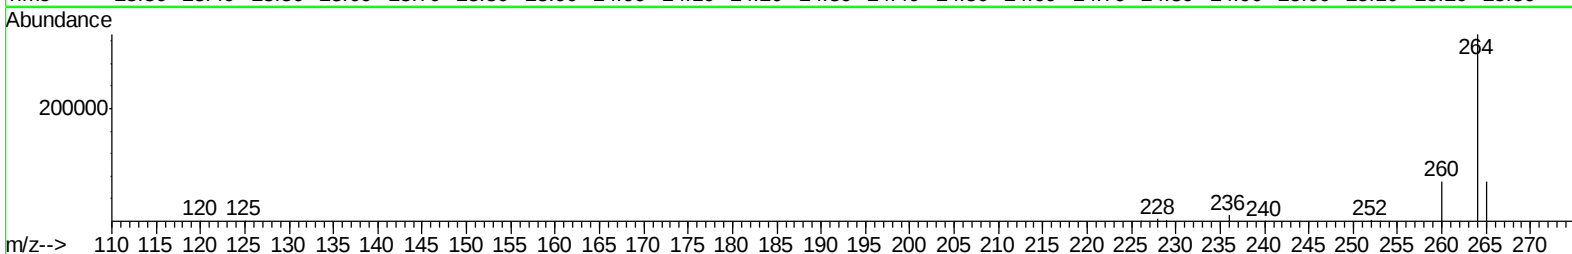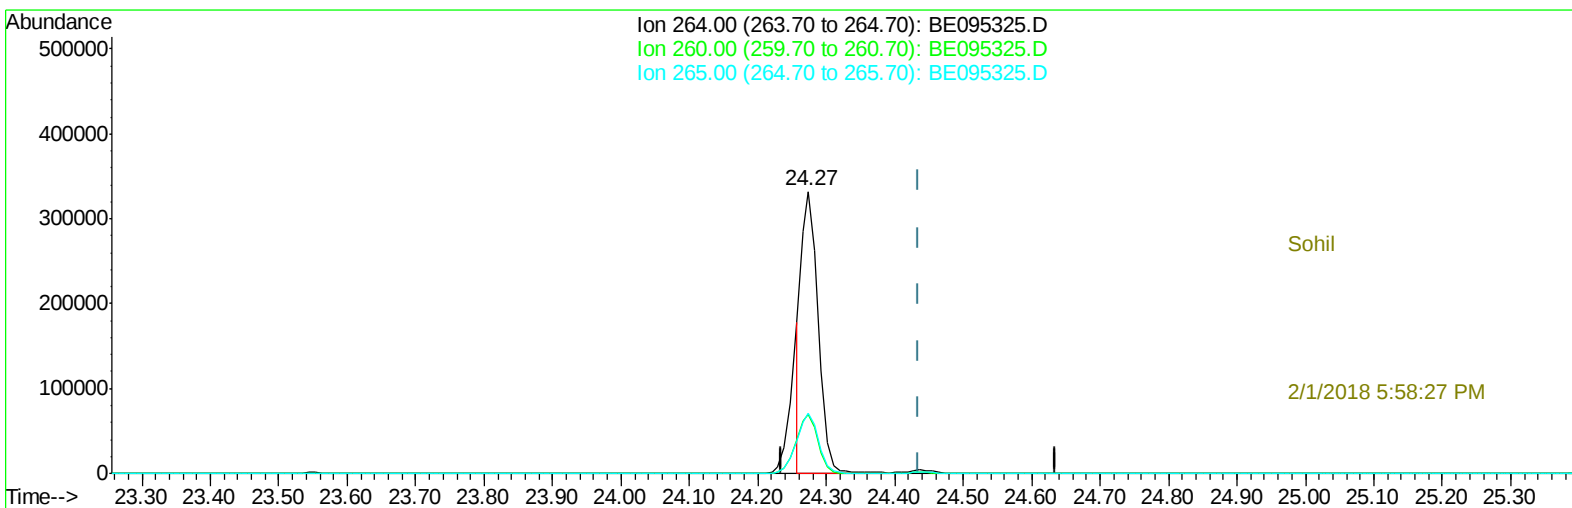

TIC: BE095325.D

(20) Perylene-d12 (I)

24.274min (-0.162) 0.40ng/ul

response 566864


Ion	Exp%	Act%
264.00	100	100
260.00	30.10	21.08#
265.00	103.50	21.33#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE013118\
Data File : BE095325.D
Acq On : 31 Jan 2018 19:57
Operator : SJ/JU
Sample : PB106079BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK79



Manual Integrations
APPROVED

Quant Time: Feb 01 04:21:08 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 01 04:05:22 2018
Response via : Initial Calibration

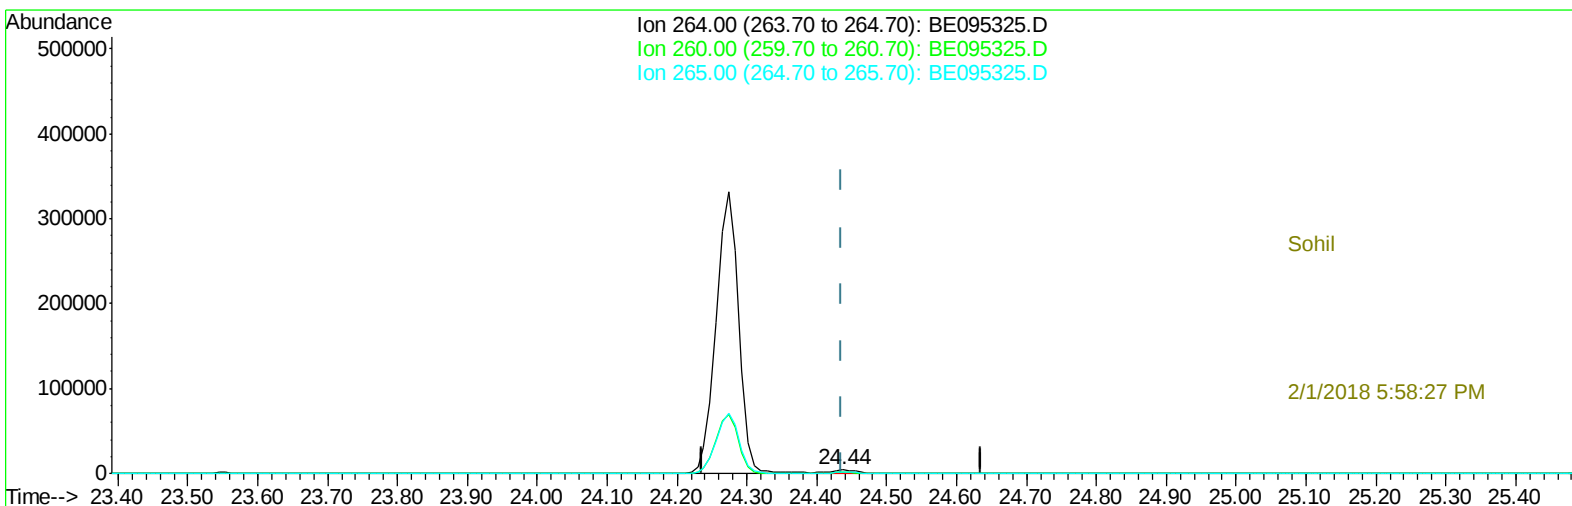

Sohil

2/1/2018 5:58:27 PM

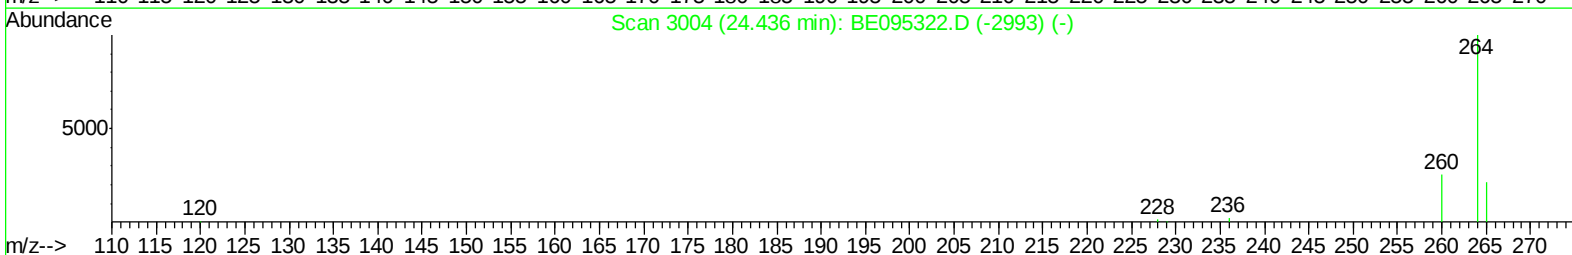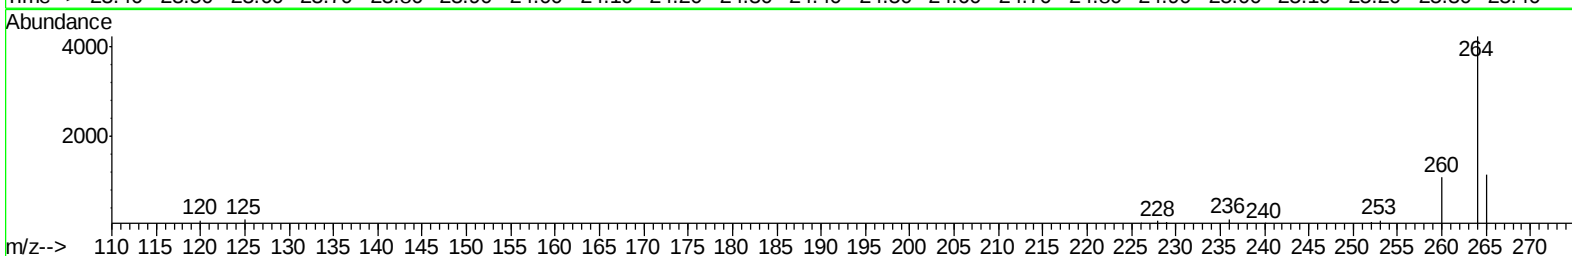

TIC: BE095325.D

(20) Perylene-d12 (I)

24.436min (+0.001) 0.40ng/ul m

response 8239

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	25.68
265.00	103.50	27.15#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE013118\
 Data File : BE095325.D
 Acq On : 31 Jan 2018 19:57
 Operator : SJ/JU
 Sample : PB106079BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 SBLK79

Manual Integrations
 APPROVED

Quant Time: Feb 01 04:21:55 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Feb 01 04:05:22 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.44	152	2213	0.40	ng/ul	0.00
2) Naphthalene-d8	11.26	136	6724	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.02	164	4359	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	8813m	0.40	ng/ul	0.00
16) Chrysene-d12	21.81	240	8883	0.40	ng/ul	0.00
20) Perylene-d12	24.44	264	8239m	0.40	ng/ul	0.00

Sohil

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.81	152	3969	0.36	ng/ul	0.00
14) Fluoranthene-d10	19.70	212	10413	0.31	ng/ul	0.00

Target Compounds	Ovalue
------------------	--------

2/1/2018 5:58:27 PM

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE013118\
Data File : BE095325.D
Acq On : 31 Jan 2018 19:57
Operator : SJ/JU
Sample : PB106079BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampled :
SBLK79

Manual Integrations
APPROVED

Quant Time: Feb 01 04:21:55 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 01 04:05:22 2018
Response via : Initial Calibration

