




Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA_E\Data\BE013118\
Data File : BE095346.D
Acq On : 1 Feb 2018 8:29
Operator : SJ/JU
Sample : J1245-19
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F6B80

Manual Integrations
APPROVED

Sohil
2/1/2018 5:59:22 PM

Quant Time: Feb 01 12:50:40 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 01 06:27:03 2018
Response via : Initial Calibration

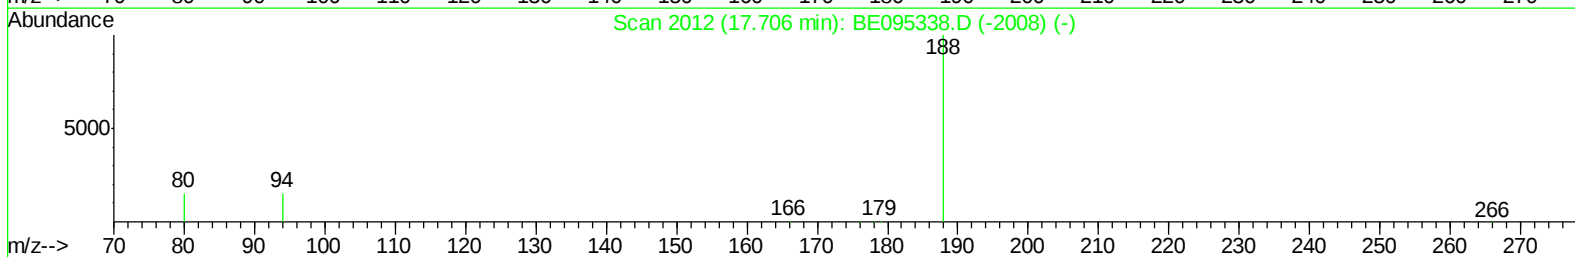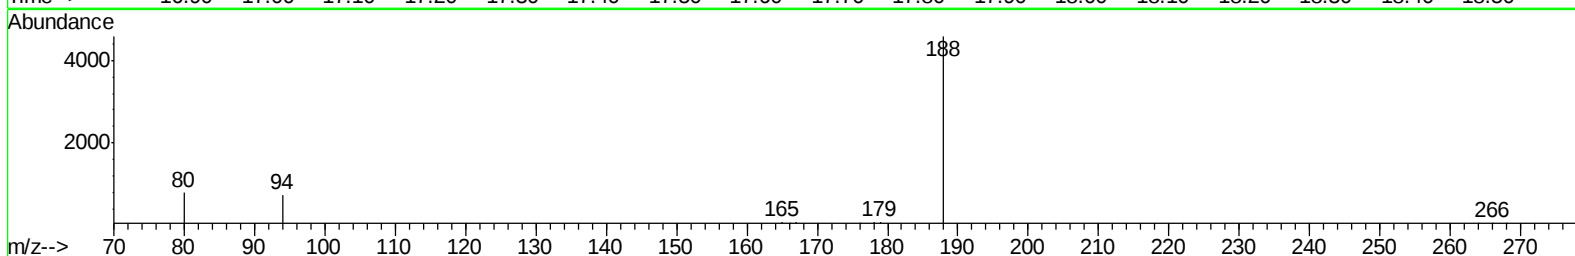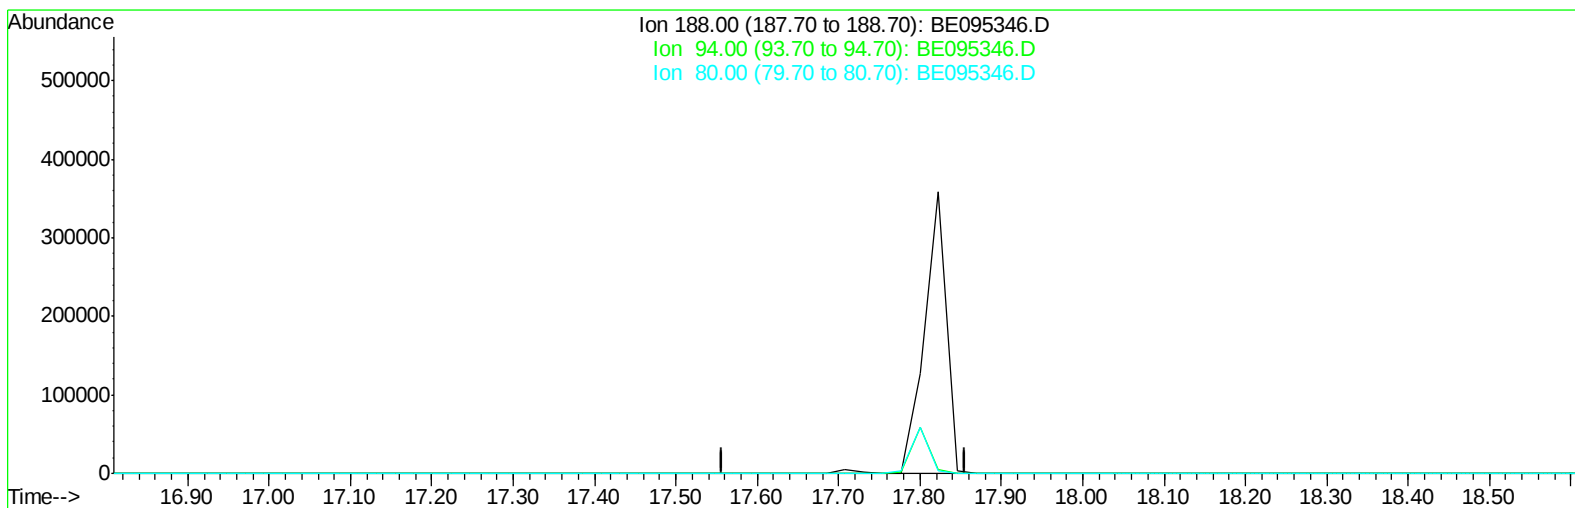

TIC: BE095346.D

(10) Phenanthrene-d10 (I)

17.706min (-17.706) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.00	0.00#
80.00	11.80	0.00#
0.00	0.00	0.00




Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA_E\Data\BE013118\
Data File : BE095346.D
Acq On : 1 Feb 2018 8:29
Operator : SJ/JU
Sample : J1245-19
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F6B80

Manual Integrations
APPROVED

Sohil
2/1/2018 5:59:22 PM

Quant Time: Feb 01 12:50:40 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 01 06:27:03 2018
Response via : Initial Calibration

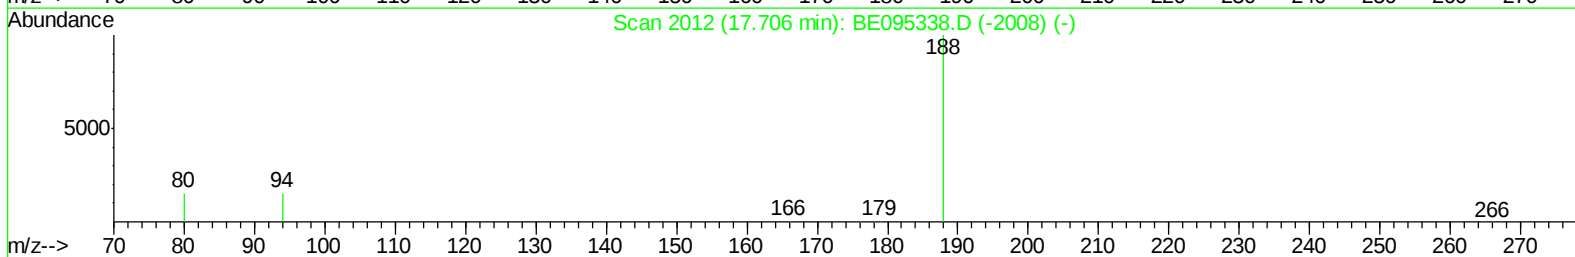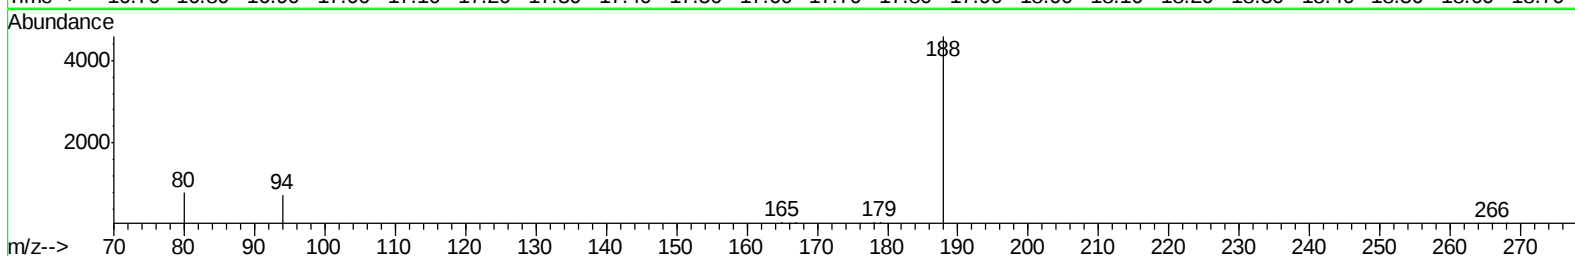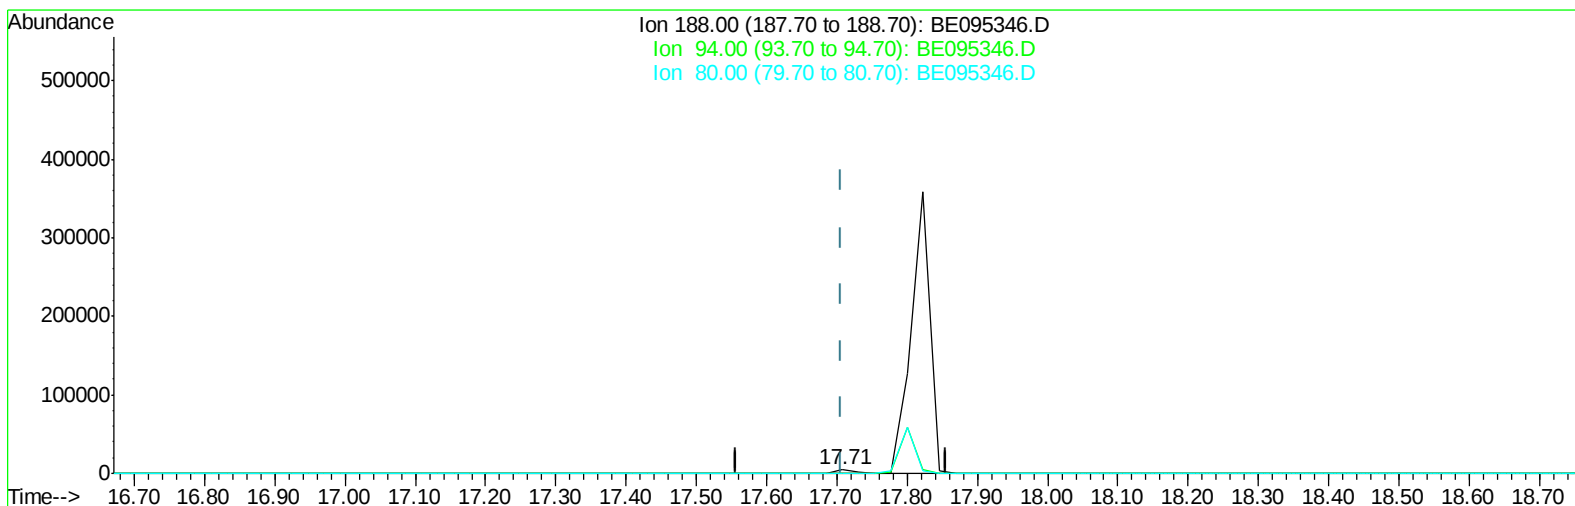

TIC: BE095346.D

(10) Phenanthrene-d10 (I)

17.708min (+0.001) 0.40ng/ul m

response 9437

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	16.37#
80.00	11.80	17.09#
0.00	0.00	0.00




Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA_E\Data\BE013118\
Data File : BE095346.D
Acq On : 1 Feb 2018 8:29
Operator : SJ/JU
Sample : J1245-19
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F6B80

Manual Integrations
APPROVED

Sohil
2/1/2018 5:59:22 PM

Quant Time: Feb 01 12:51:44 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 01 06:27:03 2018
Response via : Initial Calibration

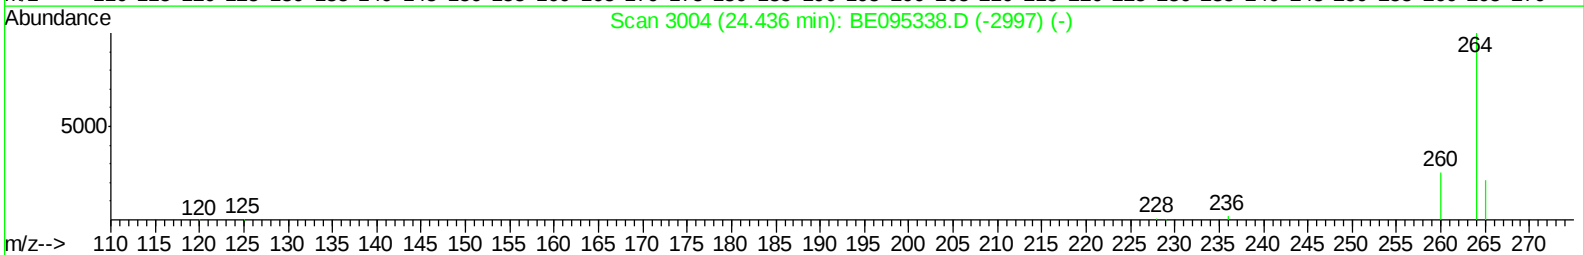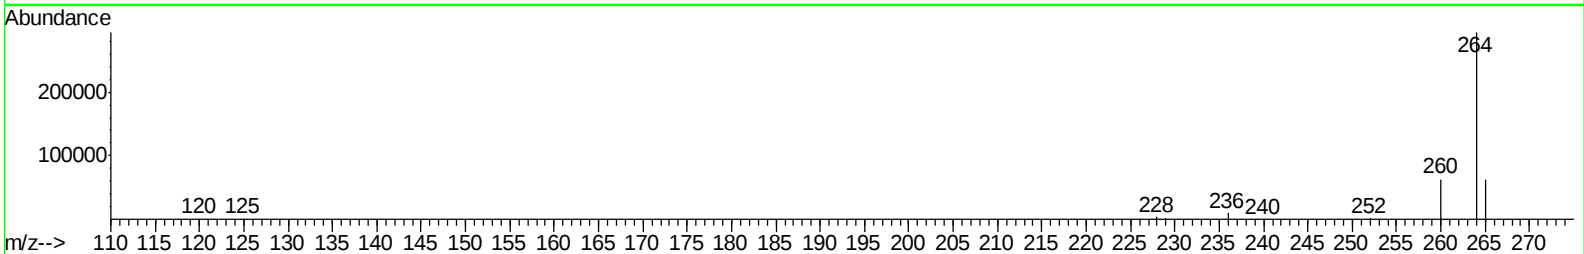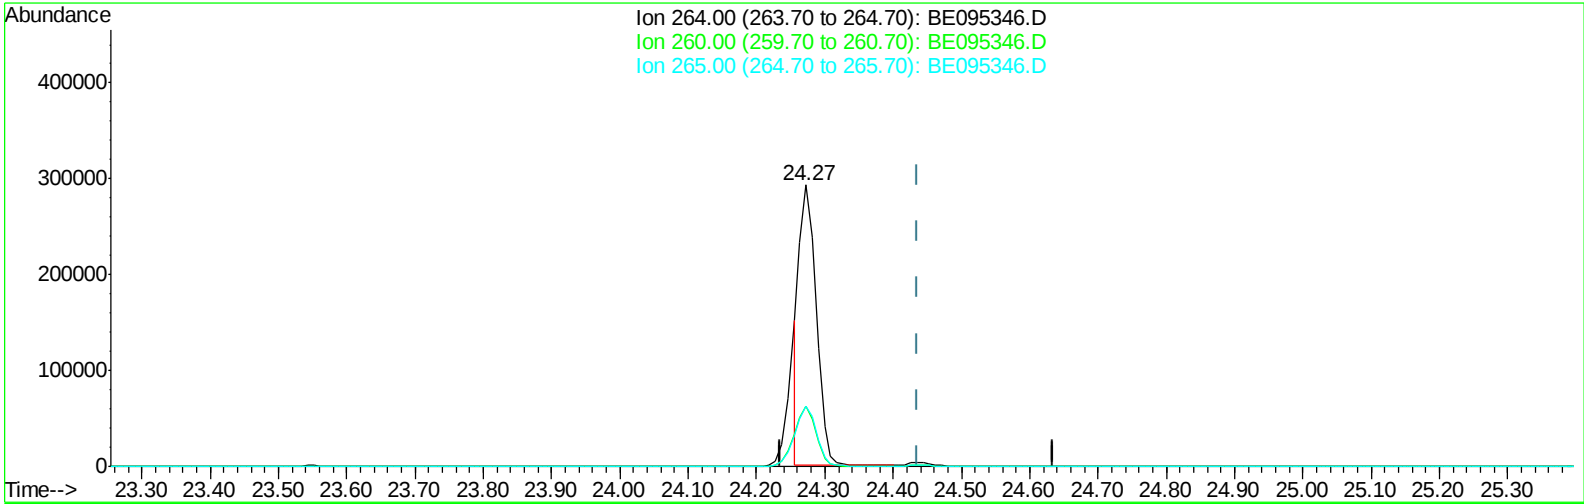

TIC: BE095346.D

(20) Perylene-d12 (I)
24.273min (-0.163) 0.40ng/ul
response 510378

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	21.33#
265.00	103.50	21.31#
0.00	0.00	0.00




Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA_E\Data\BE013118\
Data File : BE095346.D
Acq On : 1 Feb 2018 8:29
Operator : SJ/JU
Sample : J1245-19
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F6B80

Manual Integrations
APPROVED

Sohil
2/1/2018 5:59:22 PM

Quant Time: Feb 01 12:51:44 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 01 06:27:03 2018
Response via : Initial Calibration

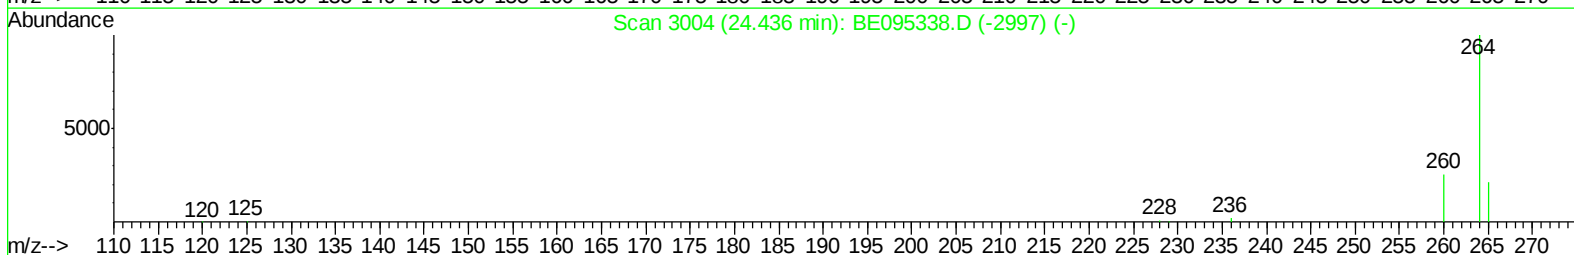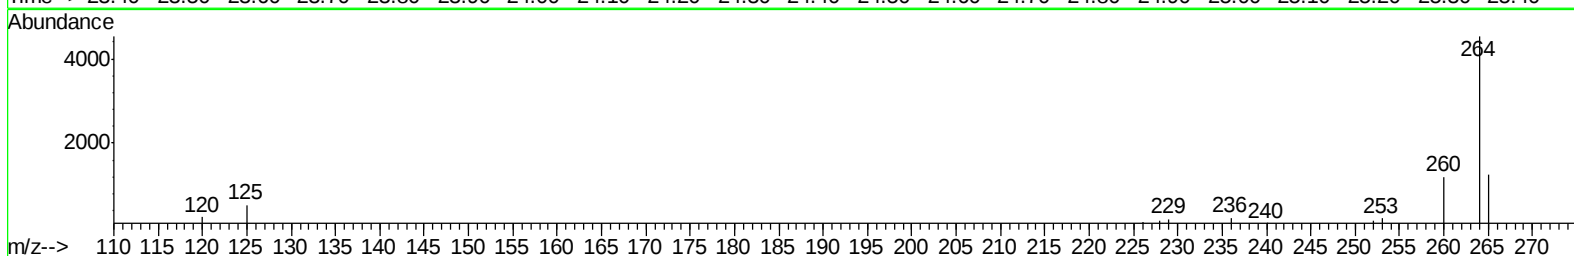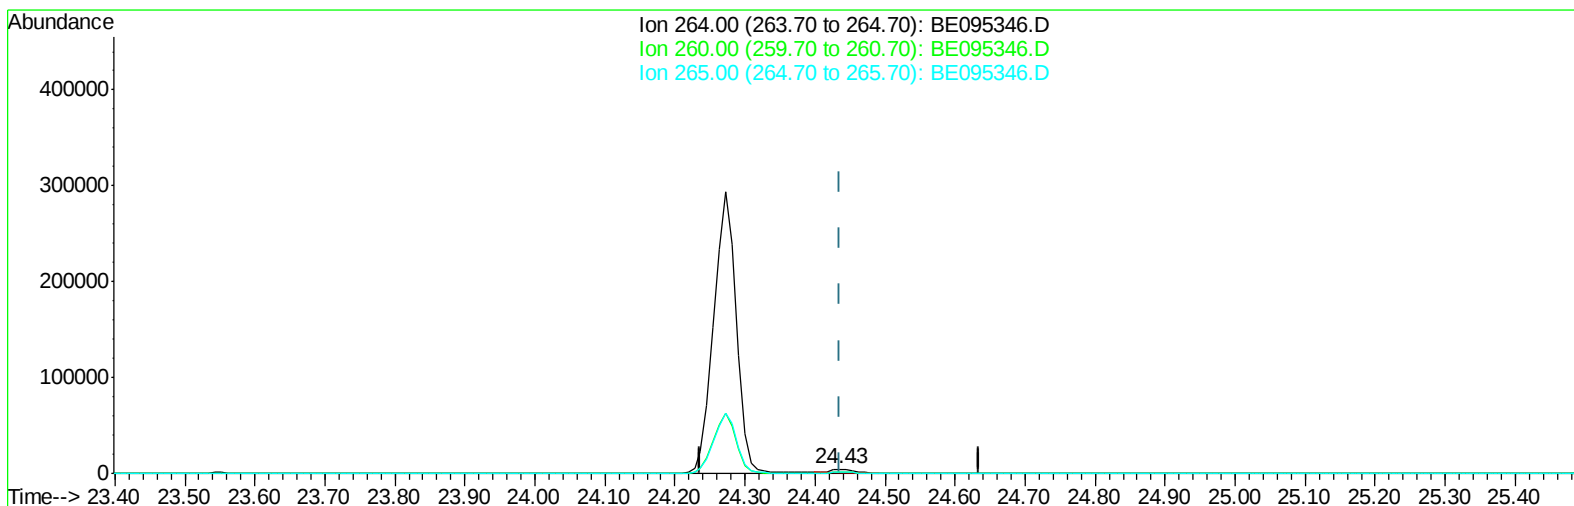

TIC: BE095346.D

(20) Perylene-d12 (I)

24.435min (-0.001) 0.40ng/ul m

response 8496

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	26.43
265.00	103.50	27.35#
0.00	0.00	0.00

Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA_E\Data\BE013118\
 Data File : BE095346.D
 Acq On : 1 Feb 2018 8:29
 Operator : SJ/JU
 Sample : J1245-19
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 F6B80

Manual Integrations
 APPROVED

Sohil
 2/1/2018 5:59:22 PM

Quant Time: Feb 01 12:52:36 2018
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Feb 01 06:27:03 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.44	152	2291	0.40	ng/ul	0.00
2) Naphthalene-d8	11.26	136	7331	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.02	164	4709	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	9437m	0.40	ng/ul	0.00
16) Chrysene-d12	21.80	240	9412	0.40	ng/ul	0.00
20) Perylene-d12	24.43	264	8496m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	3932	0.33	ng/ul	0.00
14) Fluoranthene-d10	19.70	212	9946	0.28	ng/ul	0.00
Target Compounds						
11) Pentachlorophenol	17.36	266	279	0.153	ng/ul	96
12) Phenanthrene	17.75	178	1135	0.036	ng/ul#	88
15) Fluoranthene	19.72	202	1212	0.029	ng/ul	85

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA_E\Data\BE013118\
Data File : BE095346.D
Acq On : 1 Feb 2018 8:29
Operator : SJ/JU
Sample : J1245-19
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F6B80

Manual Integrations
APPROVED

Sohil
2/1/2018 5:59:22 PM

Quant Time: Feb 01 12:52:36 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 01 06:27:03 2018
Response via : Initial Calibration

