




Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA_E\Data\BE013118\
Data File : BE095351.D
Acq On : 1 Feb 2018 11:28
Operator : SJ/JU
Sample : J1282-01
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F6B82

Manual Integrations
APPROVED

Sohil
2/1/2018 5:59:36 PM

Quant Time: Feb 01 13:18:41 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 01 06:27:03 2018
Response via : Initial Calibration

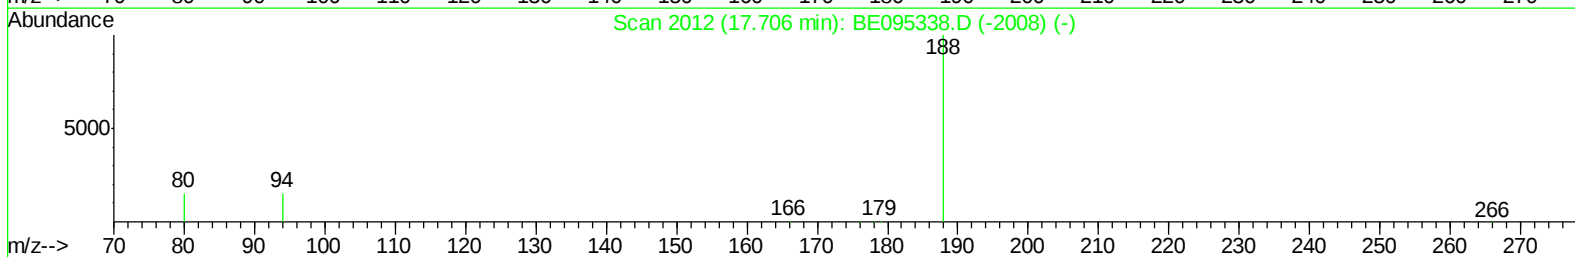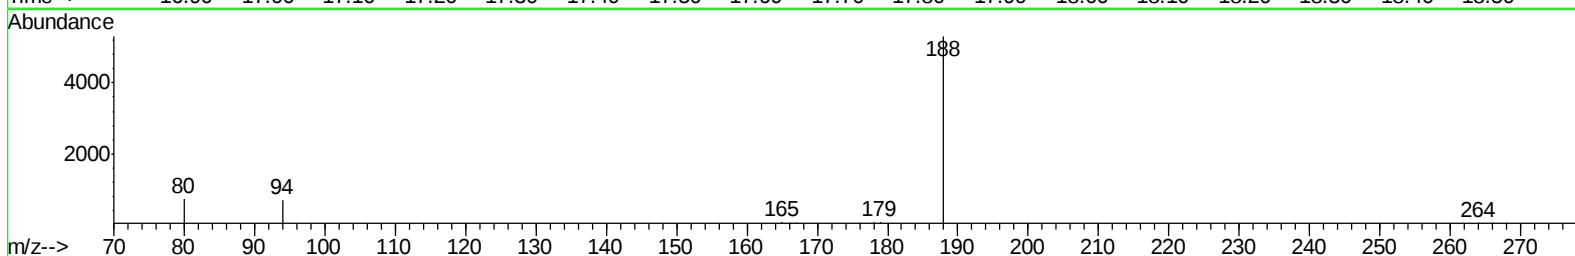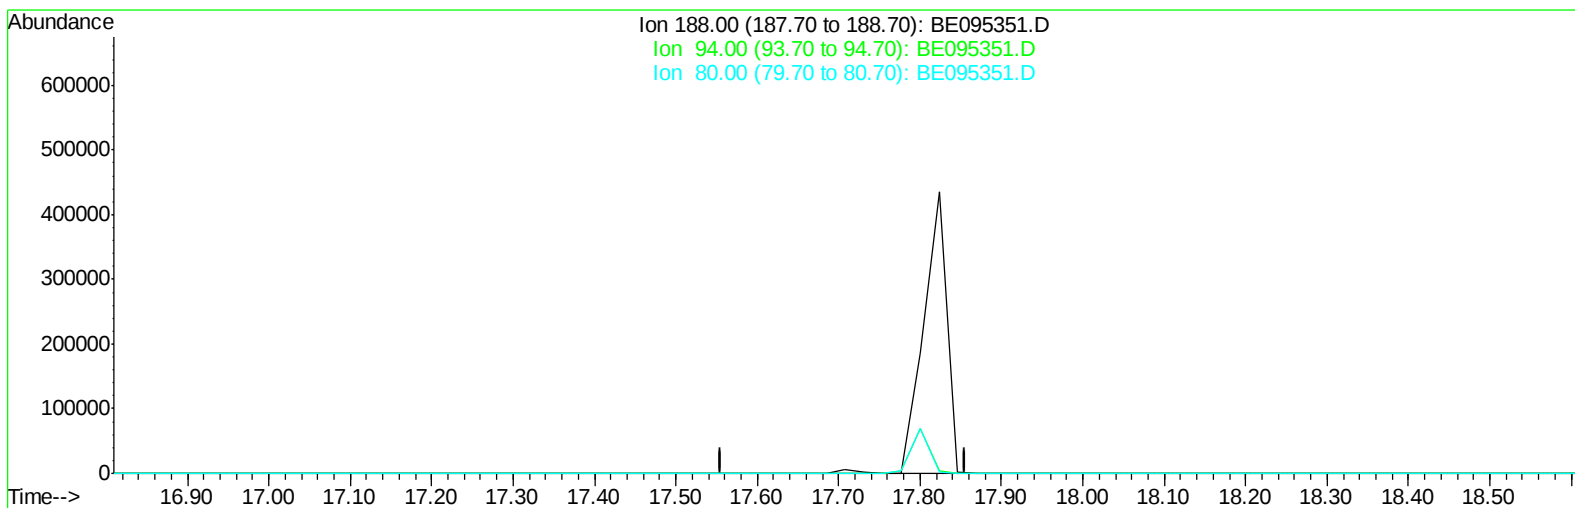

TIC: BE095351.D

(10) Phenanthrene-d10 (I)

17.706min (-17.706) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.00	0.00#
80.00	11.80	0.00#
0.00	0.00	0.00




Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA_E\Data\BE013118\
Data File : BE095351.D
Acq On : 1 Feb 2018 11:28
Operator : SJ/JU
Sample : J1282-01
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F6B82

Manual Integrations
APPROVED

Sohil
2/1/2018 5:59:36 PM

Quant Time: Feb 01 13:18:41 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 01 06:27:03 2018
Response via : Initial Calibration

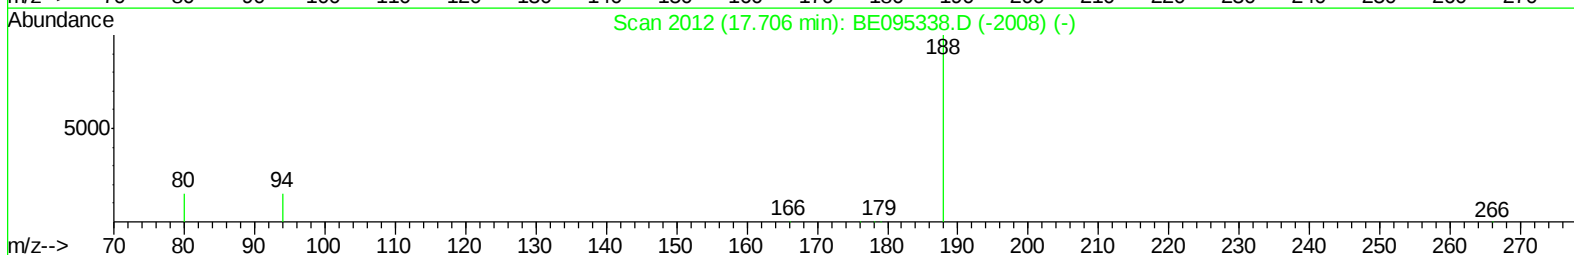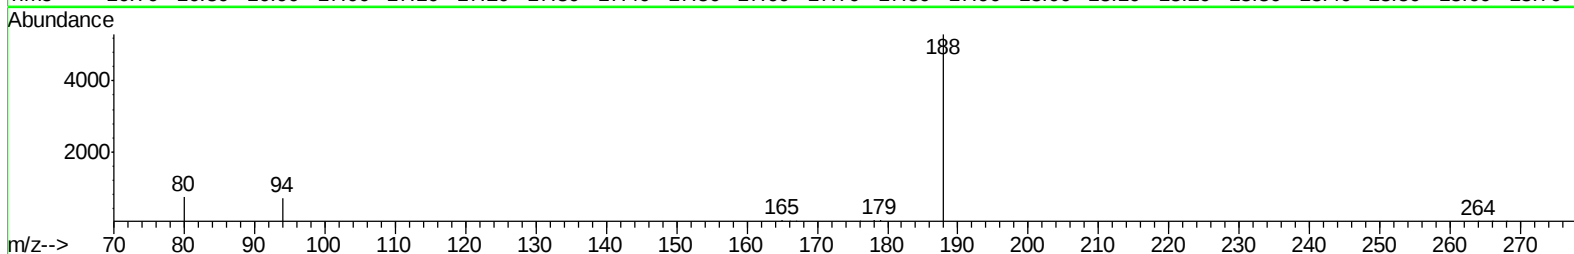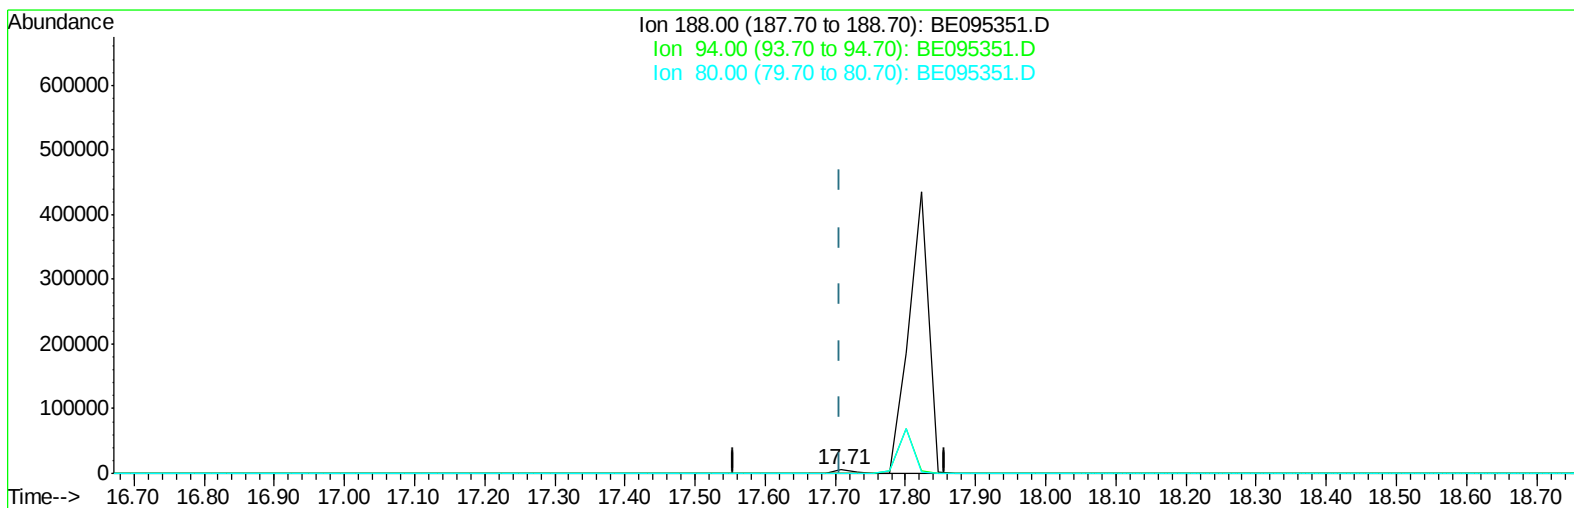

TIC: BE095351.D

(10) Phenanthrene-d10 (I)

17.708min (+0.002) 0.40ng/ul m

response 10326

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	13.50#
80.00	11.80	14.16
0.00	0.00	0.00




Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA_E\Data\BE013118\
Data File : BE095351.D
Acq On : 1 Feb 2018 11:28
Operator : SJ/JU
Sample : J1282-01
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F6B82

Manual Integrations
APPROVED

Sohil
2/1/2018 5:59:36 PM

Quant Time: Feb 01 13:19:44 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 01 06:27:03 2018
Response via : Initial Calibration

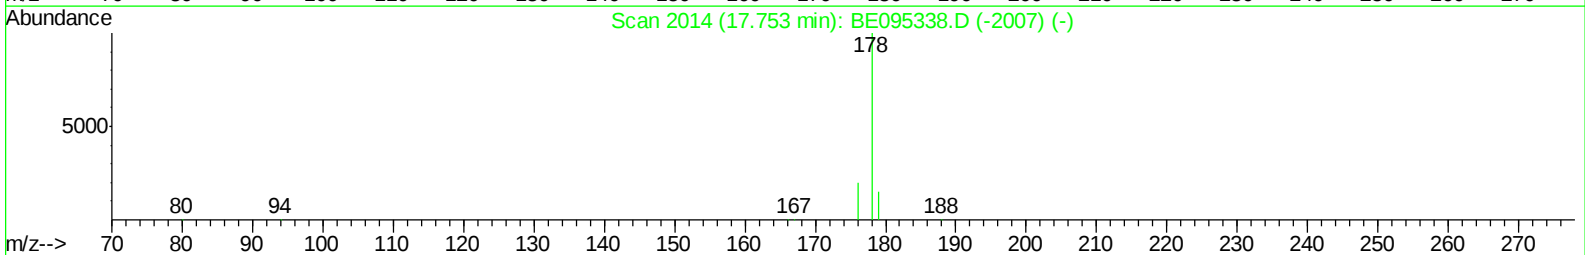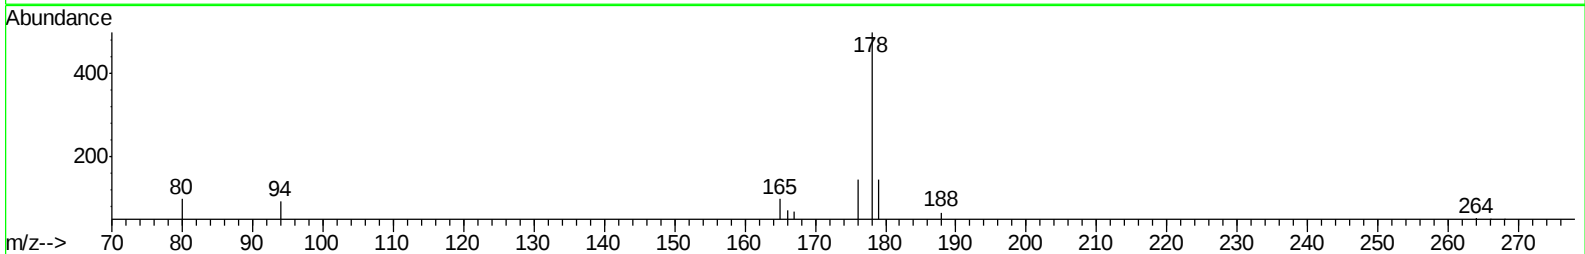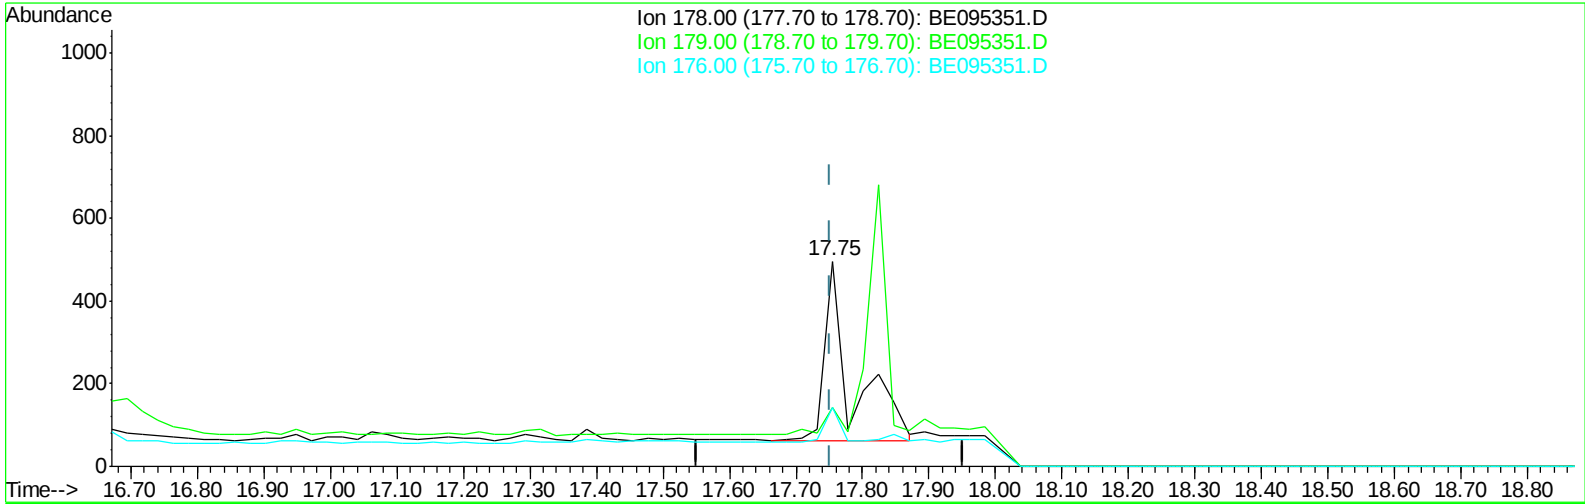

TIC: BE095351.D

(12) Phenanthrene

17.754min (+0.002) 0.04ng/ul

response 1222

Ion	Exp%	Act%
178.00	100	100
179.00	23.00	28.97#
176.00	17.00	28.97#
0.00	0.00	0.00




Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA_E\Data\BE013118\
Data File : BE095351.D
Acq On : 1 Feb 2018 11:28
Operator : SJ/JU
Sample : J1282-01
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F6B82

Manual Integrations
APPROVED

Sohil
2/1/2018 5:59:36 PM

Quant Time: Feb 01 13:19:44 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 01 06:27:03 2018
Response via : Initial Calibration

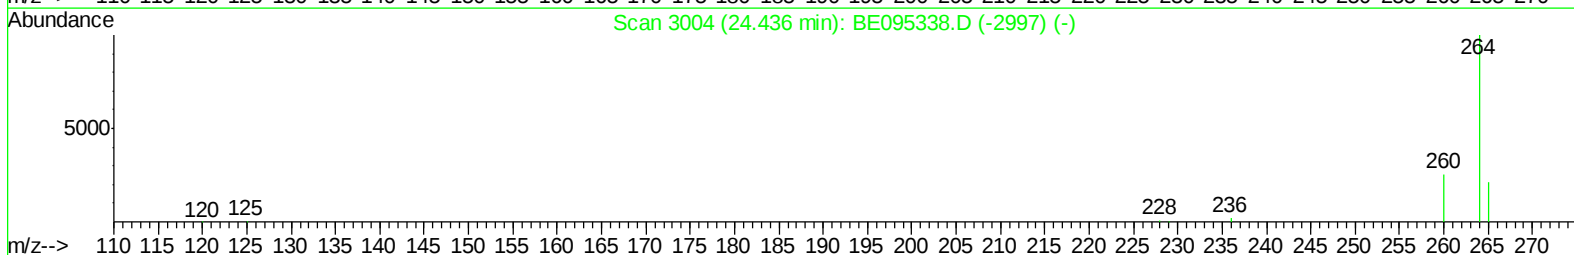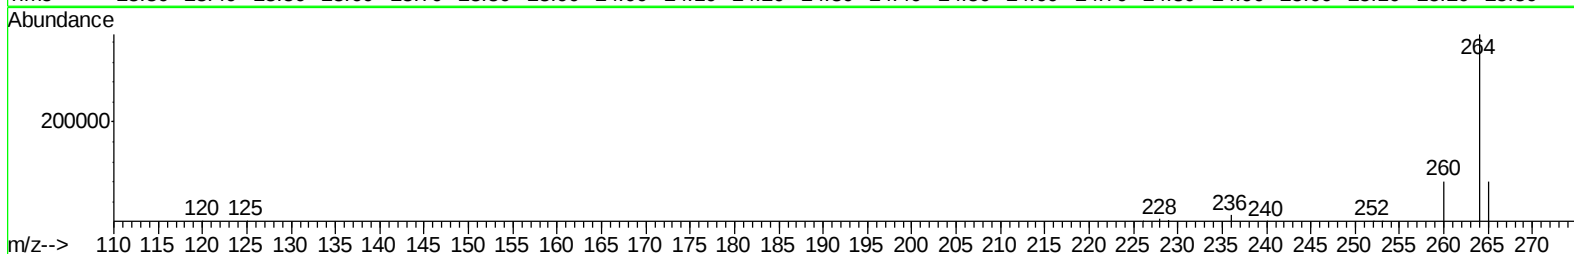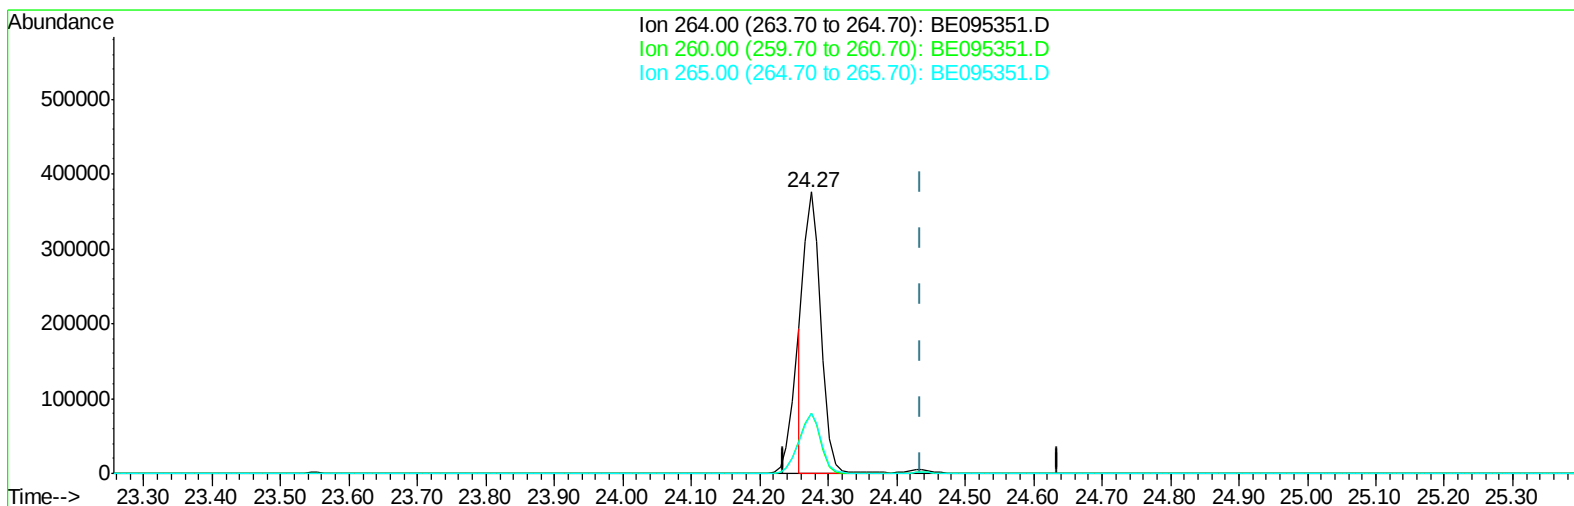

TIC: BE095351.D

(20) Perylene-d12 (I)

24.275min (-0.161) 0.40ng/ul

response 652750

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	21.33#
265.00	103.50	21.43#
0.00	0.00	0.00




Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA_E\Data\BE013118\
Data File : BE095351.D
Acq On : 1 Feb 2018 11:28
Operator : SJ/JU
Sample : J1282-01
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F6B82

Manual Integrations
APPROVED

Sohil
2/1/2018 5:59:36 PM

Quant Time: Feb 01 13:19:44 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 01 06:27:03 2018
Response via : Initial Calibration

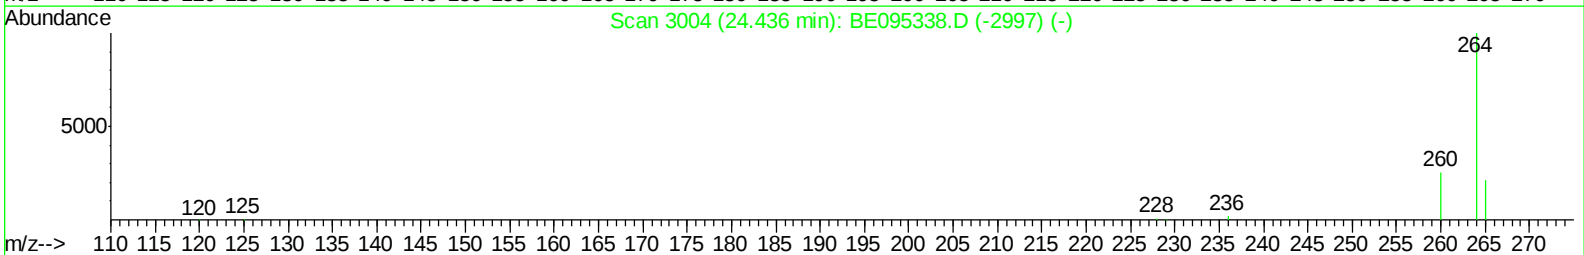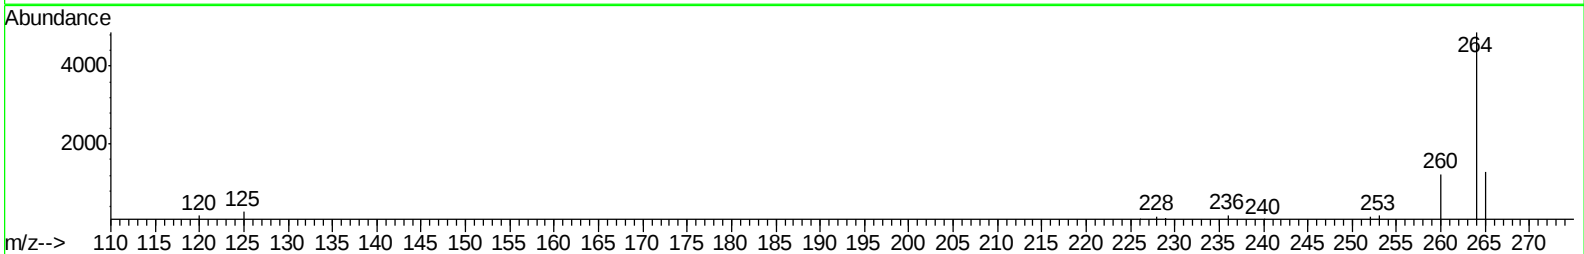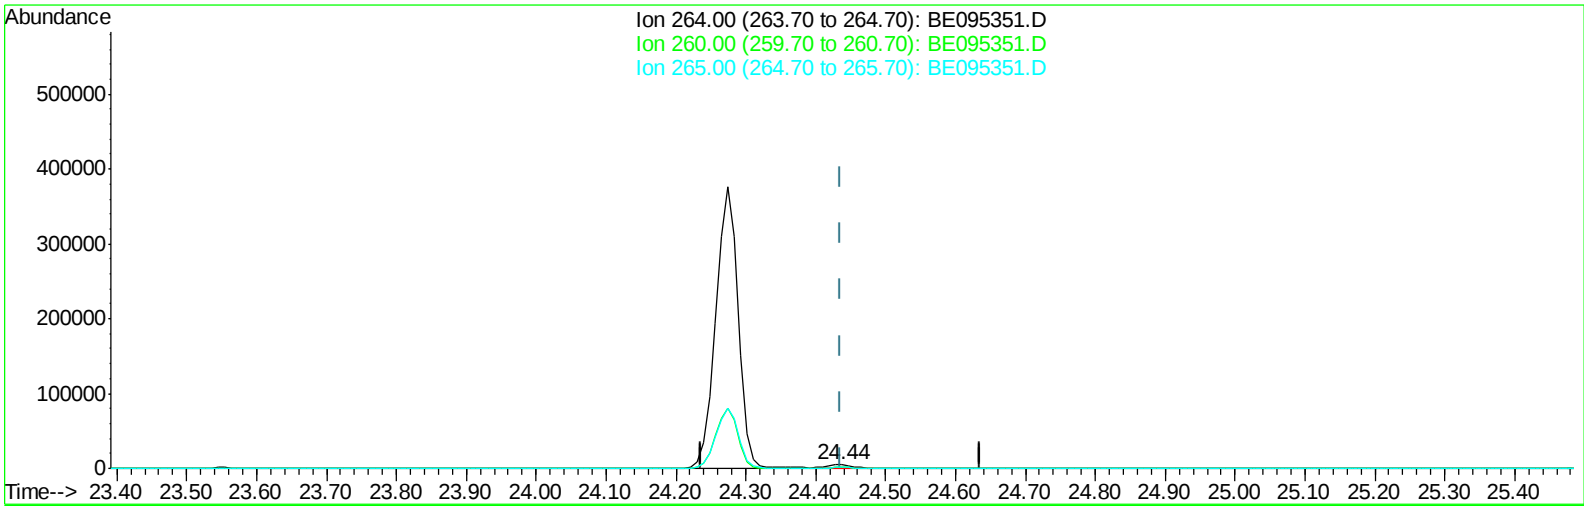

TIC: BE095351.D

(20) Perylene-d12 (I)

24.437min (+0.001) 0.40ng/ul m

response 8777

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	25.45
265.00	103.50	26.73#
0.00	0.00	0.00

Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA_E\Data\BE013118\
Data File : BE095351.D
Acq On : 1 Feb 2018 11:28
Operator : SJ/JU
Sample : J1282-01
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F6B82

Manual Integrations
APPROVED

Sohil
2/1/2018 5:59:36 PM

Quant Time: Feb 01 13:21:46 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 01 06:27:03 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.44	152	2343	0.40	ng/ul	0.00
2) Naphthalene-d8	11.26	136	7509	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.02	164	5044	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	10326m	0.40	ng/ul	0.00
16) Chrysene-d12	21.81	240	9917	0.40	ng/ul	0.00
20) Perylene-d12	24.44	264	8777m	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.81	152	4928	0.40	ng/ul	0.00
14) Fluoranthene-d10	19.70	212	12446	0.31	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA_E\Data\BE013118\
Data File : BE095351.D
Acq On : 1 Feb 2018 11:28
Operator : SJ/JU
Sample : J1282-01
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F6B82

Manual Integrations
APPROVED

Sohil
2/1/2018 5:59:36 PM

Quant Time: Feb 01 13:21:46 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 01 06:27:03 2018
Response via : Initial Calibration

