




Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA_E\Data\BE013118\
Data File : BE095352.D
Acq On : 1 Feb 2018 12:04
Operator : SJ/JU
Sample : J1282-07
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F6B87

Manual Integrations
APPROVED

Sohil
2/1/2018 5:59:39 PM

Quant Time: Feb 01 13:24:15 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 01 06:27:03 2018
Response via : Initial Calibration

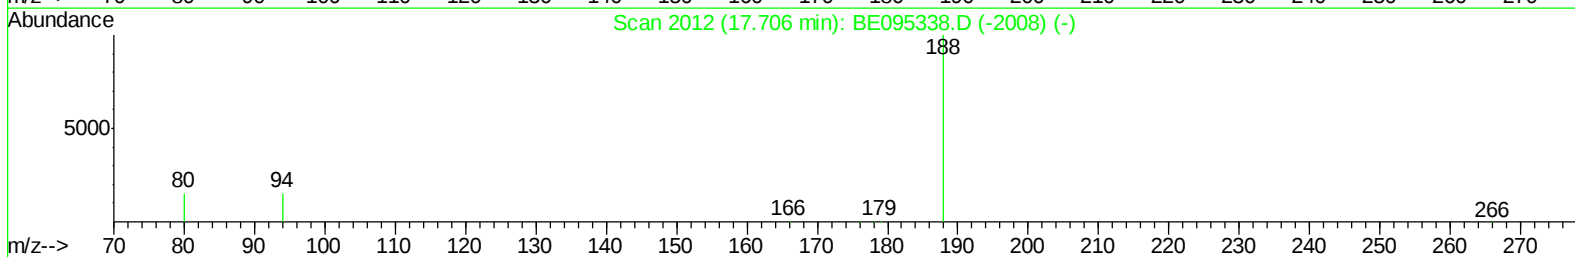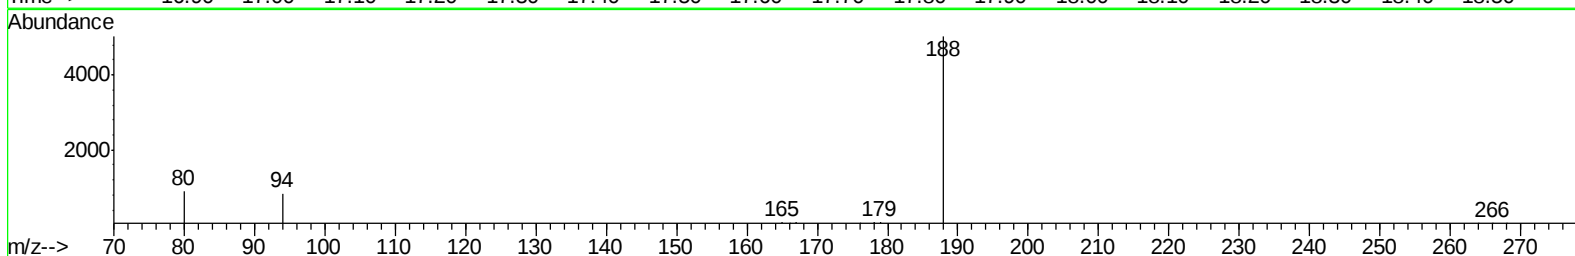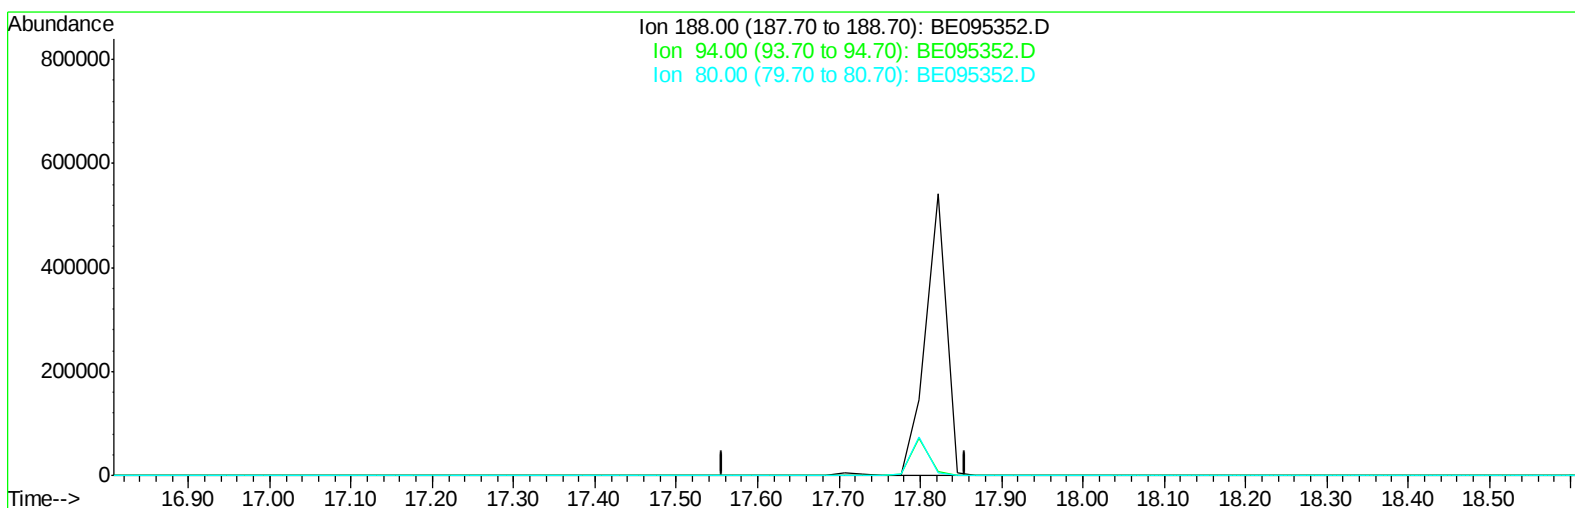

TIC: BE095352.D

(10) Phenanthrene-d10 (I)

17.706min (-17.706) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.00	0.00#
80.00	11.80	0.00#
0.00	0.00	0.00




Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA_E\Data\BE013118\
Data File : BE095352.D
Acq On : 1 Feb 2018 12:04
Operator : SJ/JU
Sample : J1282-07
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F6B87

Manual Integrations
APPROVED

Sohil
2/1/2018 5:59:39 PM

Quant Time: Feb 01 13:24:15 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 01 06:27:03 2018
Response via : Initial Calibration

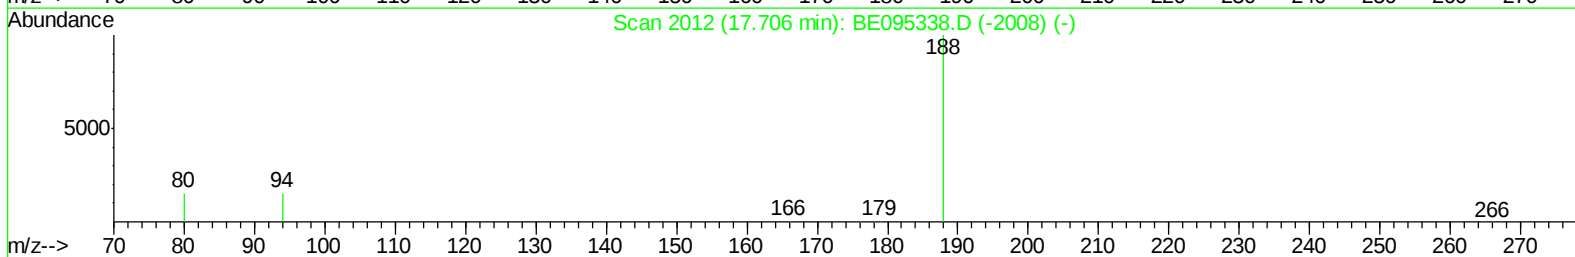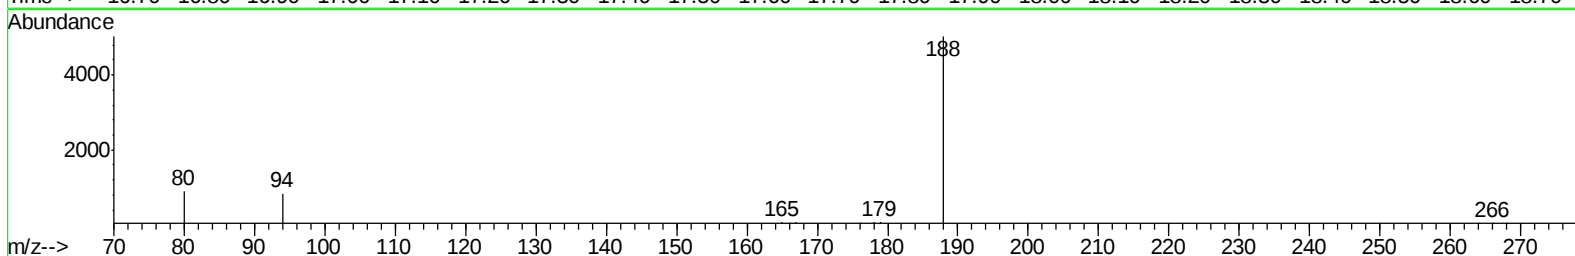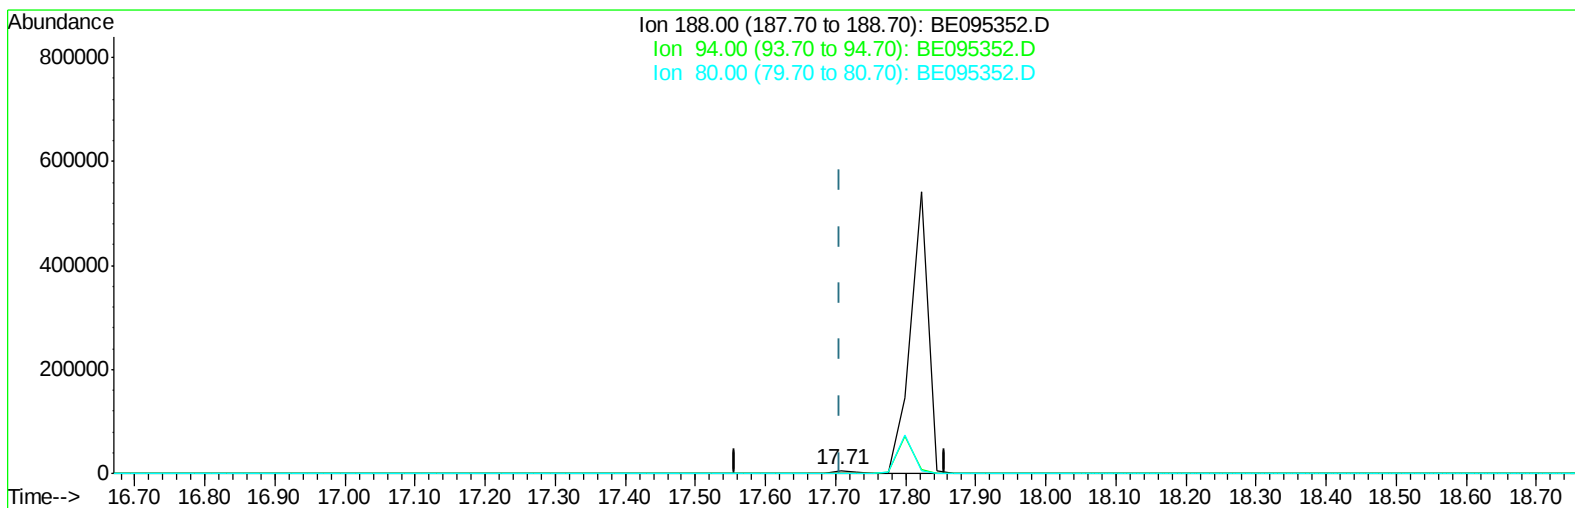

TIC: BE095352.D

(10) Phenanthrene-d10 (I)

17.707min (+0.000) 0.40ng/ul m

response 11298

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	16.88#
80.00	11.80	18.18#
0.00	0.00	0.00




Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA_E\Data\BE013118\
Data File : BE095352.D
Acq On : 1 Feb 2018 12:04
Operator : SJ/JU
Sample : J1282-07
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F6B87

Manual Integrations
APPROVED

Sohil
2/1/2018 5:59:39 PM

Quant Time: Feb 01 13:29:55 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 01 06:27:03 2018
Response via : Initial Calibration

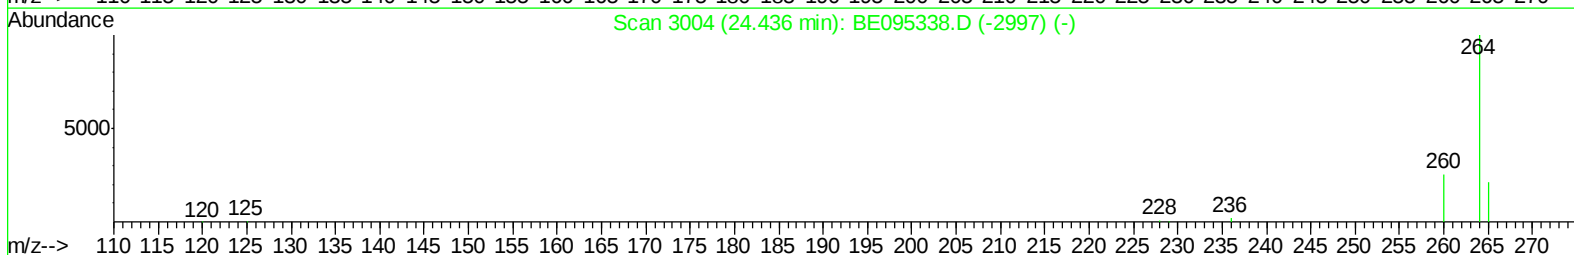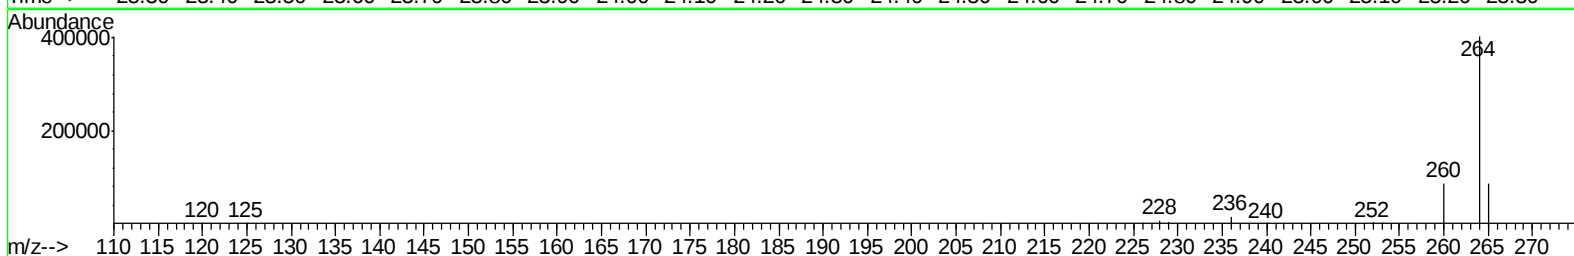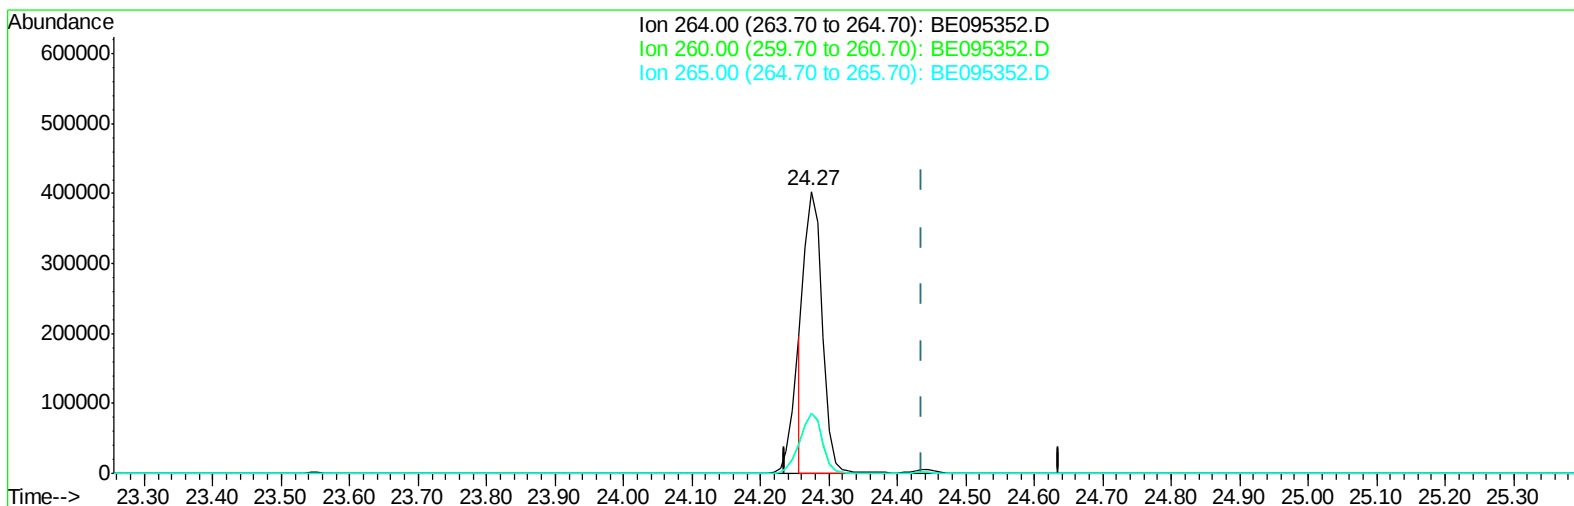

TIC: BE095352.D

(20) Perylene-d12 (I)

24.274min (-0.162) 0.40ng/ul

response 734790

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	21.42#
265.00	103.50	21.45#
0.00	0.00	0.00




Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA_E\Data\BE013118\
Data File : BE095352.D
Acq On : 1 Feb 2018 12:04
Operator : SJ/JU
Sample : J1282-07
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F6B87

Manual Integrations
APPROVED

Sohil
2/1/2018 5:59:39 PM

Quant Time: Feb 01 13:29:55 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 01 06:27:03 2018
Response via : Initial Calibration

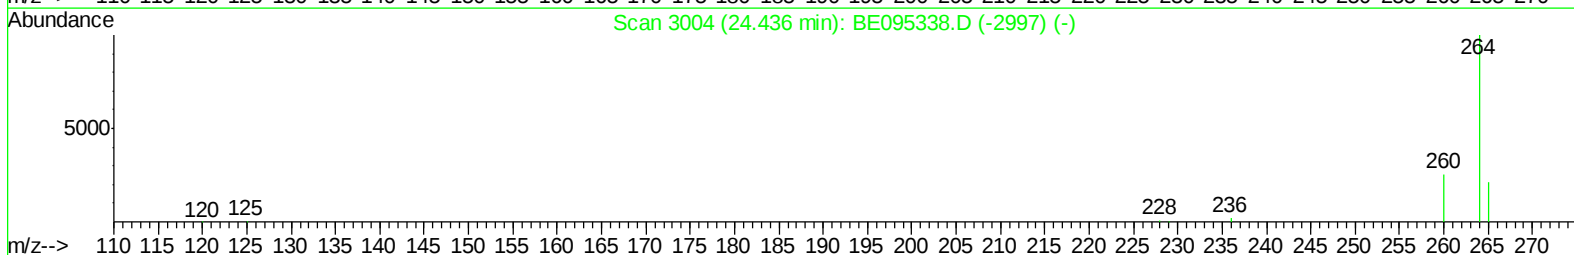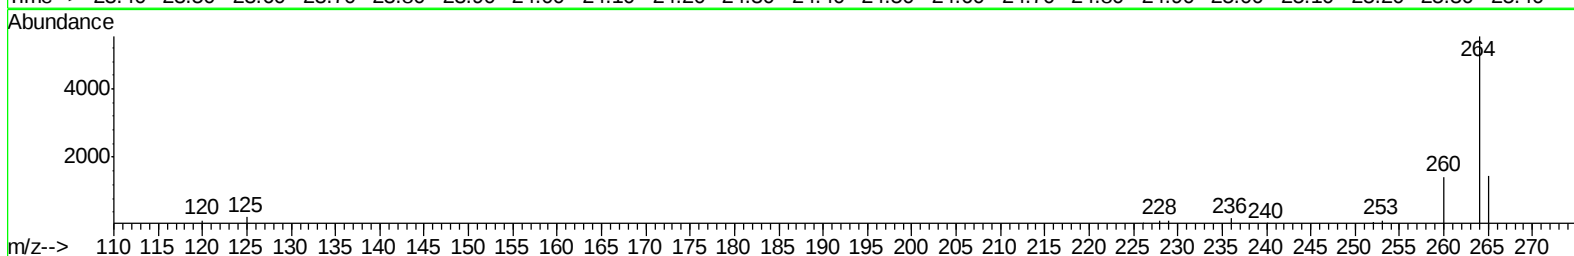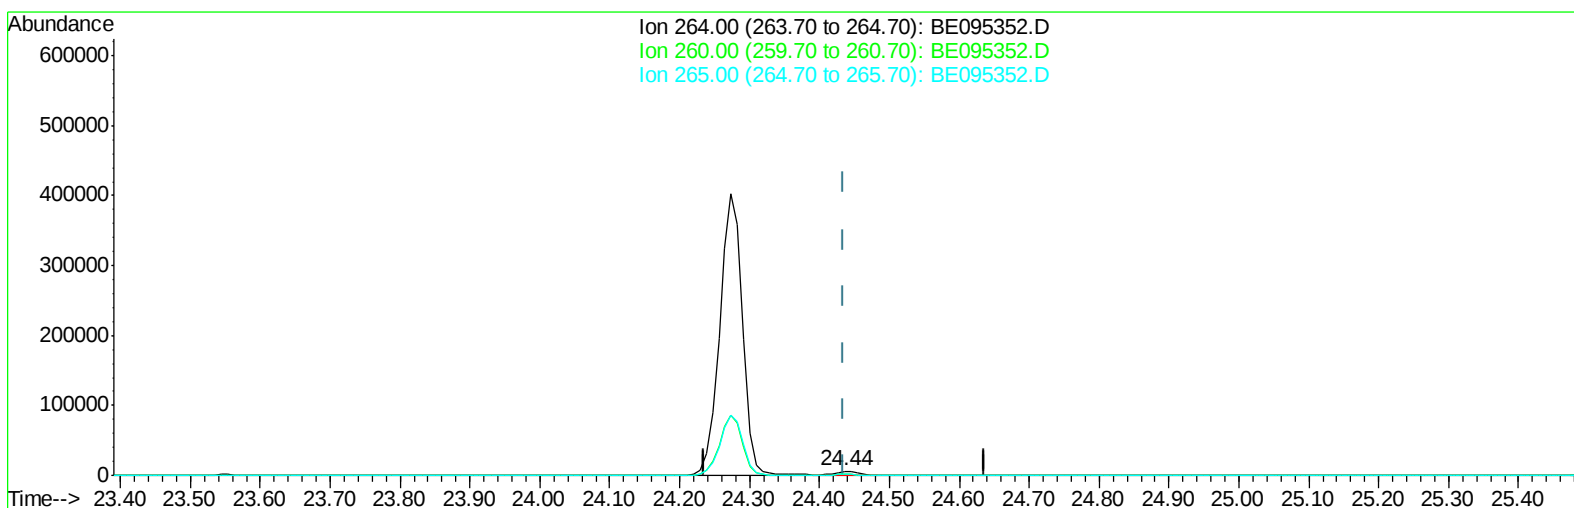

TIC: BE095352.D

(20) Perylene-d12 (I)

24.436min (+0.000) 0.40ng/ul m

response 10550

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	25.81
265.00	103.50	26.35#
0.00	0.00	0.00

Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA_E\Data\BE013118\
Data File : BE095352.D
Acq On : 1 Feb 2018 12:04
Operator : SJ/JU
Sample : J1282-07
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F6B87

Manual Integrations
APPROVED

Sohil
2/1/2018 5:59:39 PM

Quant Time: Feb 01 13:30:49 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 01 06:27:03 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.44	152	2625	0.40	ng/ul	0.00
2) Naphthalene-d8	11.26	136	8515	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.01	164	5528	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	11298m	0.40	ng/ul	0.00
16) Chrysene-d12	21.80	240	11295	0.40	ng/ul	0.00
20) Perylene-d12	24.44	264	10550m	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.81	152	5292	0.38	ng/ul	0.00
14) Fluoranthene-d10	19.70	212	13549	0.31	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA_E\Data\BE013118\
Data File : BE095352.D
Acq On : 1 Feb 2018 12:04
Operator : SJ/JU
Sample : J1282-07
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F6B87

Manual Integrations
APPROVED

Sohil
2/1/2018 5:59:39 PM

Quant Time: Feb 01 13:30:49 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 01 06:27:03 2018
Response via : Initial Calibration

