


Data Path : Z:\HPCHEM1\BNA E\DATA\BE020117\
 Data File : BE092706.D
 Acq On : 1 Feb 2017 9:22
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE011617.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jan 17 10:14:01 2017

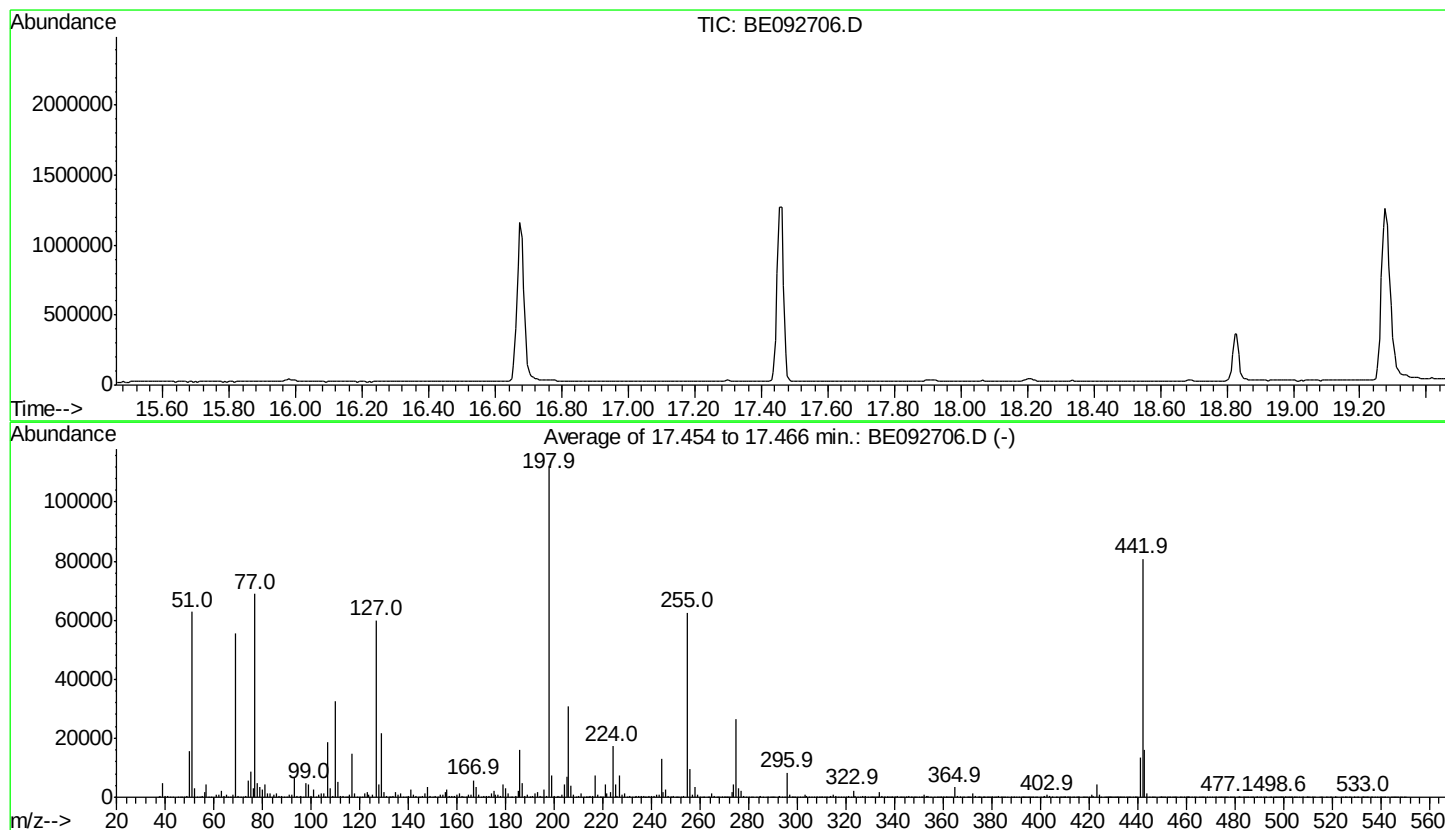

AutoFind: Scans 2530, 2531, 2532; Background Corrected with Scan 2522

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	55.9	62781	PASS
68	69	0.00	2	1.6	867	PASS
69	198	0.00	100	49.4	55448	PASS
70	69	0.00	2	0.7	383	PASS
127	198	10	80	53.3	59833	PASS
197	198	0.00	2	0.2	246	PASS
198	198	100	100	100.0	112340	PASS
199	198	5	9	6.6	7446	PASS
275	198	10	60	23.4	26275	PASS
365	198	1	100	3.0	3394	PASS
441	442	0.01	24	16.9	13671	PASS
442	198	50	100	72.0	80855	PASS
443	442	15	24	19.7	15938	PASS