

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020118\
 Data File : BE095371.D
 Acq On : 1 Feb 2018 23:30
 Operator : SJ/JU
 Sample : J1295-19
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Feb 02 04:09:33 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 02 04:07:20 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.44	152	2059	0.40	ng/ul	0.00
2) Naphthalene-d8	11.26	136	6347	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.02	164	4282	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.71
16) Chrysene-d12	21.80	240	8206	0.40	ng/ul	0.00
20) Perylene-d12	24.27	264	634557	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	5011	0.48	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	12182	0.00	ng/ul	0.00
Target Compounds						
17) Pyrene	20.05	202	2540	0.092	ng/ul#	1
18) Benzo(a)anthracene	21.79	228	659	0.026	ng/ul#	79


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020118\
Data File : BE095371.D
Acq On : 1 Feb 2018 23:30
Operator : SJ/JU
Sample : J1295-19
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Feb 02 04:09:33 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 02 04:07:20 2018
Response via : Initial Calibration

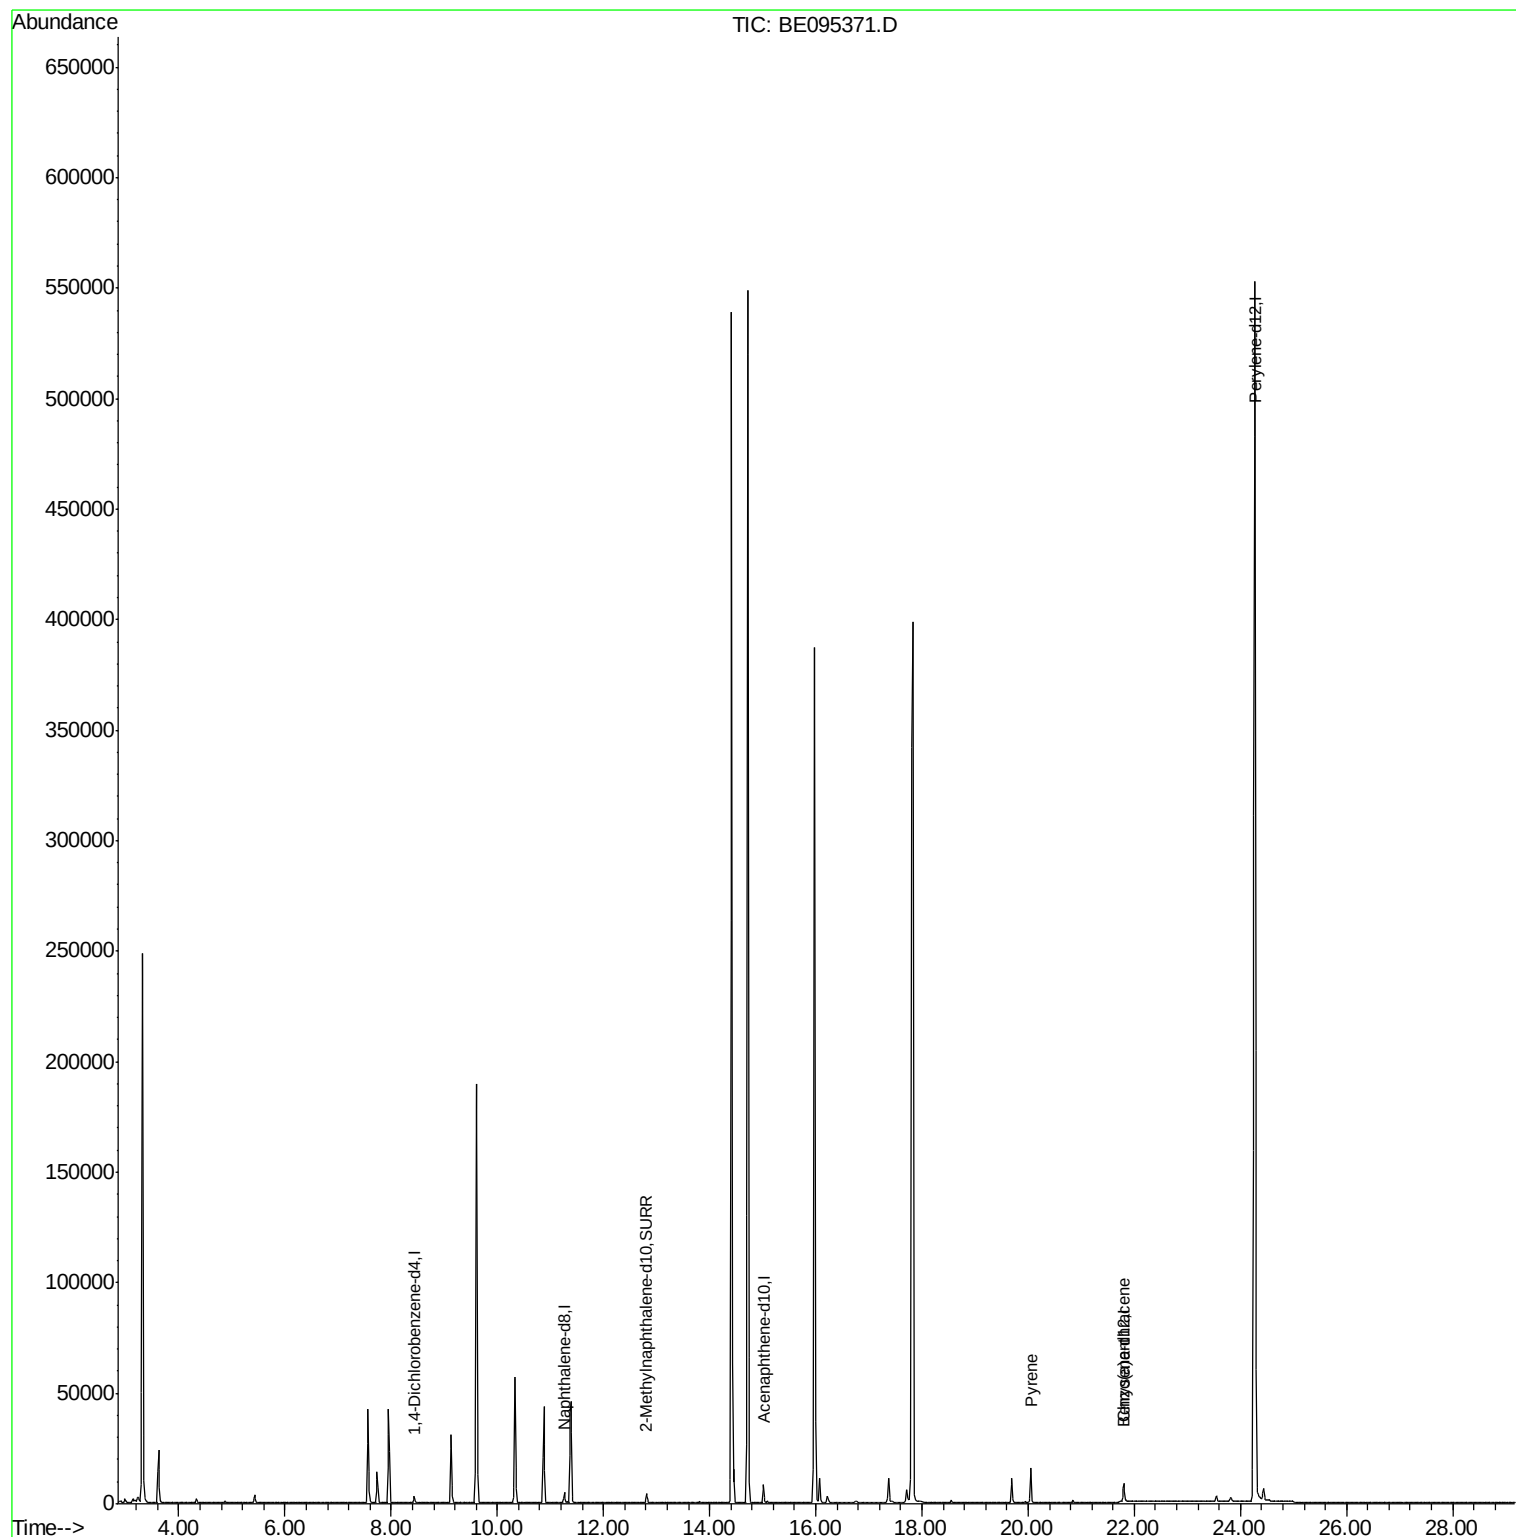

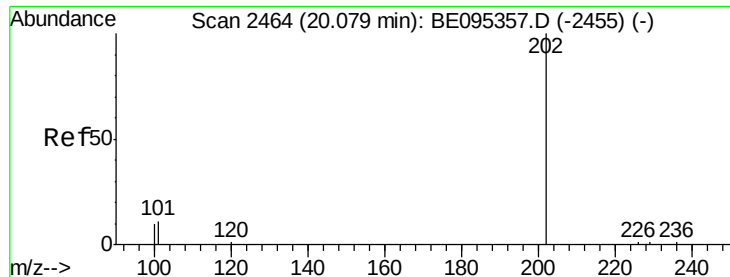

#17

Pvrene

Concen: 0.092 ng/ul

RT: 20.05 min Scan# 2460

Delta R.T. -0.03 min

Lab File: BE095371.D

Acq: 1 Feb 2018 23:30

Instrument :

BNA_E

ClientSampleId :






Tot Ion:202 Resp: 2540

Ion Ratio Lower Upper

202 100

101 172.5 18.2 27.4#

100 1142.0 15.6 23.4#

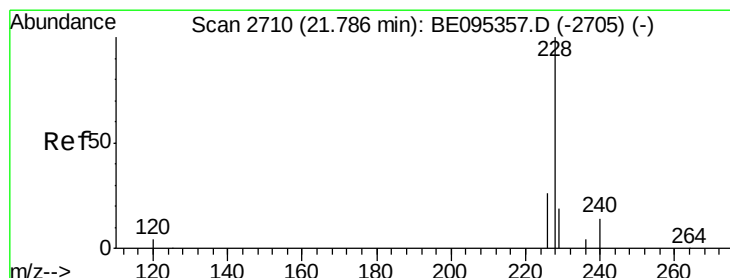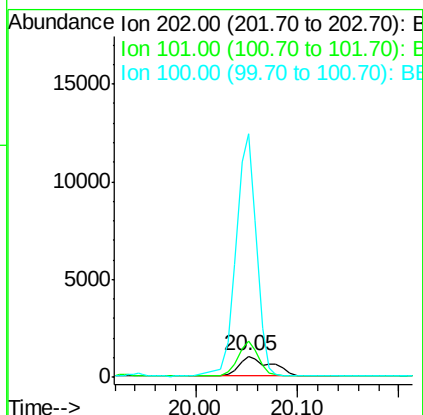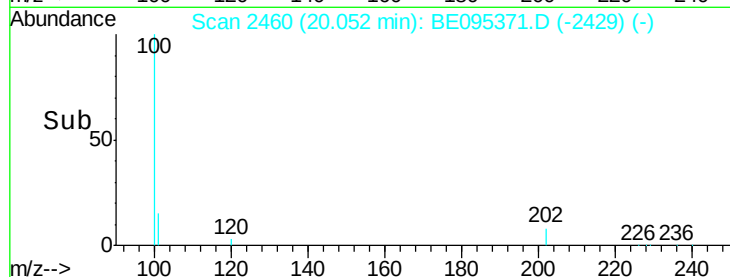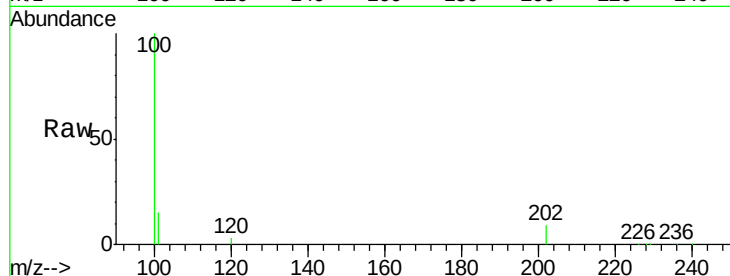

#18

Benzo(a)anthracene

Concen: 0.026 ng/ul

RT: 21.79 min Scan# 2710

Delta R.T. -0.00 min

Lab File: BE095371.D

Acq: 1 Feb 2018 23:30

Tgt Ion:228 Resp: 659

Ion Ratio Lower Upper

228 100

229 34.9 22.8 34.2#

226 36.8 17.0 25.6#

