

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020118\
 Data File : BE095374.D
 Acq On : 2 Feb 2018 1:17
 Operator : SJ/JU
 Sample : J1295-08
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Feb 02 04:57:01 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 02 04:53:51 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.44	152	2136	0.40	ng/ul	0.00
2) Naphthalene-d8	11.26	136	6623	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.02	164	4364	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.71
16) Chrysene-d12	21.80	240	8492	0.40	ng/ul	0.00
20) Perylene-d12	24.27	264	637576	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	4923	0.46	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	12327	0.00	ng/ul	0.00
Target Compounds						
3) Naphthalene	11.31	128	509	0.027	ng/ul#	51
5) 2-Methylnaphthalene	12.89	142	1107	0.089	ng/ul	98
17) Pyrene	20.05	202	1805	0.063	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020118\
Data File : BE095374.D
Acq On : 2 Feb 2018 1:17
Operator : SJ/JU
Sample : J1295-08
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Feb 02 04:57:01 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 02 04:53:51 2018
Response via : Initial Calibration

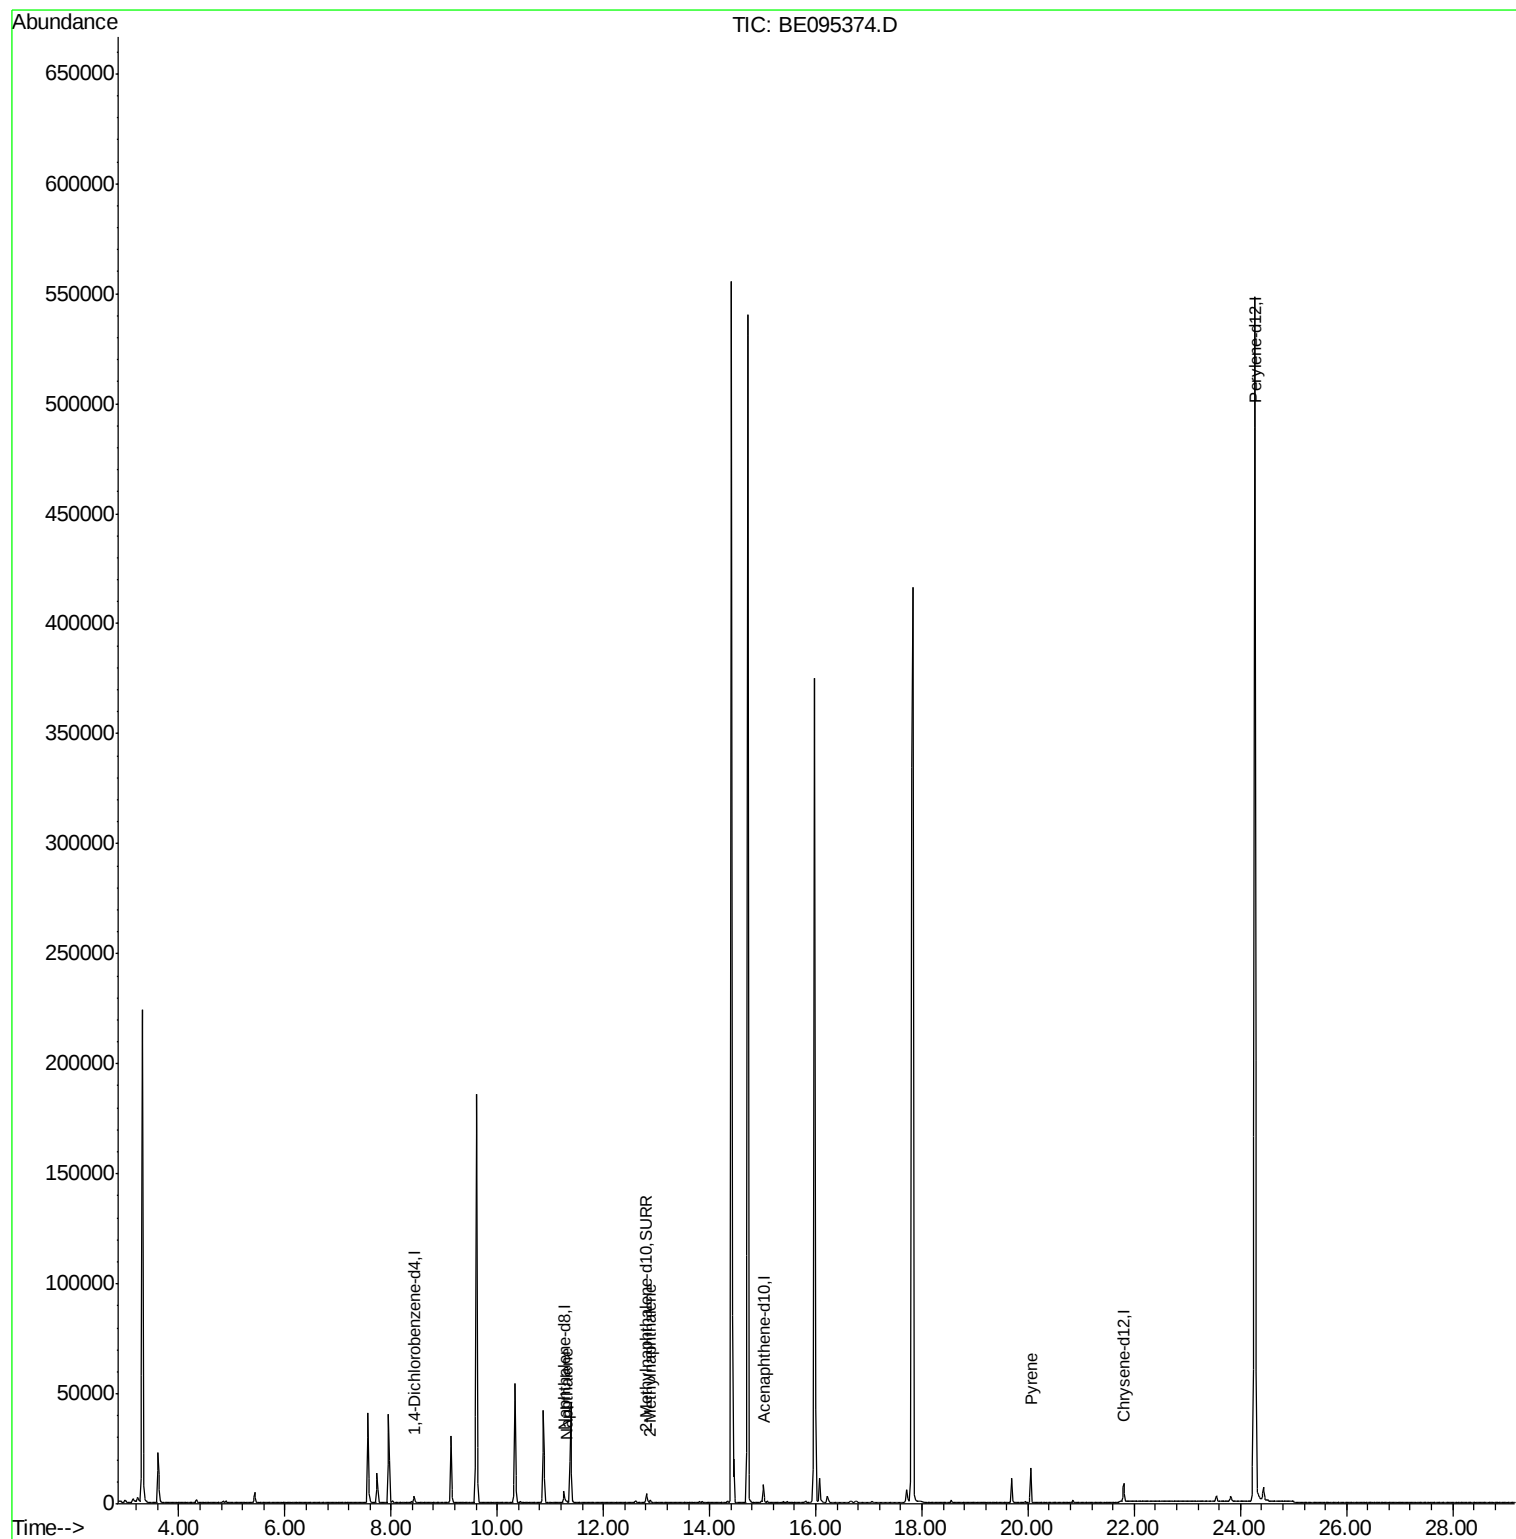

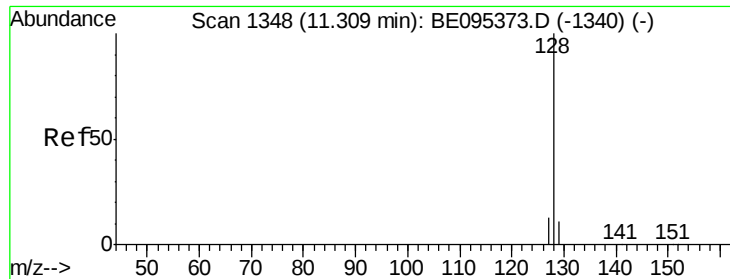

#3

Naphthalene

Concen: 0.027 ng/ul

RT: 11.31 min Scan# 1348

Delta R.T. 0.00 min

Lab File: BE095374.D

Acq: 2 Feb 2018 1:17

Instrument :

BNA_E

ClientSampleId :


Tot Ion:128 Resp: 509

Ion Ratio Lower Upper

128 100

129 31.2 11.3 16.9#




127 28.0 4.0 6.0#

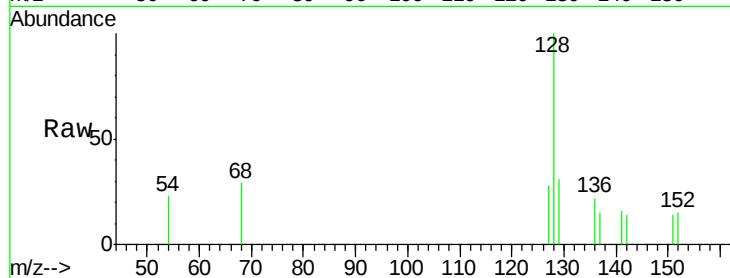

Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

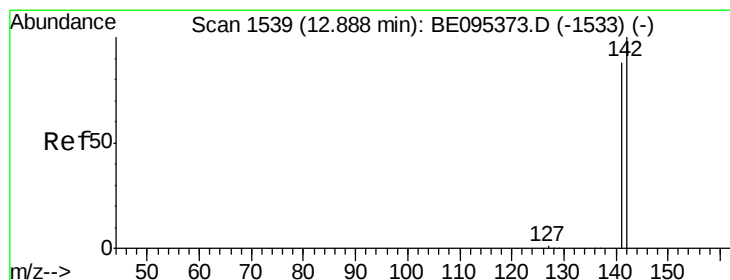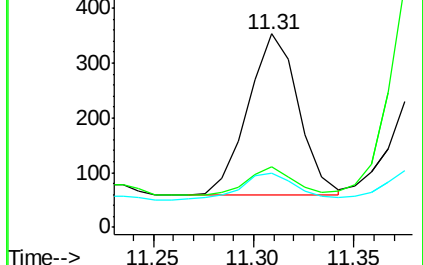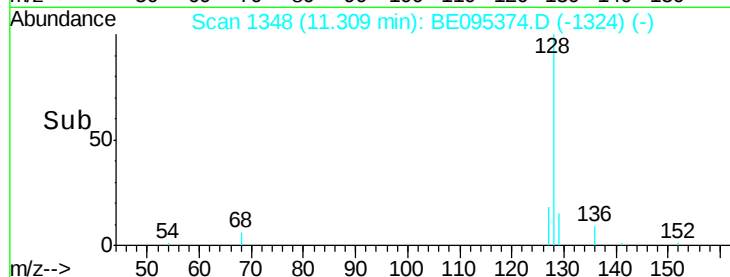

#5

2-Methylnaphthalene

Concen: 0.089 ng/ul

RT: 12.89 min Scan# 1539

Delta R.T. 0.00 min

Lab File: BE095374.D


Acq: 2 Feb 2018 1:17

Tgt Ion:142 Resp: 1107

Ion Ratio Lower Upper



142 100


141 92.5 72.6 108.8

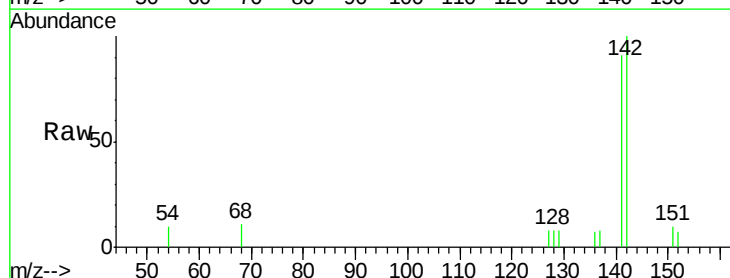

Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

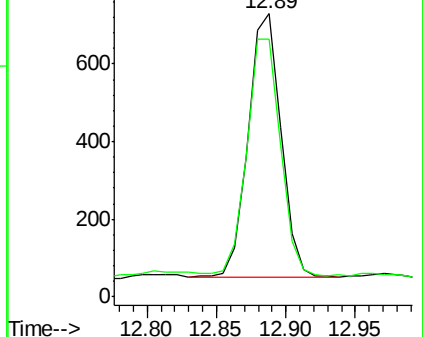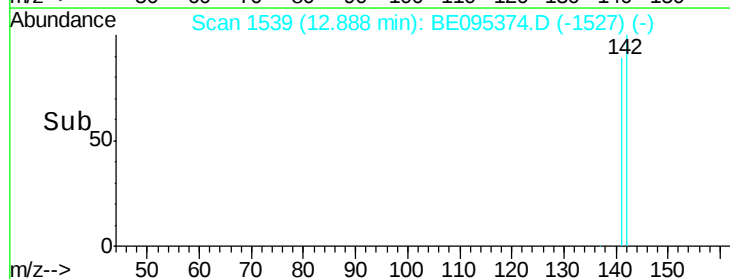

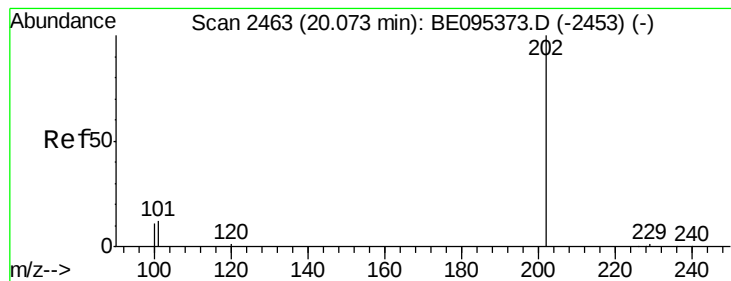

#17

Pvrene

Concen: 0.063 ng/ul

RT: 20.05 min Scan# 2460

Delta R.T. -0.02 min

Lab File: BE095374.D

Acq: 2 Feb 2018 1:17

Instrument :

BNA_E

ClientSampleId :


Tot Ion: 202 Resp: 1805

Ion Ratio Lower Upper

202 100

101 163.3 18.2 27.4#

100 1110.5 15.6 23.4#

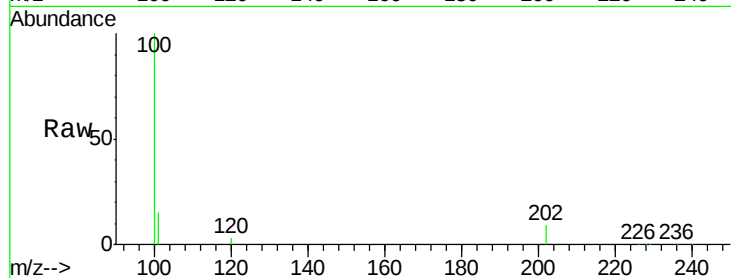

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): E

