


Data Path : Z:\HPCHEM1\BNA E\DATA\BE020118\
Data File : BE095370.D
Acq On : 1 Feb 2018 22:54
Operator : SJ/JU
Sample : J1295-17
Misc :
ALS Vial : 15 Sample Multiplier: 1




Quant Time: Feb 02 04:44:53 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 02 04:07:20 2018
Response via : Initial Calibration

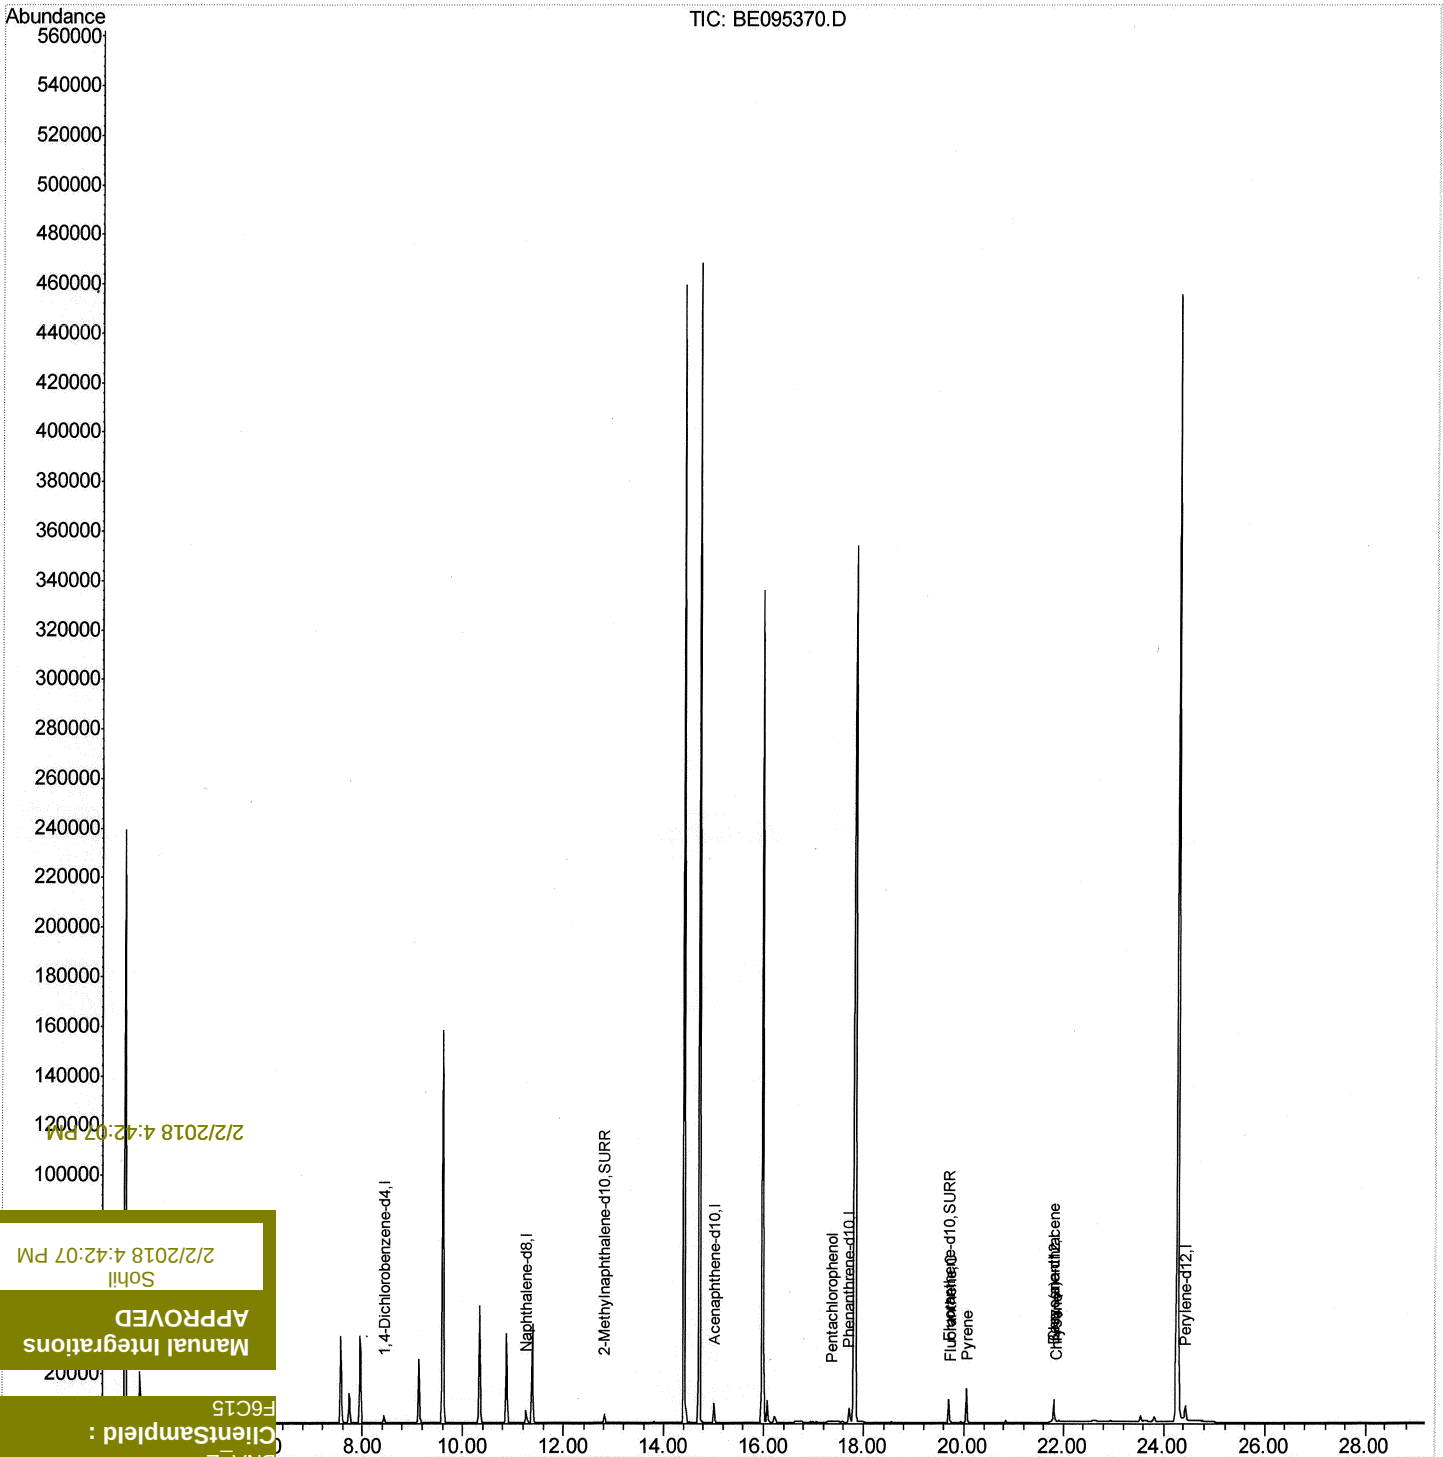

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020118\
 Data File : BE095370.D
 Acq On : 1 Feb 2018 22:54
 Operator : SJ/JU
 Sample : J1295-17
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Quant Time: Feb 02 04:09:25 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 02 04:07:20 2018
 Response via : Initial Calibration

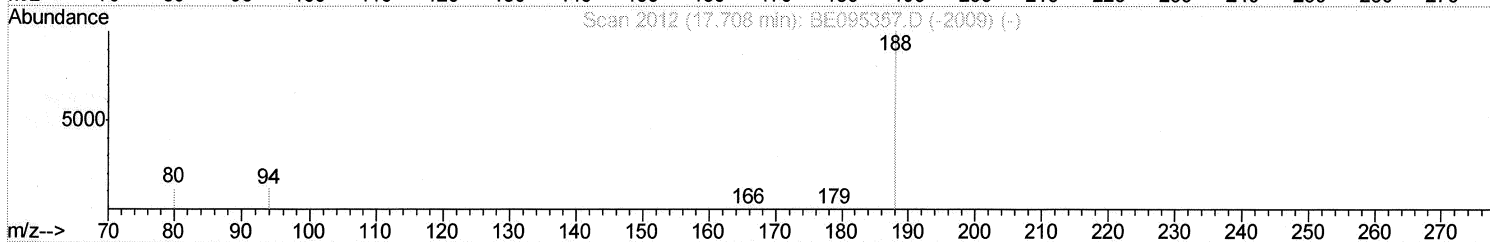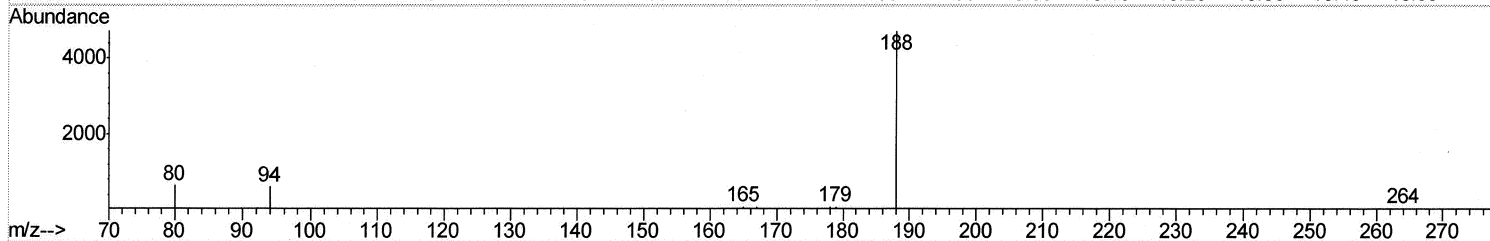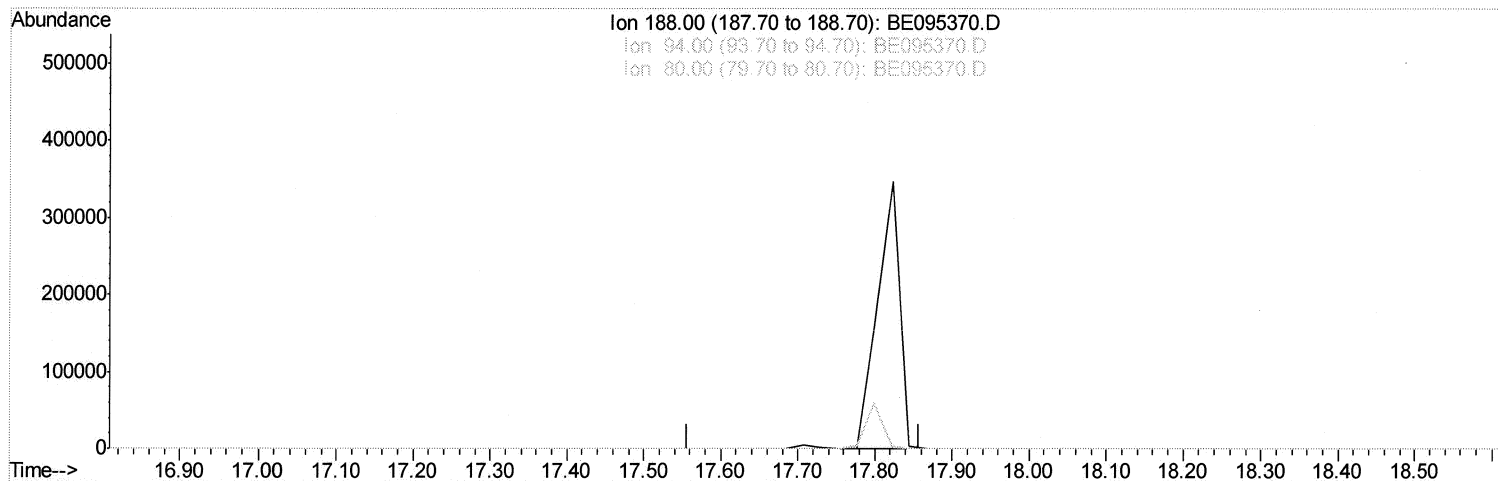

TIC: BE095370.D

(10) Phenanthrene-d10 (I)

17.708min (-17.708) 0.00ng/ul

response 0

Ion Exp% Act%

2/2/2018 4:42:07 PM

Sohil

APPROVED

Manual Integrations

F6C15

ClientSampled :

BNA_E




Instrument :

SOM-EPA-SIM-BE012618.M Fri Feb 02 04:44:23 2018

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020118\
 Data File : BE095370.D
 Acq On : 1 Feb 2018 22:54
 Operator : SJ/JU
 Sample : J1295-17
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Quant Time: Feb 02 04:09:25 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 02 04:07:20 2018
 Response via : Initial Calibration

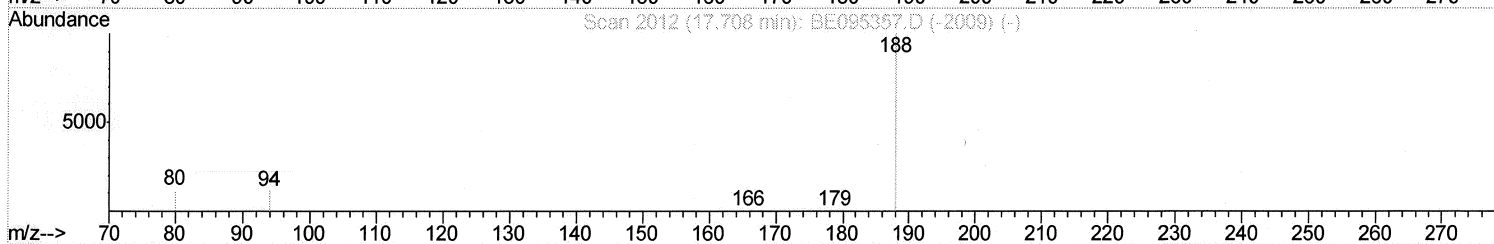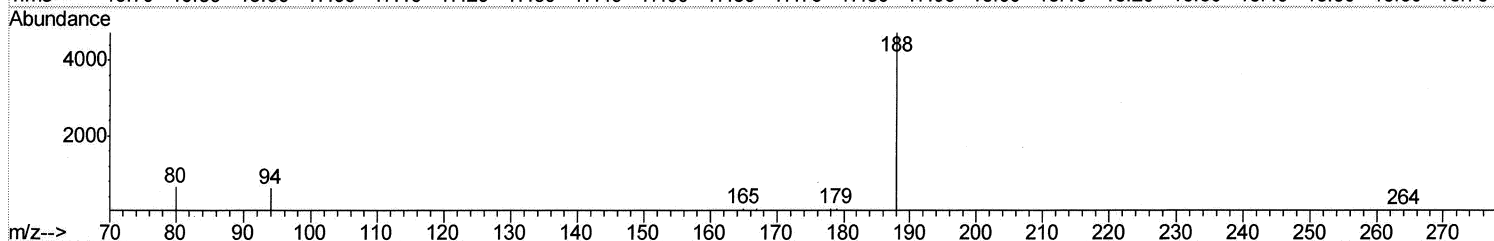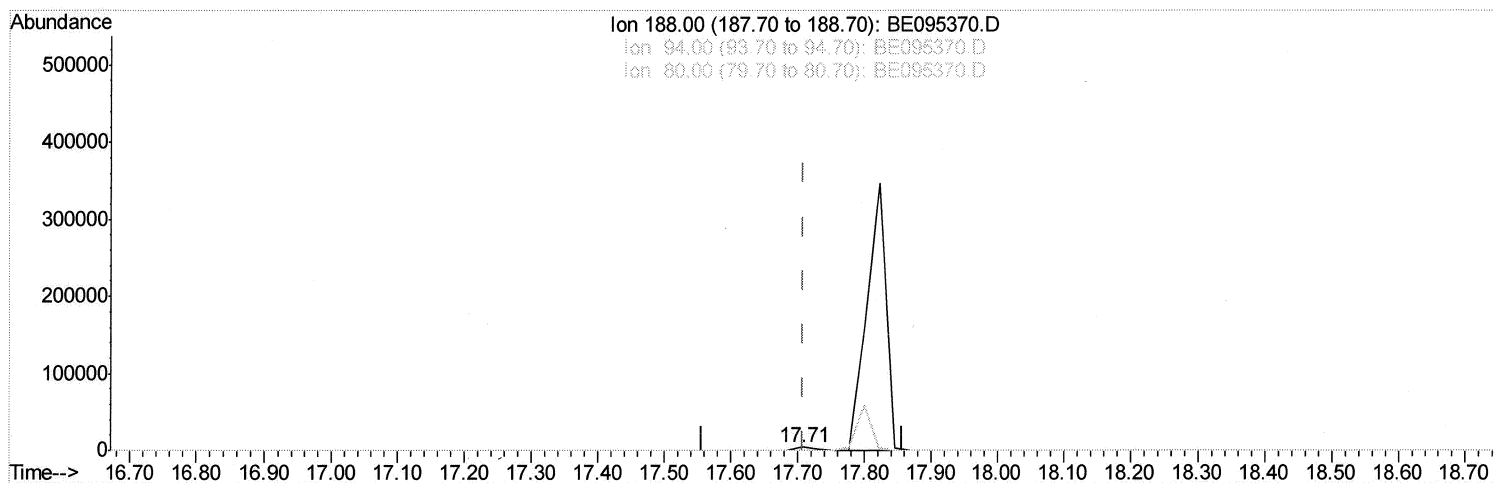

TIC: BE095370.D

(10) Phenanthrene-d10 (I)

17.707min (-0.001) 0.40ng/ul m

2/2/2018 4:42:07 PM

response 8937

Ion Exp% Act%

188.00 100

2/2/2018 4:42:07 PM 3.13

Sohil

APPROVED 3.81

Manual Integrations 00

FC15

Client Sampled :

BNA_E




Instrument :

SOM-EPA-SIM-BE012618.M Fri Feb 02 04:44:37 2018

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020118\
 Data File : BE095370.D
 Acq On : 1 Feb 2018 22:54
 Operator : SJ/JU
 Sample : J1295-17
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Quant Time: Feb 02 04:44:09 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 02 04:07:20 2018
 Response via : Initial Calibration

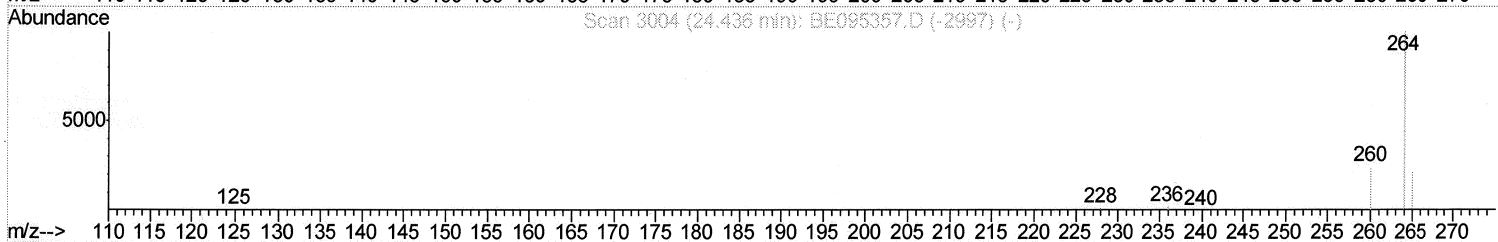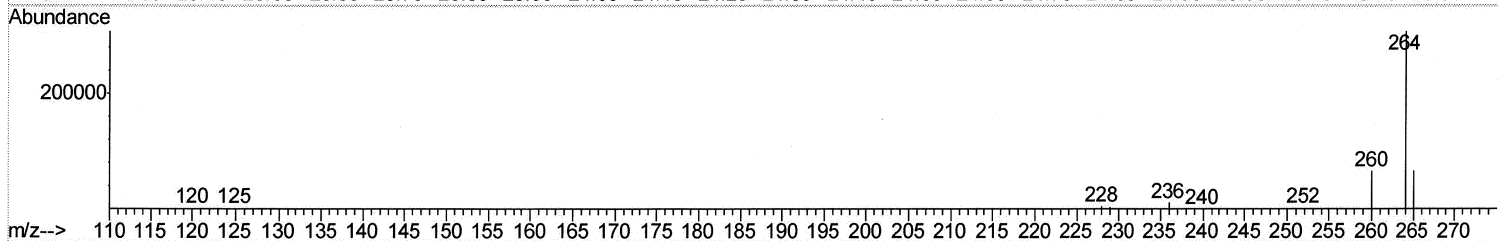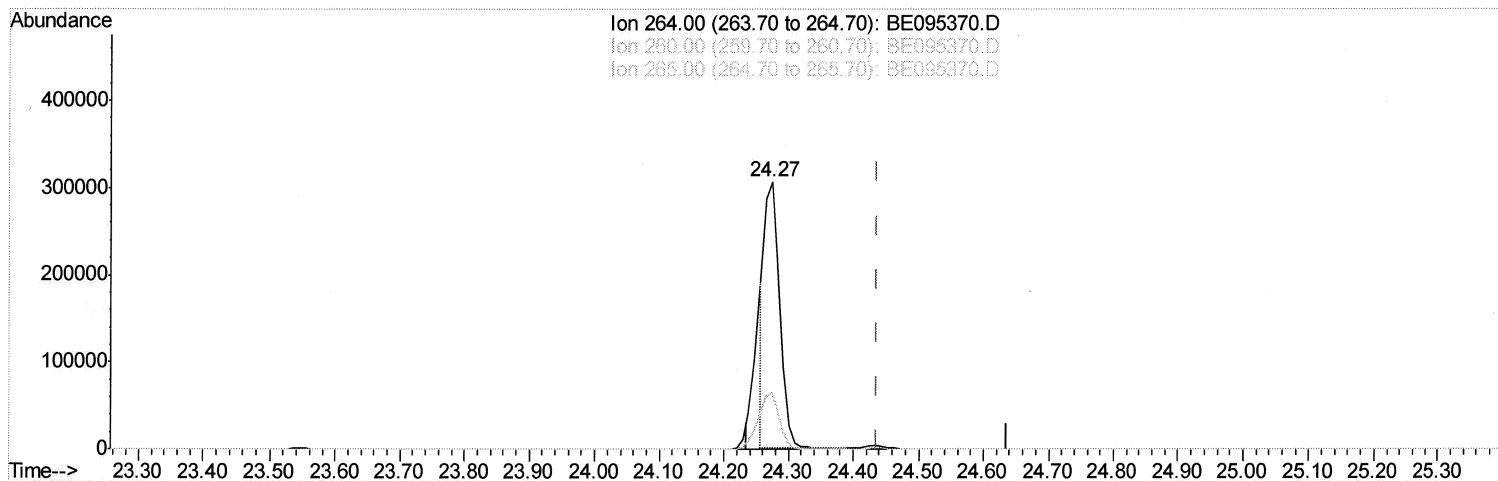

TIC: BE095370.D

(20) Perylene-d12 (I)

24.274min (-0.162) 0.40ng/ul

response 509441

Ion Exp% Act%

2/2/2018 4:42:07 PM 1.04#

APPROVED 21.55#

Manual Integrations

ClientSampled : F6C15

BNA_E




Instrument :

SOM-EPA-SIM-BE012618.M Fri Feb 02 04:45:06 2018

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020118\
 Data File : BE095370.D
 Acq On : 1 Feb 2018 22:54
 Operator : SJ/JU
 Sample : J1295-17
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Quant Time: Feb 02 04:44:09 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 02 04:07:20 2018
 Response via : Initial Calibration

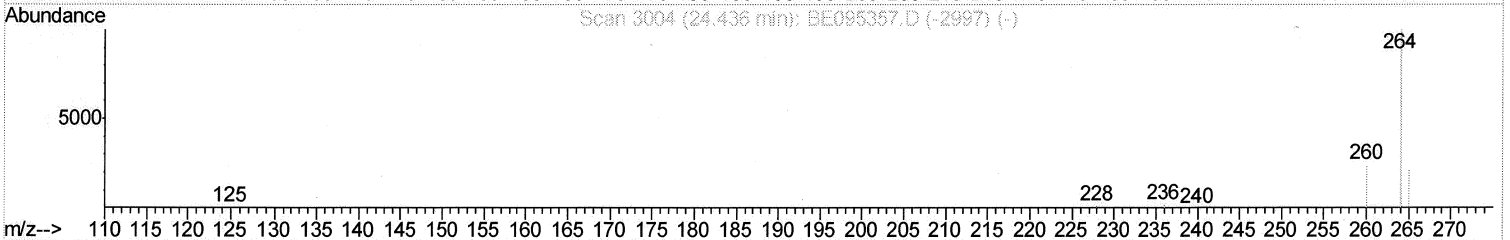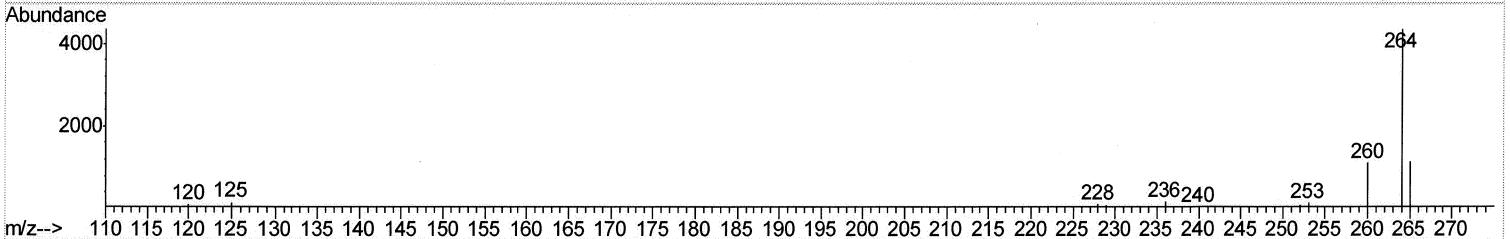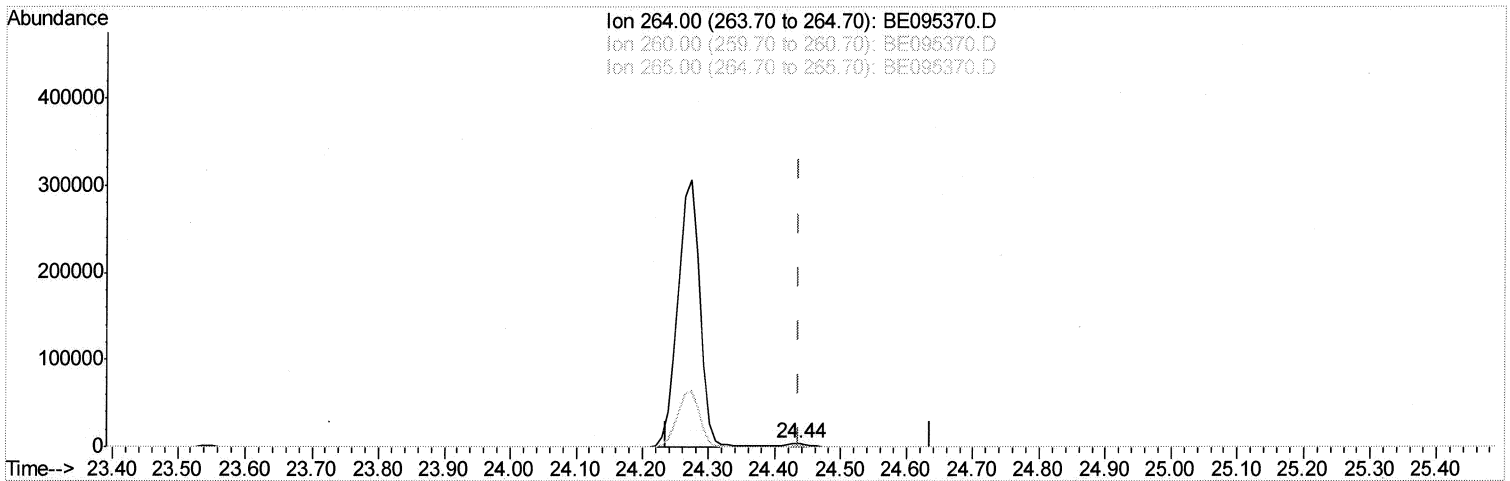

TIC: BE095370.D

(20) Perylene-d12 (I)

24.436min (+0.000) 0.40ng/ul m

2/2/18

response 8248

Ion Exp% Act%

264.00 100 100

2/2/2018 4:42:07 PM 25.36

Sohil

APPROVED 26.35#

Manual Integrations 00

F6C15

Client Sampled :

BNA_E

Instrument :

SOM-EPA-SIM-BE012618.M Fri Feb 02 04:45:21 2018

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020118\
 Data File : BE095370.D
 Acq On : 1 Feb 2018 22:54
 Operator : SJ/JU
 Sample : J1295-17
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Quant Time: Feb 02 04:44:53 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 02 04:07:20 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.44	152	2100	0.40	ng/ul	0.00
2) Naphthalene-d8	11.26	136	6489	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.02	164	4338	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	8937m>	0.40	ng/ul	> 0.00
16) Chrysene-d12	21.80	240	8780	0.40	ng/ul	0.00
20) Perylene-d12	24.44	264	8248m>	0.40	ng/ul	> 0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	4230	0.40	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	10202	0.30	ng/ul	0.00
Target Compounds						Ovalue
11) Pentachlorophenol	17.36	266	173	0.100	ng/ul	87
15) Fluoranthene	19.72	202	1088	0.028	ng/ul	86
17) Pyrene	20.08	202	1002	0.034	ng/ul	95
18) Benzo(a)anthracene	21.79	228	643	0.023	ng/ul#	84
19) Chrysene	21.84	228	677	0.024	ng/ul#	80

(#) = qualifier out of range (m) = manual integration (+) = signals summed

2/2/2018 4:42:07 PM

2/2/2018 4:42:07 PM

Sohil

Manual Integrations
APPROVED

Instrument :
BNA_E
Client Sampled :
F6C15

2/2/2018 4:46:39 PM Fri Feb 02 04:46:39 2018