


Data Path : Z:\HPCHEM1\BNA E\DATA\BE020118\
Data File : BE095383.D
Acq On : 2 Feb 2018 6:39
Operator : SJ/JU
Sample : J1295-15
Misc :
ALS Vial : 27 Sample Multiplier: 1




Quant Time: Feb 02 07:51:59 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 02 04:53:51 2018
Response via : Initial Calibration

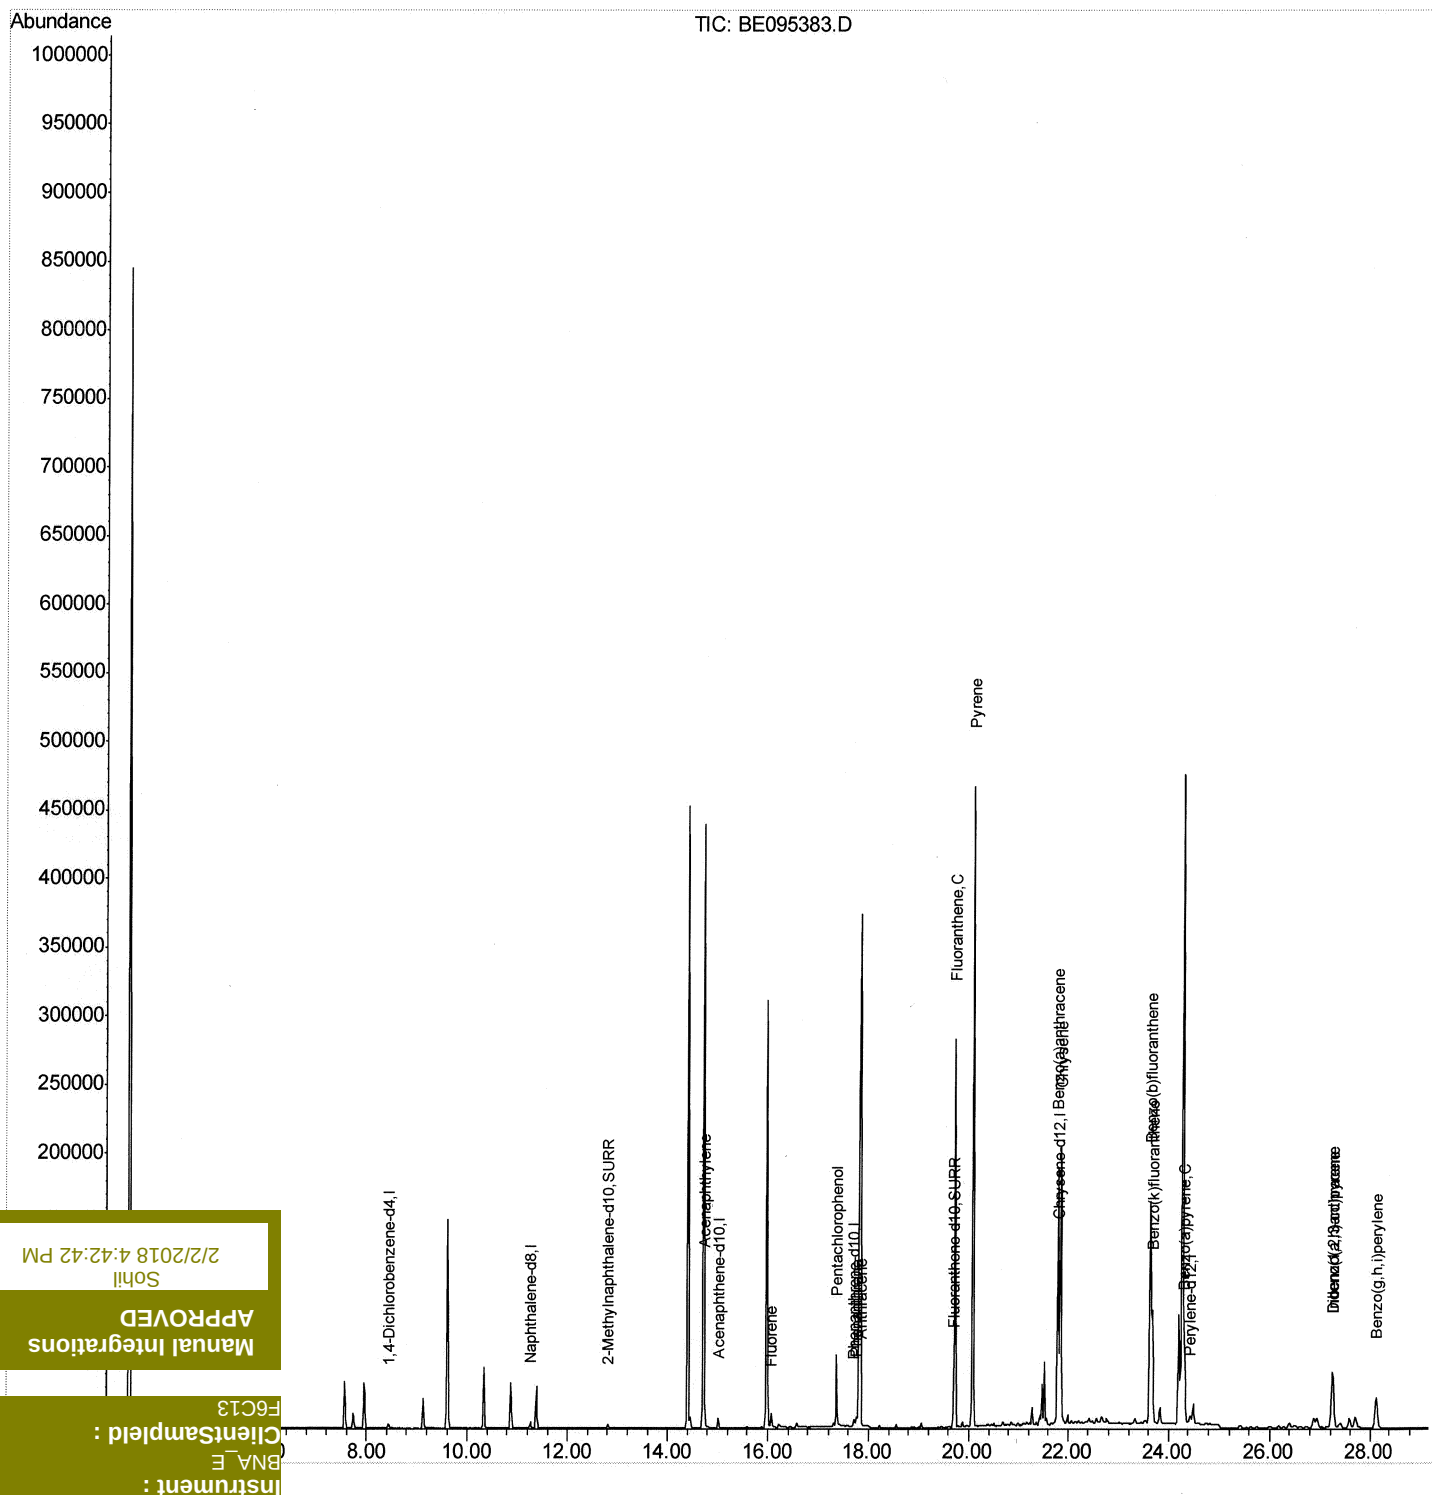

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020118\
 Data File : BE095383.D
 Acq On : 2 Feb 2018 6:39
 Operator : SJ/JU
 Sample : J1295-15
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Quant Time: Feb 02 07:15:30 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 02 04:53:51 2018
 Response via : Initial Calibration

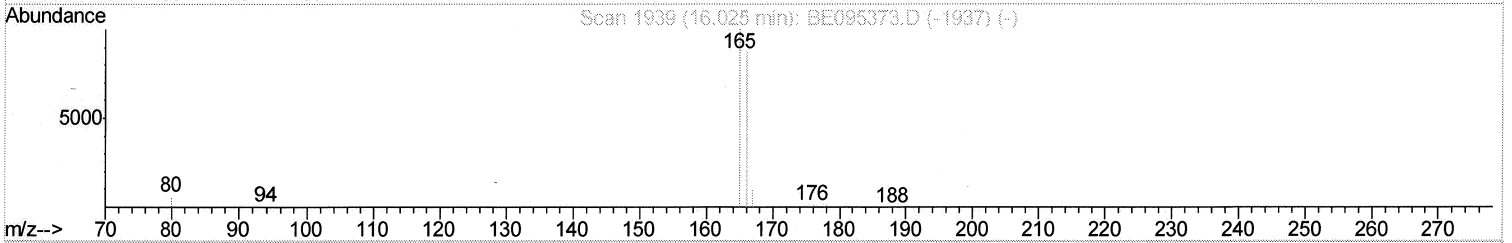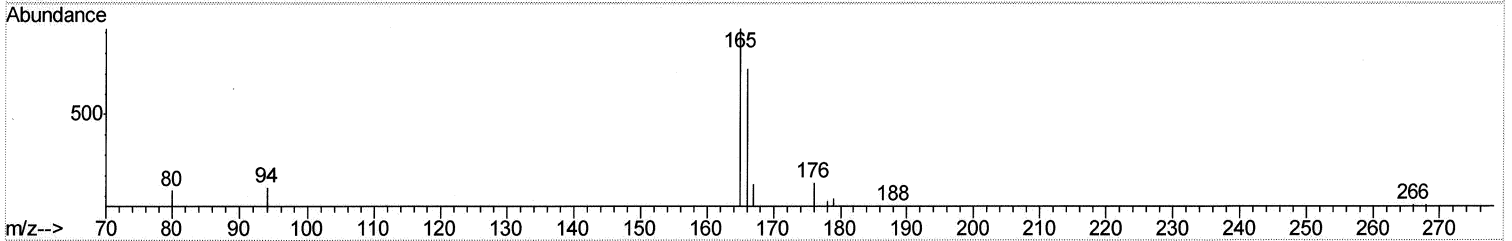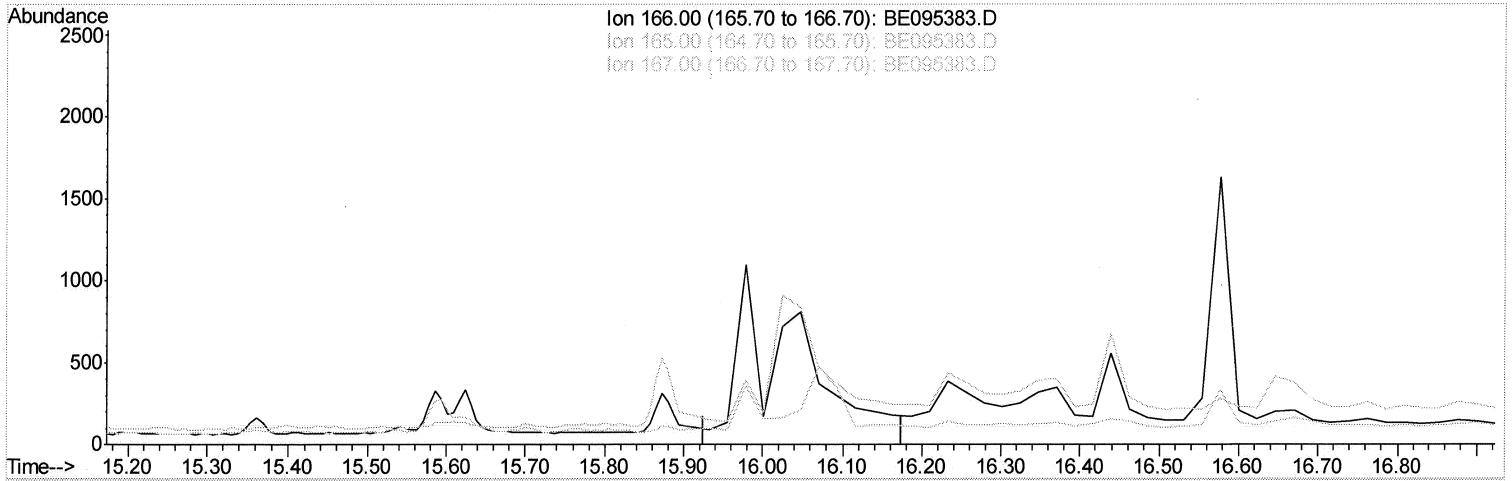

TIC: BE095383.D

(9) Fluorene

16.025min (-16.025) 0.00ng/ul

response 0

Ion	Exp%	Act%
165	100.00	0.00
166	0.00	0.00
167	0.00	0.00

2/2/2018 4:42:42 PM

Sohil

APPROVED




Manual Integrations

Instrument : BNA_E
 ClientSampled : F6C13

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020118\
 Data File : BE095383.D
 Acq On : 2 Feb 2018 6:39
 Operator : SJ/JU
 Sample : J1295-15
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Quant Time: Feb 02 07:15:30 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 02 04:53:51 2018
 Response via : Initial Calibration

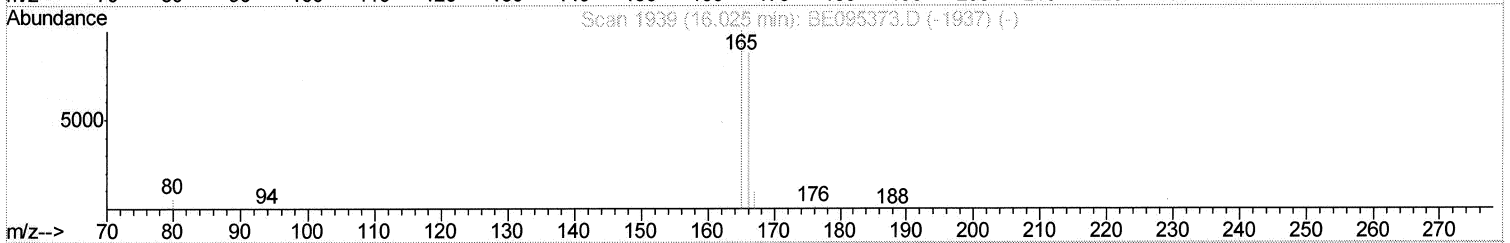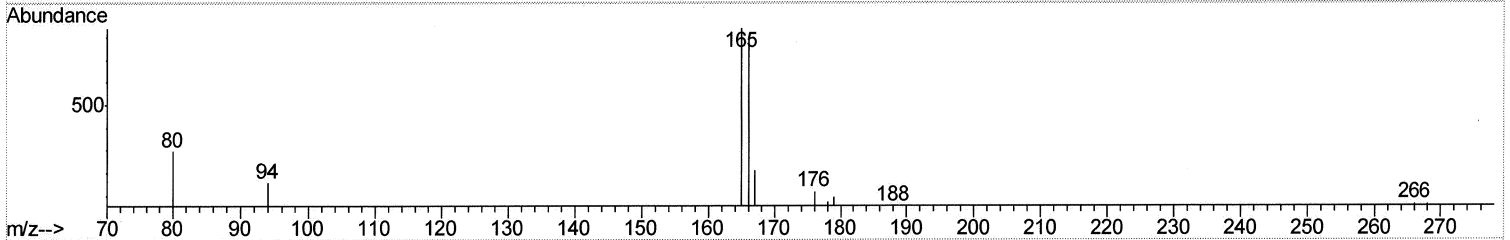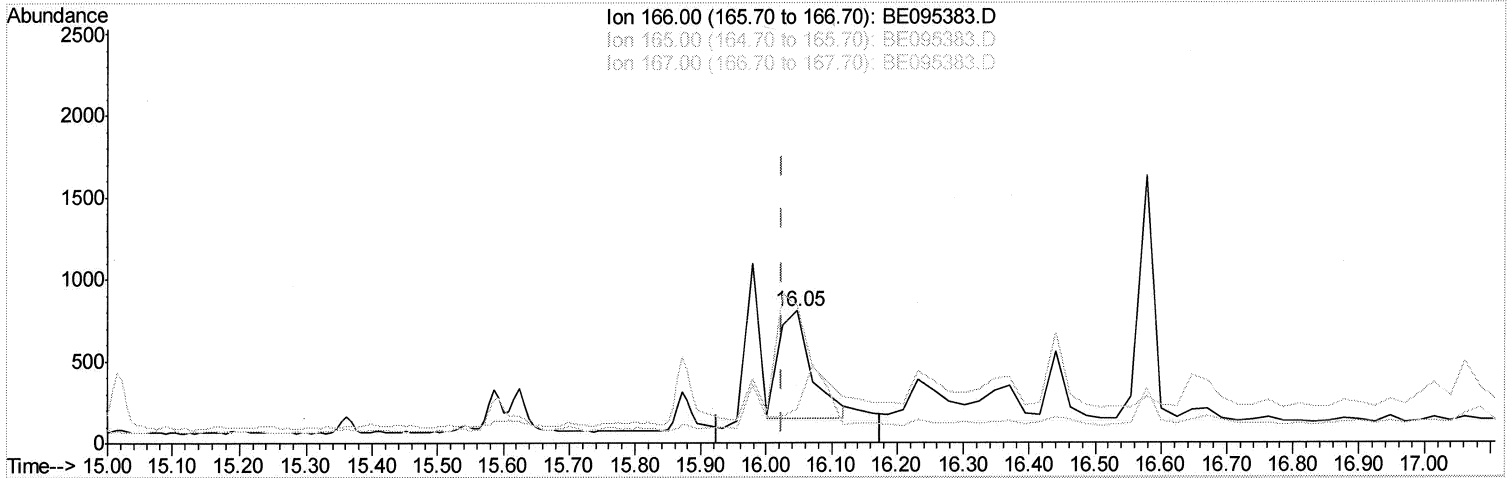

TIC: BE095383.D

(9) Fluorene

16.048min (+0.023) 0.15ng/ul m

response 2318

Ion Exp% Act%




00
 2/2/2018 4:42:42 PM
 Sohll
 APPROVED
 Manual Integrations
 26.11#
 00

F6C13
 ClientSampled :
 BNA_E
 Instrument :

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020118\
 Data File : BE095383.D
 Acq On : 2 Feb 2018 6:39
 Operator : SJ/JU
 Sample : J1295-15
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Quant Time: Feb 02 07:15:30 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 02 04:53:51 2018
 Response via : Initial Calibration

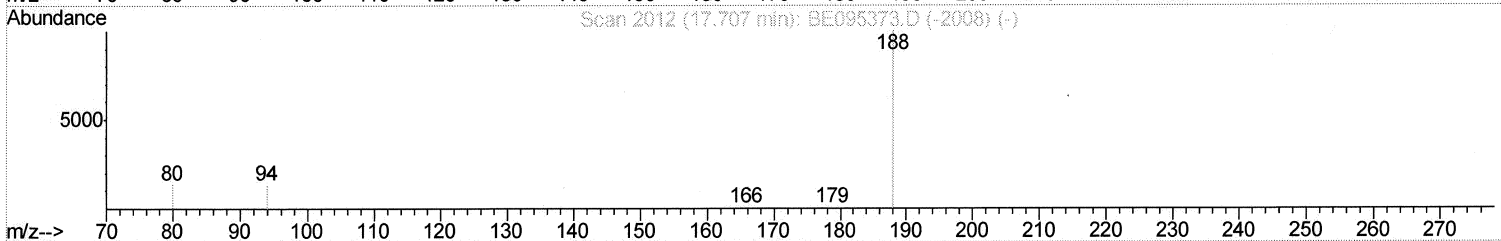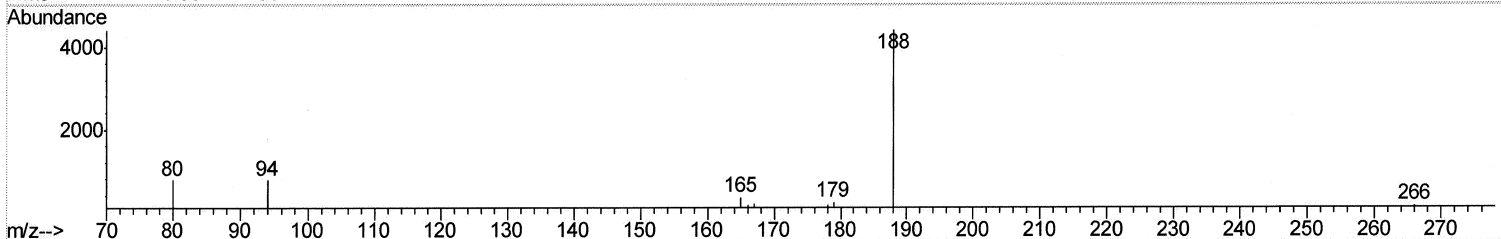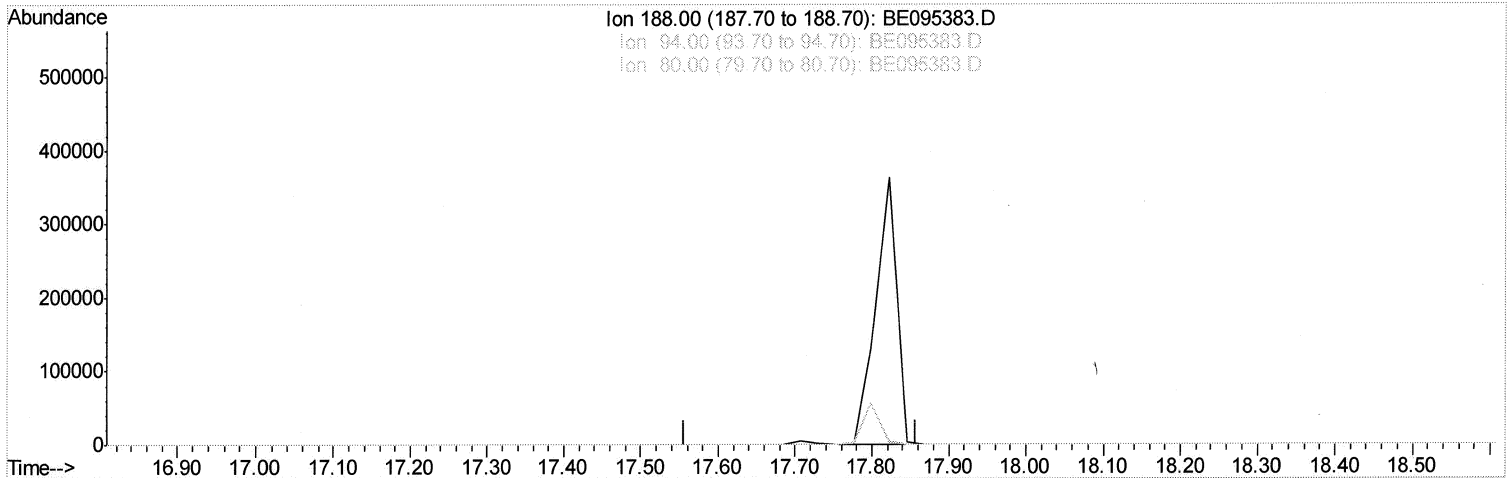

TIC: BE095383.D

(10) Phenanthrene-d10 (I)

17.707min (-17.707) 0.00ng/ul

response 0

Ion	Exp%	Act%
188	100	100
94	100	100
80	100	100




2/2/2018 4:42:42 PM
 Sohll
 APPROVED
 Manual Integrations

Instrument : BNA_E
 ClientSampled : F6C13

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020118\
 Data File : BE095383.D
 Acq On : 2 Feb 2018 6:39
 Operator : SJ/JU
 Sample : J1295-15
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Quant Time: Feb 02 07:15:30 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 02 04:53:51 2018
 Response via : Initial Calibration

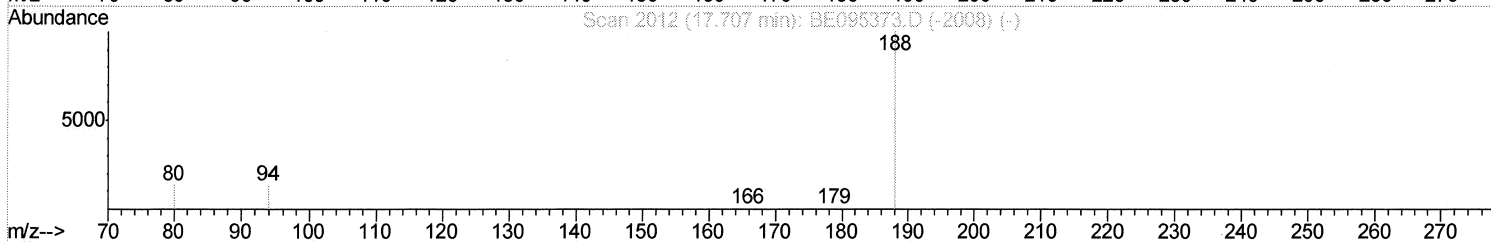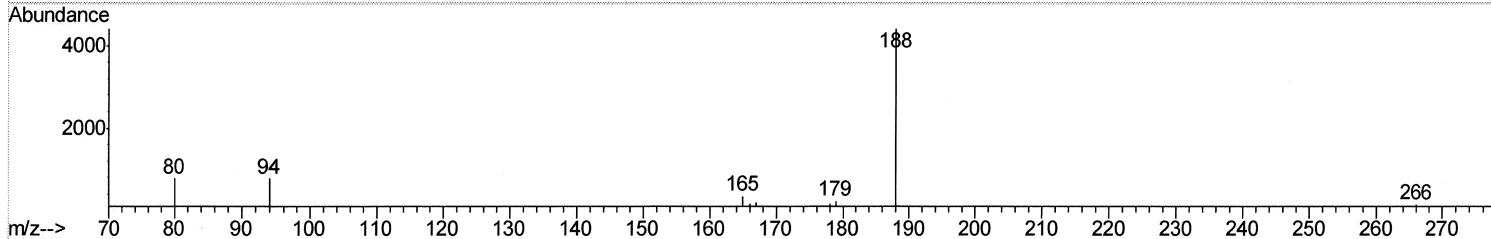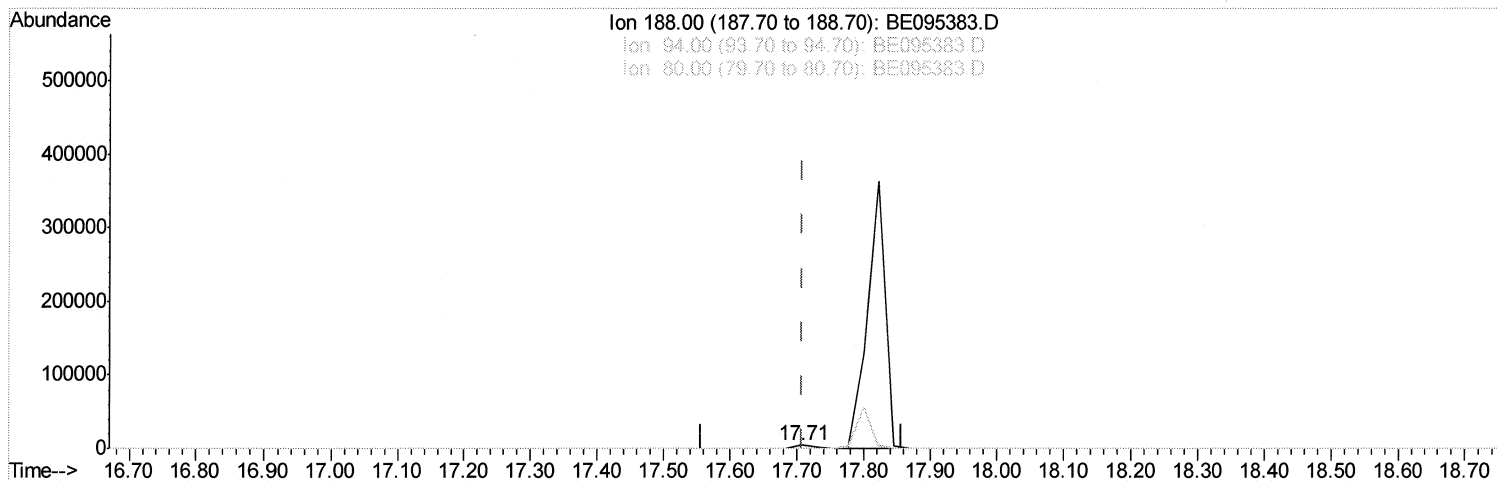

TIC: BE095383.D

(10) Phenanthrene-d10 (I)

17.707min (-0.000) 0.40ng/ul m

response 8811

Ion	Exp%	Act%
188.00	100	100
94.00	7.59	7.52
80.00	0.00	0.00

2/2/2018 4:42:42 PM

Sohil

APPROVED

Manual Integrations

Client Sampled :




Instrument :

BE012618.M Fri Feb 02 07:48:43 2018

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020118\
 Data File : BE095383.D
 Acq On : 2 Feb 2018 6:39
 Operator : SJ/JU
 Sample : J1295-15
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Quant Time: Feb 02 07:48:17 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 02 04:53:51 2018
 Response via : Initial Calibration

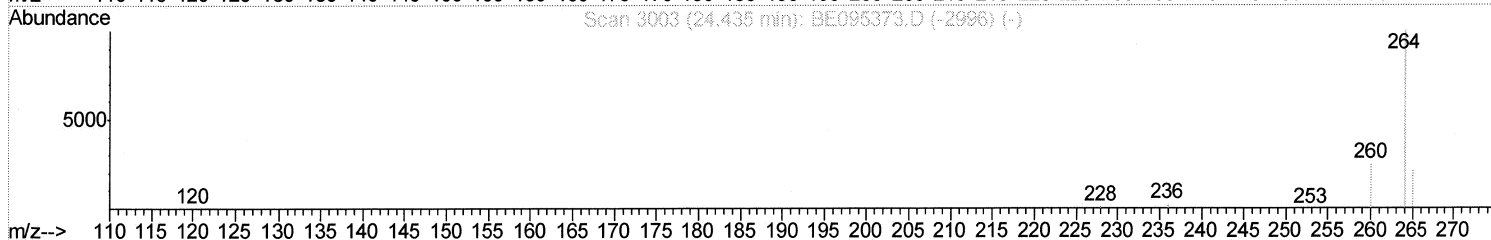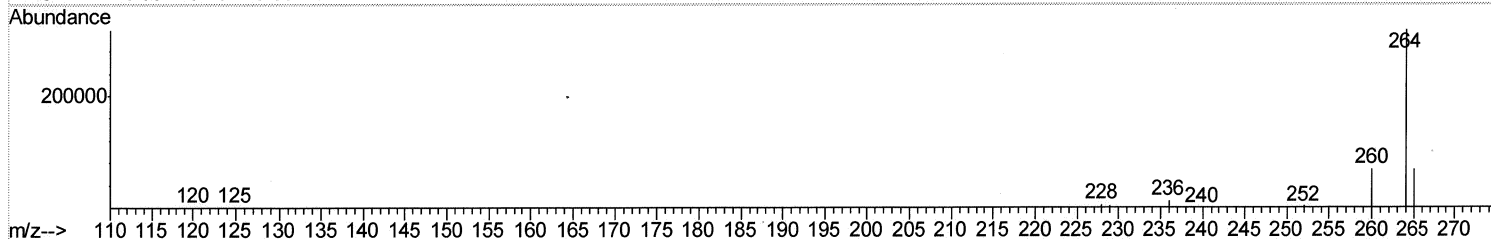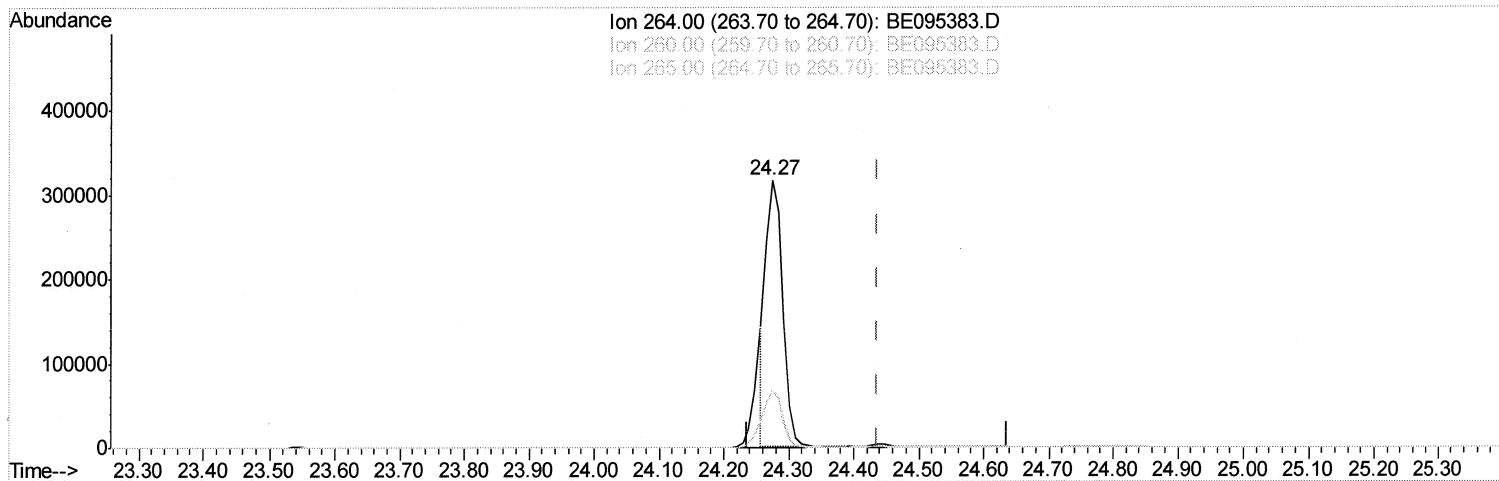

TIC: BE095383.D

(20) Perylene-d12 (I)

24.274min (-0.161) 0.40ng/ul




response 571510

Ion	Exp%	Act%
264.00	21.35	21.43

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020118\
 Data File : BE095383.D
 Acq On : 2 Feb 2018 6:39
 Operator : SJ/JU
 Sample : J1295-15
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Quant Time: Feb 02 07:48:17 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 02 04:53:51 2018
 Response via : Initial Calibration

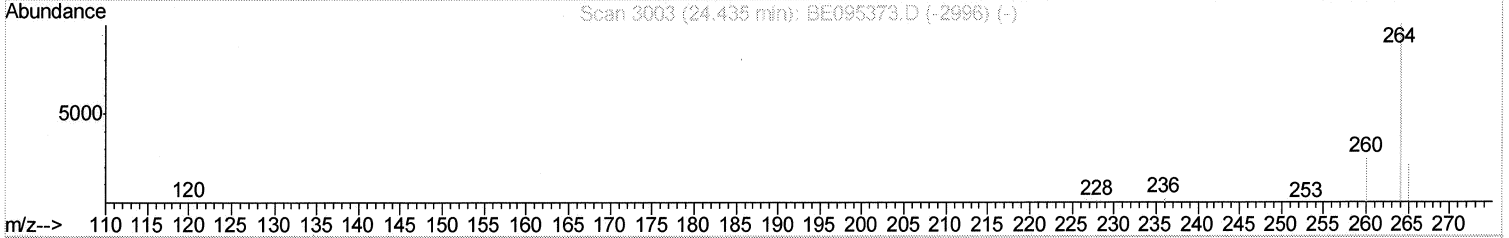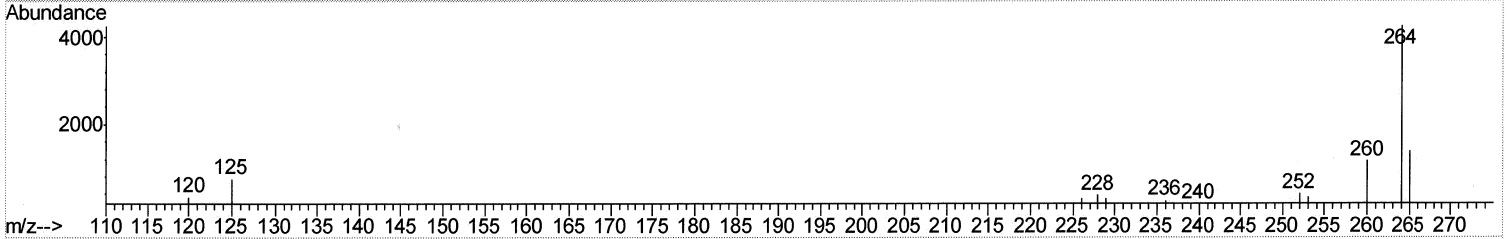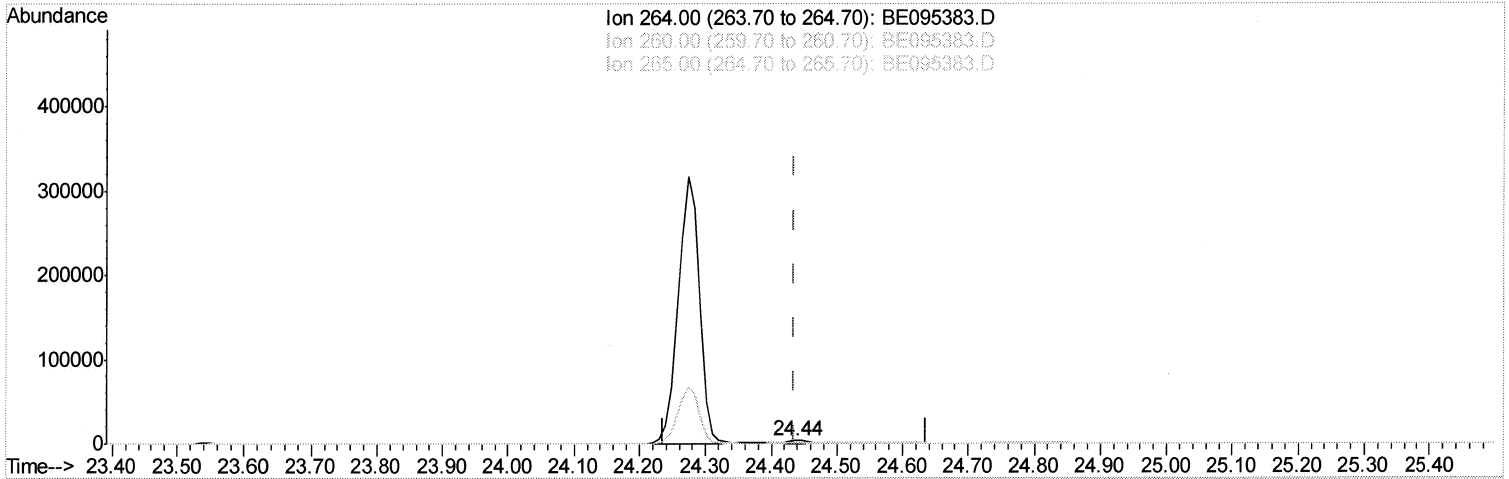

TIC: BE095383.D

(20) Perylene-d12 (I)

24.436min (+0.001) 0.40ng/ul

response 8188

Ion	Exp%	Act%
264.00	100	100
260.00	32.64	32.64
272.00	27.32	27.32

2/2/2018 4:42:42 PM

Sohil

APPROVED




Manual Integrations

Instrument : BNA_E
 Client/SampleId : F6C13

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020118\
 Data File : BE095383.D
 Acq On : 2 Feb 2018 6:39
 Operator : SJ/JU
 Sample : J1295-15
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Quant Time: Feb 02 07:49:09 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 02 04:53:51 2018
 Response via : Initial Calibration

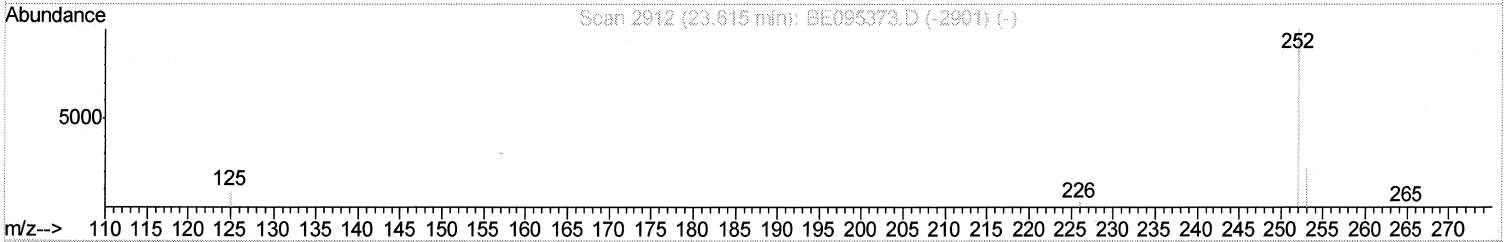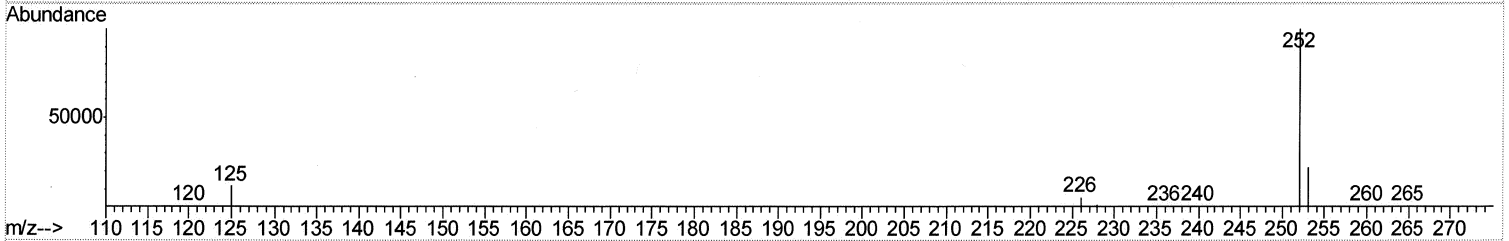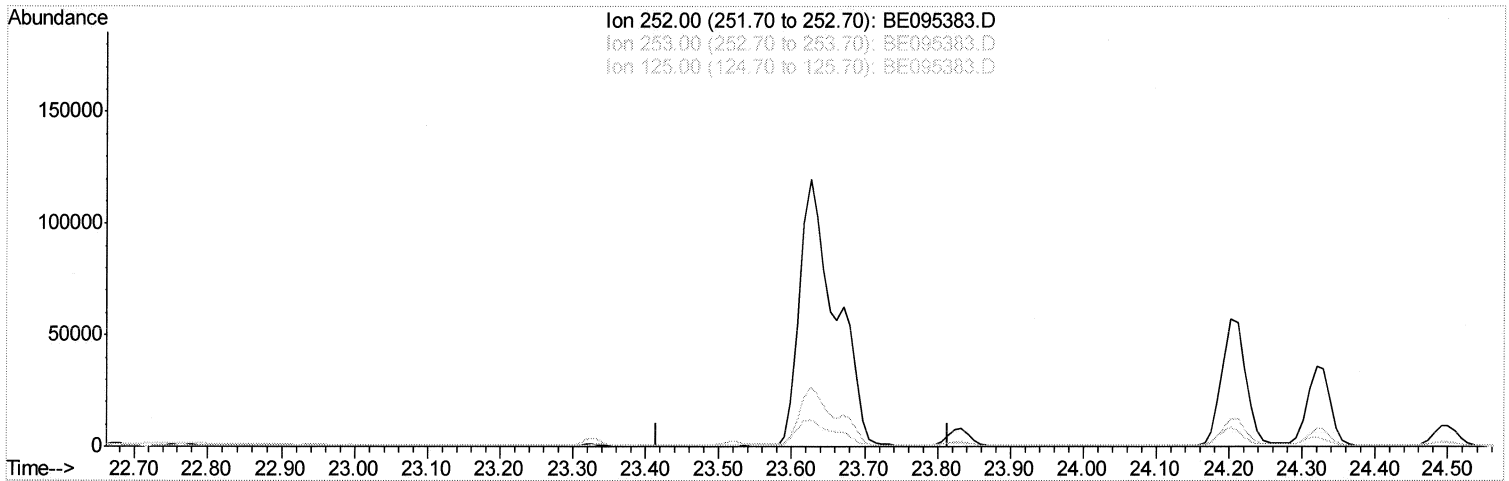

TIC: BE095383.D

(21) Benzo(b)fluoranthene

23.615min (-23.615) 0.00ng/ul

response 0

Ion	Exp%	Act%
252.00	100	0.00
253.00	100	0.00
125.00	100	0.00

2/2/2018 4:42:42 PM

Sohil

APPROVED

Manual Integrations

Client Sample ID : F6C13




Instrument : BNA_E

SOM-EPA-SIM-BE012618.M Fri Feb 02 07:49:55 2018

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020118\
 Data File : BE095383.D
 Acq On : 2 Feb 2018 6:39
 Operator : SJ/JU
 Sample : J1295-15
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Quant Time: Feb 02 07:49:09 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 02 04:53:51 2018
 Response via : Initial Calibration

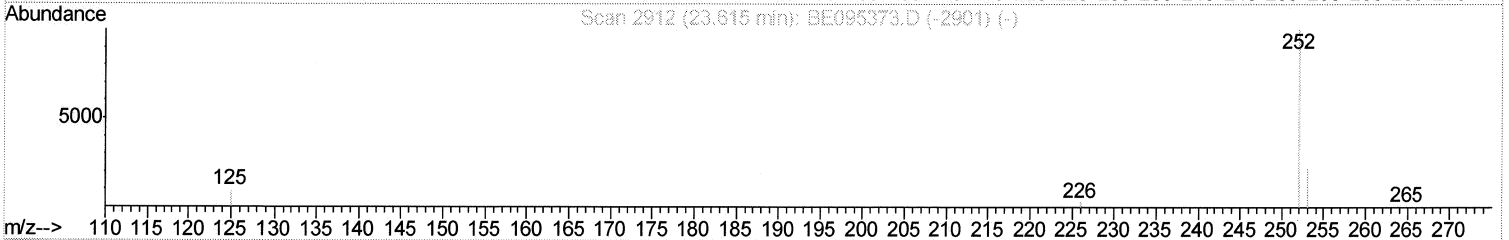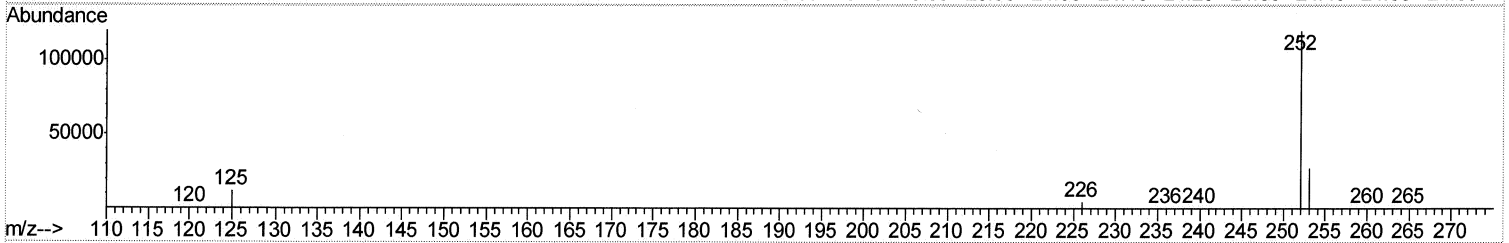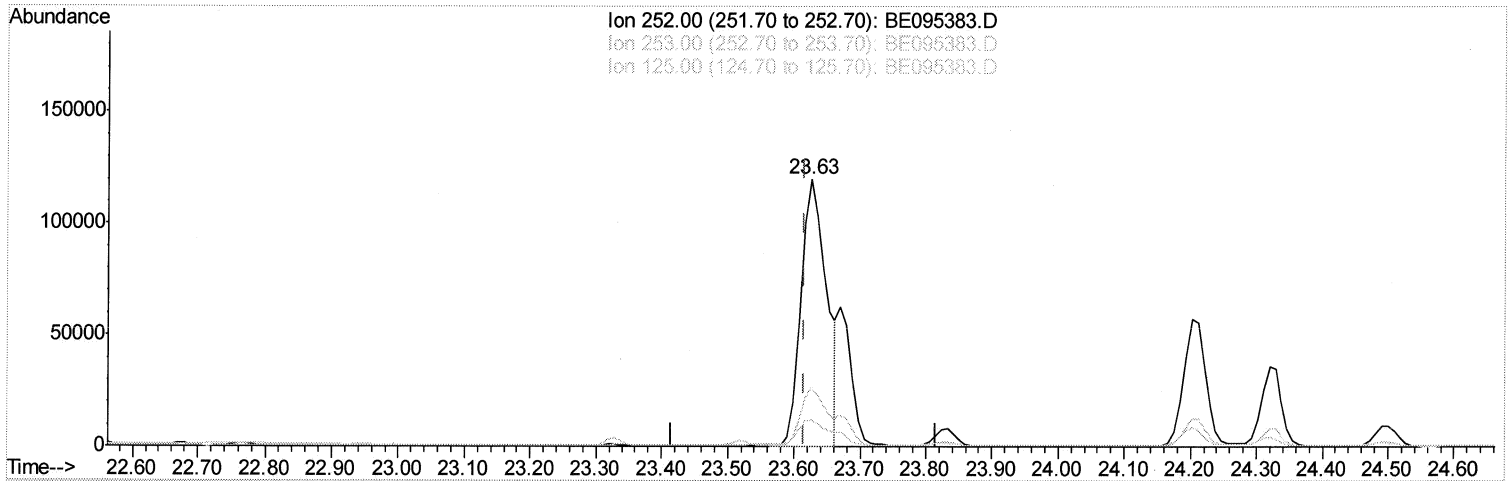

(21) Benzo(b)fluoranthene

23.625min (+0.010) 11.23ng/ul m

response 324316

Ion Exp% Act%

2/2/2018 4:42:42 PM

Sohil

APPROVED

Manual Integrations

Client Sampled : F6C13

BNA_E




Instrument :

SOM-EPA-SIM-BE012618.M Fri Feb 02 07:51:00 2018

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020118\
 Data File : BE095383.D
 Acq On : 2 Feb 2018 6:39
 Operator : SJ/JU
 Sample : J1295-15
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Quant Time: Feb 02 07:49:09 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 02 04:53:51 2018
 Response via : Initial Calibration

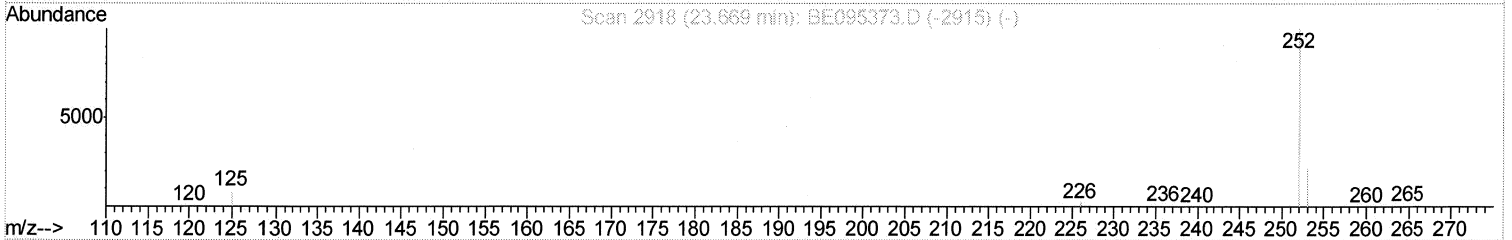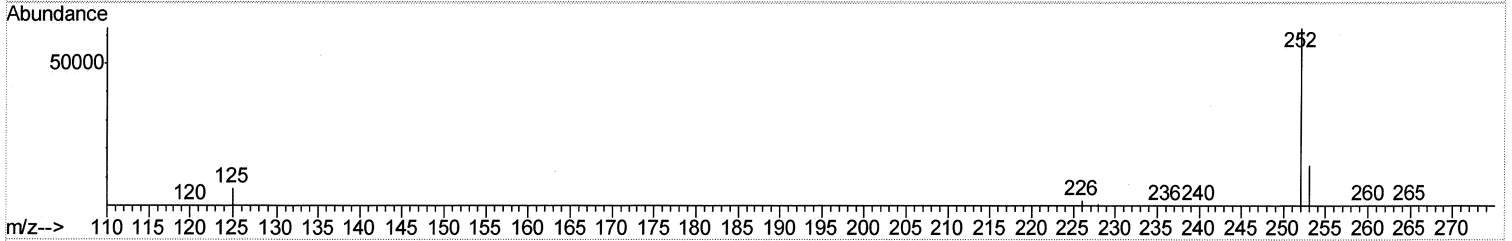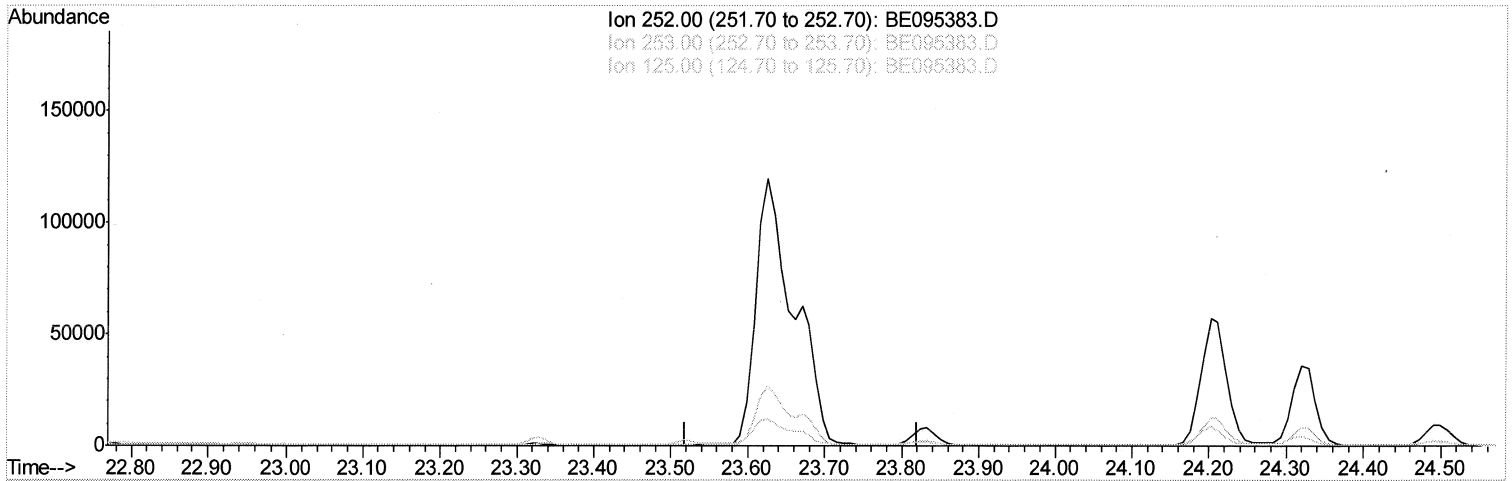

TIC: BE095383.D

(22) Benzo(k)fluoranthene

23.669min (-23.669) 0.00ng/ul

response 0

Ion	Exp%	Act%
252.00	100	0.00
253.00	100	0.00
254.00	100	0.00
255.00	100	0.00
256.00	100	0.00
257.00	100	0.00
258.00	100	0.00
259.00	100	0.00
260.00	100	0.00
261.00	100	0.00
262.00	100	0.00
263.00	100	0.00
264.00	100	0.00
265.00	100	0.00
266.00	100	0.00
267.00	100	0.00
268.00	100	0.00
269.00	100	0.00
270.00	100	0.00

2/2/2018 4:42:42 PM

Sohil

APPROVED

Manual Integrations

Client Sampled : F6C13

BNA_E




Instrument :

SOM-EPA-SIM-BE012618.M Fri Feb 02 07:51:05 2018

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020118\
 Data File : BE095383.D
 Acq On : 2 Feb 2018 6:39
 Operator : SJ/JU
 Sample : J1295-15
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Quant Time: Feb 02 07:49:09 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 02 04:53:51 2018
 Response via : Initial Calibration

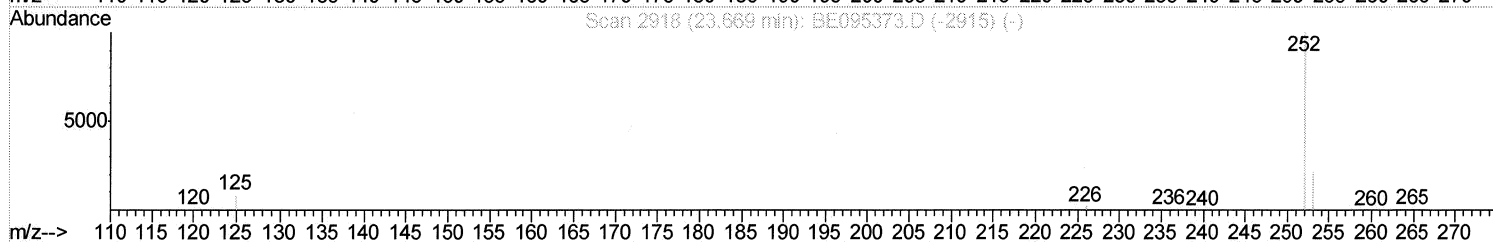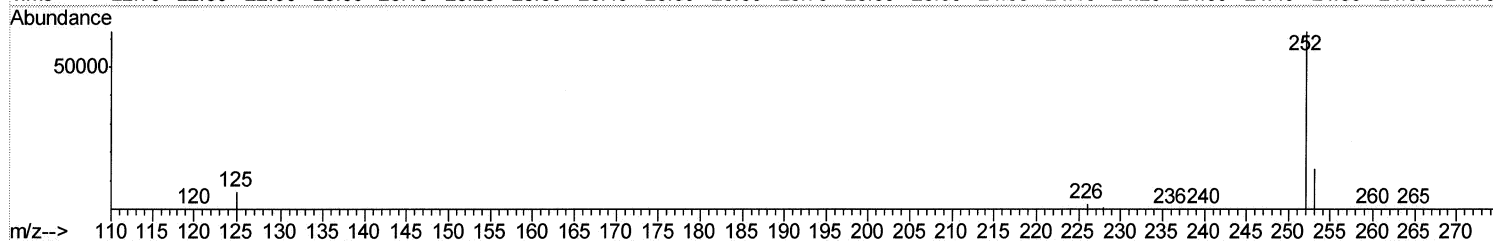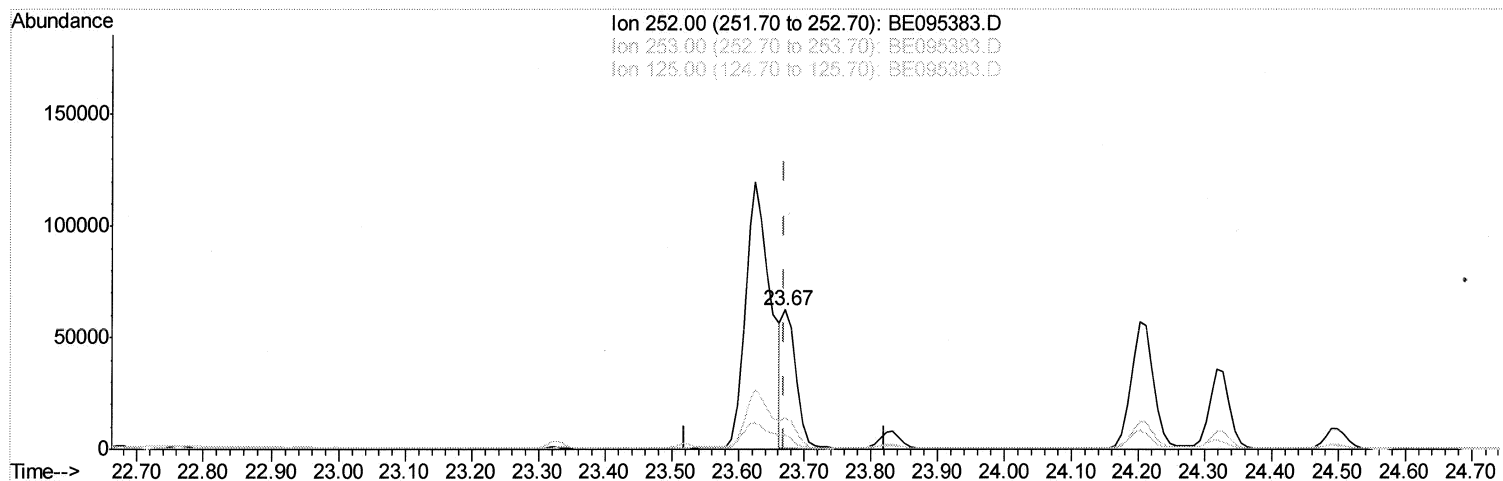

TIC: BE095383.D

(22) Benzo(k)fluoranthene

23.670min (+0.001) 3.34ng/ul m

response 88390

Ion Exp% Act%

202/02/18

2/2/2018 4:42:42 PM

Sohil

APPROVED

Manual Integrations




Client Sampled :

Instrument :

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020118\
 Data File : BE095383.D
 Acq On : 2 Feb 2018 6:39
 Operator : SJ/JU
 Sample : J1295-15
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Quant Time: Feb 02 07:49:09 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 02 04:53:51 2018
 Response via : Initial Calibration

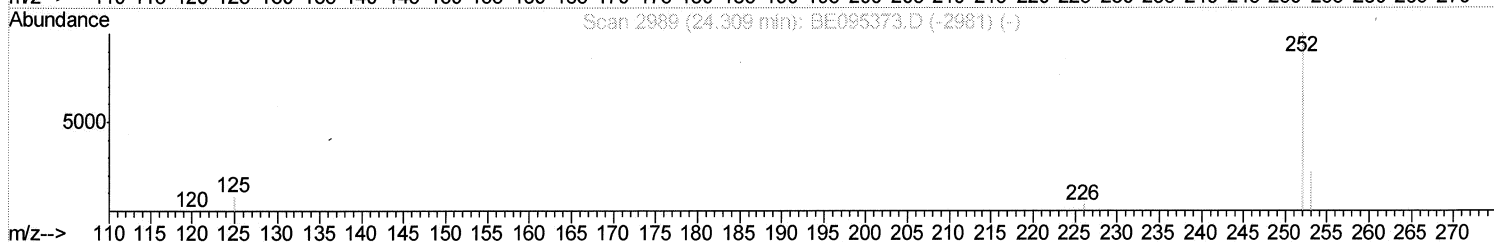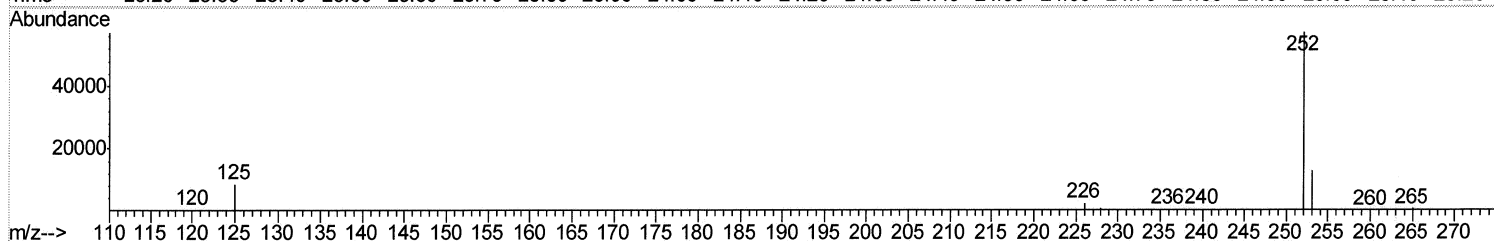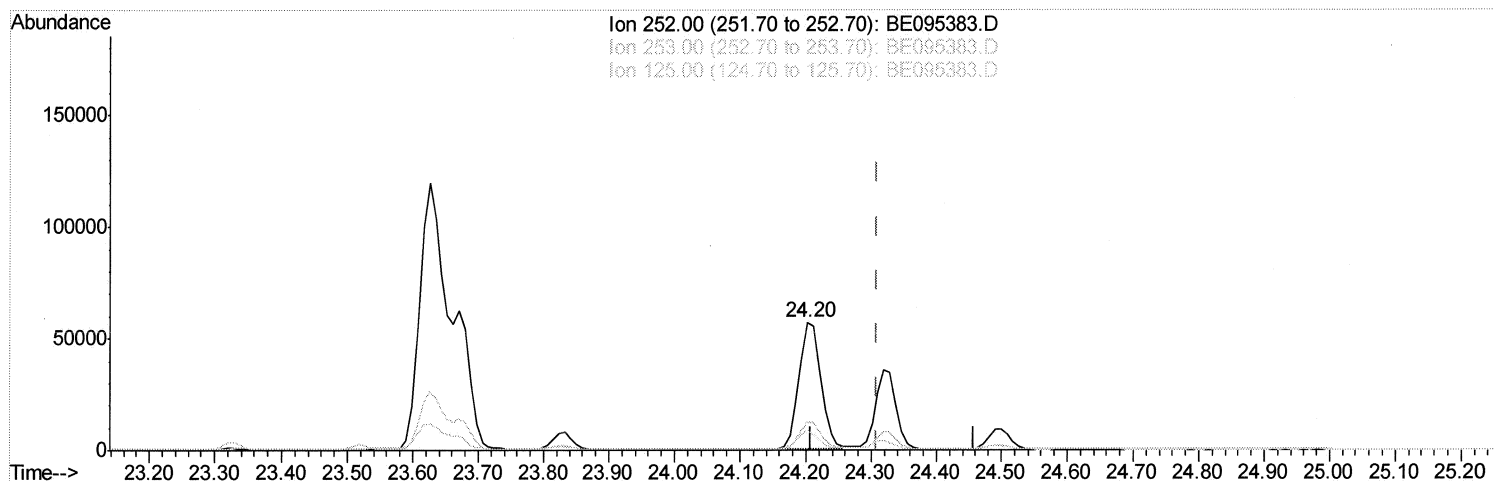

TIC: BE095383.D

(23) Benzo(a)pyrene (C)

24.202min (-0.107) 5.11ng/ul

response 131759

Ion	Exp%	Act%
252	100	100
253	1.98	1.98
254	4.94	4.94

00

2/2/2018 4:42:42 PM

Sohil

1.98#

APPROVED

4.94#

Manual Integrations

00

F6C13

ClientSampled :




BNA_E

Instrument :

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020118\
 Data File : BE095383.D
 Acq On : 2 Feb 2018 6:39
 Operator : SJ/JU
 Sample : J1295-15
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Quant Time: Feb 02 07:49:09 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 02 04:53:51 2018
 Response via : Initial Calibration

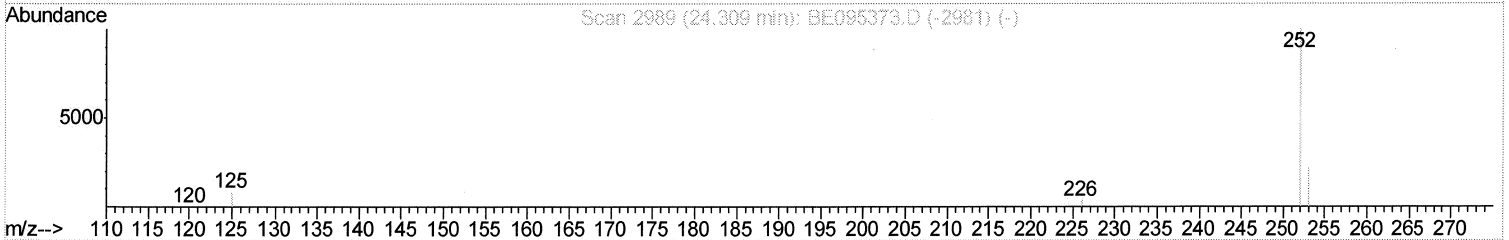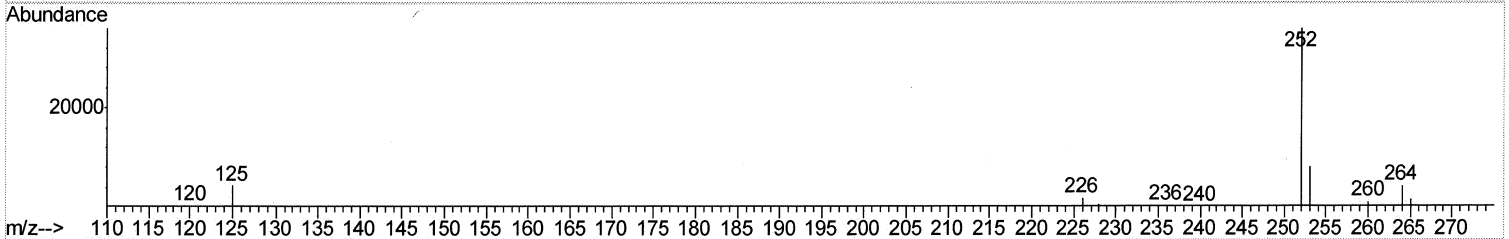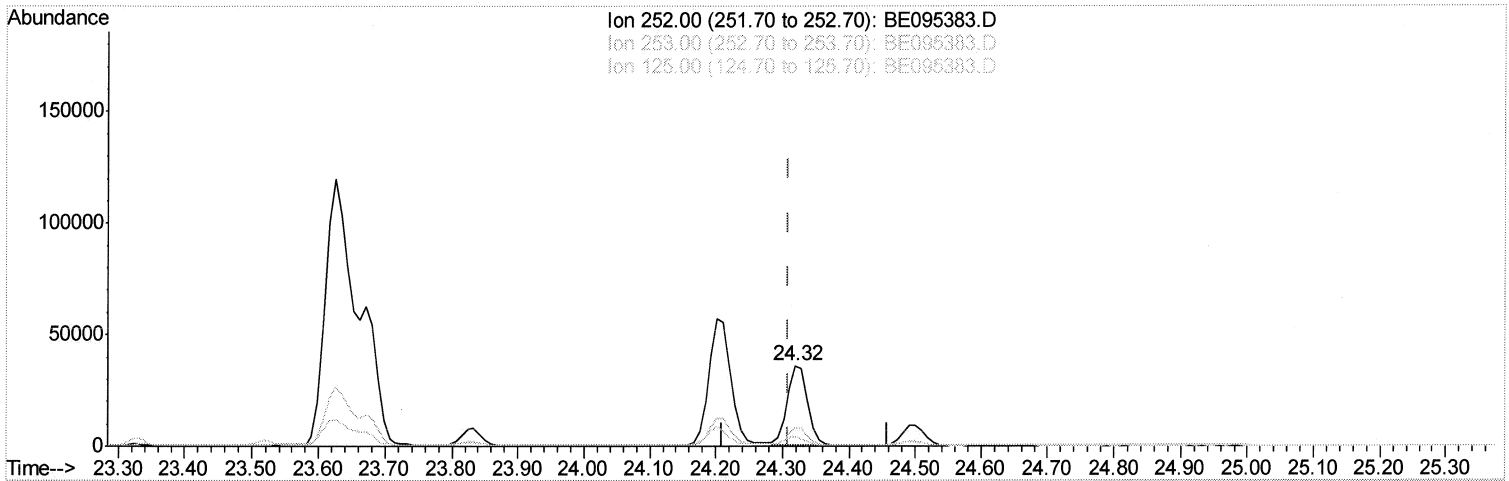

TIC: BE095383.D

(23) Benzo(a)pyrene (C)

24.319min (+0.010) 2.97ng/ul m

response 76686

Ion	Exp%	Act%
252.00	100	100
22.18#		
22.09#		
00		

2/2/2018 4:42:42 PM

Sohil

APPROVED

Manual Integrations

Client Sampled : F6C13




Instrument : BNA_E

SOM-EPA-SIM-BE012618.M Fri Feb 02 07:51:36 2018

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020118\
 Data File : BE095383.D
 Acq On : 2 Feb 2018 6:39
 Operator : SJ/JU
 Sample : J1295-15
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Quant Time: Feb 02 07:49:09 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 02 04:53:51 2018
 Response via : Initial Calibration

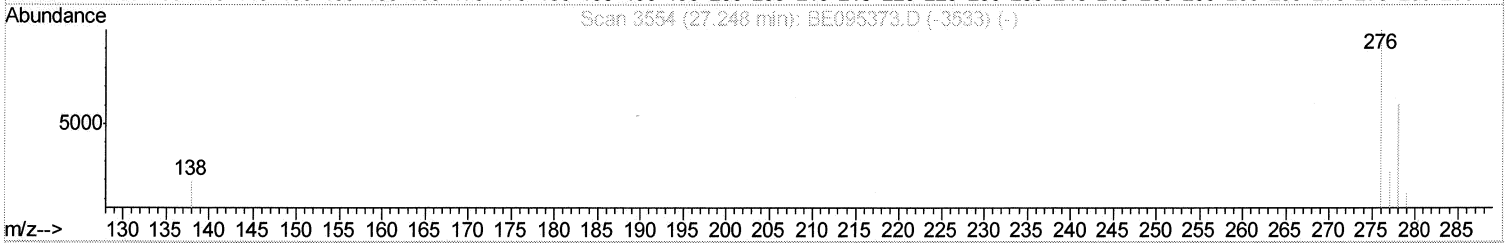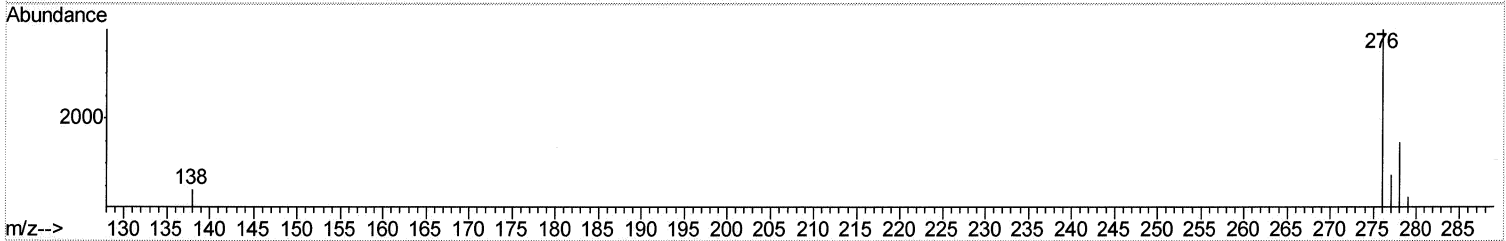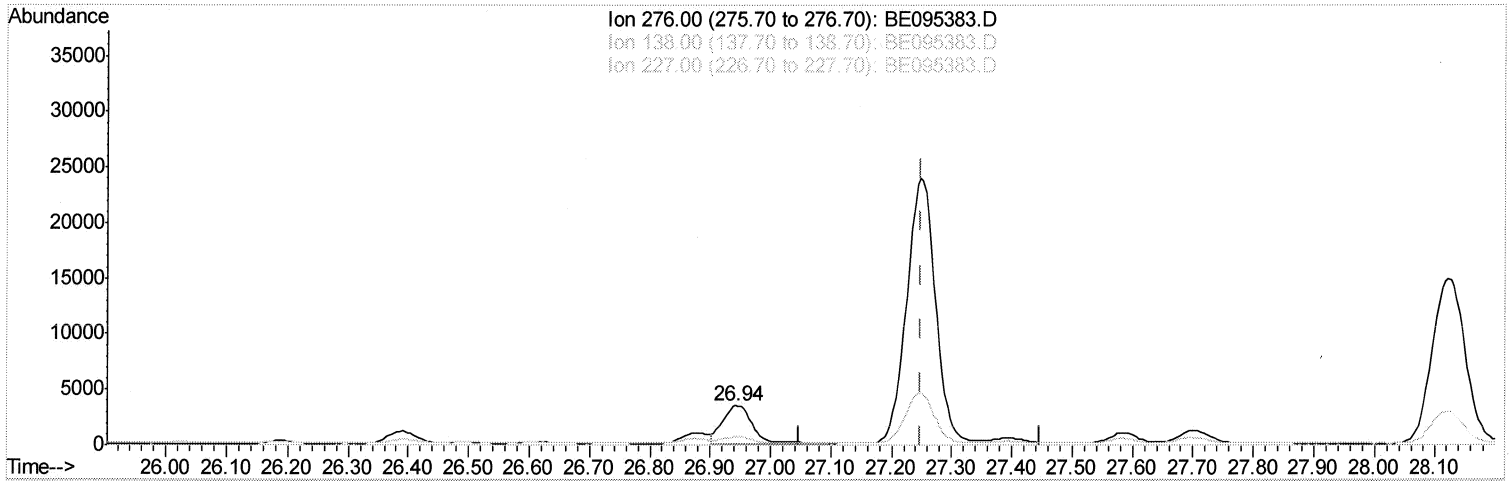

TIC: BE095383.D

(24) Indeno(1,2,3-cd)pyrene

26.942min (-0.306) 0.42ng/ul

response 11802

Ion	Exp%	Act%
276	100.00	100.00
138	4.44	0.00

100.00

2/2/2018 4:42:42 PM

Sohil

4.44#

APPROVED

0.00#

Manual Integrations

100.00

F6C13

ClientSampled :




BNA_E

Instrument :

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020118\
 Data File : BE095383.D
 Acq On : 2 Feb 2018 6:39
 Operator : SJ/JU
 Sample : J1295-15
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Quant Time: Feb 02 07:49:09 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 02 04:53:51 2018
 Response via : Initial Calibration

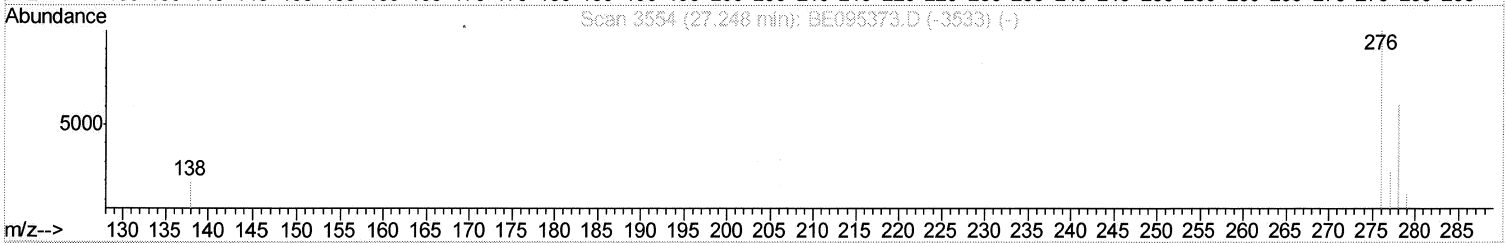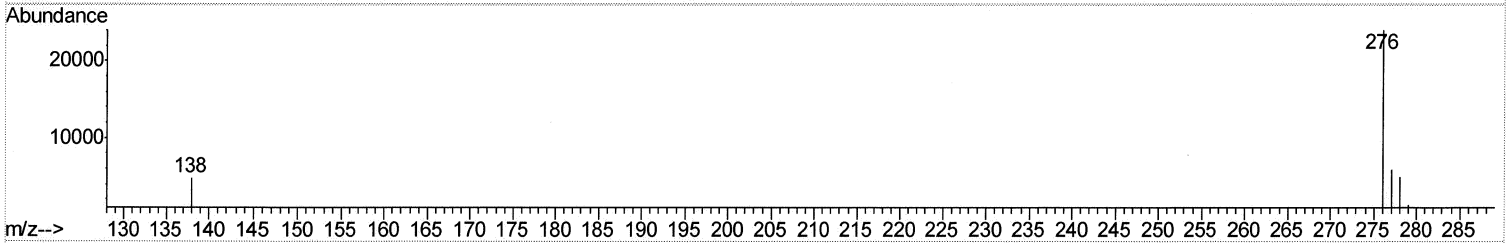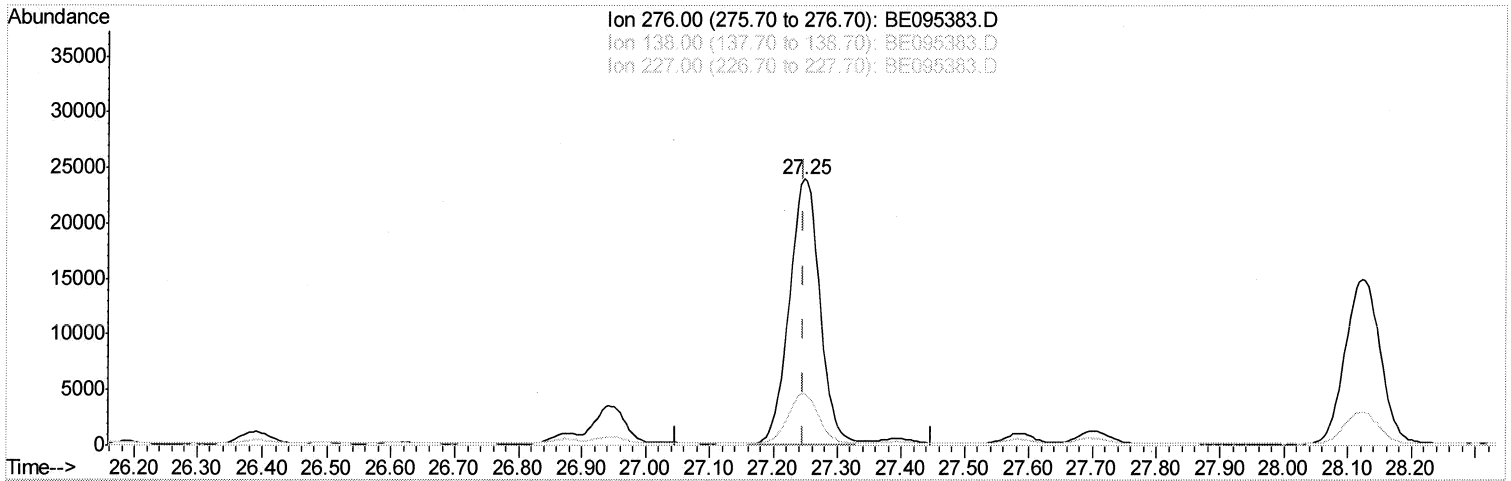

TIC: BE095383.D

(24) Indeno(1,2,3-cd)pyrene

27.247min (-0.000) 2.85ng/ul m

response 80762

Ion Exp% Act%

2/2/2018




Manual Integrations
 APPROVED
 2/2/2018 4:42:42 PM
 00
 2.11#
 0.00#
 00

Instrument :
 BNA_E
 ClientSampleId :
 F6C13

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020118\
 Data File : BE095383.D
 Acq On : 2 Feb 2018 6:39
 Operator : SJ/JU
 Sample : J1295-15
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Quant Time: Feb 02 07:49:09 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 02 04:53:51 2018
 Response via : Initial Calibration

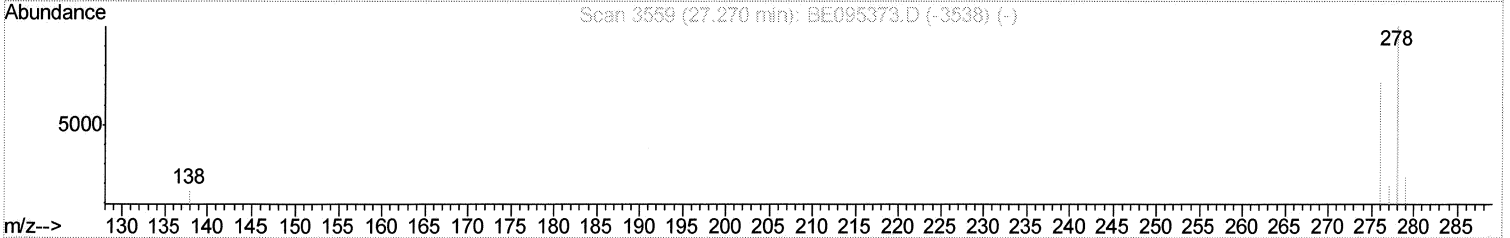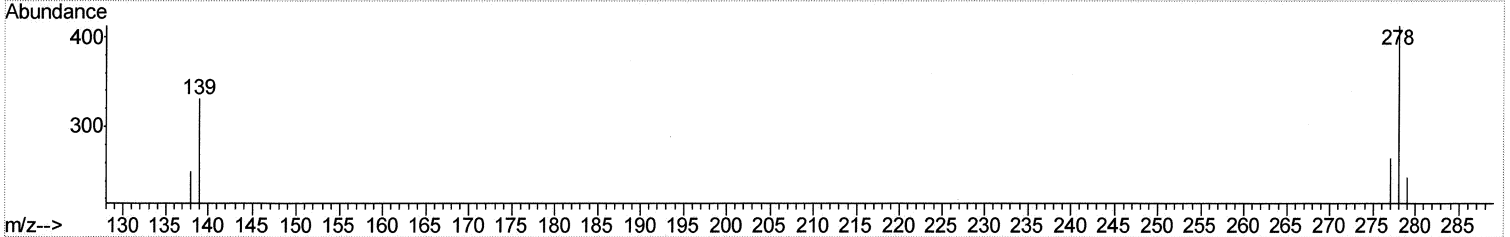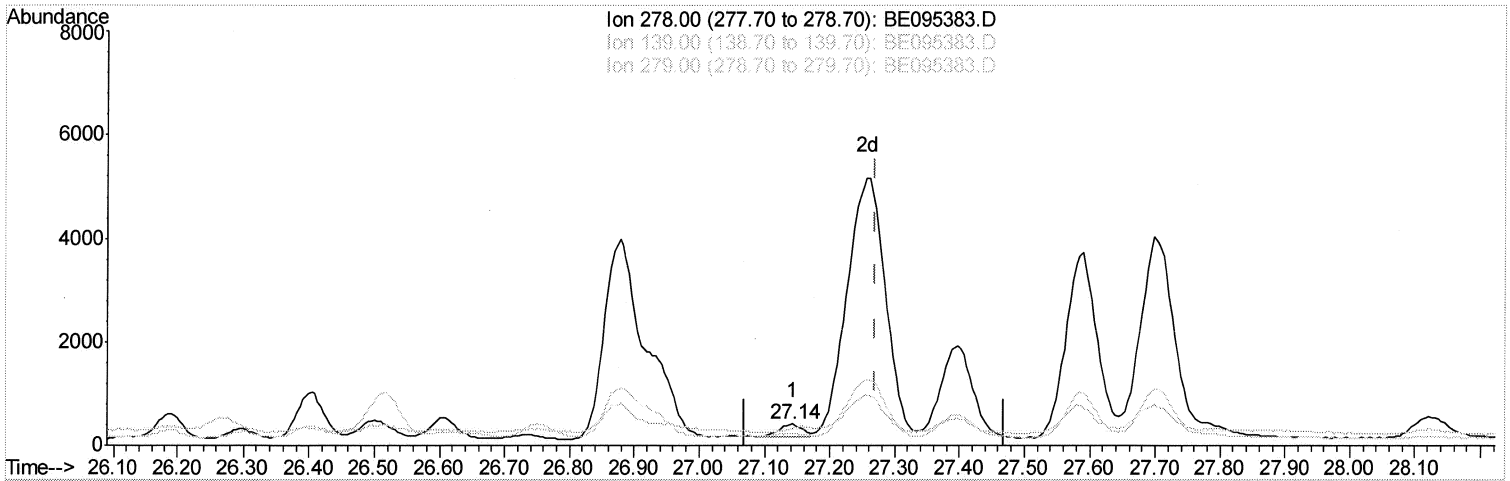

TIC: BE095383.D

(25) Dibenzo(a,h)anthracene

27.142min (-0.128) 0.03ng/ul

response 594

Ion	Exp%	Act%
278.00	100	100
139.00	100	100

2/2/2018 4:42:42 PM

Sohil

APPROVED

Manual Integrations

Client Sampled : F6C13

BNA_E




Instrument :

SOM-EPA-SIM-BE012618.M Fri Feb 02 07:51:55 2018

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020118\
 Data File : BE095383.D
 Acq On : 2 Feb 2018 6:39
 Operator : SJ/JU
 Sample : J1295-15
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Quant Time: Feb 02 07:49:09 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 02 04:53:51 2018
 Response via : Initial Calibration

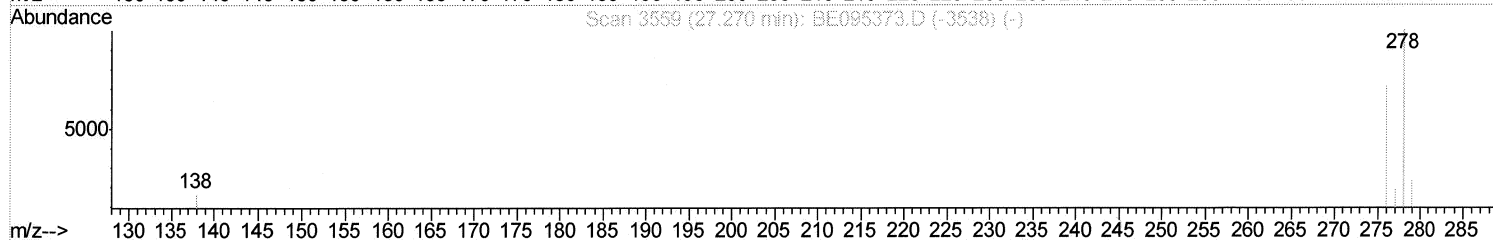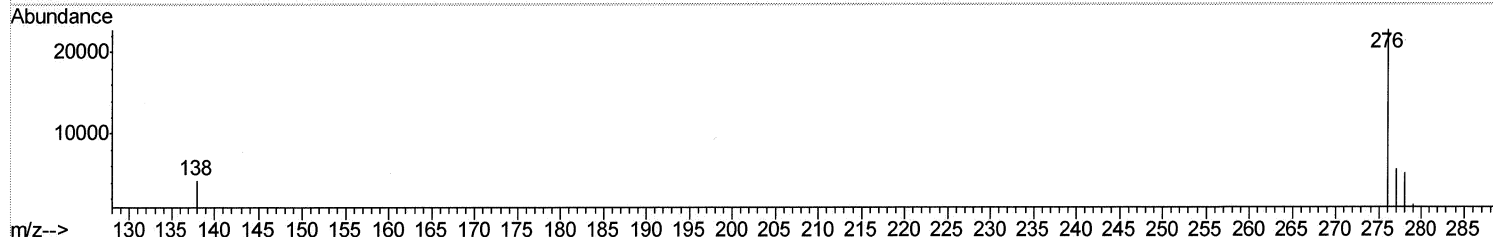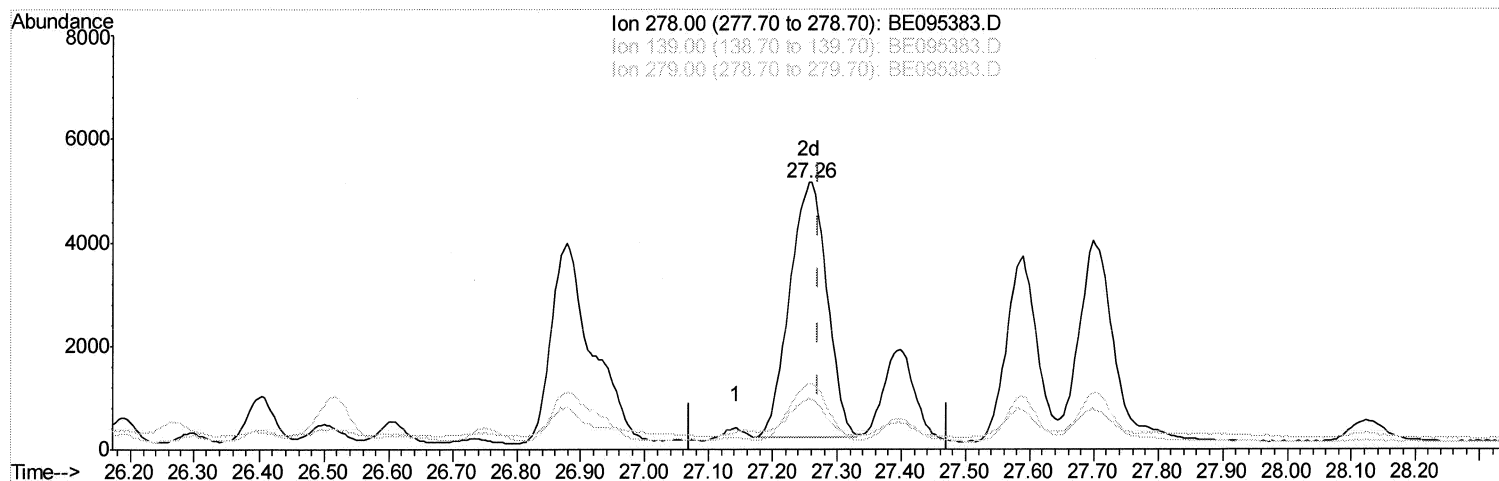

(25) Dibenzo(a,h)anthracene

27.256min (-0.014) 0.86ng/ul m

response 19881

Ion Exp% Act%

27.256min




00
 2/2/2018 4:42:42 PM
 Sohll
 APPROVED
 Manual Integrations
 24.52#
 00

F6C13
 ClientSampled :
 BNA_E
 Instrument :

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020118\
 Data File : BE095383.D
 Acq On : 2 Feb 2018 6:39
 Operator : SJ/JU
 Sample : J1295-15
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Quant Time: Feb 02 07:49:09 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 02 04:53:51 2018
 Response via : Initial Calibration

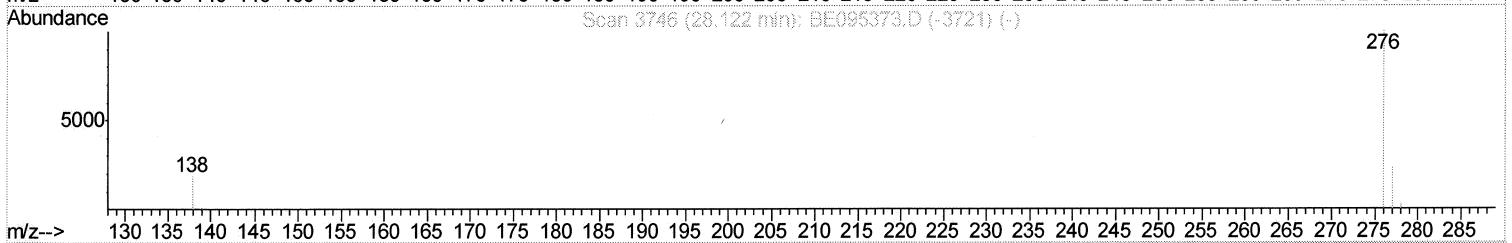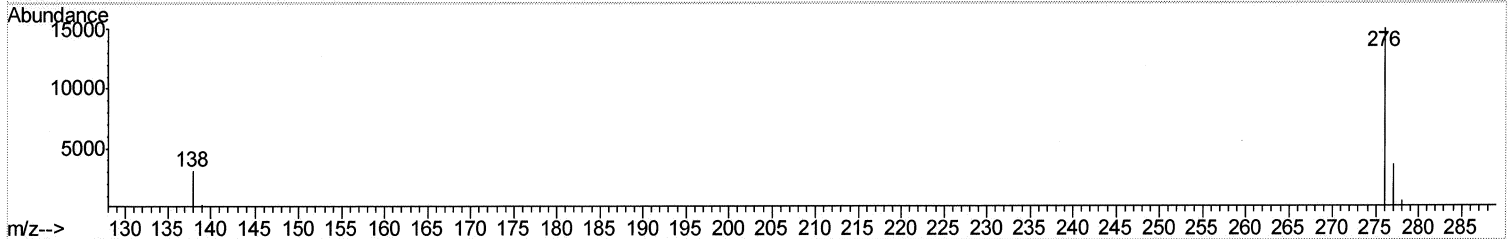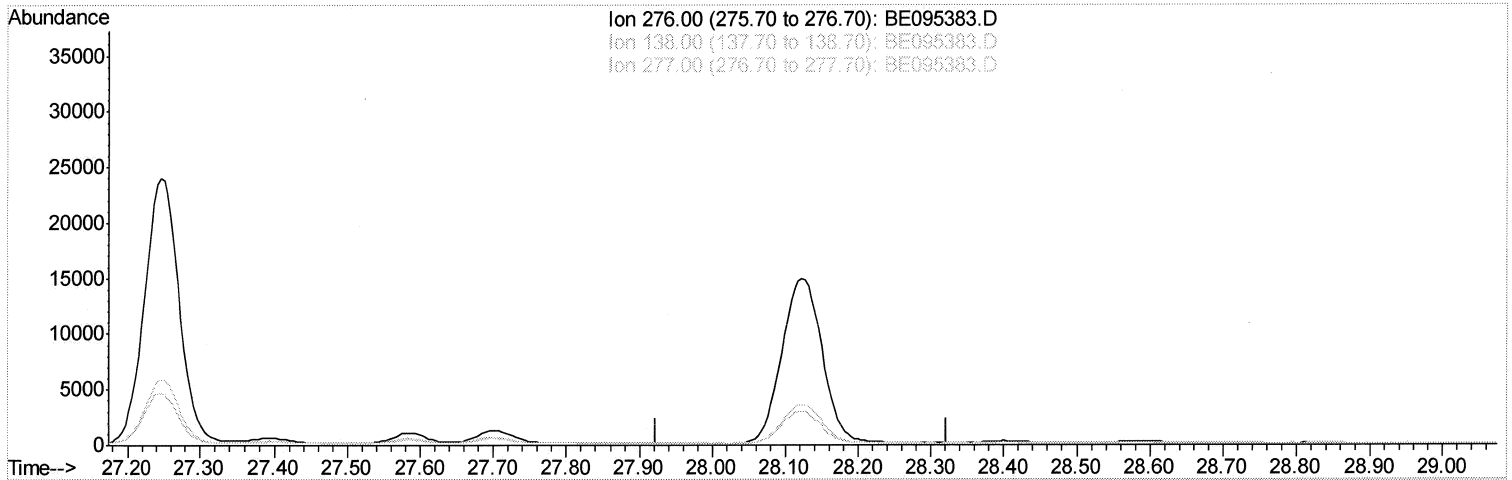

TIC: BE095383.D

(26) Benzo(g,h,i)perylene
 28.122min (-28.122) 0.00ng/ul
 response 0

Ion	Exp%	Act%
276	100	100
138	0.00	0.00
277	0.00	0.00
275	0.00	0.00
279	0.00	0.00
281	0.00	0.00
283	0.00	0.00
285	0.00	0.00

Ion Exp% Act%




2/2/2018 4:42:42 PM
 Sohll
 APPROVED
 Manual Integrations

Instrument :
 BNA_E
 ClientSampled :
 F6C13

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020118\
 Data File : BE095383.D
 Acq On : 2 Feb 2018 6:39
 Operator : SJ/JU
 Sample : J1295-15
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Quant Time: Feb 02 07:49:09 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 02 04:53:51 2018
 Response via : Initial Calibration

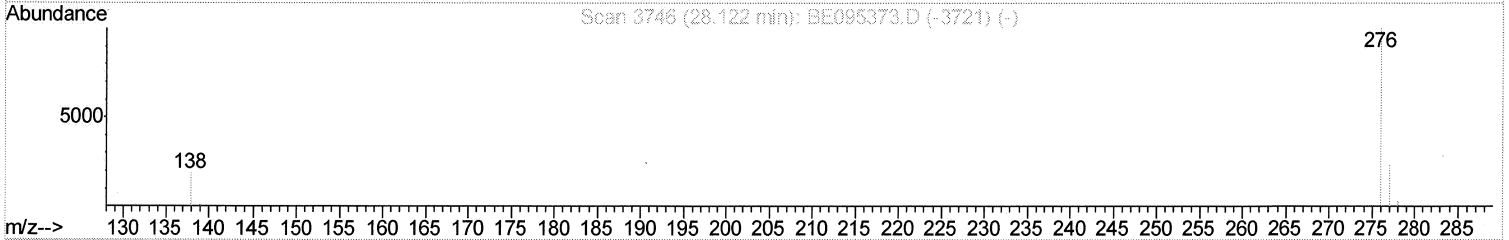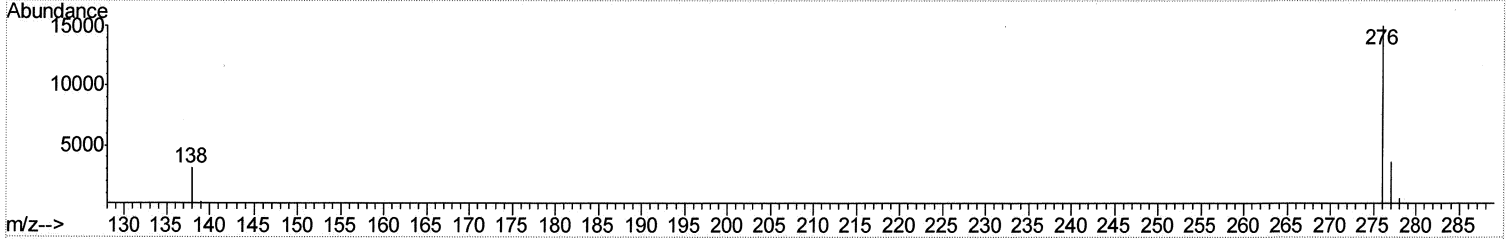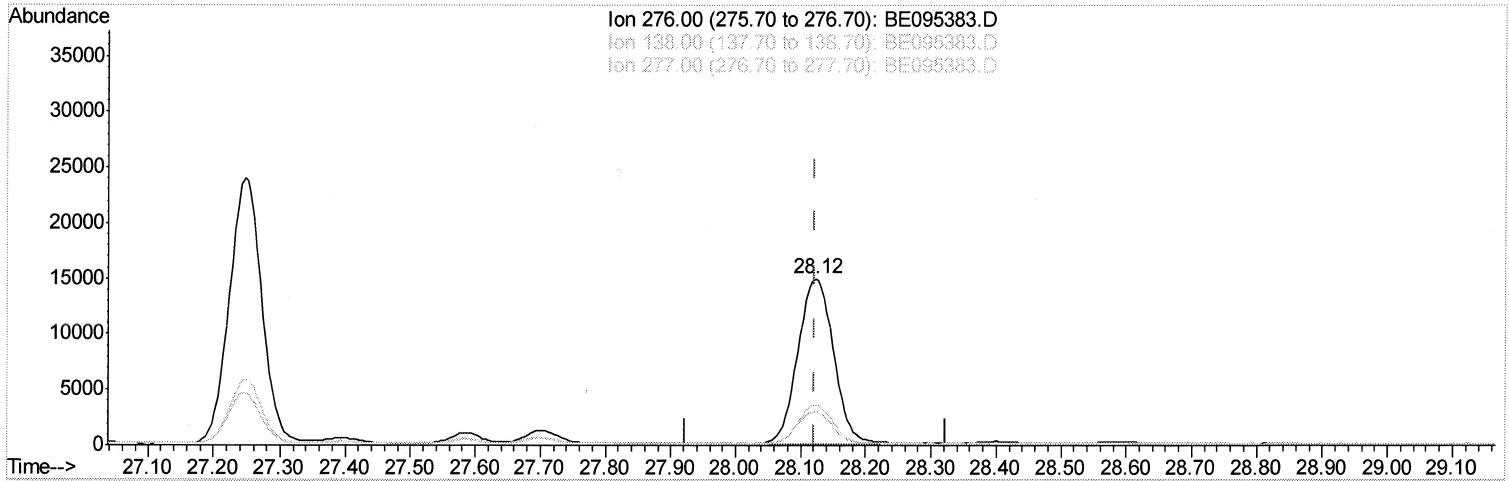

TIC: BE095383.D

(26) Benzo(g,h,i)perylene

28.122min (-0.000) 2.41ng/ul m

response 57729

Ion	Exp%	Act%
276.00	100	100
138.00	20.60	24.34

2/2/2018 4:42:42 PM
 Sohll

APPROVED
 Manual Integrations

Instrument : BNA_E
 ClientSample : F6C13

SOM-EPA-SIM-BE012618.M Fri Feb 02 07:52:25 2018

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020118\
 Data File : BE095383.D
 Acq On : 2 Feb 2018 6:39
 Operator : SJ/JU
 Sample : J1295-15
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Quant Time: Feb 02 07:51:59 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 02 04:53:51 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.44	152	2069	0.40	ng/ul	0.00
2) Naphthalene-d8	11.26	136	6492	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.01	164	4148	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	8811m	0.40	ng/ul	0.00
16) Chrysene-d12	21.80	240	8862	0.40	ng/ul	0.00
20) Perylene-d12	24.44	264	8188m	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.81	152	3901	0.37	ng/ul	0.00
14) Fluoranthene-d10	19.70	212	10631	0.32	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
7) Acenaphthylene	14.74	152	27021	1.354	ng/ul	97
9) Fluorene	16.05	166	2318m	0.145	ng/ul	
11) Pentachlorophenol	17.36	266	31387	18.392	ng/ul	96
12) Phenanthrene	17.75	178	8372	0.283	ng/ul#	90
13) Anthracene	17.84	178	21595	0.796	ng/ul#	93
15) Fluoranthene	19.72	202	308574	8.042	ng/ul	83
17) Pyrene	20.08	202	490369	16.490	ng/ul#	78
18) Benzo(a)anthracene	21.79	228	221388	7.990	ng/ul#	85
19) Chrysene	21.84	228	239411	8.321	ng/ul	96
21) Benzo(b)fluoranthene	23.63	252	324316m	11.227	ng/ul	
22) Benzo(k)fluoranthene	23.67	252	88390m	3.345	ng/ul	
23) Benzo(a)pyrene	24.32	252	76686m	2.973	ng/ul	
24) Indeno(1,2,3-cd)pyrene	27.25	276	80762m	2.855	ng/ul	
25) Dibenzo(a,h)anthracene	27.26	278	19881m	0.859	ng/ul	
26) Benzo(a,h,i)perylene	28.12	276	57729m	2.410	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

2/2/2018 4:42:42 PM

Sohil

APPROVED
Manual Integrations

Instrument : BNA_E
 Client Sample : F6C13

SOM-EPA-SIM-BE012618.M Fri Feb 02 07:53:14 2018