

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020118\
 Data File : BE095369.D
 Acq On : 1 Feb 2018 22:18
 Operator : SJ/JU
 Sample : J1295-18
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 F6C16

Manual Integrations
 APPROVED

Sohil
 2/2/2018 4:42:04 PM

Quant Time: Feb 02 04:43:20 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 02 04:07:20 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.44	152	2095	0.40	ng/ul	0.00
2) Naphthalene-d8	11.26	136	6487	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.02	164	4276	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	8794m	0.40	ng/ul	0.00
16) Chrysene-d12	21.80	240	8368	0.40	ng/ul	0.00
20) Perylene-d12	24.44	264	7867m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	3897	0.37	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	9628	0.29	ng/ul	0.00
Target Compounds						
11) Pentachlorophenol	17.36	266	6621	3.887	ng/ul	Ovalue 95
12) Phenanthrene	17.75	178	951m	0.032	ng/ul	
15) Fluoranthene	19.72	202	908	0.024	ng/ul	87

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA E\DATA\BE020118\
Data File : BE095369.D
Acq On : 1 Feb 2018 22:18
Operator : SJ/JU
Sample : J1295-18
Misc :
ALS Vial : 14 Sample Multiplier: 1


Instrument :
BNA_E
ClientSampleId :
F6C16

Manual Integrations
APPROVED

Sohil
2/2/2018 4:42:04 PM

Quant Time: Feb 02 04:43:20 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 02 04:07:20 2018
Response via : Initial Calibration

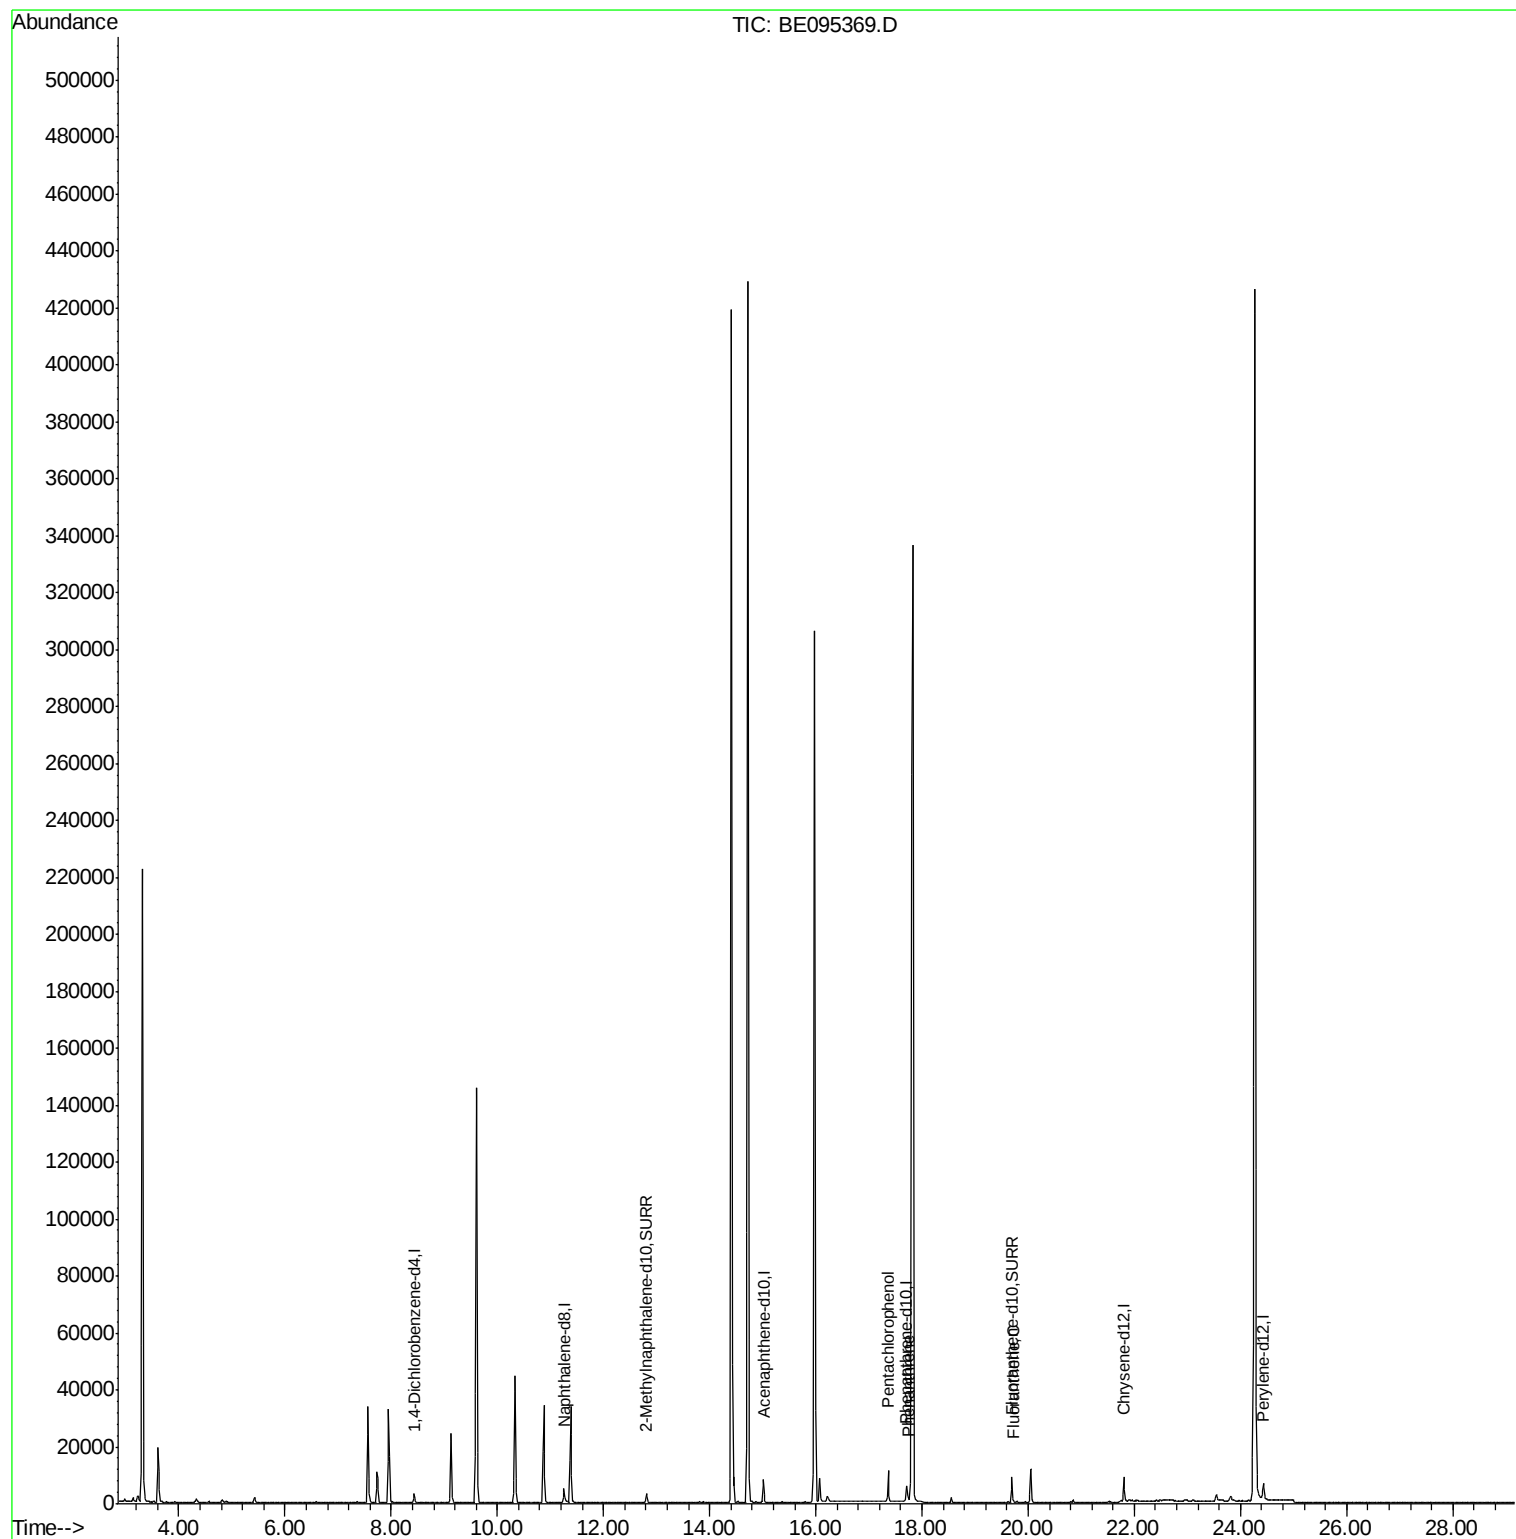

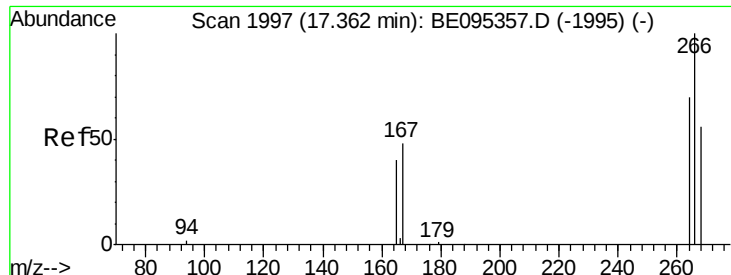





#11
 Pentachlorophenol
 Concen: 3.887 ng/ul
 RT: 17.36 min Scan# 1997
 Delta R.T. -0.00 min
 Lab File: BE095369.D
 Acq: 1 Feb 2018 22:18

Instrument :
 BNA_E
 ClientSampleId :
 F6C16

Tot Ion	Ratio	Lower	Upper
266	100		
264	65.8	47.9	71.9
268	59.8	49.8	74.8




Manual Integrations
 APPROVED


Sohil
 2/2/2018 4:42:04 PM

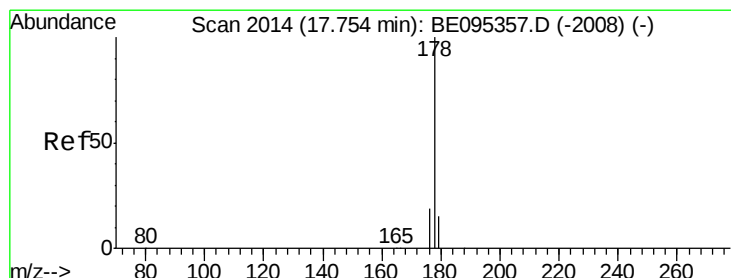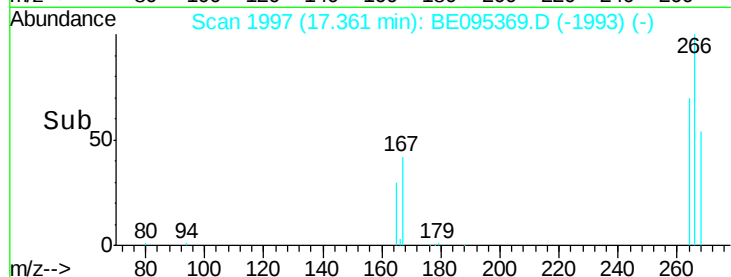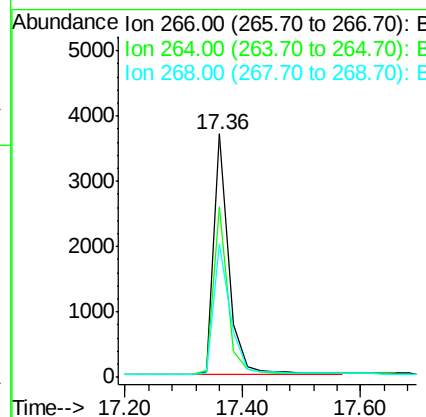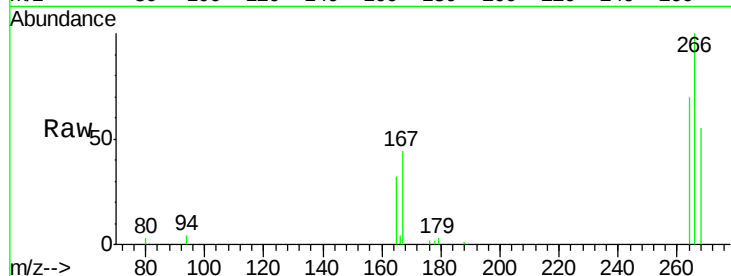

#12
 Phenanthrene
 Concen: 0.032 ng/ul m
 RT: 17.75 min Scan# 2014
 Delta R.T. -0.00 min
 Lab File: BE095369.D
 Acq: 1 Feb 2018 22:18

Tgt Ion	Ratio	Lower	Upper
178	100		
179	27.6	18.4	27.6
176	28.1	13.6	20.4

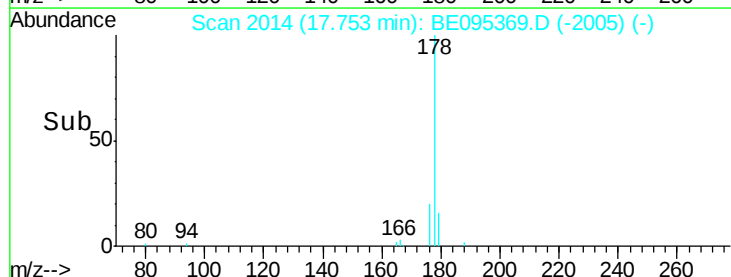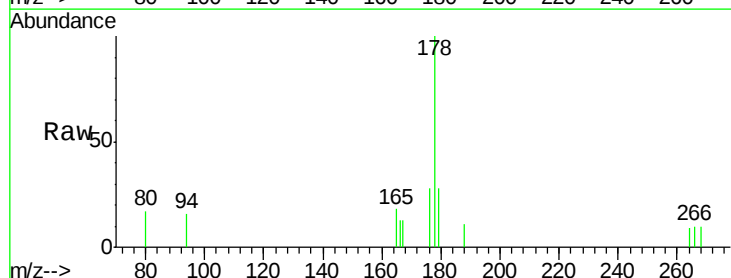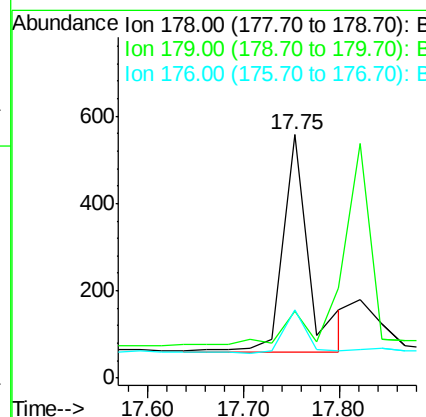

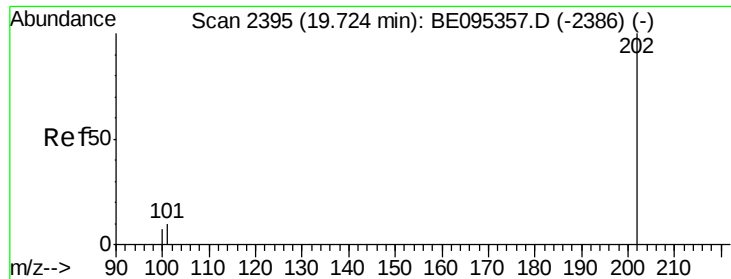

#15

Fluoranthene

Concen: 0.024 ng/ul

RT: 19.72 min Scan# 2395

Delta R.T. 0.00 min

Lab File: BE095369.D


Acq: 1 Feb 2018 22:18

Instrument :

BNA_E

ClientSampleId :

F6C16

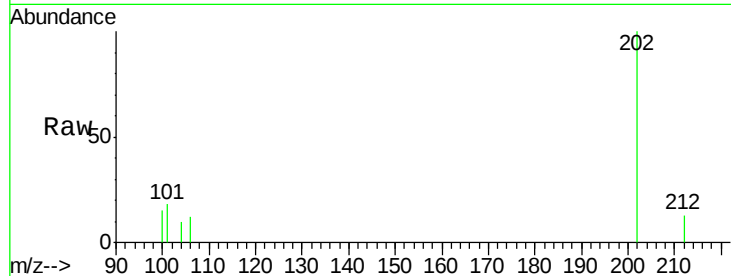

Tot Ion:	202	Resp:	908
Ion Ratio	Lower	Upper	
202	100		
101	17.8	0.0	30.3
100	15.3	0.0	39.5

Manual Integrations
APPROVED

Sohil
2/2/2018 4:42:04 PM

