


Data Path : Z:\HPCHEM1\BNA\_E\DATA\BE020215\  
Data File : BE089454.D  
Acq On : 2 Feb 2015 13:53  
Operator : TP/IZ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_E  
ClientSampleId :  
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA\_E\METHODS\SIM-BE020215.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Tue Feb 03 04:09:03 2015

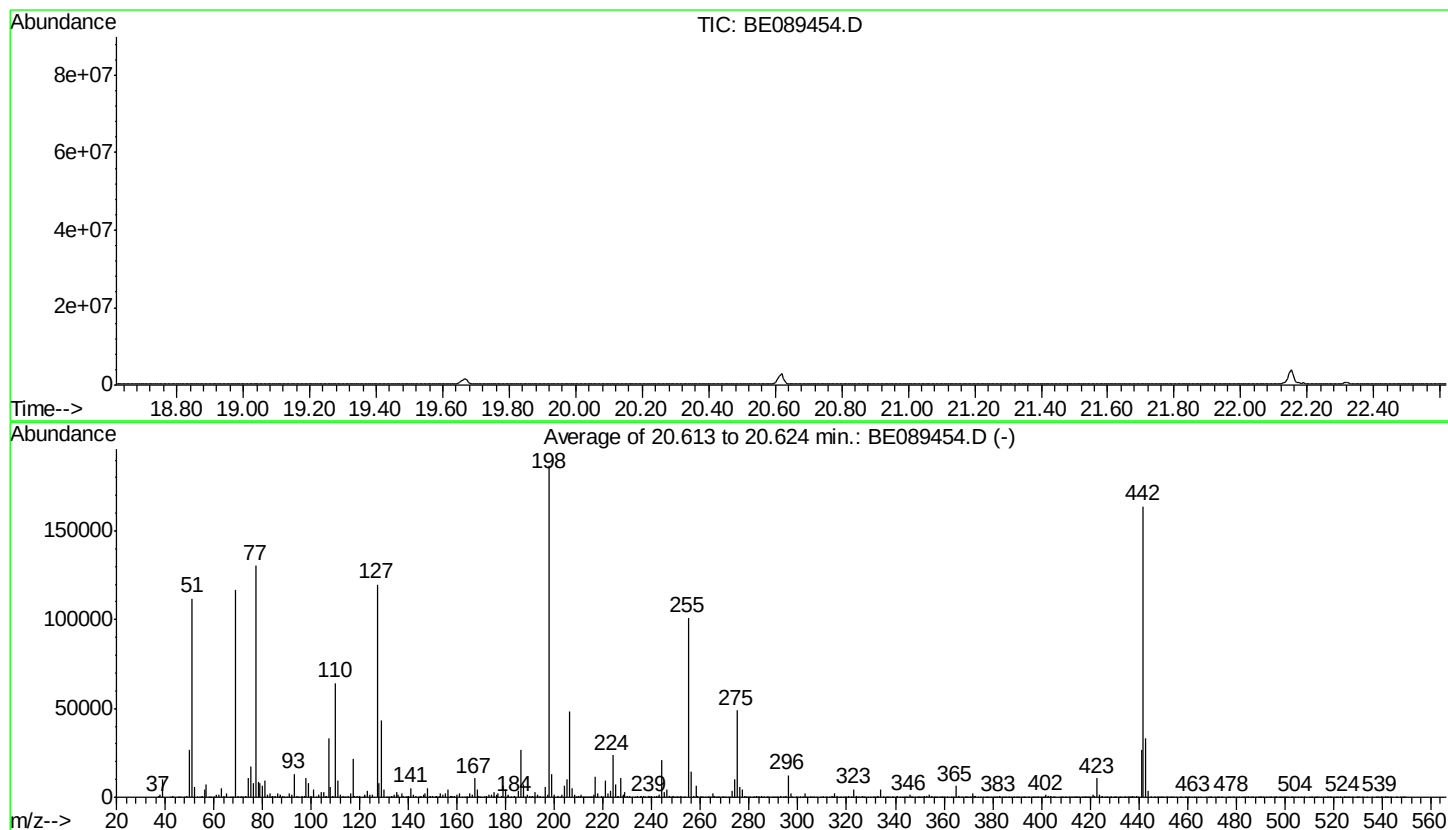

AutoFind: Scans 3272, 3273, 3274; Background Corrected with Scan 3264

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 60.0         | 112102     | PASS                |
| 68             | 69              | 0.00            | 2               | 0.3          | 337        | PASS                |
| 69             | 198             | 0.00            | 100             | 62.6         | 116855     | PASS                |
| 70             | 69              | 0.00            | 2               | 0.4          | 436        | PASS                |
| 127            | 198             | 10              | 80              | 64.2         | 119849     | PASS                |
| 197            | 198             | 0.00            | 2               | 0.8          | 1446       | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 186792     | PASS                |
| 199            | 198             | 5               | 9               | 6.9          | 12962      | PASS                |
| 275            | 198             | 10              | 60              | 26.1         | 48747      | PASS                |
| 365            | 198             | 1               | 100             | 3.3          | 6229       | PASS                |
| 441            | 442             | 0.01            | 24              | 16.5         | 26968      | PASS                |
| 442            | 198             | 50              | 100             | 87.7         | 163739     | PASS                |
| 443            | 442             | 15              | 24              | 20.1         | 32936      | PASS                |