


Data Path : Z:\HPCHEM1\BNA\_E\DATA\BE020215\  
Data File : BE089470.D  
Acq On : 3 Feb 2015 00:23  
Operator : TP/IZ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_E  
ClientSampleId :

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA\_E\METHODS\SIM-BE020215.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Tue Feb 03 04:09:03 2015

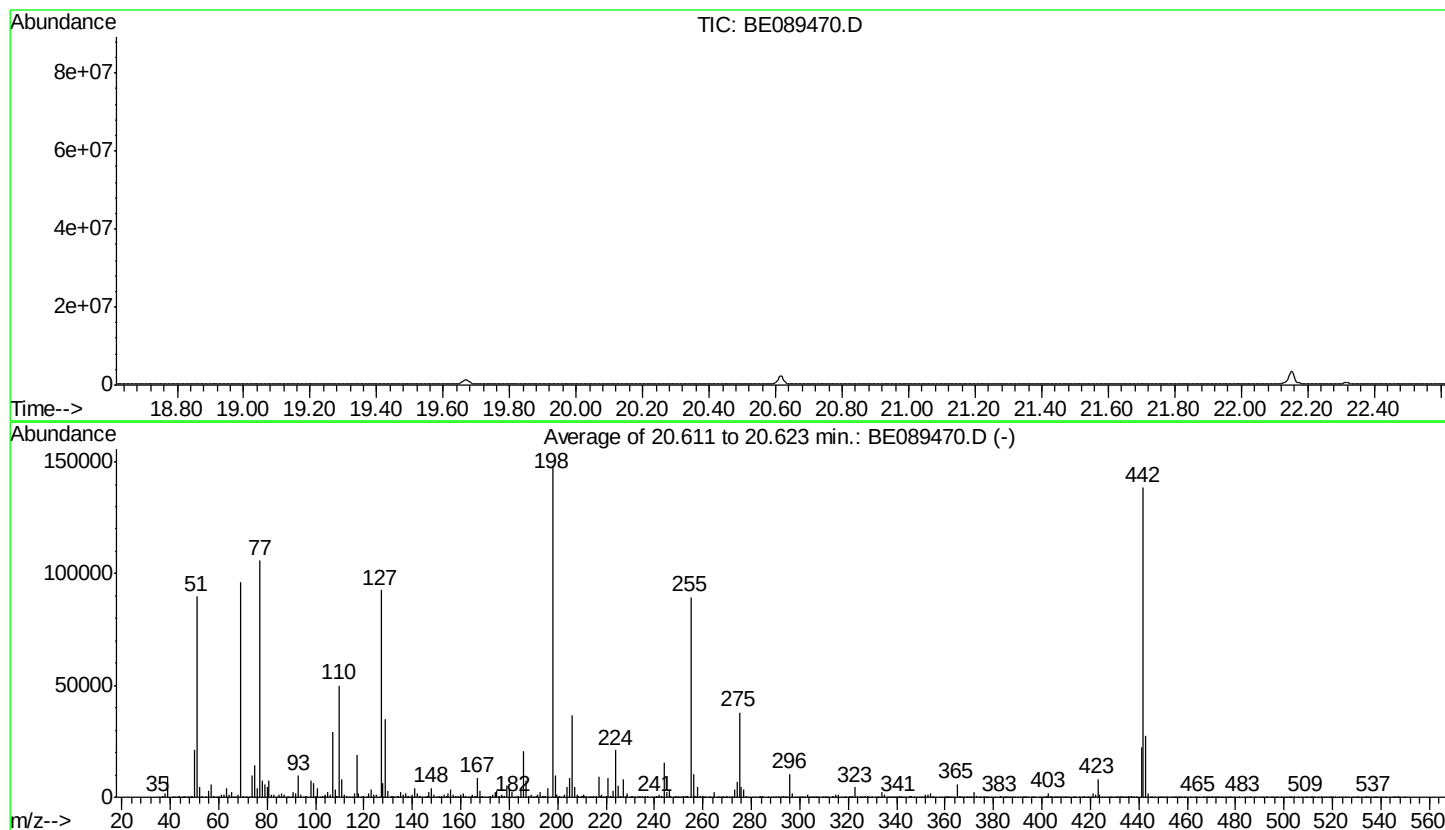

AutoFind: Scans 3272, 3273, 3274; Background Corrected with Scan 3265

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 60.4      | 89640   | PASS             |
| 68          | 69           | 0.00         | 2            | 0.9       | 896     | PASS             |
| 69          | 198          | 0.00         | 100          | 64.7      | 96033   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.7       | 648     | PASS             |
| 127         | 198          | 10           | 80           | 62.5      | 92742   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.0       | 0       | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 148341  | PASS             |
| 199         | 198          | 5            | 9            | 6.5       | 9610    | PASS             |
| 275         | 198          | 10           | 60           | 25.6      | 38047   | PASS             |
| 365         | 198          | 1            | 100          | 4.0       | 5931    | PASS             |
| 441         | 442          | 0.01         | 24           | 16.1      | 22325   | PASS             |
| 442         | 198          | 50           | 100          | 93.3      | 138347  | PASS             |
| 443         | 442          | 15           | 24           | 20.1      | 27739   | PASS             |