



n-Nitrosodimethylamine

Response Ratio

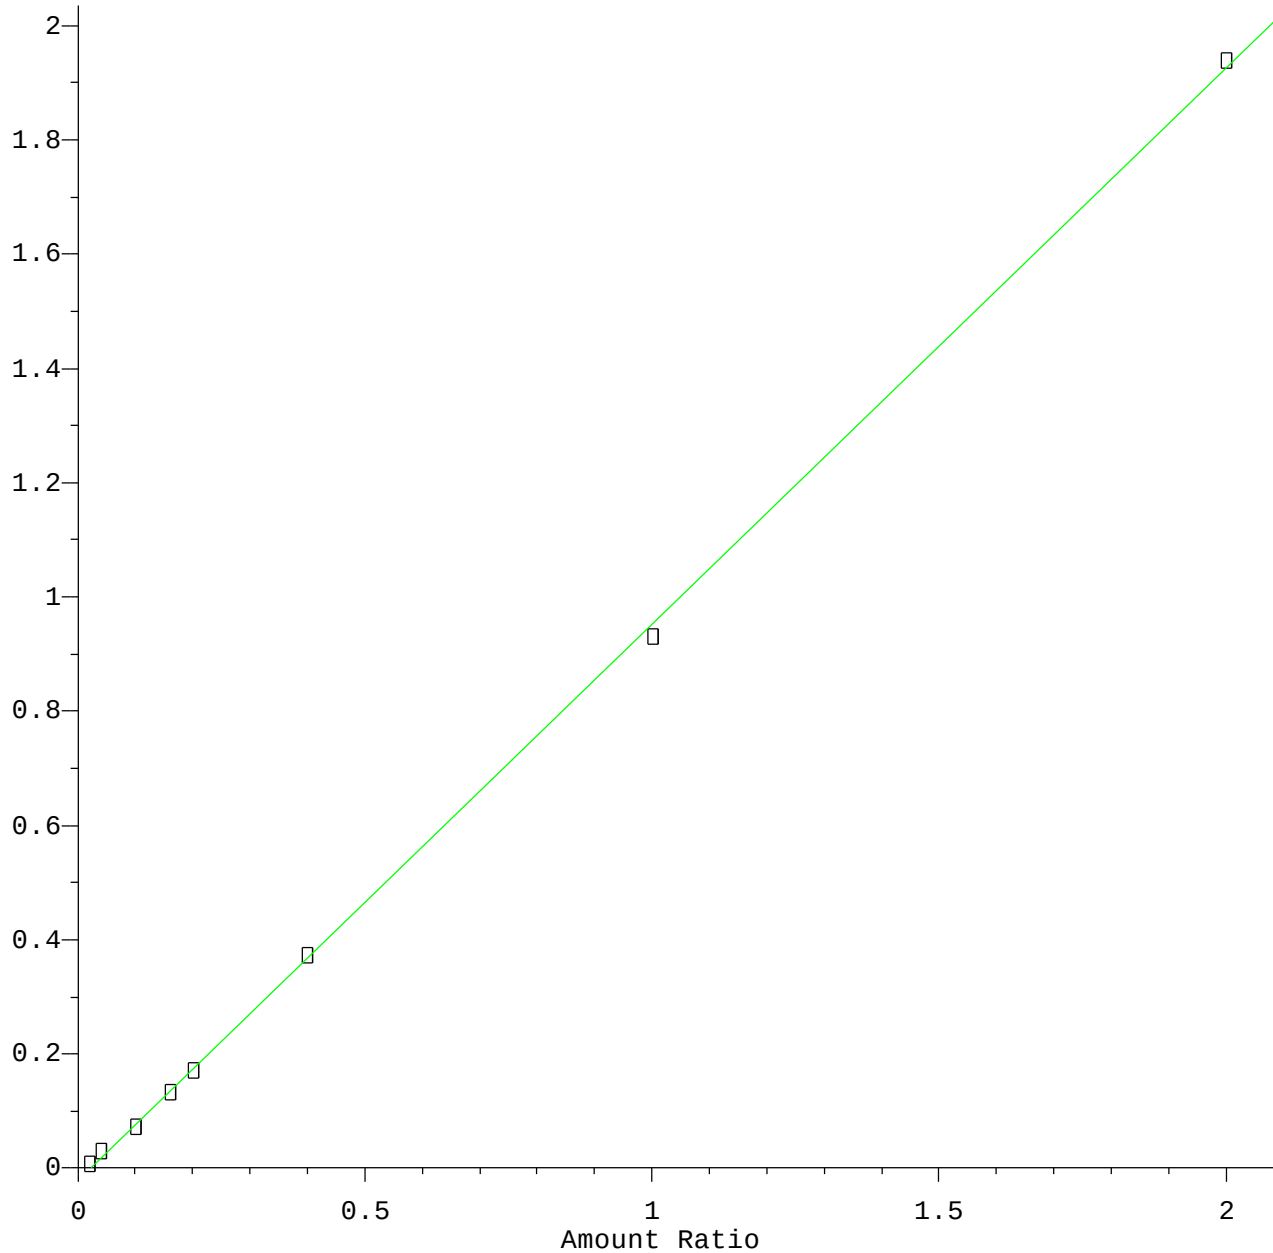


Resp Ratio = $9.74 \times 10^{-1} \times \text{Amt} - 2.11 \times 10^{-2}$
Coef of Det (r^2) = 1.000 Curve Fit: Linear


Method Name: Z:\HPCHEM1\BNA_E\METHODS\SIM-BE020215.M
Calibration Table Last Updated: Tue Feb 03 03:33:16 2015

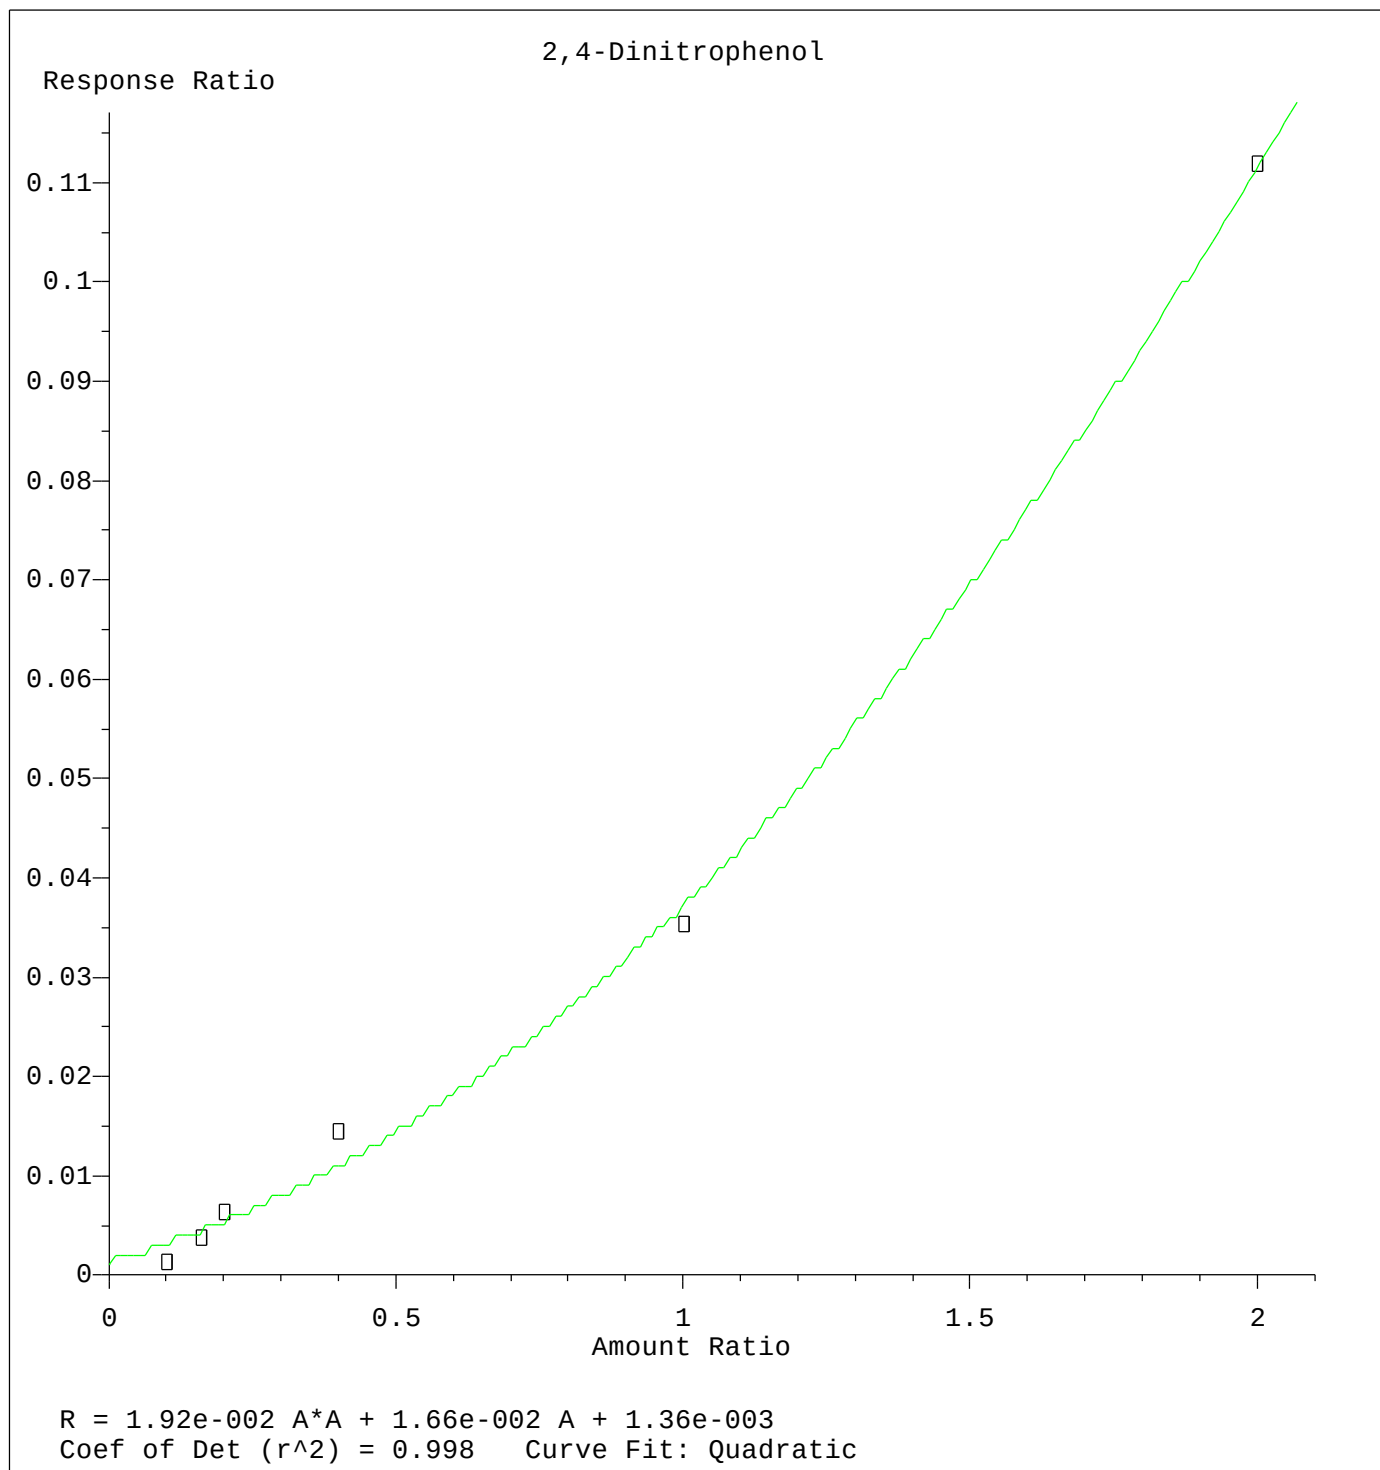

Method Name: Z:\HPCHEM1\BNA_E\METHODS\SIM-BE020215.M
Calibration Table Last Updated: Tue Feb 03 04:06:11 2015

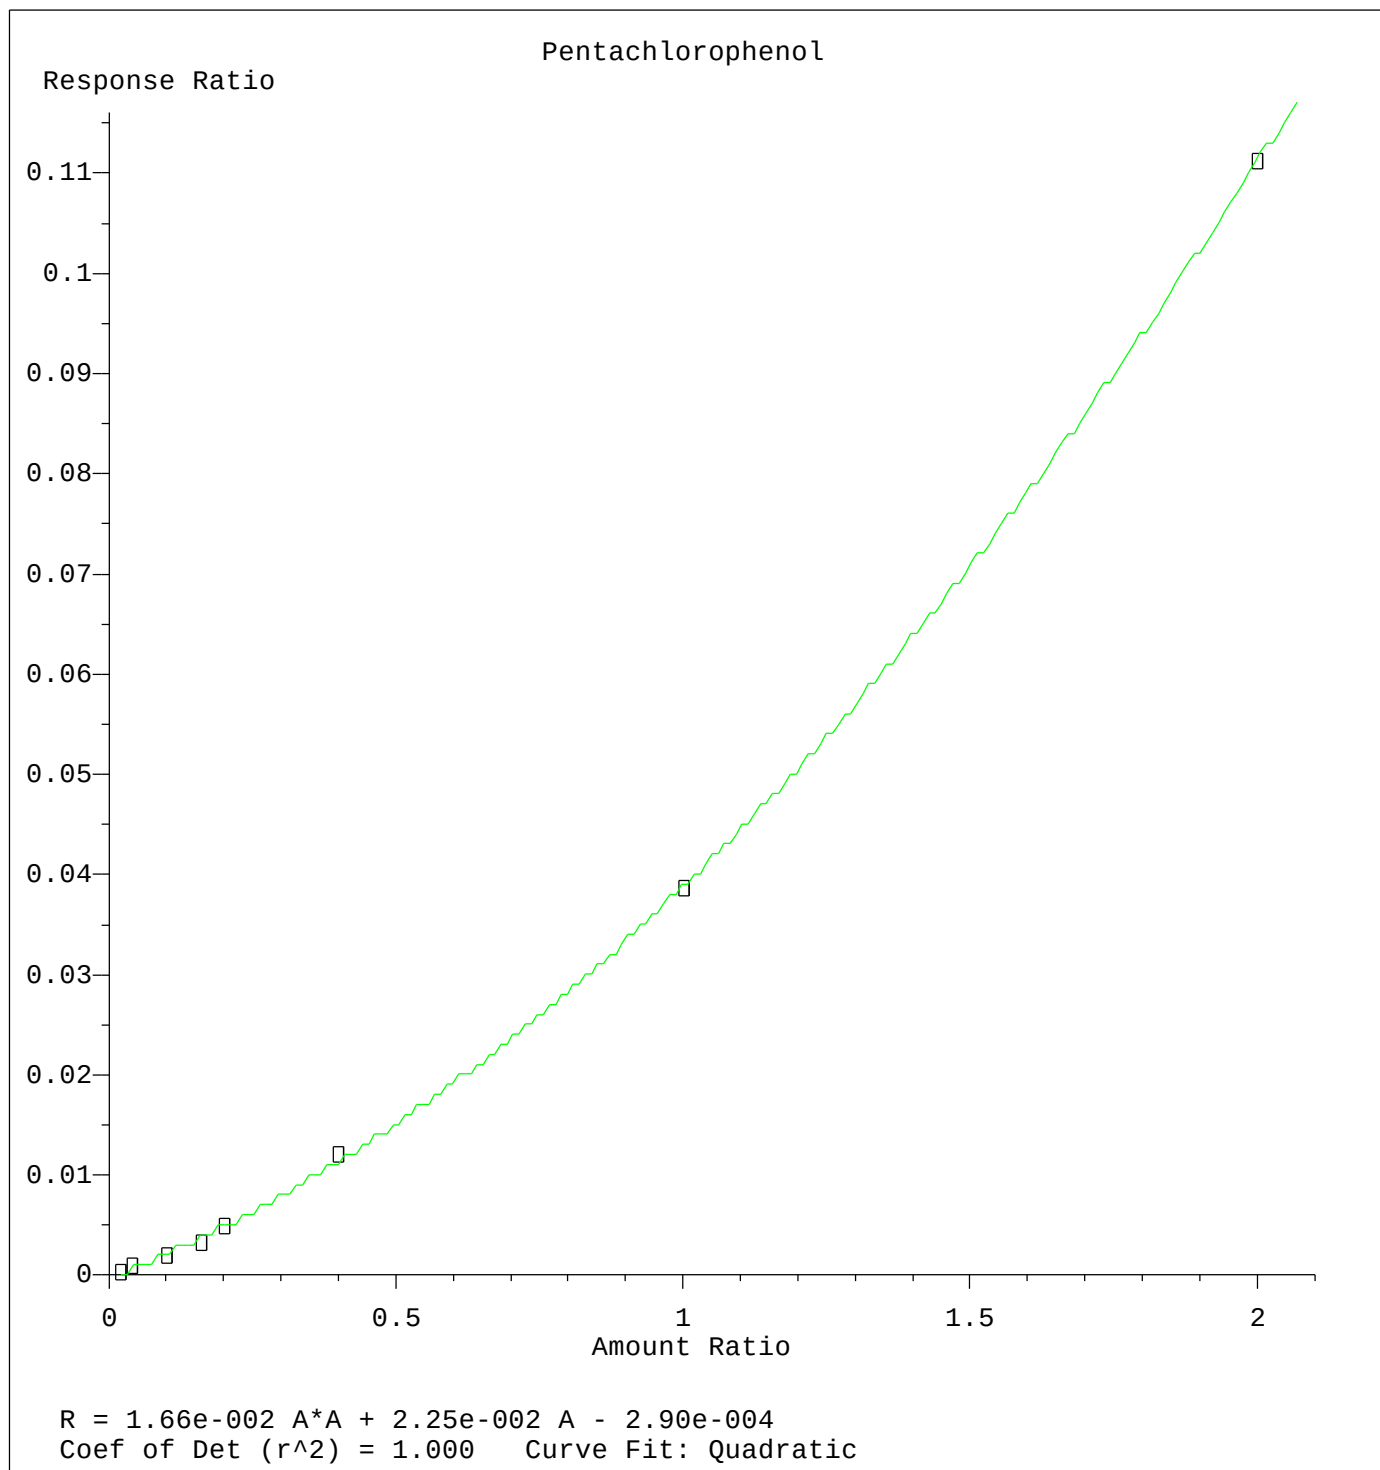


Method Name: Z:\HPCHEM1\BNA_E\METHODS\SIM-BE020215.M
Calibration Table Last Updated: Tue Feb 03 04:06:47 2015

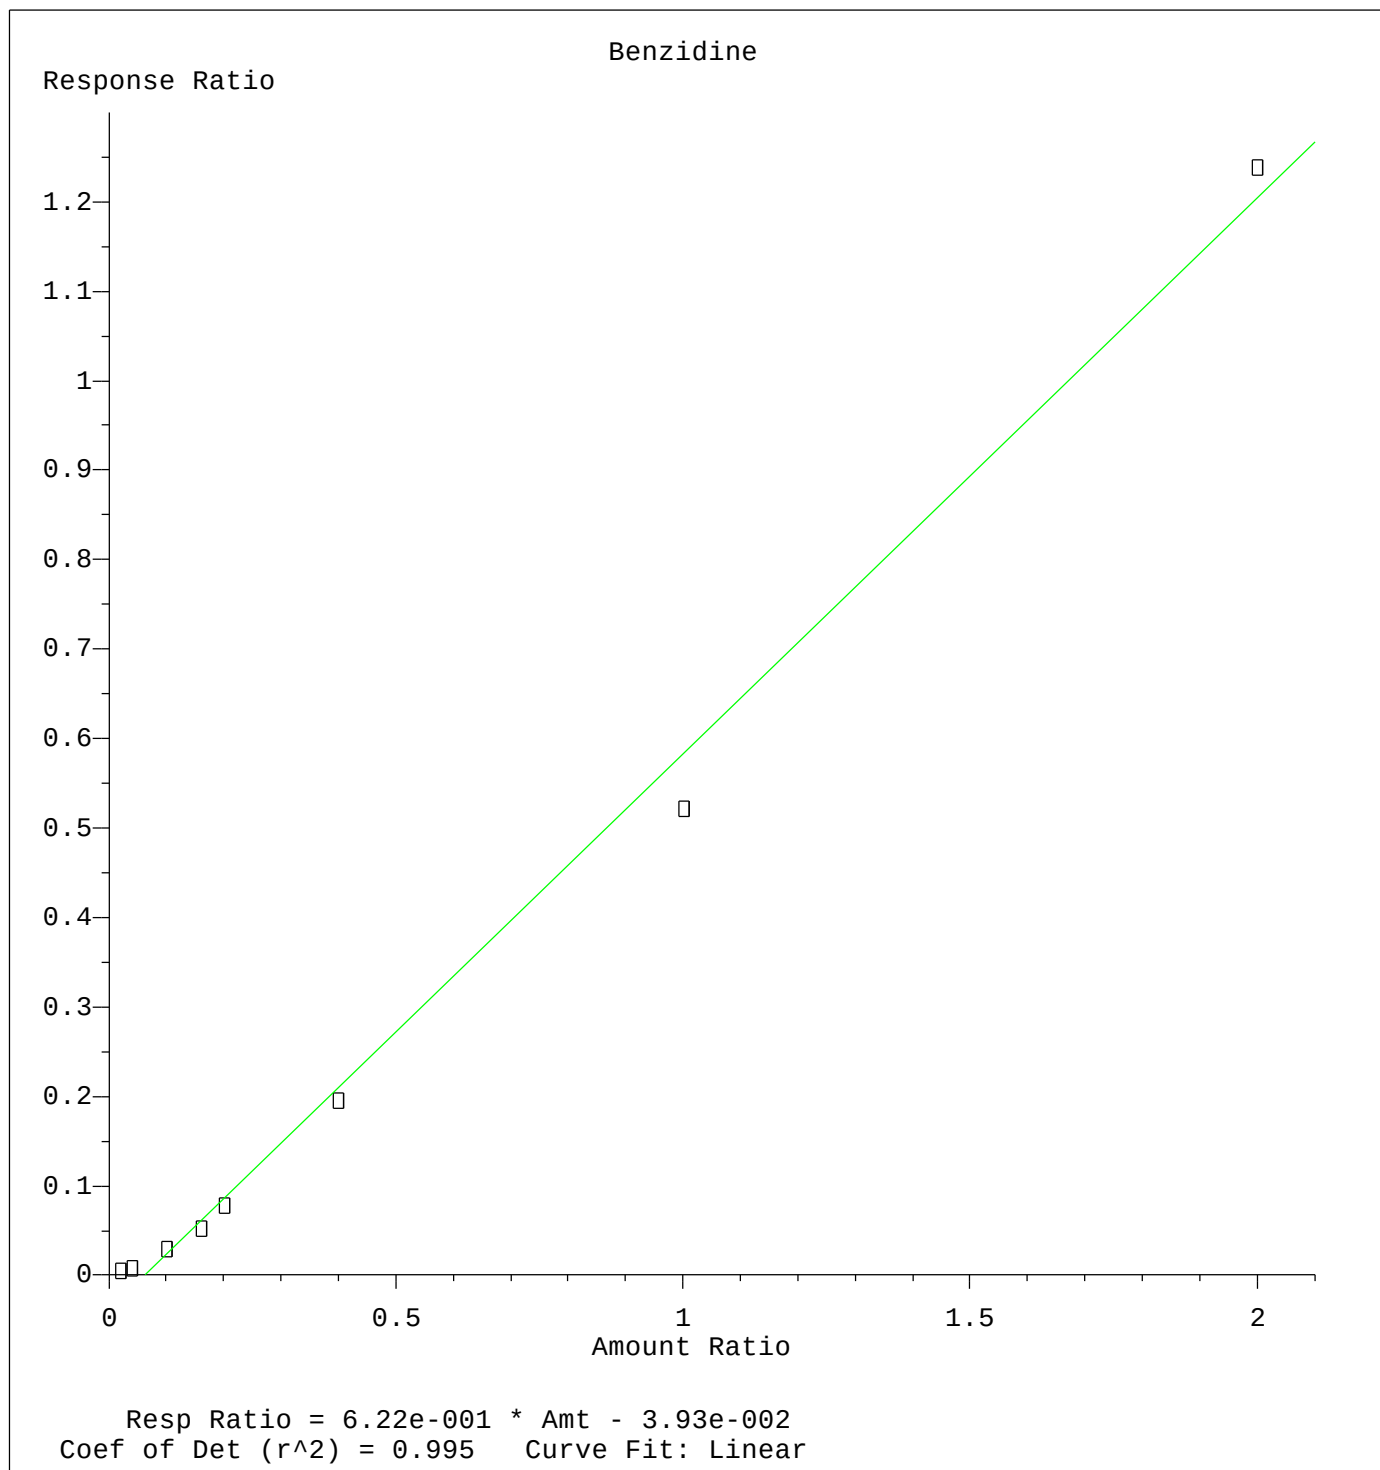

Method Name: Z:\HPCHEM1\BNA_E\METHODS\SIM-BE020215.M
Calibration Table Last Updated: Tue Feb 03 04:07:12 2015


3,3'-Dichlorobenzidine

Response Ratio

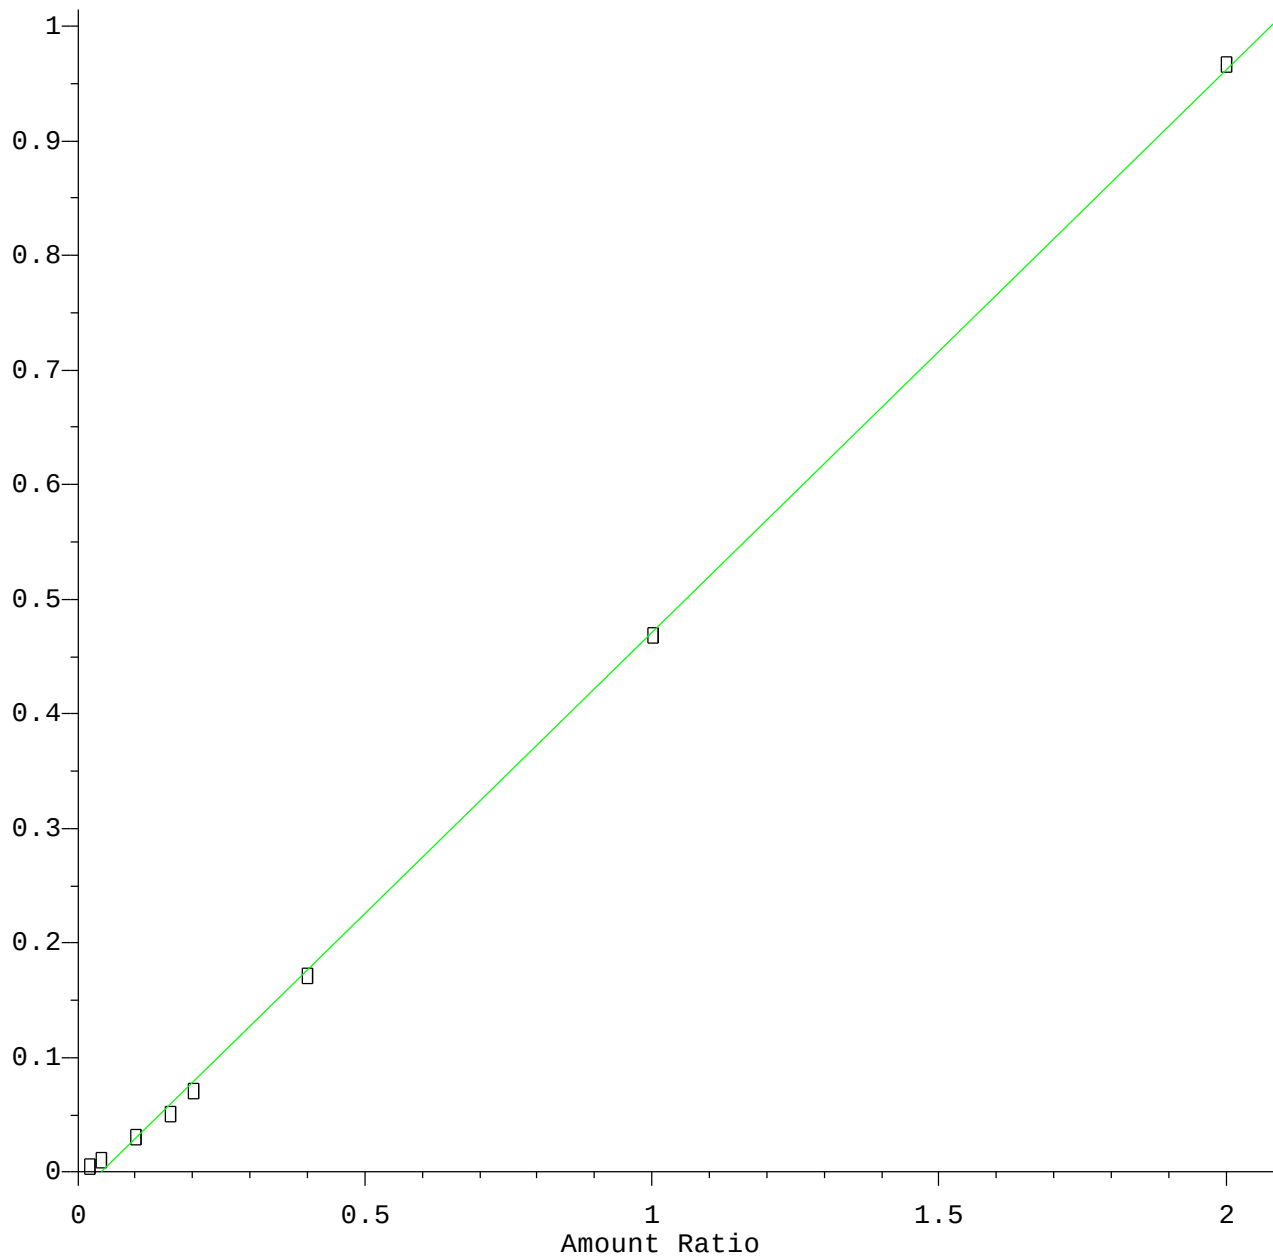


Resp Ratio = $4.90 \times 10^{-1} \times \text{Amt} - 1.90 \times 10^{-2}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear


Method Name: Z:\HPCHEM1\BNA_E\METHODS\SIM-BE020215.M
Calibration Table Last Updated: Tue Feb 03 04:07:30 2015

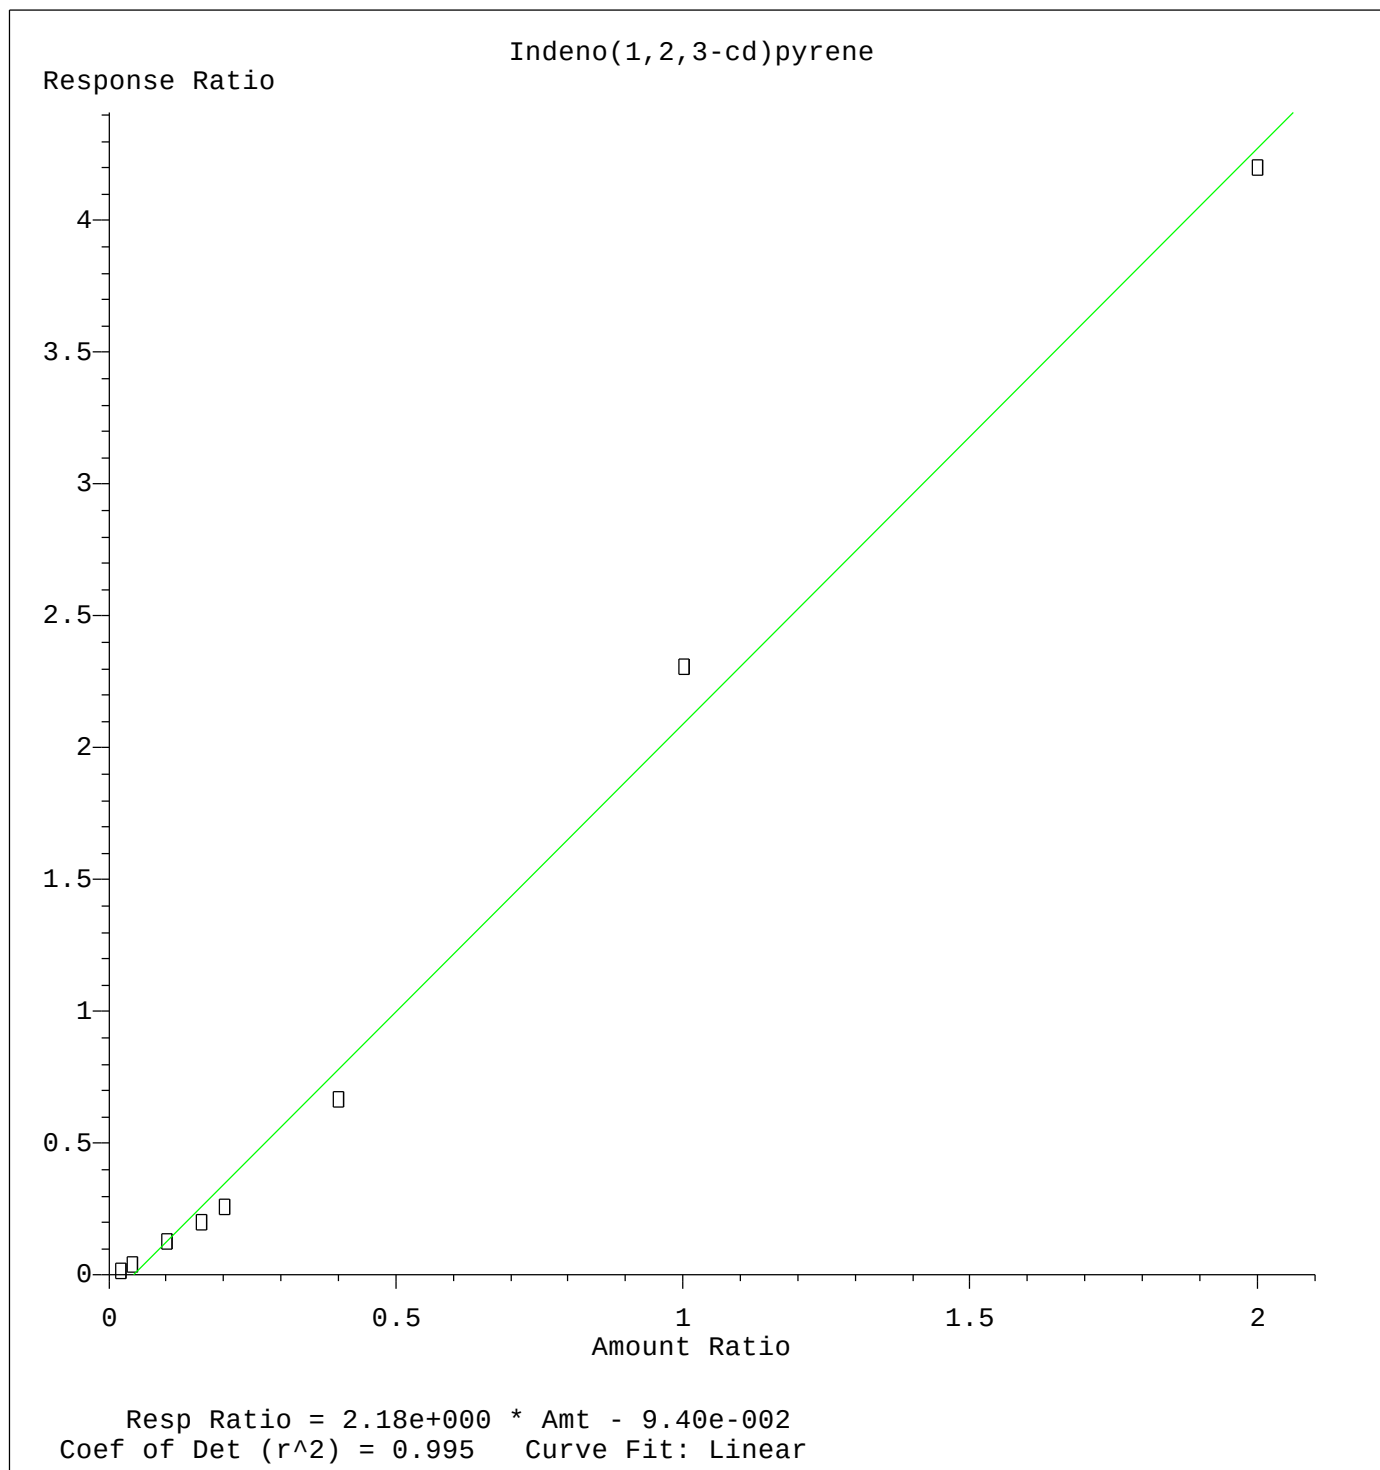

Method Name: Z:\HPCHEM1\BNA_E\METHODS\SIM-BE020215.M
Calibration Table Last Updated: Tue Feb 03 04:07:53 2015

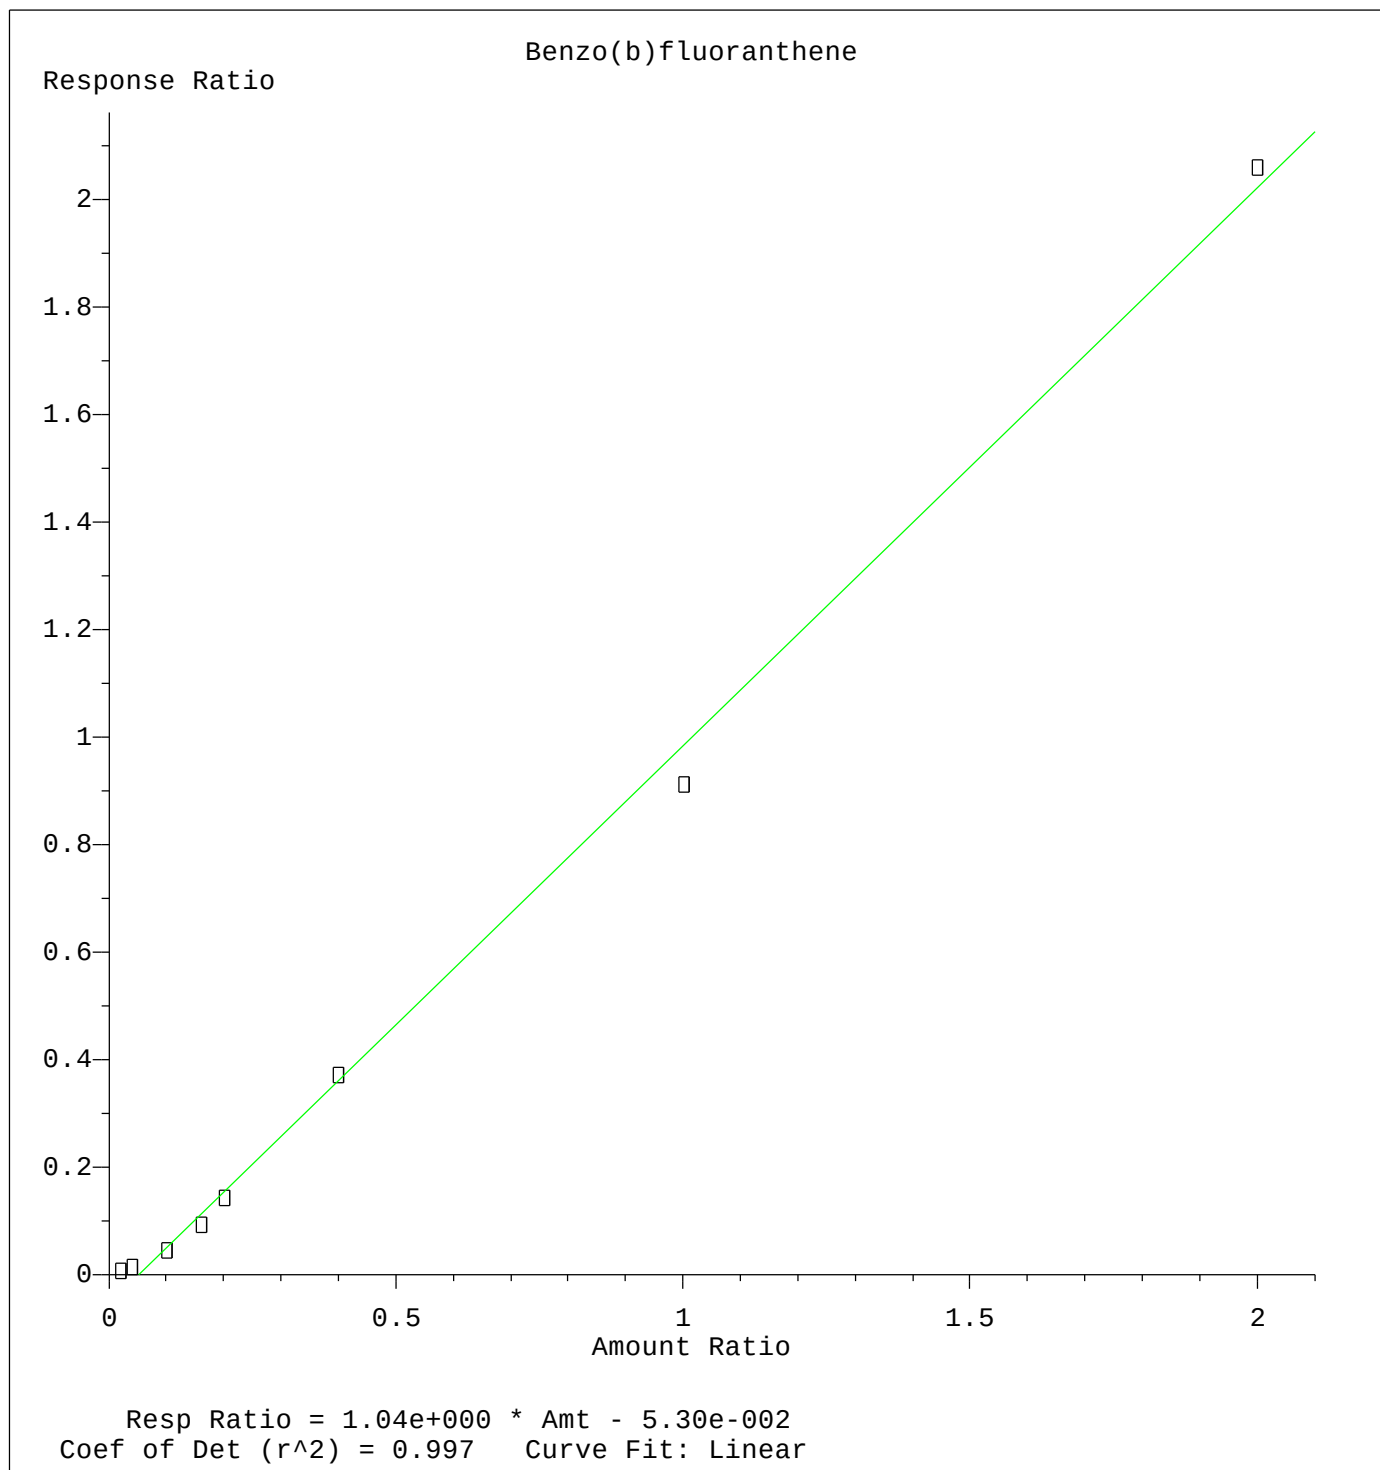


Method Name: Z:\HPCHEM1\BNA_E\METHODS\SIM-BE020215.M
Calibration Table Last Updated: Tue Feb 03 04:08:13 2015

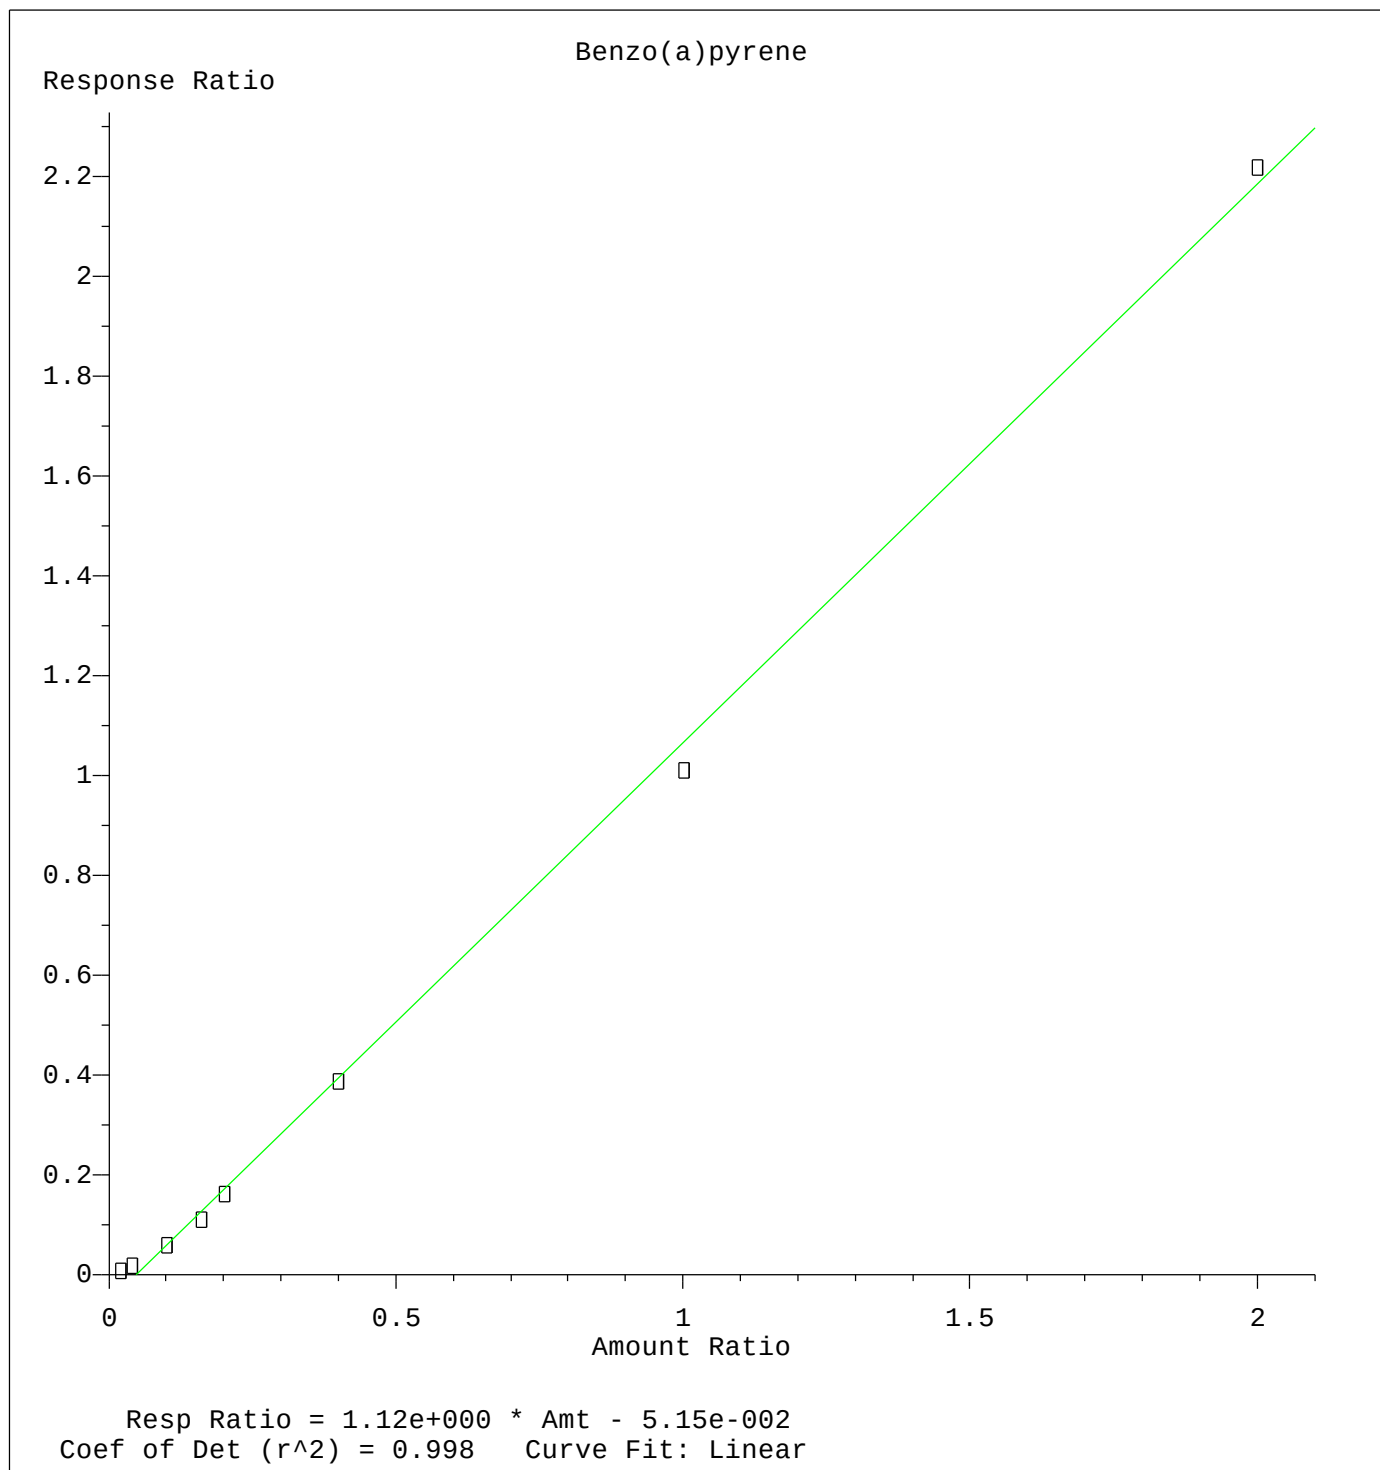

Method Name: Z:\HPCHEM1\BNA_E\METHODS\SIM-BE020215.M
Calibration Table Last Updated: Tue Feb 03 04:08:31 2015

Dibenzo(a,h)anthracene

Response Ratio

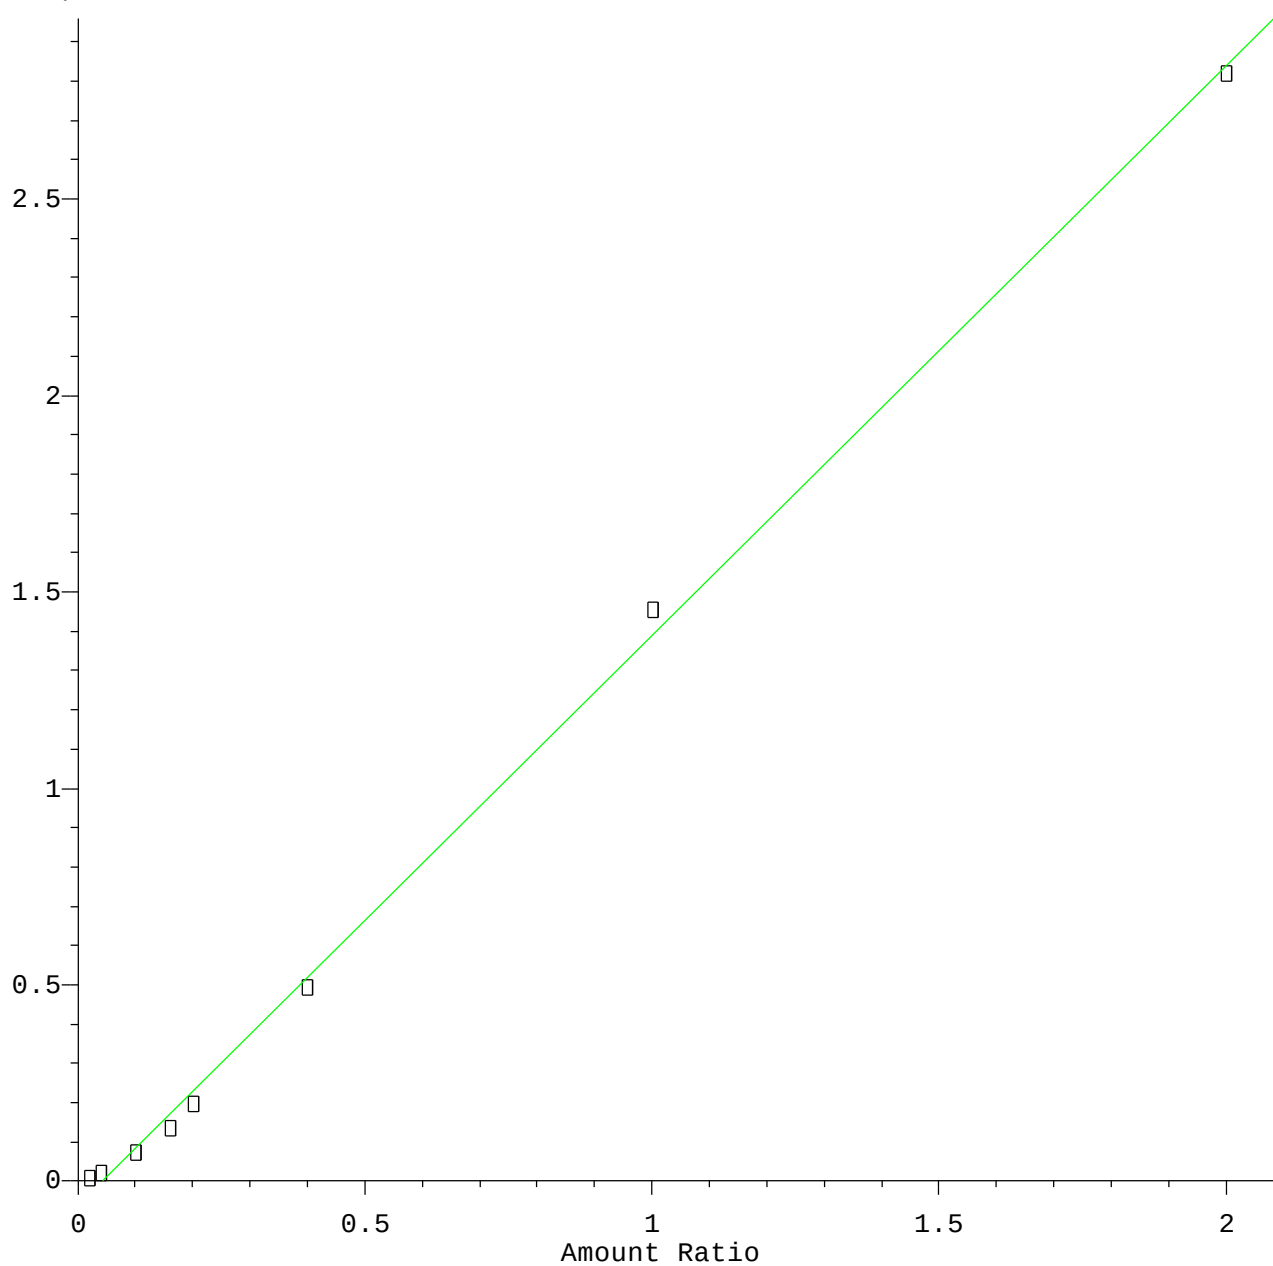

Resp Ratio = 1.45e+000 * Amt - 6.27e-002
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA_E\METHODS\SIM-BE020215.M
Calibration Table Last Updated: Tue Feb 03 04:08:48 2015