


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE020215\
 Data File : BE089454.D
 Acq On : 2 Feb 2015 13:53
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\SIM-BE020215.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Feb 03 11:20:27 2015

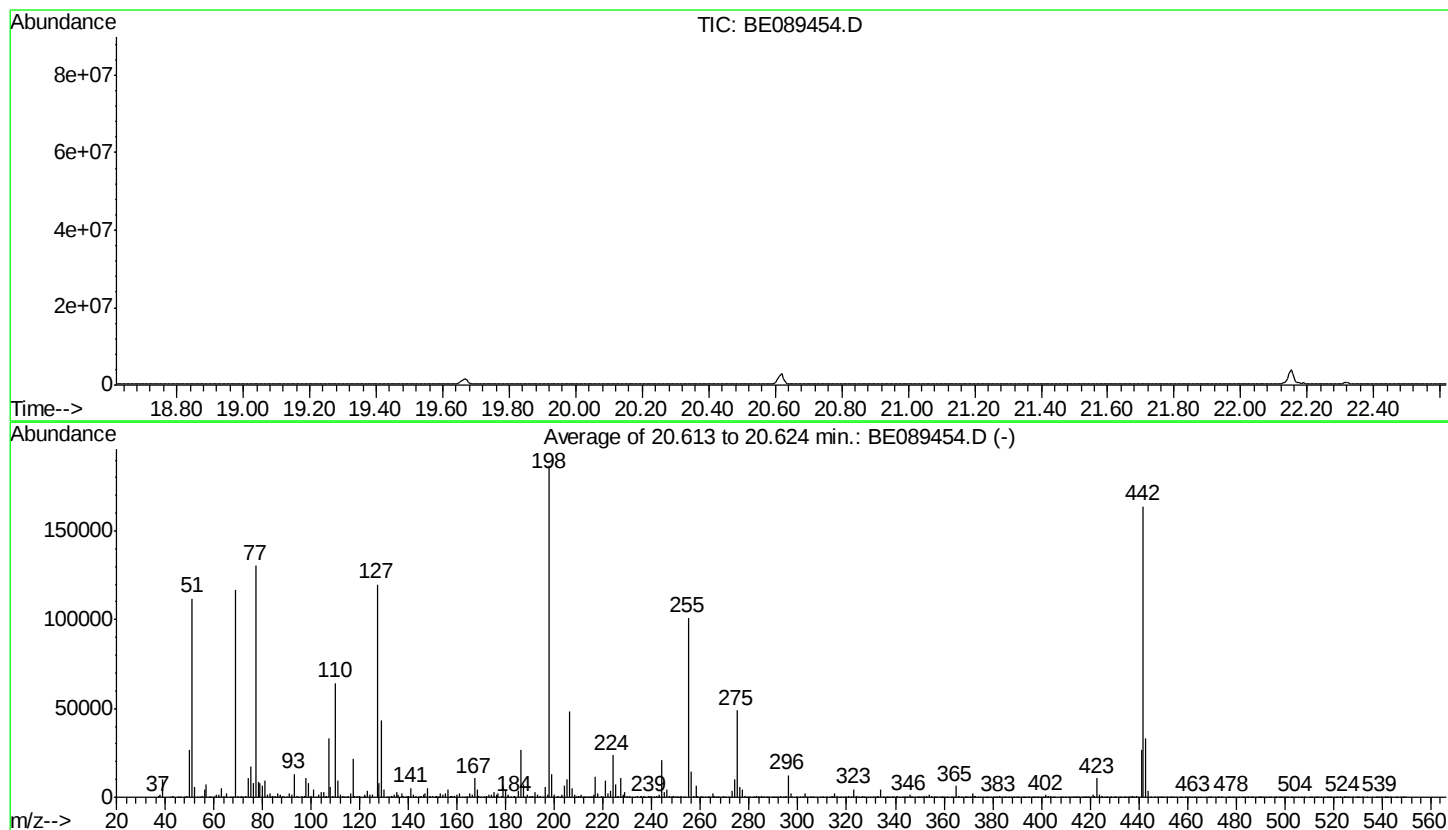

AutoFind: Scans 3272, 3273, 3274; Background Corrected with Scan 3264

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	60.0	112102	PASS
68	69	0.00	2	0.3	337	PASS
69	198	0.00	100	62.6	116855	PASS
70	69	0.00	2	0.4	436	PASS
127	198	10	80	64.2	119849	PASS
197	198	0.00	2	0.8	1446	PASS
198	198	100	100	100.0	186792	PASS
199	198	5	9	6.9	12962	PASS
275	198	10	60	26.1	48747	PASS
365	198	1	100	3.3	6229	PASS
441	442	0.01	24	16.5	26968	PASS
442	198	50	100	87.7	163739	PASS
443	442	15	24	20.1	32936	PASS