




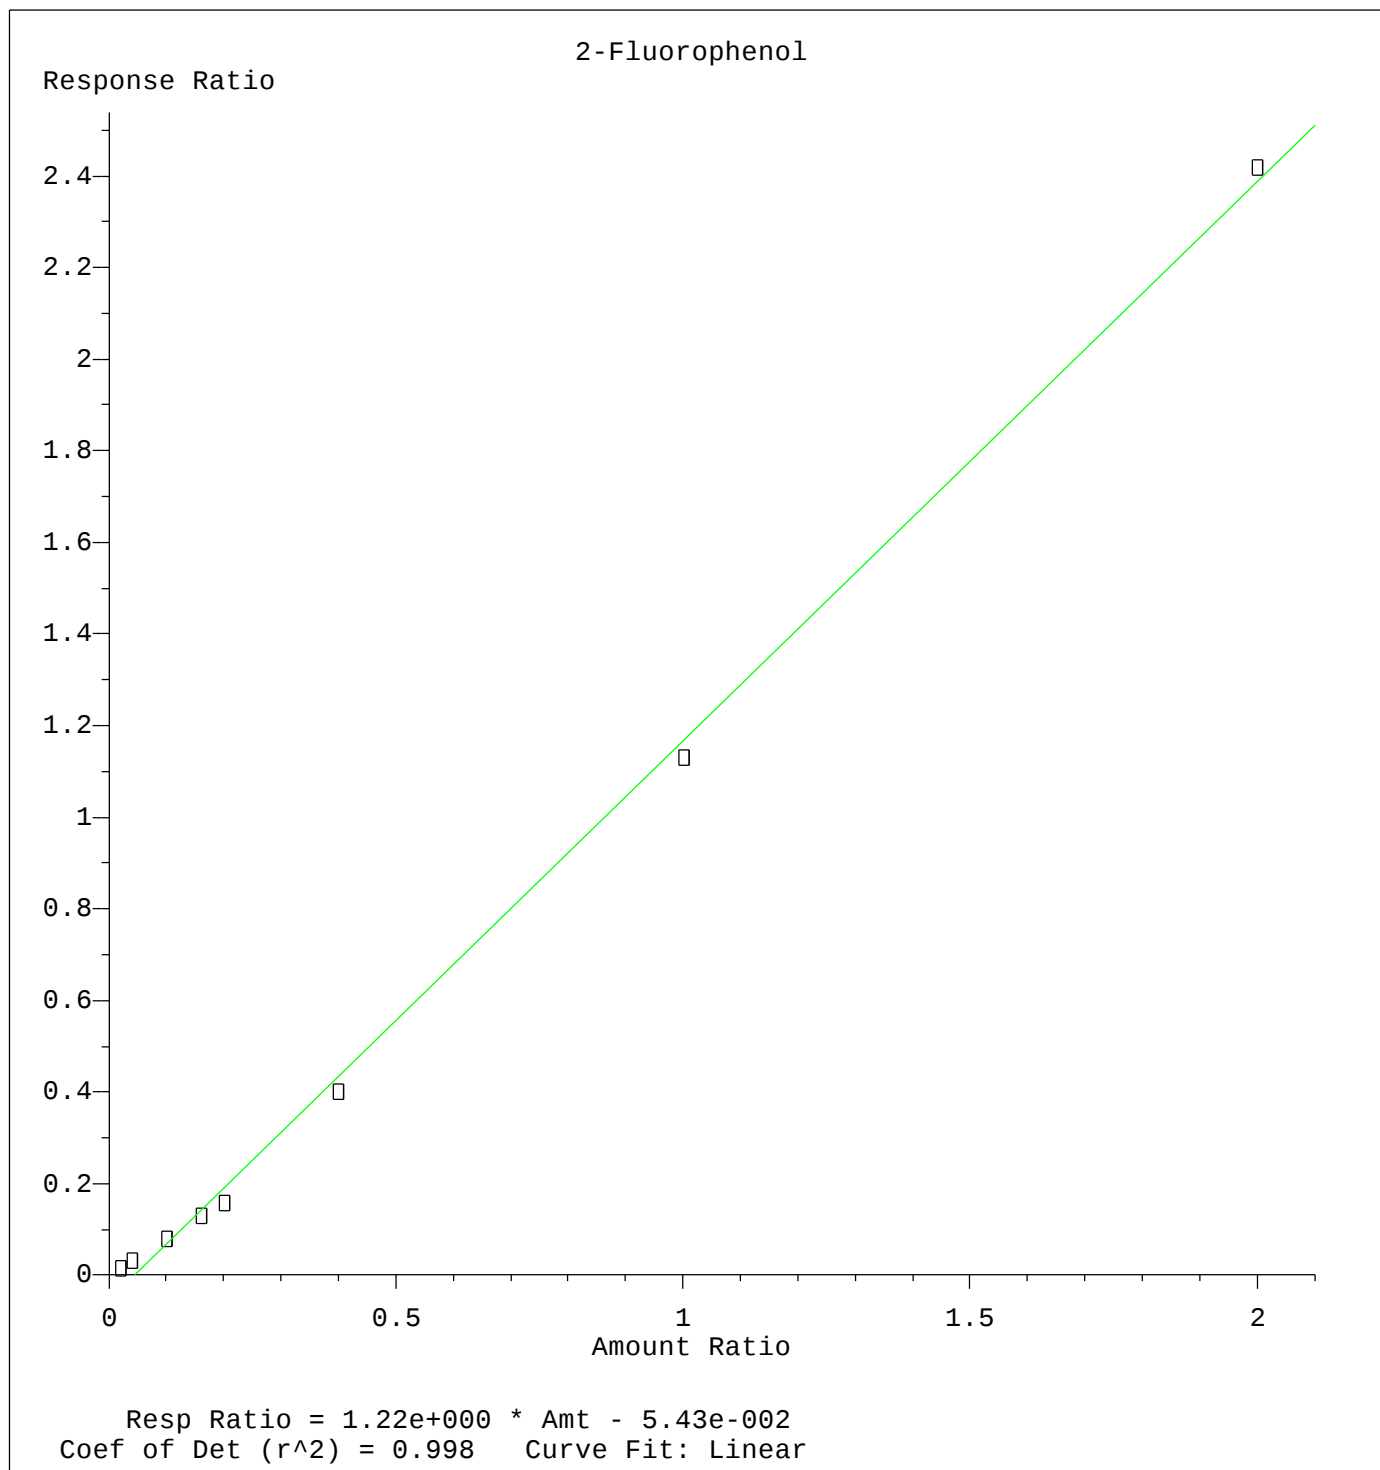

Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE020216.M
Calibration Table Last Updated: Wed Feb 03 00:27:53 2016

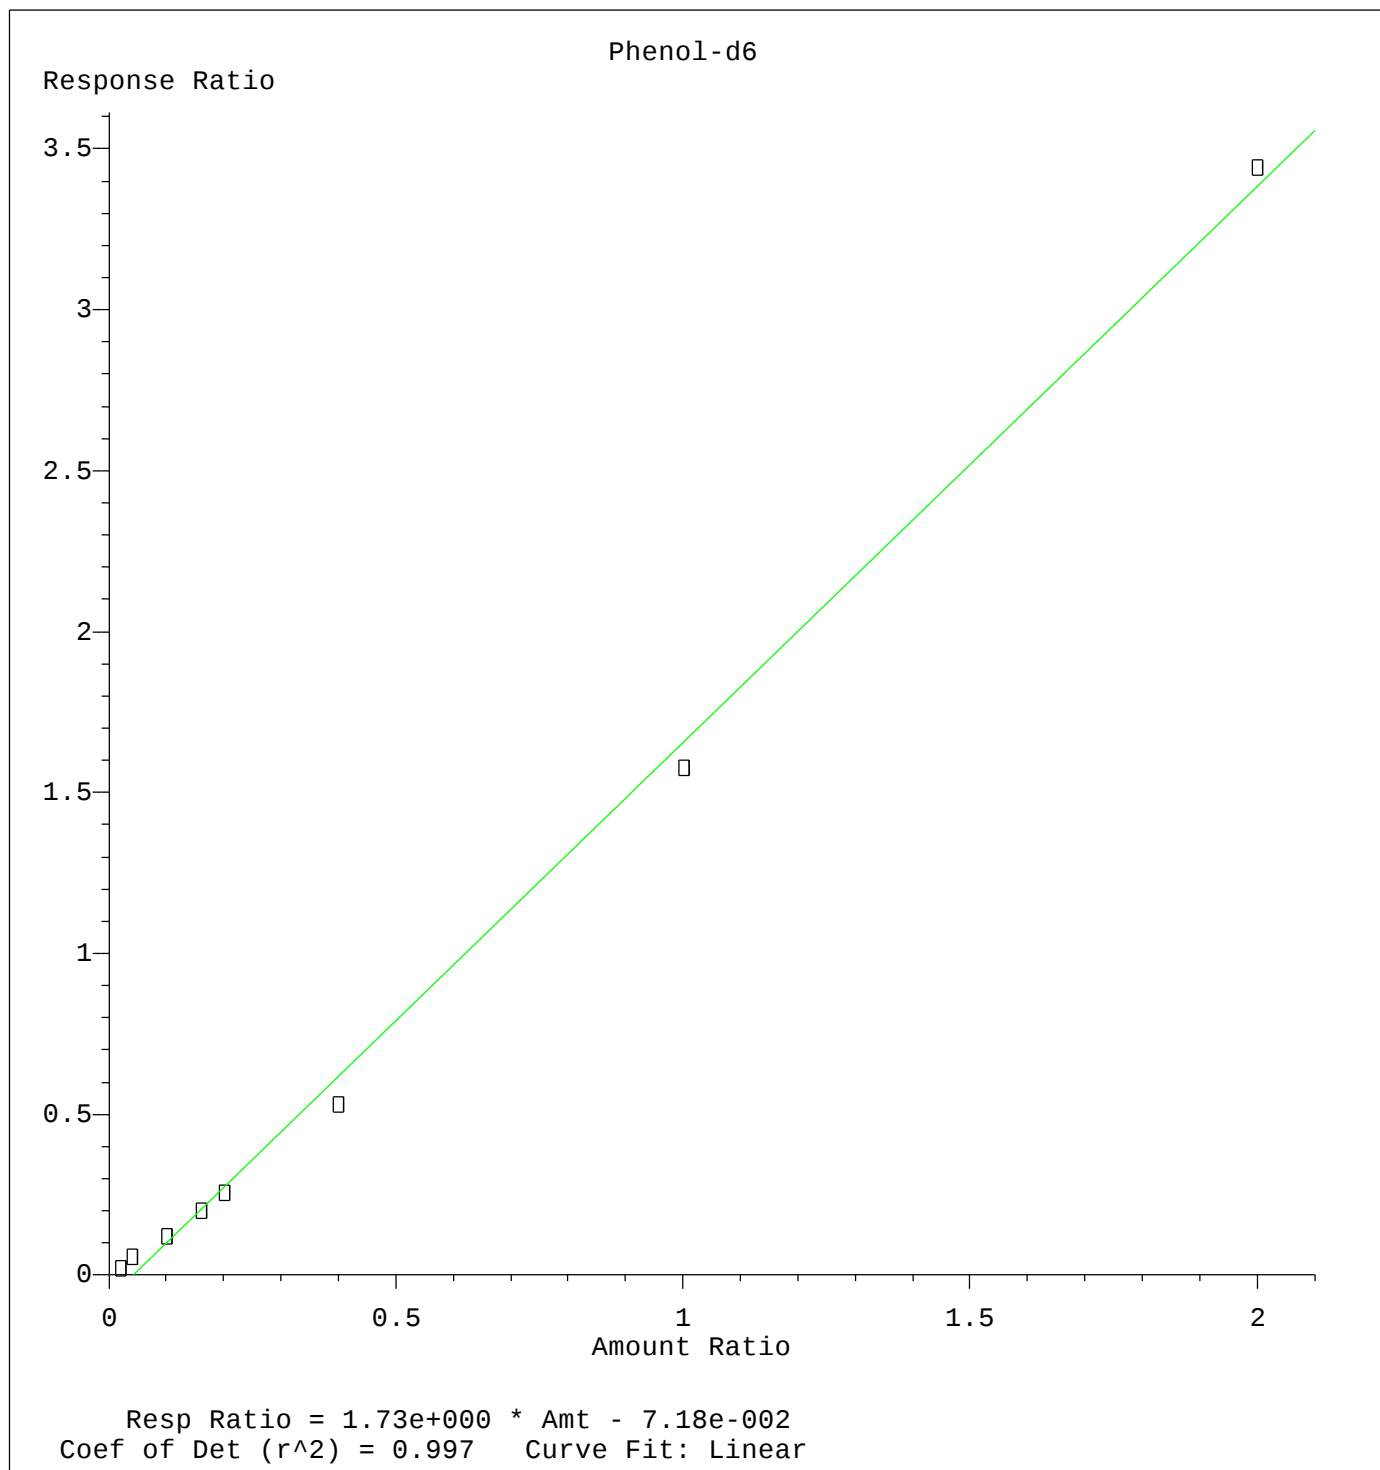


Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE020216.M
Calibration Table Last Updated: Wed Feb 03 00:27:53 2016

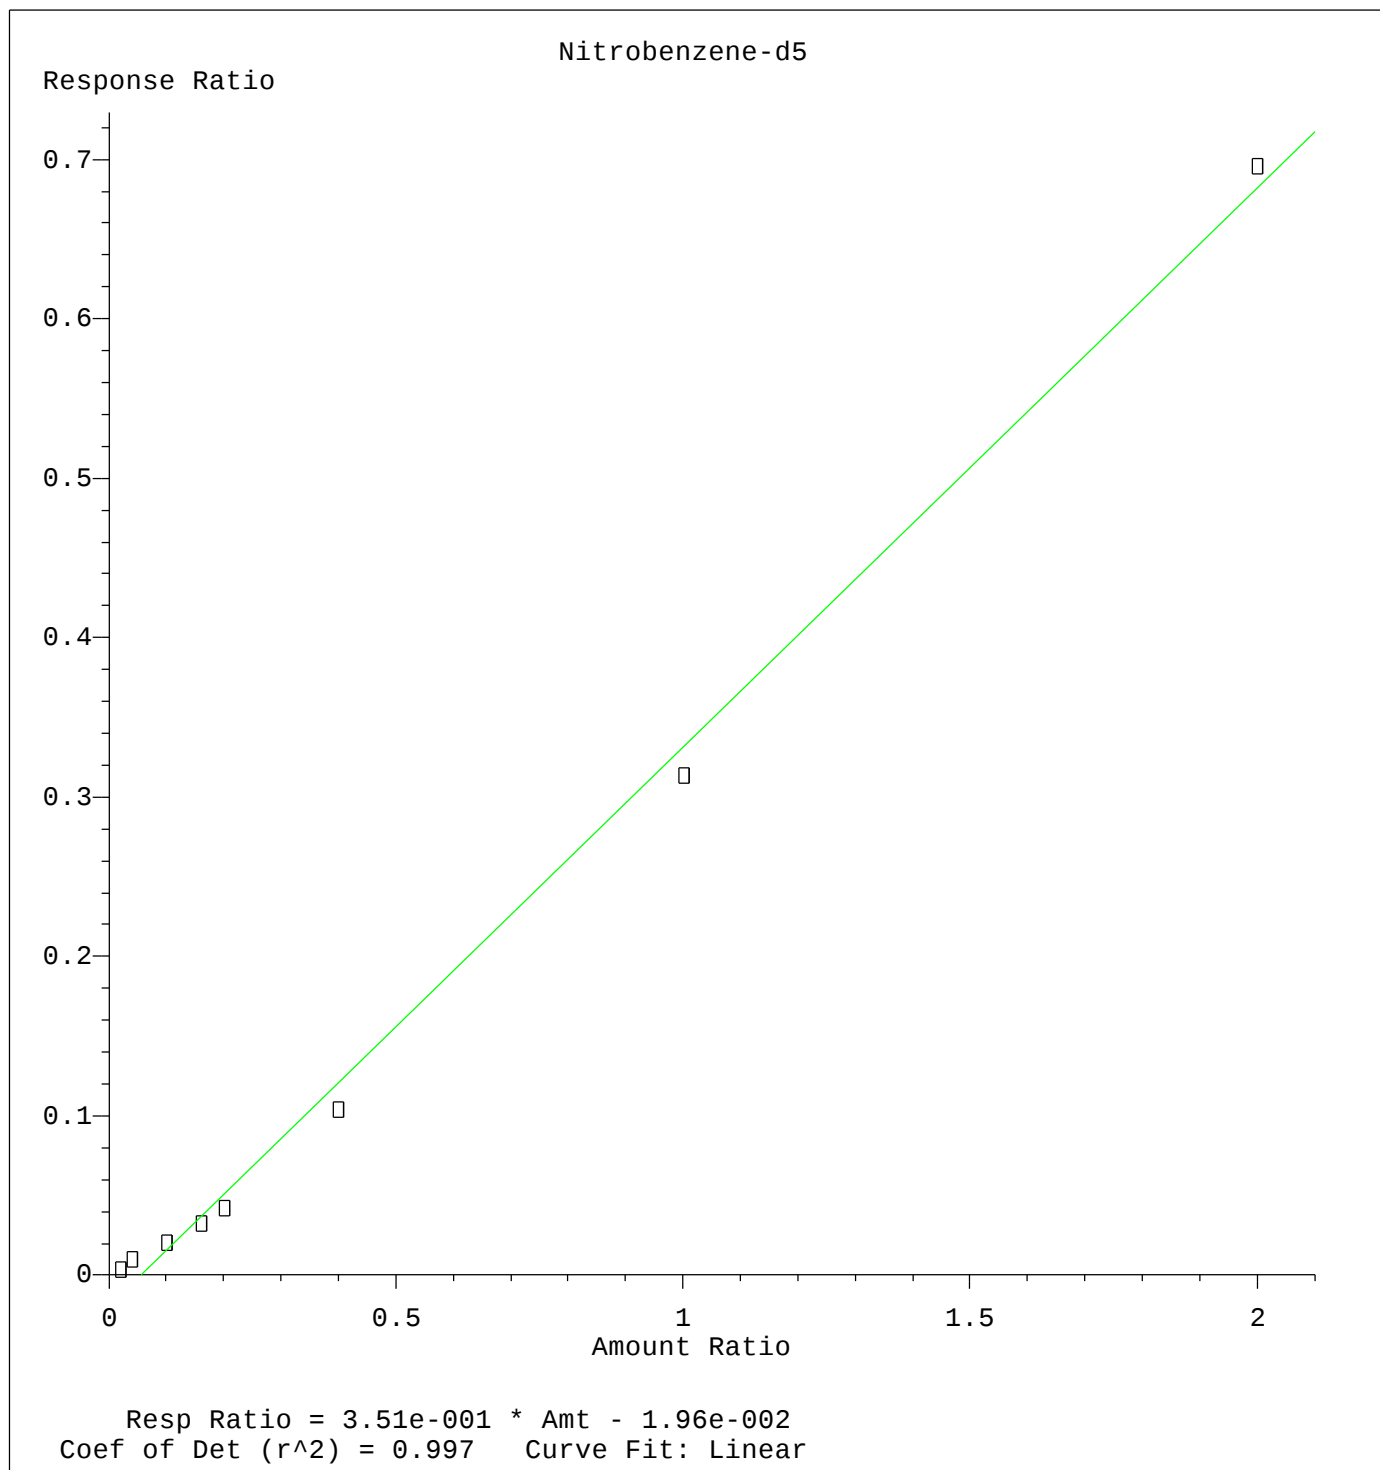

Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE020216.M
Calibration Table Last Updated: Wed Feb 03 00:27:53 2016


2-Methylnaphthalene

Response Ratio

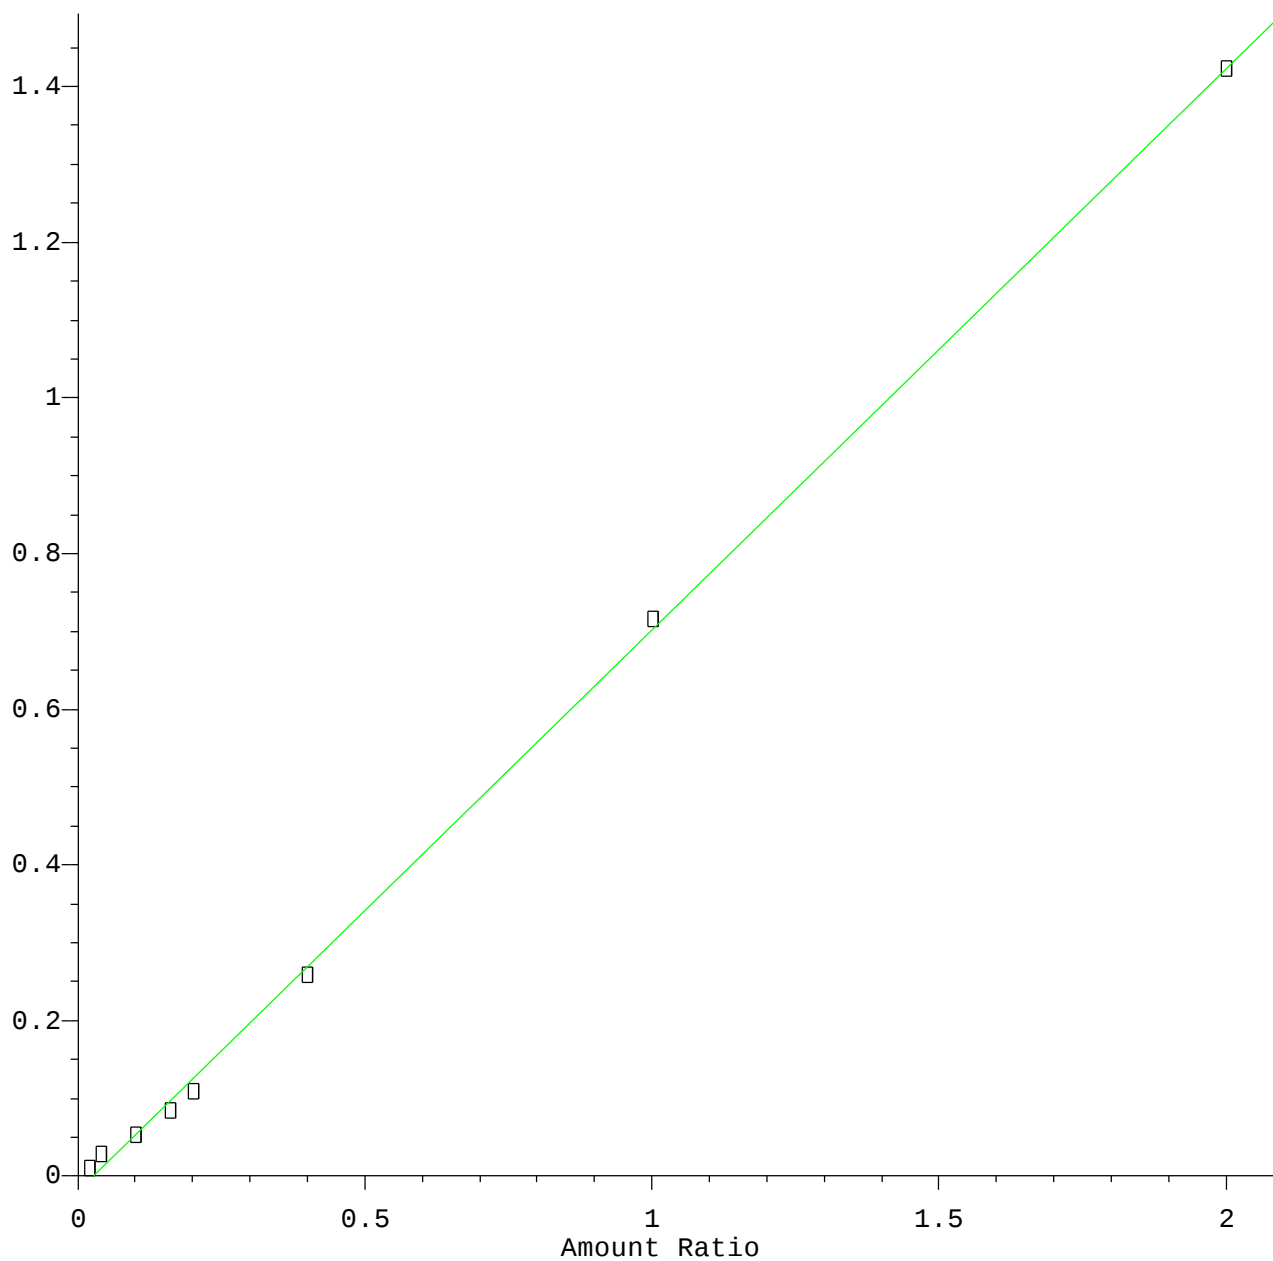

Resp Ratio = $7.21 \times 10^{-1} \times \text{Amt} - 1.86 \times 10^{-2}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear


Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE020216.M
Calibration Table Last Updated: Wed Feb 03 00:27:53 2016

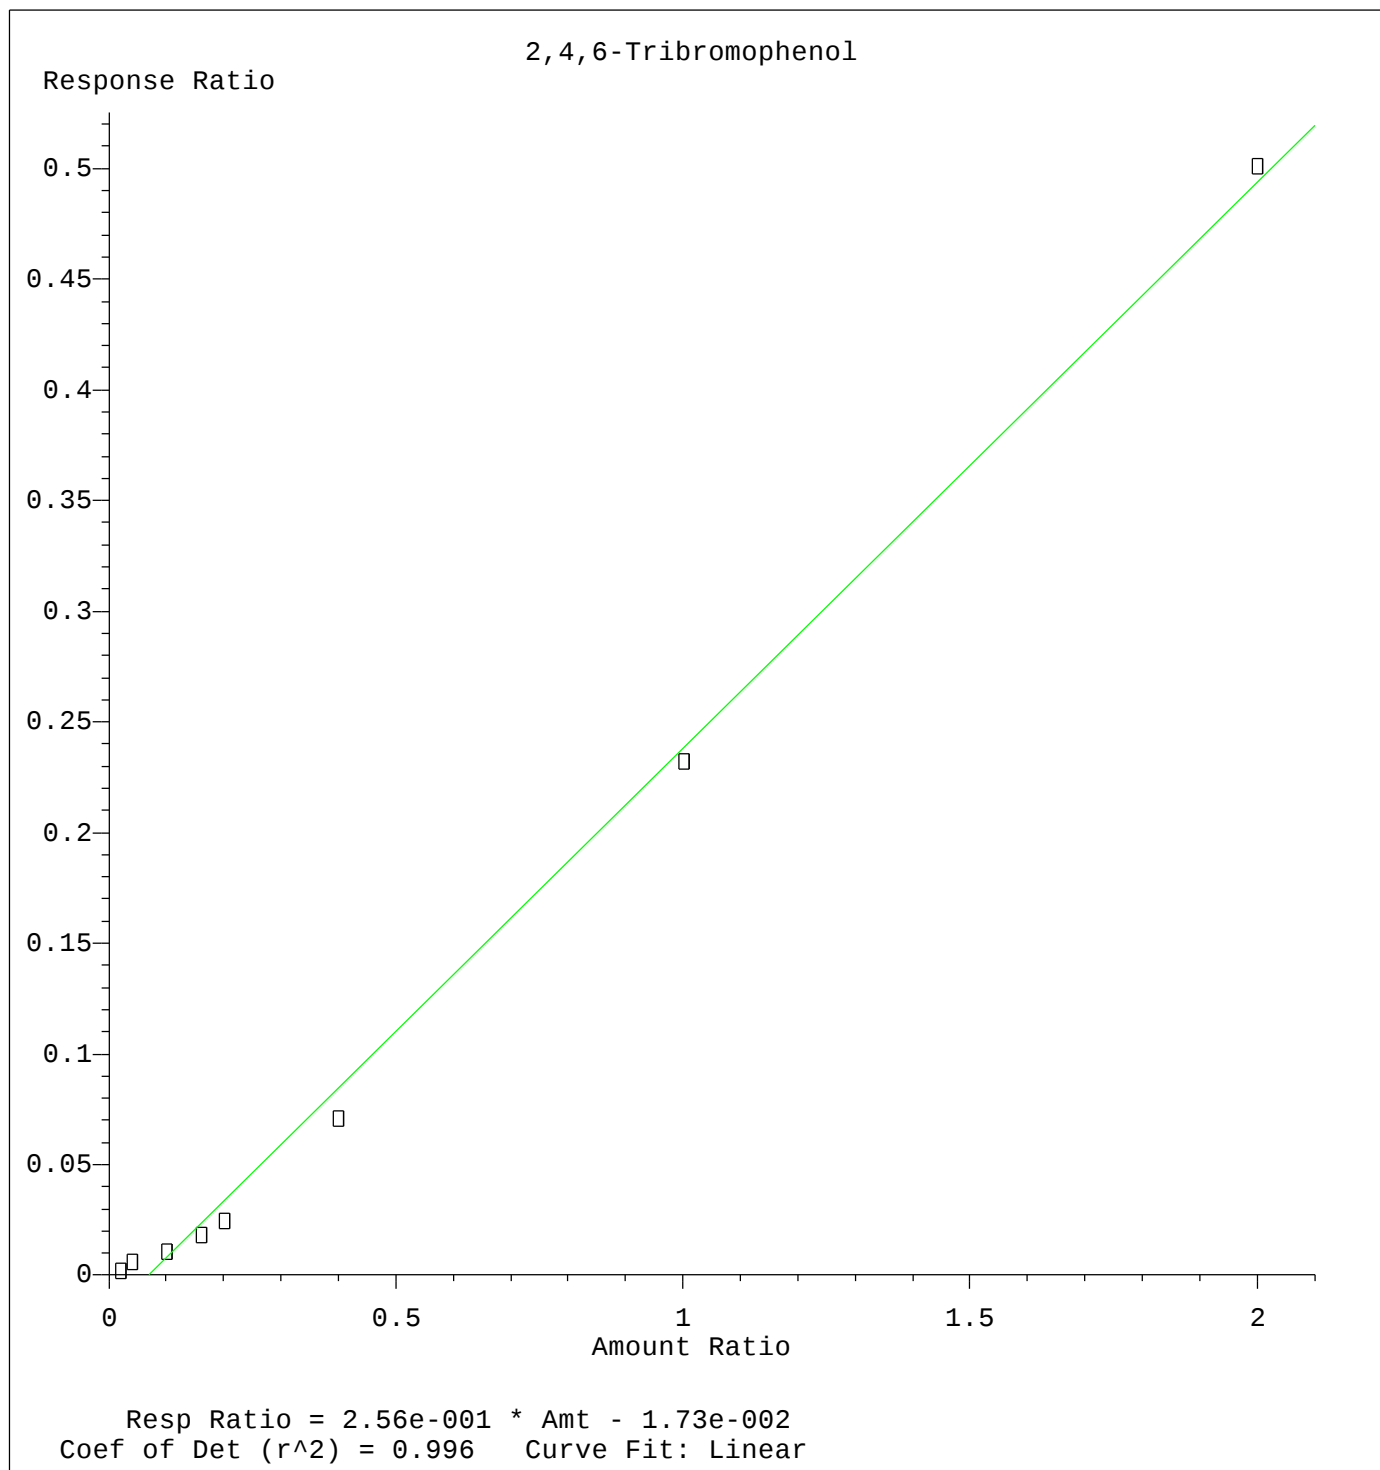

Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE020216.M
Calibration Table Last Updated: Wed Feb 03 00:27:53 2016


Acenaphthylene

Response Ratio

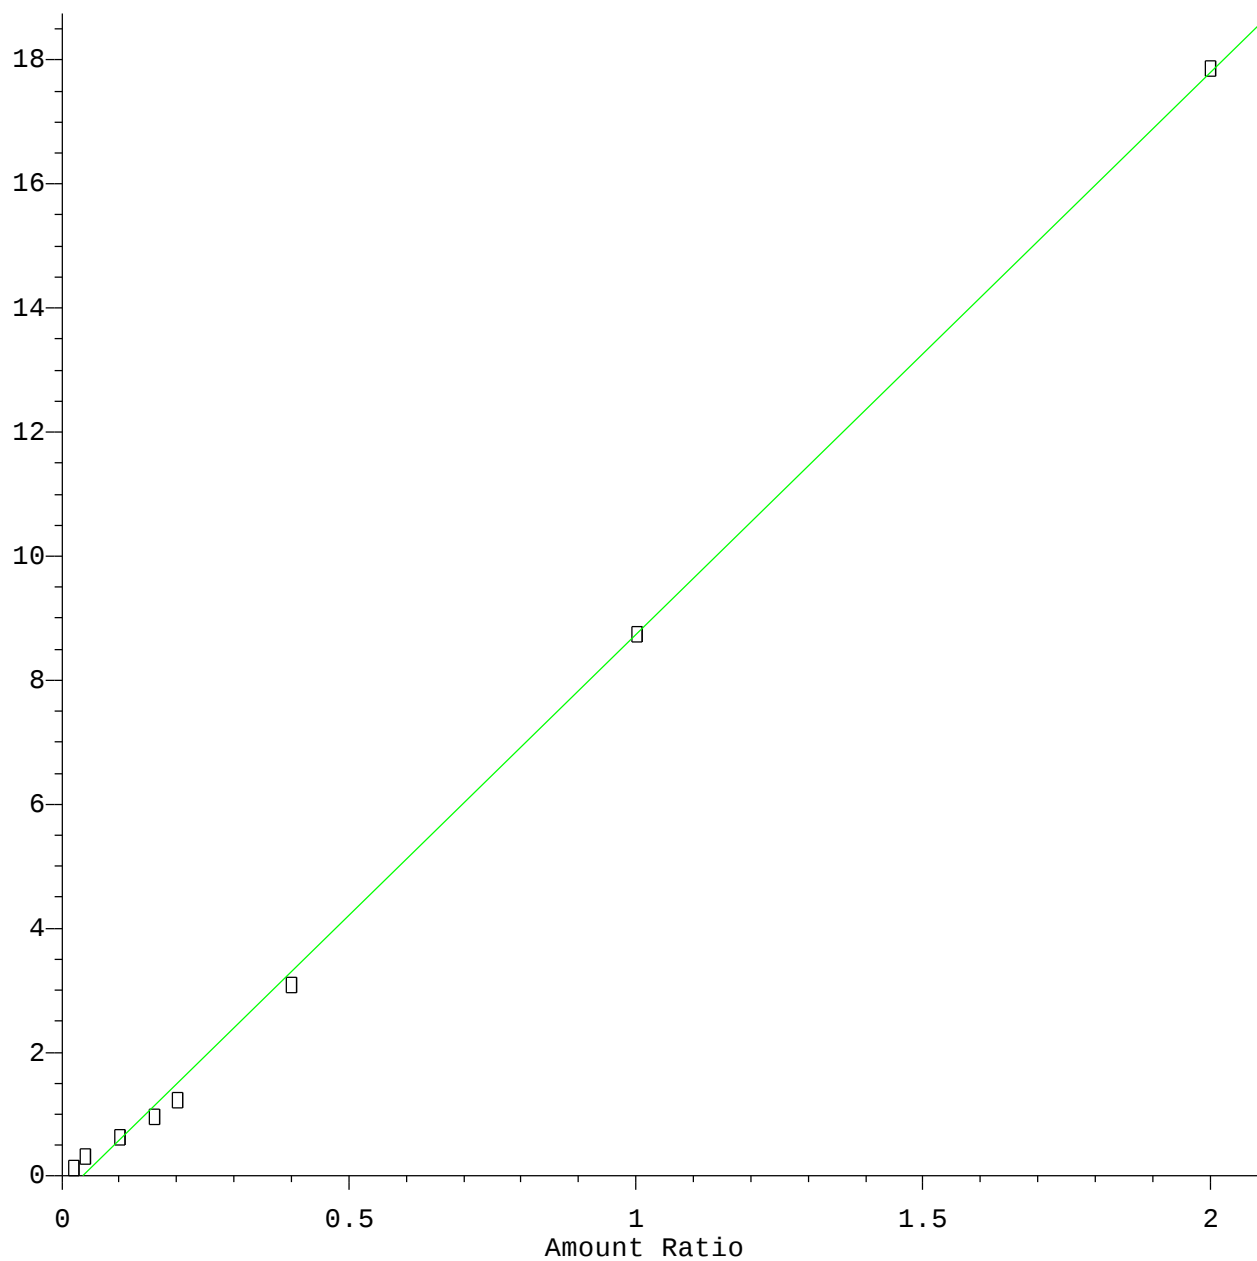


Resp Ratio = 9.05×10^0 * Amt - 3.26×10^{-1}
Coef of Det (r^2) = 0.999 Curve Fit: Linear


Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE020216.M
Calibration Table Last Updated: Wed Feb 03 00:27:53 2016

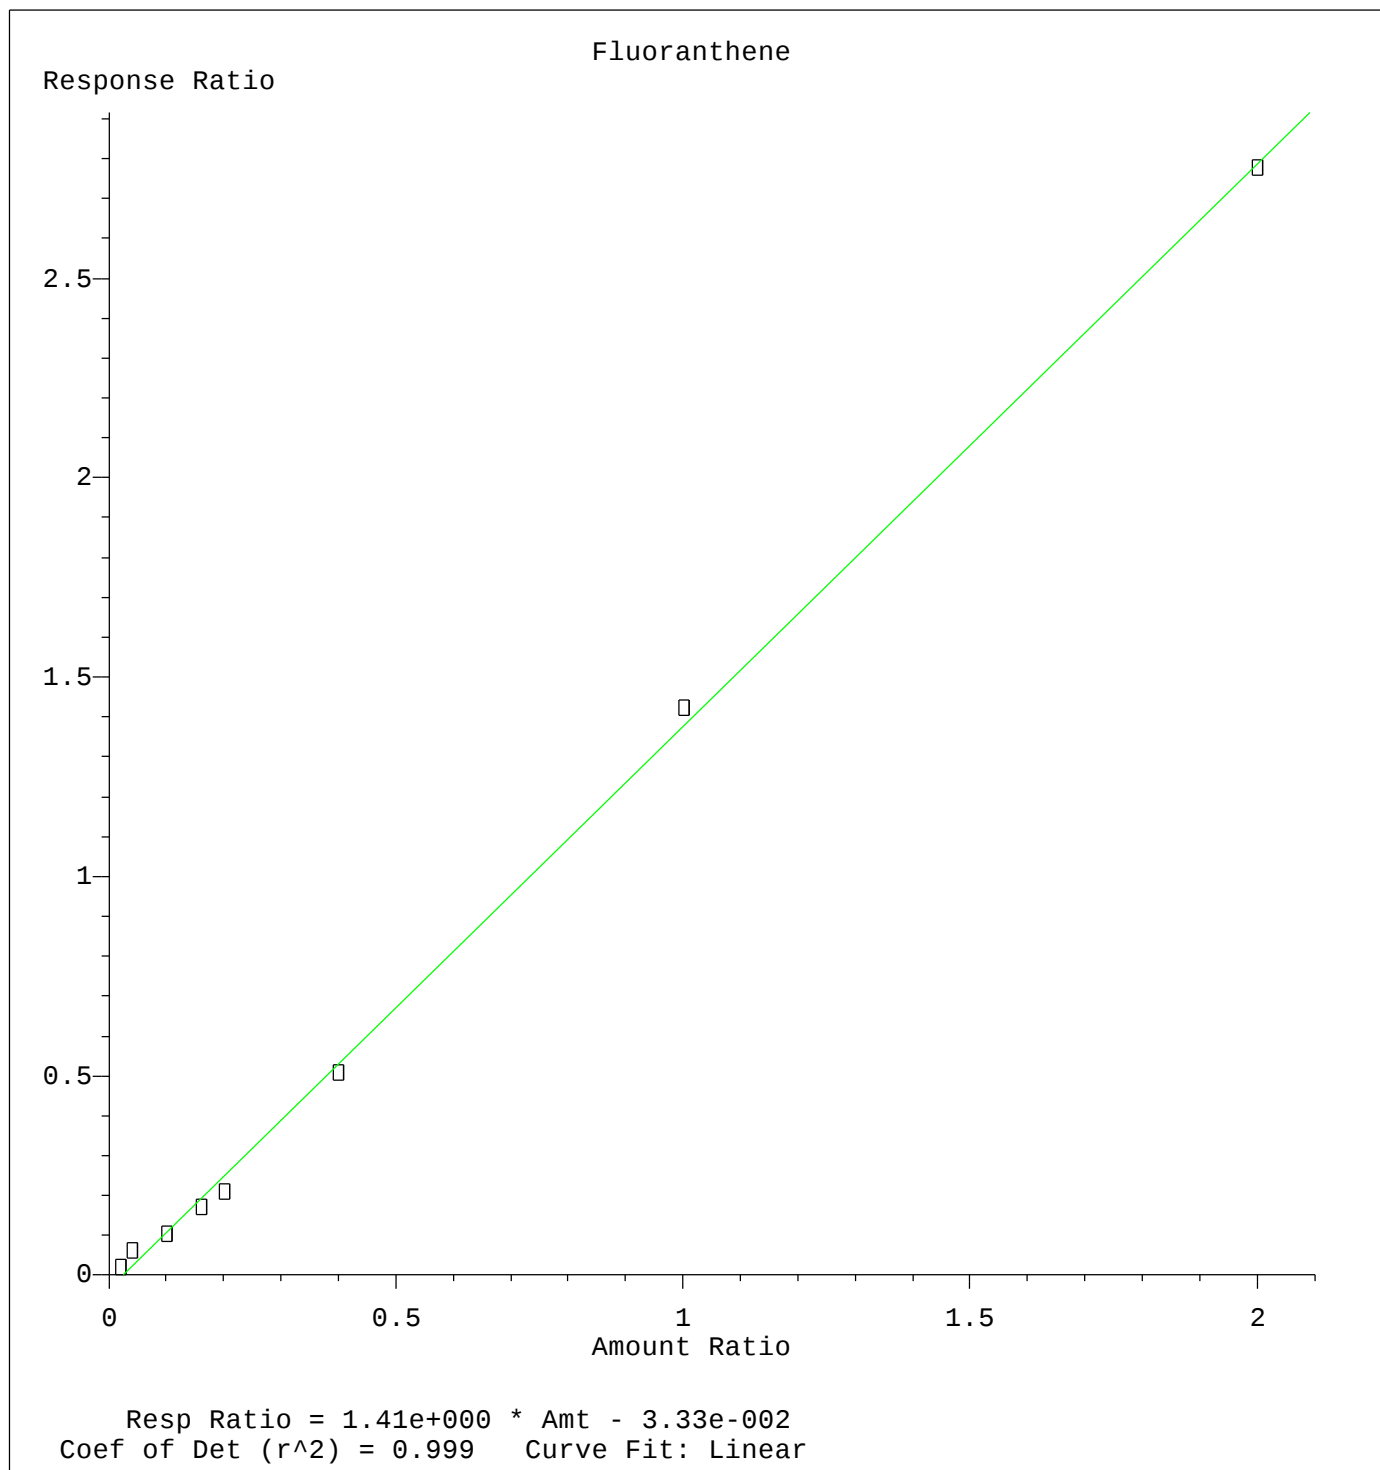


Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE020216.M
Calibration Table Last Updated: Wed Feb 03 00:27:53 2016

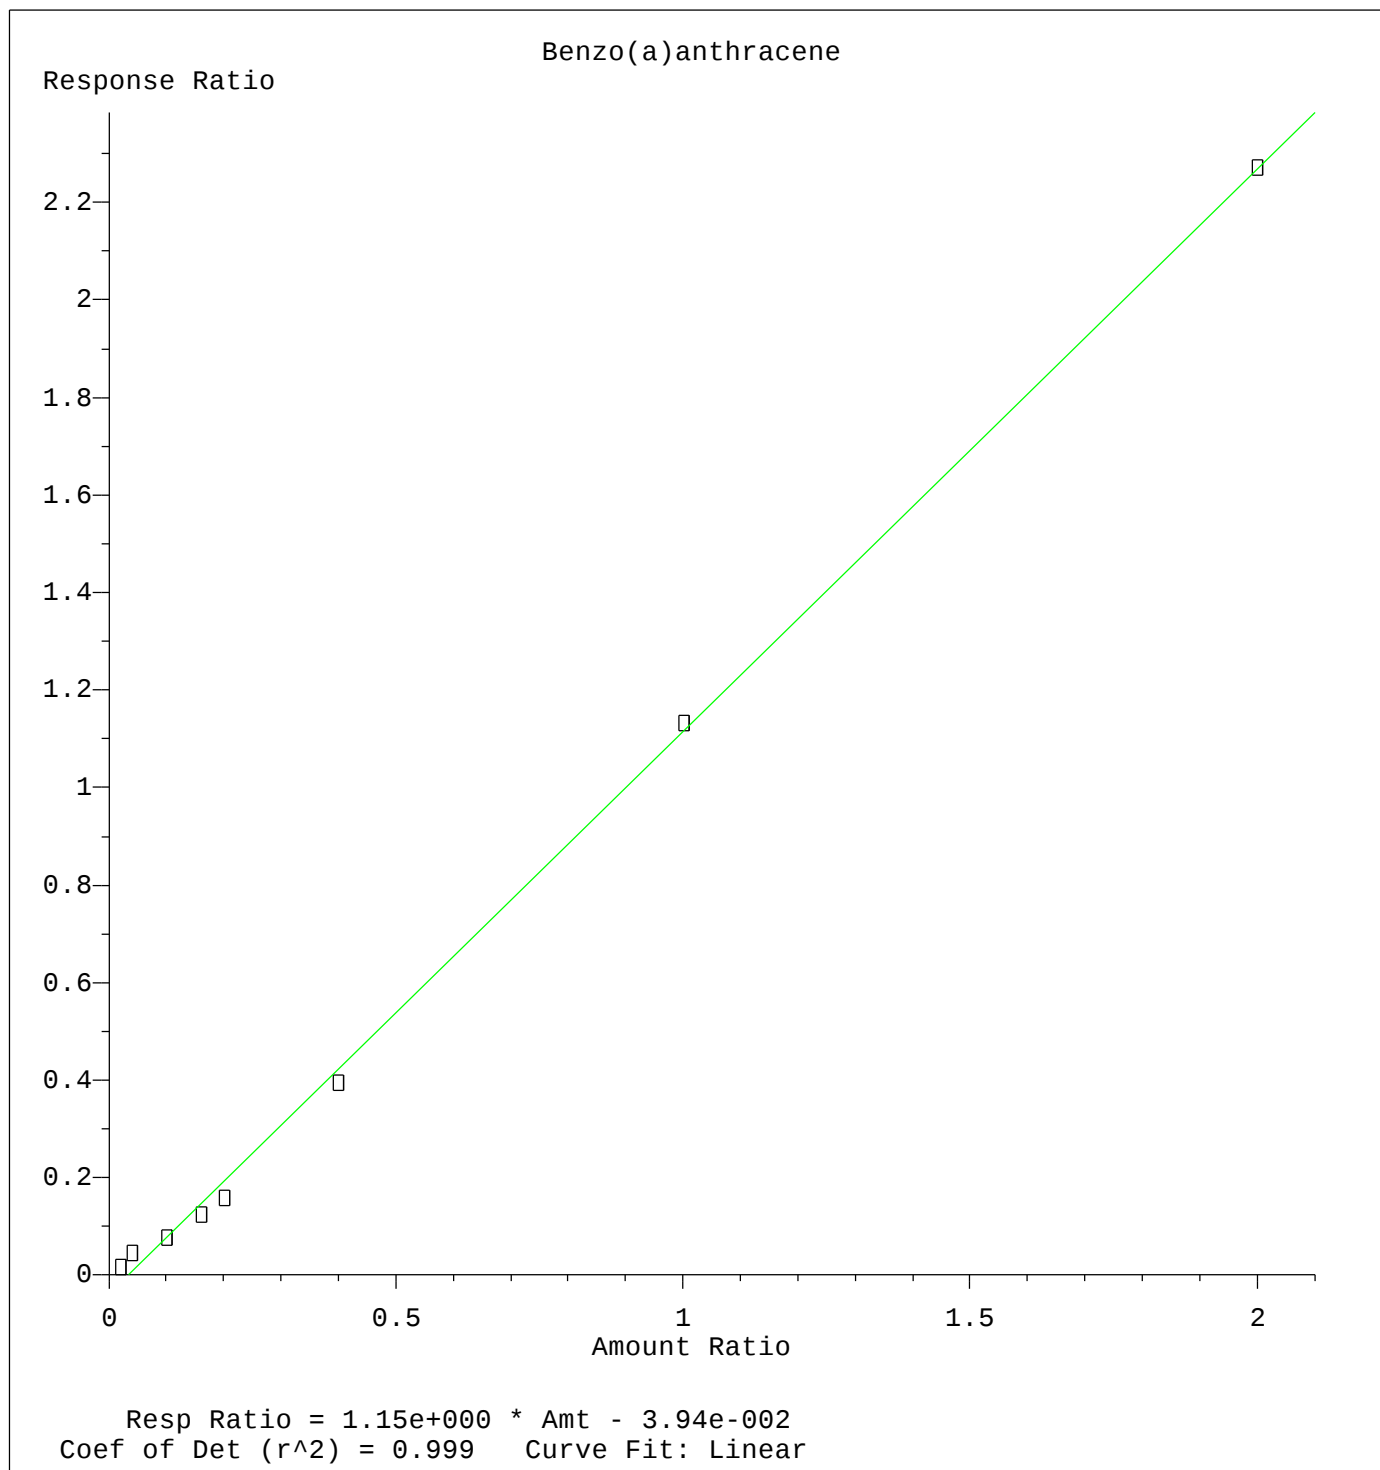


Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE020216.M
Calibration Table Last Updated: Wed Feb 03 00:27:53 2016

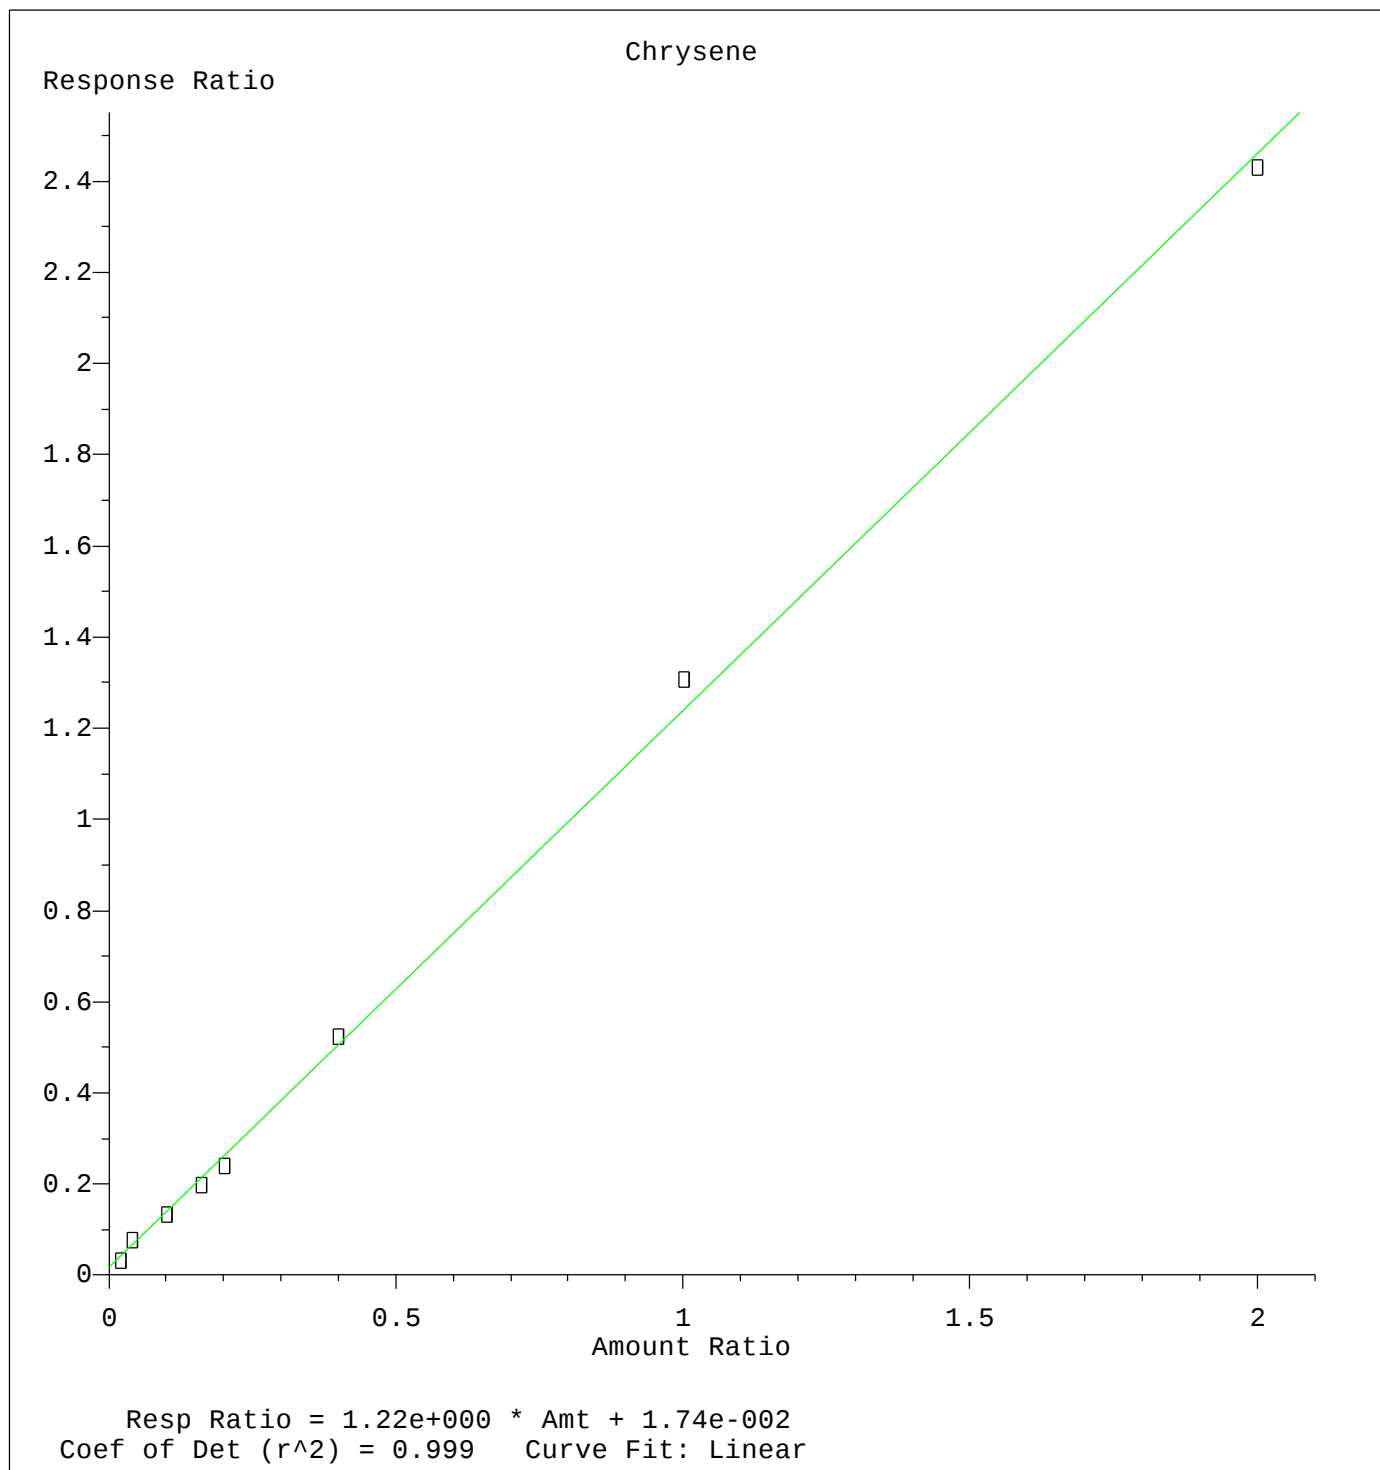

Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE020216.M
Calibration Table Last Updated: Wed Feb 03 00:27:53 2016

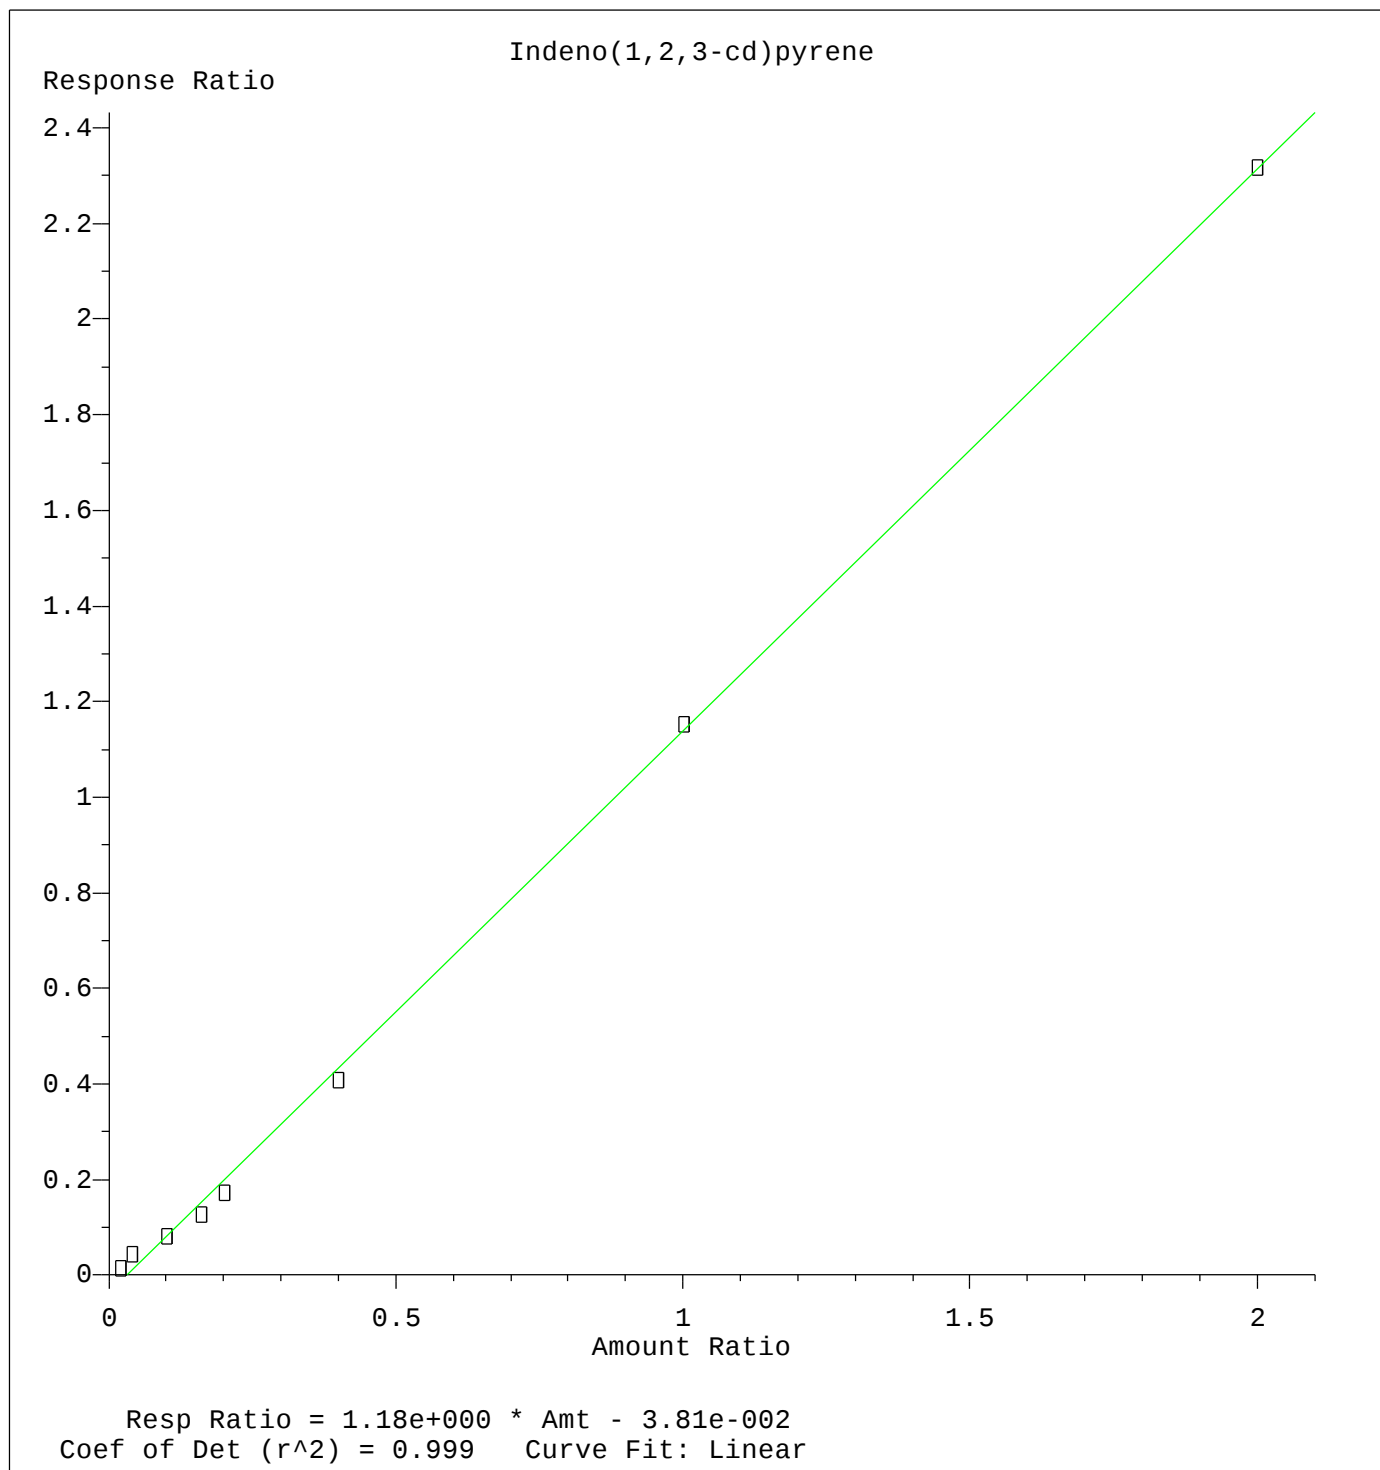


Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE020216.M
Calibration Table Last Updated: Wed Feb 03 00:27:53 2016

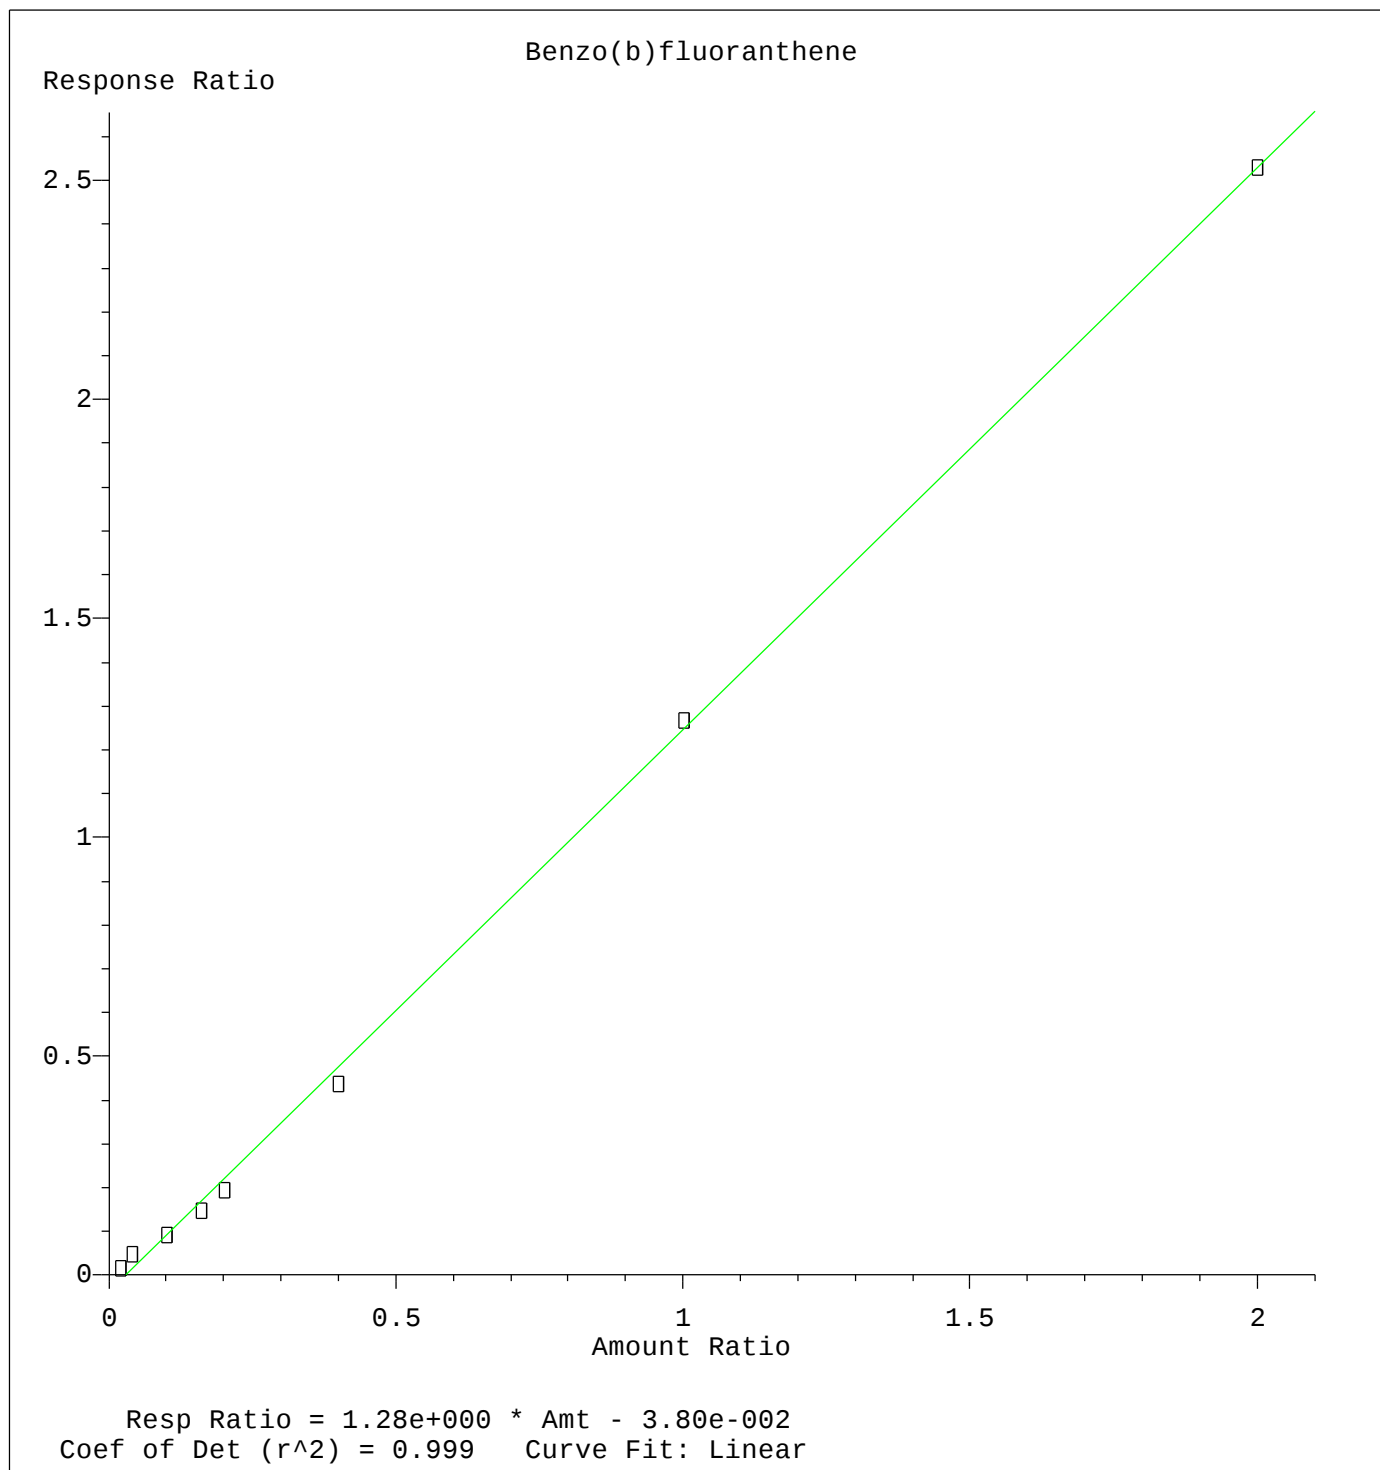

Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE020216.M
Calibration Table Last Updated: Wed Feb 03 00:27:53 2016


Benzo(k)fluoranthene

Response Ratio

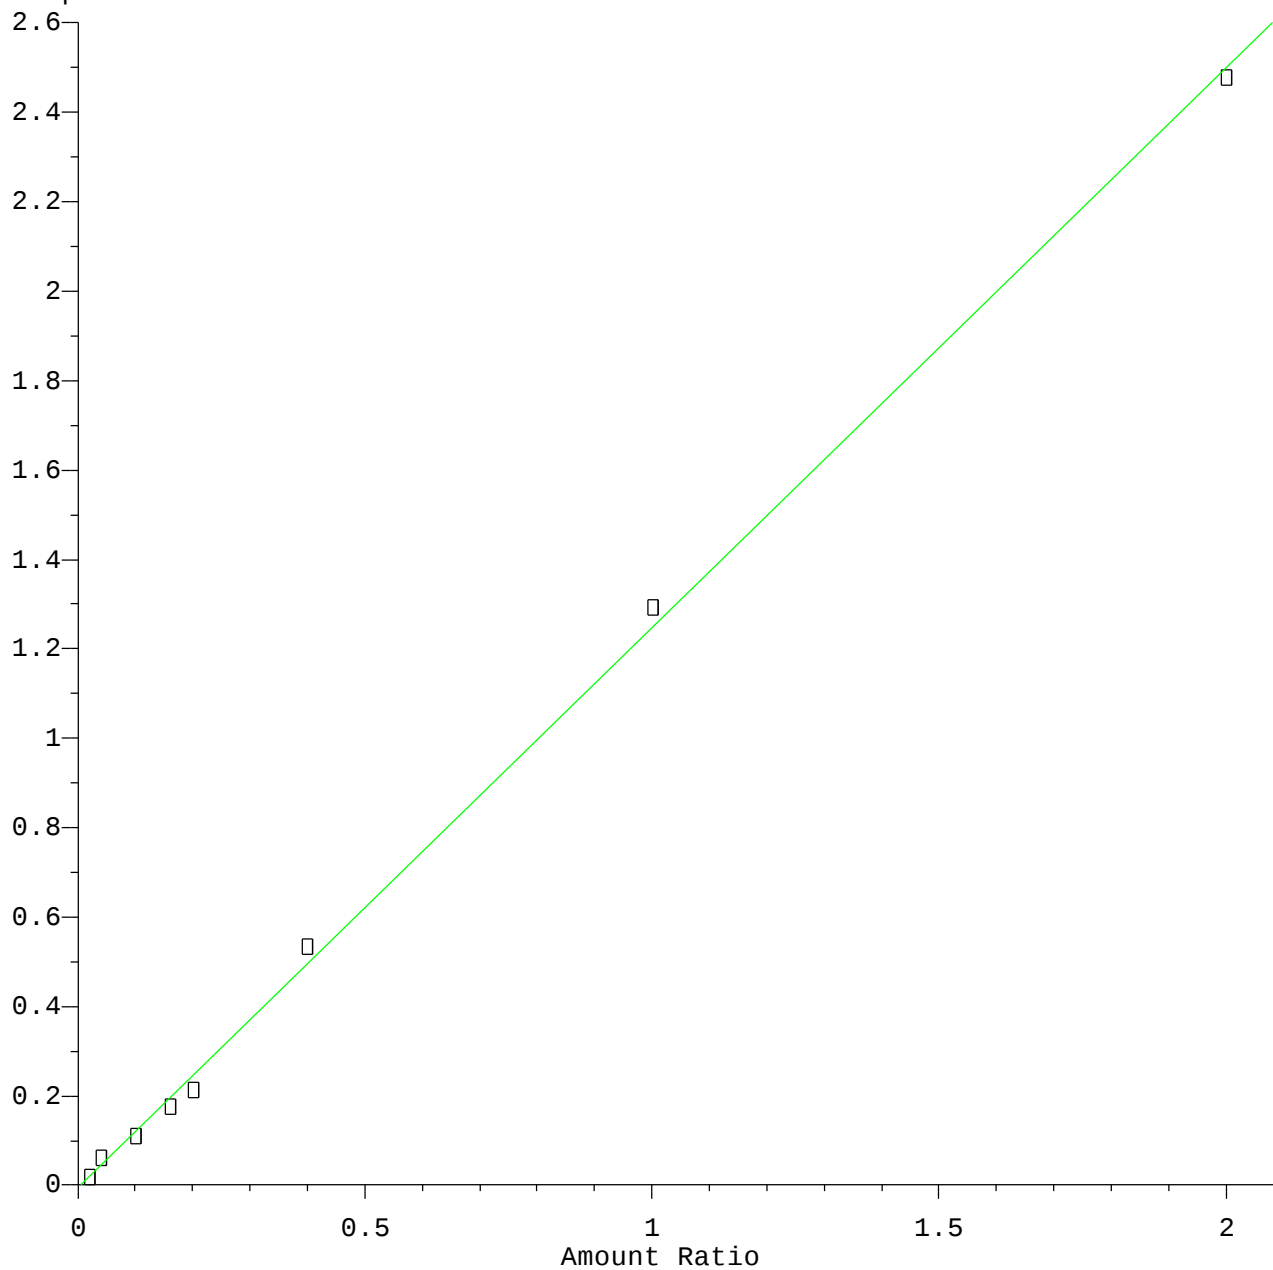

Resp Ratio = 1.25e+000 * Amt - 4.45e-003
Coef of Det (r^2) = 0.999 Curve Fit: Linear


Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE020216.M
Calibration Table Last Updated: Wed Feb 03 00:27:53 2016

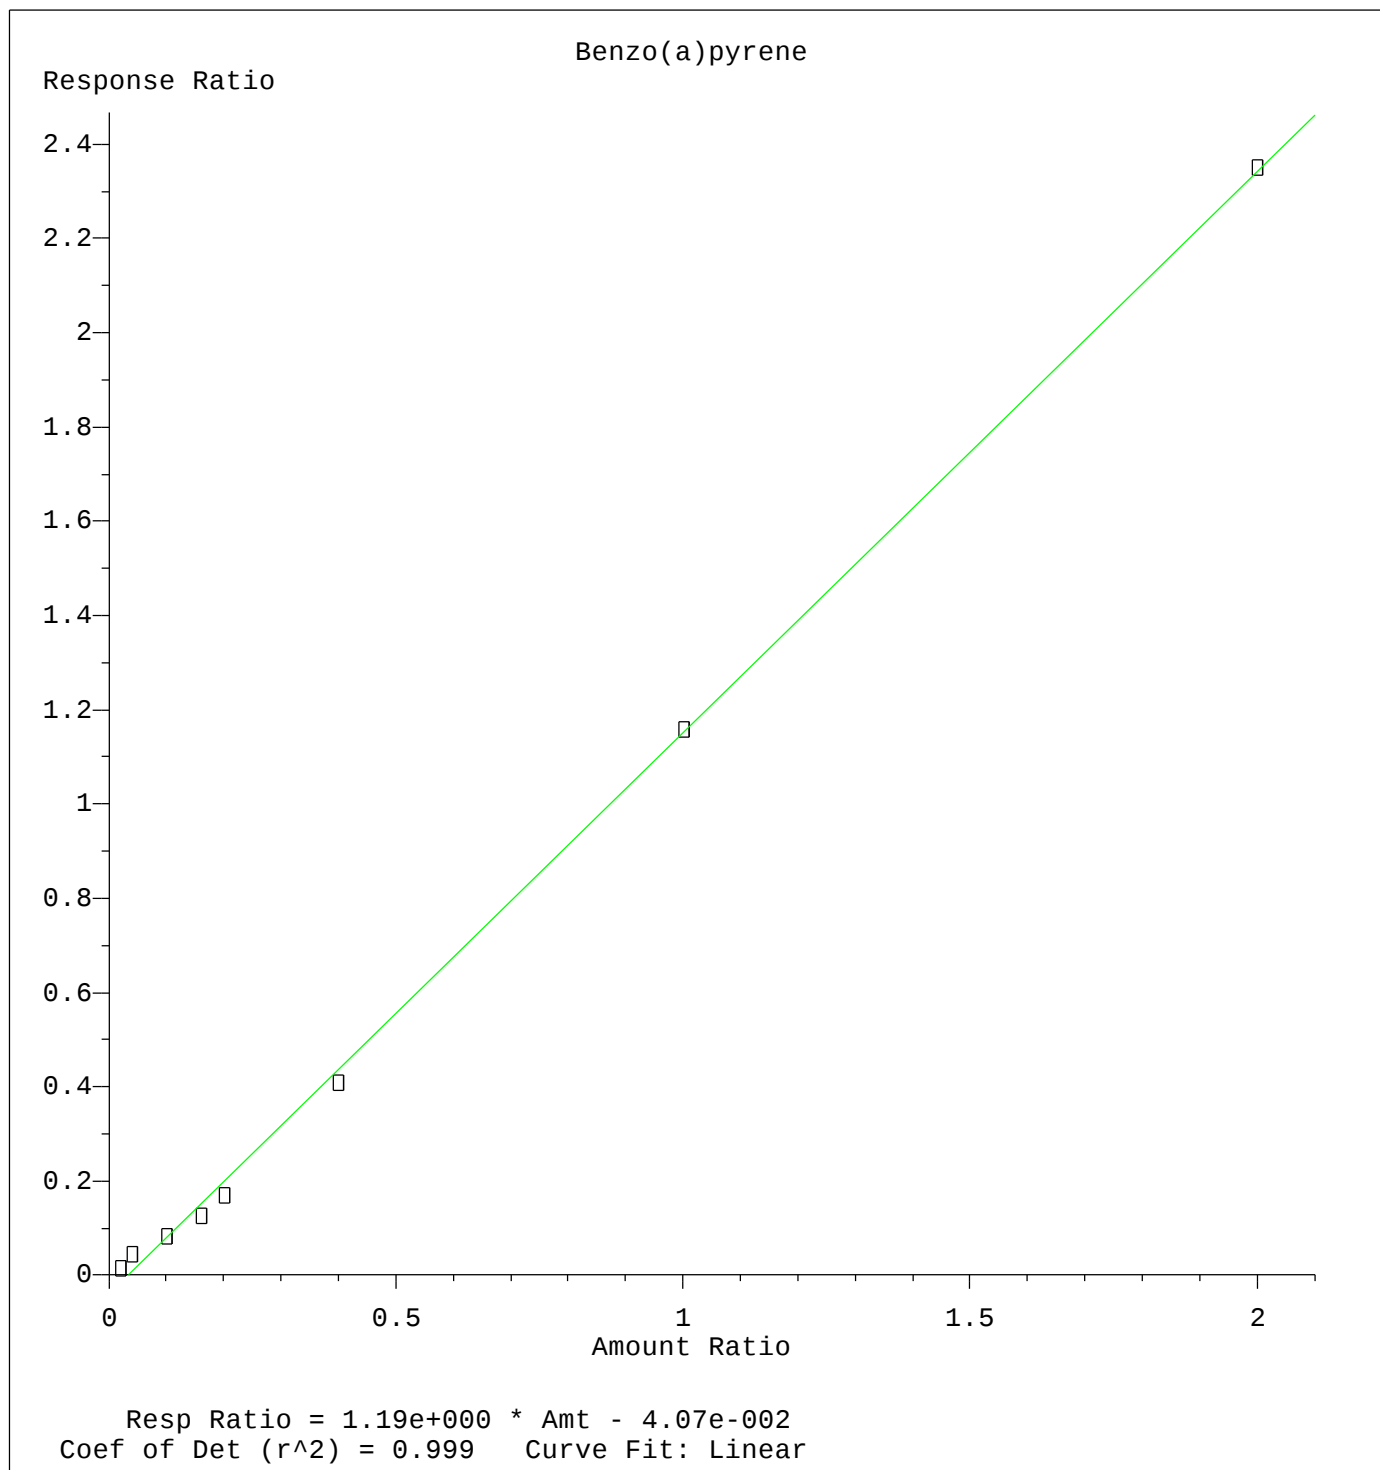

Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE020216.M
Calibration Table Last Updated: Wed Feb 03 00:27:53 2016


Dibenzo(a,h)anthracene

Response Ratio

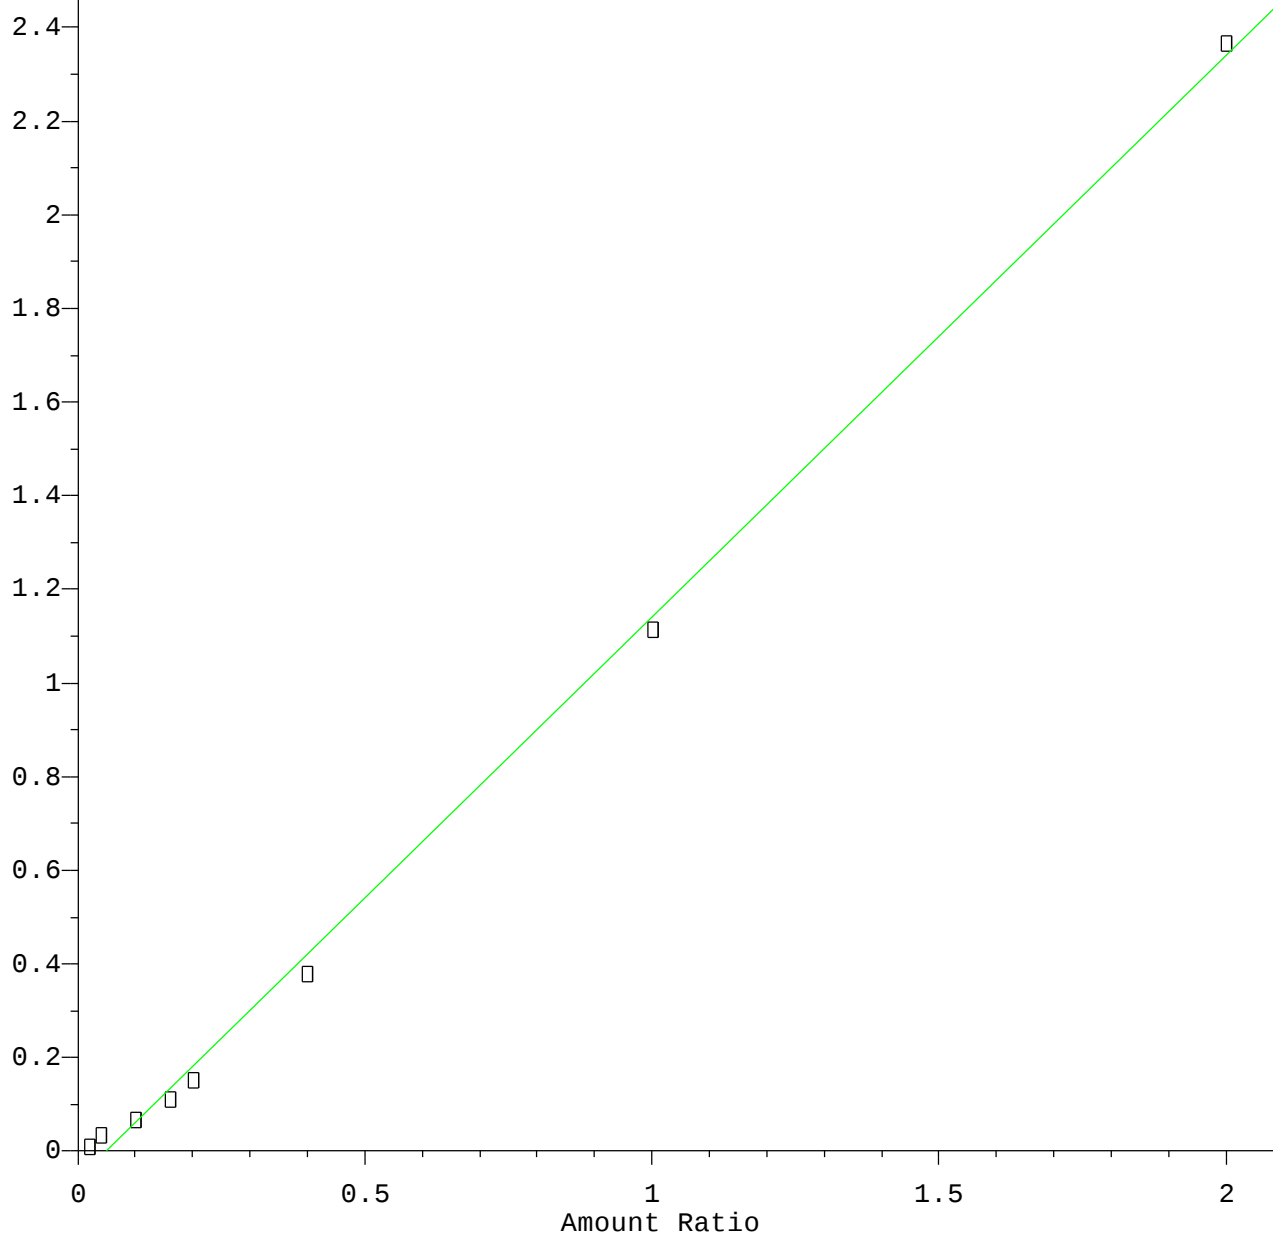

Resp Ratio = 1.20e+000 * Amt - 6.00e-002
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE020216.M
Calibration Table Last Updated: Wed Feb 03 00:27:53 2016

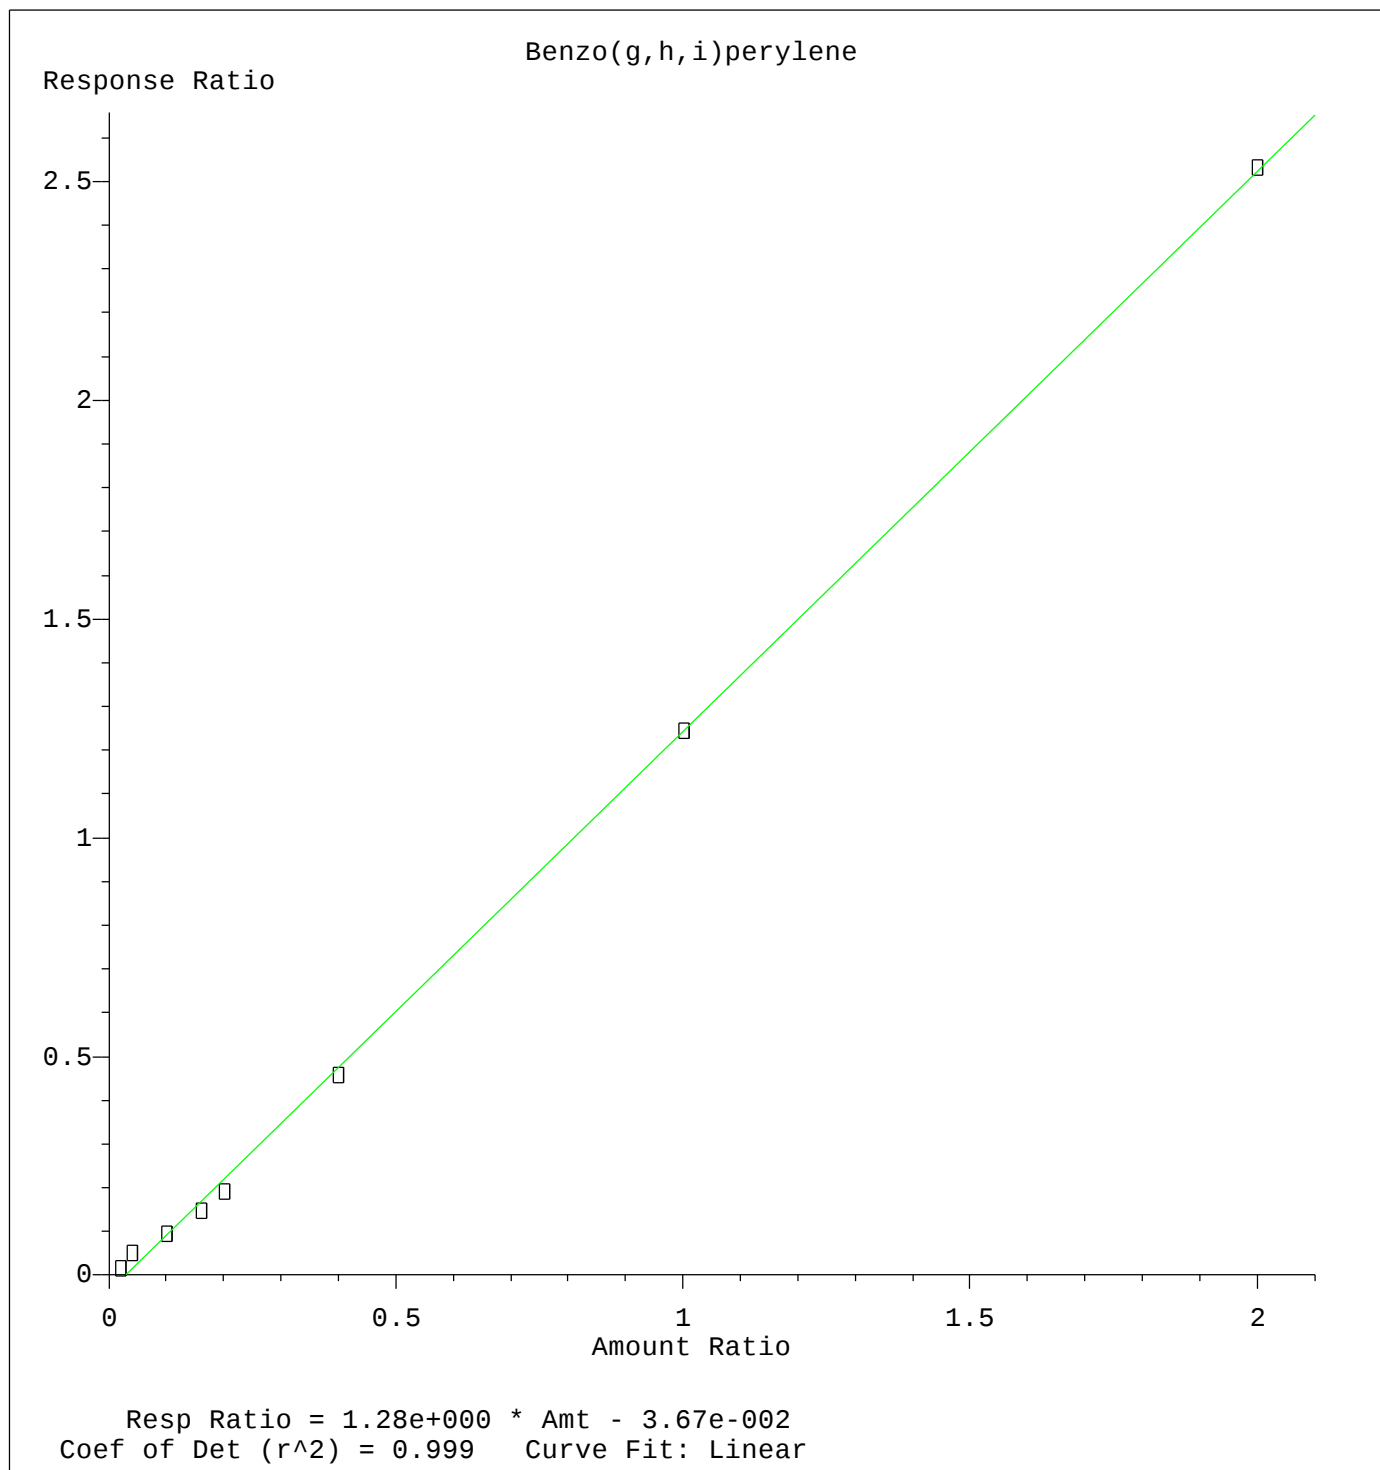

Method Name: Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE020216.M
Calibration Table Last Updated: Wed Feb 03 00:27:53 2016