

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020218\
 Data File : BE095413.D
 Acq On : 3 Feb 2018 00:43
 Operator : SJ/JU
 Sample : J1296-16
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Feb 03 05:27:57 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Feb 03 05:26:35 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.44	152	2137	0.40	ng/ul	0.00
2) Naphthalene-d8	11.26	136	6746	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.02	164	4332	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	8894	0.40	ng/ul	0.00
16) Chrysene-d12	21.80	240	8709	0.40	ng/ul	0.00
20) Perylene-d12	24.27	264	510149	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	3939	0.36	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	10284	0.30	ng/ul	0.00
Target Compounds						
11) Pentachlorophenol	17.36	266	97	0.056	ng/ul	98
12) Phenanthrene	17.75	178	998	0.033	ng/ul#	77
17) Pyrene	20.05	202	1677	0.057	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020218\
Data File : BE095413.D
Acq On : 3 Feb 2018 00:43
Operator : SJ/JU
Sample : J1296-16
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Feb 03 05:27:57 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 03 05:26:35 2018
Response via : Initial Calibration




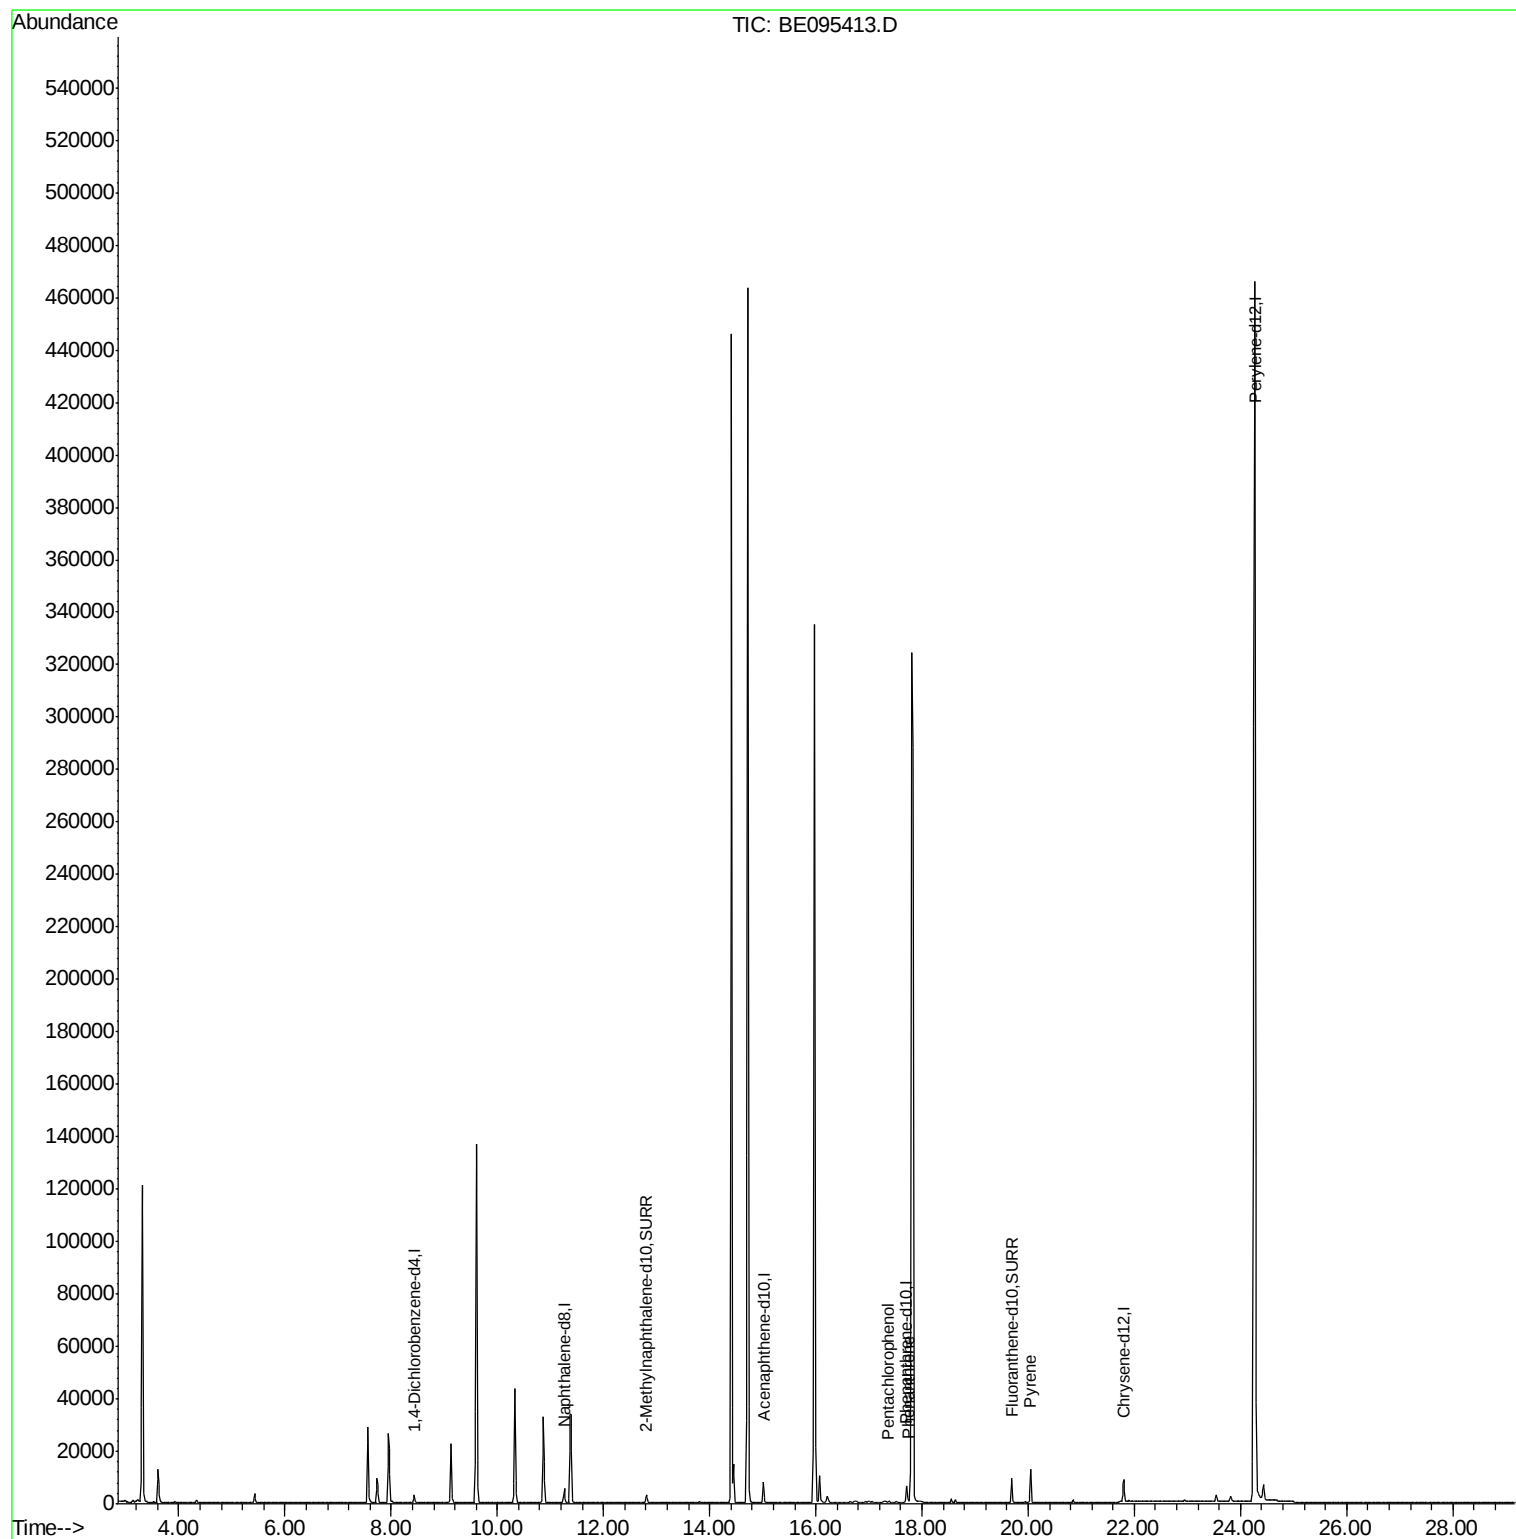


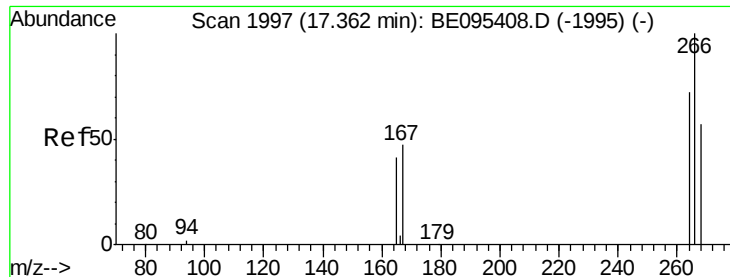

#11
 Pentachlorophenol
 Concen: 0.056 ng/ul
 RT: 17.36 min Scan# 1997
 Delta R.T. 0.00 min
 Lab File: BE095413.D
 Acq: 3 Feb 2018 00:43




Instrument :
 BNA_E
 ClientSampleId :


Tot Ion:266 Resp: 97
 Ion Ratio Lower Upper
 266 100
 264 59.8 47.9 71.9
 268 59.8 49.8 74.8

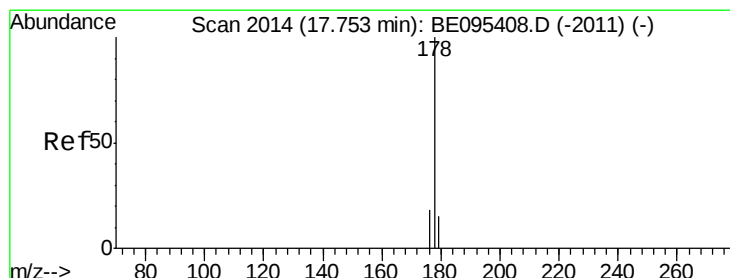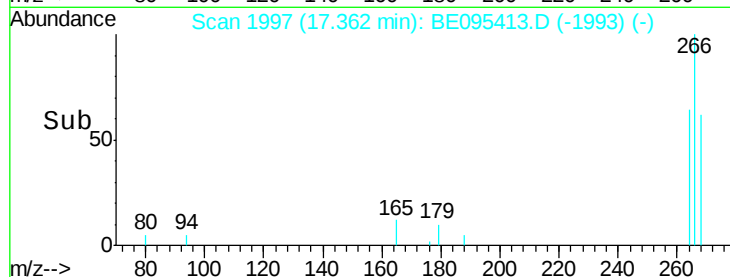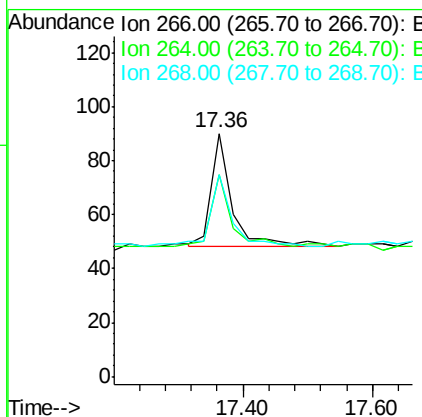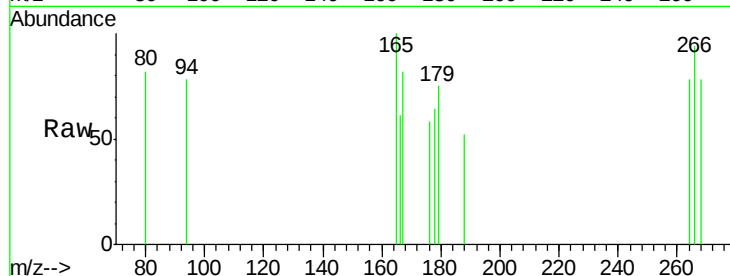

#12
 Phenanthrene
 Concen: 0.033 ng/ul
 RT: 17.75 min Scan# 2014
 Delta R.T. 0.00 min
 Lab File: BE095413.D
 Acq: 3 Feb 2018 00:43

Tgt Ion:178 Resp: 998
 Ion Ratio Lower Upper
 178 100
 179 32.6 18.4 27.6#
 176 29.1 13.6 20.4#

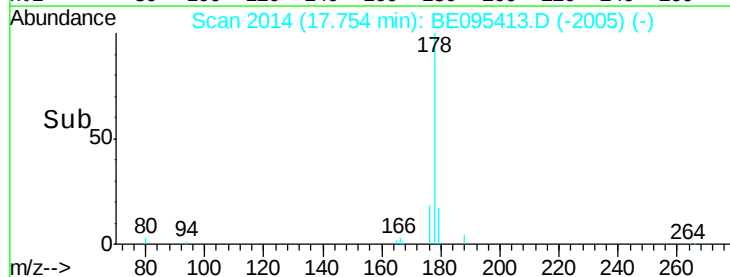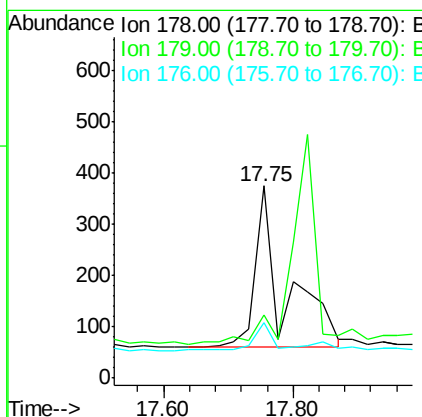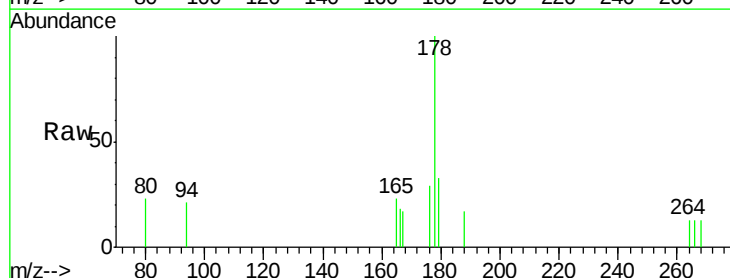

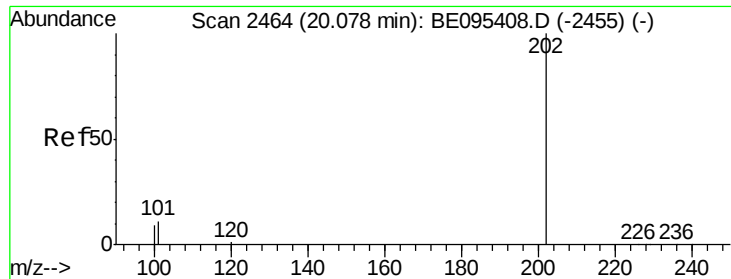

#17
 Pvrene
 Concen: 0.057 ng/ul
 RT: 20.05 min Scan# 2460
 Delta R.T. -0.03 min
 Lab File: BE095413.D
 Acq: 3 Feb 2018 00:43

Instrument :
 BNA_E
 ClientSampleId :

Tot Ion: 202 Resp: 1677
 Ion Ratio Lower Upper
 202 100
 101 164.7 18.2 27.4#
 100 1043.3 15.6 23.4#

