

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020218\
 Data File : BE095414.D
 Acq On : 3 Feb 2018 1:19
 Operator : SJ/JU
 Sample : J1296-18
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Feb 03 05:28:03 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Feb 03 05:26:35 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.44	152	2113	0.40	ng/ul	0.00
2) Naphthalene-d8	11.26	136	6580	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.01	164	4300	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	8745	0.40	ng/ul	0.00
16) Chrysene-d12	21.80	240	8506	0.40	ng/ul	0.00
20) Perylene-d12	24.26	264	401847	0.40	ng/ul	-0.17
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	3499	0.33	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	8756	0.26	ng/ul	0.00
Target Compounds						
11) Pentachlorophenol	17.36	266	93	0.055	ng/ul	94
12) Phenanthrene	17.75	178	1377	0.047	ng/ul#	90
17) Pyrene	20.05	202	1524	0.053	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020218\
Data File : BE095414.D
Acq On : 3 Feb 2018 1:19
Operator : SJ/JU
Sample : J1296-18
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Feb 03 05:28:03 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 03 05:26:35 2018
Response via : Initial Calibration




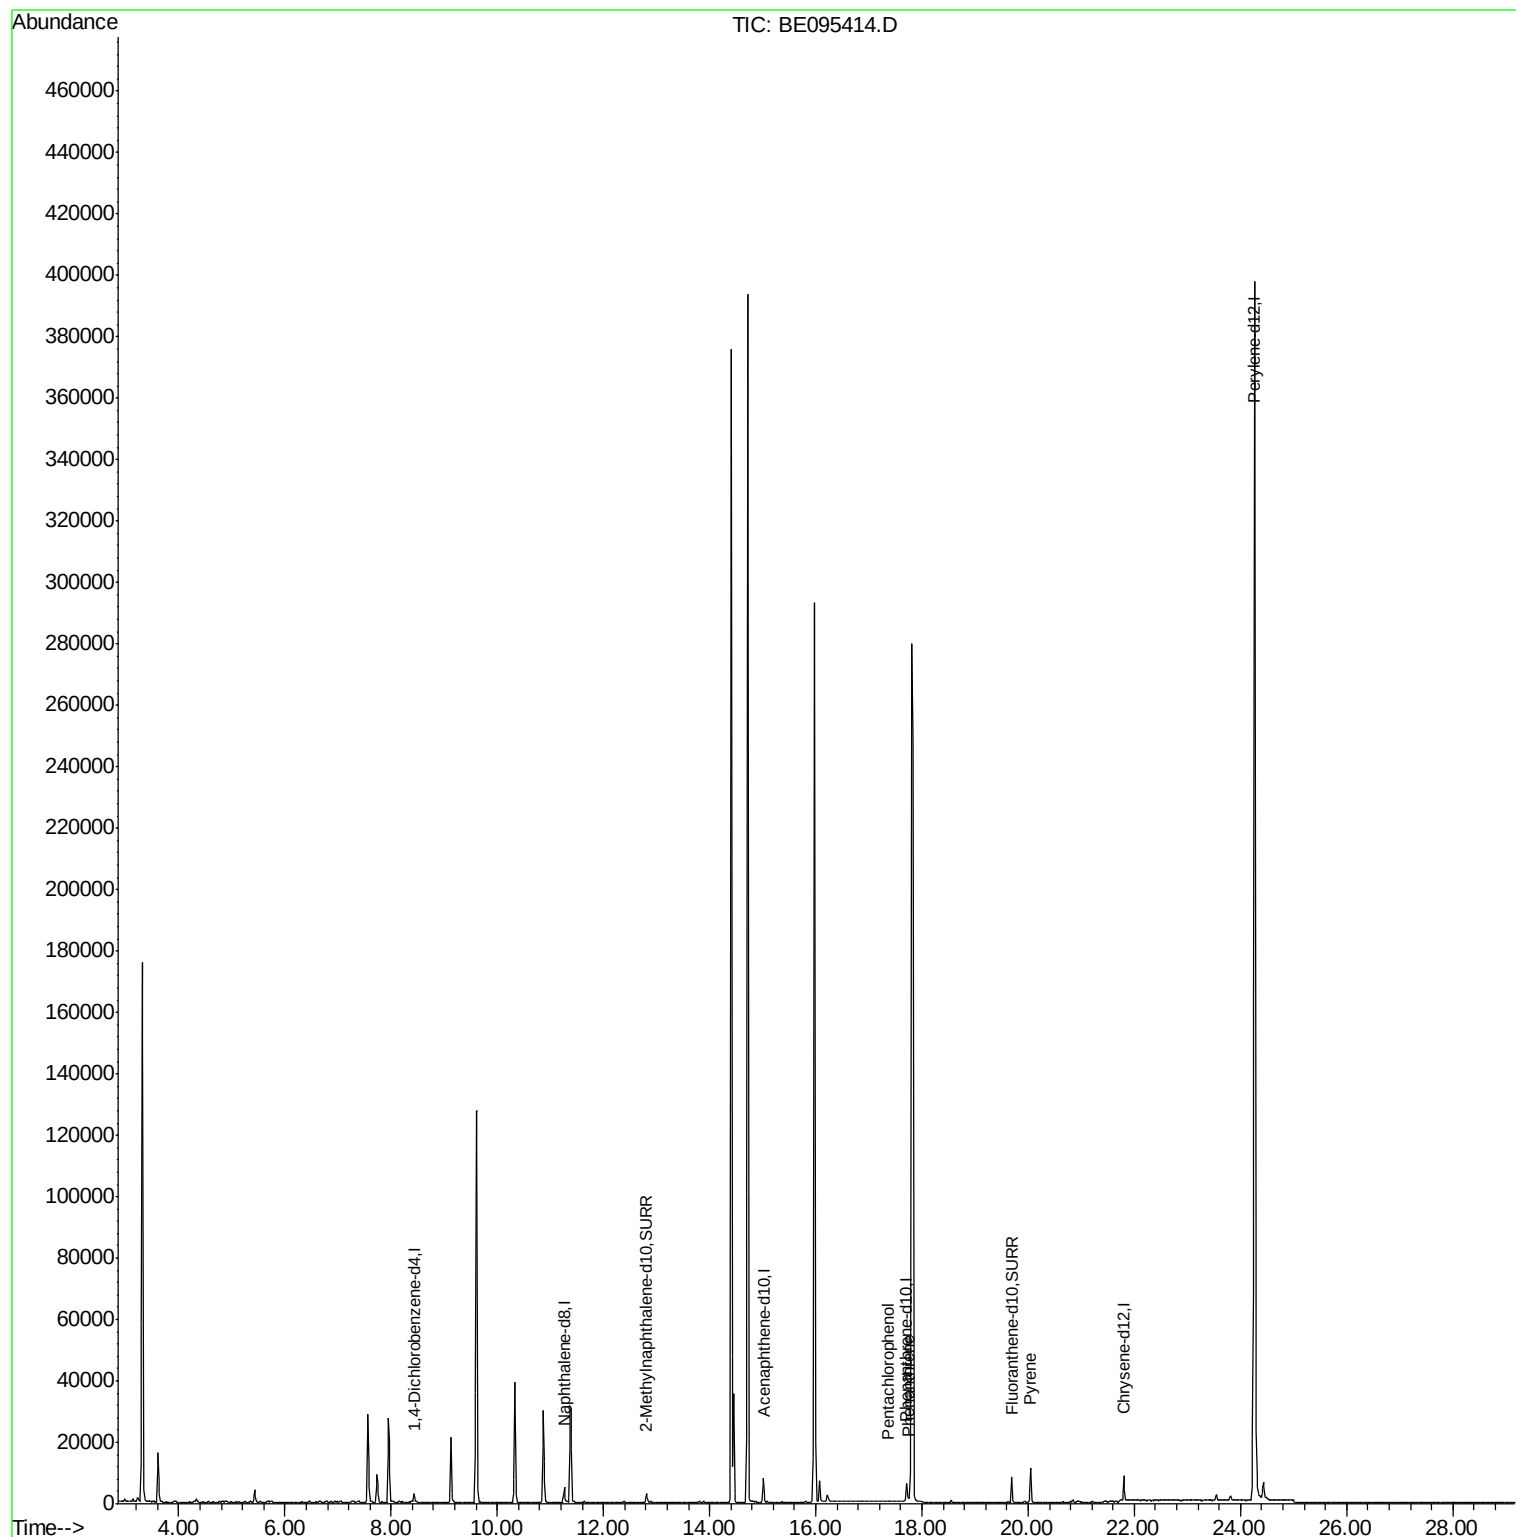


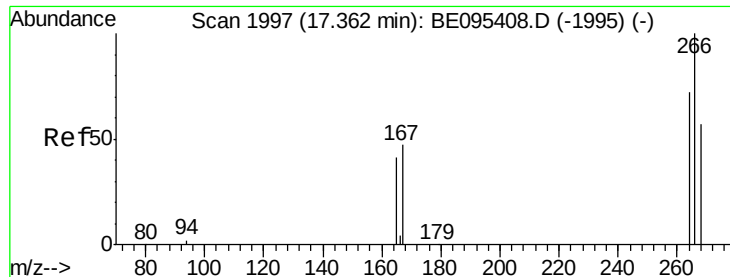

#11
 Pentachlorophenol
 Concen: 0.055 ng/ul
 RT: 17.36 min Scan# 1997
 Delta R.T. -0.00 min
 Lab File: BE095414.D
 Acq: 3 Feb 2018 1:19




Instrument :
 BNA_E
 ClientSampled :




Tot Ion:266 Resp: 93
 Ion Ratio Lower Upper
 266 100
 264 54.8 47.9 71.9
 268 66.7 49.8 74.8

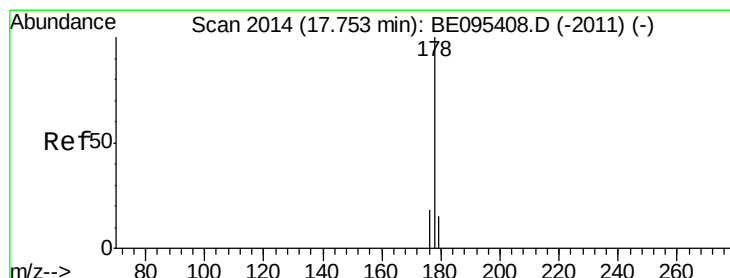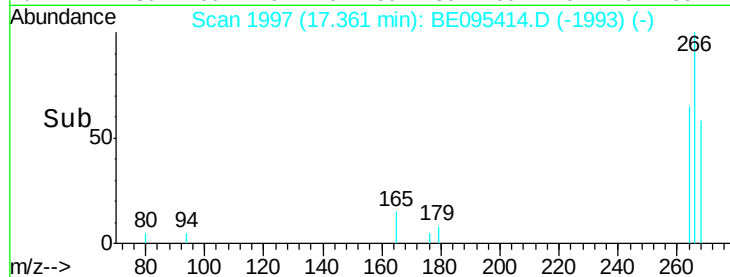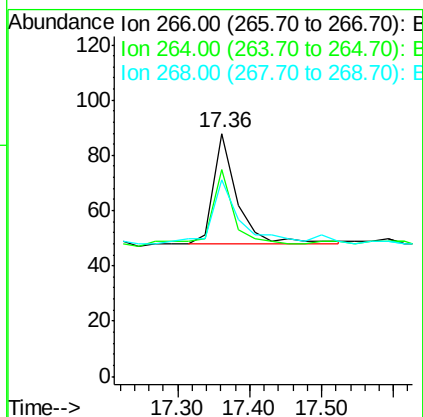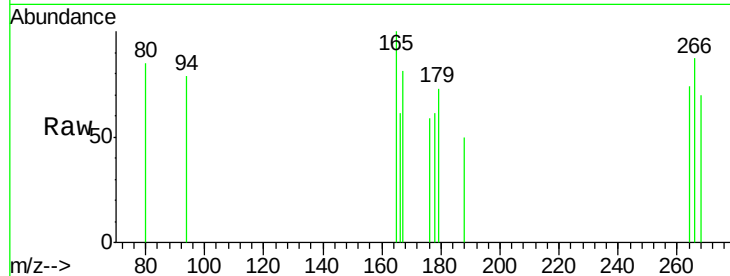

#12
 Phenanthrene
 Concen: 0.047 ng/ul
 RT: 17.75 min Scan# 2014
 Delta R.T. -0.00 min
 Lab File: BE095414.D
 Acq: 3 Feb 2018 1:19

Tgt Ion:178 Resp: 1377
 Ion Ratio Lower Upper
 178 100
 179 24.7 18.4 27.6
 176 25.3 13.6 20.4#

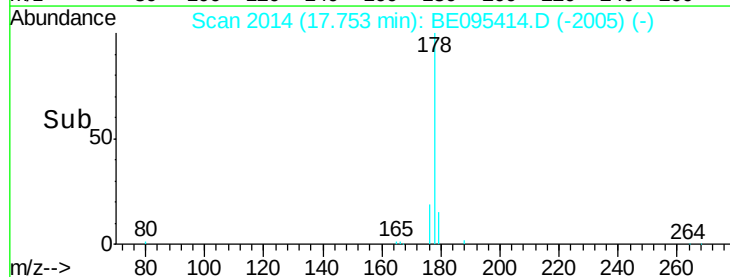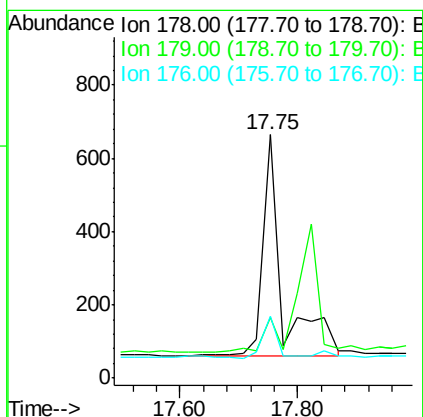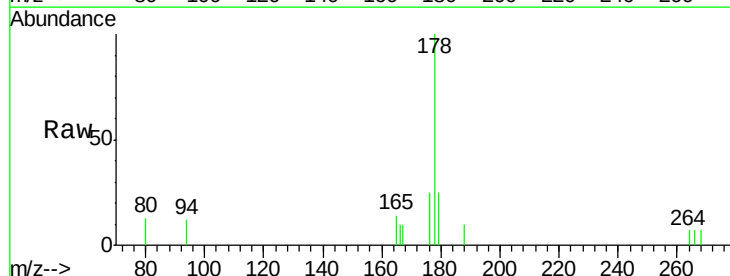

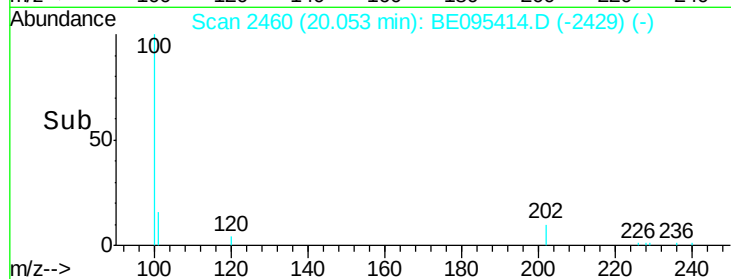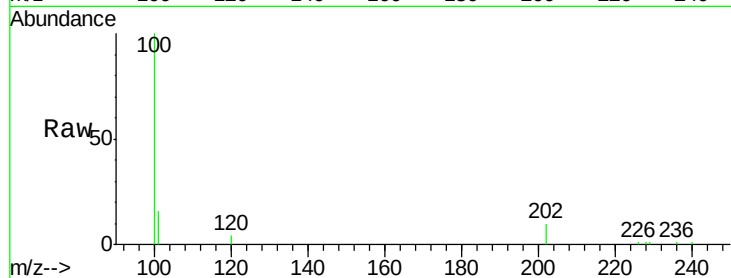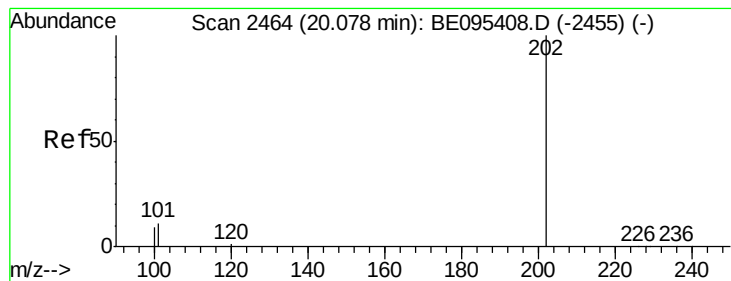

#17

Pvrene

Concen: 0.053 ng/ul

RT: 20.05 min Scan# 2460

Delta R.T. -0.03 min

Lab File: BE095414.D

Acq: 3 Feb 2018 1:19

Instrument :

BNA_E

ClientSampleId :

Tot Ion: 202 Resp: 1524

Ion Ratio Lower Upper

202 100

101 159.6 18.2 27.4#

100 971.7 15.6 23.4#

