

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020218\
 Data File : BE095416.D
 Acq On : 3 Feb 2018 2:30
 Operator : SJ/JU
 Sample : J1296-15
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Feb 03 05:28:16 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Feb 03 05:26:35 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.44	152	2077	0.40	ng/ul	0.00
2) Naphthalene-d8	11.26	136	6393	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.02	164	4033	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	8143	0.40	ng/ul	0.00
16) Chrysene-d12	21.80	240	8191	0.40	ng/ul	0.00
20) Perylene-d12	24.44	264	9530	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	2897	0.28	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	6939	0.22	ng/ul	0.00
Target Compounds						
11) Pentachlorophenol	17.36	266	104	0.066	ng/ul	Ovalue 97
17) Pyrene	20.05	202	1026	0.037	ng/ul#	1
23) Benzo(a)pyrene	24.26	252	1889	0.063	ng/ul#	58


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020218\
Data File : BE095416.D
Acq On : 3 Feb 2018 2:30
Operator : SJ/JU
Sample : J1296-15
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Feb 03 05:28:16 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 03 05:26:35 2018
Response via : Initial Calibration




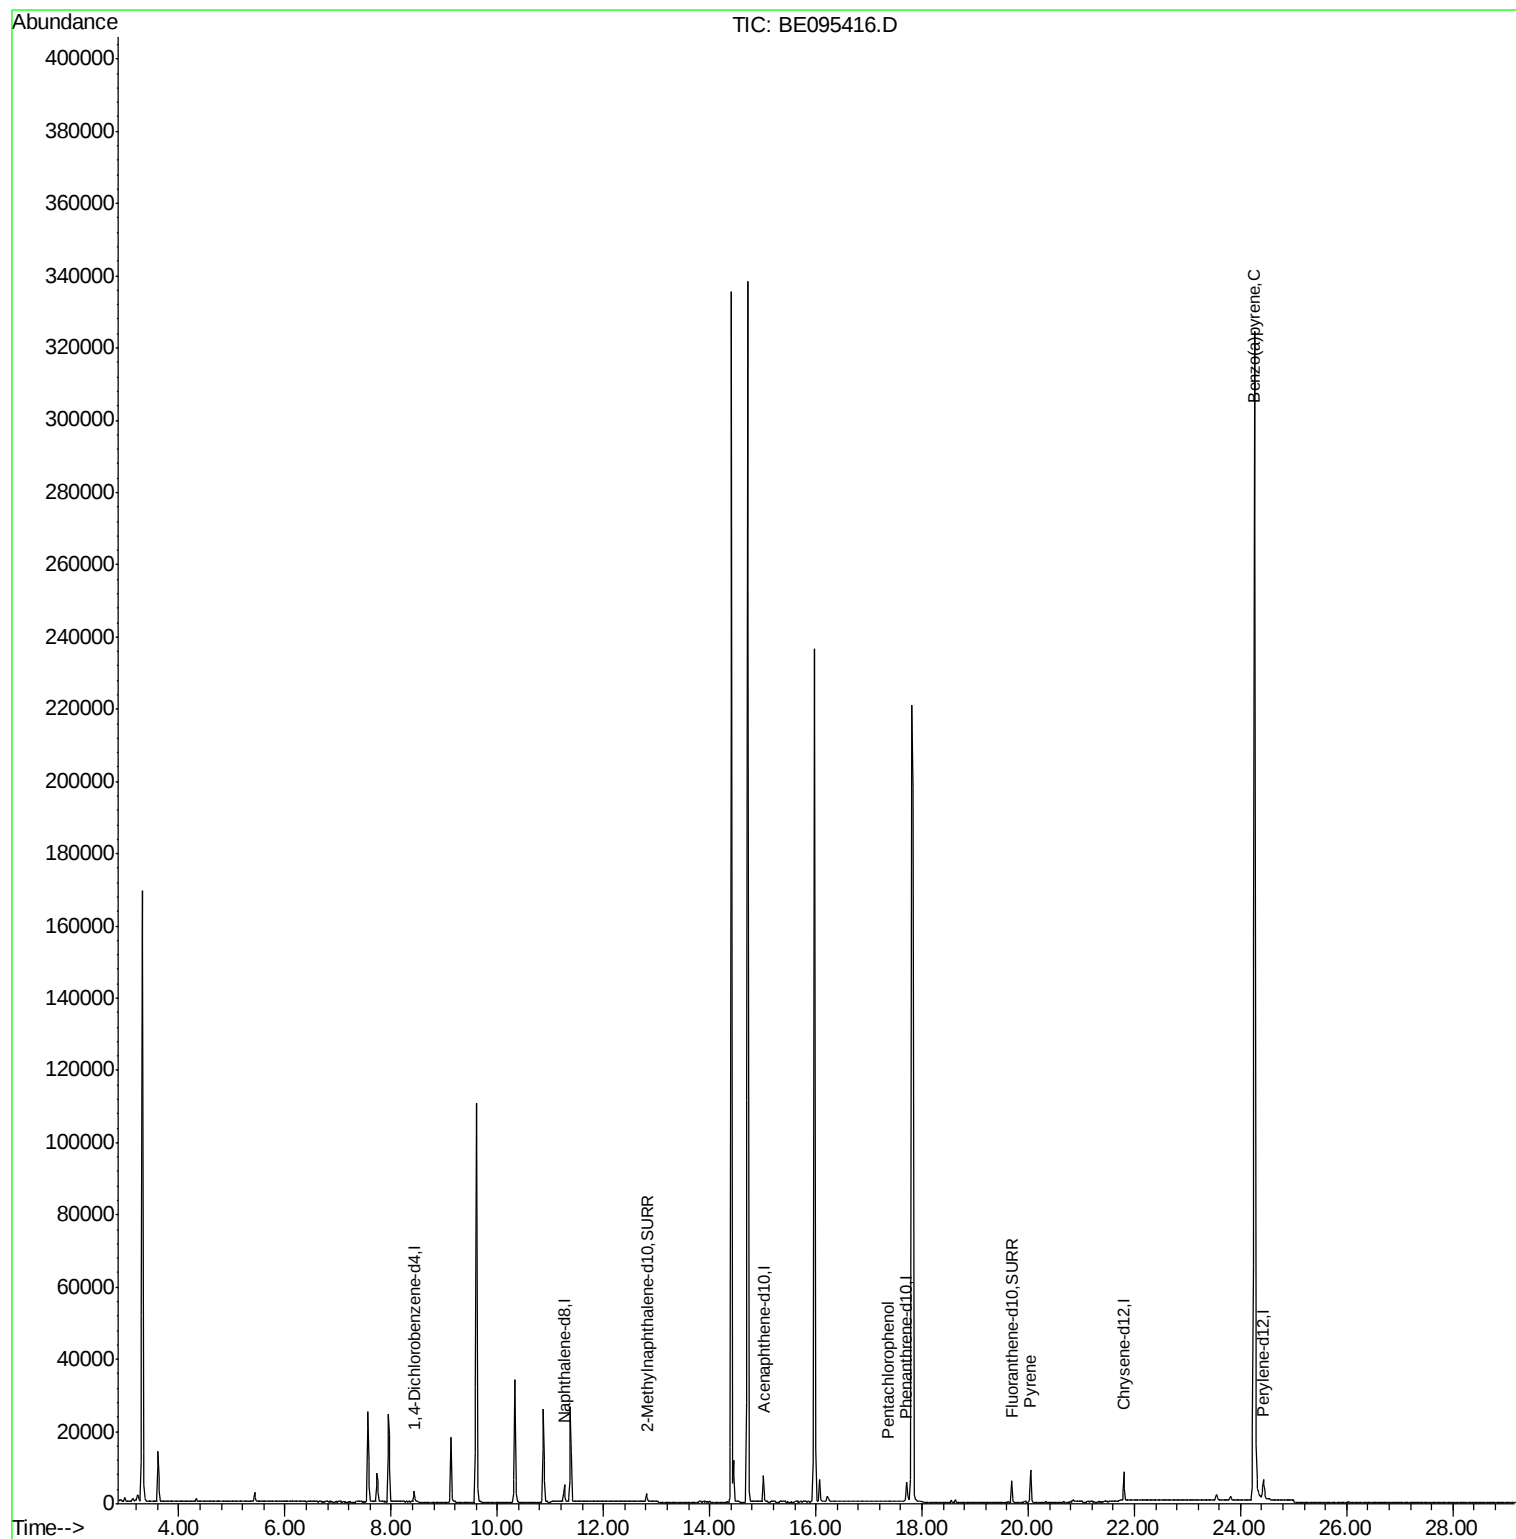


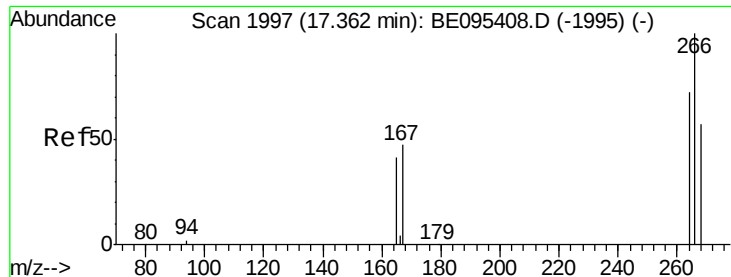

#11
 Pentachlorophenol
 Concen: 0.066 ng/ul
 RT: 17.36 min Scan# 1997
 Delta R.T. -0.00 min
 Lab File: BE095416.D
 Acq: 3 Feb 2018 2:30




Instrument :
 BNA_E
 ClientSampleId :


Tot Ion:266 Resp: 104
 Ion Ratio Lower Upper
 266 100
 264 59.6 47.9 71.9
 268 66.3 49.8 74.8

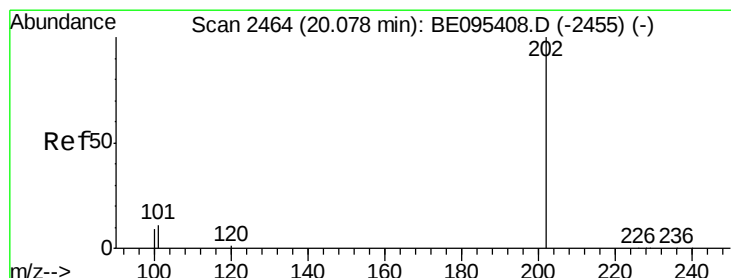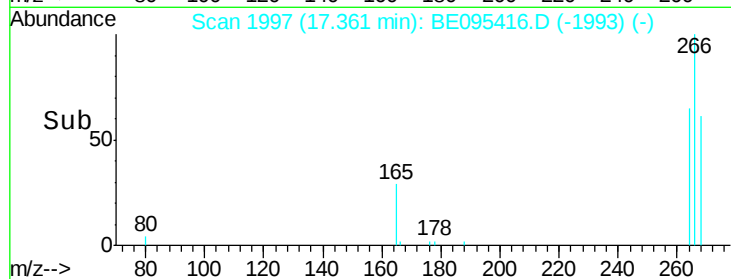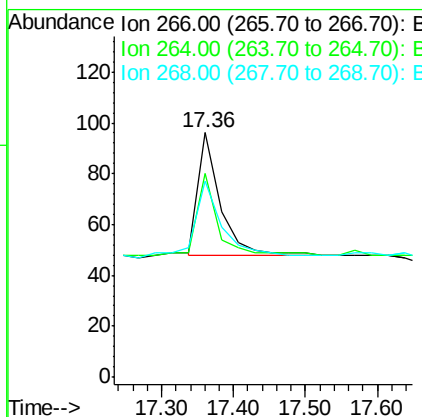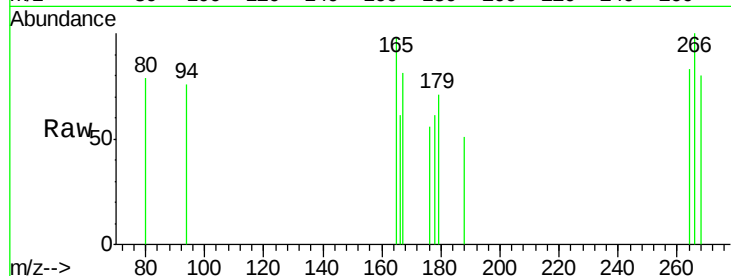

#17
 Pyrene
 Concen: 0.037 ng/ul
 RT: 20.05 min Scan# 2460
 Delta R.T. -0.03 min
 Lab File: BE095416.D
 Acq: 3 Feb 2018 2:30

Tgt Ion:202 Resp: 1026
 Ion Ratio Lower Upper
 202 100
 101 162.1 18.2 27.4#
 100 988.5 15.6 23.4#

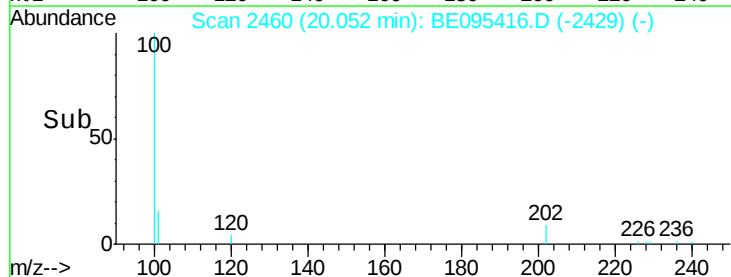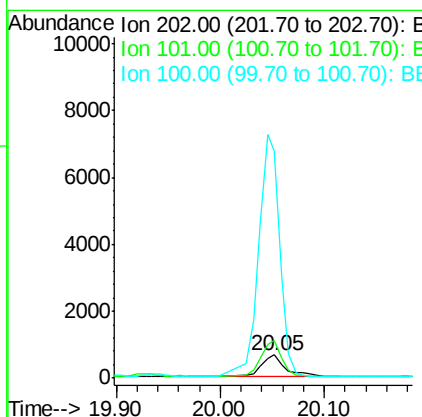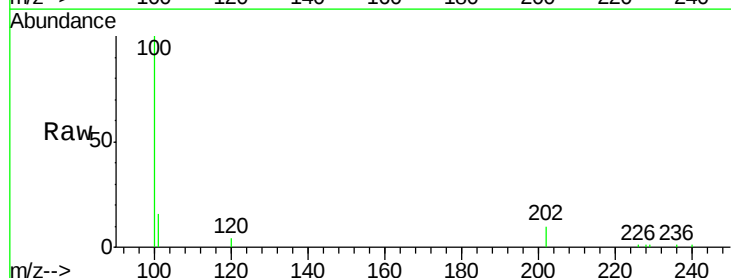

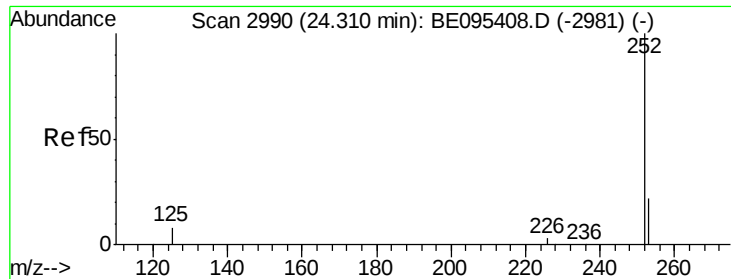

#23

Benzo(a)pyrene

Concen: 0.063 ng/ul

RT: 24.26 min Scan# 2985

Delta R.T. -0.05 min


Lab File: BE095416.D

Acq: 3 Feb 2018 2:30

Instrument :

BNA_E

ClientSampleId :

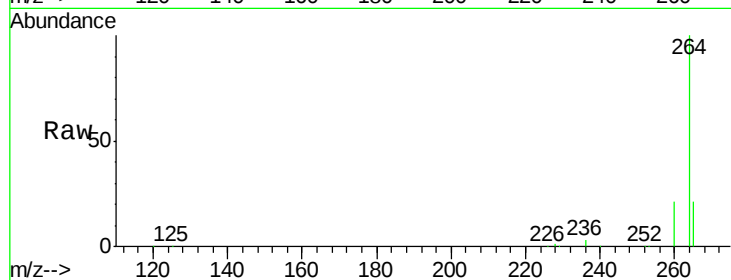

Tot Ion: 252 Resp: 1889

Ion Ratio Lower Upper

252 100

253 47.9 28.5 42.7#

125 58.7 18.1 27.1#

