

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020218\
 Data File : BE095418.D
 Acq On : 3 Feb 2018 3:42
 Operator : SJ/JU
 Sample : J1296-12
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Feb 03 05:28:28 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Feb 03 05:26:35 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.43	152	1999	0.40	ng/ul	0.00
2) Naphthalene-d8	11.26	136	6221	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.02	164	4020	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	8192	0.40	ng/ul	0.00
16) Chrysene-d12	21.80	240	8482	0.40	ng/ul	0.00
20) Perylene-d12	24.27	264	383704	0.40	ng/ul	-0.17
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	3356	0.33	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	8329	0.27	ng/ul	0.00
Target Compounds						
					Ovalue	
11) Pentachlorophenol	17.36	266	65	0.041	ng/ul#	83
12) Phenanthrene	17.75	178	863	0.031	ng/ul#	73
17) Pyrene	20.05	202	1584	0.056	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020218\
Data File : BE095418.D
Acq On : 3 Feb 2018 3:42
Operator : SJ/JU
Sample : J1296-12
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Feb 03 05:28:28 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 03 05:26:35 2018
Response via : Initial Calibration




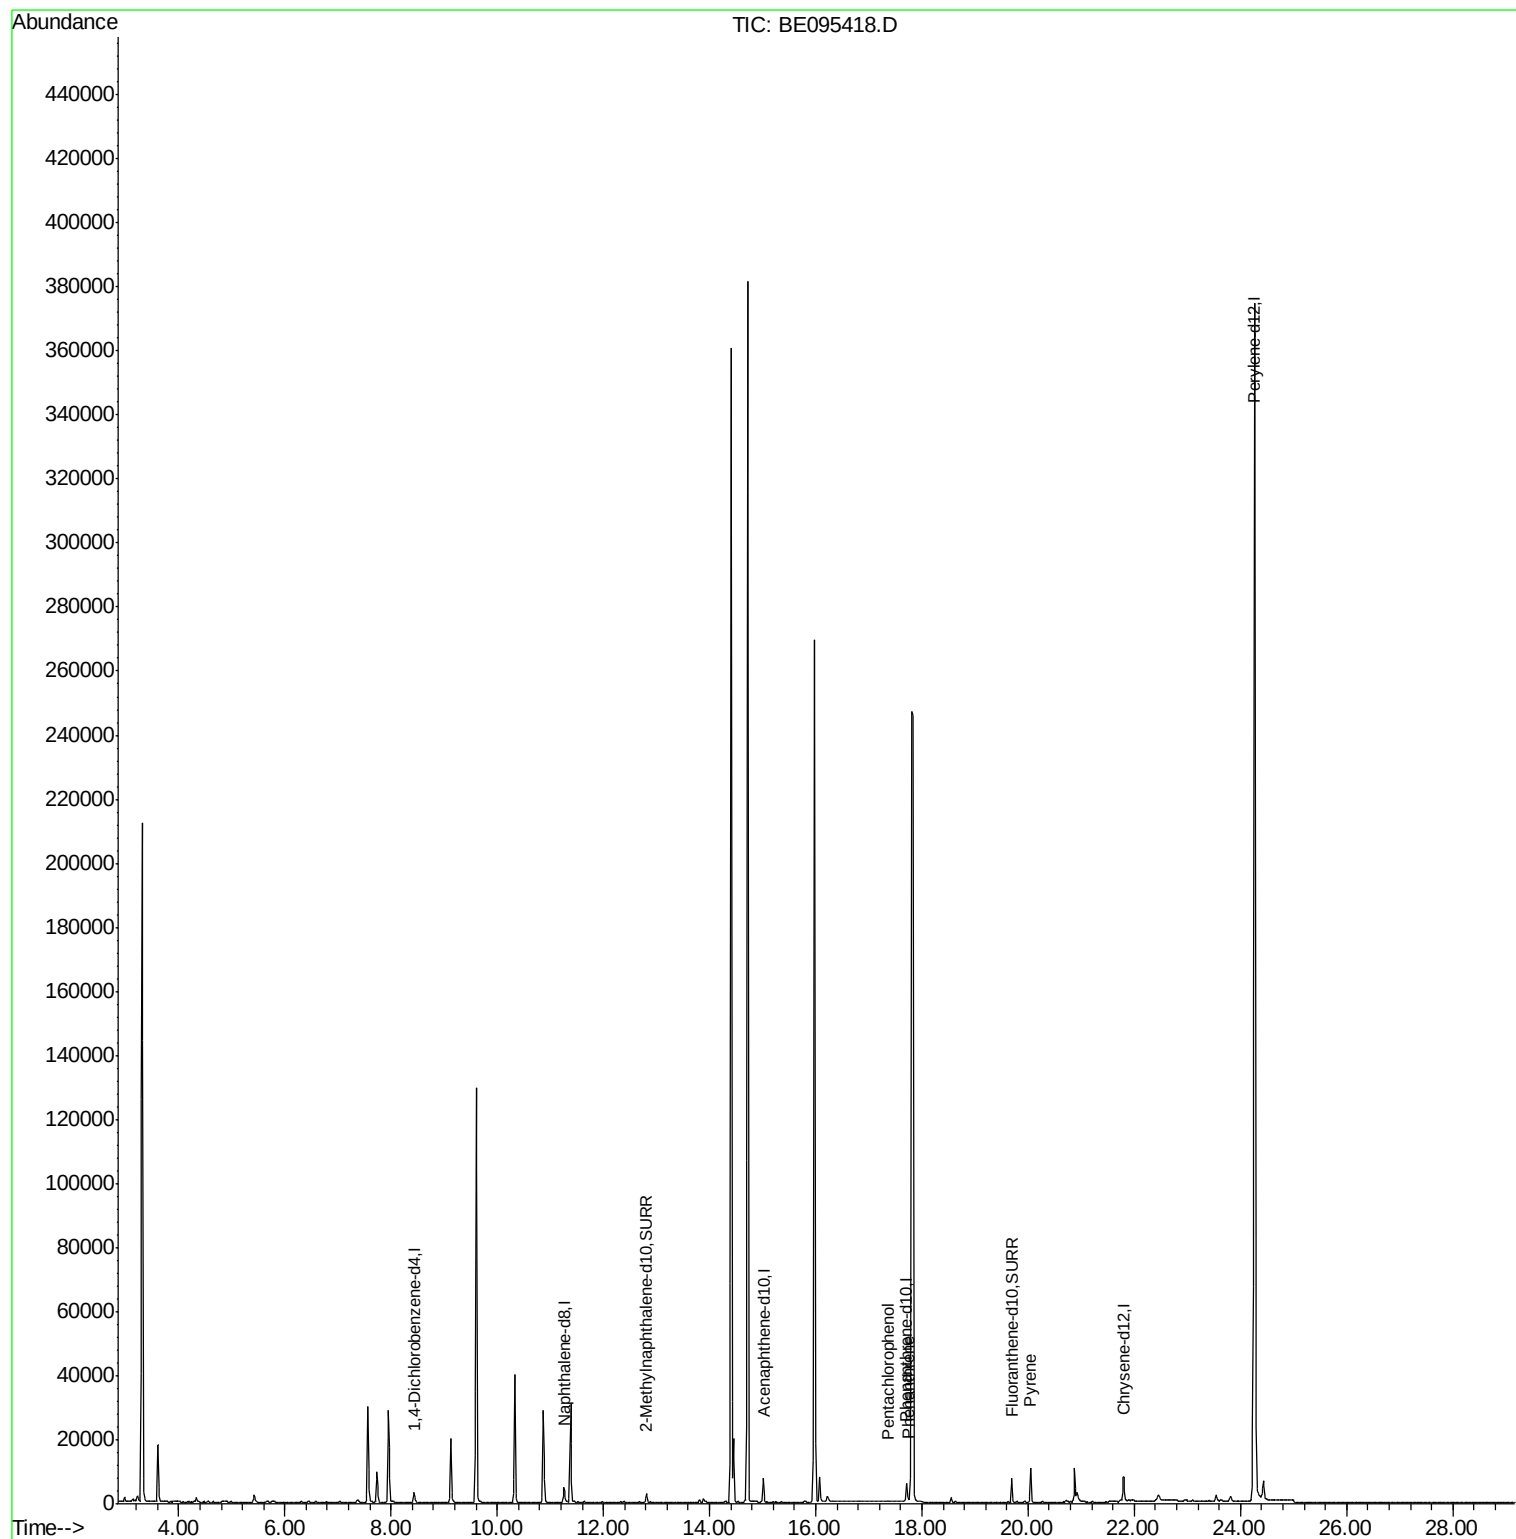


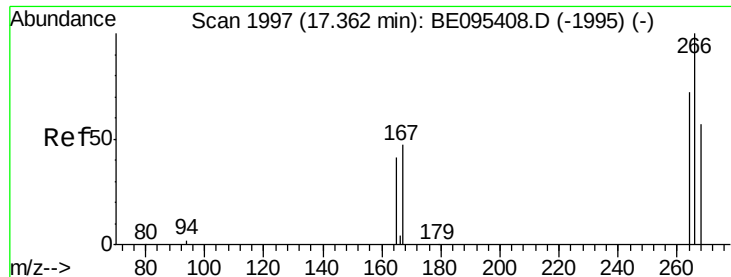

#11
 Pentachlorophenol
 Concen: 0.041 ng/ul
 RT: 17.36 min Scan# 1997
 Delta R.T. 0.00 min
 Lab File: BE095418.D
 Acq: 3 Feb 2018 3:42




Instrument :
 BNA_E
 ClientSampleId :


Tot Ion:266 Resp: 65
 Ion Ratio Lower Upper
 266 100
 264 43.1 47.9 71.9#
 268 70.8 49.8 74.8

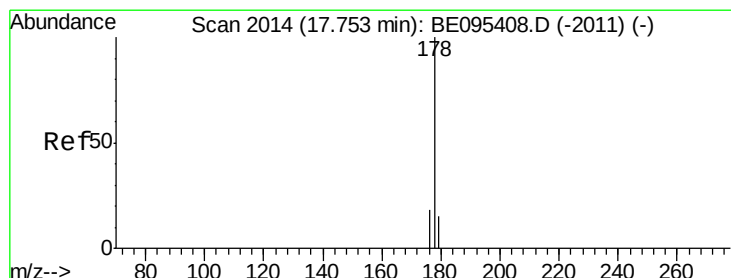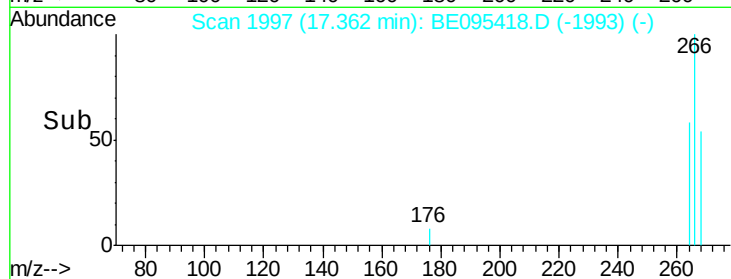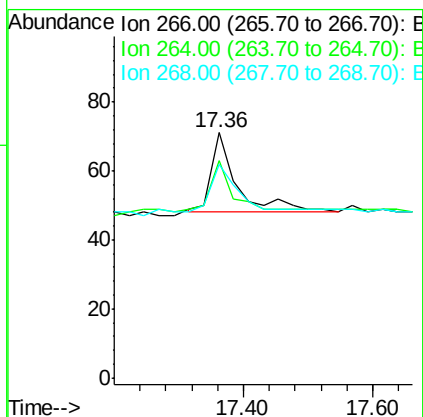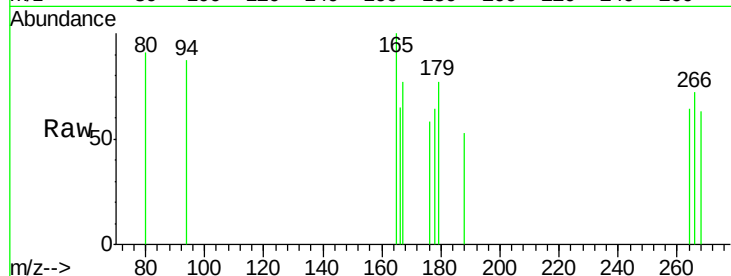

#12
 Phenanthrene
 Concen: 0.031 ng/ul
 RT: 17.75 min Scan# 2014
 Delta R.T. 0.00 min
 Lab File: BE095418.D
 Acq: 3 Feb 2018 3:42

Tgt Ion:178 Resp: 863
 Ion Ratio Lower Upper
 178 100
 179 34.7 18.4 27.6#
 176 30.5 13.6 20.4#

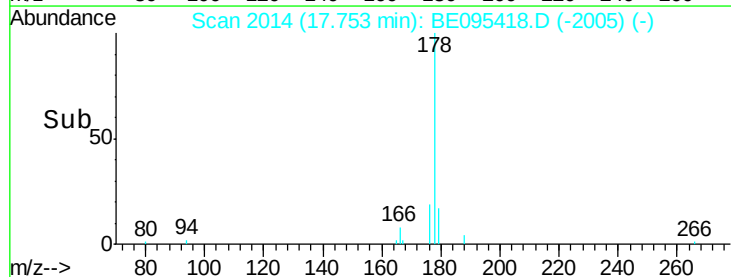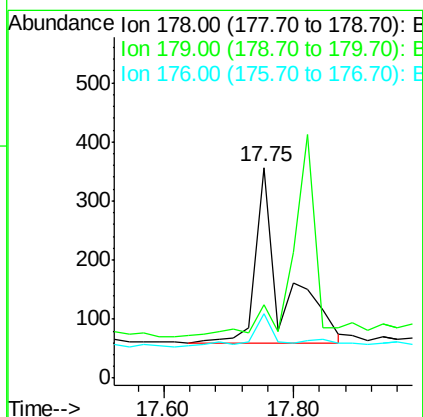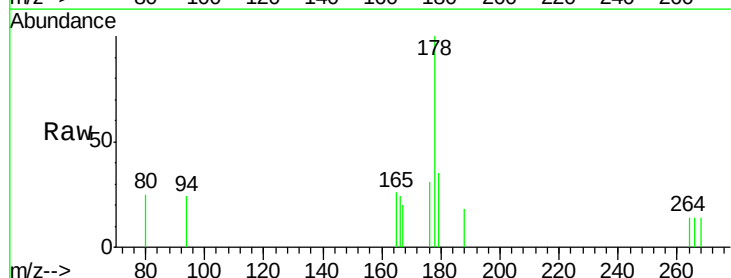

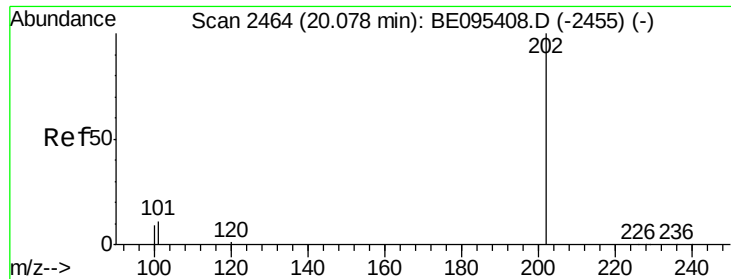

#17

Pvrene

Concen: 0.056 ng/ul

RT: 20.05 min Scan# 2460

Delta R.T. -0.03 min

Lab File: BE095418.D

Acq: 3 Feb 2018 3:42

Instrument :

BNA_E

ClientSampleId :


Tot Ion:202 Resp: 1584

Ion Ratio Lower Upper

202 100

101 152.9 18.2 27.4#

100 984.1 15.6 23.4#

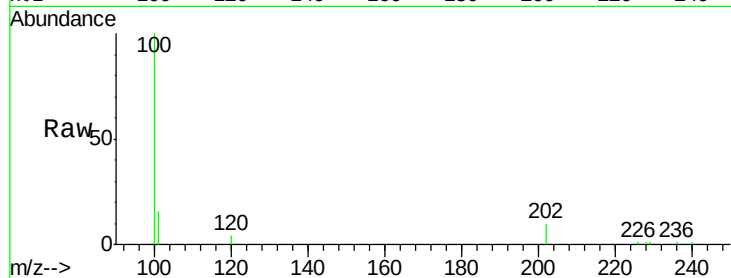

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): BE

