

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020218\
 Data File : BE095422.D
 Acq On : 3 Feb 2018 6:05
 Operator : SJ/JU
 Sample : J1296-05
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Feb 05 01:11:48 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Feb 03 05:26:35 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.44	152	1888	0.40	ng/ul	0.00
2) Naphthalene-d8	11.26	136	5824	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.02	164	3925	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.71
16) Chrysene-d12	21.80	240	7871	0.40	ng/ul	0.00
20) Perylene-d12	24.27	264	526058	0.40	ng/ul	-0.17
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	4342	0.46	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	11168	0.00	ng/ul	0.00
Target Compounds						
3) Naphthalene	11.31	128	760	0.047	ng/ul#	75
17) Pyrene	20.05	202	1912	0.072	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020218\
Data File : BE095422.D
Acq On : 3 Feb 2018 6:05
Operator : SJ/JU
Sample : J1296-05
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Feb 05 01:11:48 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 03 05:26:35 2018
Response via : Initial Calibration

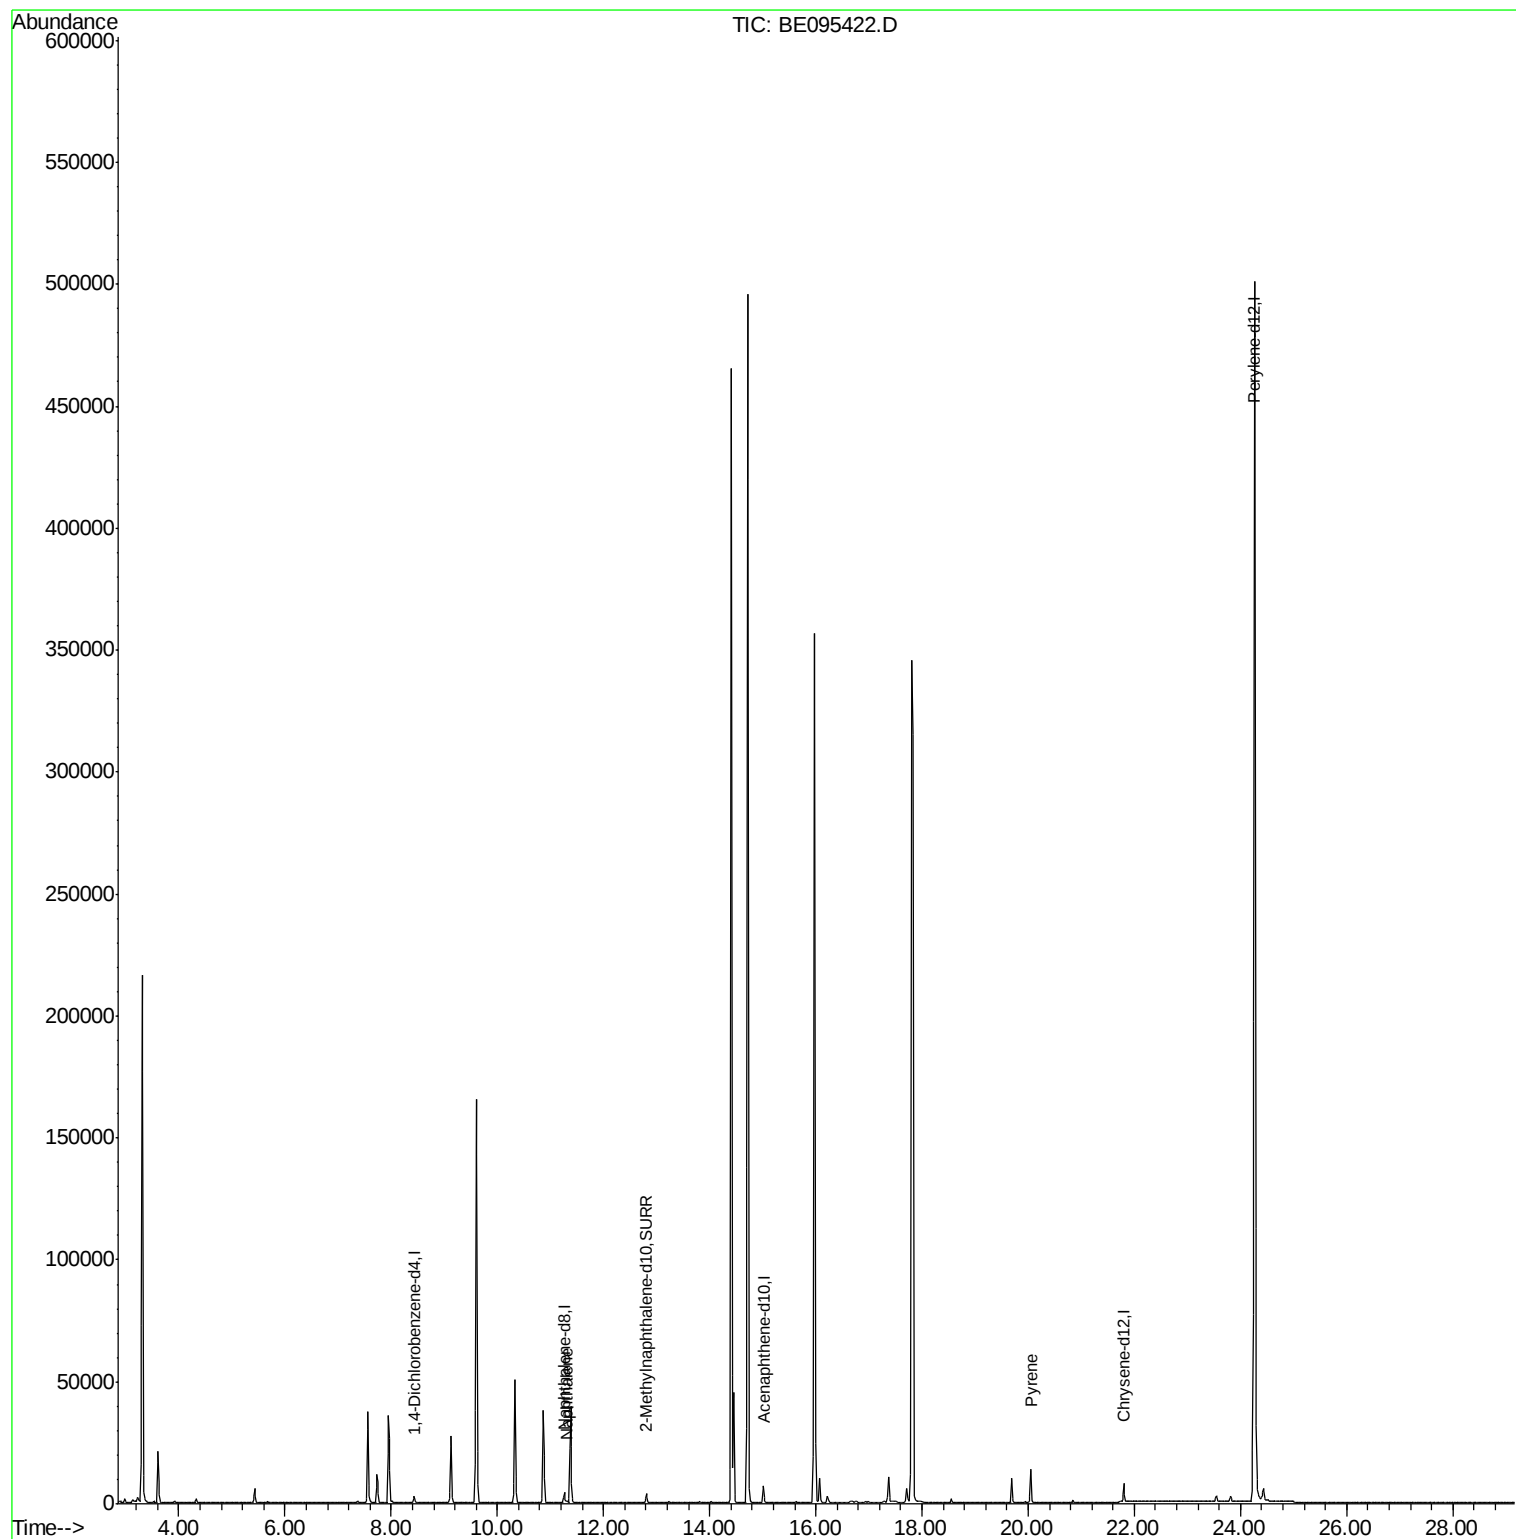

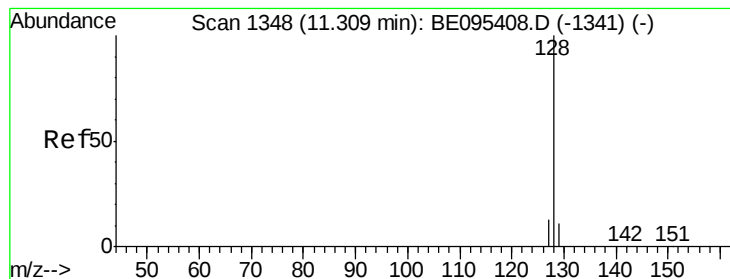

#3

Naphthalene

Concen: 0.047 ng/ul

RT: 11.31 min Scan# 1348

Delta R.T. 0.00 min

Lab File: BE095422.D

Acq: 3 Feb 2018 6:05

Instrument :

BNA_E

ClientSampleId :


Tot Ion:128 Resp: 760

Ion Ratio Lower Upper




128 100

129 20.7 11.3 16.9#

127 21.7 4.0 6.0#

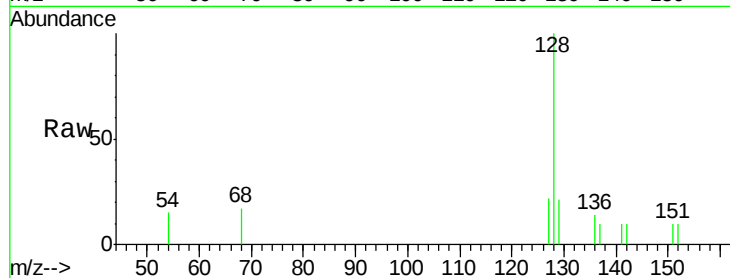

Abundance Ion 128.00 (127.70 to 128.70): E
Ion 129.00 (128.70 to 129.70): E
Ion 127.00 (126.70 to 127.70): E

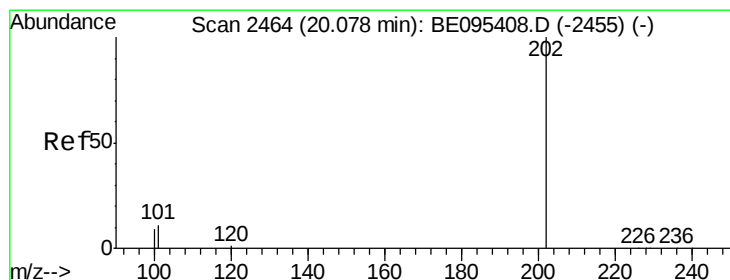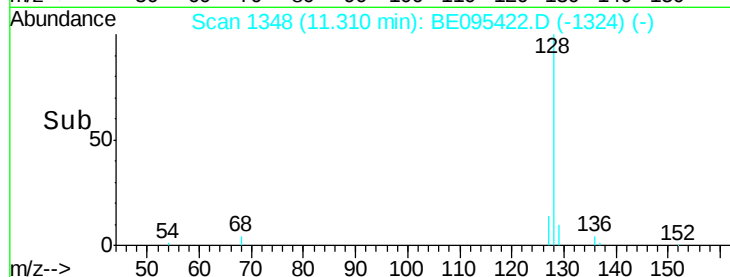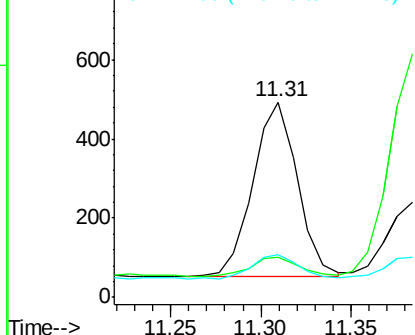

#17

Pyrene

Concen: 0.072 ng/ul

RT: 20.05 min Scan# 2460

Delta R.T. -0.03 min

Lab File: BE095422.D

Acq: 3 Feb 2018 6:05


Tgt Ion:202 Resp: 1912

Ion Ratio Lower Upper

202 100

101 166.8 18.2 27.4#

100 1107.7 15.6 23.4#

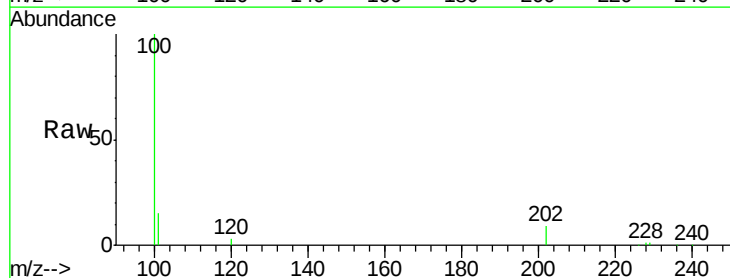

Abundance Ion 202.00 (201.70 to 202.70): E
Ion 101.00 (100.70 to 101.70): E
Ion 100.00 (99.70 to 100.70): E

