


Data Path : Z:\HPCHEM1\BNA E\DATA\BE020218\
Data File : BE095410.D
Acq On : 2 Feb 2018 22:58
Operator : SJ/JU
Sample : J1296-11
Misc :
ALS Vial : 18 Sample Multiplier: 1




Quant Time: Feb 03 05:35:46 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 03 05:26:35 2018
Response via : Initial Calibration

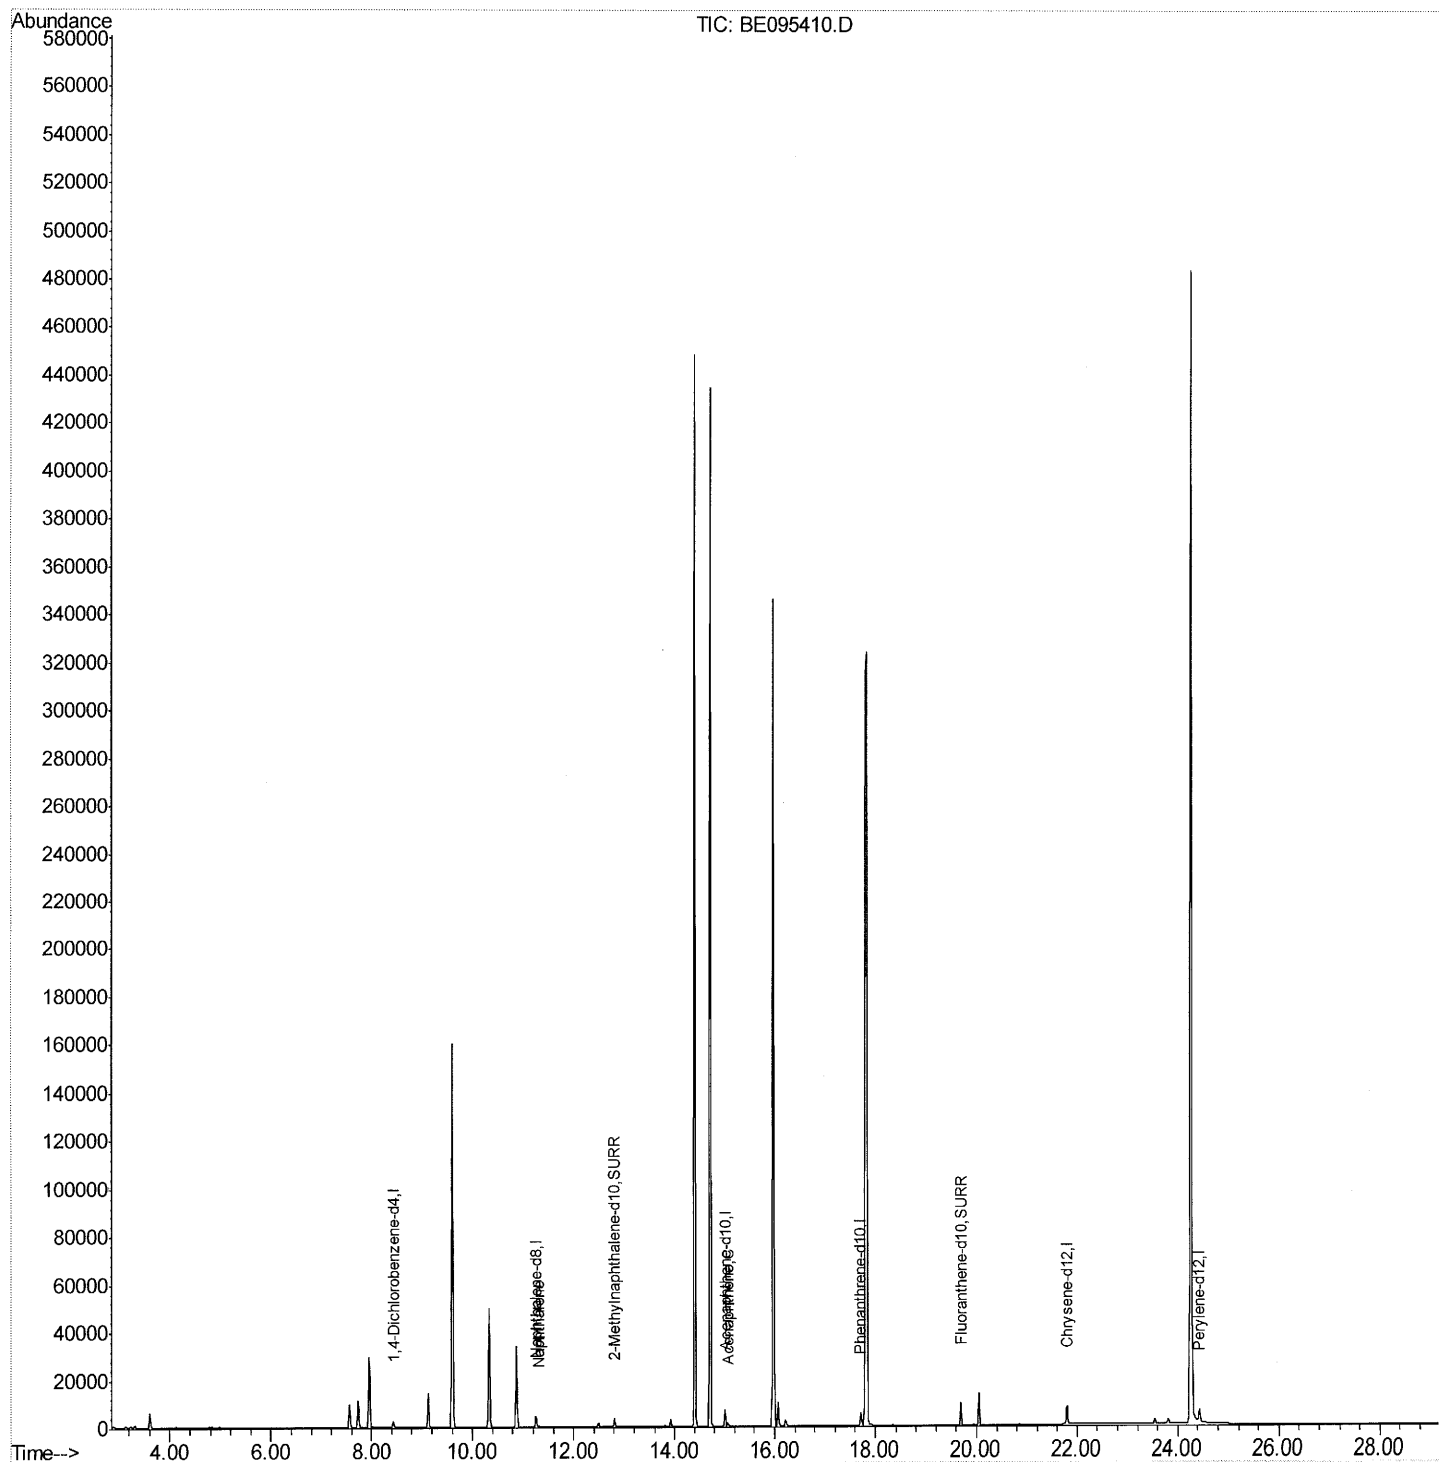

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020218\
 Data File : BE095410.D
 Acq On : 2 Feb 2018 22:58
 Operator : SJ/JU
 Sample : J1296-11
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Quant Time: Feb 03 05:27:36 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Feb 03 05:26:35 2018
 Response via : Initial Calibration

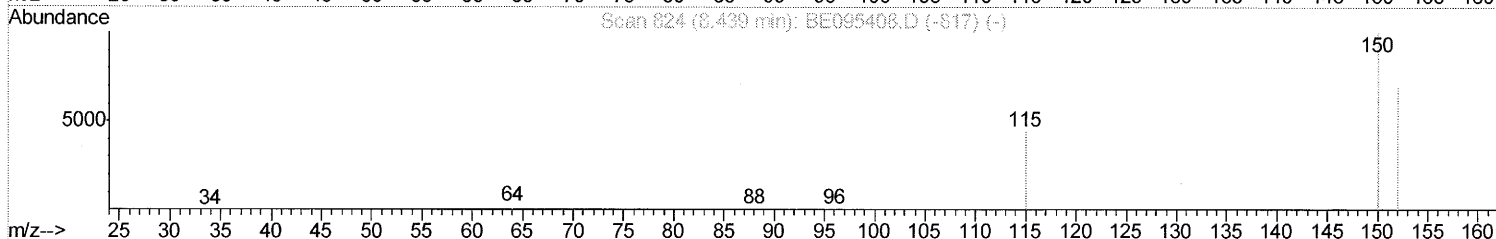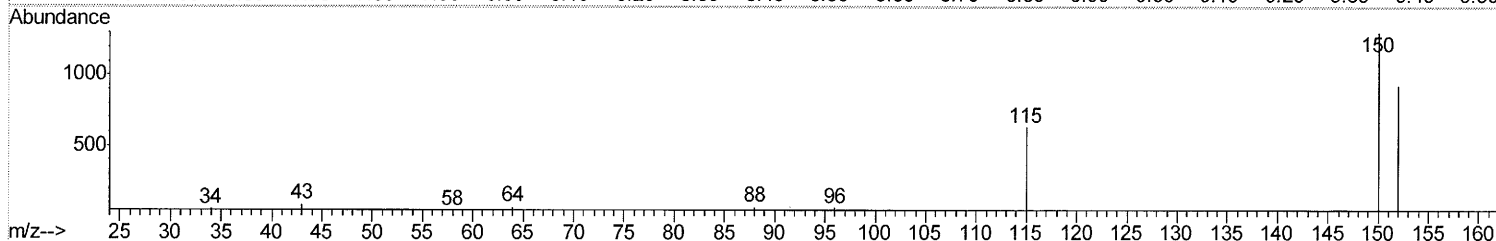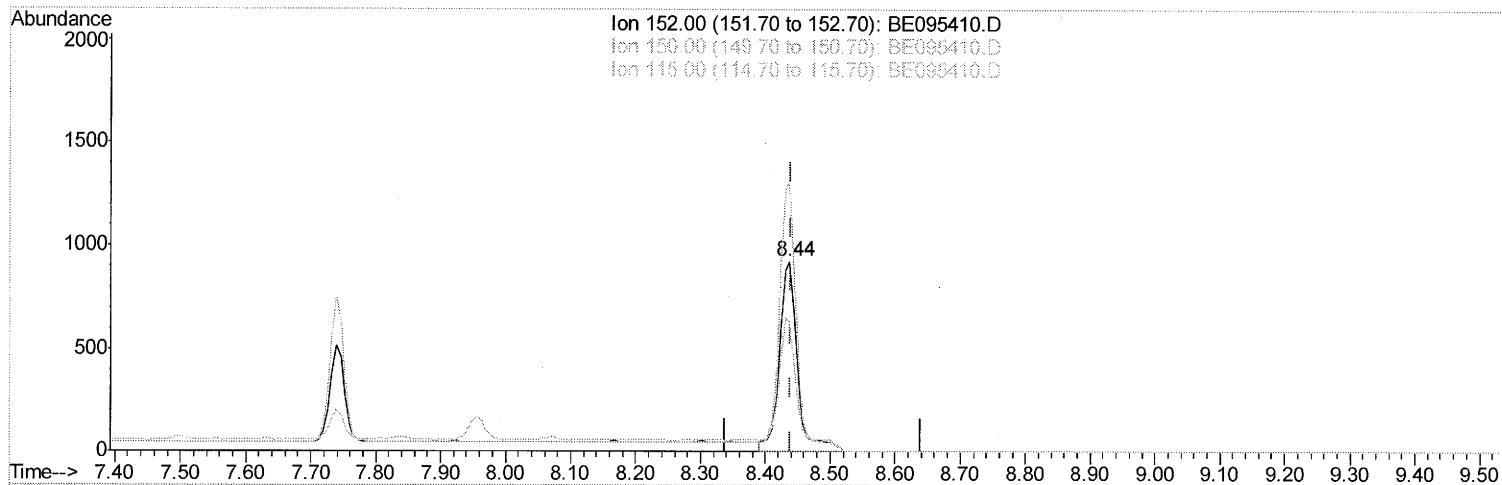

TIC: BE095410.D

(1) 1,4-Dichlorobenzene-d4 (I)

8.437min (-0.002) 0.40ng/ul




response 2028

Ion	Exp%	Act%
152.00	100	100
150.00	143.40	140.97
115.00	64.90	68.43
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020218\
 Data File : BE095410.D
 Acq On : 2 Feb 2018 22:58
 Operator : SJ/JU
 Sample : J1296-11
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Quant Time: Feb 03 05:27:36 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Feb 03 05:26:35 2018
 Response via : Initial Calibration

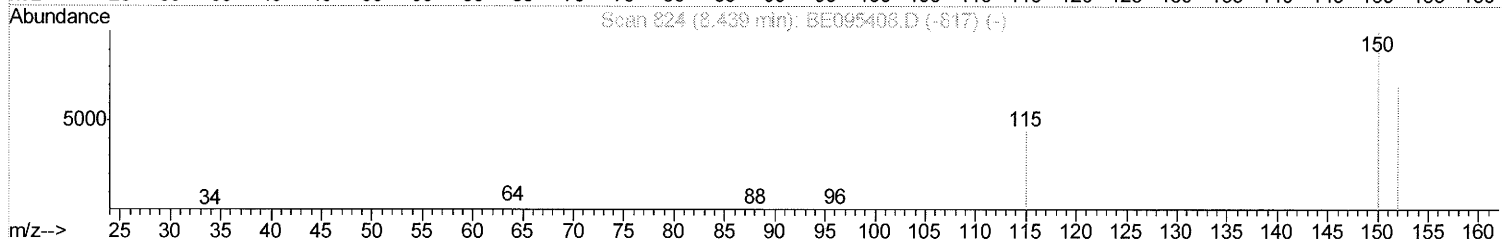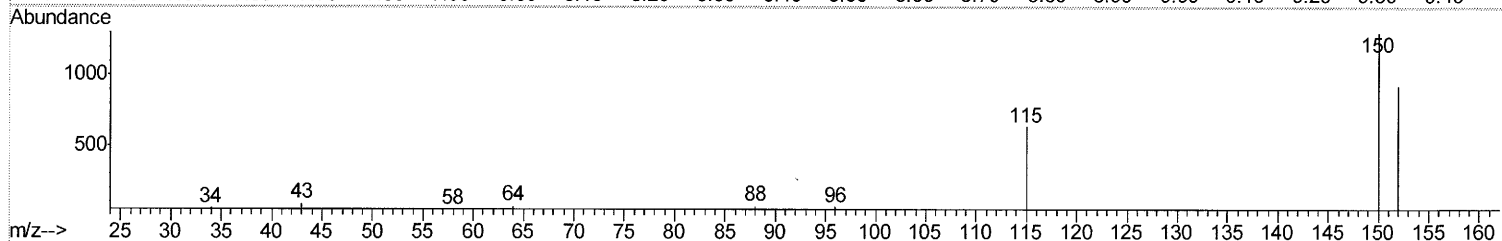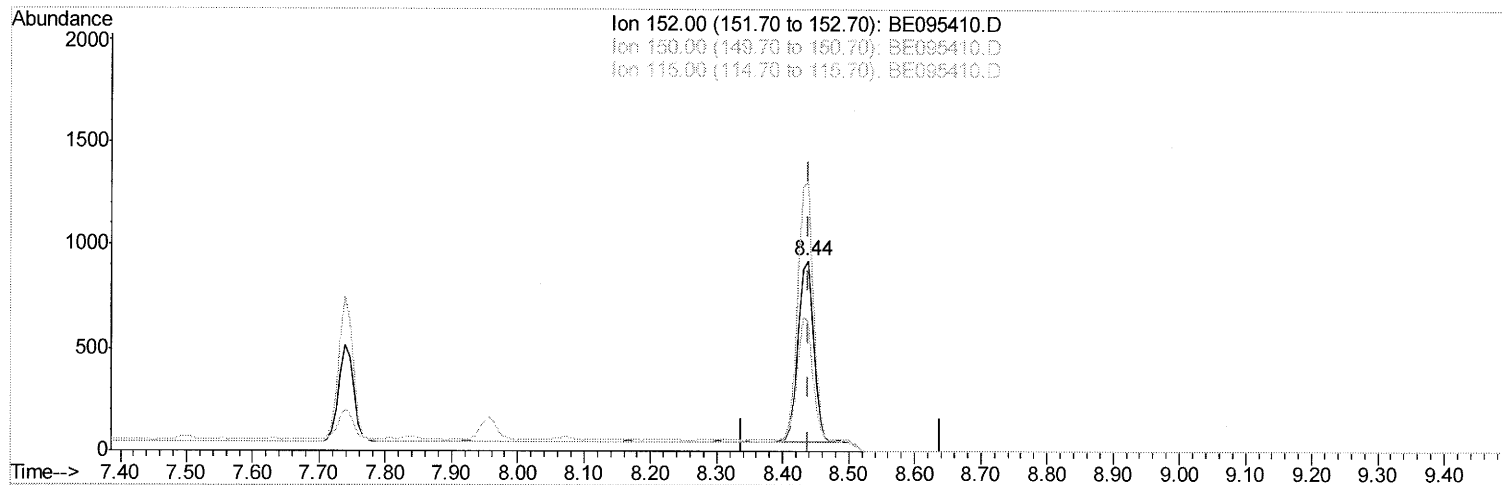

TIC: BE095410.D

(1) 1,4-Dichlorobenzene-d4 (I)

8.437min (-0.002) 0.40ng/ul m

SJ 2/7/18

response 1479

Ion	Exp%	Act%
152.00	100	100
150.00	143.40	140.97
115.00	64.90	68.43
0.00	0.00	0.00