


Data Path : Z:\HPCHEM1\BNA E\DATA\BE020218\
Data File : BE095411.D
Acq On : 2 Feb 2018 23:34
Operator : SJ/JU
Sample : J1317-02
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F6D48

Manual Integrations
APPROVED

Sohil
2/5/2018 5:48:26 PM

Quant Time: Feb 03 05:38:31 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 03 05:26:35 2018
Response via : Initial Calibration

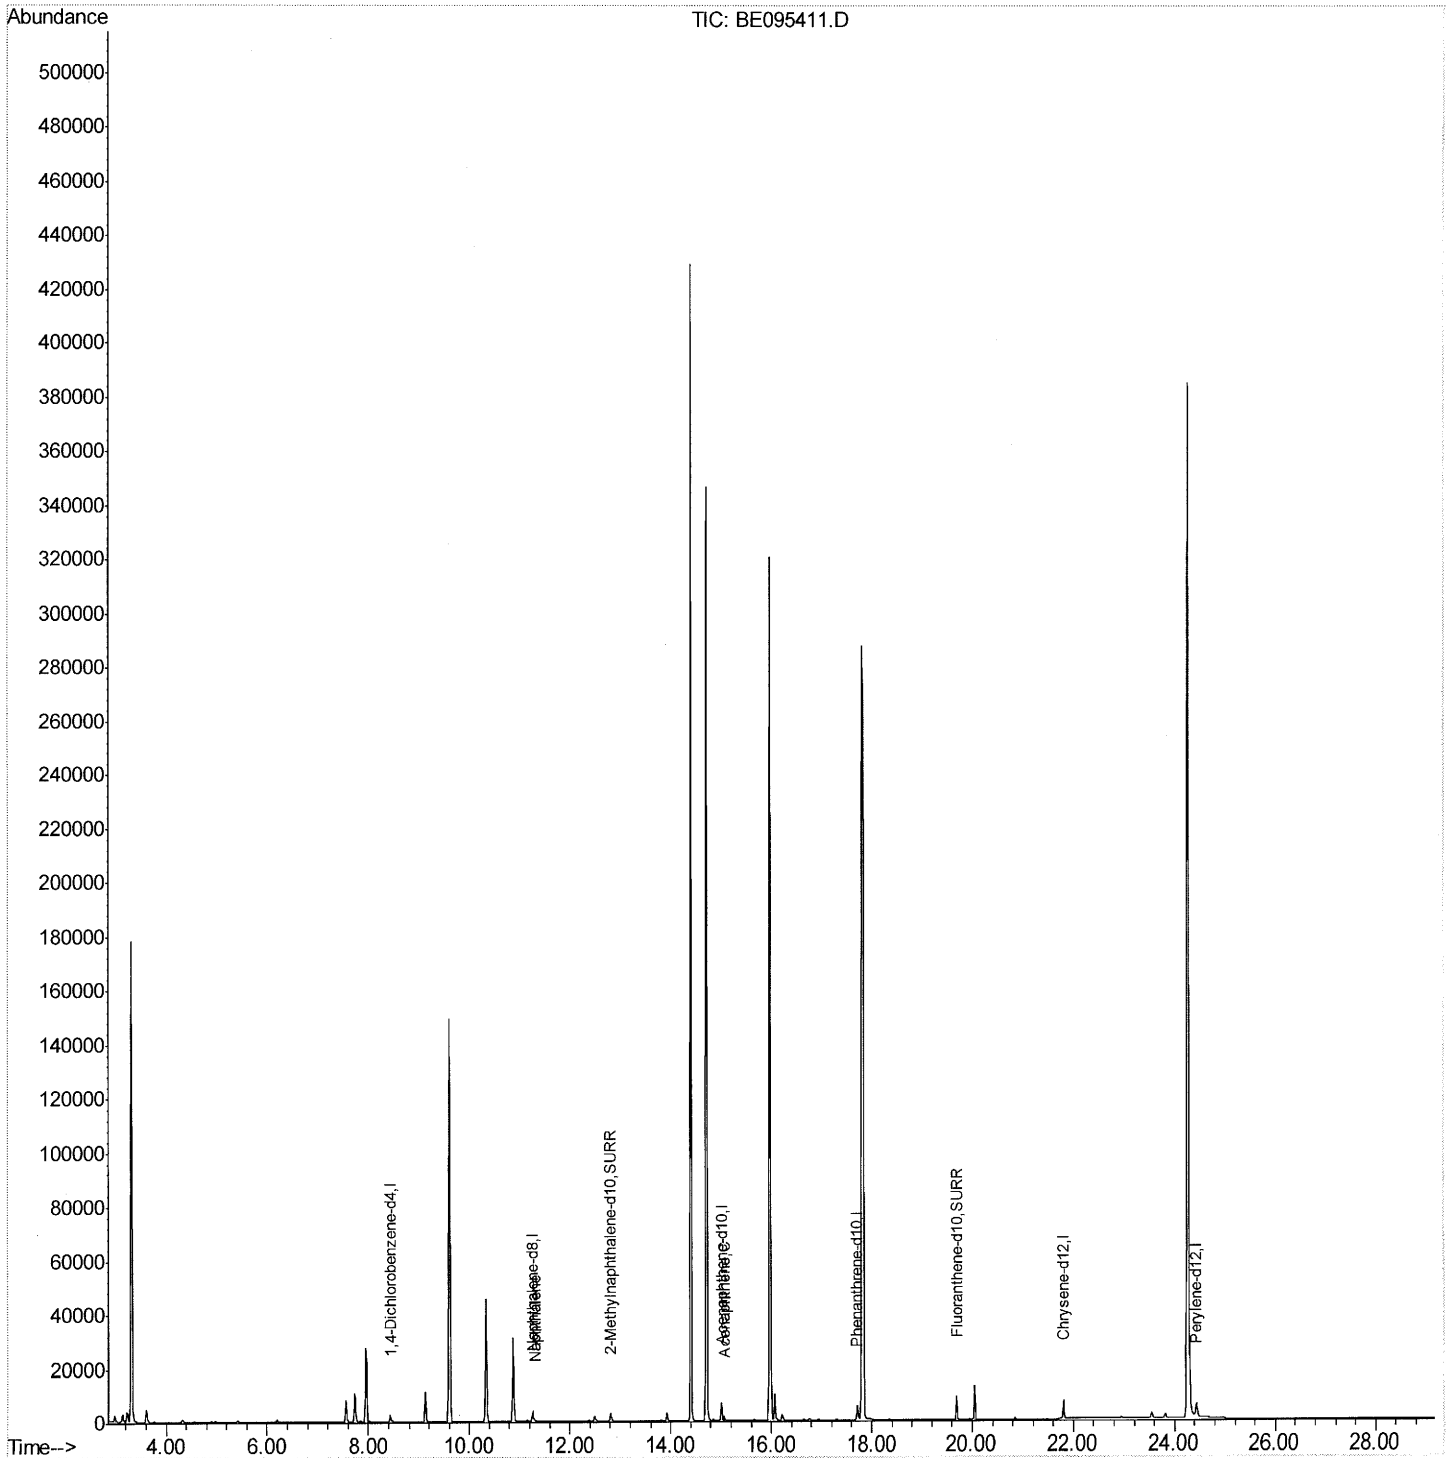

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE020218\
Data File : BE095411.D
Acq On : 2 Feb 2018 23:34
Operator : SJ/JU
Sample : J1317-02
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampled :
F6D48

Manual Integrations
APPROVED

Sohil
2/5/2018 5:48:26 PM

Quant Time: Feb 03 05:27:42 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 03 05:26:35 2018
Response via : Initial Calibration

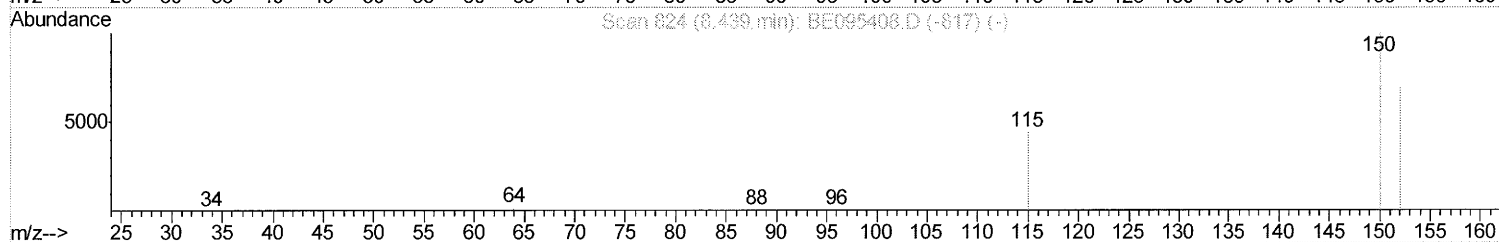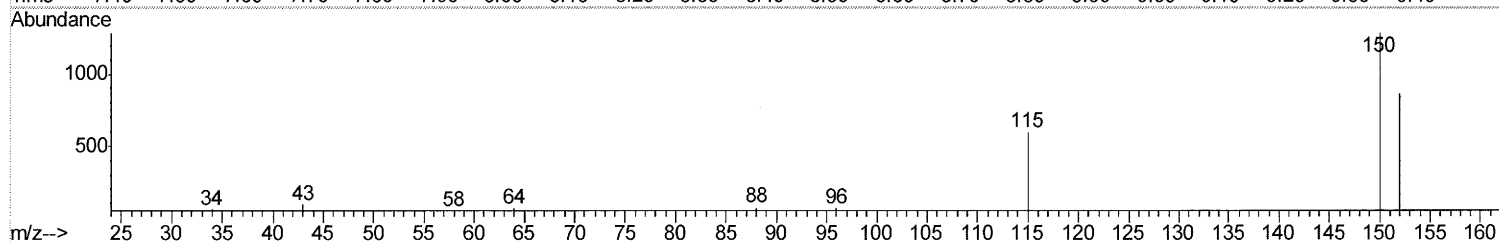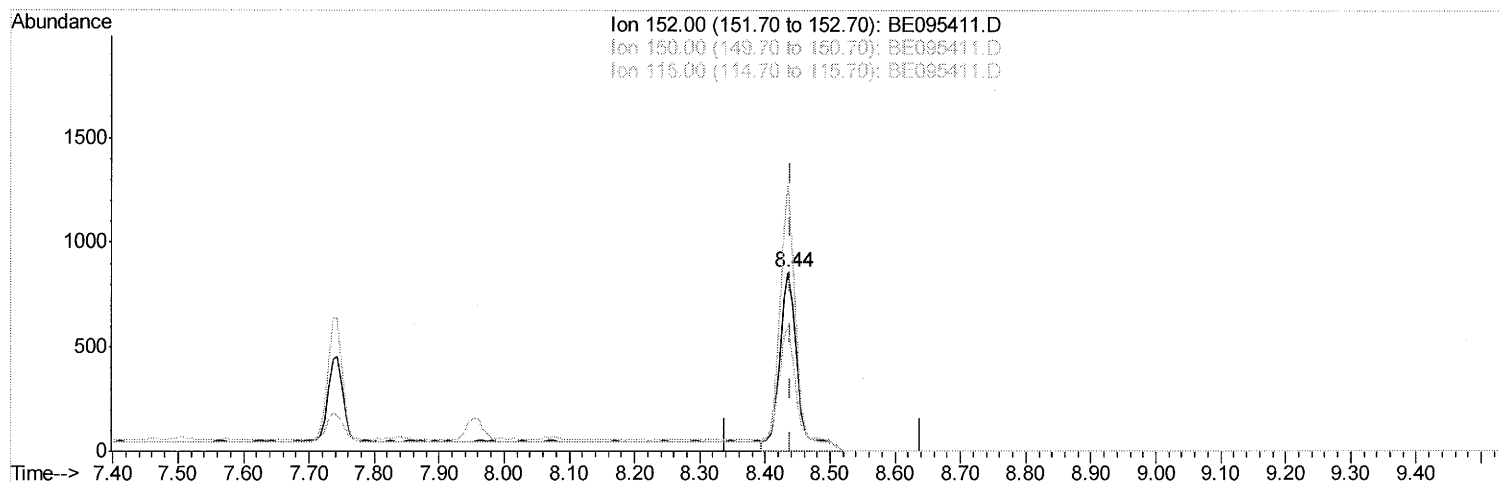

TIC: BE095411.D

(1) 1,4-Dichlorobenzene-d4 (I)

8.435min (-0.004) 0.40ng/ul

response 1860

Ion	Exp%	Act%
152.00	100	100
150.00	143.40	149.59
115.00	64.90	69.43
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE020218\
Data File : BE095411.D
Acq On : 2 Feb 2018 23:34
Operator : SJ/JU
Sample : J1317-02
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampled :
F6D48

Manual Integrations
APPROVED

Sohil
2/5/2018 5:48:26 PM

Quant Time: Feb 03 05:27:42 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 03 05:26:35 2018
Response via : Initial Calibration

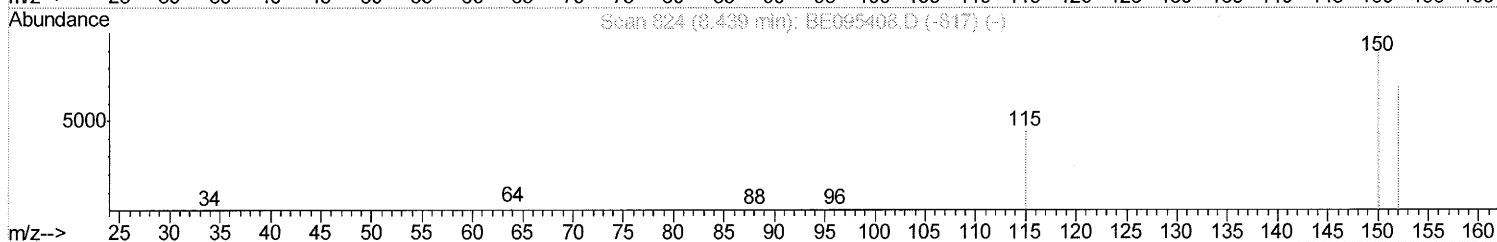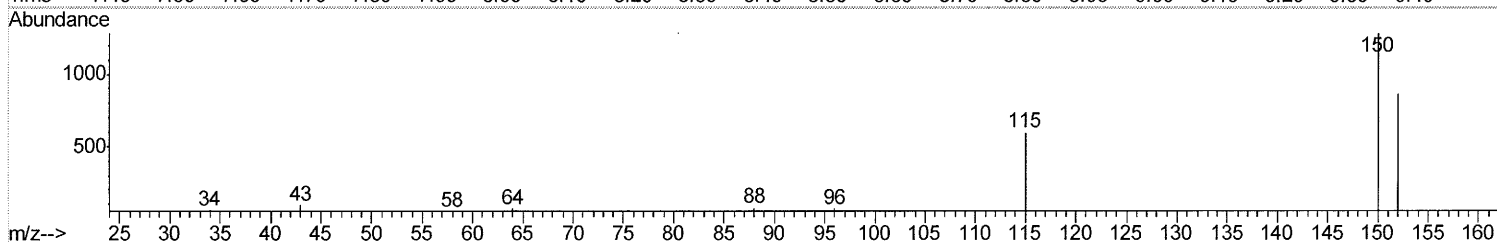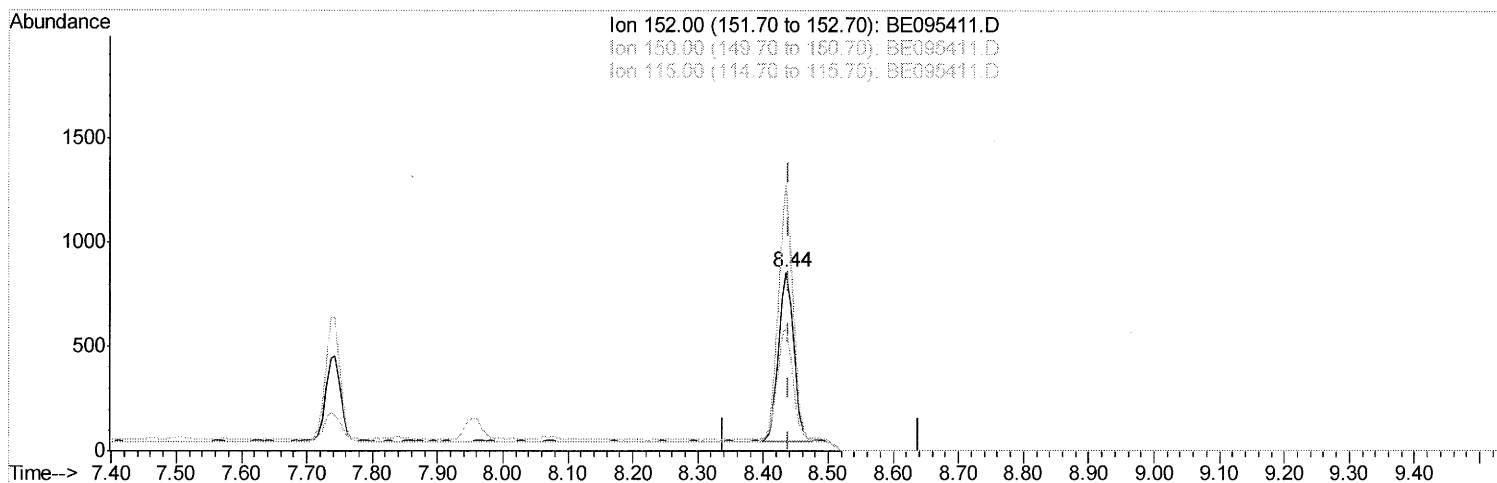

TIC: BE095411.D

(1) 1,4-Dichlorobenzene-d4 (I)

8.435min (-0.004) 0.40ng/ul m

SJ 2/7/18

response 1318

Ion	Exp%	Act%
152.00	100	100
150.00	143.40	149.59
115.00	64.90	69.43
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE020218\
 Data File : BE095411.D
 Acq On : 2 Feb 2018 23:34
 Operator : SJ/JU
 Sample : J1317-02
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 F6D48

Manual Integrations
 APPROVED

Sohil
 2/5/2018 5:48:26 PM

Quant Time: Feb 03 05:37:28 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Feb 03 05:26:35 2018
 Response via : Initial Calibration

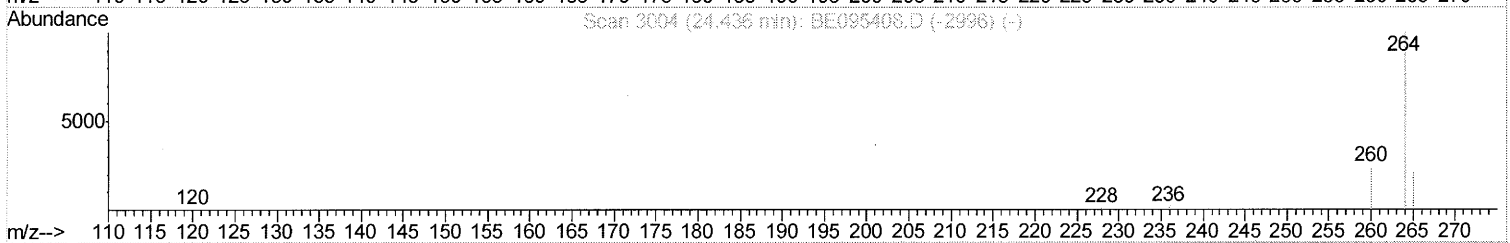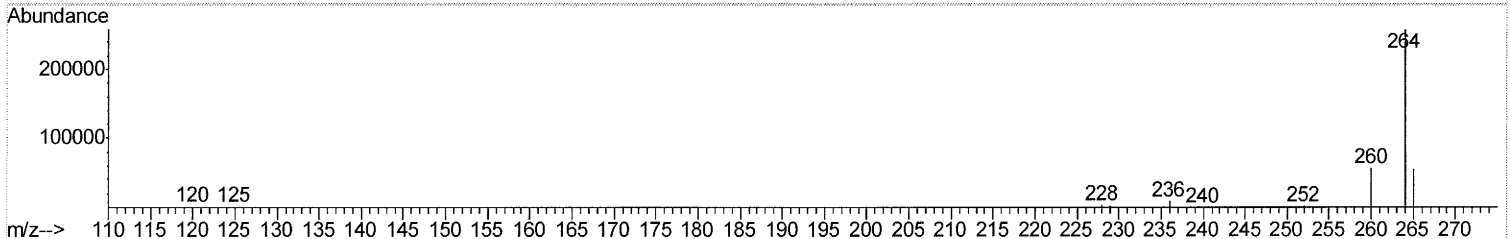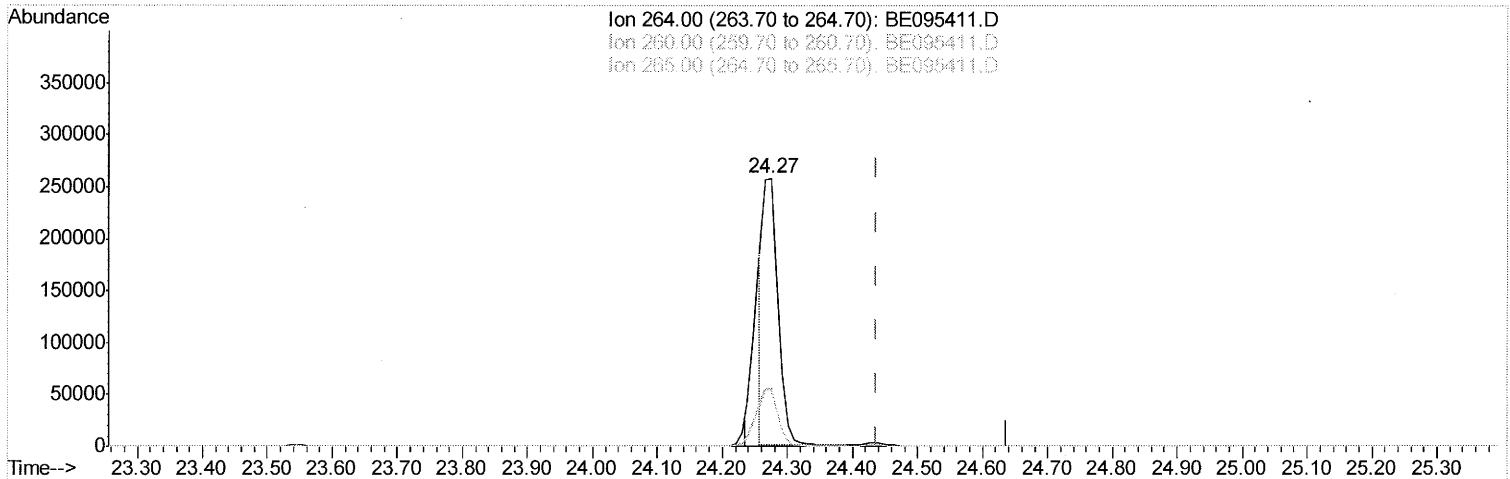

TIC: BE095411.D

(20) Perylene-d12 (I)

24.274min (-0.162) 0.40ng/ul

response 421493

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	21.65#
265.00	103.50	21.19#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE020218\
 Data File : BE095411.D
 Acq On : 2 Feb 2018 23:34
 Operator : SJ/JU
 Sample : J1317-02
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 F6D48

Manual Integrations
 APPROVED

Sohil
 2/5/2018 5:48:26 PM

Quant Time: Feb 03 05:37:28 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Feb 03 05:26:35 2018
 Response via : Initial Calibration

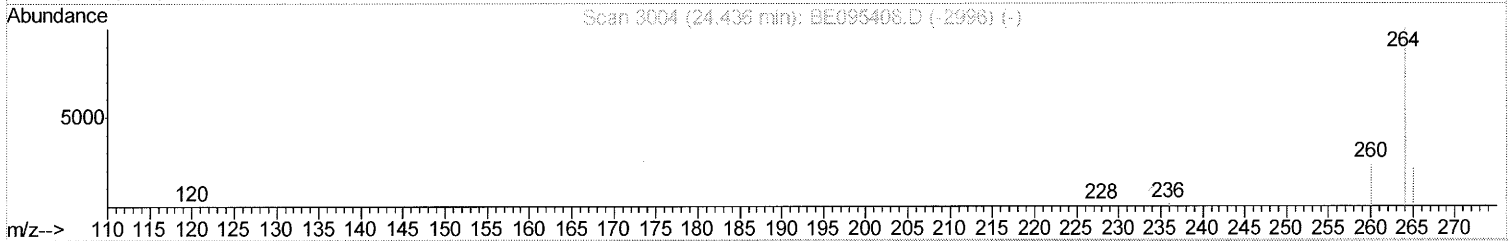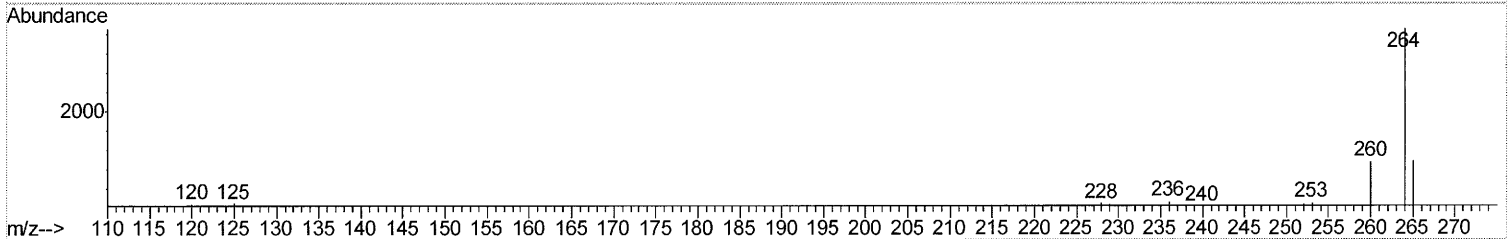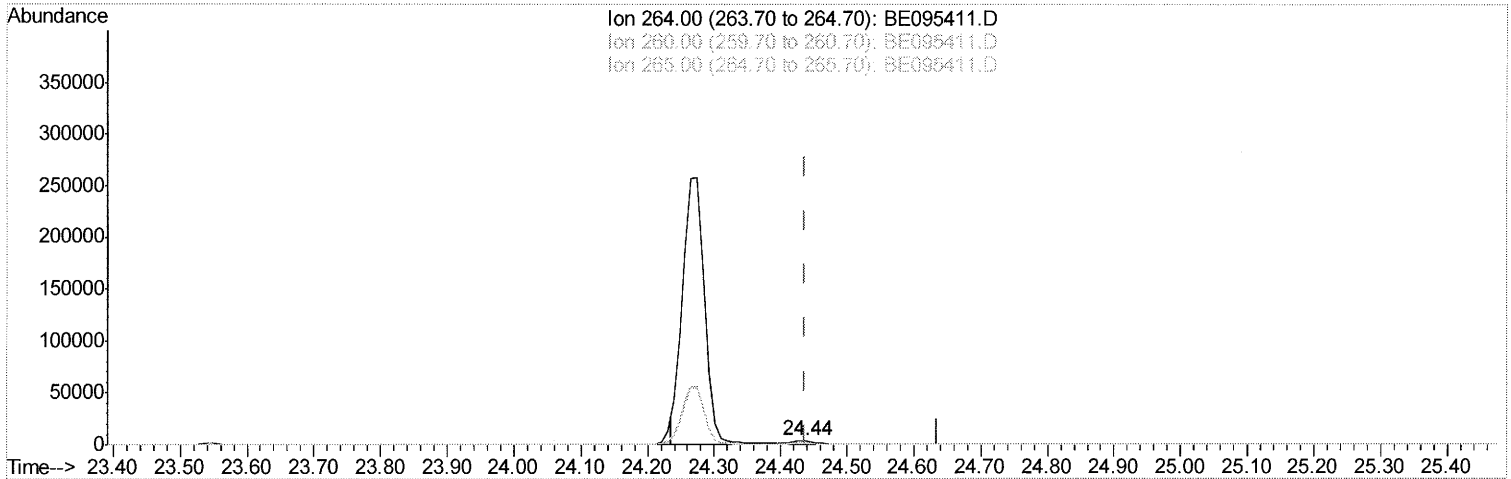

TIC: BE095411.D

(20) Perylene-d12 (I)

24.437min (+0.000) 0.40ng/ul m

SJ 2/7/18

response 6482

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	25.75
265.00	103.50	26.51#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020218\
 Data File : BE095411.D
 Acq On : 2 Feb 2018 23:34
 Operator : SJ/JU
 Sample : J1317-02
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 F6D48

Manual Integrations
 APPROVED

Sohil
 2/5/2018 5:48:26 PM

Quant Time: Feb 03 05:38:31 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Feb 03 05:26:35 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.44	152	1318m	0.40	ng/ul	0.00
2) Naphthalene-d8	11.26	136	5544	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.02	164	3671	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	7595	0.40	ng/ul	0.00
16) Chrysene-d12	21.81	240	7445	0.40	ng/ul	0.00
20) Perylene-d12	24.44	264	6482m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	3729	0.41	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	10225	0.35	ng/ul	0.00
Target Compounds						Ovalue
3) Naphthalene	11.31	128	460	0.030	ng/ul#	62
8) Acenaphthene	15.07	153	1802	0.132	ng/ul#	25

(#) = qualifier out of range (m) = manual integration (+) = signals summed