


Data Path : Z:\HPCHEM1\BNA E\DATA\BE020218\
 Data File : BE095418.D
 Acq On : 3 Feb 2018 3:42
 Operator : SJ/JU
 Sample : J1296-12
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 F6C29

Manual Integrations
 APPROVED
 Sohil
 2/5/2018 5:48:45 PM

Quant Time: Feb 03 06:03:03 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Feb 03 05:26:35 2018
 Response via : Initial Calibration

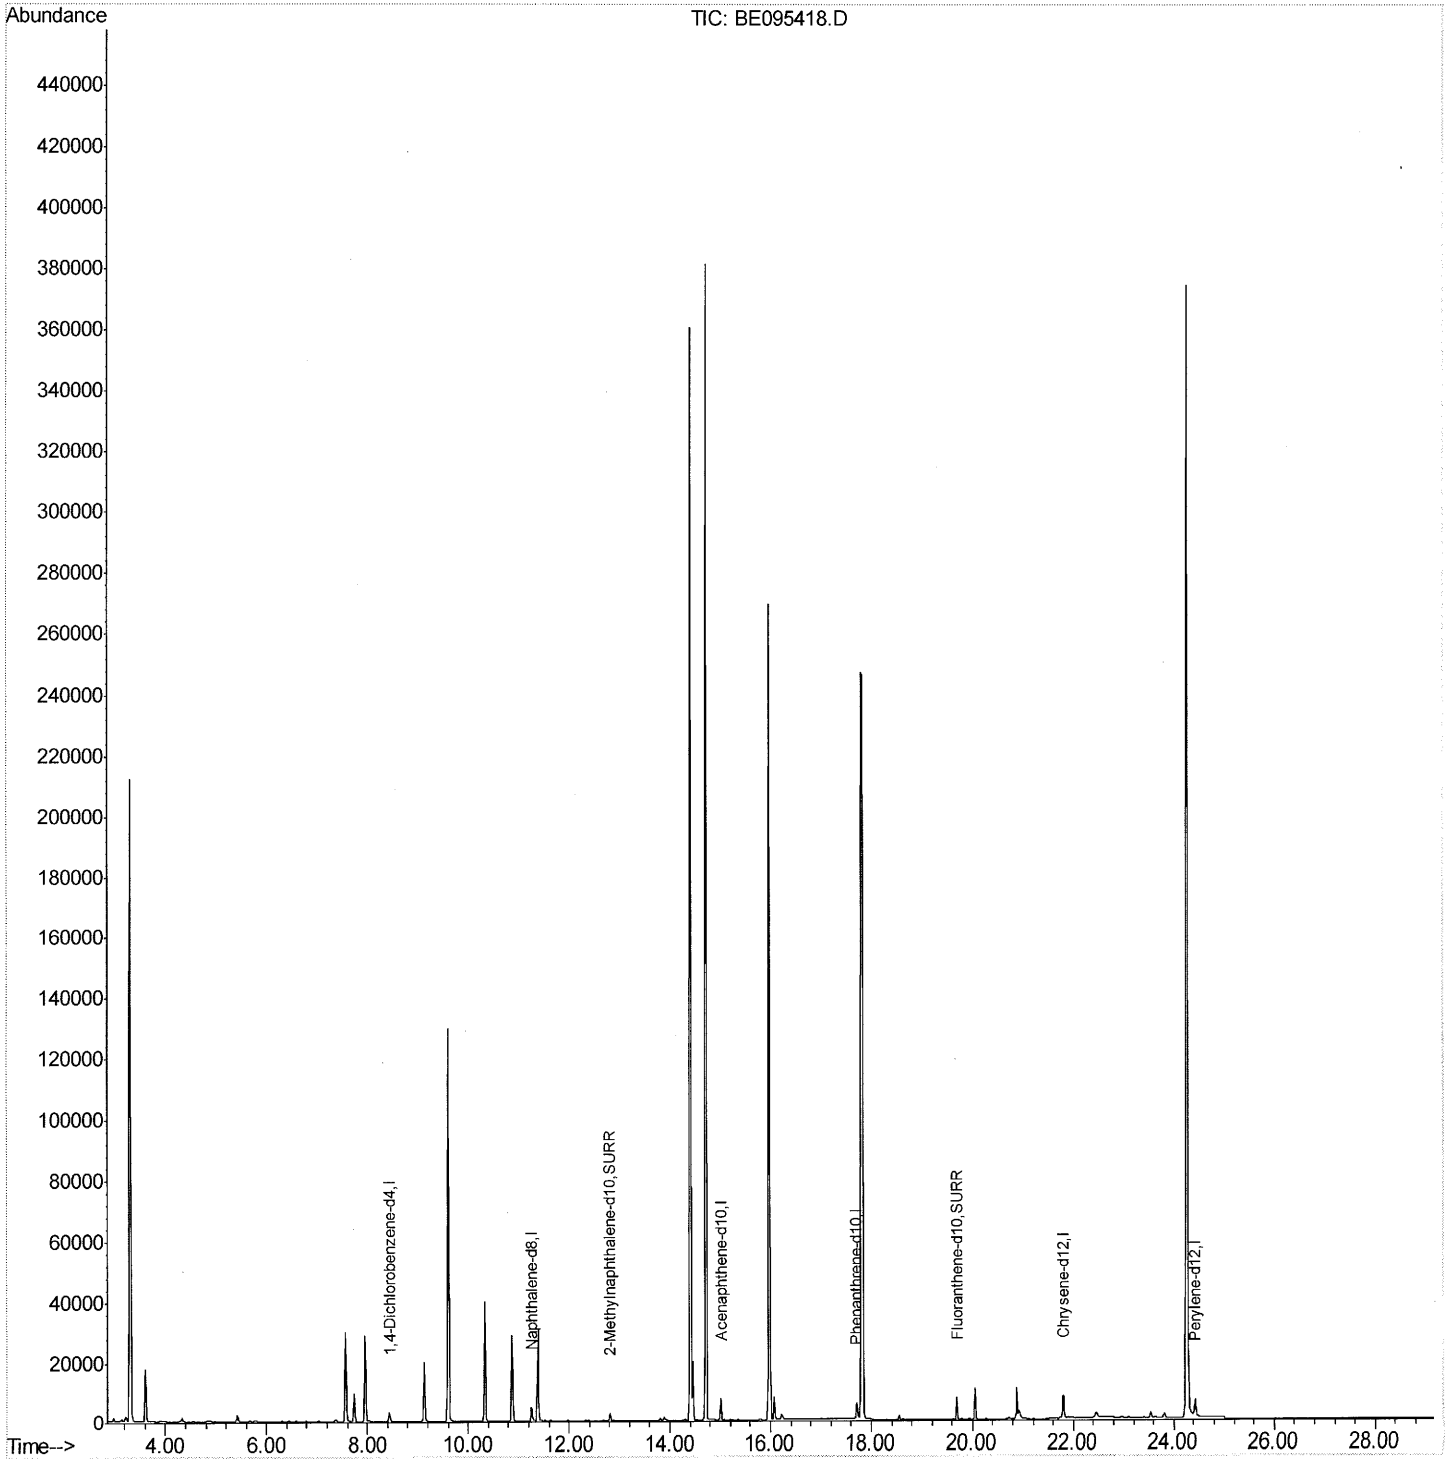




Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020218\
Data File : BE095418.D
Acq On : 3 Feb 2018 3:42
Operator : SJ/JU
Sample : J1296-12
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampled :
F6C29

Manual Integrations
APPROVED
Sohil
2/5/2018 5:48:45 PM

Quant Time: Feb 03 06:02:00 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 03 05:26:35 2018
Response via : Initial Calibration

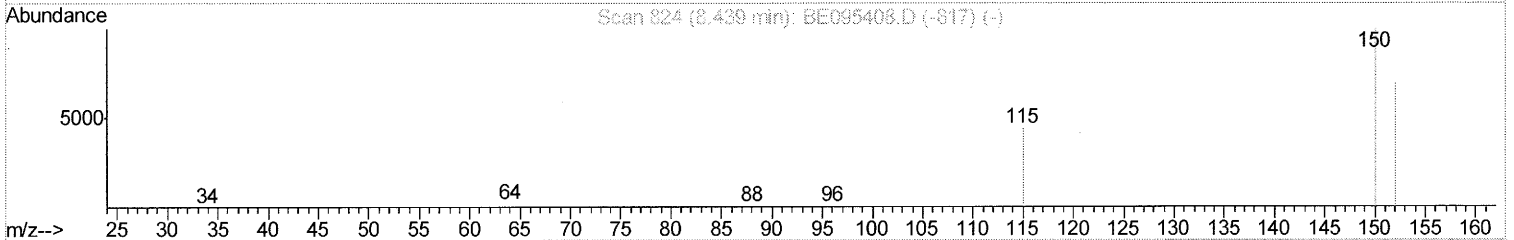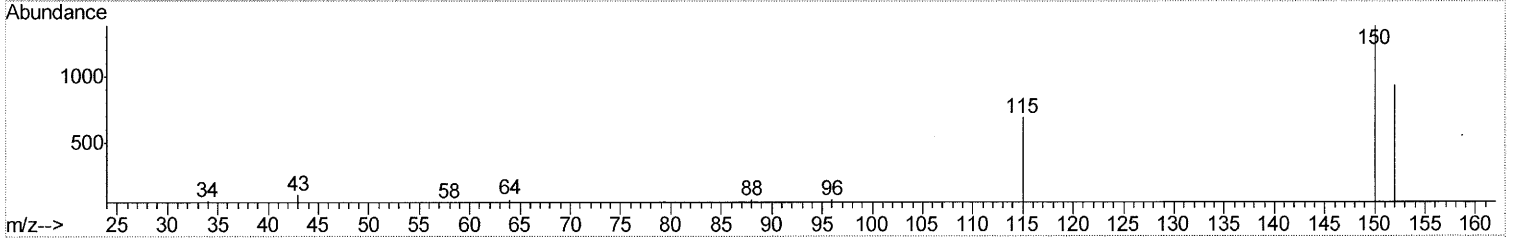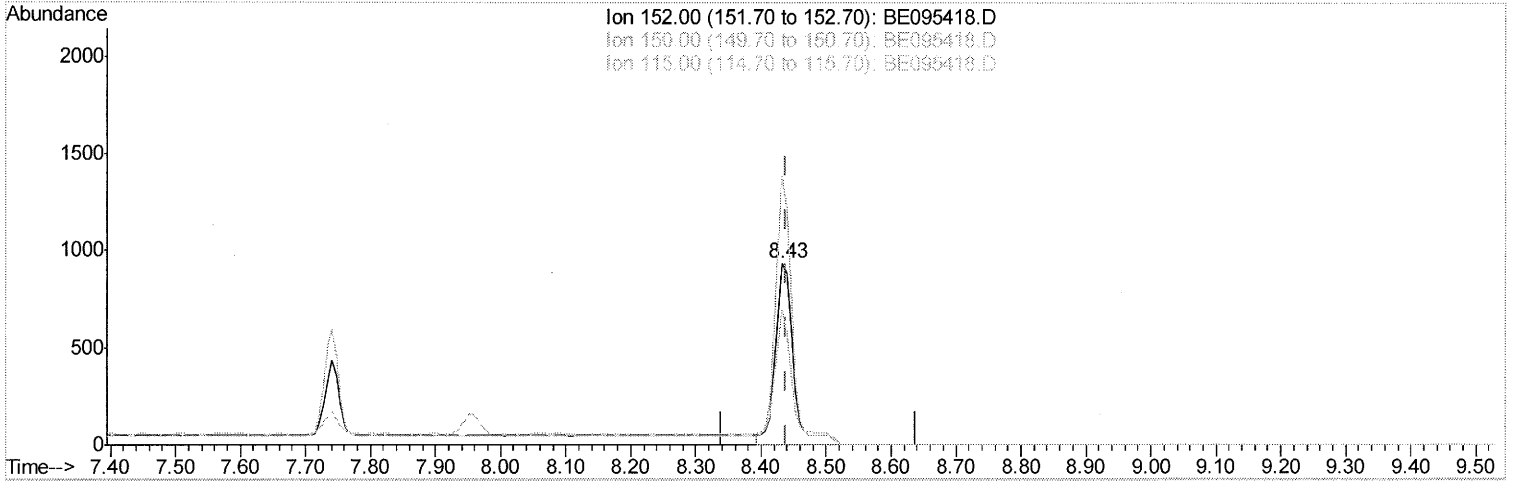

TIC: BE095418.D

(1) 1,4-Dichlorobenzene-d4 (l)

8.433min (-0.006) 0.40ng/ul

response 1999

Ion	Exp%	Act%
152.00	100	100
150.00	143.40	148.29
115.00	64.90	73.98
0.00	0.00	0.00




Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020218\
 Data File : BE095418.D
 Acq On : 3 Feb 2018 3:42
 Operator : SJ/JU
 Sample : J1296-12
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 F6C29

Manual Integrations
 APPROVED
 Sohil
 2/5/2018 5:48:45 PM

Quant Time: Feb 03 06:02:00 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Feb 03 05:26:35 2018
 Response via : Initial Calibration

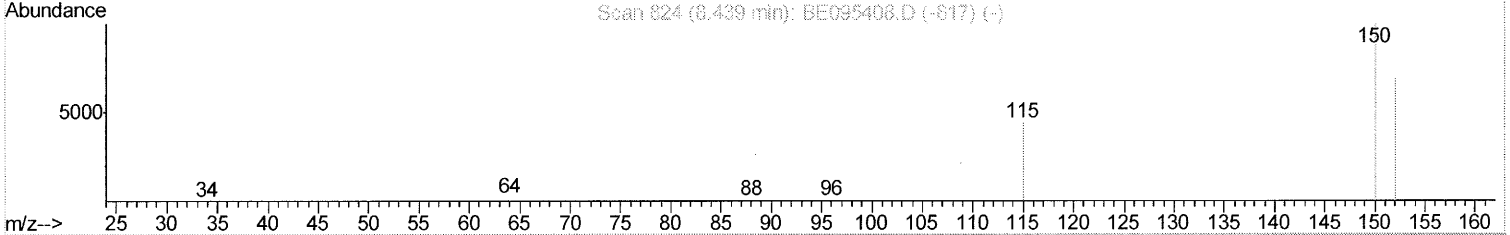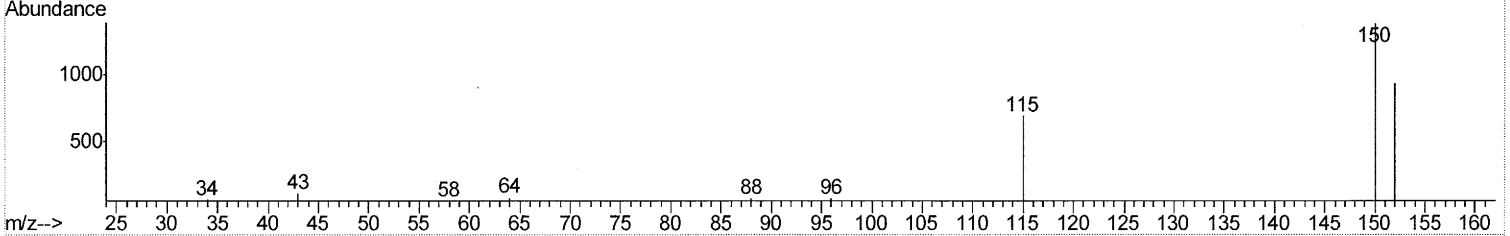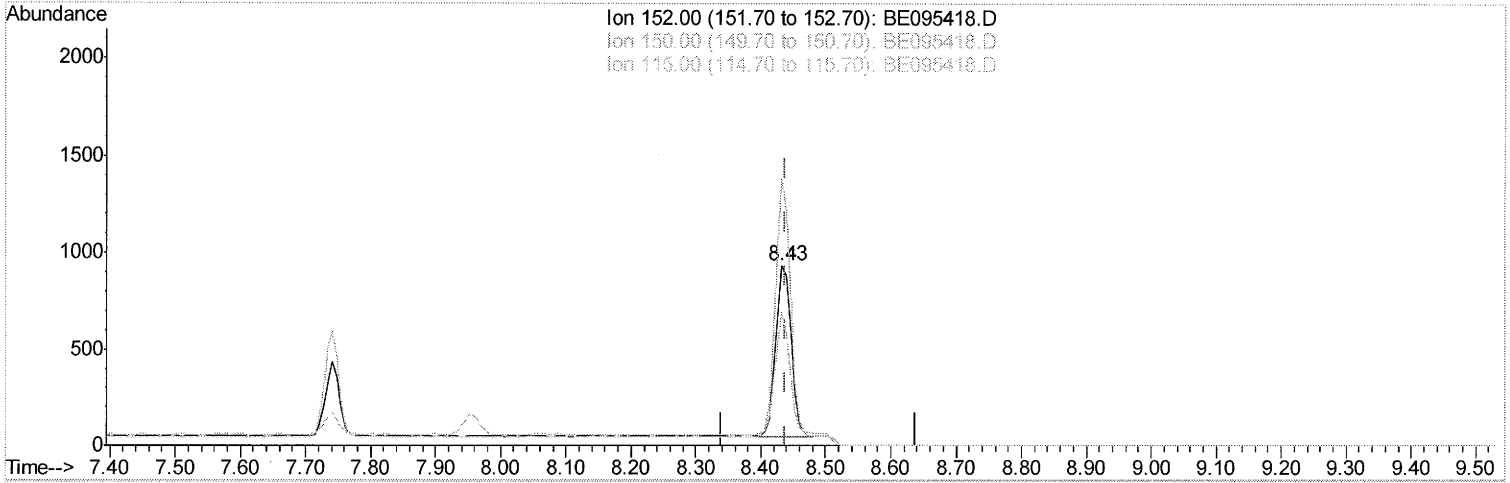

TIC: BE095418.D

(1) 1,4-Dichlorobenzene-d4 (l)

8.433min (-0.006) 0.40ng/ul m

SJ 2/7/18

response 1498

Ion	Exp%	Act%
152.00	100	100
150.00	143.40	148.29
115.00	64.90	73.98
0.00	0.00	0.00




Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020218\
Data File : BE095418.D
Acq On : 3 Feb 2018 3:42
Operator : SJ/JU
Sample : J1296-12
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_E
Client Sampled :
F6C29

Manual Integrations
APPROVED
Sohil
2/5/2018 5:48:45 PM

Quant Time: Feb 03 06:02:16 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 03 05:26:35 2018
Response via : Initial Calibration

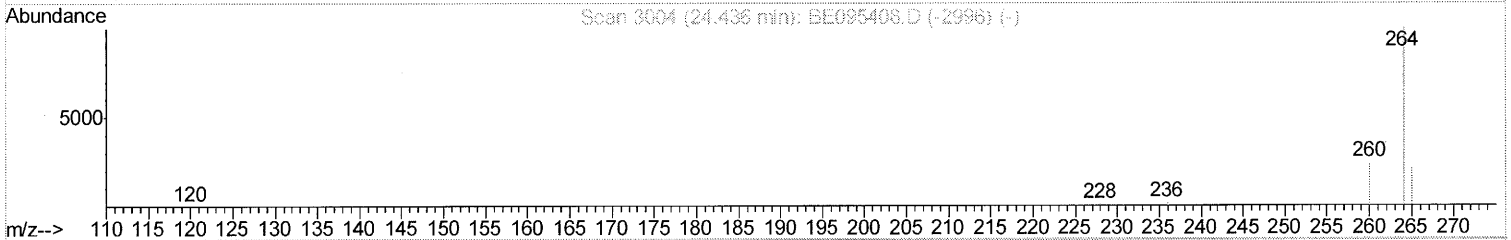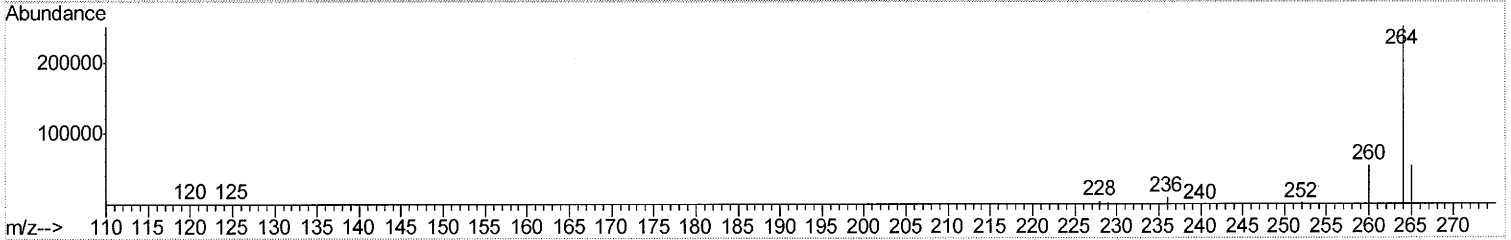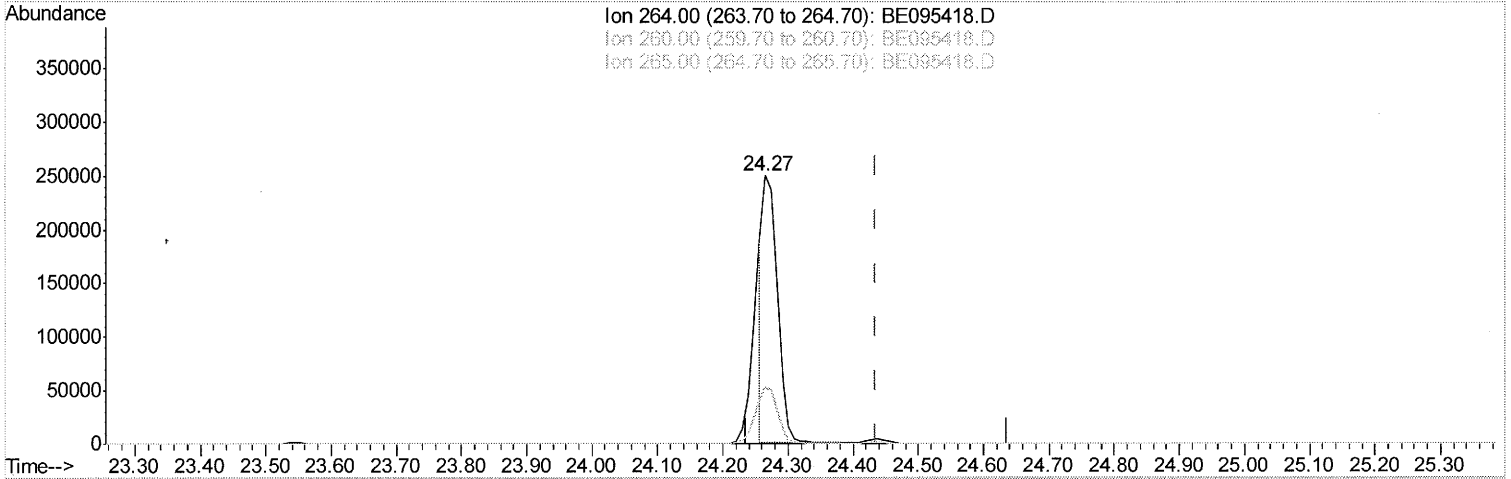

TIC: BE095418.D

(20) Perylene-d12 (I)
24.265min (-0.171) 0.40ng/ul
response 383704

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	21.37#
265.00	103.50	21.34#
0.00	0.00	0.00




Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020218\
Data File : BE095418.D
Acq On : 3 Feb 2018 3:42
Operator : SJ/JU
Sample : J1296-12
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_E
Client Sampled :
F6C29

Manual Integrations
APPROVED
Sohil
2/5/2018 5:48:45 PM

Quant Time: Feb 03 06:02:16 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 03 05:26:35 2018
Response via : Initial Calibration

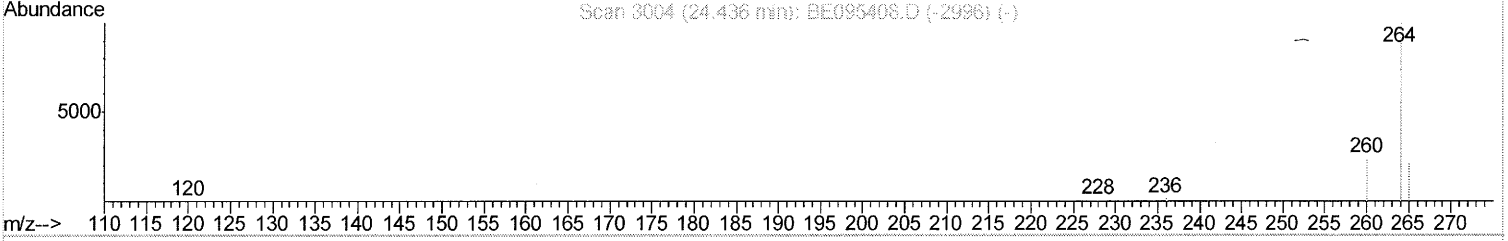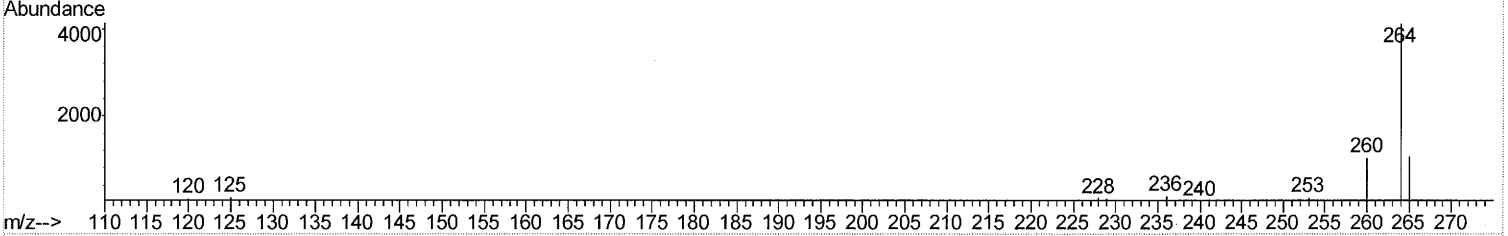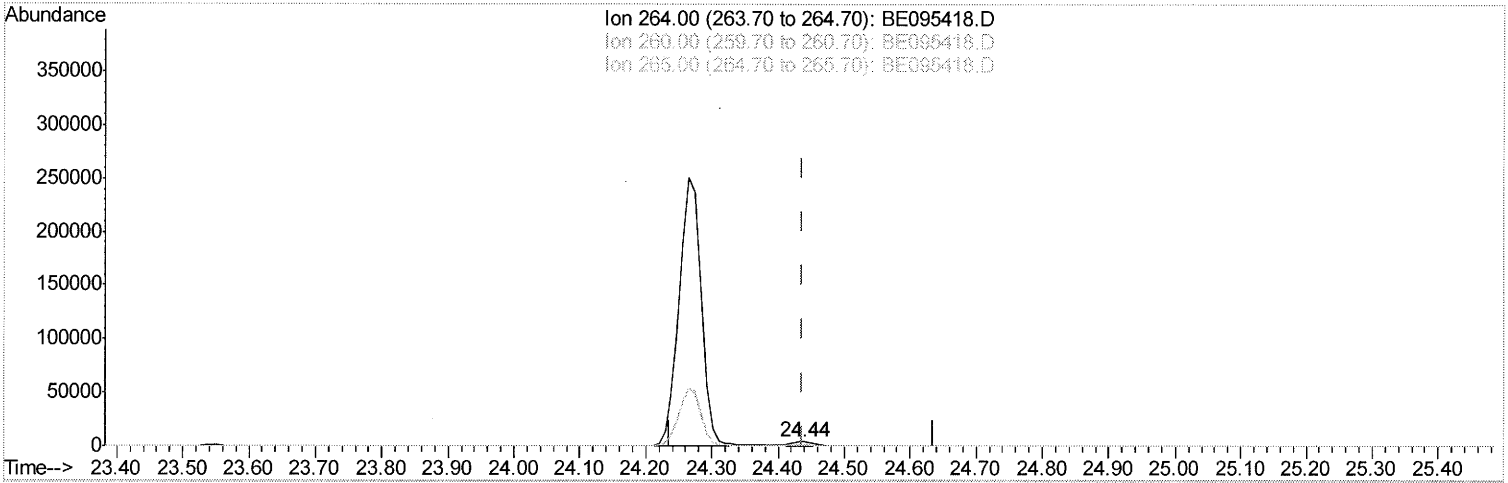

TIC: BE095418.D

(20) Perylene-d12 (I)

24.436min (+0.000) 0.40ng/ul m

SS 2/7/18

response 7658

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	25.17
265.00	103.50	25.46#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020218\
 Data File : BE095418.D
 Acq On : 3 Feb 2018 3:42
 Operator : SJ/JU
 Sample : J1296-12
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 F6C29

Manual Integrations
 APPROVED
 Sohil
 2/5/2018 5:48:45 PM

Quant Time: Feb 03 06:03:03 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Feb 03 05:26:35 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.43	152	1498m	0.40	ng/ul	0.00
2) Naphthalene-d8	11.26	136	6221	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.02	164	4020	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	8192	0.40	ng/ul	0.00
16) Chrysene-d12	21.80	240	8482	0.40	ng/ul	0.00
20) Perylene-d12	24.44	264	7658m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	3356	0.33	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	8329	0.27	ng/ul	0.00

SS 2/7/18

SS 2/7/18

Target Compounds Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed