


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA_E\Data\BE020218\
Data File : BE095419.D
Acq On : 3 Feb 2018 4:18
Operator : SJ/JU
Sample : J1296-10
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F6C28

Manual Integrations
APPROVED

Sohil
2/5/2018 5:48:47 PM

Quant Time: Feb 05 17:16:28 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 05 04:46:10 2018
Response via : Initial Calibration

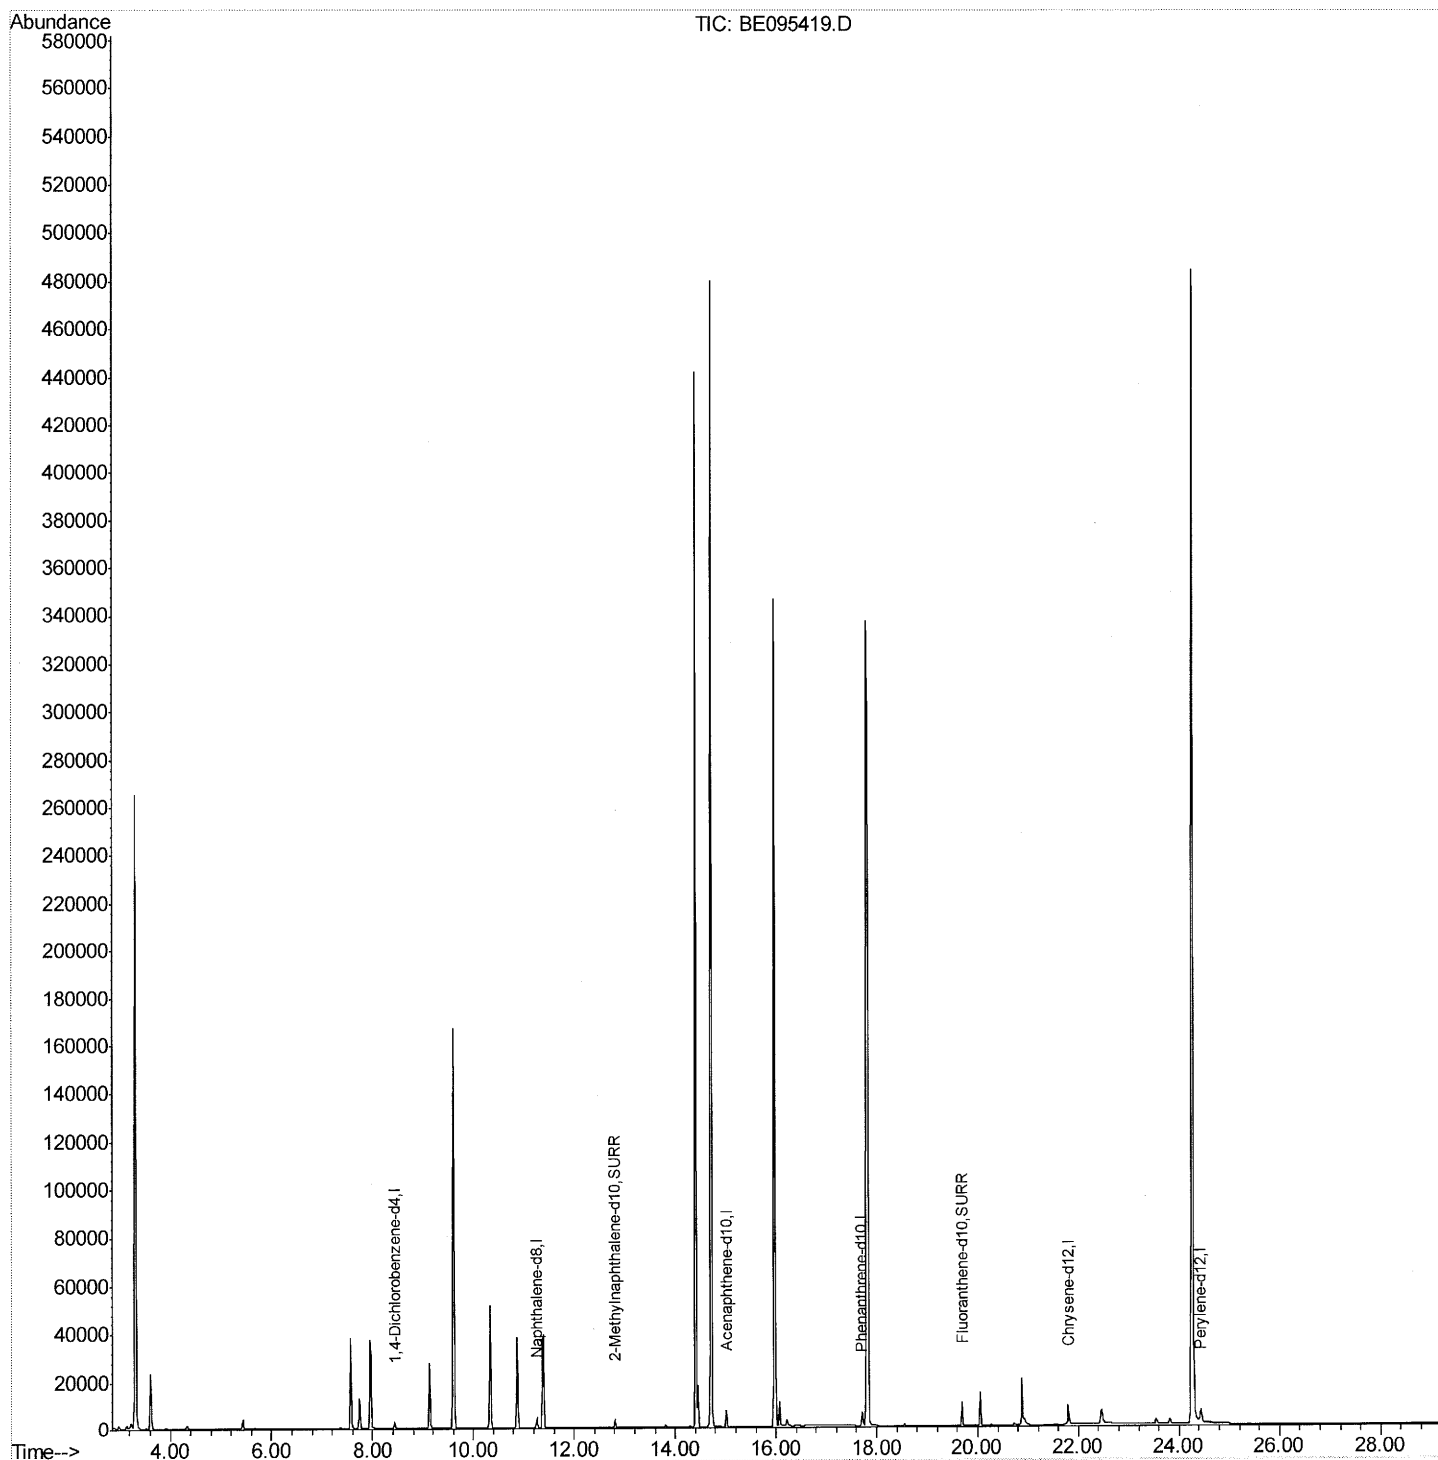

Quantitation Report (Qedit)




Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA_E\Data\BE020218\
 Data File : BE095419.D
 Acq On : 3 Feb 2018 4:18
 Operator : SJ/JU
 Sample : J1296-10
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 F6C28

Manual Integrations
 APPROVED

Sohil
 2/5/2018 5:48:47 PM

Quant Time: Feb 05 17:14:52 2018
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 05 04:46:10 2018
 Response via : Initial Calibration

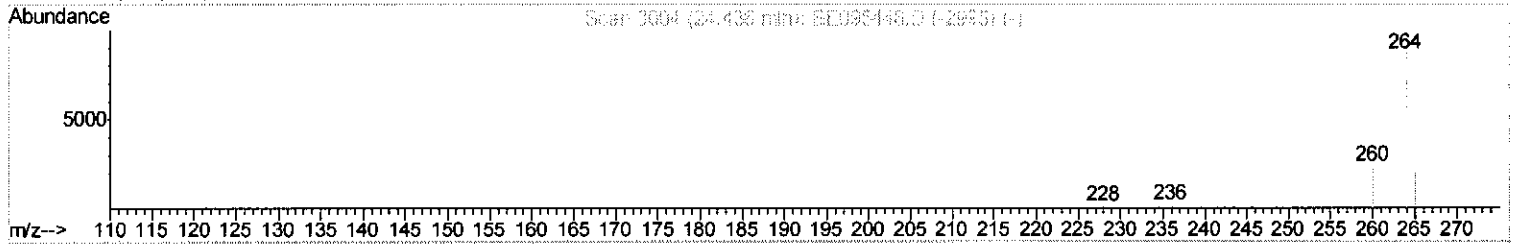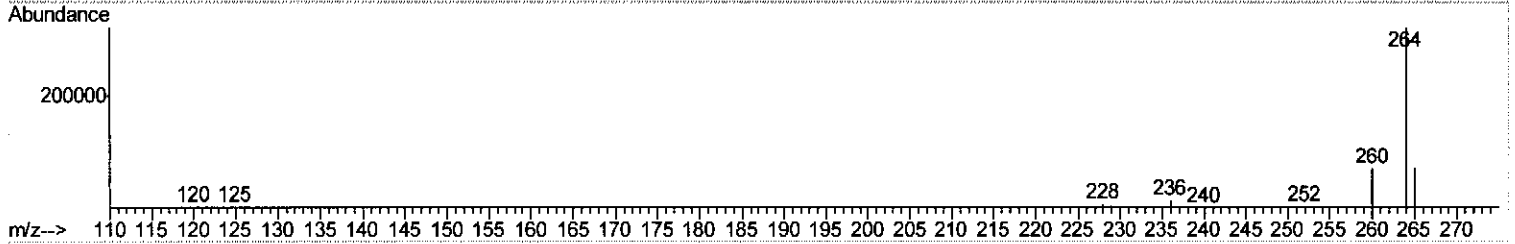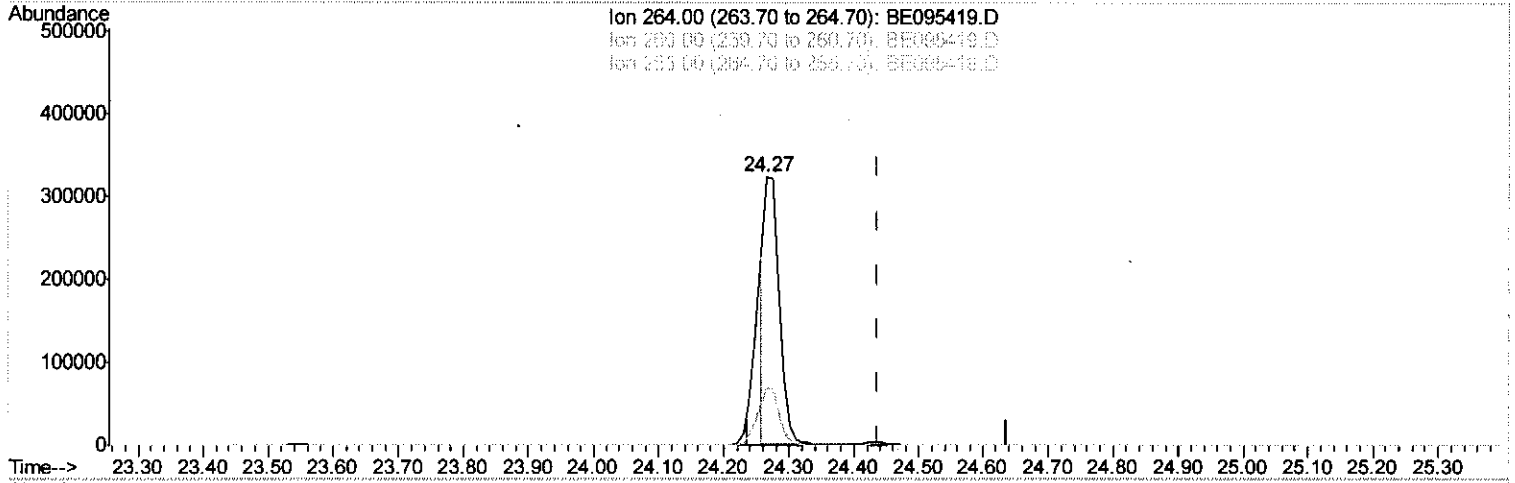

TIC: BE095419.D

(20) Perylene-d12 (I)

24.265min (-0.171) 0.40ng/ul

response 524229

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	21.58#
265.00	103.50	21.27#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA_E\Data\BE020218\
Data File : BE095419.D
Acq On : 3 Feb 2018 4:18
Operator : SJ/JU
Sample : J1296-10
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_E
Client Sampled :
F6C28

Manual Integrations
APPROVED

Sohil
2/5/2018 5:48:47 PM

Quant Time: Feb 05 17:14:52 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 05 04:46:10 2018
Response via : Initial Calibration

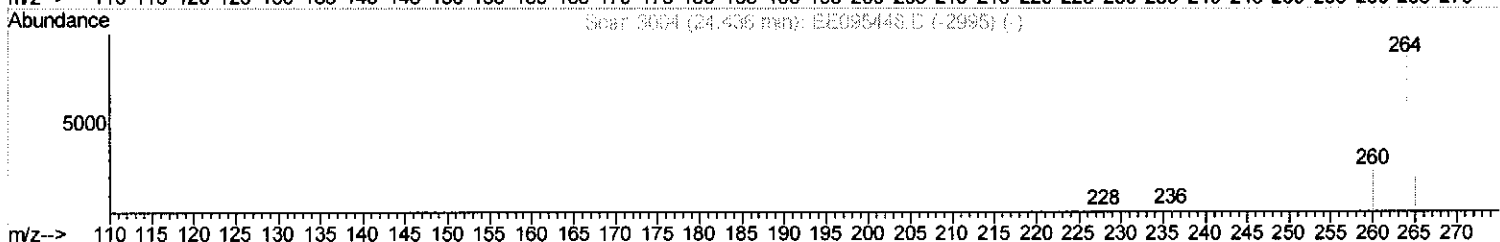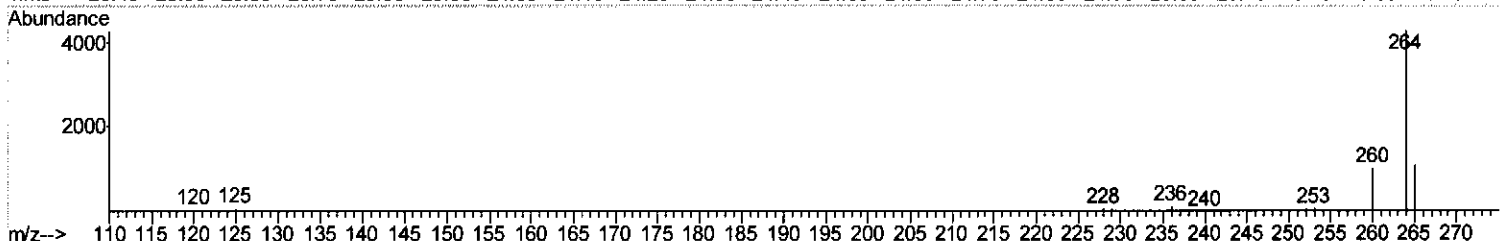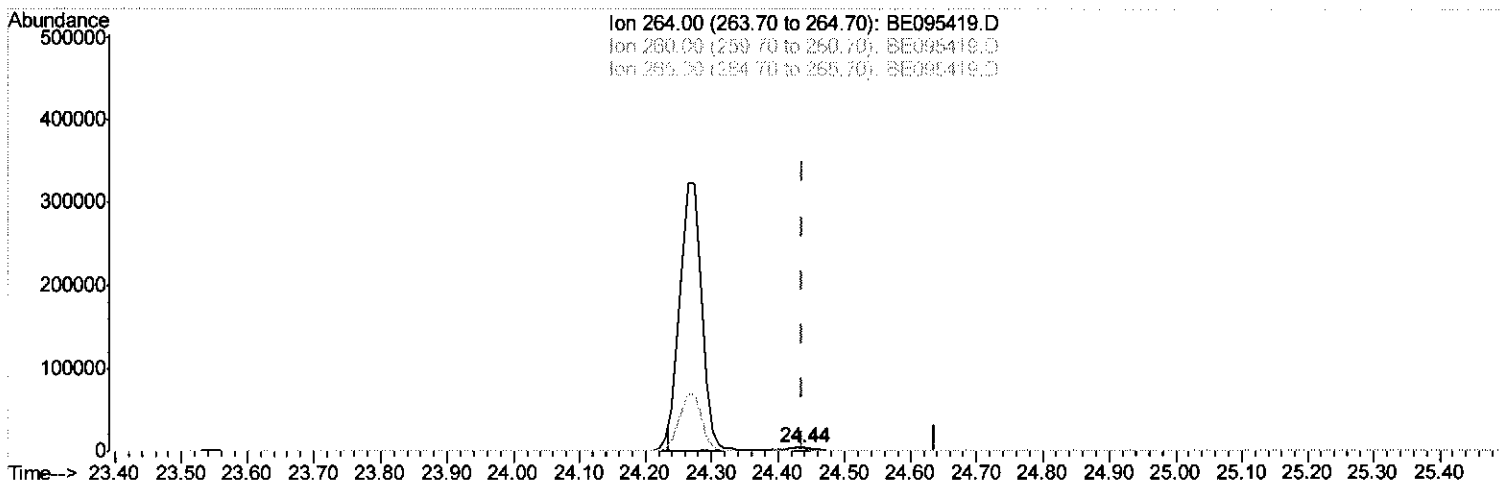

TIC: BE095419.D

(20) Perylene-d12 (I)

24.437min (+0.000) 0.40ng/ul m

SS 2/7/18

response 7689

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	24.56
265.00	103.50	25.41#
0.00	0.00	0.00

Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA_E\Data\BE020218\
Data File : BE095419.D
Acq On : 3 Feb 2018 4:18
Operator : SJ/JU
Sample : J1296-10
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleID :
F6C28

Manual Integrations
APPROVED

Sohil
2/5/2018 5:48:47 PM

Quant Time: Feb 05 17:16:28 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 05 04:46:10 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.44	152	2065	0.40	ng/ul	0.00
2) Naphthalene-d8	11.26	136	6274	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.02	164	4089	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	8684	0.40	ng/ul	0.00
16) Chrysene-d12	21.81	240	8652	0.40	ng/ul	0.00
20) Perylene-d12	24.44	264	7689m	0.40	ng/ul	0.00

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	12.81	152	4308	0.42	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	10972	0.33	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

12/7/18