


Data Path : Z:\HPCHEM1\BNA E\DATA\BE020218\
Data File : BE095420.D
Acq On : 3 Feb 2018 4:54
Operator : SJ/JU
Sample : J1296-07
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F6C25

Manual Integrations
APPROVED

Sohil
2/5/2018 5:48:50 PM

Quant Time: Feb 03 06:08:36 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 03 05:26:35 2018
Response via : Initial Calibration

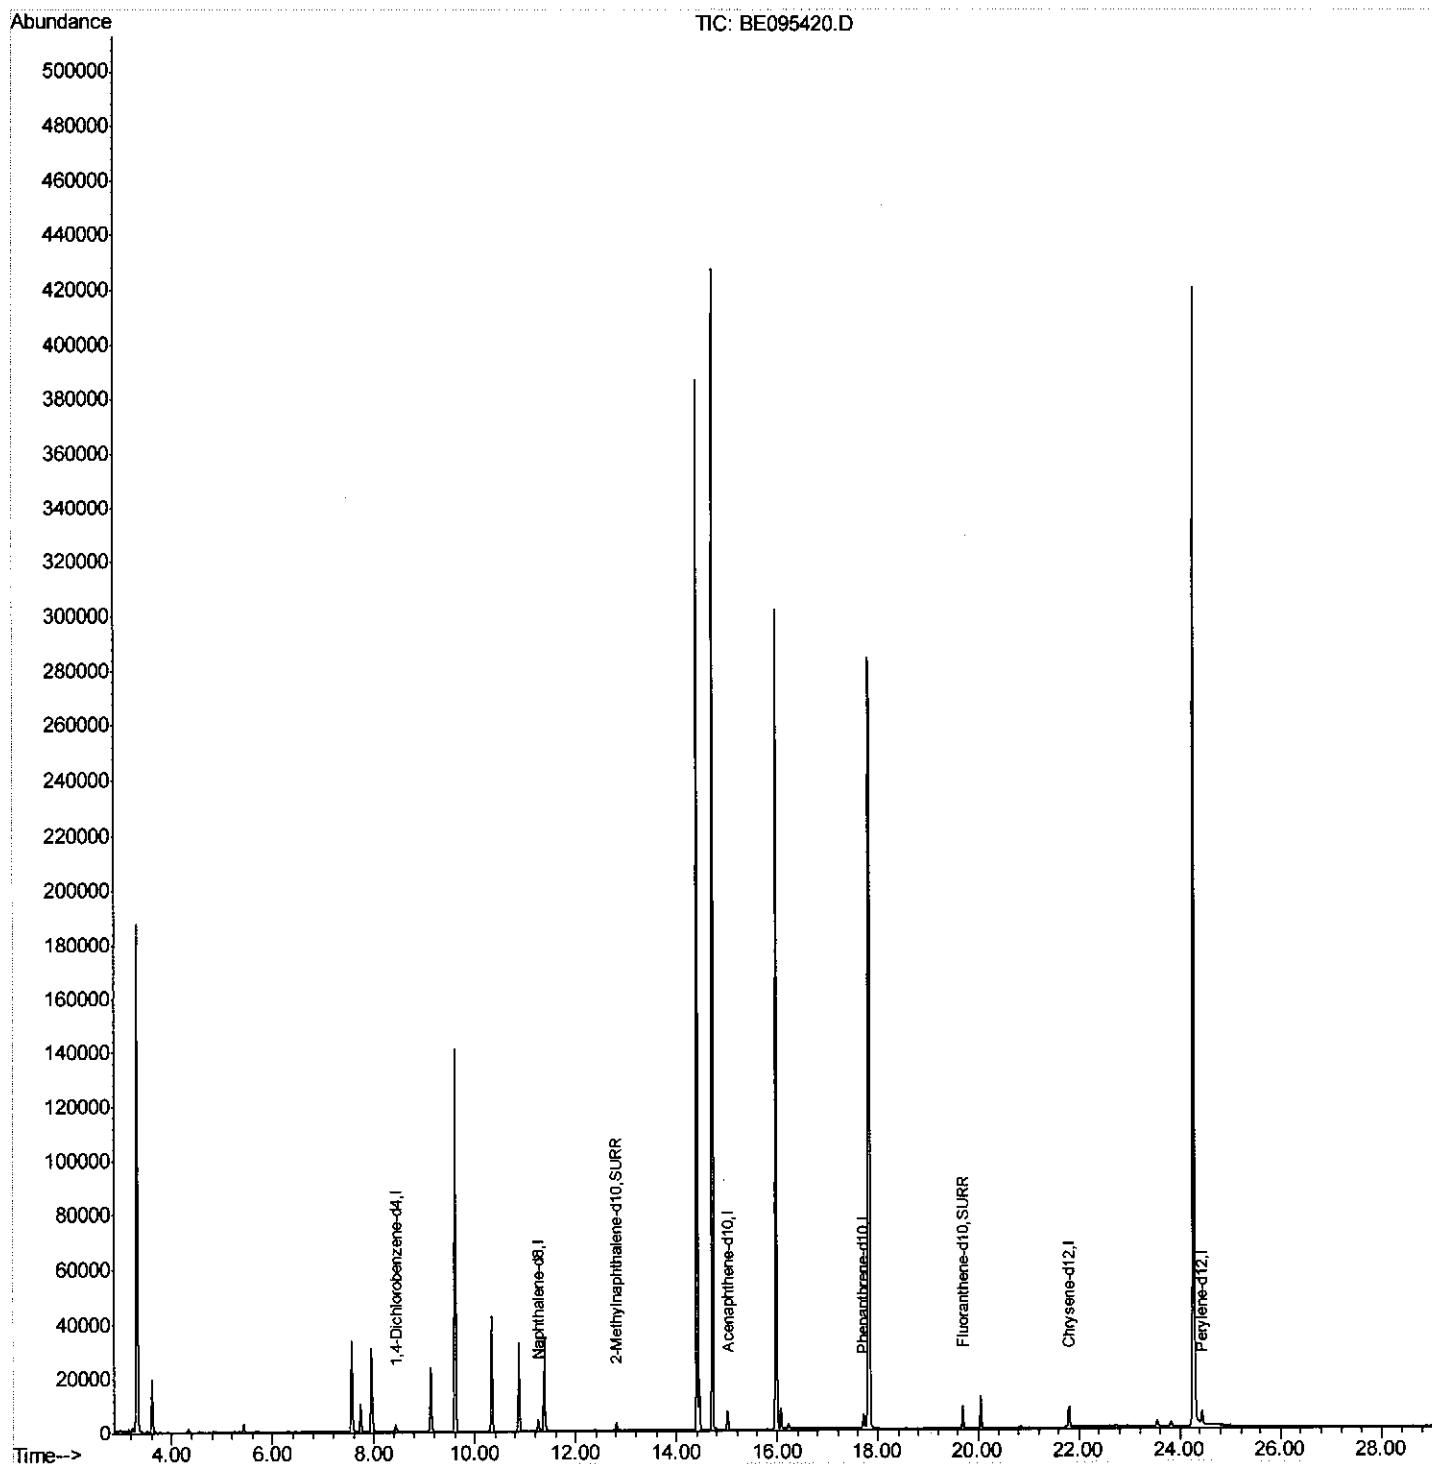

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE020218\
 Data File : BE095420.D
 Acq On : 3 Feb 2018 4:54
 Operator : SJ/JU
 Sample : J1296-07
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 F6C25

Manual Integrations
 APPROVED

Sohil
 2/5/2018 5:48:50 PM

Quant Time: Feb 03 06:06:47 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Feb 03 05:26:35 2018
 Response via : Initial Calibration

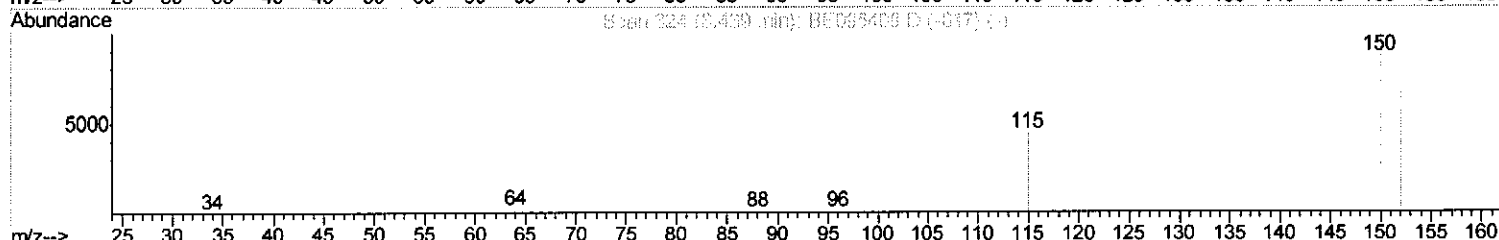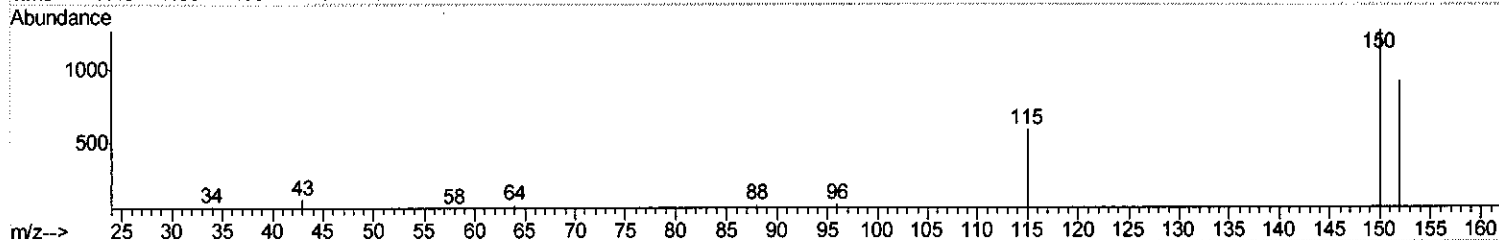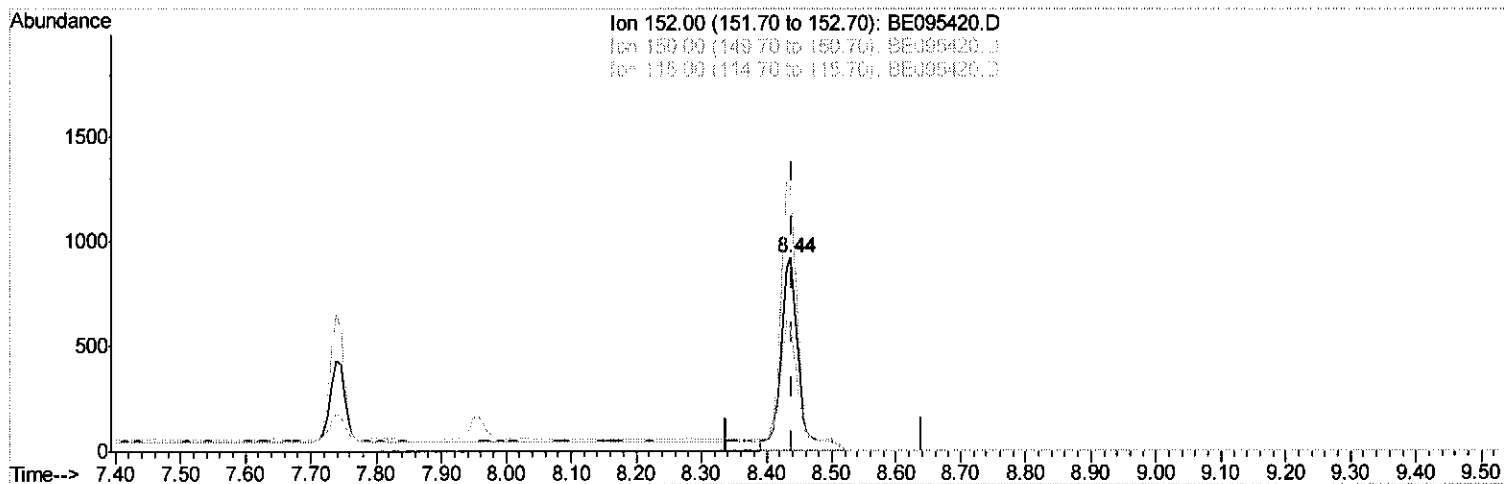

TIC: BE095420.D

(1) 1,4-Dichlorobenzene-d4 (I)

8.437min (-0.002) 0.40ng/ul

response 1969

Ion	Exp%	Act%
152.00	100	100
150.00	143.40	137.61
115.00	64.90	63.26
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE020218\
 Data File : BE095420.D
 Acq On : 3 Feb 2018 4:54
 Operator : SJ/JU
 Sample : J1296-07
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 F6C25

Manual Integrations
 APPROVED

Sohil
 2/5/2018 5:48:50 PM

Quant Time: Feb 03 06:06:47 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Feb 03 05:26:35 2018
 Response via : Initial Calibration

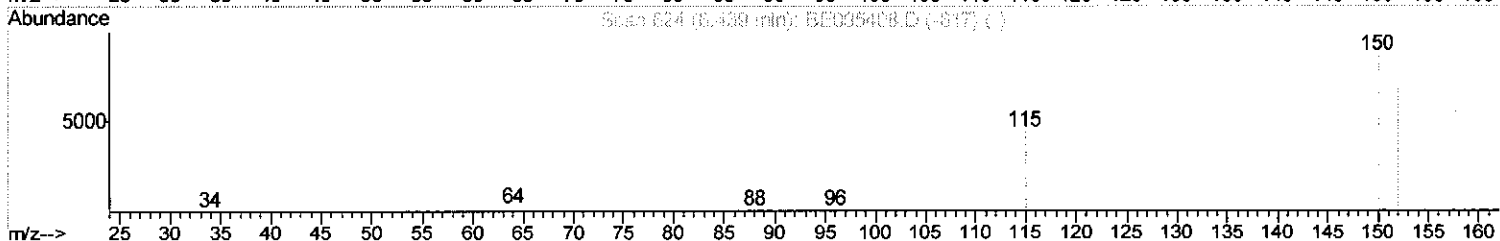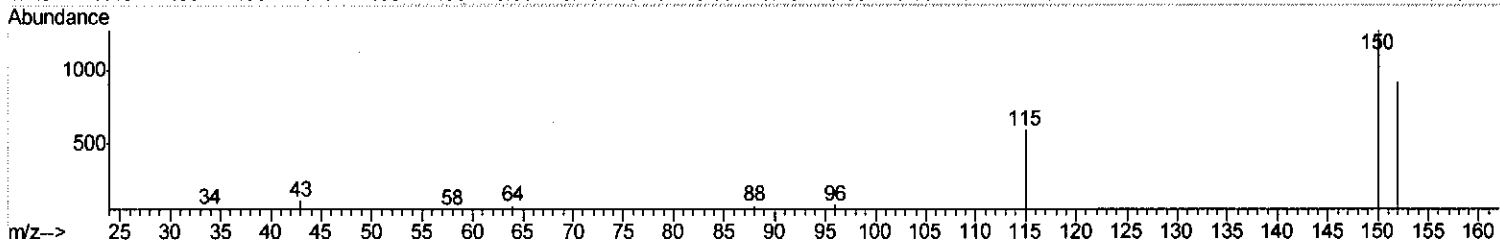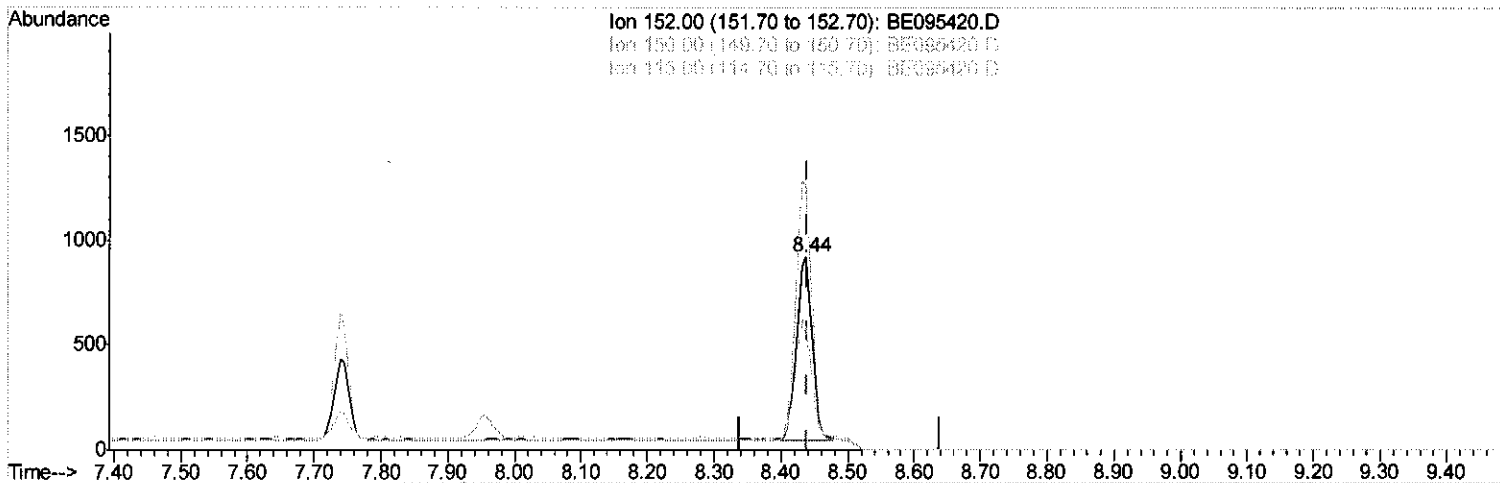

TIC: BE095420.D

(1) 1,4-Dichlorobenzene-d4 (I)

8.437min (-0.002) 0.40ng/ul m

SJ 2/7/18

response 1428

Ion	Exp%	Act%
152.00	100	100
150.00	143.40	137.61
115.00	64.90	63.26
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE020218\
 Data File : BE095420.D
 Acq On : 3 Feb 2018 4:54
 Operator : SJ/JU
 Sample : J1296-07
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 F6C25

Manual Integrations
 APPROVED

Sohil
 2/5/2018 5:48:50 PM

Quant Time: Feb 03 06:07:27 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Feb 03 05:26:35 2018
 Response via : Initial Calibration

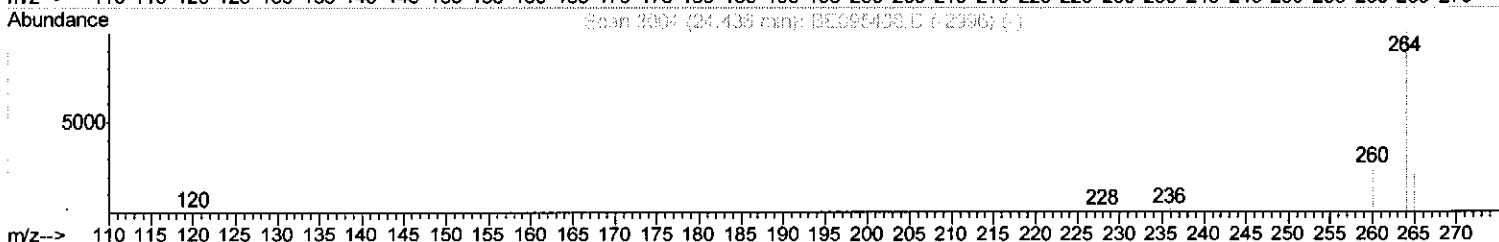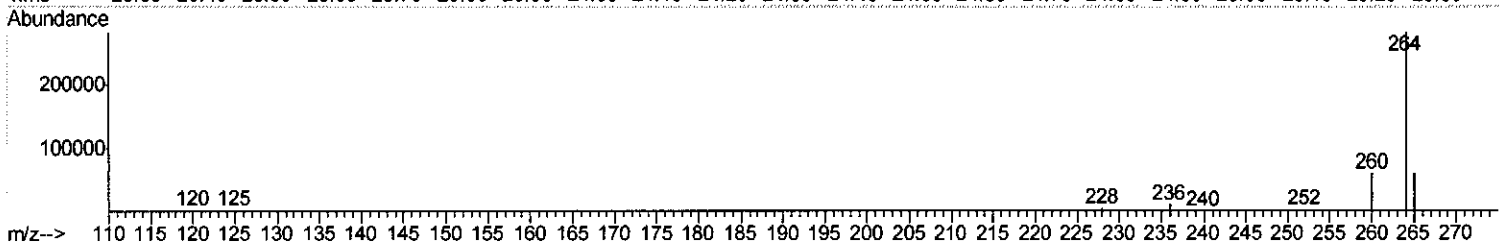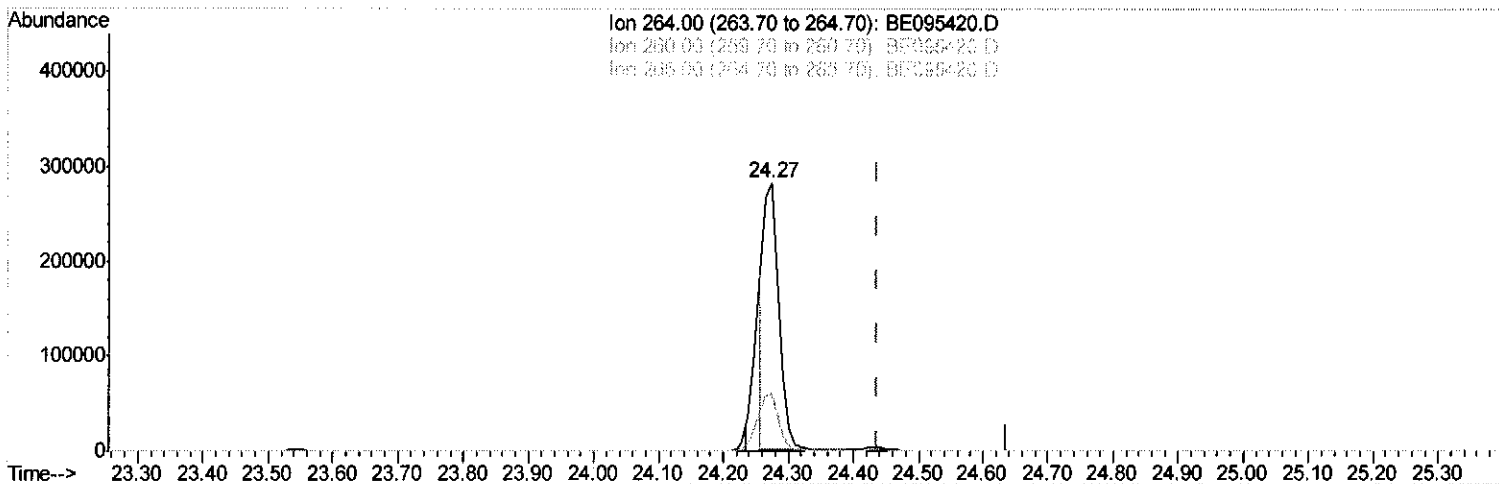

TIC: BE095420.D

(20) Perylene-d12 (I)

24.274min (-0.163) 0.40ng/ul

response 461307

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	21.15#
265.00	103.50	21.58#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE020218\
 Data File : BE095420.D
 Acq On : 3 Feb 2018 4:54
 Operator : SJ/JU
 Sample : J1296-07
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 F6C25

Manual Integrations
 APPROVED

Sohil
 2/5/2018 5:48:50 PM

Quant Time: Feb 03 06:07:27 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Feb 03 05:26:35 2018
 Response via : Initial Calibration

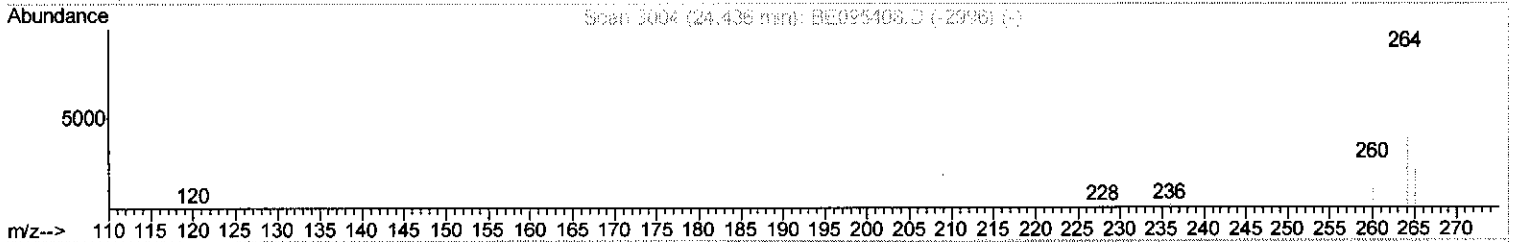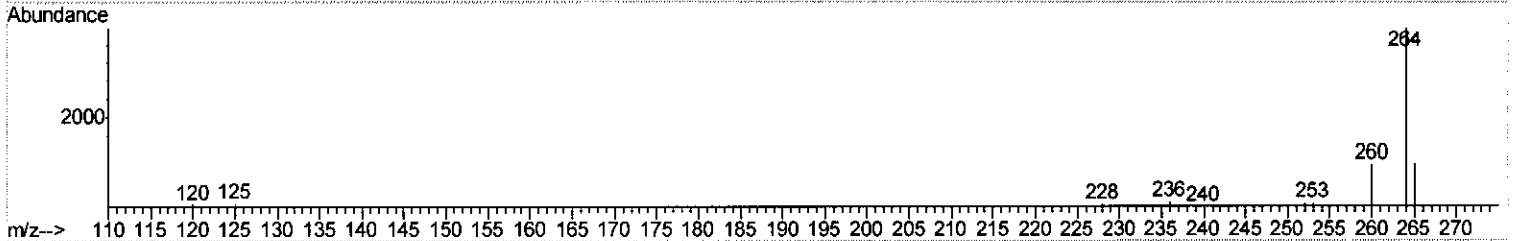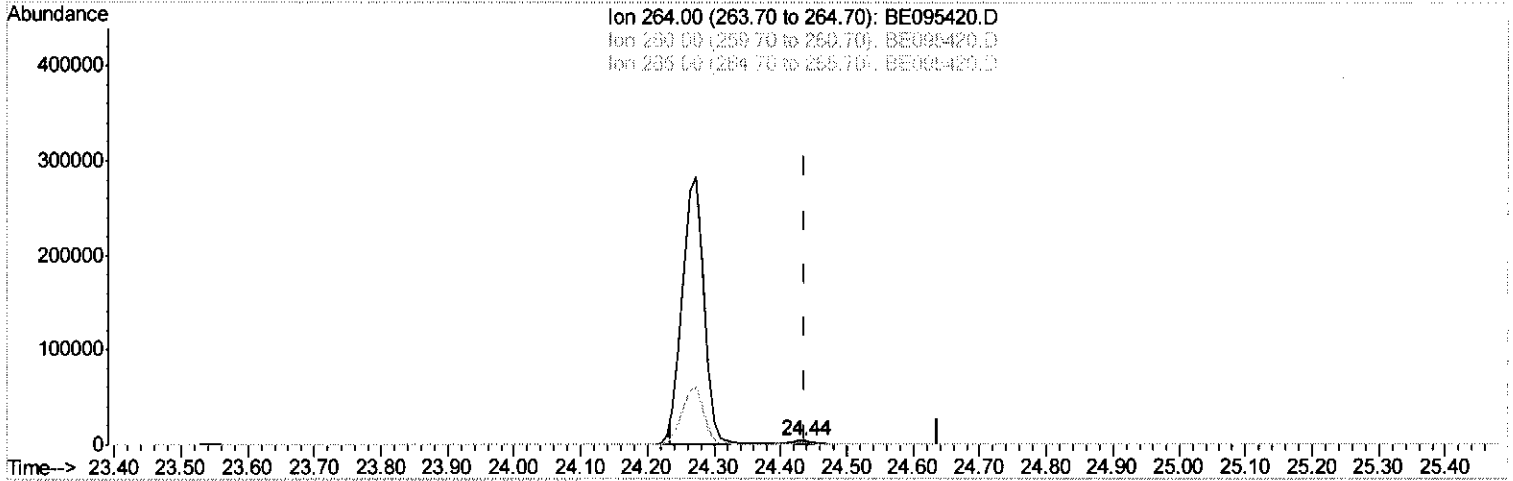

TIC: BE095420.D

(20) Perylene-d12 (I)

24.436min (-0.000) 0.40ng/ul m

SJ 2/7/18

response 7096

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	24.56
265.00	103.50	25.32#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020218\
Data File : BE095420.D
Acq On : 3 Feb 2018 4:54
Operator : SJ/JU
Sample : J1296-07
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampled :
F6C25

Manual Integrations
APPROVED

Sohil
2/5/2018 5:48:50 PM

Quant Time: Feb 03 06:08:36 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 03 05:26:35 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.44	152	1428m	0.40	ng/ul	0.00
2) Naphthalene-d8	11.26	136	5999	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.02	164	3936	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	8148	0.40	ng/ul	0.00
16) Chrysene-d12	21.80	240	8044	0.40	ng/ul	0.00
20) Perylene-d12	24.44	264	7096m	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.81	152	3693	0.38	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	9220	0.30	ng/ul	0.00

Target Compounds	Ovalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

SJ 2/7/18
SJ 2/7/18