


Data Path : Z:\HPCHEM1\BNA E\DATA\BE020218\
Data File : BE095427.D
Acq On : 3 Feb 2018 9:02
Operator : SJ/JU
Sample : J1295-19DL 2X
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F6C17DL

Manual Integrations
APPROVED

Sohil
2/5/2018 5:49:04 PM

Quant Time: Feb 05 01:55:49 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 05 01:47:56 2018
Response via : Initial Calibration

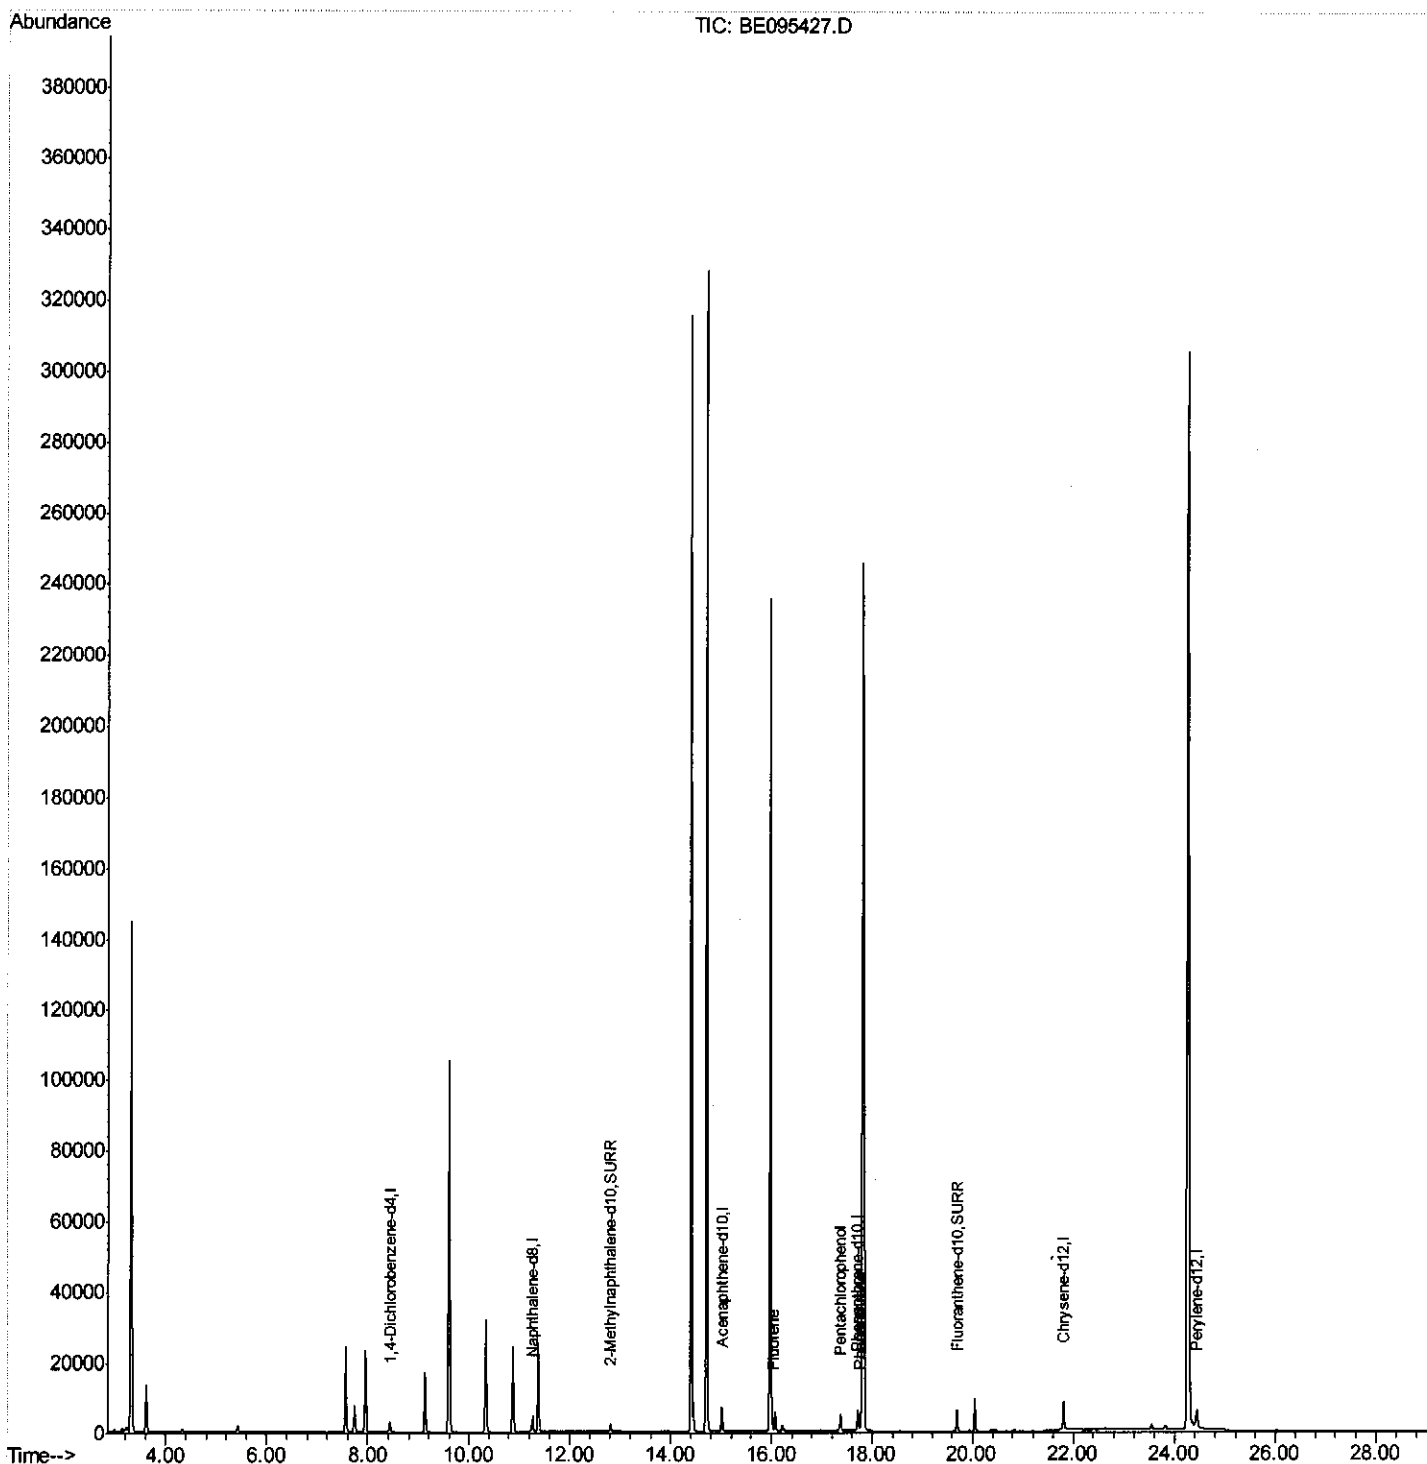

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE020218\
 Data File : BE095427.D
 Acq On : 3 Feb 2018 9:02
 Operator : SJ/JU
 Sample : J1295-19DL 2X
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 F6C17DL

Manual Integrations
 APPROVED

Sohil
 2/5/2018 5:49:04 PM

Quant Time: Feb 05 01:50:23 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 05 01:47:56 2018
 Response via : Initial Calibration

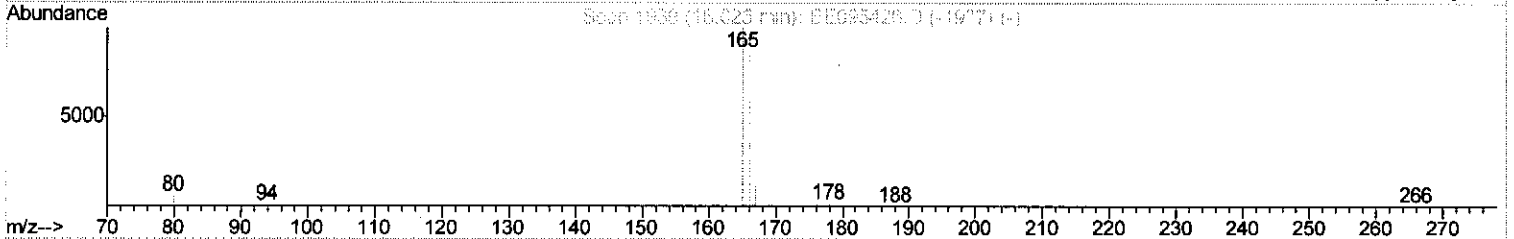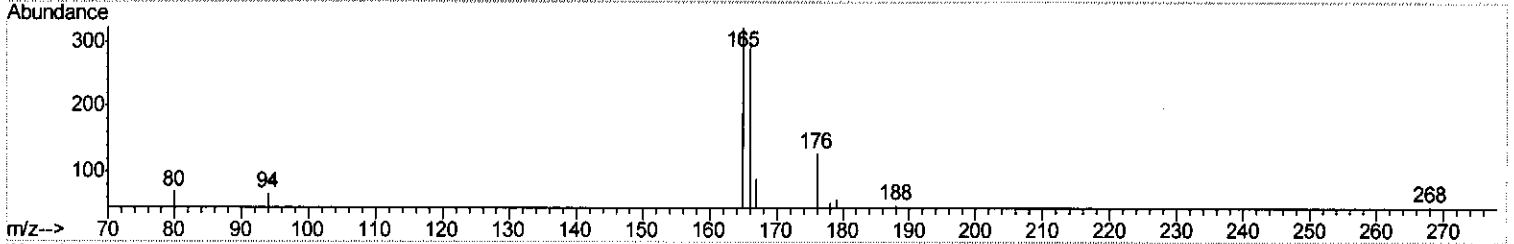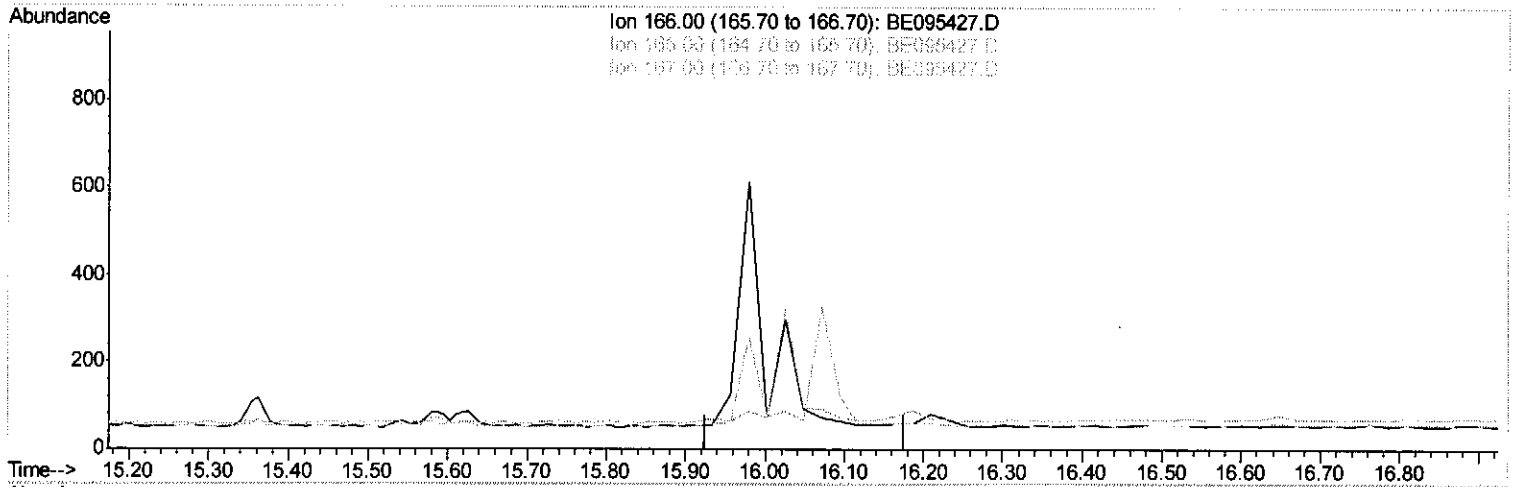

TIC: BE095427.D

(9) Fluorene

16.025min (-16.025) 0.00ng/ul

response 0

Ion	Exp%	Act%
166.00	100	0.00
165.00	91.80	0.00#
167.00	18.30	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE020218\
Data File : BE095427.D
Acq On : 3 Feb 2018 9:02
Operator : SJ/JU
Sample : J1295-19DL 2X
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F6C17DL

Manual Integrations
APPROVED

Sohil
2/5/2018 5:49:04 PM

Quant Time: Feb 05 01:50:23 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 05 01:47:56 2018
Response via : Initial Calibration

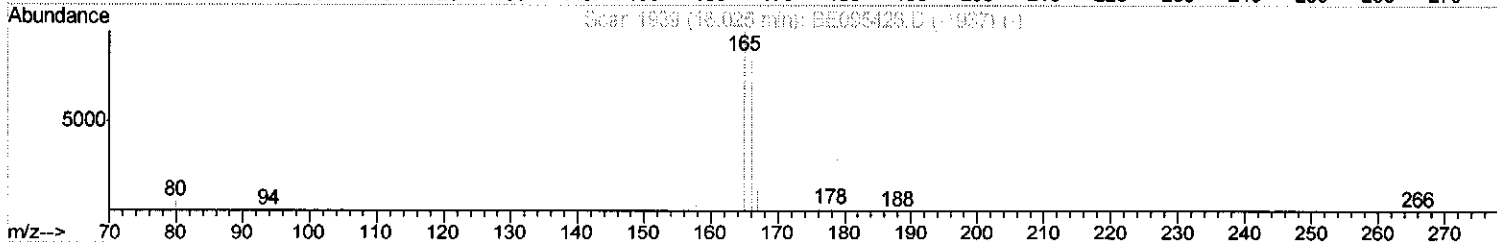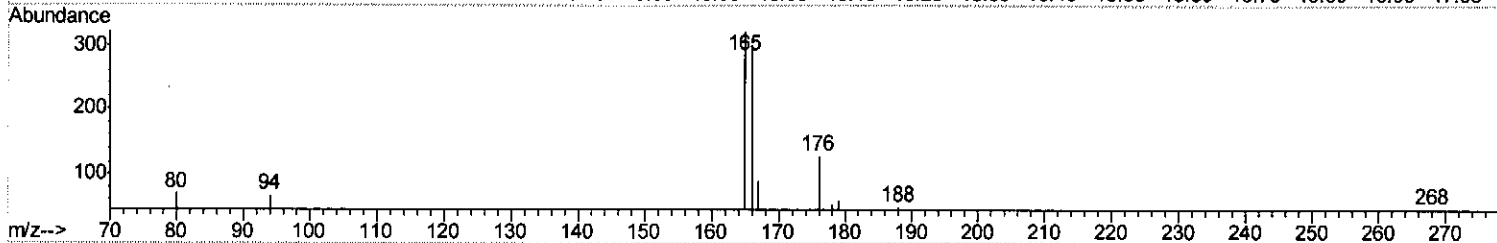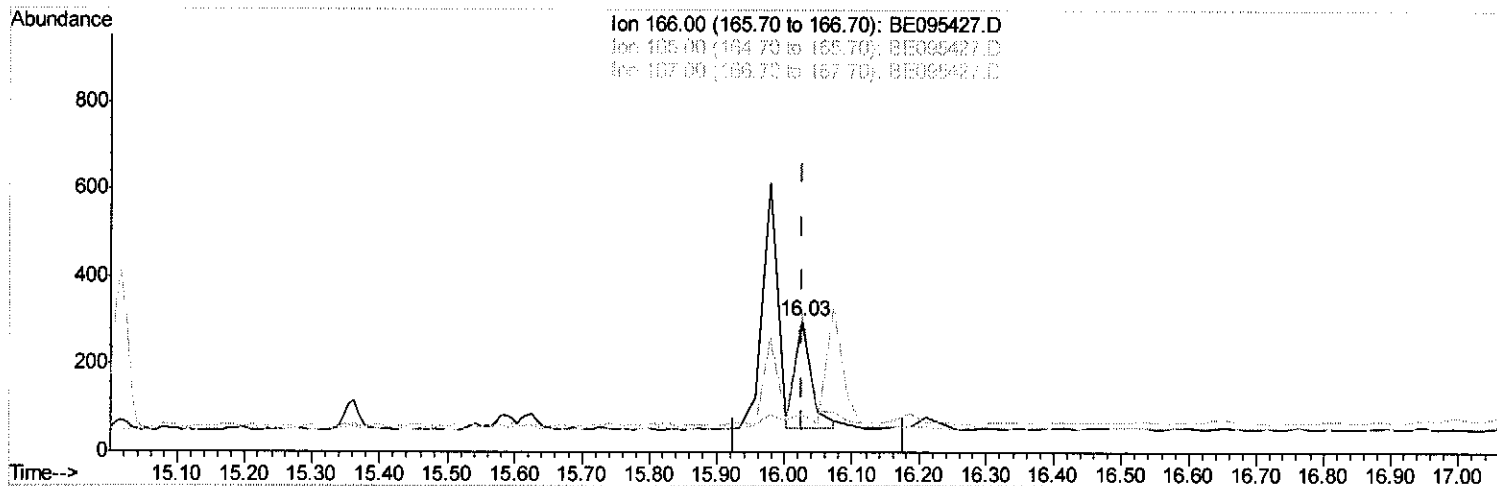

TIC: BE095427.D

(9) Fluorene

16.025min (-0.000) 0.03ng/ul m

response 408

Ion	Exp%	Act%
166.00	100	100
165.00	91.80	107.33
167.00	18.30	29.33#
0.00	0.00	0.00

SJ 2/7/18

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE020218\
 Data File : BE095427.D
 Acq On : 3 Feb 2018 9:02
 Operator : SJ/JU
 Sample : J1295-19DL 2X
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 F6C17DL

Manual Integrations
 APPROVED

Sohil
 2/5/2018 5:49:04 PM

Quant Time: Feb 05 01:52:47 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 05 01:47:56 2018
 Response via : Initial Calibration

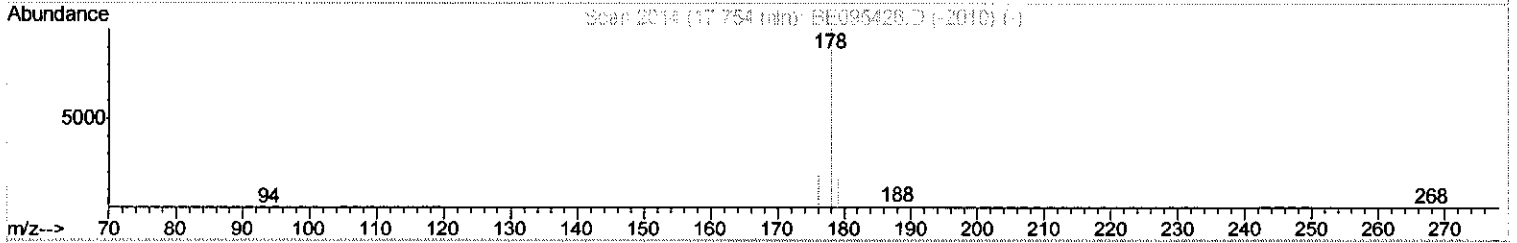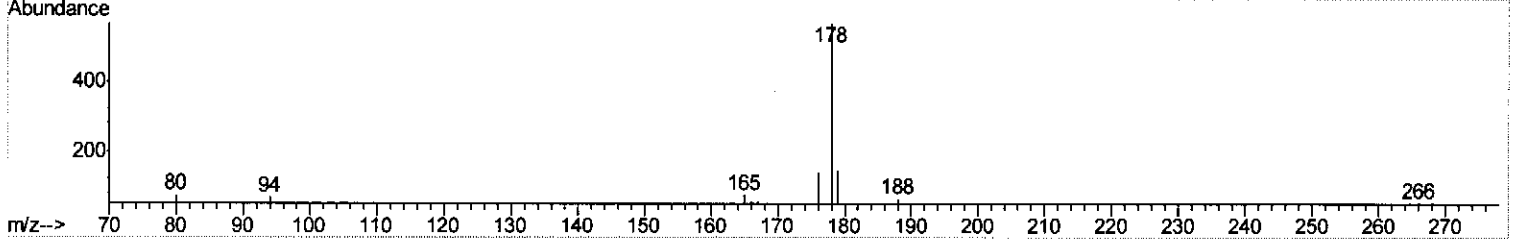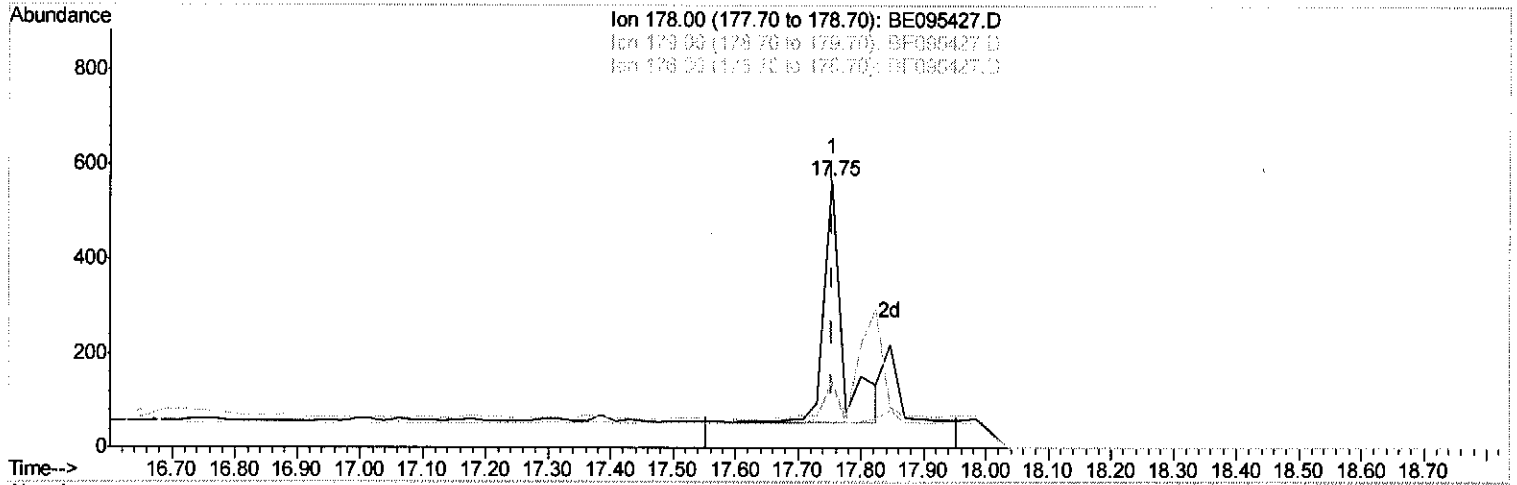

TIC: BE095427.D

(12) Phenanthrene
 17.753min (-0.000) 0.04ng/ul
 response 1077

Ion	Exp%	Act%
178.00	100	100
179.00	23.00	24.96
176.00	17.00	24.60#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA E\DATA\BE020218\
 Data File : BE095427.D
 Acq On : 3 Feb 2018 9:02
 Operator : SJ/JU
 Sample : J1295-19DL 2X
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 F6C17DL

Manual Integrations
 APPROVED

Sohil
 2/5/2018 5:49:04 PM

Quant Time: Feb 05 01:52:47 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 05 01:47:56 2018
 Response via : Initial Calibration

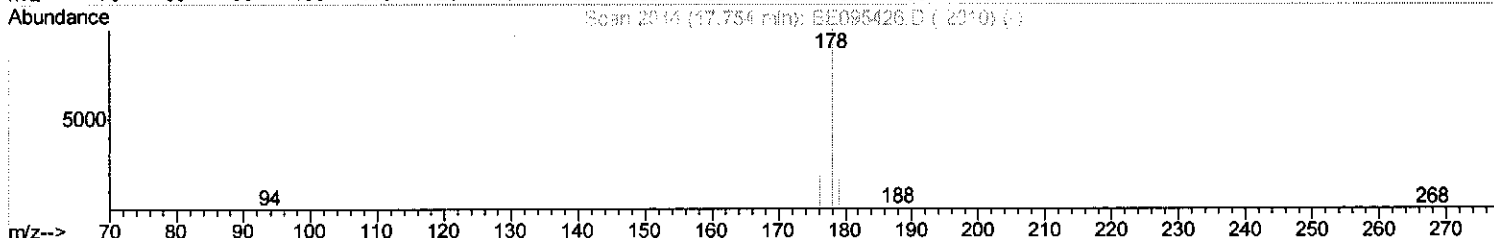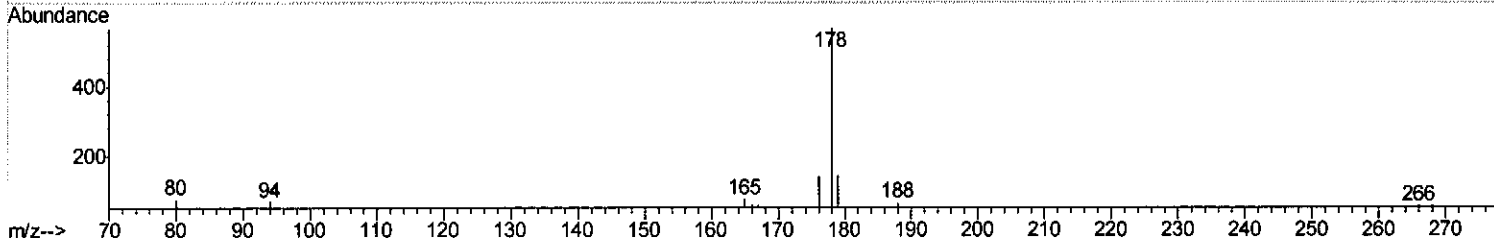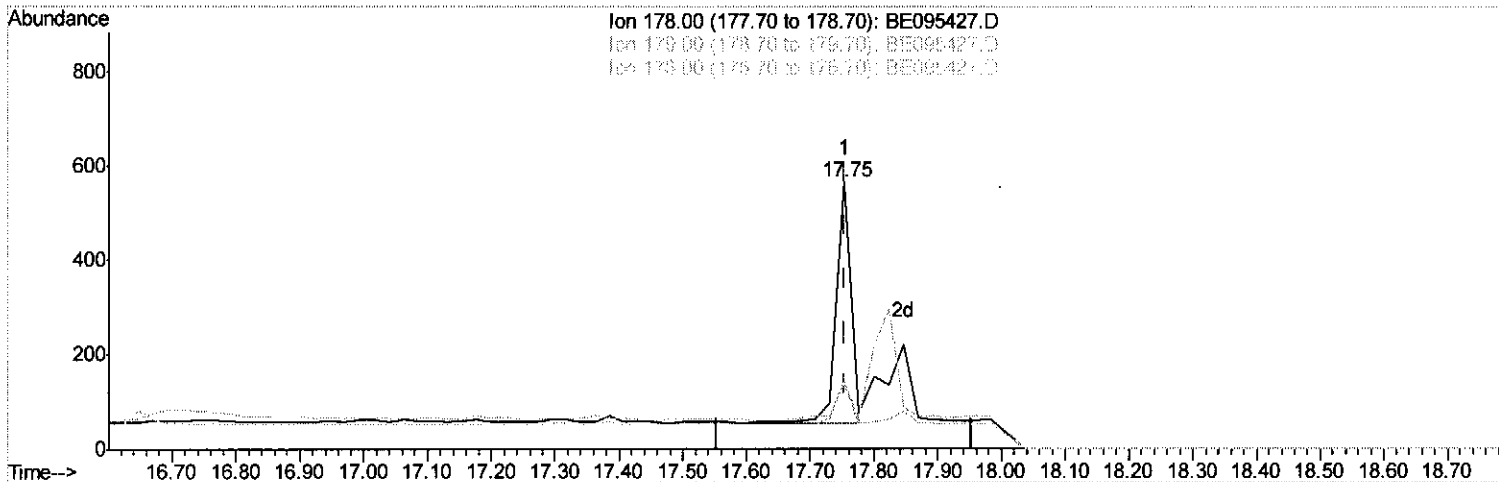

TIC: BE095427.D

(12) Phenanthrene

17.753min (-0.000) 0.03ng/ul m

SJ 2/2/18

response 831

Ion	Exp%	Act%
178.00	100	100
179.00	23.00	24.96
176.00	17.00	24.60#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020218\
Data File : BE095427.D
Acq On : 3 Feb 2018 9:02
Operator : SJ/JU
Sample : J1295-19DL 2X
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_E
Client Sample ID :
F6C17DL

Manual Integrations
APPROVED

Sohil
2/5/2018 5:49:04 PM

Quant Time: Feb 05 01:55:49 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 05 01:47:56 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.44	152	2064	0.40	ng/ul	0.00
2) Naphthalene-d8	11.26	136	6277	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.02	164	3949	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	8511	0.40	ng/ul	0.00
16) Chrysene-d12	21.80	240	8157	0.40	ng/ul	0.00
20) Perylene-d12	24.44	264	9602	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.81	152	2765	0.27	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	6722	0.21	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)	Ovalue
9) Fluorene	16.03	166	408m	0.027	ng/ul		
11) Pentachlorophenol	17.36	266	3133	1.901	ng/ul		98
12) Phenanthrene	17.75	178	831m	0.029	ng/ul		

(#) = qualifier out of range (m) = manual integration (+) = signals summed

SJ 2/7/18
SJ 2/7/18