

Data Path : U:\HPCHEM1\BNA E\DATA\BE020218\
 Data File : BE095410.D
 Acq On : 2 Feb 2018 22:58
 Operator : SJ/JU
 Sample : J1296-11
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 F6A78

Manual Integrations
 APPROVED

Sohil
 2/5/2018 5:48:24 PM

Quant Time: Feb 03 05:35:46 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Feb 03 05:26:35 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.44	152	1479m	0.40	ng/ul	0.00
2) Naphthalene-d8	11.26	136	6040	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.02	164	4084	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	7891m	0.40	ng/ul	0.00
16) Chrysene-d12	21.80	240	8138	0.40	ng/ul	0.00
20) Perylene-d12	24.44	264	7043m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	4181	0.43	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	10687	0.35	ng/ul	0.00
Target Compounds						
3) Naphthalene	11.31	128	436	0.026	ng/ul#	56
8) Acenaphthene	15.07	153	1576	0.103	ng/ul#	26

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : U:\HPCHEM1\BNA E\DATA\BE020218\
Data File : BE095410.D
Acq On : 2 Feb 2018 22:58
Operator : SJ/JU
Sample : J1296-11
Misc :
ALS Vial : 18 Sample Multiplier: 1


Instrument :
BNA_E
ClientSampleId :
F6A78

Manual Integrations
APPROVED

Sohil
2/5/2018 5:48:24 PM

Quant Time: Feb 03 05:35:46 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 03 05:26:35 2018
Response via : Initial Calibration

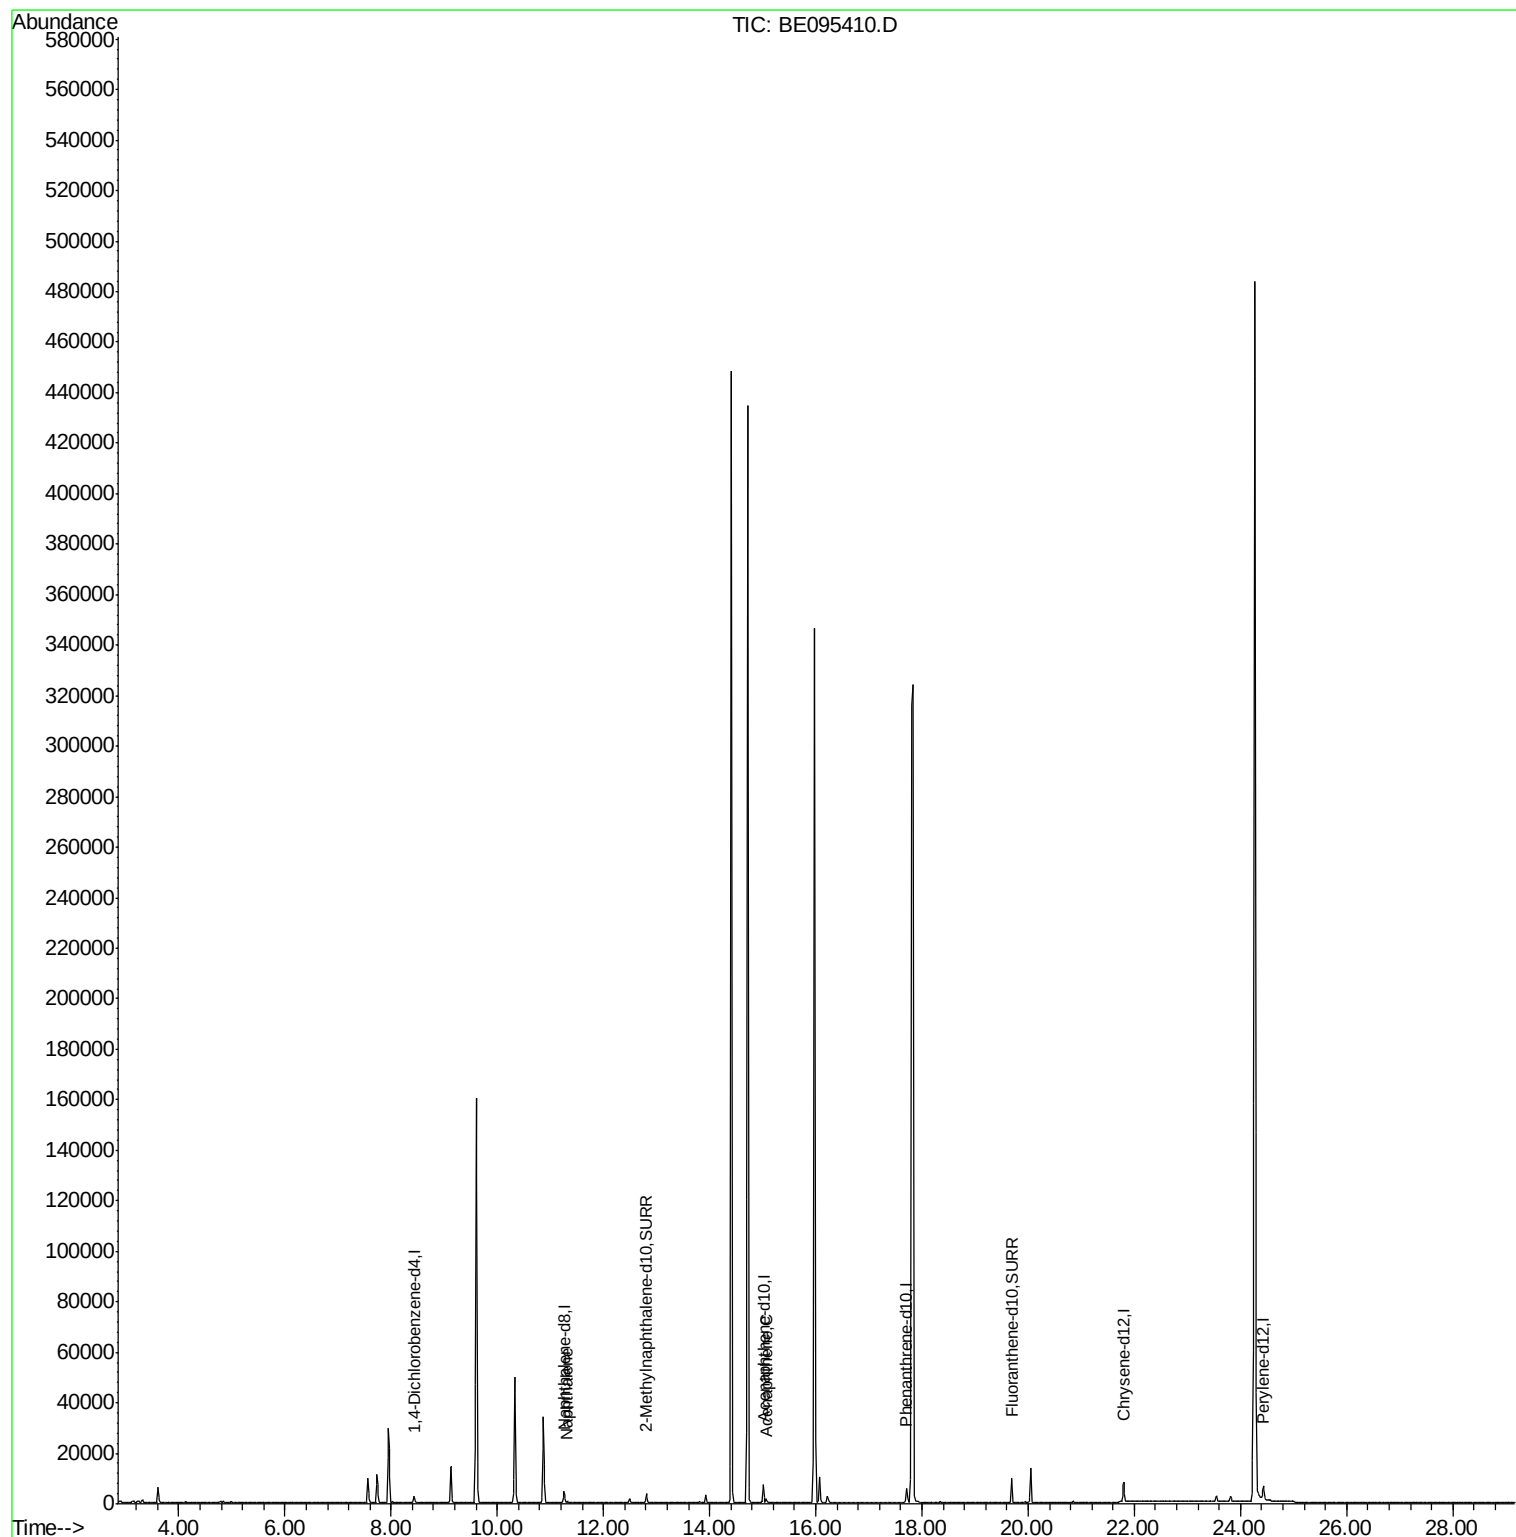

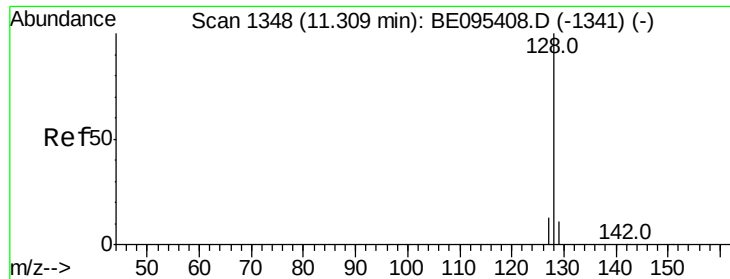

#3

Naphthalene

Concen: 0.026 ng/ul

RT: 11.31 min Scan# 1348

Delta R.T. -0.00 min

Lab File: BE095410.D

Acq: 2 Feb 2018 22:58

Instrument :

BNA_E





ClientSampleId :

F6A78

Tot Ion:128	Resp:	436
Ion Ratio	Lower	Upper
128 100		
129 27.5	11.3	16.9#
127 30.2	4.0	6.0#

Manual Integrations
APPROVED

Sohil
2/5/2018 5:48:24 PM

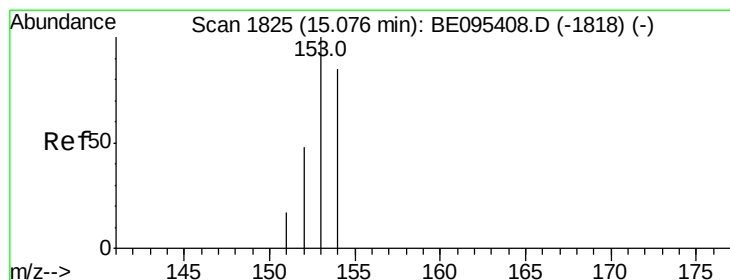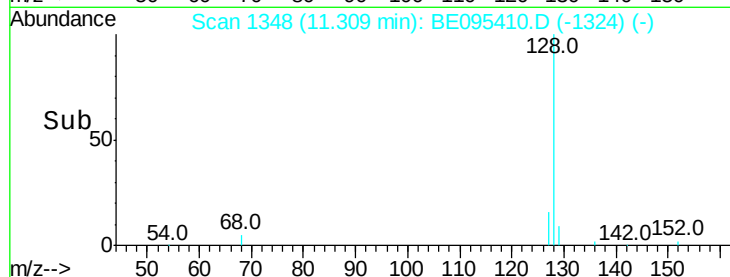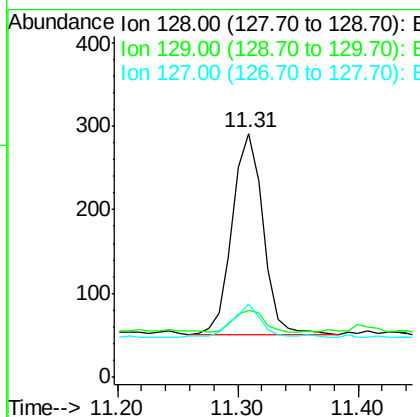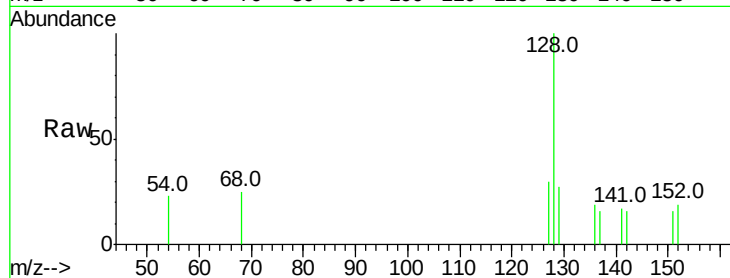

#8

Acenaphthene

Concen: 0.103 ng/ul

RT: 15.07 min Scan# 1824

Delta R.T. -0.01 min

Lab File: BE095410.D

Acq: 2 Feb 2018 22:58

Tgt Ion:153	Resp:	1576
Ion Ratio	Lower	Upper
153 100		
152 5.6	36.0	54.0#
154 13.4	72.0	108.0#

