

Data Path : U:\HPCHEM1\BNA E\DATA\BE020218\
 Data File : BE095413.D
 Acq On : 3 Feb 2018 00:43
 Operator : SJ/JU
 Sample : J1296-16
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 F6C33

Manual Integrations
 APPROVED

Sohil
 2/5/2018 5:48:32 PM

Quant Time: Feb 03 05:44:16 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Feb 03 05:26:35 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.44	152	1574m	0.40	ng/ul	0.00
2) Naphthalene-d8	11.26	136	6746	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.02	164	4332	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	8894	0.40	ng/ul	0.00
16) Chrysene-d12	21.80	240	8709	0.40	ng/ul	0.00
20) Perylene-d12	24.44	264	7726m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	3939	0.36	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	10284	0.30	ng/ul	0.00
Target Compounds						
11) Pentachlorophenol	17.36	266	97	0.056	ng/ul	Ovalue 98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : U:\HPCHEM1\BNA E\DATA\BE020218\
Data File : BE095413.D
Acq On : 3 Feb 2018 00:43
Operator : SJ/JU
Sample : J1296-16
Misc :
ALS Vial : 21 Sample Multiplier: 1


Instrument :
BNA_E
ClientSampleId :
F6C33

Manual Integrations
APPROVED

Sohil
2/5/2018 5:48:32 PM

Quant Time: Feb 03 05:44:16 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 03 05:26:35 2018
Response via : Initial Calibration

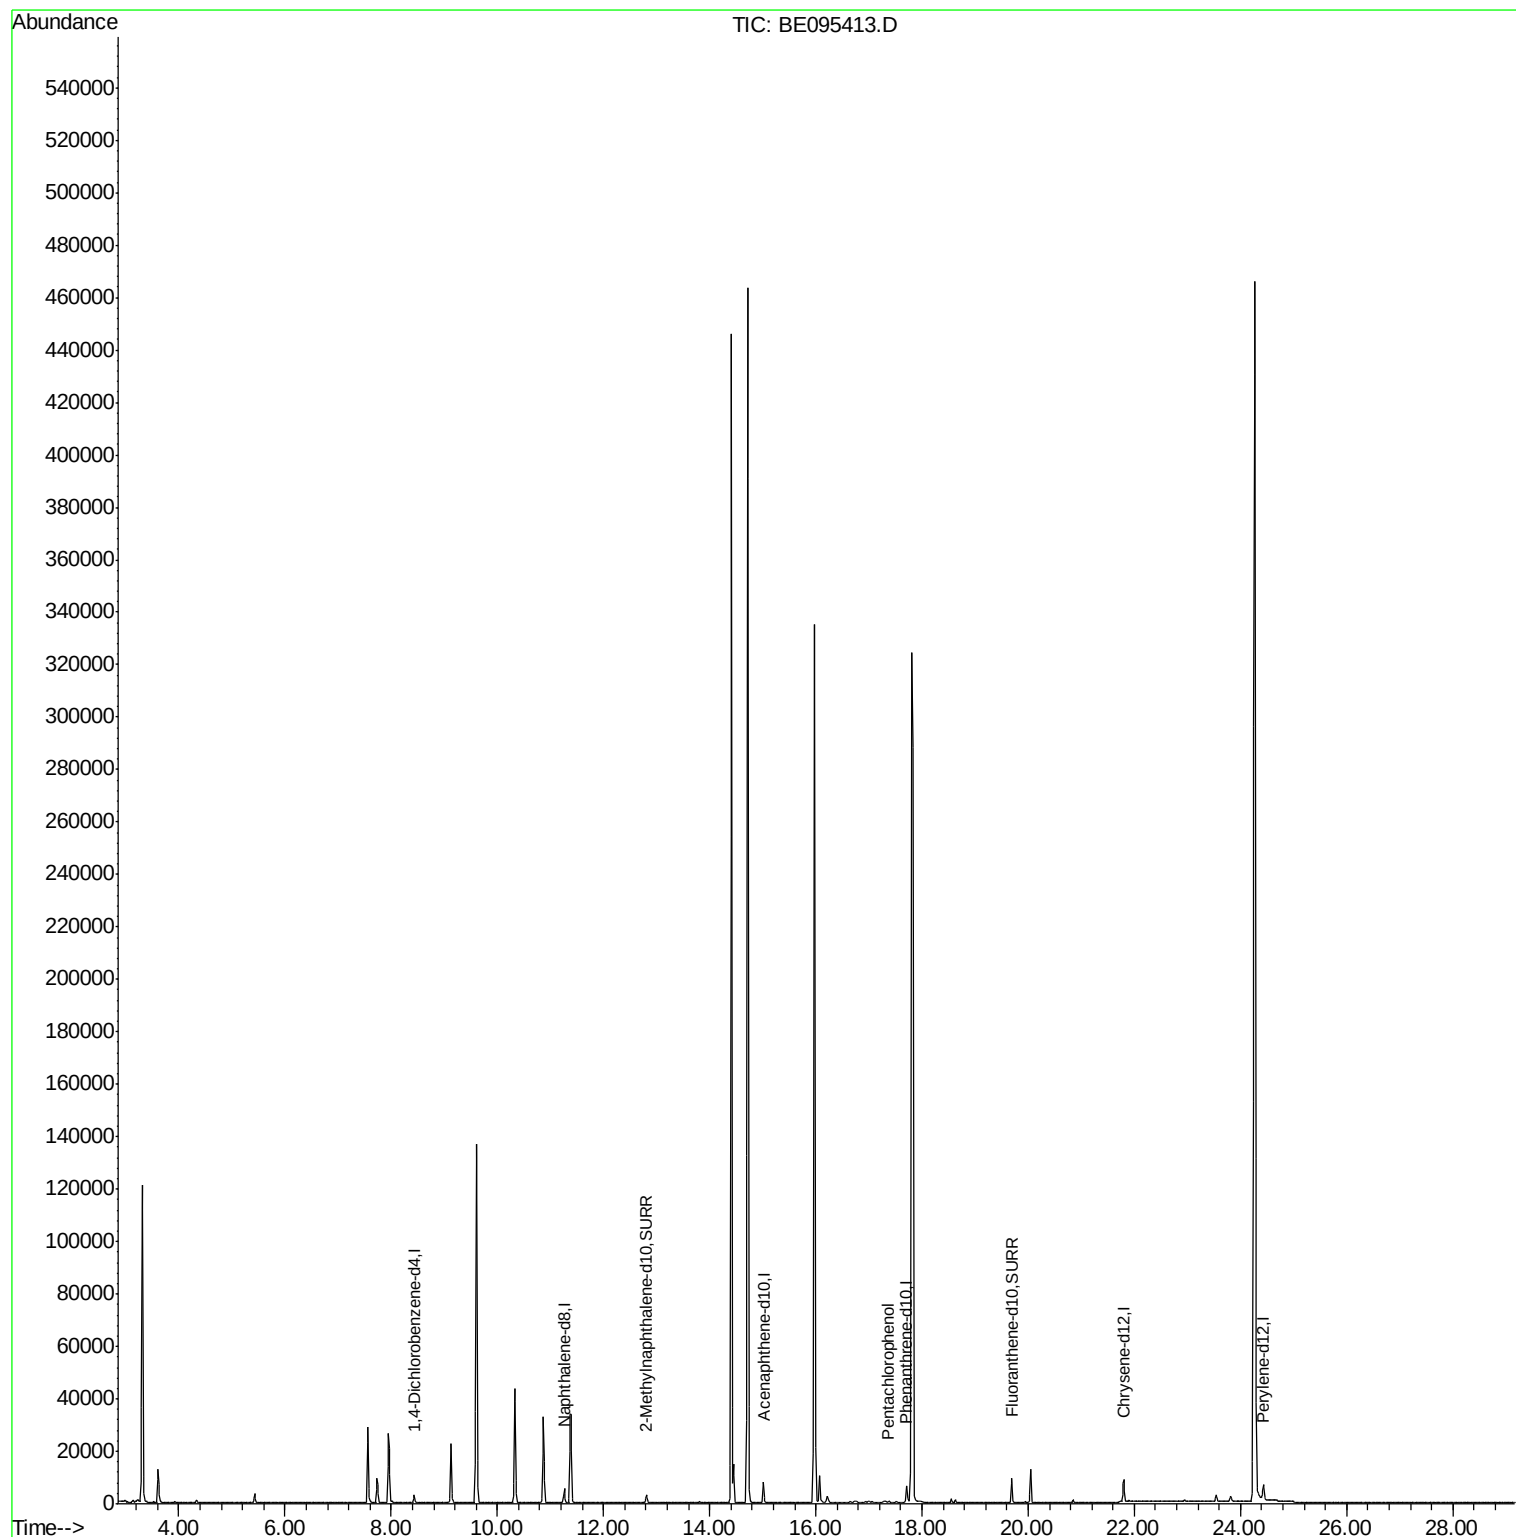

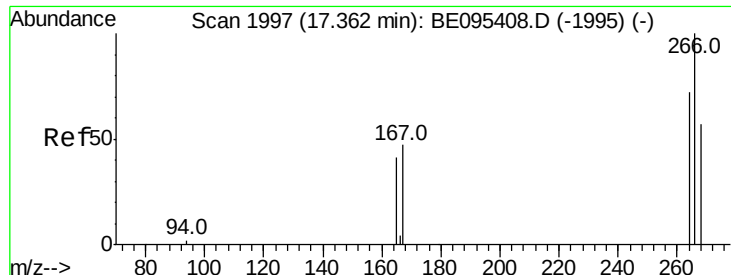


#11
 Pentachlorophenol
 Concen: 0.056 ng/ul
 RT: 17.36 min Scan# 1997
 Delta R.T. 0.00 min
 Lab File: BE095413.D
 Acq: 3 Feb 2018 00:43

Instrument :
 BNA_E
 ClientSampleId :
 F6C33

Tot Ion:	266	Resp:	97
Ion Ratio	Lower	Upper	
266	100		
264	59.8	47.9	71.9
268	59.8	49.8	74.8

Manual Integrations
 APPROVED

Sohil
 2/5/2018 5:48:32 PM

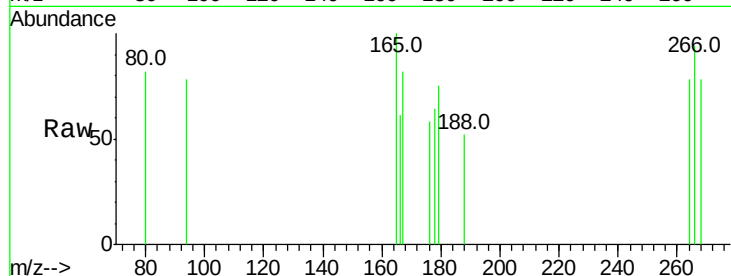

Abundance Ion 266.00 (265.70 to 266.70): E
 Ion 264.00 (263.70 to 264.70): E
 Ion 268.00 (267.70 to 268.70): E

