

Data Path : U:\HPCHEM1\BNA E\DATA\BE020218\
 Data File : BE095417.D
 Acq On : 3 Feb 2018 3:06
 Operator : SJ/JU
 Sample : J1296-03
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 F6C21

Manual Integrations
 APPROVED

Sohil
 2/5/2018 5:48:43 PM

Quant Time: Feb 03 05:52:16 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Feb 03 05:26:35 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.44	152	1378m	0.40	ng/ul	0.00
2) Naphthalene-d8	11.26	136	5752	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.02	164	3774	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	7928	0.40	ng/ul	0.00
16) Chrysene-d12	21.80	240	7600	0.40	ng/ul	0.00
20) Perylene-d12	24.44	264	6648m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	3361	0.36	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	7924	0.26	ng/ul	0.00
Target Compounds						
3) Naphthalene	11.31	128	5120	0.318	ng/ul#	90
11) Pentachlorophenol	17.36	266	12522	8.155	ng/ul	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : U:\HPCHEM1\BNA E\DATA\BE020218\
Data File : BE095417.D
Acq On : 3 Feb 2018 3:06
Operator : SJ/JU
Sample : J1296-03
Misc :
ALS Vial : 25 Sample Multiplier: 1


Instrument :
BNA_E
ClientSampleId :
F6C21

Manual Integrations
APPROVED

Sohil
2/5/2018 5:48:43 PM

Quant Time: Feb 03 05:52:16 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 03 05:26:35 2018
Response via : Initial Calibration

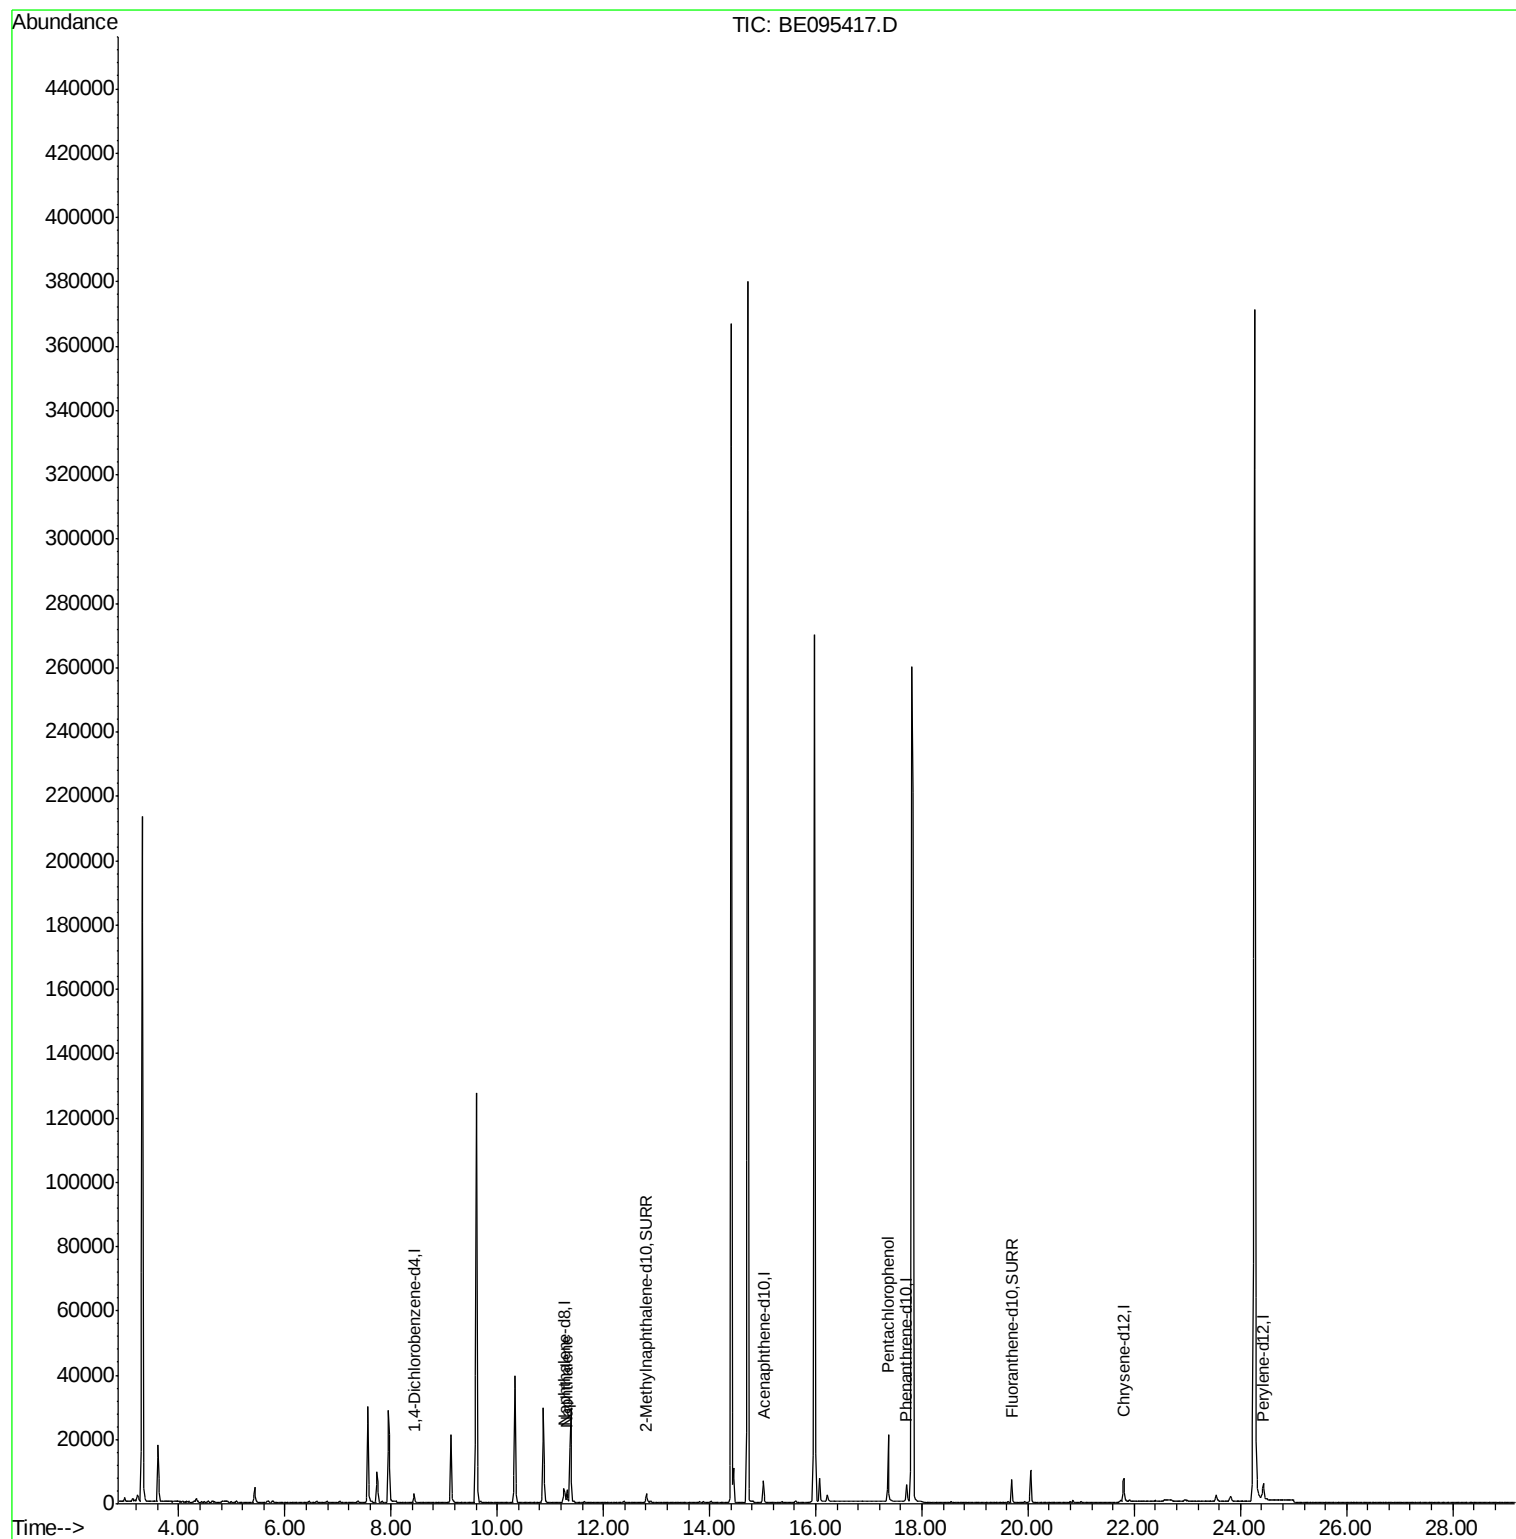

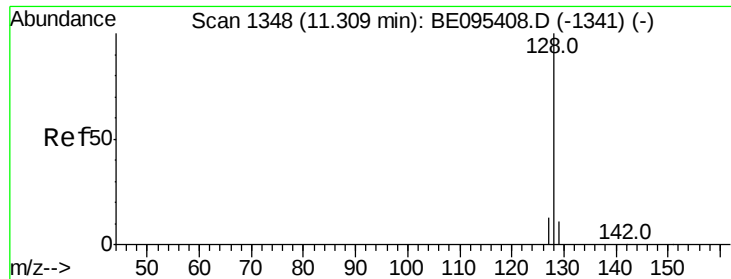

#3

Naphthalene

Concen: 0.318 ng/ul

RT: 11.31 min Scan# 1348

Delta R.T. -0.00 min

Lab File: BE095417.D

Acq: 3 Feb 2018 3:06

Instrument :

BNA_E





ClientSampleId :

F6C21

Tot Ion:	128	Resp:	5120
Ion Ratio	Lower	Upper	
128	100		
129	12.8	11.3	16.9
127	14.3	4.0	6.0#

Manual Integrations
APPROVED

Sohil
2/5/2018 5:48:43 PM

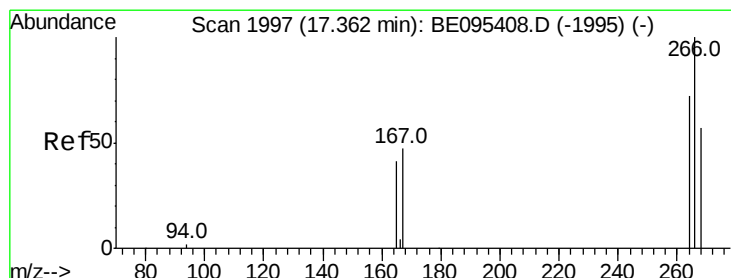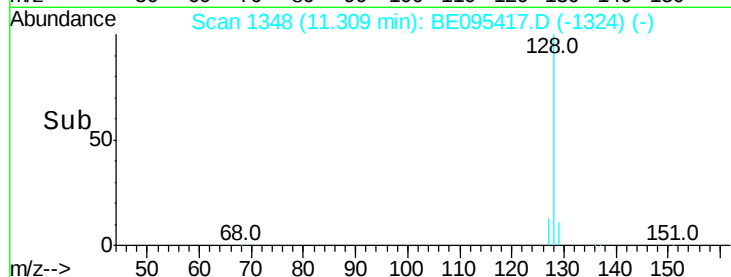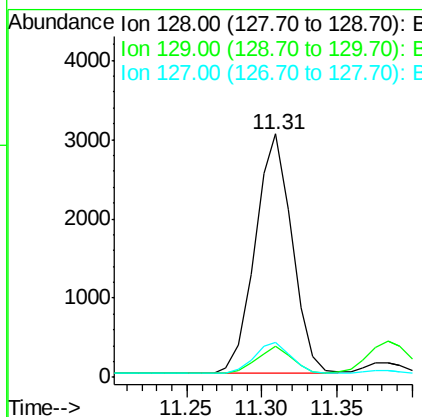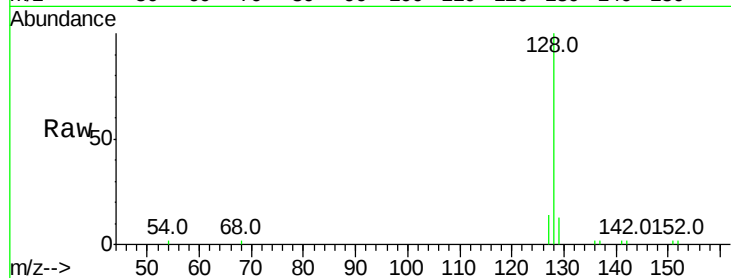

#11

Pentachlorophenol

Concen: 8.155 ng/ul

RT: 17.36 min Scan# 1997

Delta R.T. -0.00 min

Lab File: BE095417.D

Acq: 3 Feb 2018 3:06

Tgt Ion:	266	Resp:	12522
Ion Ratio	Lower	Upper	
266	100		
264	63.9	47.9	71.9
268	61.6	49.8	74.8

