

Data Path : U:\HPCHEM1\BNA E\DATA\BE020218\
 Data File : BE095425.D
 Acq On : 3 Feb 2018 7:50
 Operator : SJ/JU
 Sample : J1295-18DL 2X
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 F6C16DL

Quant Time: Feb 05 01:39:53 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Feb 03 05:26:35 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.44	152	1946	0.40	ng/ul	0.00
2) Naphthalene-d8	11.26	136	5660	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.02	164	3599	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	7839	0.40	ng/ul	0.00
16) Chrysene-d12	21.81	240	7754	0.40	ng/ul	0.00
20) Perylene-d12	24.43	264	8860	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	1972	0.21	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	5081	0.17	ng/ul	0.00
Target Compounds						
11) Pentachlorophenol	17.36	266	3047	2.007	ng/ul	Ovalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : U:\HPCHEM1\BNA E\DATA\BE020218\
Data File : BE095425.D
Acq On : 3 Feb 2018 7:50
Operator : SJ/JU
Sample : J1295-18DL 2X
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F6C16DL

Quant Time: Feb 05 01:39:53 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 03 05:26:35 2018
Response via : Initial Calibration

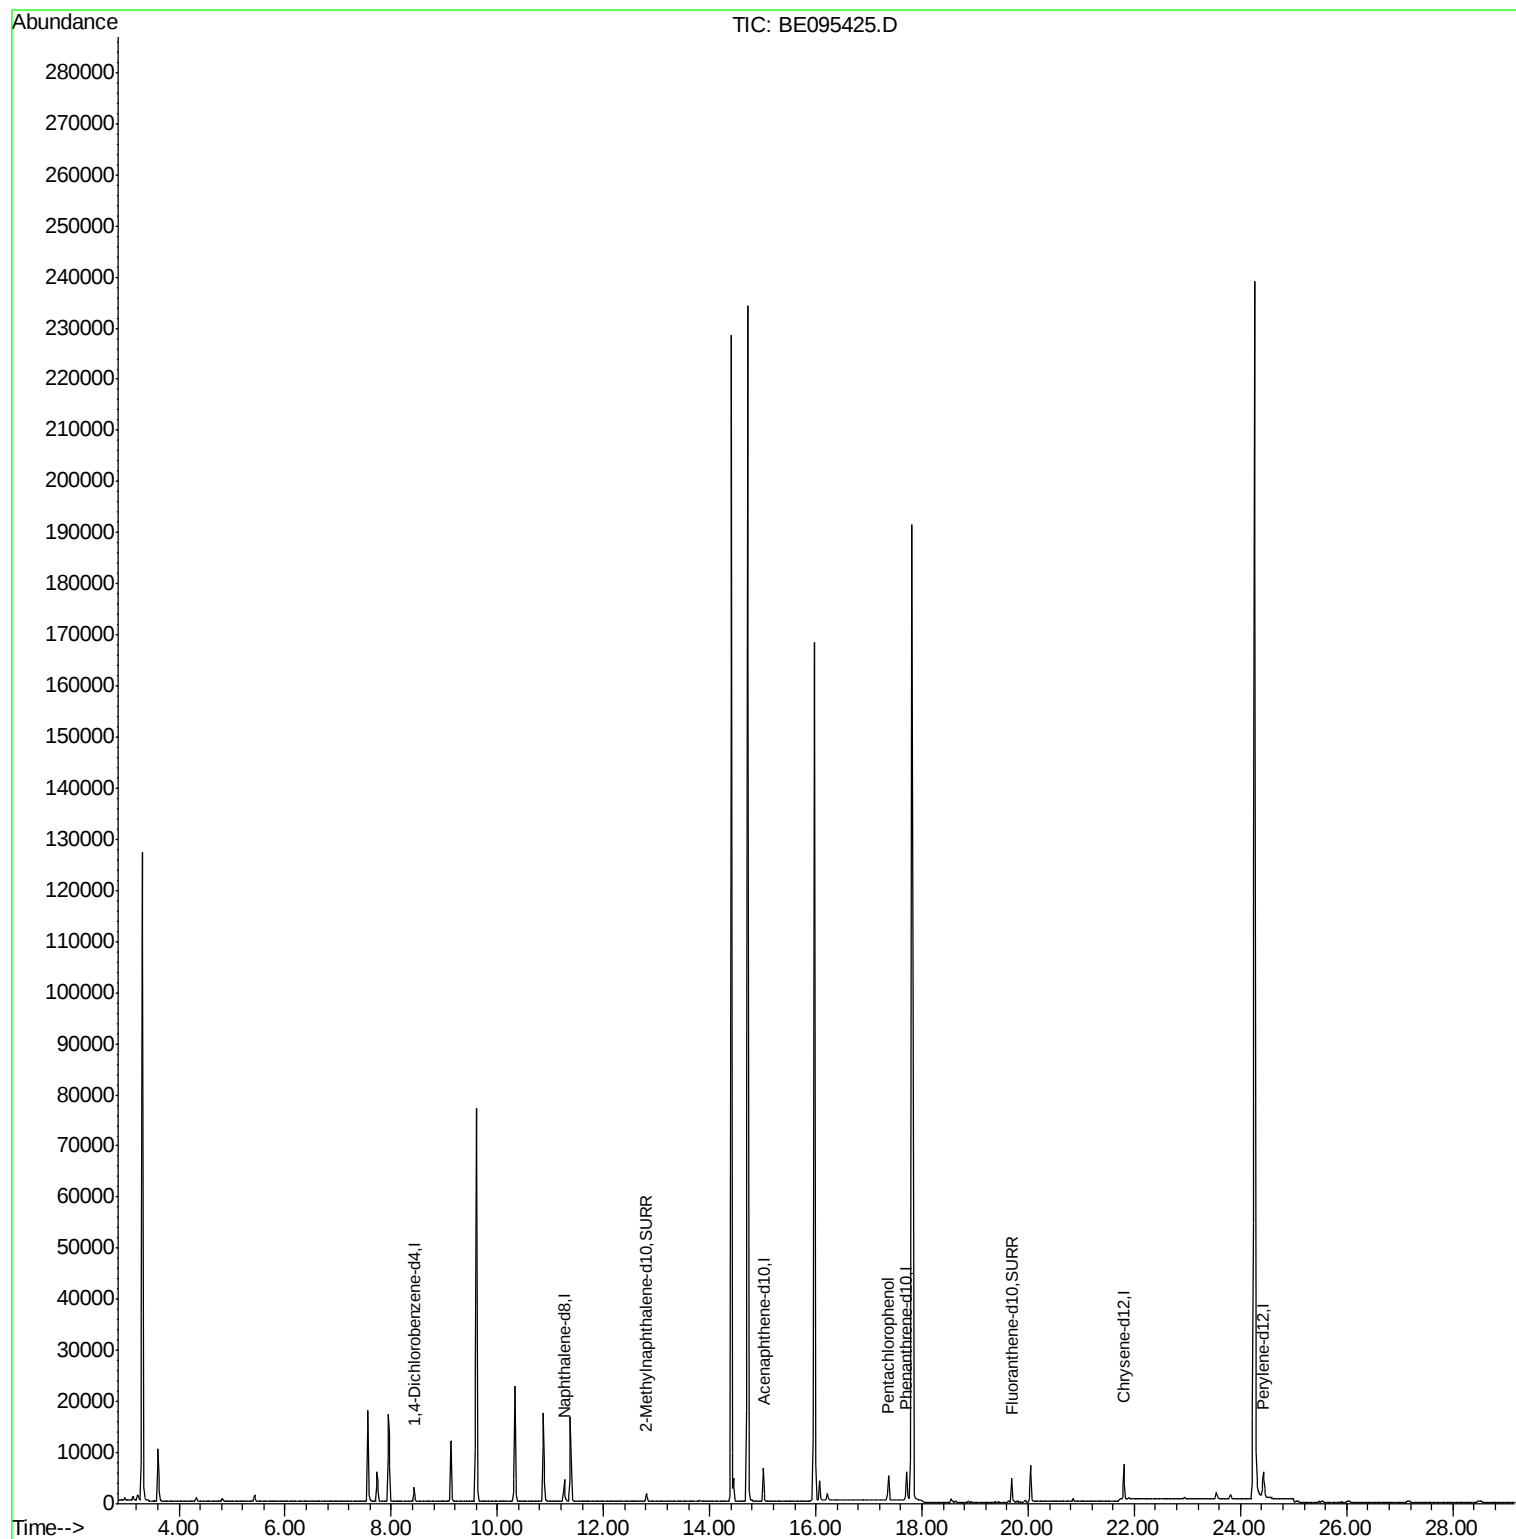


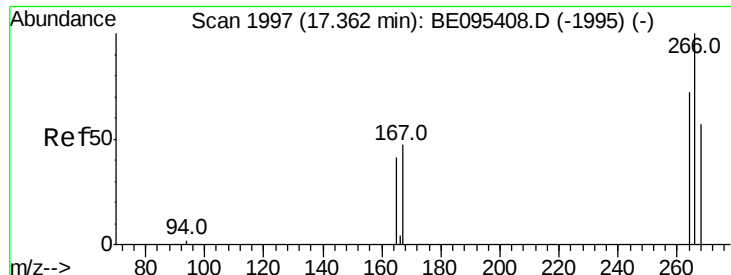

#11
 Pentachlorophenol
 Concen: 2.007 ng/ul
 RT: 17.36 min Scan# 1997
 Delta R.T. 0.00 min
 Lab File: BE095425.D
 Acq: 3 Feb 2018 7:50

Instrument :
 BNA_E
 ClientSampleId :
 F6C16DL

Tot Ion	Ratio	Lower	Upper
266	100		
264	61.6	47.9	71.9
268	63.5	49.8	74.8

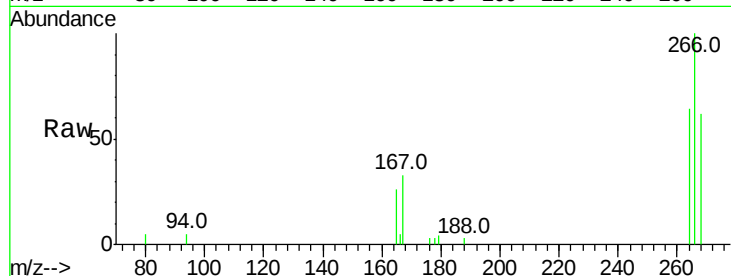

Abundance Ion 266.00 (265.70 to 266.70): E
 Ion 264.00 (263.70 to 264.70): E
 Ion 268.00 (267.70 to 268.70): E

