


Data Path : Z:\HPCHEM1\BNA\_E\DATA\BE020315\  
 Data File : Be089464.d  
 Acq On : 3 Feb 2015 14:59  
 Operator : TP/IZ  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_E  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA\_E\METHODS\SIM-BE020315.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Wed Feb 04 00:53:32 2015

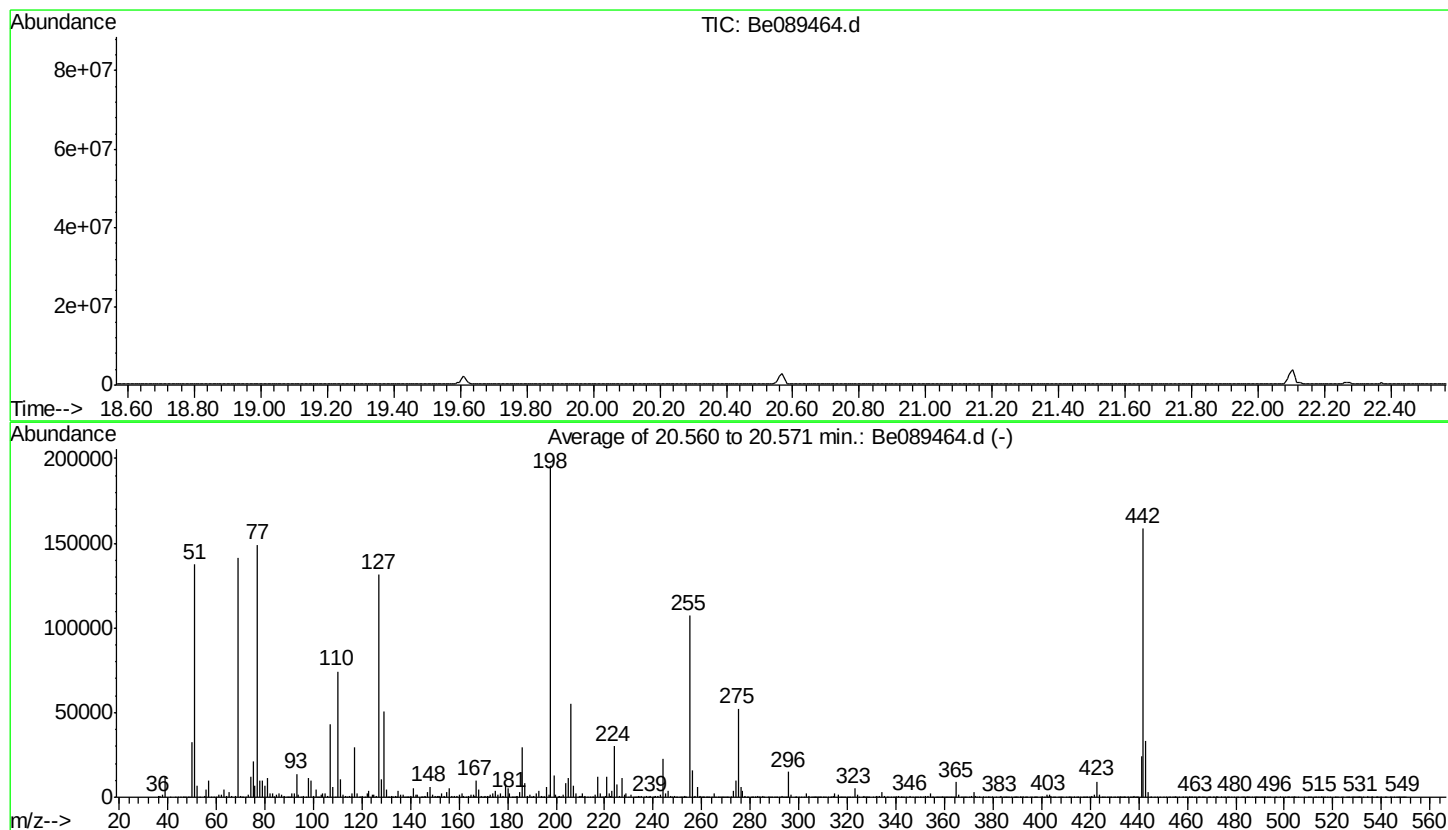

AutoFind: Scans 3263, 3264, 3265; Background Corrected with Scan 3257

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 70.1      | 137314  | PASS             |
| 68          | 69           | 0.00         | 2            | 0.6       | 804     | PASS             |
| 69          | 198          | 0.00         | 100          | 72.1      | 141295  | PASS             |
| 70          | 69           | 0.00         | 2            | 0.5       | 668     | PASS             |
| 127         | 198          | 10           | 80           | 67.1      | 131464  | PASS             |
| 197         | 198          | 0.00         | 2            | 0.6       | 1174    | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 195837  | PASS             |
| 199         | 198          | 5            | 9            | 6.6       | 12837   | PASS             |
| 275         | 198          | 10           | 60           | 26.8      | 52501   | PASS             |
| 365         | 198          | 1            | 100          | 4.5       | 8876    | PASS             |
| 441         | 442          | 0.01         | 24           | 15.3      | 24221   | PASS             |
| 442         | 198          | 50           | 100          | 81.1      | 158742  | PASS             |
| 443         | 442          | 15           | 24           | 21.1      | 33536   | PASS             |