


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE020315\
 Data File : BE089481.D
 Acq On : 4 Feb 2015 2:07
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\SIM-BE020315.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Feb 04 00:53:32 2015

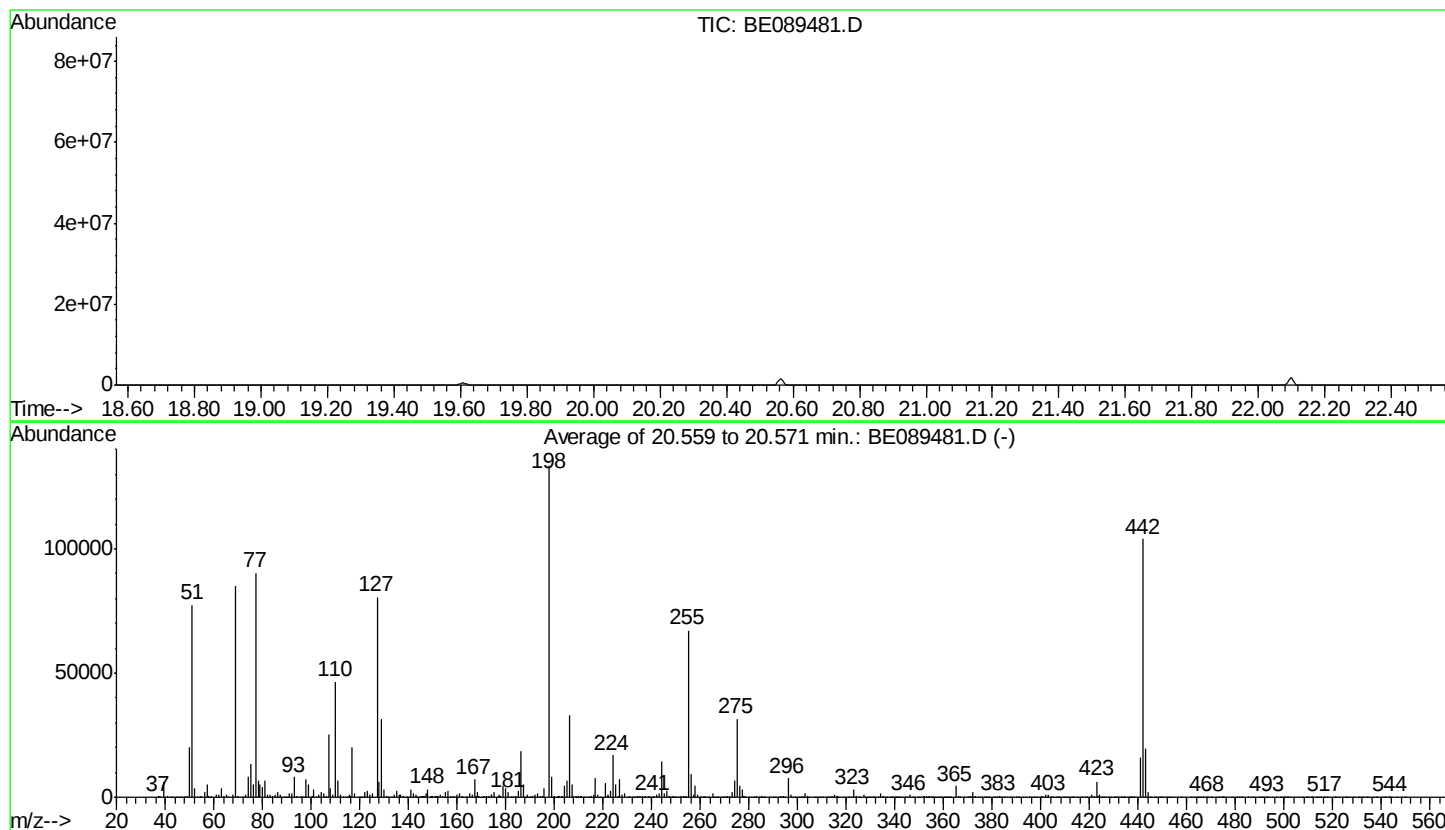

AutoFind: Scans 3263, 3264, 3265; Background Corrected with Scan 3257

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	57.9	77355	PASS
68	69	0.00	2	1.5	1259	PASS
69	198	0.00	100	63.7	85050	PASS
70	69	0.00	2	0.5	391	PASS
127	198	10	80	60.3	80501	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	133569	PASS
199	198	5	9	6.2	8263	PASS
275	198	10	60	23.6	31474	PASS
365	198	1	100	3.4	4509	PASS
441	442	0.01	24	15.2	15843	PASS
442	198	50	100	77.9	104025	PASS
443	442	15	24	19.0	19751	PASS