


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE020315\
 Data File : Be089464.d
 Acq On : 3 Feb 2015 14:59
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\SIM-BE020315.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Feb 04 00:53:32 2015

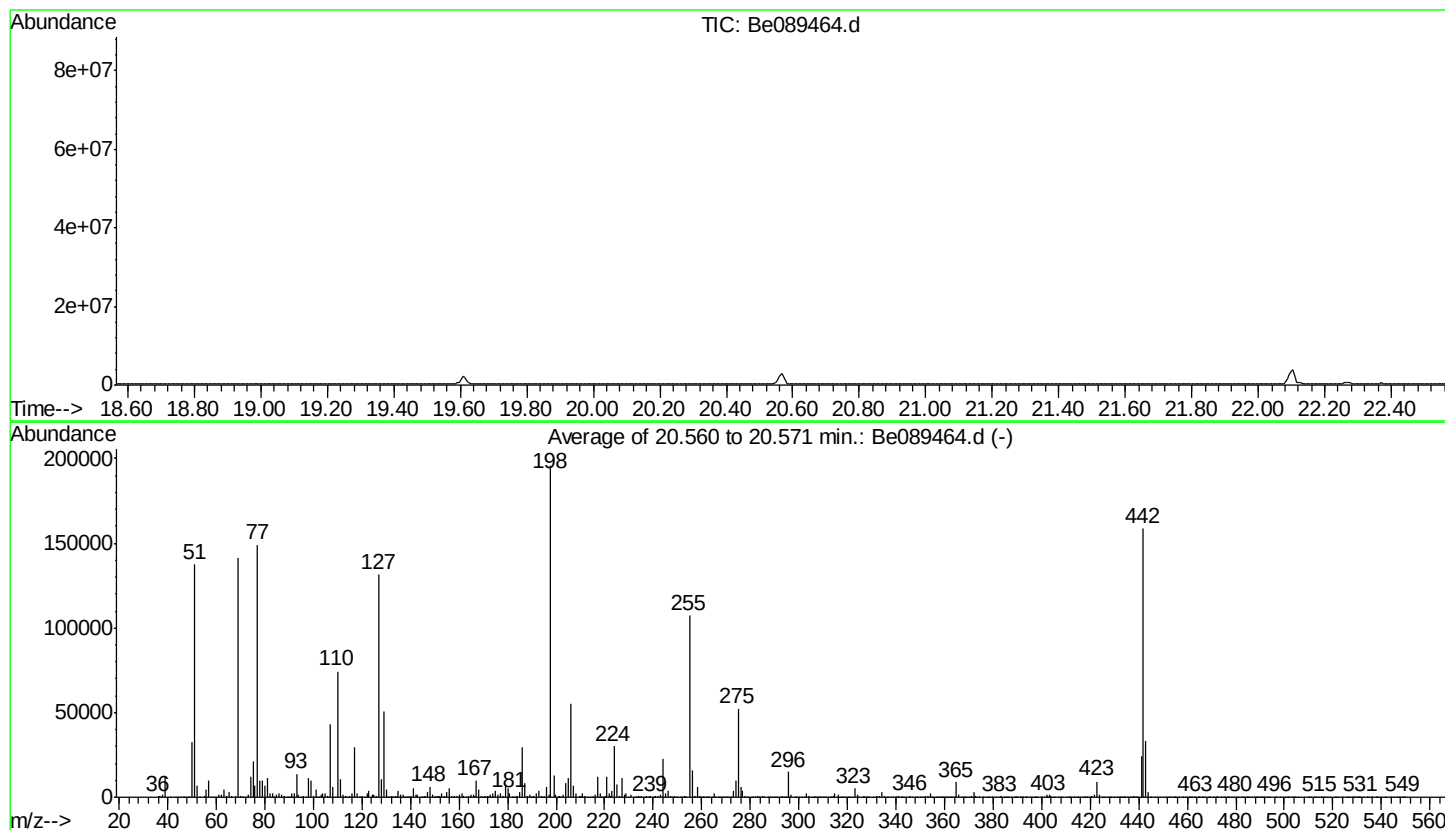

AutoFind: Scans 3263, 3264, 3265; Background Corrected with Scan 3257

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	70.1	137314	PASS
68	69	0.00	2	0.6	804	PASS
69	198	0.00	100	72.1	141295	PASS
70	69	0.00	2	0.5	668	PASS
127	198	10	80	67.1	131464	PASS
197	198	0.00	2	0.6	1174	PASS
198	198	100	100	100.0	195837	PASS
199	198	5	9	6.6	12837	PASS
275	198	10	60	26.8	52501	PASS
365	198	1	100	4.5	8876	PASS
441	442	0.01	24	15.3	24221	PASS
442	198	50	100	81.1	158742	PASS
443	442	15	24	21.1	33536	PASS