

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020318\
 Data File : BE095435.D
 Acq On : 3 Feb 2018 13:49
 Operator : SJ/JU
 Sample : J1314-16
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Feb 05 03:34:05 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 05 03:32:57 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.44	152	1693	0.40	ng/ul	0.00
2) Naphthalene-d8	11.26	136	4991	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.01	164	3286	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	6947	0.40	ng/ul	0.00
16) Chrysene-d12	21.80	240	6988	0.40	ng/ul	0.00
20) Perylene-d12	24.26	264	339216	0.40	ng/ul	-0.17
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	2887	0.36	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	7755	0.29	ng/ul	0.00
Target Compounds				Ovalue		
11) Pentachlorophenol	17.36	266	61	0.045	ng/ul#	87
12) Phenanthrene	17.75	178	740	0.032	ng/ul#	76
17) Pyrene	20.05	202	1070	0.046	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020318\
Data File : BE095435.D
Acq On : 3 Feb 2018 13:49
Operator : SJ/JU
Sample : J1314-16
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Feb 05 03:34:05 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 05 03:32:57 2018
Response via : Initial Calibration




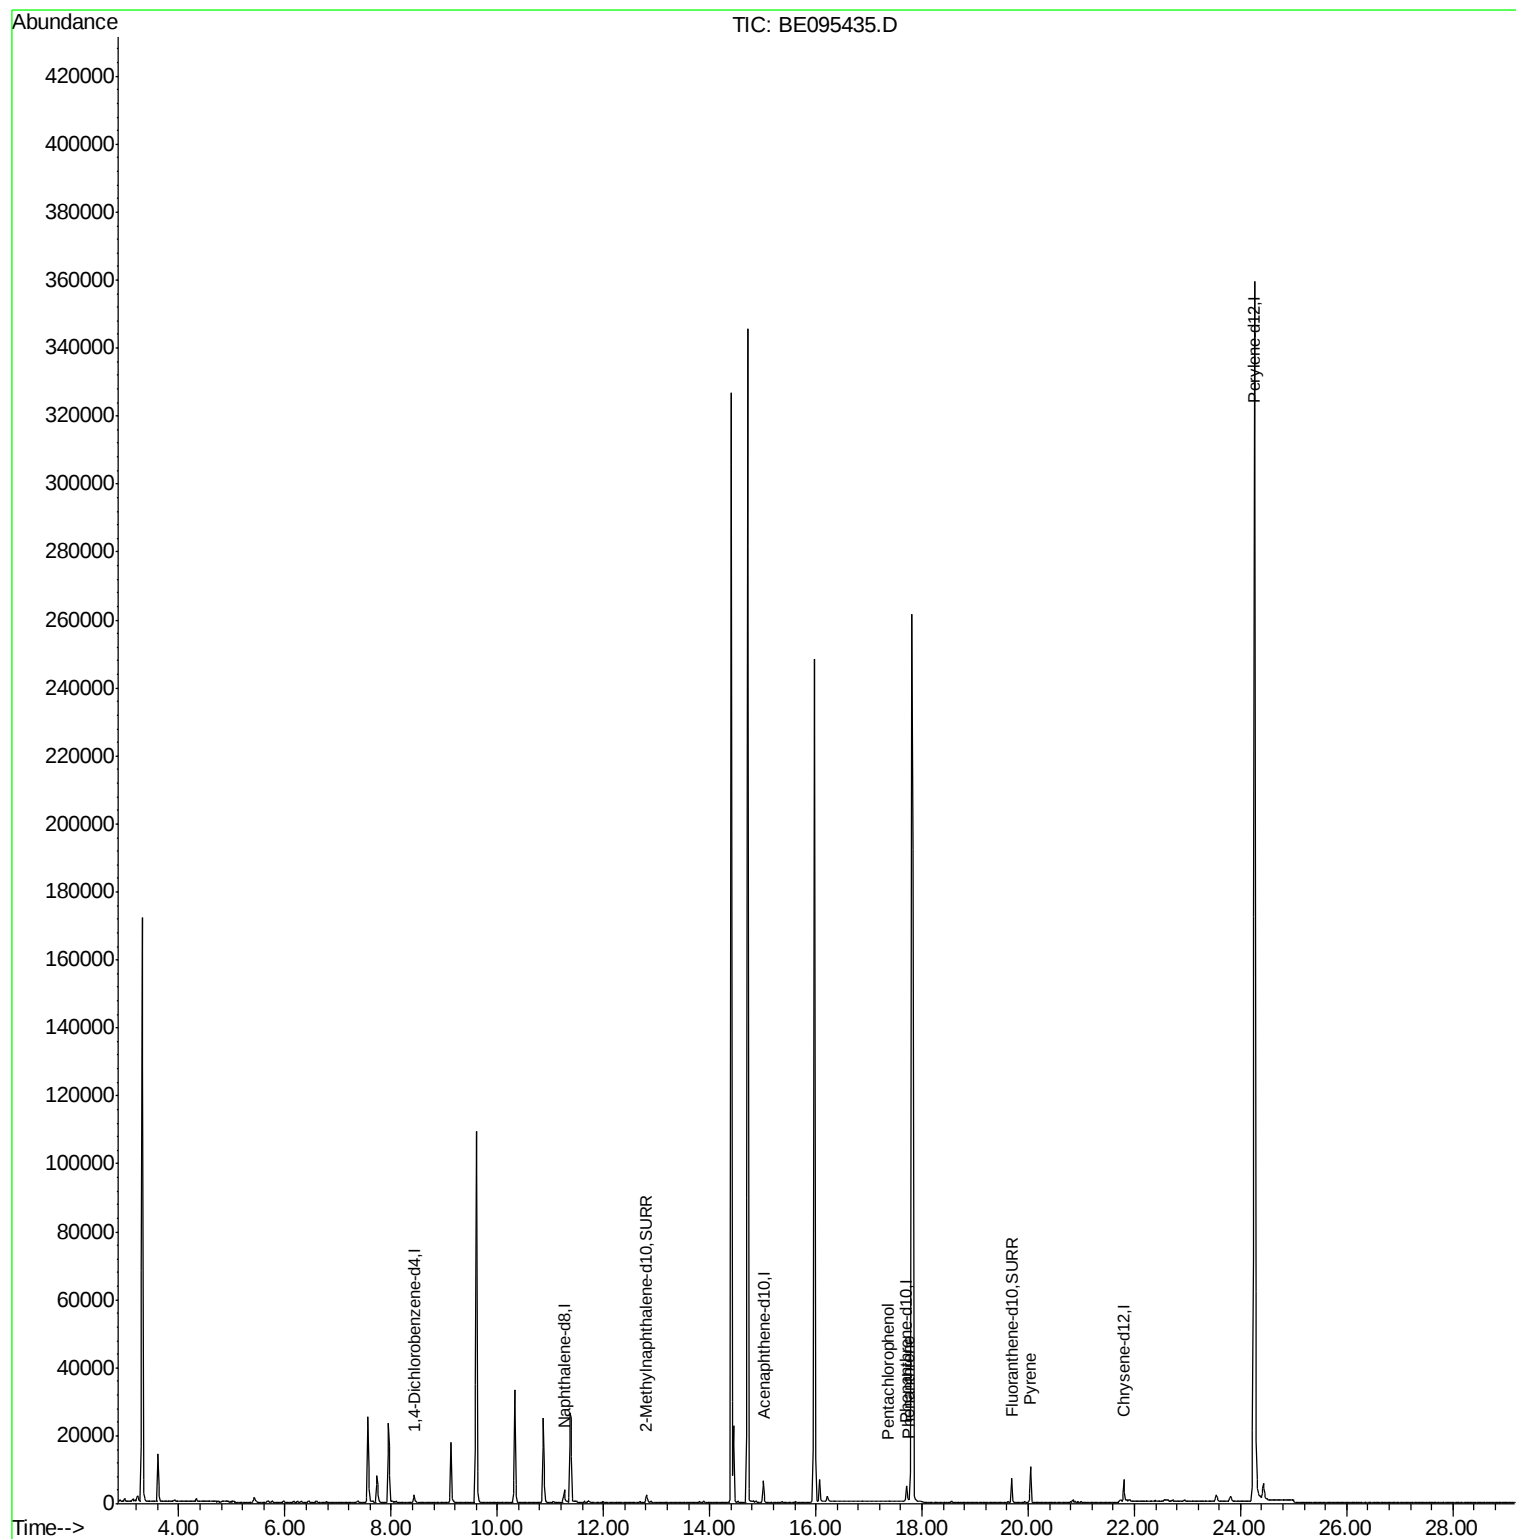


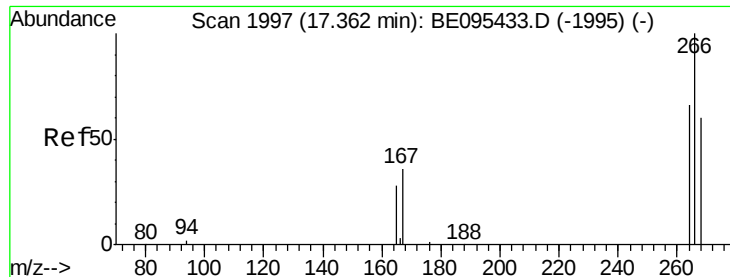

#11
 Pentachlorophenol
 Concen: 0.045 ng/ul
 RT: 17.36 min Scan# 1997
 Delta R.T. -0.00 min
 Lab File: BE095435.D
 Acq: 3 Feb 2018 13:49




Instrument :
 BNA_E
 ClientSampleId :


Tot Ion:266 Resp: 61
 Ion Ratio Lower Upper
 266 100
 264 52.5 47.9 71.9
 268 49.2 49.8 74.8#

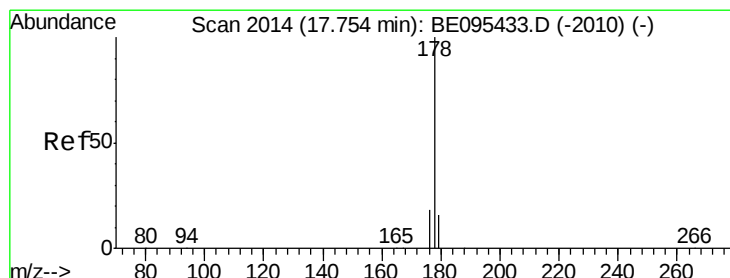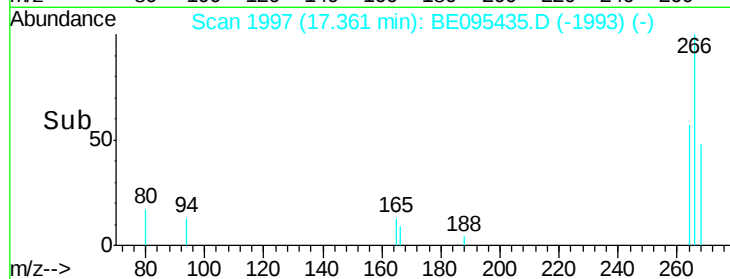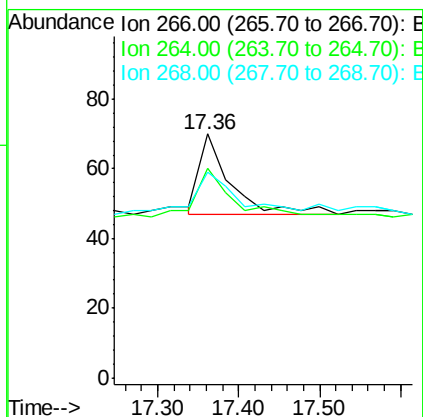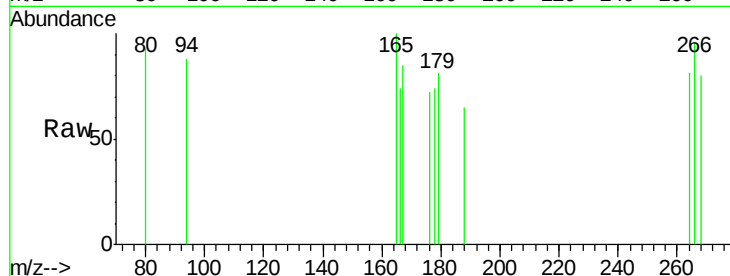

#12
 Phenanthrene
 Concen: 0.032 ng/ul
 RT: 17.75 min Scan# 2014
 Delta R.T. -0.00 min
 Lab File: BE095435.D
 Acq: 3 Feb 2018 13:49

Tgt Ion:178 Resp: 740
 Ion Ratio Lower Upper
 178 100
 179 32.4 18.4 27.6#
 176 29.8 13.6 20.4#

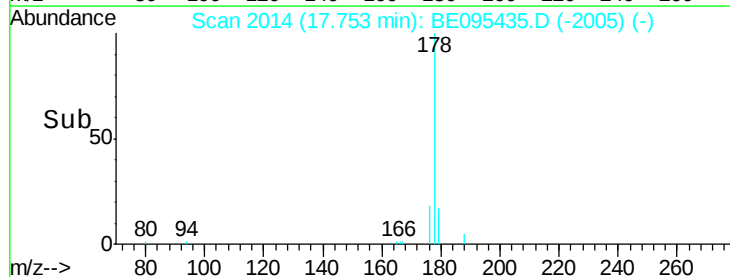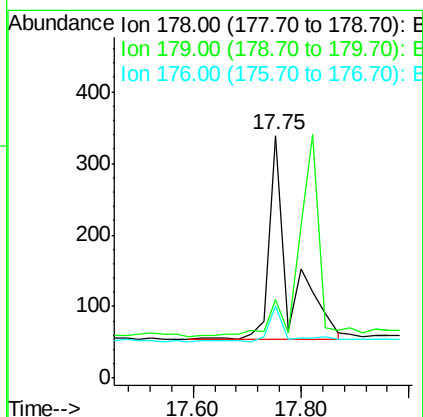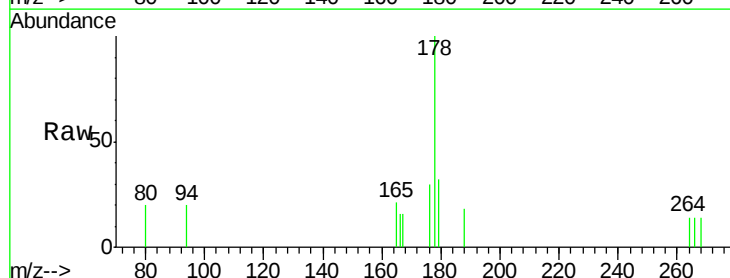


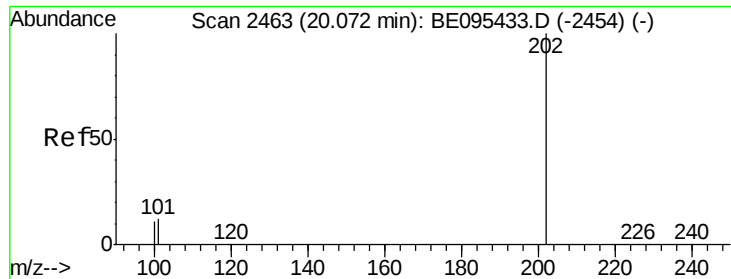

#17
 Pvrene
 Concen: 0.046 ng/ul
 RT: 20.05 min Scan# 2460
 Delta R.T. -0.02 min
 Lab File: BE095435.D
 Acq: 3 Feb 2018 13:49

Instrument :
 BNA_E
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
202	100		
101	161.1	18.2	27.4#
100	993.0	15.6	23.4#

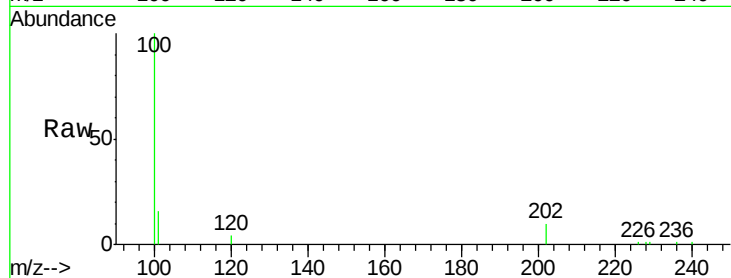

Abundance Ion 202.00 (201.70 to 202.70): E
 Ion 101.00 (100.70 to 101.70): E
 Ion 100.00 (99.70 to 100.70): BE

