

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020318\
 Data File : BE095451.D
 Acq On : 3 Feb 2018 23:22
 Operator : SJ/JU
 Sample : J1296-14
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Feb 05 04:52:58 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 05 04:46:10 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.44	152	1797	0.40	ng/ul	0.00
2) Naphthalene-d8	11.26	136	5491	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.02	164	3597	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	7498	0.40	ng/ul	0.00
16) Chrysene-d12	21.80	240	7396	0.40	ng/ul	0.00
20) Perylene-d12	24.26	264	384111	0.40	ng/ul	-0.17
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	3205	0.36	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	8157	0.28	ng/ul	0.00
Target Compounds				Ovalue		
11) Pentachlorophenol	17.36	266	40	0.028	ng/ul	95
12) Phenanthrene	17.75	178	625	0.025	ng/ul#	64
17) Pyrene	20.05	202	1213	0.049	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020318\
Data File : BE095451.D
Acq On : 3 Feb 2018 23:22
Operator : SJ/JU
Sample : J1296-14
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Feb 05 04:52:58 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 05 04:46:10 2018
Response via : Initial Calibration




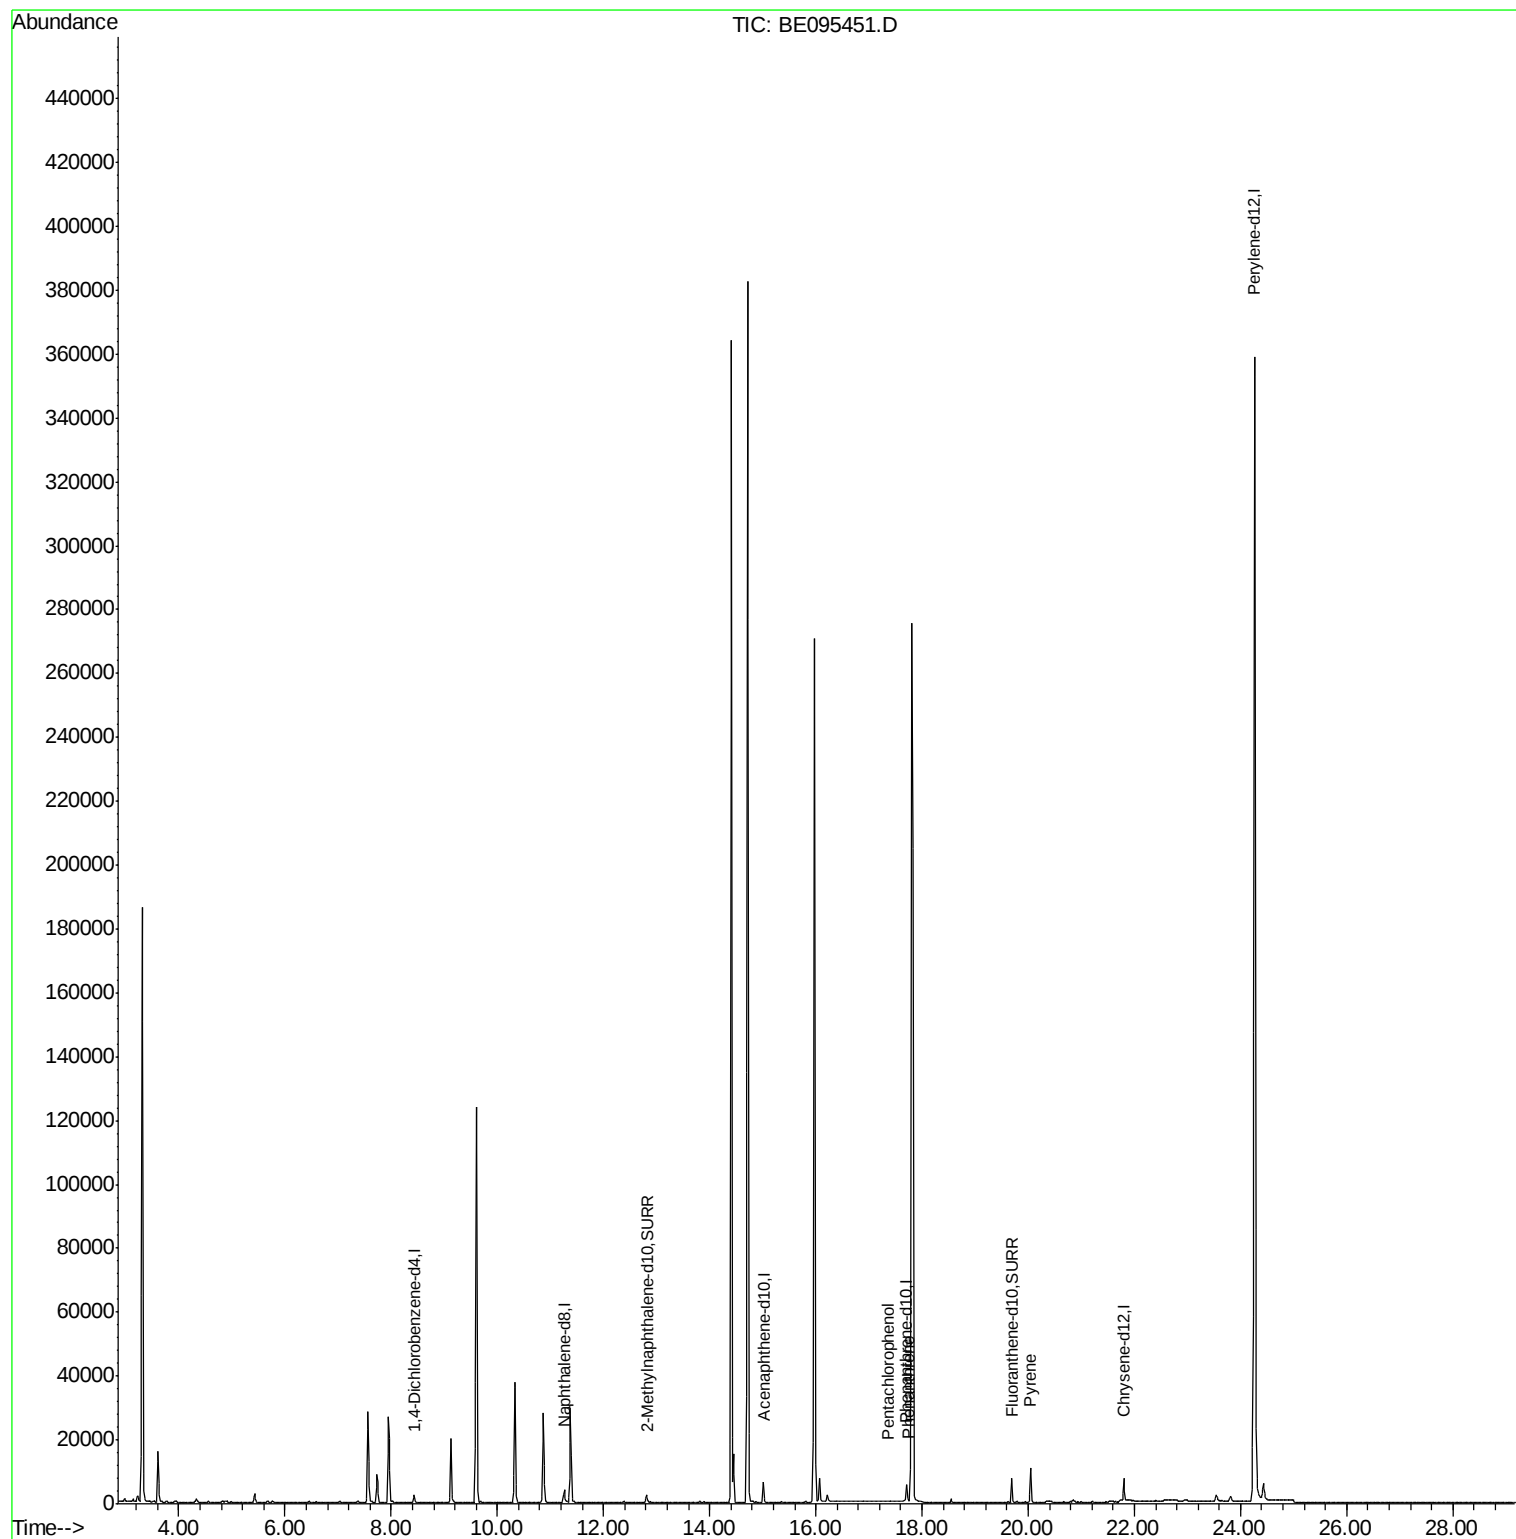


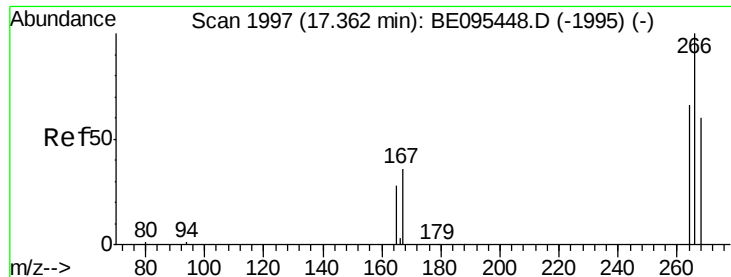

#11
 Pentachlorophenol
 Concen: 0.028 ng/ul
 RT: 17.36 min Scan# 1997
 Delta R.T. 0.00 min
 Lab File: BE095451.D
 Acq: 3 Feb 2018 23:22




Instrument :
 BNA_E
 ClientSampleId :


Tot Ion:266 Resp: 40
 Ion Ratio Lower Upper
 266 100
 264 52.5 47.9 71.9
 268 62.5 49.8 74.8

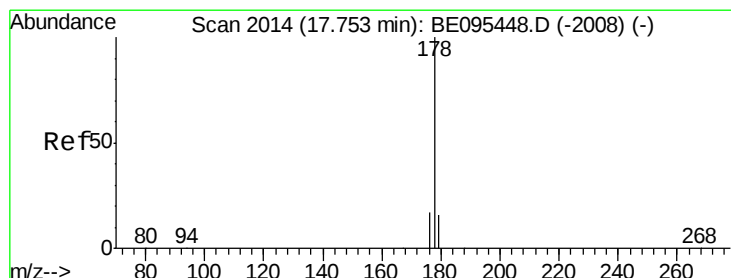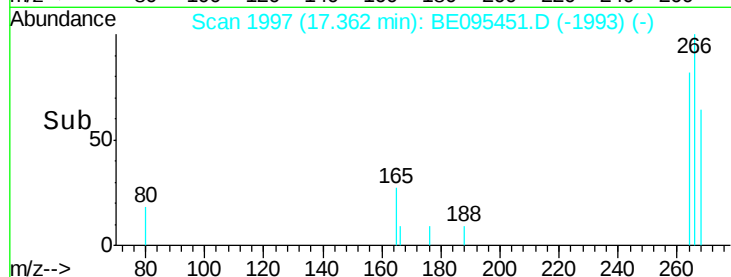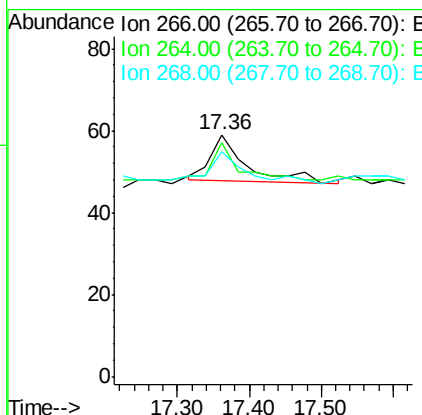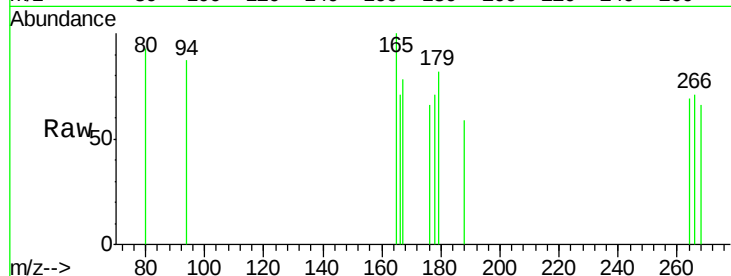

#12
 Phenanthrene
 Concen: 0.025 ng/ul
 RT: 17.75 min Scan# 2014
 Delta R.T. 0.00 min
 Lab File: BE095451.D
 Acq: 3 Feb 2018 23:22

Tgt Ion:178 Resp: 625
 Ion Ratio Lower Upper
 178 100
 179 39.0 18.4 27.6#
 176 34.7 13.6 20.4#

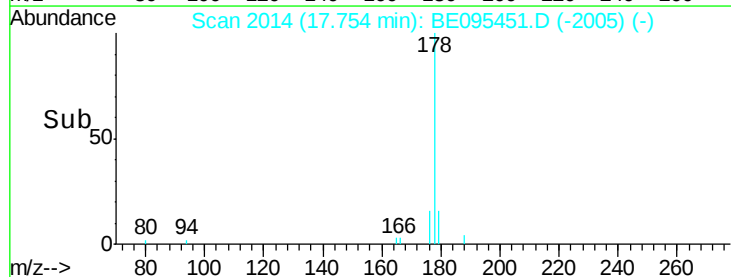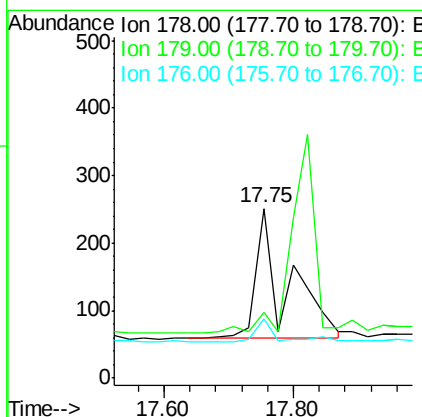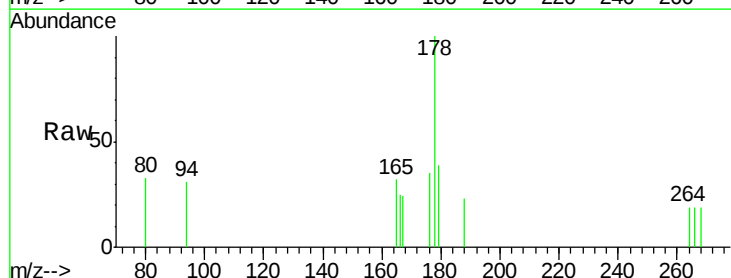

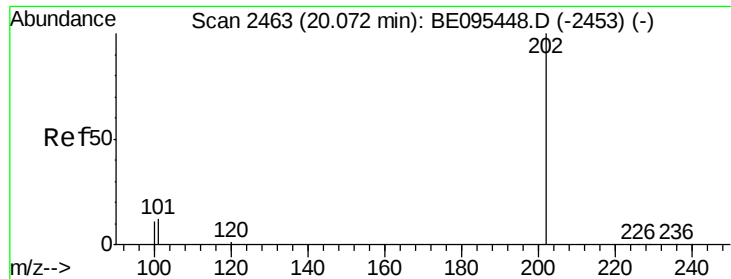

#17
 Pvrene
 Concen: 0.049 ng/ul
 RT: 20.05 min Scan# 2460
 Delta R.T. -0.02 min
 Lab File: BE095451.D
 Acq: 3 Feb 2018 23:22

Instrument :
 BNA_E
 ClientSampleId :

Tot Ion: 202 Resp: 1213
 Ion Ratio Lower Upper
 202 100
 101 162.8 18.2 27.4#
 100 1039.6 15.6 23.4#

