

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020318\
 Data File : BE095457.D
 Acq On : 4 Feb 2018 2:57
 Operator : SJ/JU
 Sample : J1314-08
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Feb 05 04:53:44 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 05 04:46:10 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.43	152	1791	0.40	ng/ul	0.00
2) Naphthalene-d8	11.26	136	5575	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.02	164	3779	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	7971	0.40	ng/ul	0.00
16) Chrysene-d12	21.80	240	7613	0.40	ng/ul	0.00
20) Perylene-d12	24.27	264	412250	0.40	ng/ul	-0.17
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	3379	0.37	ng/ul	0.00
14) Fluoranthene-d10	19.70	212	8905	0.29	ng/ul	0.00
Target Compounds				Ovalue		
11) Pentachlorophenol	17.36	266	612	0.396	ng/ul	95
12) Phenanthrene	17.75	178	861	0.032	ng/ul#	63
17) Pyrene	20.05	202	1837	0.072	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020318\
Data File : BE095457.D
Acq On : 4 Feb 2018 2:57
Operator : SJ/JU
Sample : J1314-08
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Feb 05 04:53:44 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 05 04:46:10 2018
Response via : Initial Calibration




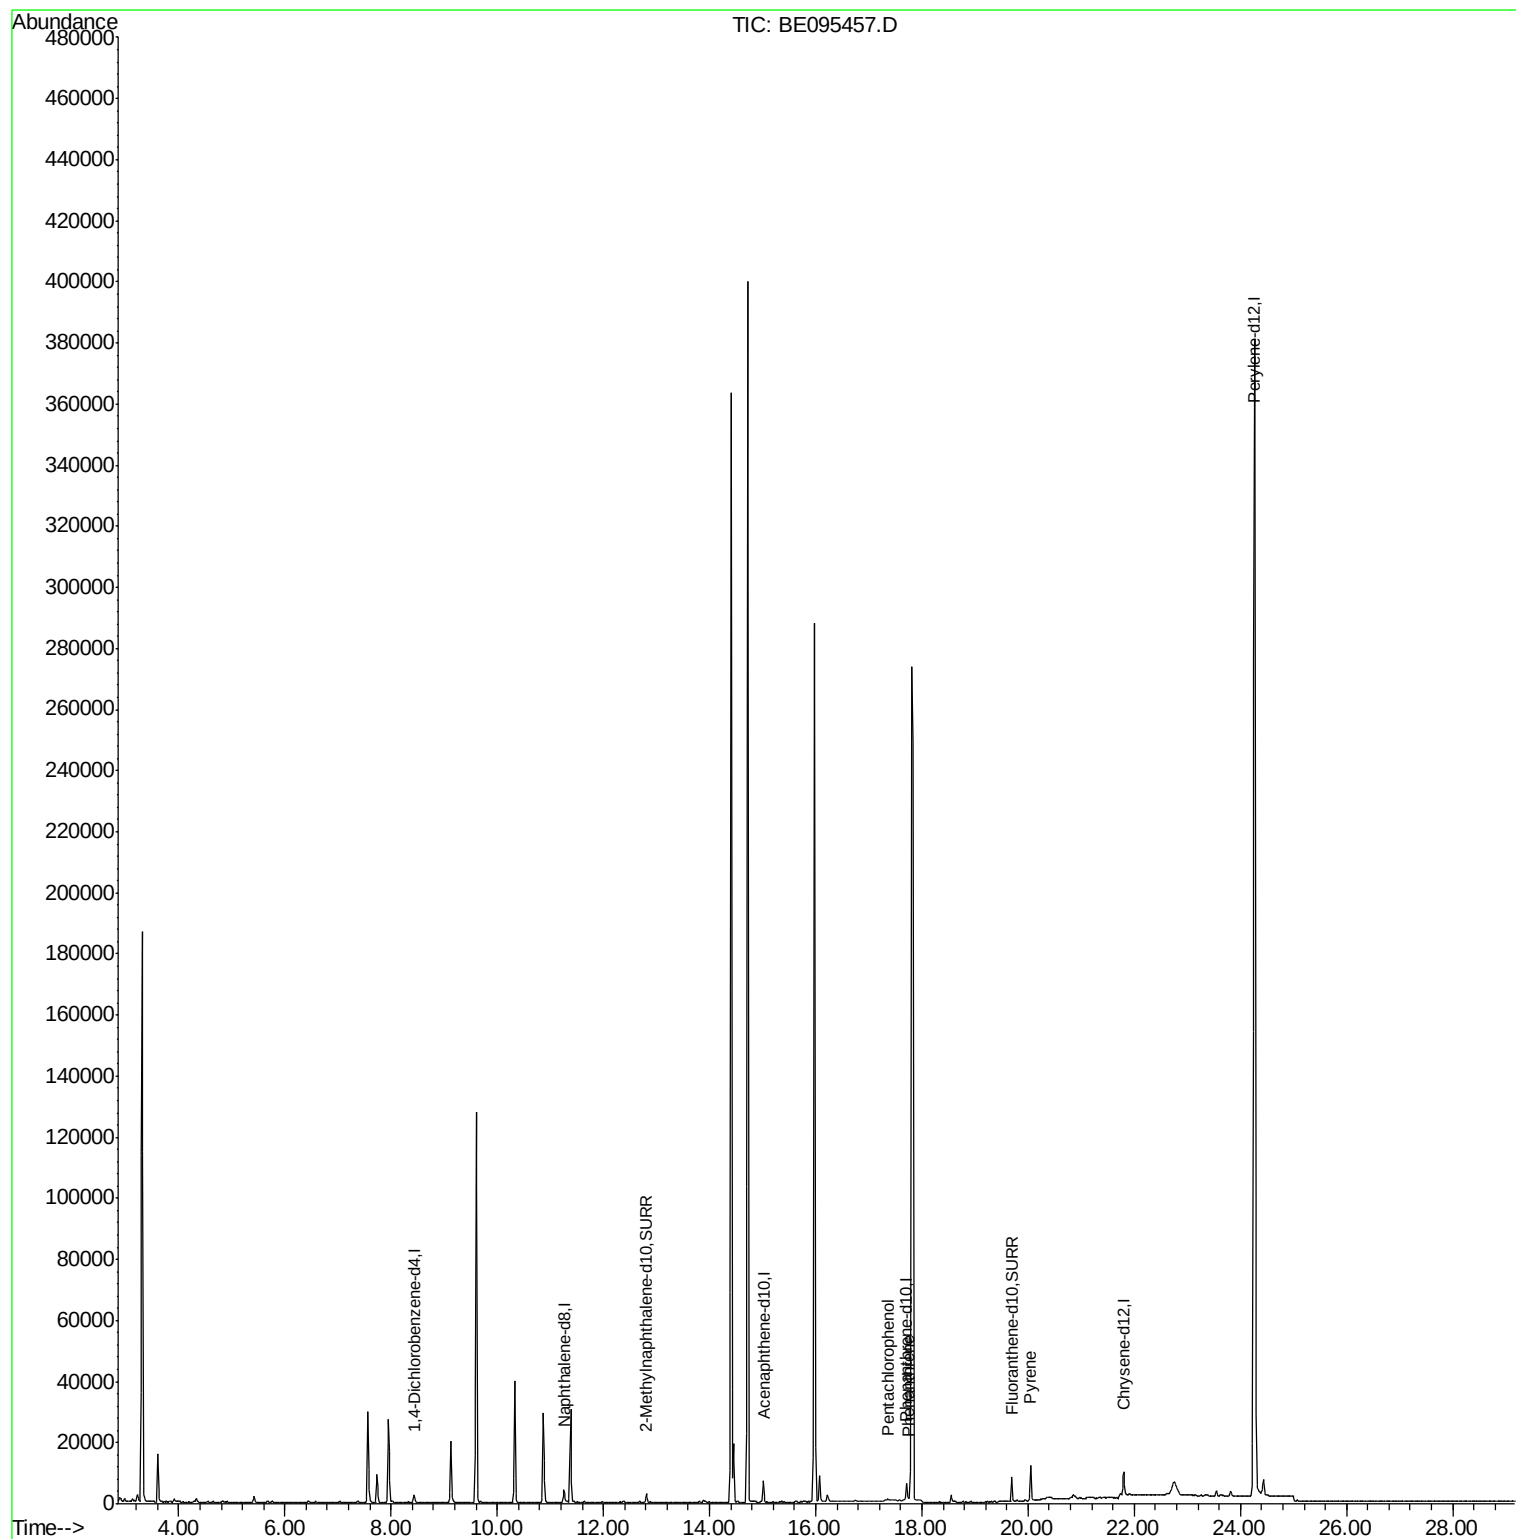


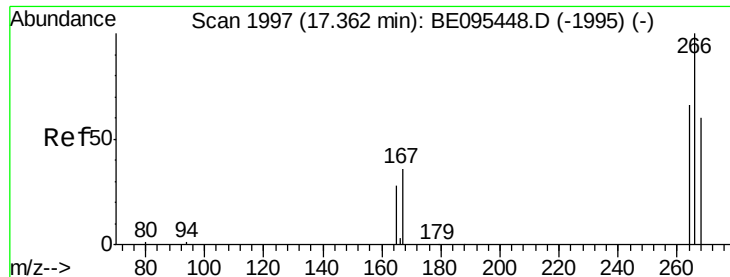

#11
 Pentachlorophenol
 Concen: 0.396 ng/ul
 RT: 17.36 min Scan# 1997
 Delta R.T. 0.00 min
 Lab File: BE095457.D
 Acq: 4 Feb 2018 2:57




Instrument :
 BNA_E
 ClientSampleId :


Tot Ion:266 Resp: 612
 Ion Ratio Lower Upper
 266 100
 264 62.7 47.9 71.9
 268 67.2 49.8 74.8

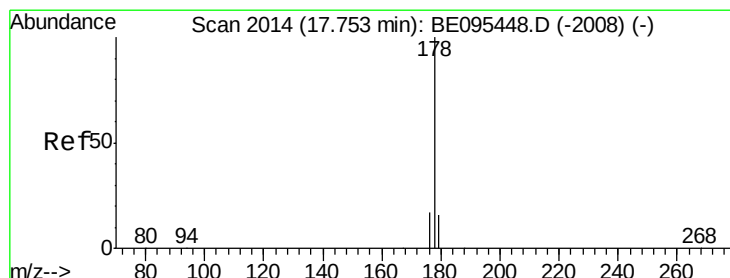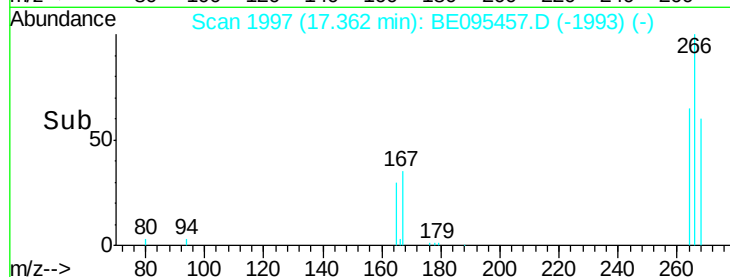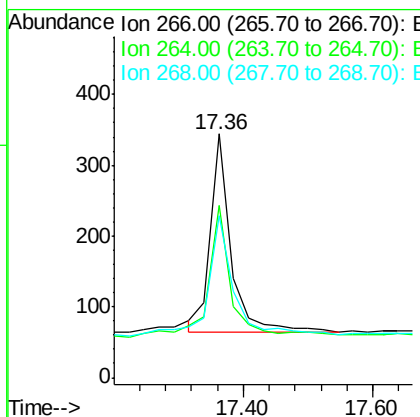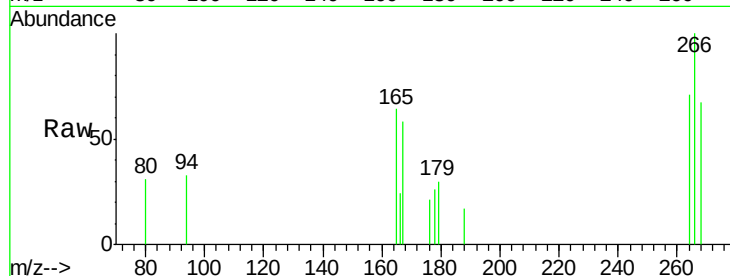

#12
 Phenanthrene
 Concen: 0.032 ng/ul
 RT: 17.75 min Scan# 2014
 Delta R.T. 0.00 min
 Lab File: BE095457.D
 Acq: 4 Feb 2018 2:57

Tgt Ion:178 Resp: 861
 Ion Ratio Lower Upper
 178 100
 179 41.9 18.4 27.6#
 176 32.1 13.6 20.4#

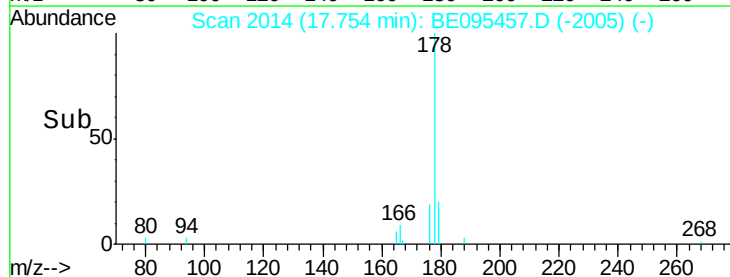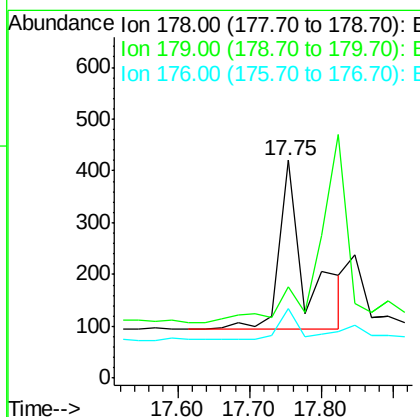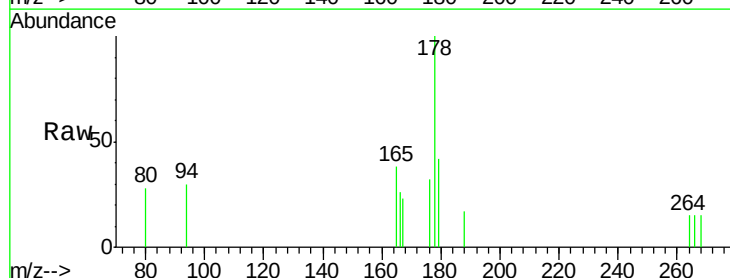

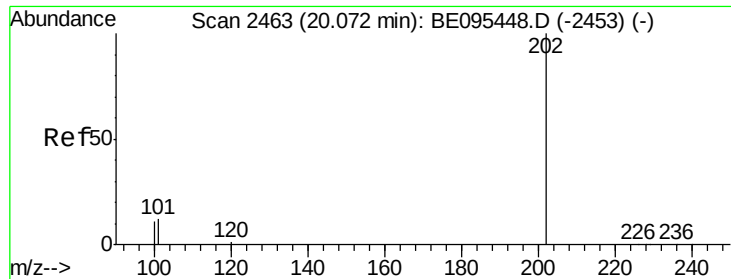

#17

Pvrene

Concen: 0.072 ng/ul

RT: 20.05 min Scan# 2460

Delta R.T. -0.02 min

Lab File: BE095457.D

Acq: 4 Feb 2018 2:57

Instrument :

BNA_E

ClientSampleId :

Tot Ion: 202 Resp: 1837

Ion Ratio Lower Upper

202 100

101 146.5 18.2 27.4#

100 927.3 15.6 23.4#

