

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020318\
 Data File : BE095462.D
 Acq On : 4 Feb 2018 5:53
 Operator : SJ/JU
 Sample : J1314-12
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Feb 05 04:54:19 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 05 04:46:10 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.44	152	2095	0.40	ng/ul	0.00
2) Naphthalene-d8	11.26	136	6613	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.02	164	4501	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.71
16) Chrysene-d12	21.80	240	8966	0.40	ng/ul	0.00
20) Perylene-d12	24.27	264	553407	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	4241	0.39	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	10975	0.00	ng/ul	0.00
Target Compounds						
17) Pyrene	20.08	202	1140	0.038	ng/ul	93
18) Benzo(a)anthracene	21.79	228	595	0.021	ng/ul#	65


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020318\
Data File : BE095462.D
Acq On : 4 Feb 2018 5:53
Operator : SJ/JU
Sample : J1314-12
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Feb 05 04:54:19 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 05 04:46:10 2018
Response via : Initial Calibration

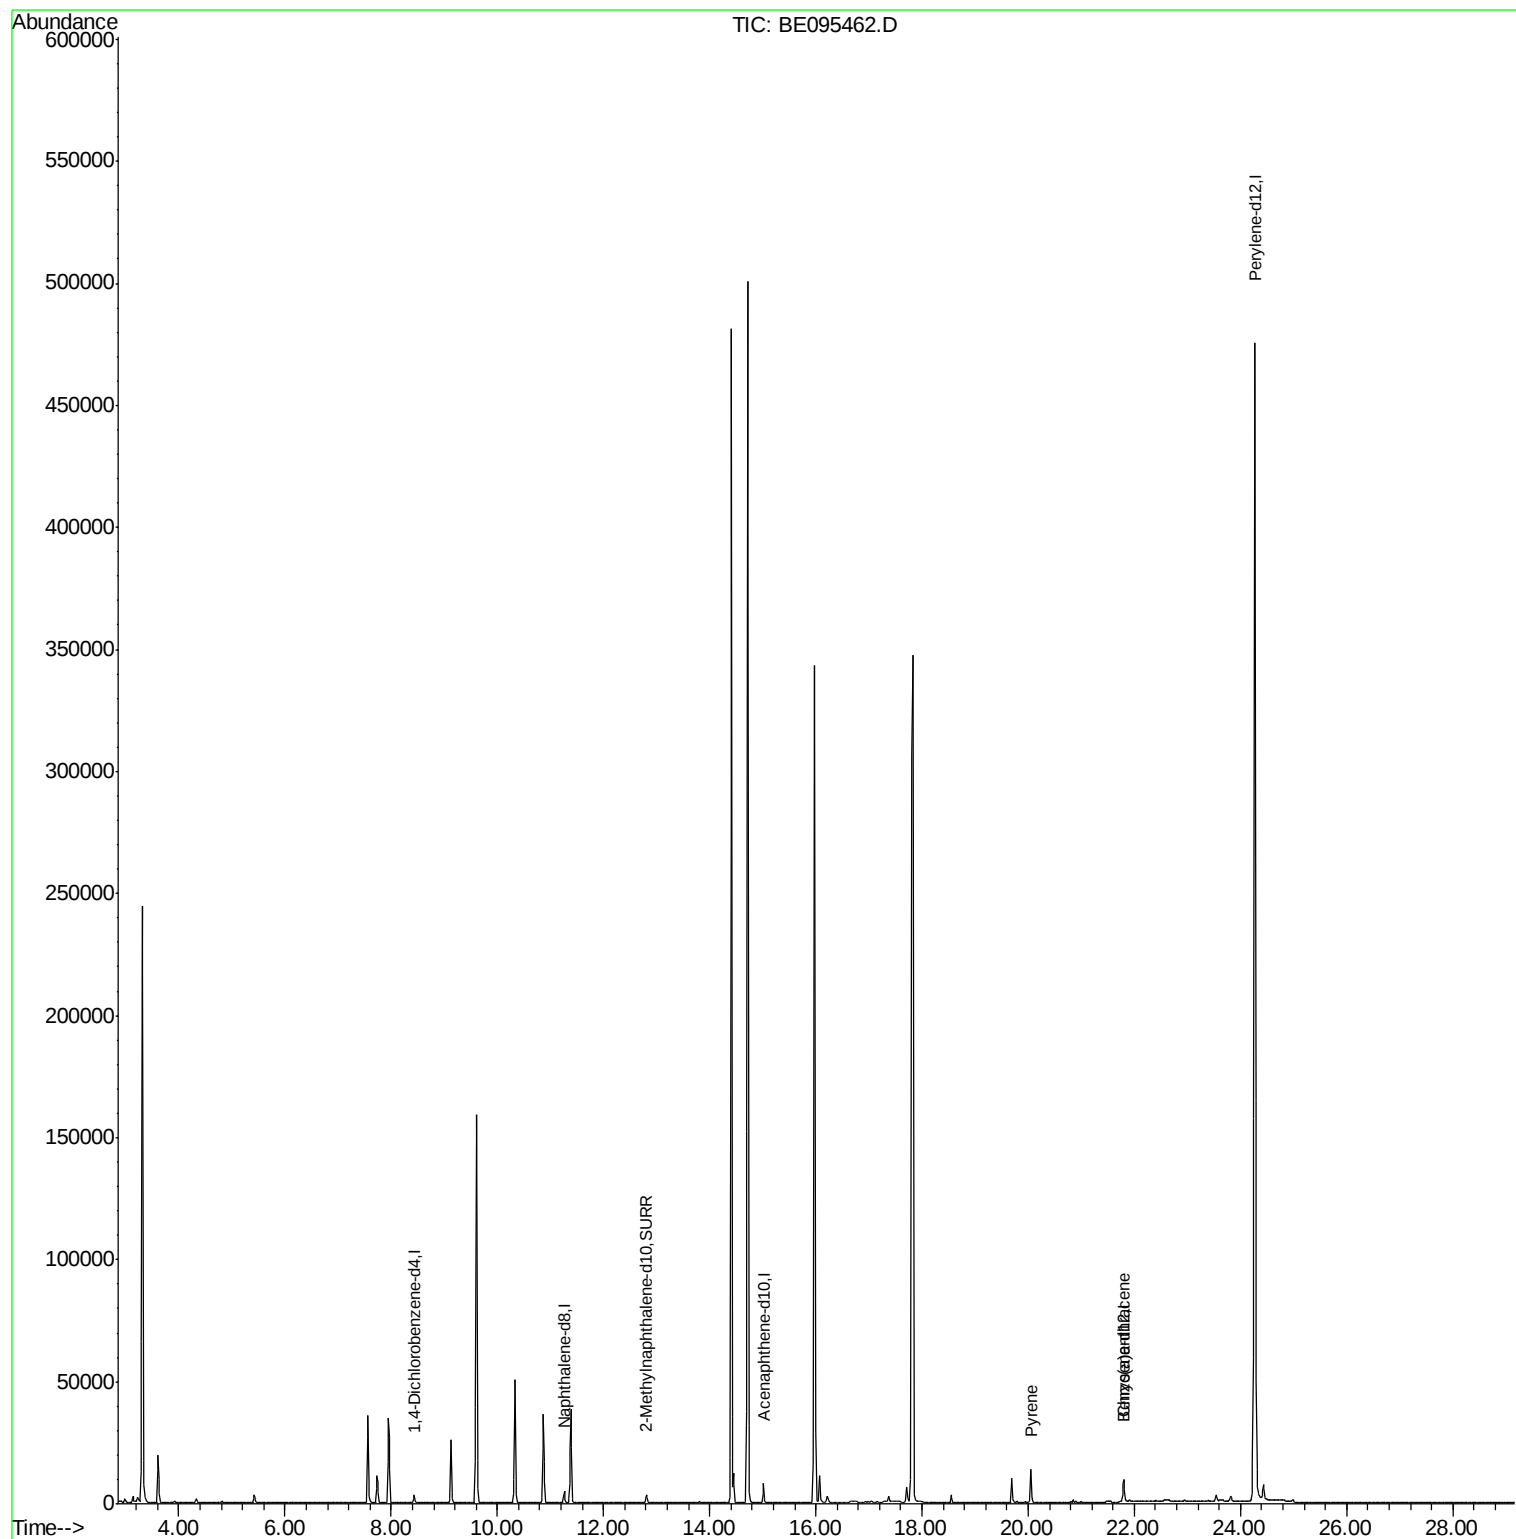


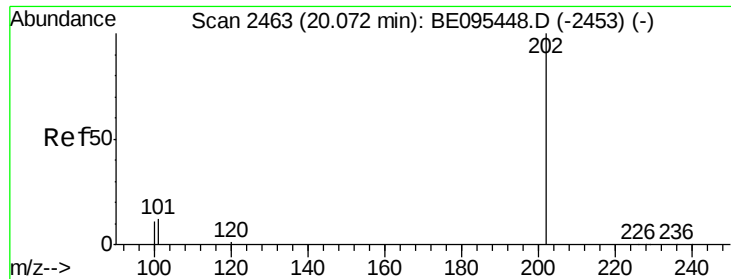




#17
Pvrene
Concen: 0.038 ng/ul
RT: 20.08 min Scan# 2465
Delta R.T. 0.01 min
Lab File: BE095462.D
Acq: 4 Feb 2018 5:53

Instrument :
BNA_E
ClientSampleId :

Tot Ion:202 Resp: 1140
Ion Ratio Lower Upper
202 100
101 18.5 18.2 27.4
100 17.4 15.6 23.4

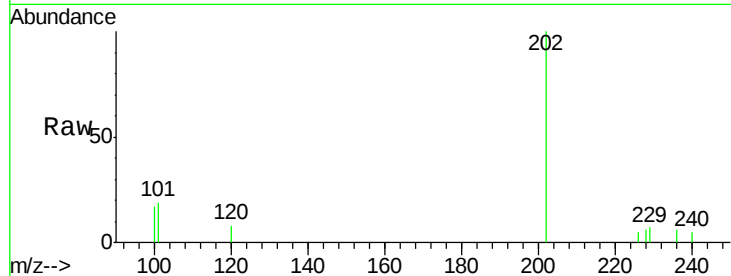


Abundance Ion 202.00 (201.70 to 202.70): E
Ion 101.00 (100.70 to 101.70): E
Ion 100.00 (99.70 to 100.70): E

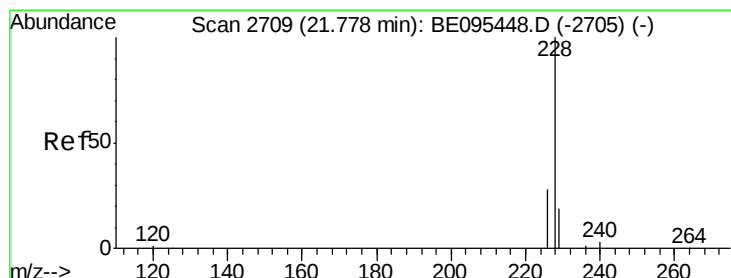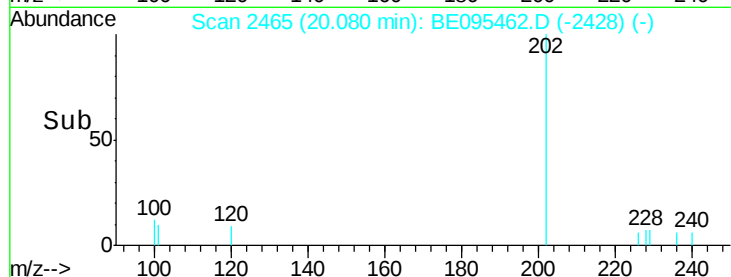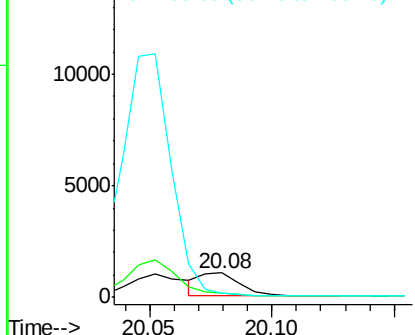

#18
Benzo(a)anthracene
Concen: 0.021 ng/ul
RT: 21.79 min Scan# 2710
Delta R.T. 0.01 min
Lab File: BE095462.D
Acq: 4 Feb 2018 5:53

Tgt Ion:228 Resp: 595
Ion Ratio Lower Upper
228 100
229 44.1 22.8 34.2#
226 41.3 17.0 25.6#

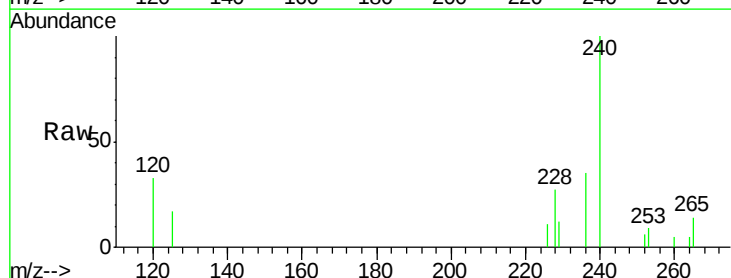

Abundance Ion 228.00 (227.70 to 228.70): E
Ion 229.00 (228.70 to 229.70): E
Ion 226.00 (225.70 to 226.70): E

