

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020318\
 Data File : BE095481.D
 Acq On : 4 Feb 2018 17:13
 Operator : SJ/JU
 Sample : J1315-13
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Feb 05 06:47:55 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 05 04:46:10 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.43	152	1845	0.40	ng/ul	0.00
2) Naphthalene-d8	11.26	136	5681	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.02	164	3775	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	7956	0.40	ng/ul	0.00
16) Chrysene-d12	21.80	240	7764	0.40	ng/ul	0.00
20) Perylene-d12	24.26	264	402766	0.40	ng/ul	-0.17
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	3375	0.36	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	8477	0.28	ng/ul	0.00
Target Compounds						
11) Pentachlorophenol	17.36	266	33	0.021	ng/ul#	88
17) Pyrene	20.05	202	1239	0.048	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020318\
Data File : BE095481.D
Acq On : 4 Feb 2018 17:13
Operator : SJ/JU
Sample : J1315-13
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Feb 05 06:47:55 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 05 04:46:10 2018
Response via : Initial Calibration




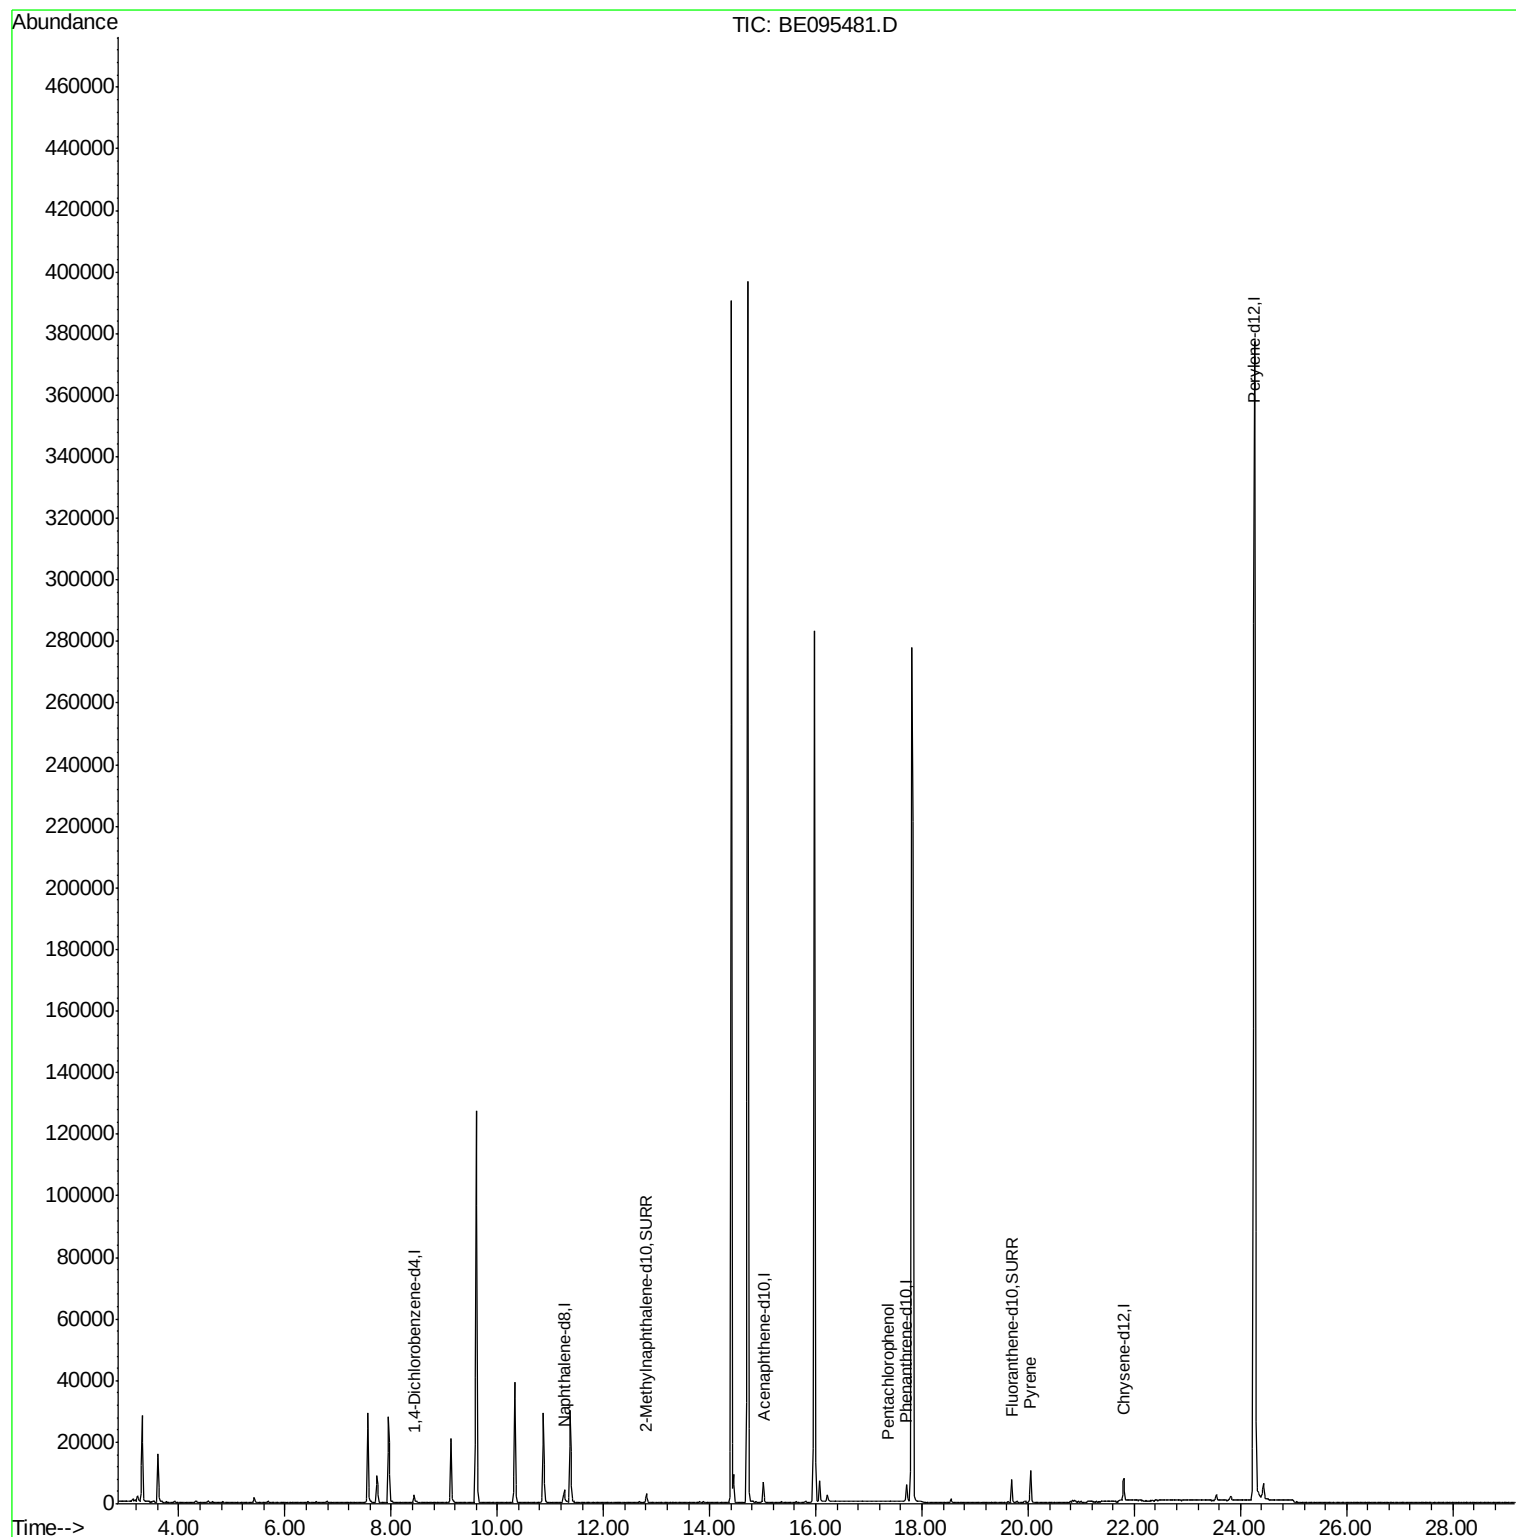


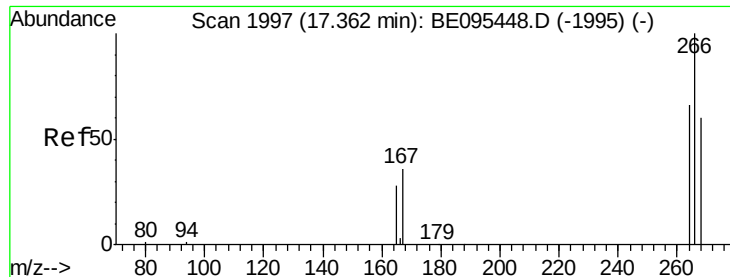

#11
 Pentachlorophenol
 Concen: 0.021 ng/ul
 RT: 17.36 min Scan# 1997
 Delta R.T. 0.00 min
 Lab File: BE095481.D
 Acq: 4 Feb 2018 17:13

Instrument :
 BNA_E
 ClientSampleId :

Tot Ion:266 Resp: 33
 Ion Ratio Lower Upper
 266 100
 264 42.4 47.9 71.9#
 268 63.6 49.8 74.8

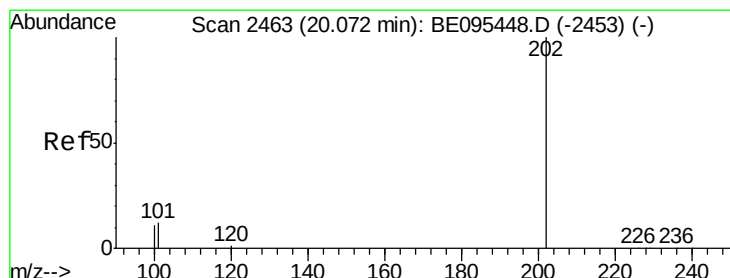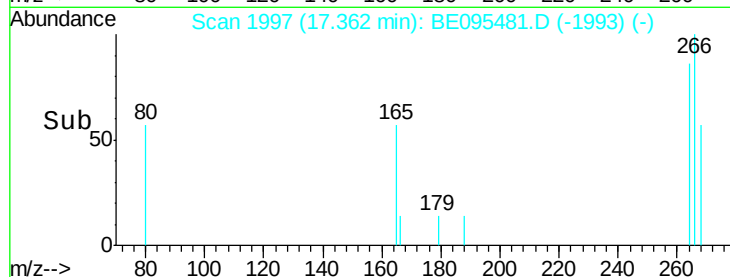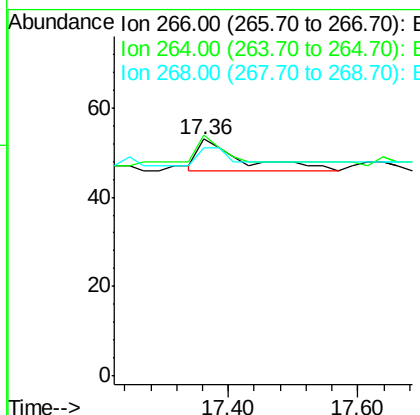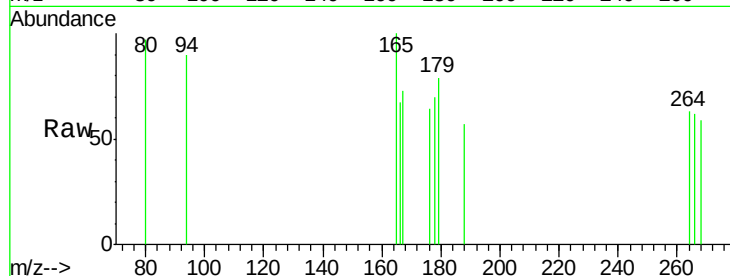

#17
 Pyrene
 Concen: 0.048 ng/ul
 RT: 20.05 min Scan# 2460
 Delta R.T. -0.02 min
 Lab File: BE095481.D
 Acq: 4 Feb 2018 17:13

Tgt Ion:202 Resp: 1239
 Ion Ratio Lower Upper
 202 100
 101 166.5 18.2 27.4#
 100 1060.4 15.6 23.4#

