

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020318\
 Data File : BE095482.D
 Acq On : 4 Feb 2018 17:49
 Operator : SJ/JU
 Sample : SSTDCCC0.4EC
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Feb 05 06:48:00 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 05 04:46:10 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.43	152	1501	0.40	ng/ul	0.00
2) Naphthalene-d8	11.26	136	4608	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.02	164	2762	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	6291	0.40	ng/ul	0.00
16) Chrysene-d12	21.80	240	6660	0.40	ng/ul	0.00
20) Perylene-d12	24.44	264	6261	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	3674	0.49	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	9077	0.38	ng/ul	0.00
Target Compounds					Ovalue	
3) Naphthalene	11.31	128	6080	0.471	ng/ul#	90
5) 2-Methylnaphthalene	12.88	142	4258	0.494	ng/ul	99
7) Acenaphthylene	14.74	152	6371	0.479	ng/ul	98
8) Acenaphthene	15.08	153	4646	0.451	ng/ul	96
9) Fluorene	16.02	166	5272	0.496	ng/ul#	85
11) Pentachlorophenol	17.36	266	402	0.330	ng/ul	98
12) Phenanthrene	17.75	178	8648	0.409	ng/ul#	91
13) Anthracene	17.85	178	7799	0.403	ng/ul#	93
15) Fluoranthene	19.72	202	10219	0.373	ng/ul	84
17) Pyrene	20.07	202	10676	0.478	ng/ul#	80
18) Benzo(a)anthracene	21.78	228	9665	0.464	ng/ul#	84
19) Chrysene	21.84	228	9330	0.432	ng/ul	97
21) Benzo(b)fluoranthene	23.62	252	9232	0.418	ng/ul	85
22) Benzo(k)fluoranthene	23.67	252	8587	0.425	ng/ul#	88
23) Benzo(a)pyrene	24.31	252	8498	0.431	ng/ul#	80
24) Indeno(1,2,3-cd)pyrene	27.25	276	8832	0.408	ng/ul#	77
25) Dibenzo(a,h)anthracene	27.26	278	7100	0.401	ng/ul	93
26) Benzo(g,h,i)perylene	28.12	276	7457	0.407	ng/ul	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020318\
Data File : BE095482.D
Acq On : 4 Feb 2018 17:49
Operator : SJ/JU
Sample : SSTDCCC0.4EC
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Feb 05 06:48:00 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 05 04:46:10 2018
Response via : Initial Calibration

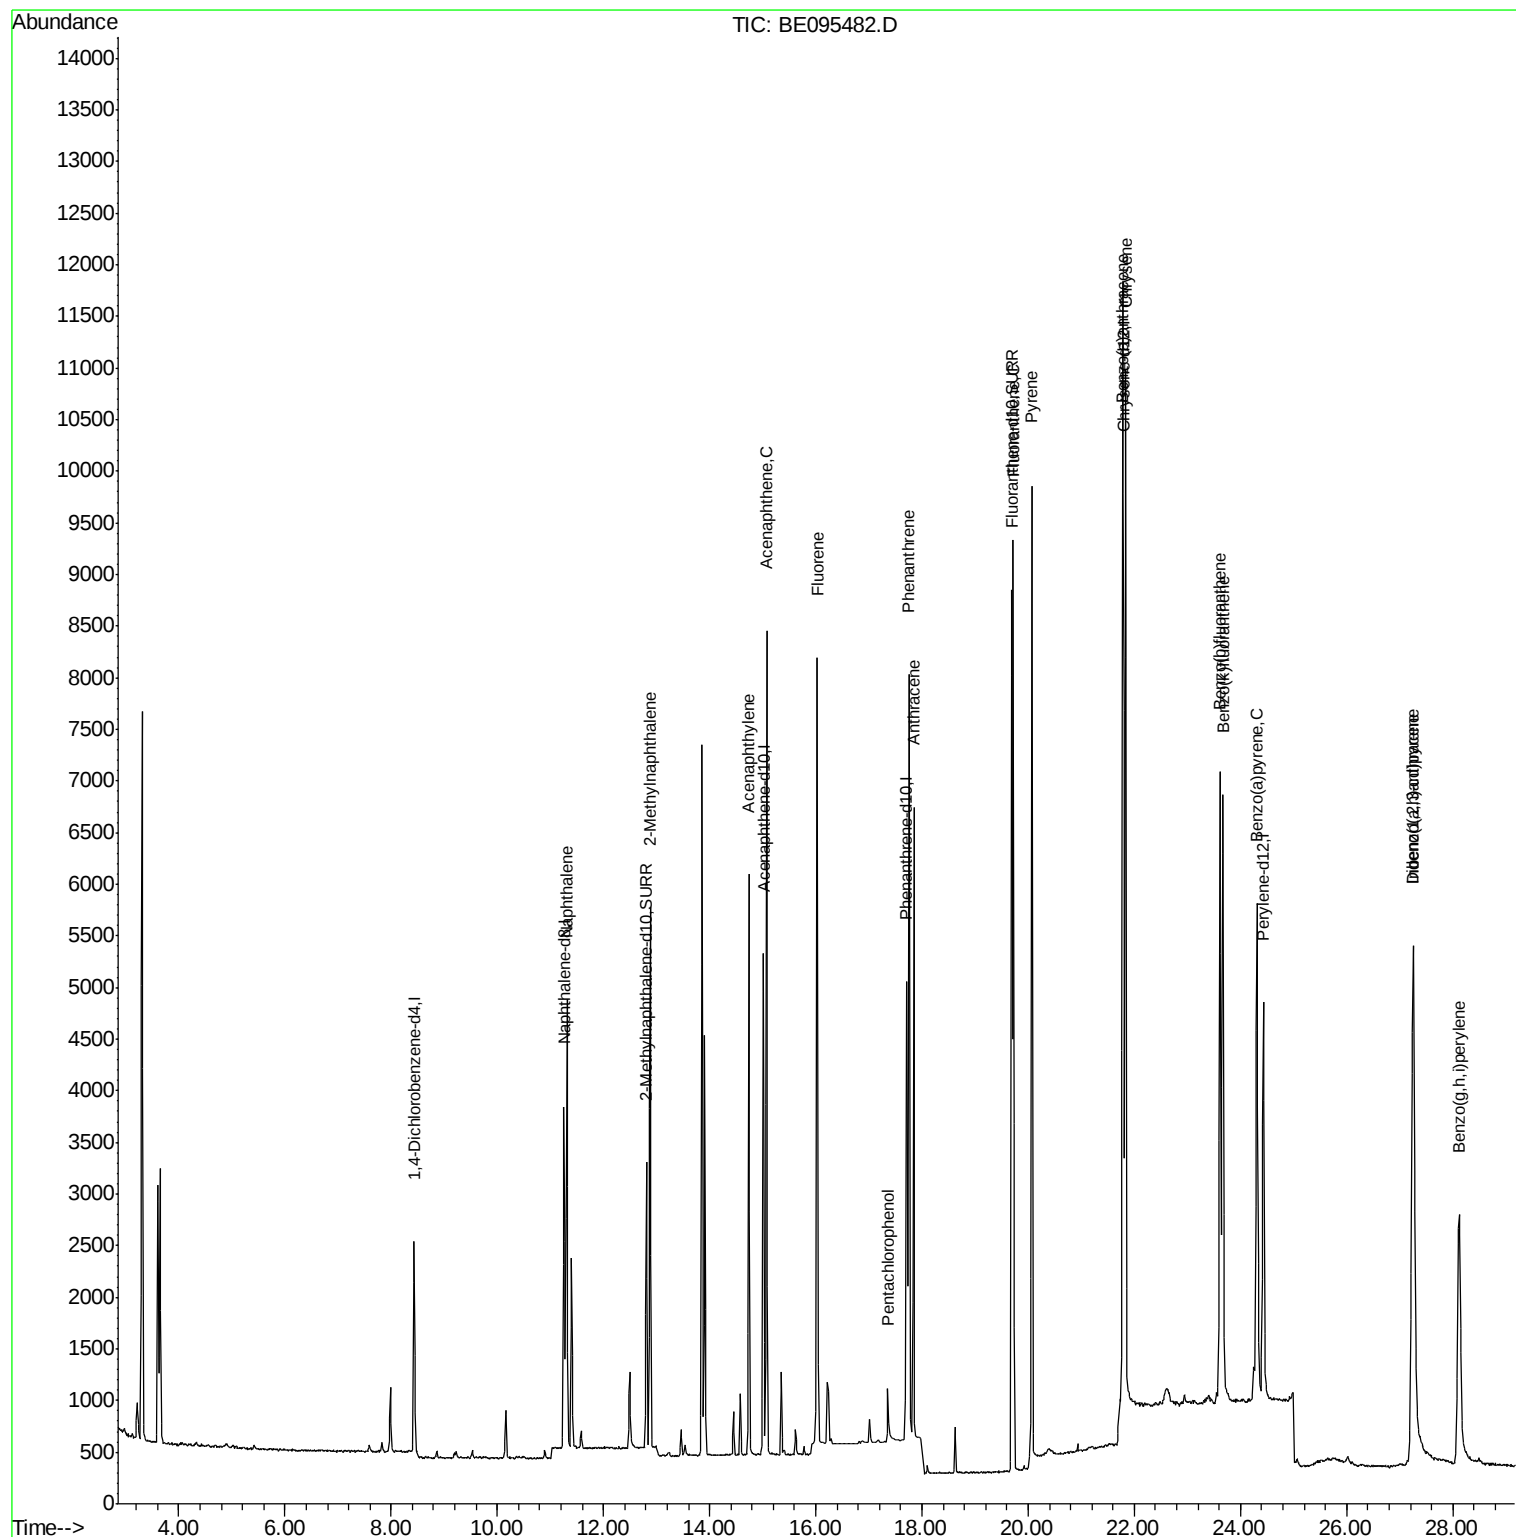

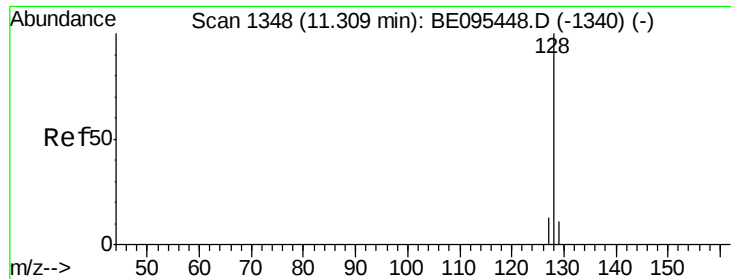

#3

Naphthalene

Concen: 0.471 ng/ul

RT: 11.31 min Scan# 1348

Delta R.T. -0.00 min

Lab File: BE095482.D

Acq: 4 Feb 2018 17:49

Instrument :

BNA_E

ClientSampleId :


Tot Ion:128 Resp: 6080

Ion Ratio Lower Upper

128 100

129 12.6 11.3 16.9




127 14.6 4.0 6.0#



Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

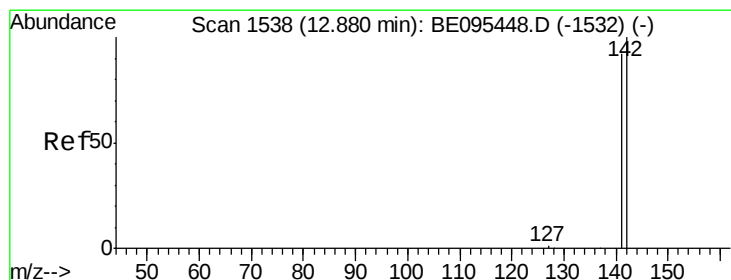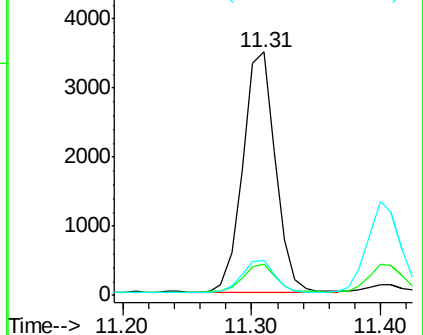

#5

2-Methylnaphthalene

Concen: 0.494 ng/ul

RT: 12.88 min Scan# 1538

Delta R.T. -0.00 min

Lab File: BE095482.D


Acq: 4 Feb 2018 17:49

Tgt Ion:142 Resp: 4258

Ion Ratio Lower Upper



142 100


141 90.0 72.6 108.8



Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

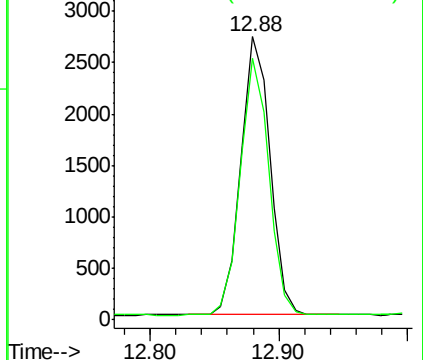



#7

Acenaphthylene

Concen: 0.479 ng/ul

RT: 14.74 min Scan# 1780

Delta R.T. -0.00 min

Lab File: BE095482.D

Acq: 4 Feb 2018 17:49

Instrument :

BNA_E

ClientSampleId :


Tot Ion:152 Resp: 6371

Ion Ratio Lower Upper

152 100

151 21.2 17.1 25.7




153 13.9 12.8 19.2

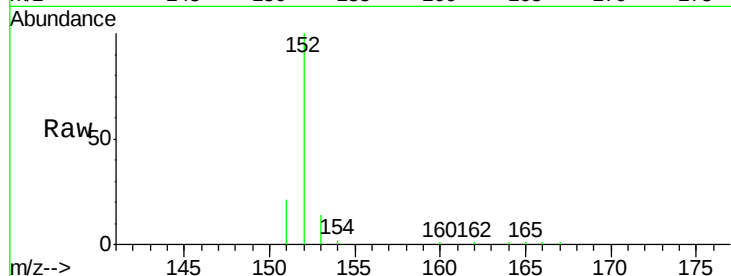

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

Ion 153.00 (152.70 to 153.70): E

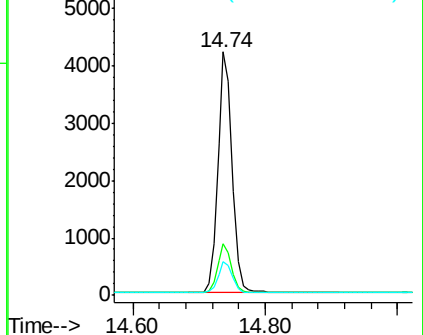

#8

Acenaphthene

Concen: 0.451 ng/ul

RT: 15.08 min Scan# 1825

Delta R.T. -0.00 min

Lab File: BE095482.D

Acq: 4 Feb 2018 17:49


Tgt Ion:153 Resp: 4646

Ion Ratio Lower Upper

153 100

152 48.9 36.0 54.0



154 87.6 72.0 108.0




Abundance Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

Ion 154.00 (153.70 to 154.70): E




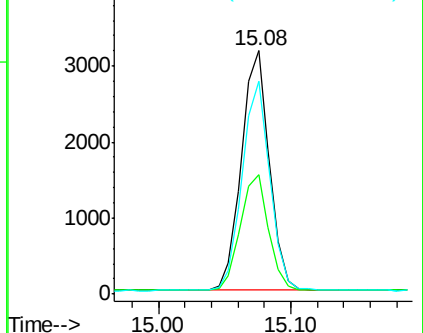


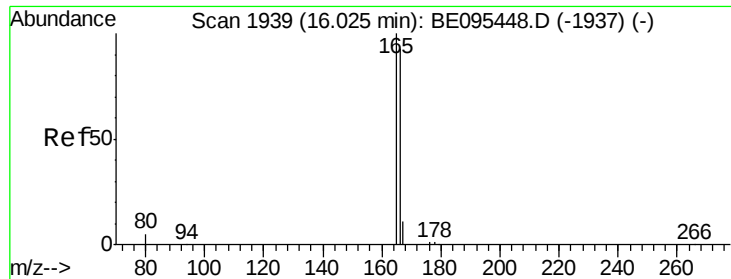

#9
Fluorene
 Concen: 0.496 ng/ul
 RT: 16.02 min Scan# 1939
 Delta R.T. -0.00 min
 Lab File: BE095482.D
 Acq: 4 Feb 2018 17:49




Instrument :
 BNA_E
 ClientSampleId :


Tot Ion:166 Resp: 5272
 Ion Ratio Lower Upper
 166 100
 165 107.3 73.4 110.2
 167 13.6 14.6 22.0#

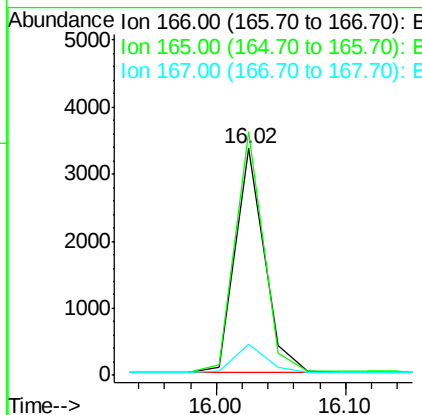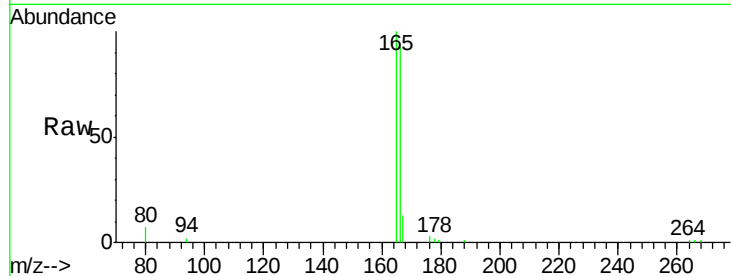

#11
Pentachlorophenol
 Concen: 0.330 ng/ul
 RT: 17.36 min Scan# 1997
 Delta R.T. -0.00 min
 Lab File: BE095482.D
 Acq: 4 Feb 2018 17:49

Tgt Ion:266 Resp: 402
 Ion Ratio Lower Upper
 266 100
 264 60.2 47.9 71.9
 268 64.9 49.8 74.8

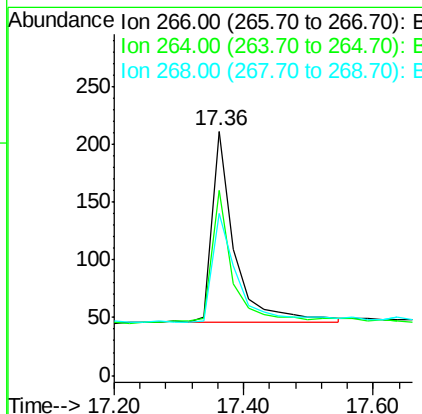



#12

Phenanthrene

Concen: 0.409 ng/ul

RT: 17.75 min Scan# 2014

Delta R.T. -0.00 min

Lab File: BE095482.D

Acq: 4 Feb 2018 17:49

Instrument :

BNA_E

ClientSampleId :


Tot Ion:178 Resp: 8648

Ion Ratio Lower Upper

178 100

179 16.7 18.4 27.6#




176 18.5 13.6 20.4

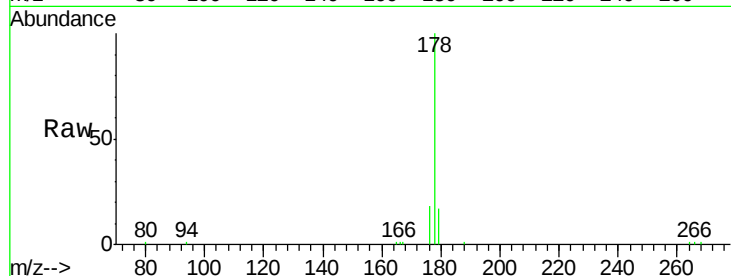

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

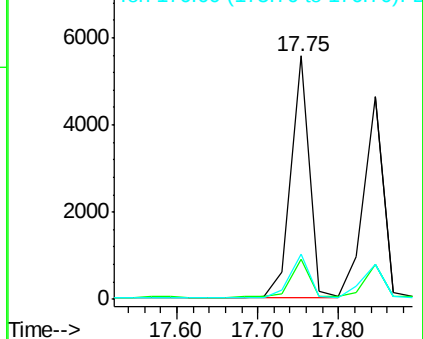

#13

Anthracene

Concen: 0.403 ng/ul

RT: 17.85 min Scan# 2018

Delta R.T. -0.00 min

Lab File: BE095482.D

Acq: 4 Feb 2018 17:49


Tgt Ion:178 Resp: 7799

Ion Ratio Lower Upper

178 100

179 17.4 18.1 27.1#



176 17.3 14.7 22.1




Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

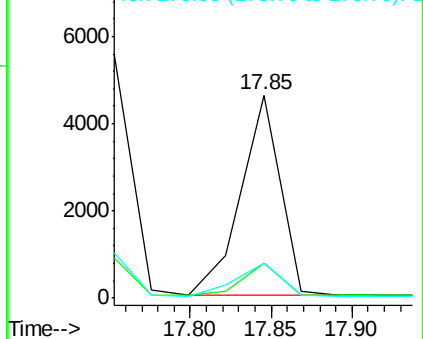

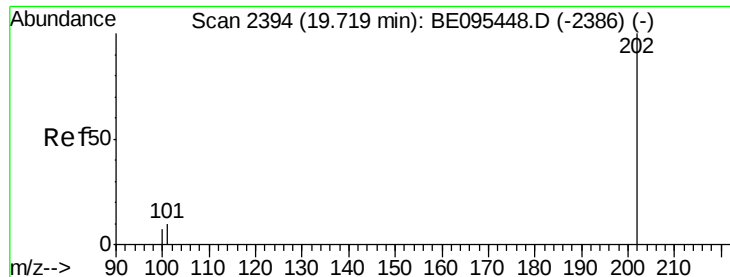

#15

Fluoranthene

Concen: 0.373 ng/ul

RT: 19.72 min Scan# 2394

Delta R.T. 0.00 min

Lab File: BE095482.D

Acq: 4 Feb 2018 17:49

Instrument :

BNA_E

ClientSampleId :


Tot Ion:202 Resp: 10219

Ion Ratio Lower Upper

202 100

101 10.9 0.0 30.3




100 9.1 0.0 39.5

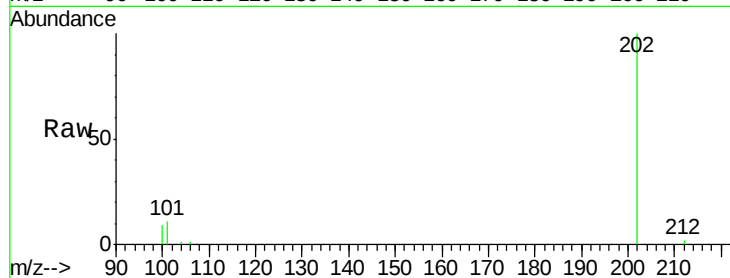

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): BE

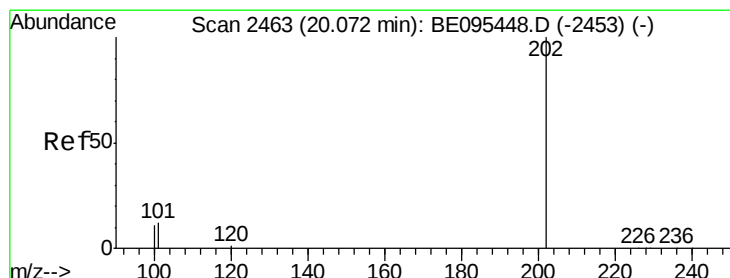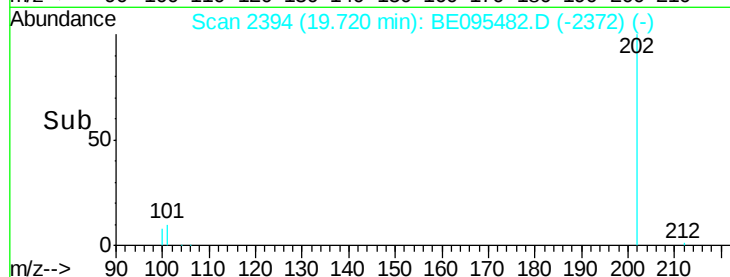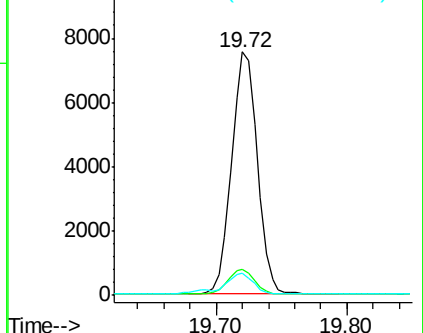

#17

Pyrene

Concen: 0.478 ng/ul

RT: 20.07 min Scan# 2463

Delta R.T. -0.00 min

Lab File: BE095482.D

Acq: 4 Feb 2018 17:49


Tgt Ion:202 Resp: 10676

Ion Ratio Lower Upper

202 100

101 12.6 18.2 27.4#



100 11.1 15.6 23.4#

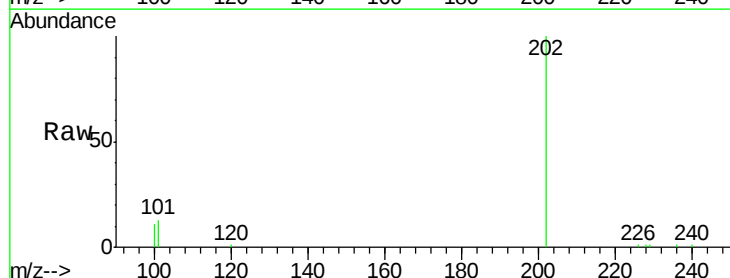


Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): BE

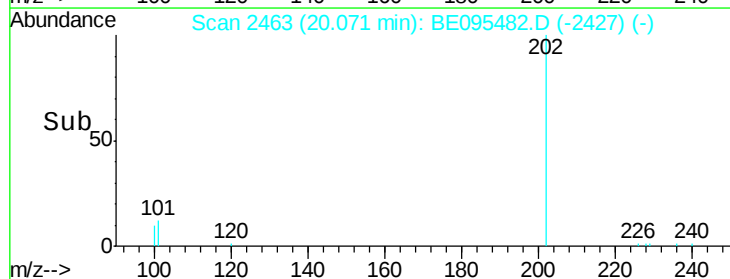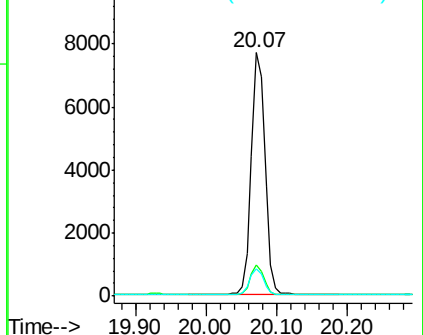

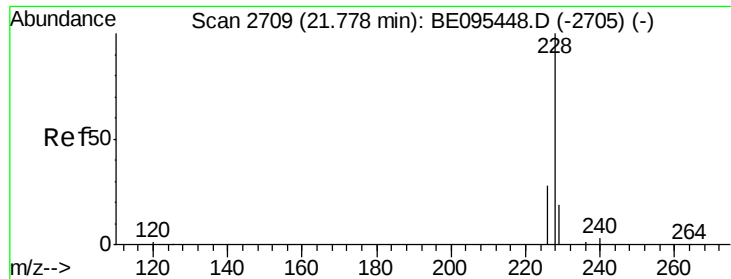

#18

Benzo(a)anthracene

Concen: 0.464 ng/ul

RT: 21.78 min Scan# 2709

Delta R.T. -0.00 min

Lab File: BE095482.D

Acq: 4 Feb 2018 17:49

Instrument :

BNA_E

ClientSampleId :


Tot Ion:228 Resp: 9665

Ion Ratio Lower Upper

228 100

229 19.7 22.8 34.2#




226 28.8 17.0 25.6#

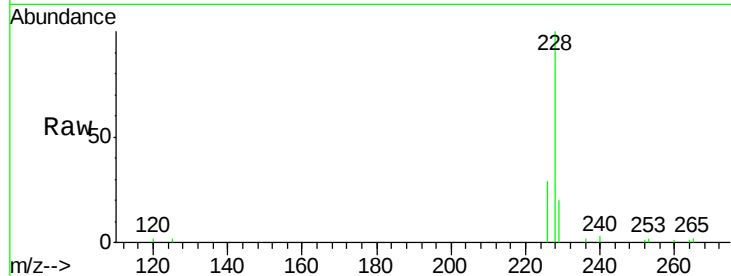

Abundance Ion 228.00 (227.70 to 228.70): E

Ion 229.00 (228.70 to 229.70): E

Ion 226.00 (225.70 to 226.70): E

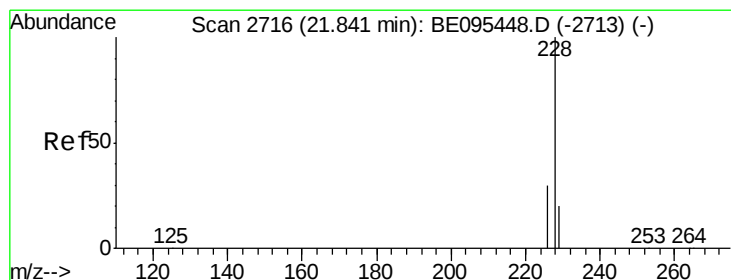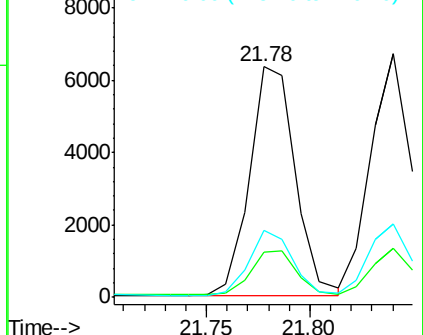

#19

Chrysene

Concen: 0.432 ng/ul

RT: 21.84 min Scan# 2716

Delta R.T. -0.00 min

Lab File: BE095482.D

Acq: 4 Feb 2018 17:49


Tgt Ion:228 Resp: 9330

Ion Ratio Lower Upper

228 100

226 30.1 23.4 35.0



229 20.3 17.7 26.5




Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

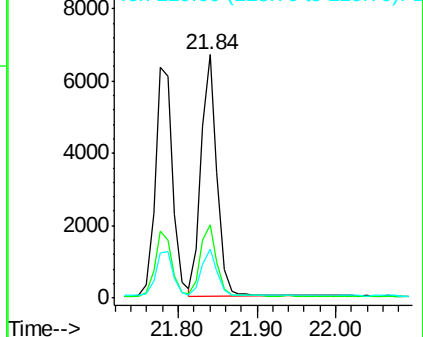



#21

Benzo(b)fluoranthene

Concen: 0.418 ng/ul

RT: 23.62 min Scan# 2913

Delta R.T. -0.00 min

Lab File: BE095482.D

Acq: 4 Feb 2018 17:49

Instrument :

BNA_E

ClientSampleId :


Tot Ion:252 Resp: 9232

Ion Ratio Lower Upper




252 100

253 23.5 0.0 64.2

125 11.0 0.0 35.0

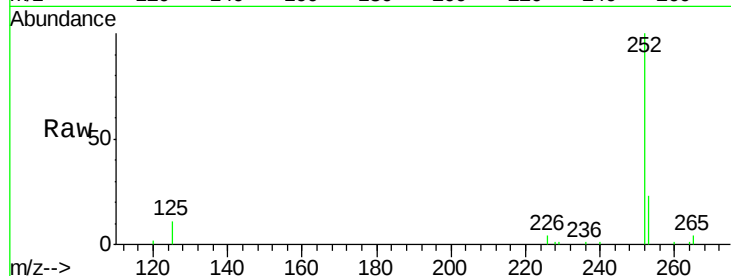

Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

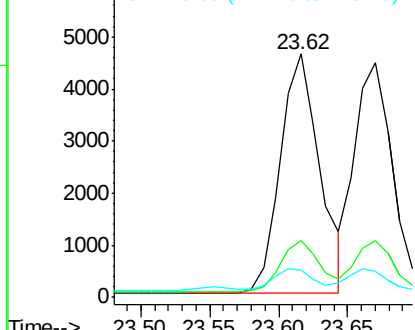

#22

Benzo(k)fluoranthene

Concen: 0.425 ng/ul

RT: 23.67 min Scan# 2919

Delta R.T. -0.00 min

Lab File: BE095482.D

Acq: 4 Feb 2018 17:49


Tgt Ion:252 Resp: 8587

Ion Ratio Lower Upper



252 100


253 24.5 24.5 36.7#

125 10.9 13.7 20.5#



Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

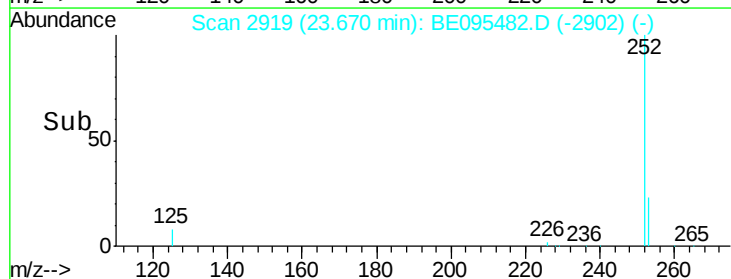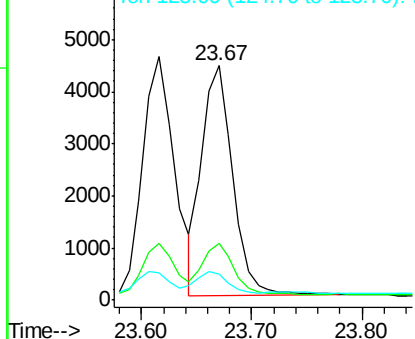

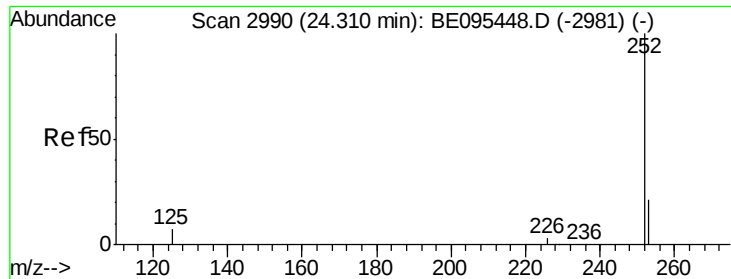

#23

Benzo(a)pyrene

Concen: 0.431 ng/ul

RT: 24.31 min Scan# 2990

Delta R.T. -0.00 min

Lab File: BE095482.D

Acq: 4 Feb 2018 17:49

Instrument :

BNA_E

ClientSampleId :


Tot Ion:252 Resp: 8498

Ion Ratio Lower Upper

252 100

253 23.4 28.5 42.7#




125 14.1 18.1 27.1#

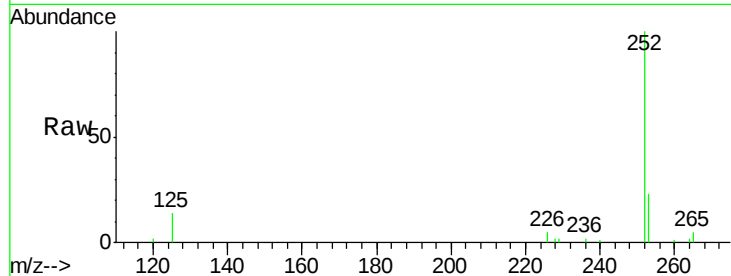

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

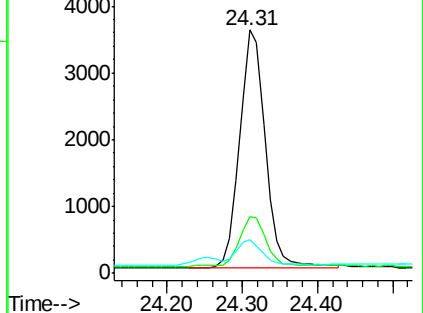

#24

Indeno(1,2,3-cd)pyrene

Concen: 0.408 ng/ul

RT: 27.25 min Scan# 3553

Delta R.T. 0.01 min

Lab File: BE095482.D

Acq: 4 Feb 2018 17:49


Tgt Ion:276 Resp: 8832

Ion Ratio Lower Upper

276 100

138 22.6 28.0 42.0#



227 0.0 8.0 12.0#




Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 227.00 (226.70 to 227.70): E

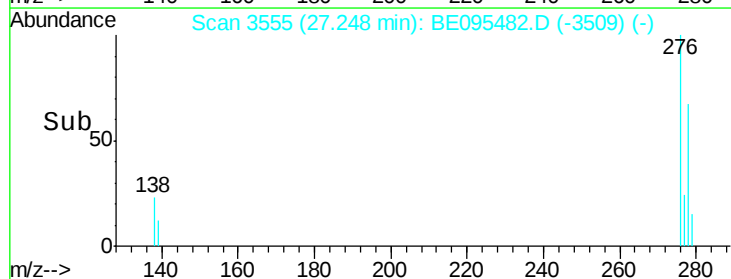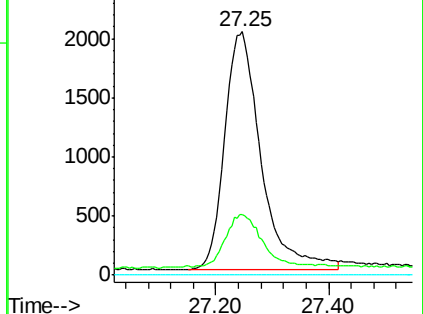

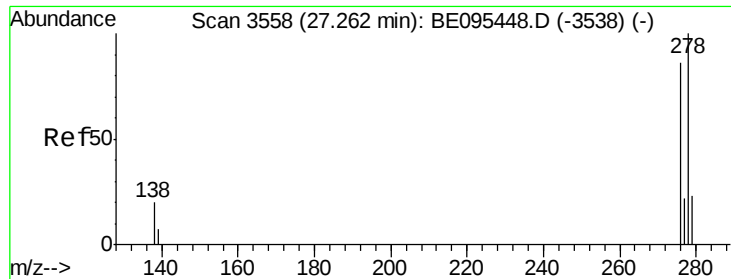

#25

Dibenzo(a,h)anthracene

Concen: 0.401 ng/ul

RT: 27.26 min Scan# 3558

Delta R.T. -0.00 min

Lab File: BE095482.D

Acq: 4 Feb 2018 17:49

Instrument :

BNA_E

ClientSampleId :


Tot Ion:278 Resp: 7100

Ion Ratio Lower Upper

278 100

139 22.7 17.4 26.0




279 26.6 25.9 38.9

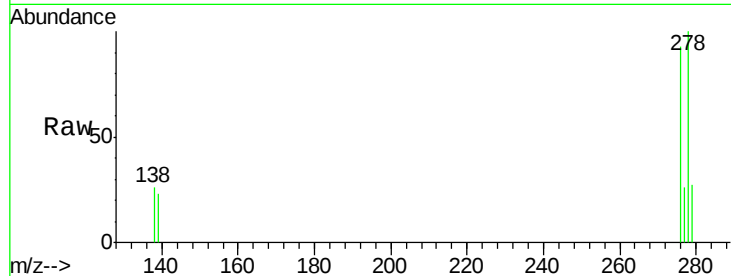

Abundance Ion 278.00 (277.70 to 278.70): E

Ion 139.00 (138.70 to 139.70): E

Ion 279.00 (278.70 to 279.70): E

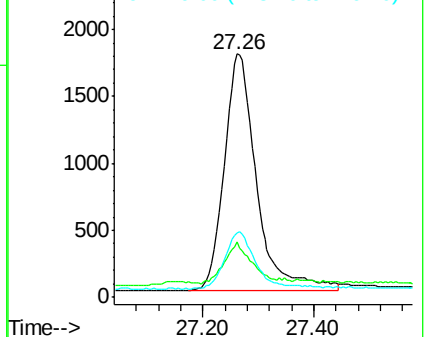

#26

Benzo(g,h,i)perylene

Concen: 0.407 ng/ul

RT: 28.12 min Scan# 3747

Delta R.T. 0.00 min

Lab File: BE095482.D

Acq: 4 Feb 2018 17:49


Tgt Ion:276 Resp: 7457

Ion Ratio Lower Upper

276 100

138 22.8 21.8 32.8

277 25.3 20.5 30.7



Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

