




Data Path : Z:\HPCHEM1\BNA E\DATA\BE020318\
Data File : BE095444.D
Acq On : 3 Feb 2018 19:11
Operator : SJ/JU
Sample : PB106121BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK21

Manual Integrations
APPROVED

Sohil
2/5/2018 7:02:12 PM

Quant Time: Feb 05 03:35:02 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 05 03:32:57 2018
Response via : Initial Calibration

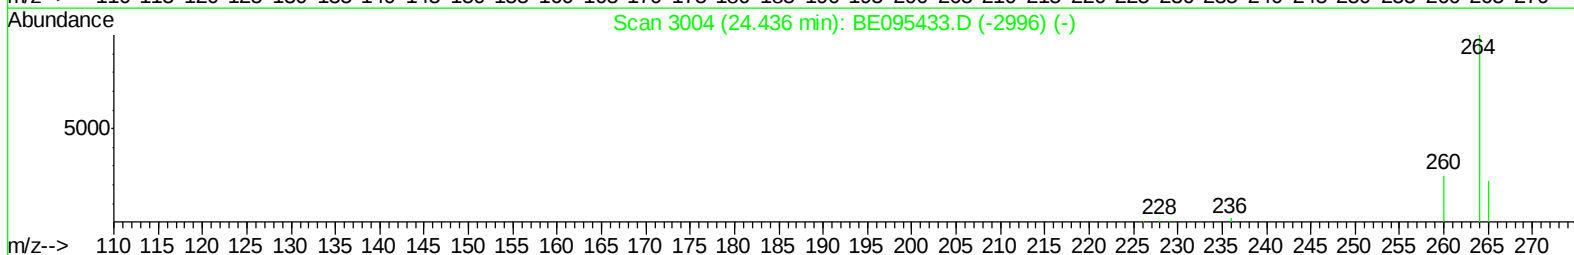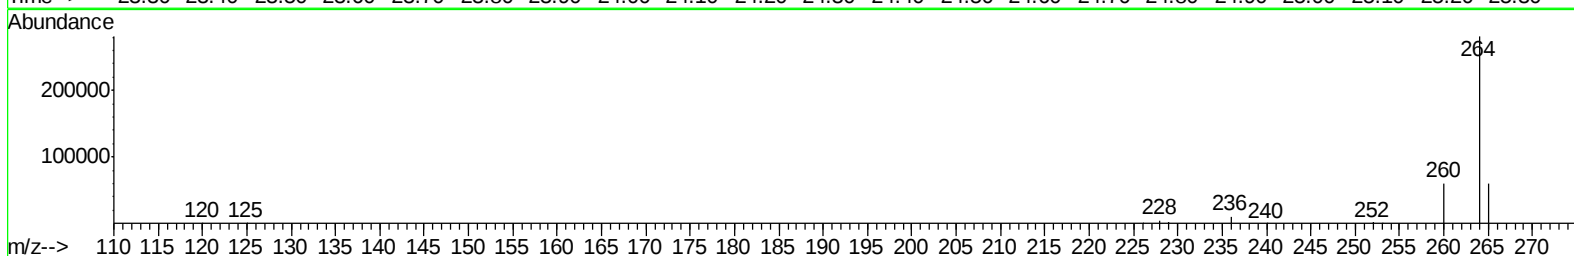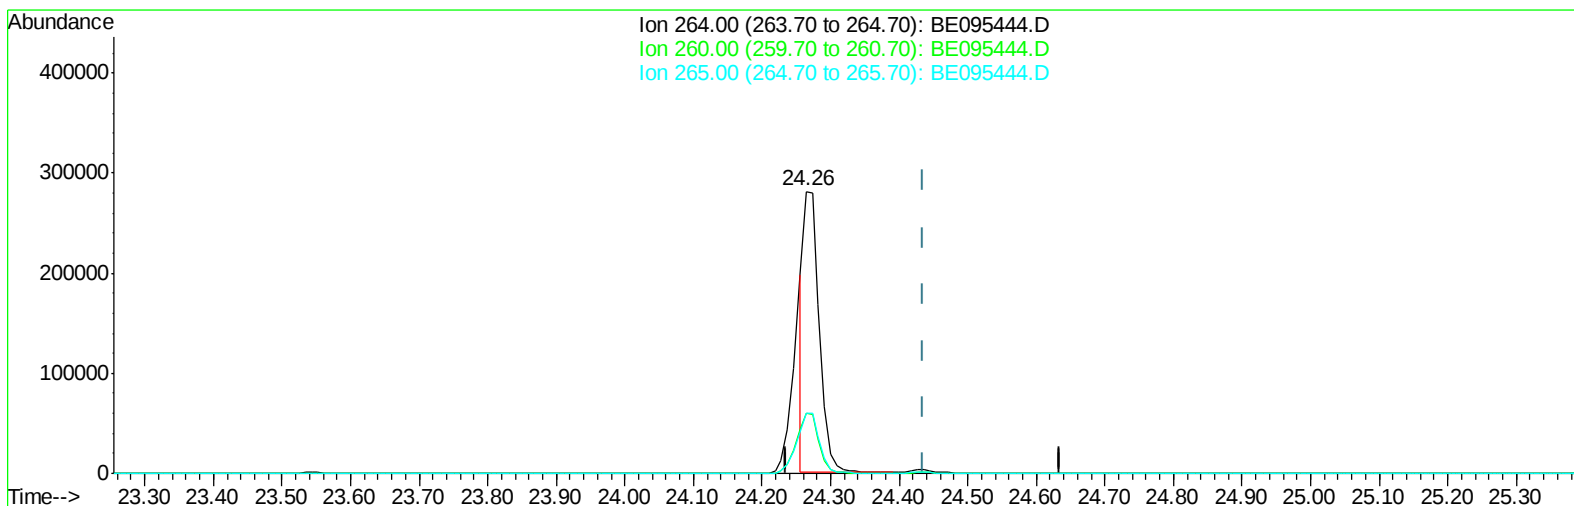

TIC: BE095444.D

(20) Perylene-d12 (I)

24.264min (-0.171) 0.40ng/ul

response 446325

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	21.45#
265.00	103.50	21.19#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA E\DATA\BE020318\
Data File : BE095444.D
Acq On : 3 Feb 2018 19:11
Operator : SJ/JU
Sample : PB106121BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK21

Manual Integrations
APPROVED

Sohil
2/5/2018 7:02:12 PM

Quant Time: Feb 05 03:35:02 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 05 03:32:57 2018
Response via : Initial Calibration

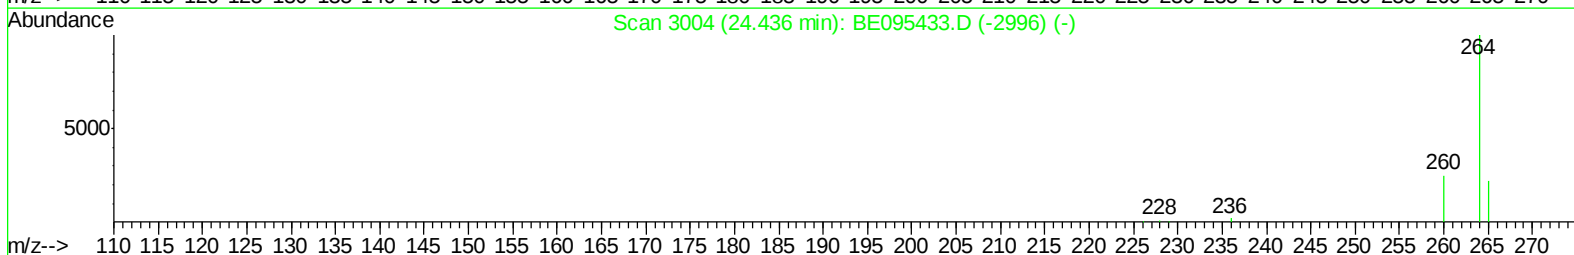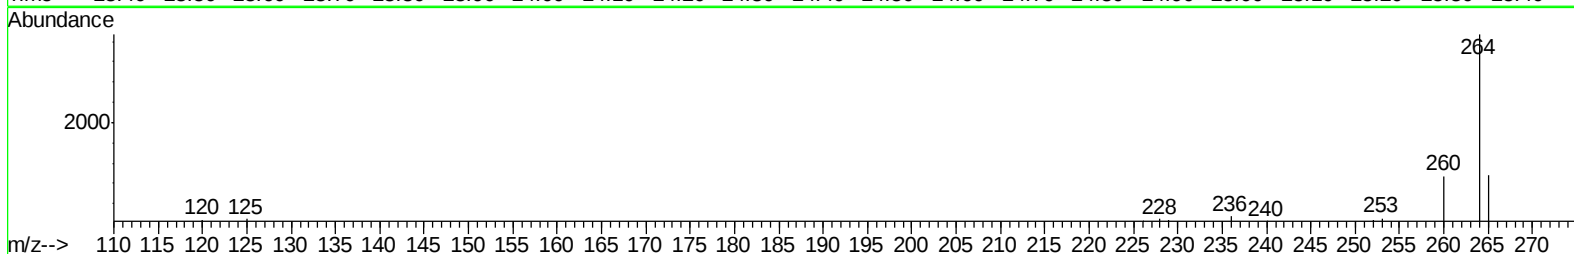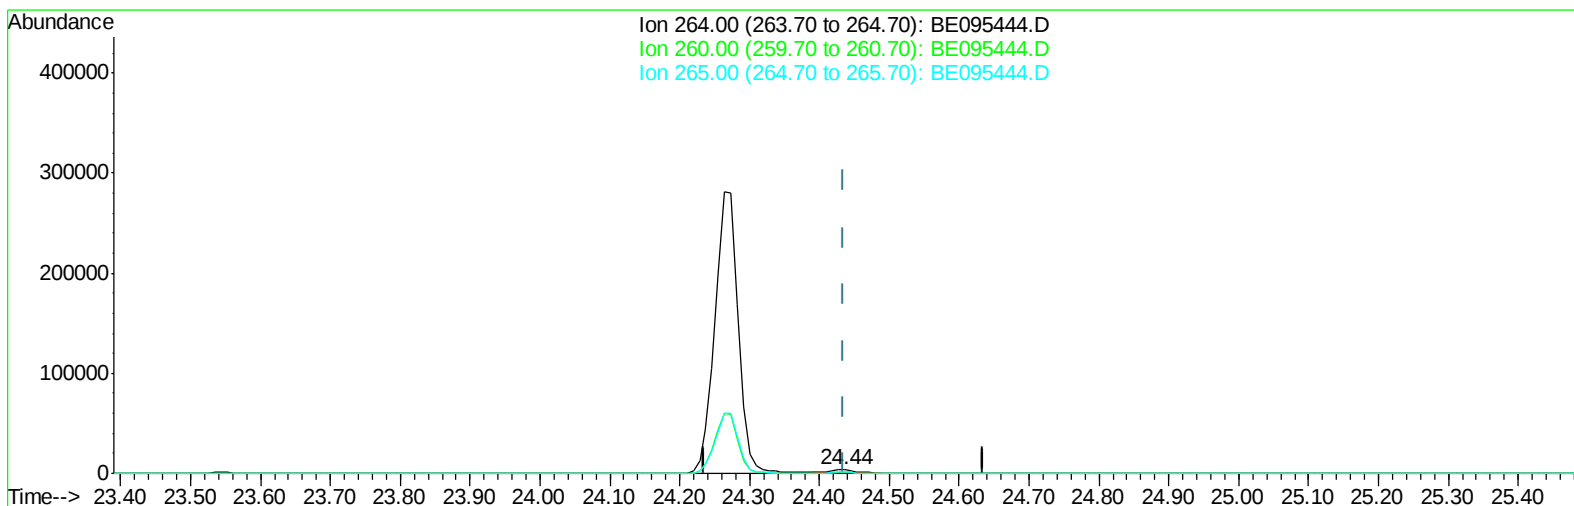

TIC: BE095444.D

(20) Perylene-d12 (I)

24.435min (-0.000) 0.40ng/ul m

response 6646

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	25.09
265.00	103.50	25.54#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020318\
 Data File : BE095444.D
 Acq On : 3 Feb 2018 19:11
 Operator : SJ/JU
 Sample : PB106121BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 SBLK21

Manual Integrations
 APPROVED

Sohil
 2/5/2018 7:02:12 PM

Quant Time: Feb 05 04:38:04 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 05 03:32:57 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.44	152	1848	0.40	ng/ul	0.00
2) Naphthalene-d8	11.26	136	5508	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.02	164	3534	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	7552	0.40	ng/ul	0.00
16) Chrysene-d12	21.80	240	7270	0.40	ng/ul	0.00
20) Perylene-d12	24.44	264	6646m	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.81	152	3273	0.36	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	8954	0.31	ng/ul	0.00

Target Compounds	Ovalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020318\
Data File : BE095444.D
Acq On : 3 Feb 2018 19:11
Operator : SJ/JU
Sample : PB106121BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
SBLK21

Manual Integrations
APPROVED

Sohil
2/5/2018 7:02:12 PM

Quant Time: Feb 05 04:38:04 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 05 03:32:57 2018
Response via : Initial Calibration

