




Data Path : Z:\HPCHEM1\BNA E\DATA\BE020318\
Data File : BE095453.D
Acq On : 4 Feb 2018 00:33
Operator : SJ/JU
Sample : J1296-04
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F6C22

Manual Integrations
APPROVED

Sohil
2/5/2018 7:02:35 PM

Quant Time: Feb 05 04:53:12 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 05 04:46:10 2018
Response via : Initial Calibration

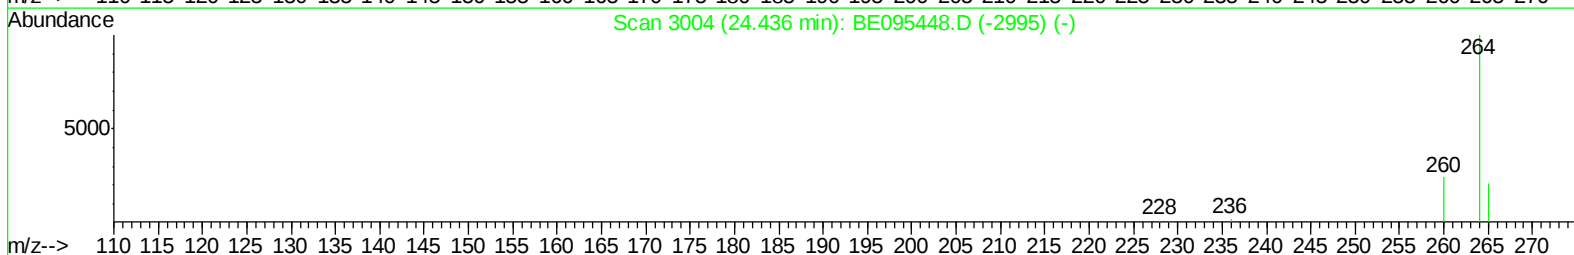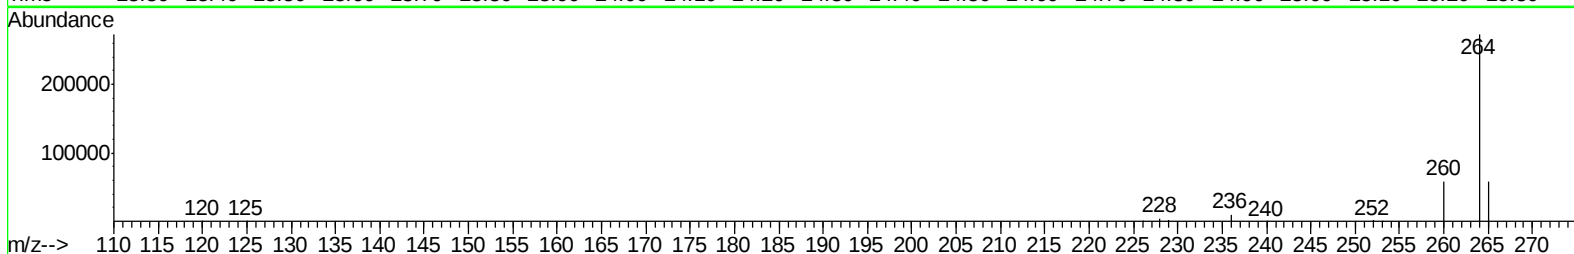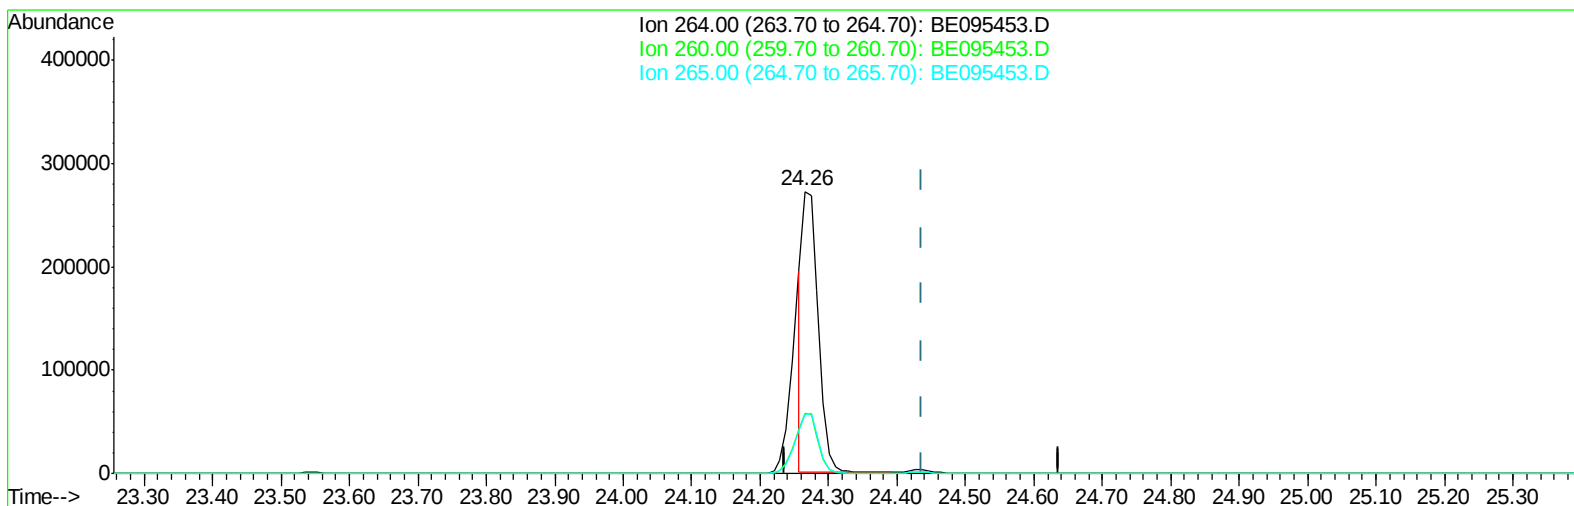

TIC: BE095453.D

(20) Perylene-d12 (I)

24.265min (-0.171) 0.40ng/ul

response 439454

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	21.54#
265.00	103.50	21.07#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA E\DATA\BE020318\
Data File : BE095453.D
Acq On : 4 Feb 2018 00:33
Operator : SJ/JU
Sample : J1296-04
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F6C22

Manual Integrations
APPROVED

Sohil
2/5/2018 7:02:35 PM

Quant Time: Feb 05 04:53:12 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 05 04:46:10 2018
Response via : Initial Calibration

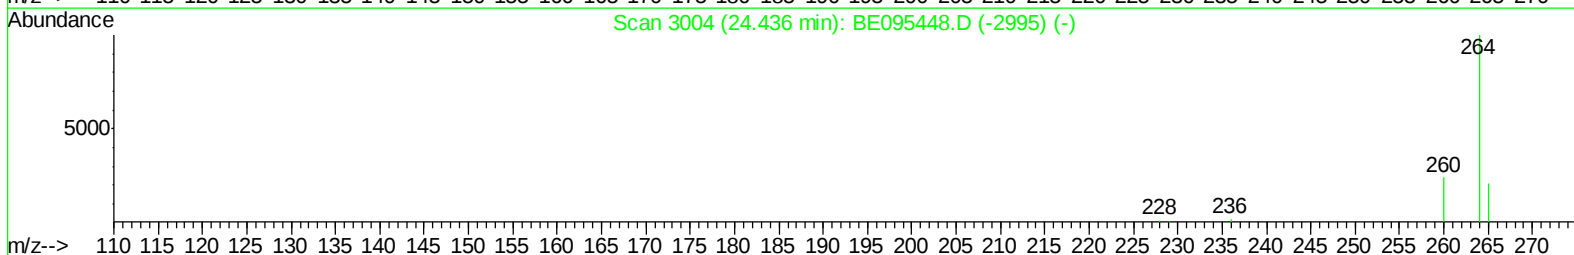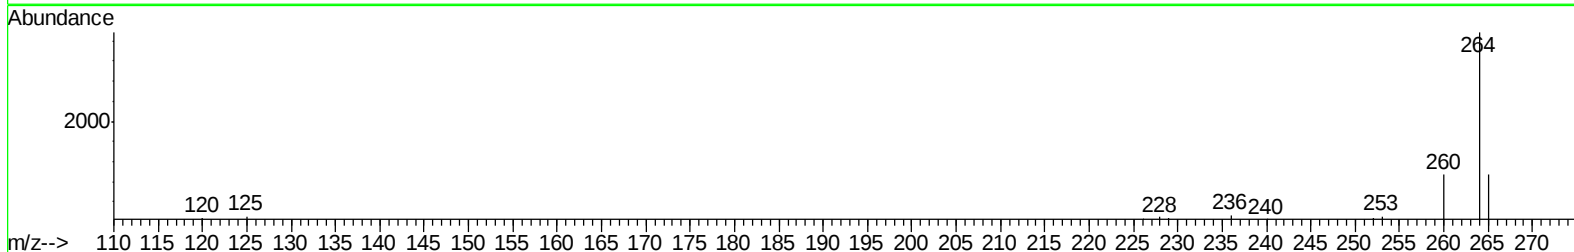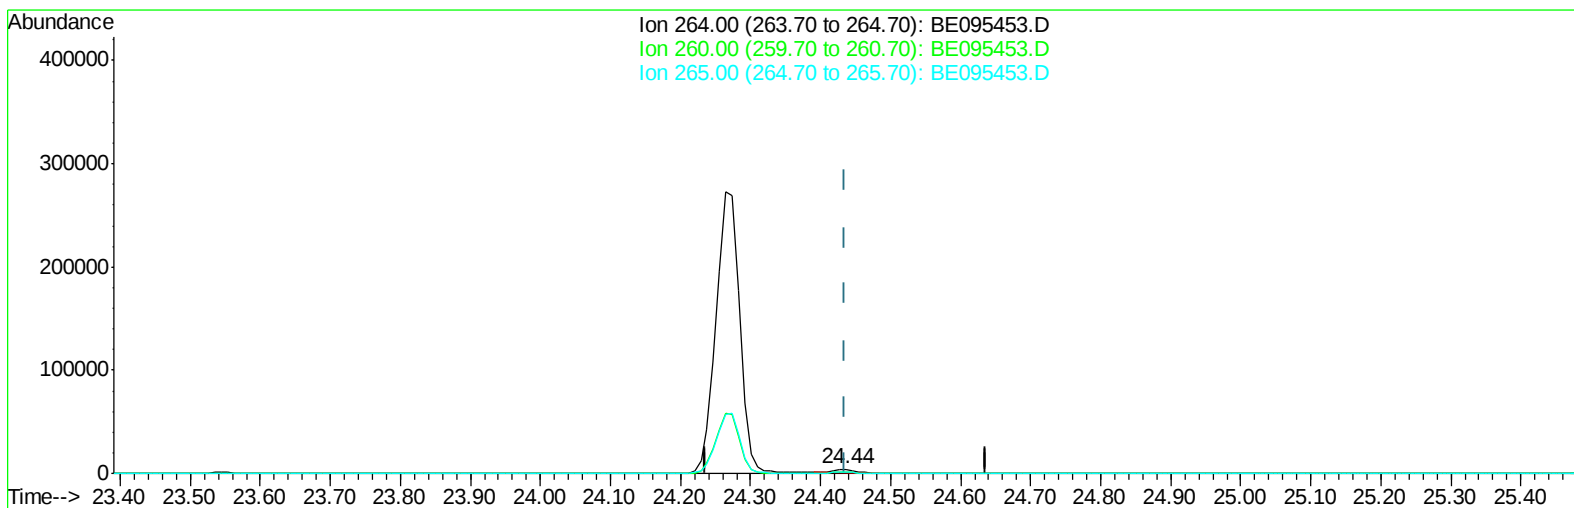

TIC: BE095453.D

(20) Perylene-d12 (I)

24.436min (+0.000) 0.40ng/ul m

response 6960

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	25.03
265.00	103.50	25.32#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020318\
 Data File : BE095453.D
 Acq On : 4 Feb 2018 00:33
 Operator : SJ/JU
 Sample : J1296-04
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 F6C22

Manual Integrations
 APPROVED

Sohil
 2/5/2018 7:02:35 PM

Quant Time: Feb 05 06:05:34 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 05 04:46:10 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.43	152	1843	0.40	ng/ul	0.00
2) Naphthalene-d8	11.26	136	5751	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.02	164	3765	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	7932	0.40	ng/ul	0.00
16) Chrysene-d12	21.80	240	7726	0.40	ng/ul	0.00
20) Perylene-d12	24.44	264	6960m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	3635	0.39	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	9143	0.30	ng/ul	0.00
Target Compounds						
3) Naphthalene	11.31	128	3844	0.239	ng/ul#	89
11) Pentachlorophenol	17.36	266	11385	7.411	ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020318\
Data File : BE095453.D
Acq On : 4 Feb 2018 00:33
Operator : SJ/JU
Sample : J1296-04
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F6C22

Manual Integrations
APPROVED

Sohil
2/5/2018 7:02:35 PM

Quant Time: Feb 05 06:05:34 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 05 04:46:10 2018
Response via : Initial Calibration

