




Data Path : Z:\HPCHEM1\BNA E\DATA\BE020318\  
Data File : BE095467.D  
Acq On : 4 Feb 2018 8:52  
Operator : SJ/JU  
Sample : J1315-19  
Misc :  
ALS Vial : 36 Sample Multiplier: 1

Instrument :  
BNA\_E  
ClientSampleId :  
F6C82

Manual Integrations  
APPROVED

Sohil  
2/5/2018 7:01:01 PM

Quant Time: Feb 05 06:46:21 2018  
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Feb 05 04:46:10 2018  
Response via : Initial Calibration

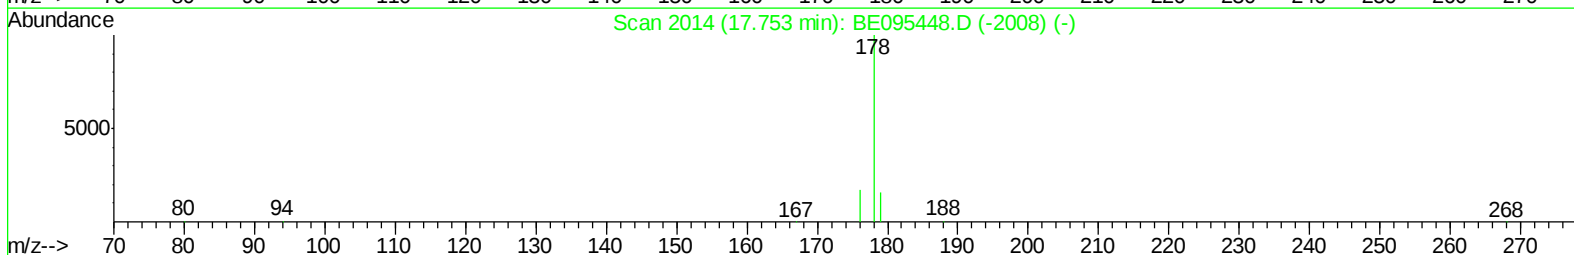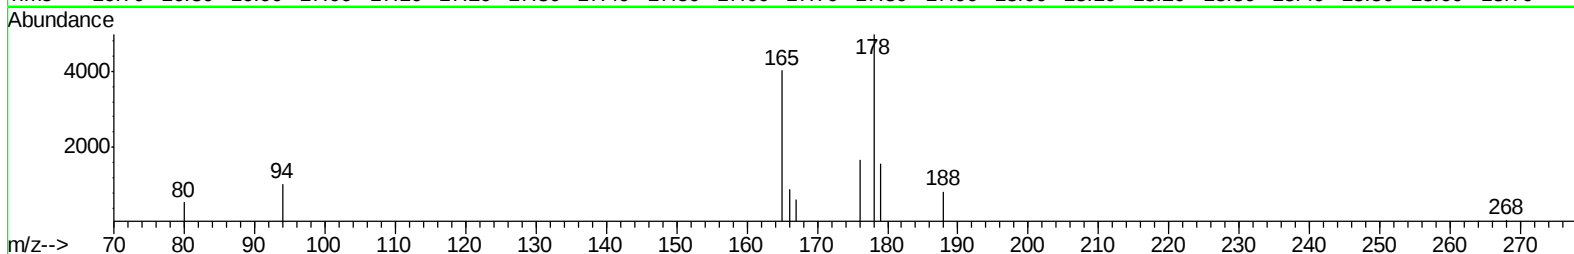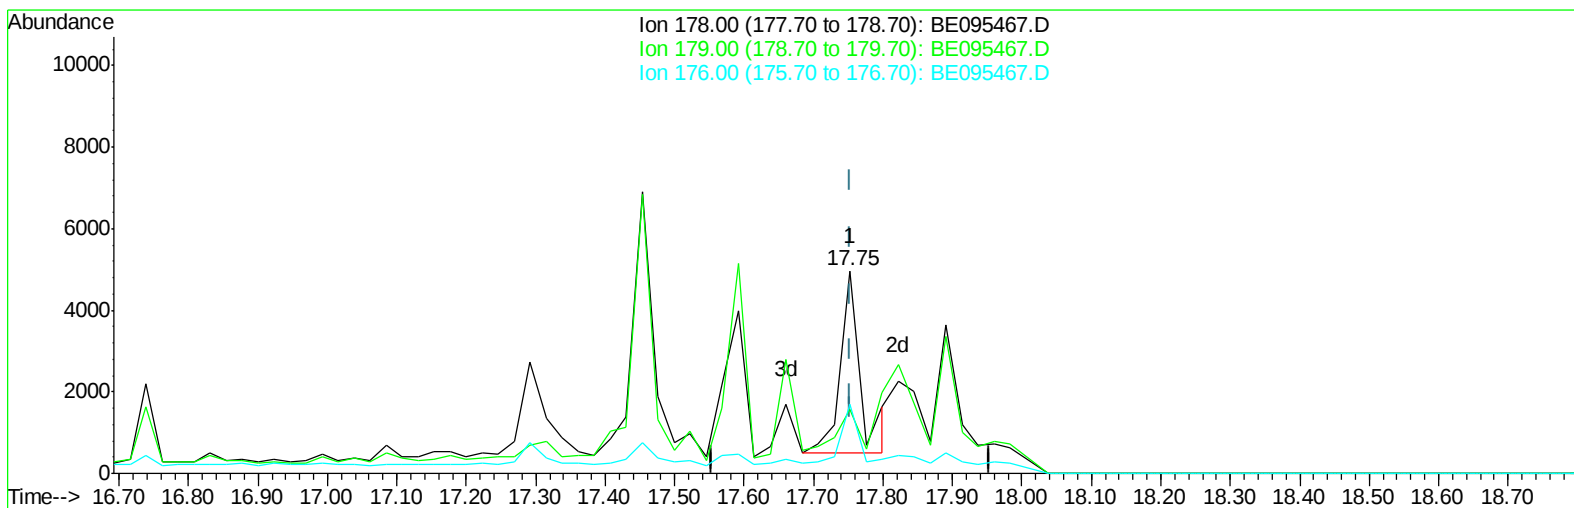

TIC: BE095467.D

(12) Phenanthrene

17.752min (-0.001) 0.35ng/ul

response 9362

| Ion    | Exp%  | Act%   |
|--------|-------|--------|
| 178.00 | 100   | 100    |
| 179.00 | 23.00 | 31.70# |
| 176.00 | 17.00 | 33.96# |
| 0.00   | 0.00  | 0.00   |




Data Path : Z:\HPCHEM1\BNA E\DATA\BE020318\  
Data File : BE095467.D  
Acq On : 4 Feb 2018 8:52  
Operator : SJ/JU  
Sample : J1315-19  
Misc :  
ALS Vial : 36 Sample Multiplier: 1

Instrument :  
BNA\_E  
ClientSampleId :  
F6C82

Manual Integrations  
APPROVED

Sohil  
2/5/2018 7:01:01 PM

Quant Time: Feb 05 06:46:21 2018  
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Feb 05 04:46:10 2018  
Response via : Initial Calibration

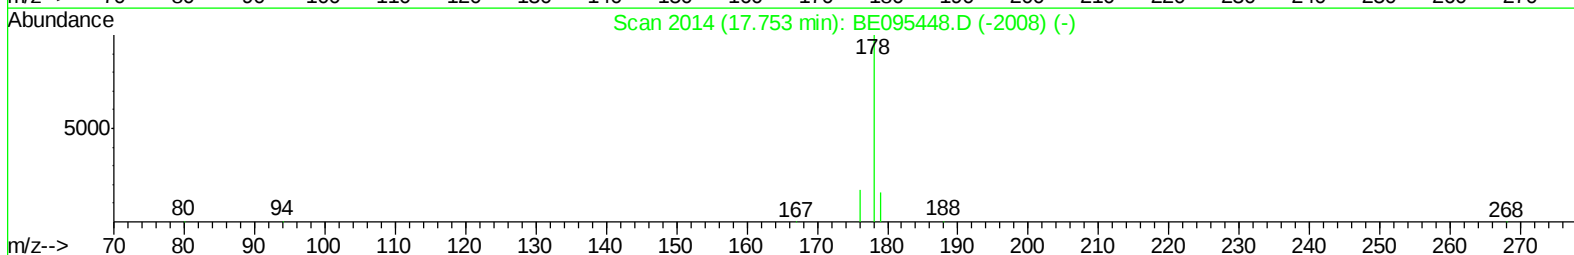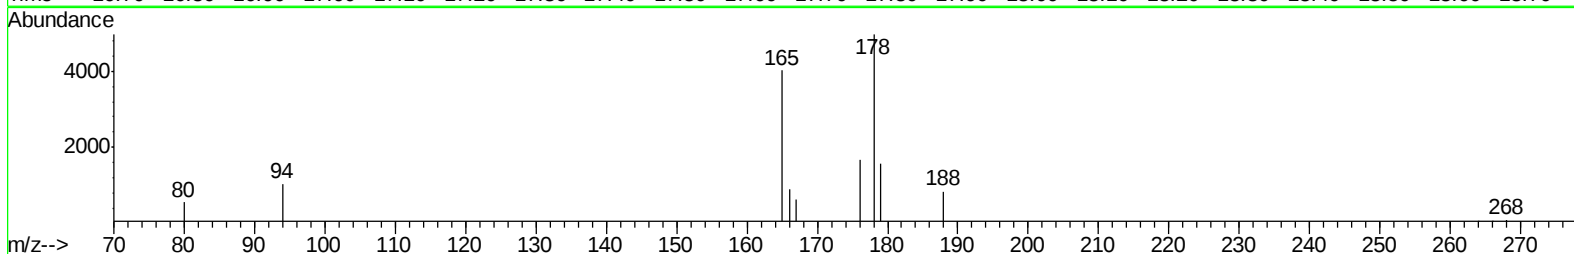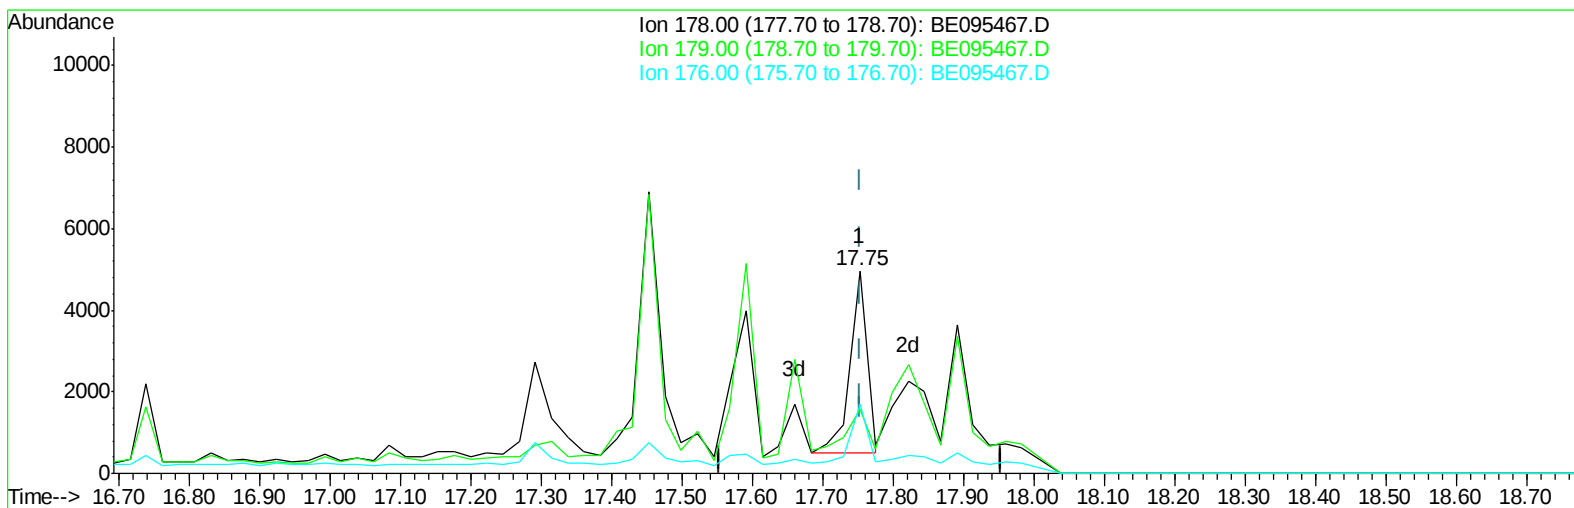

TIC: BE095467.D

(12) Phenanthrene

17.752min (-0.001) 0.29ng/ul m

response 7771

| Ion    | Exp%  | Act%   |
|--------|-------|--------|
| 178.00 | 100   | 100    |
| 179.00 | 23.00 | 31.70# |
| 176.00 | 17.00 | 33.96# |
| 0.00   | 0.00  | 0.00   |




Data Path : Z:\HPCHEM1\BNA E\DATA\BE020318\  
Data File : BE095467.D  
Acq On : 4 Feb 2018 8:52  
Operator : SJ/JU  
Sample : J1315-19  
Misc :  
ALS Vial : 36 Sample Multiplier: 1

Instrument :  
BNA\_E  
ClientSampleId :  
F6C82

Manual Integrations  
APPROVED

Sohil  
2/5/2018 7:01:01 PM

Quant Time: Feb 05 06:46:21 2018  
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Feb 05 04:46:10 2018  
Response via : Initial Calibration

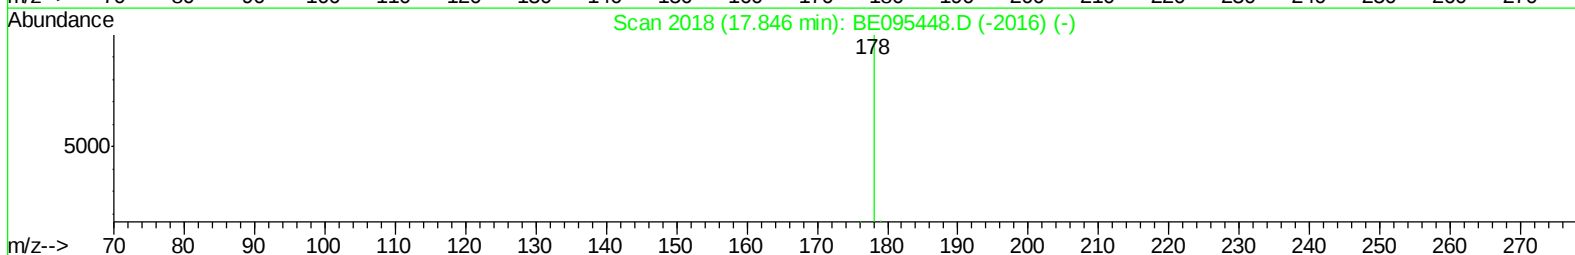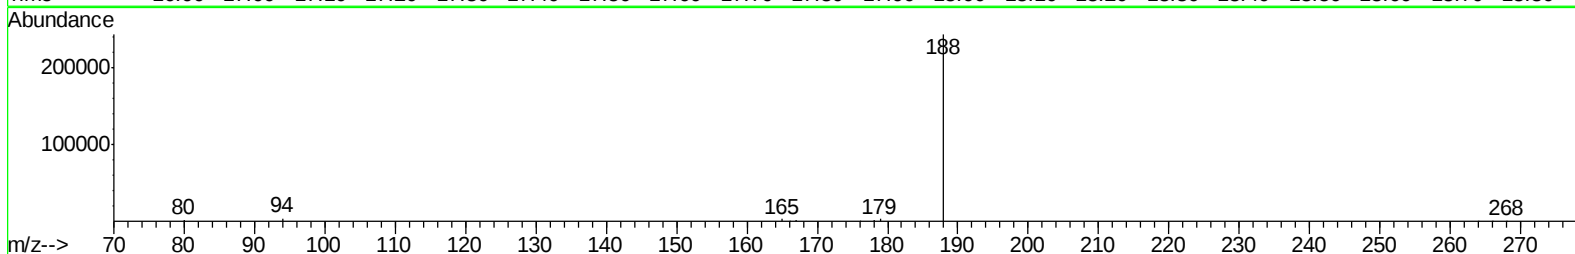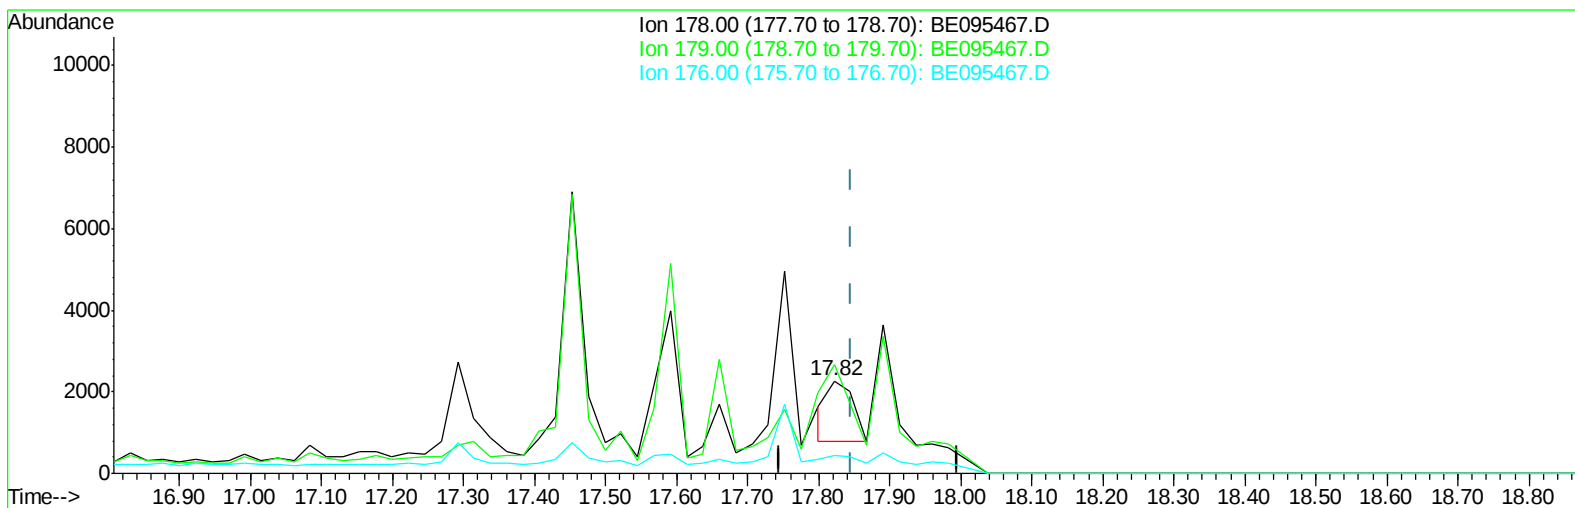

TIC: BE095467.D

(13) Anthracene

17.821min (-0.024) 0.15ng/ul

response 3761

| Ion    | Exp%  | Act%    |
|--------|-------|---------|
| 178.00 | 100   | 100     |
| 179.00 | 22.60 | 117.93# |
| 176.00 | 18.40 | 19.74   |
| 0.00   | 0.00  | 0.00    |




Data Path : Z:\HPCHEM1\BNA E\DATA\BE020318\  
Data File : BE095467.D  
Acq On : 4 Feb 2018 8:52  
Operator : SJ/JU  
Sample : J1315-19  
Misc :  
ALS Vial : 36 Sample Multiplier: 1

Instrument :  
BNA\_E  
ClientSampleId :  
F6C82

Manual Integrations  
APPROVED

Sohil  
2/5/2018 7:01:01 PM

Quant Time: Feb 05 06:46:21 2018  
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Feb 05 04:46:10 2018  
Response via : Initial Calibration

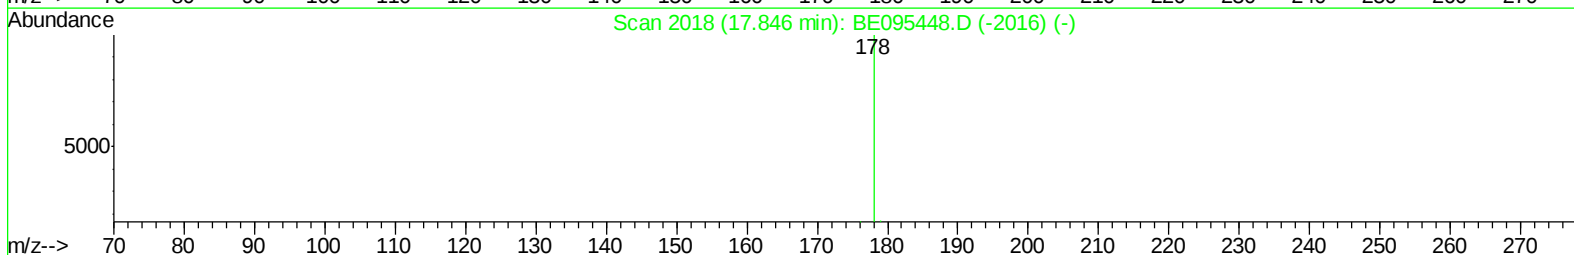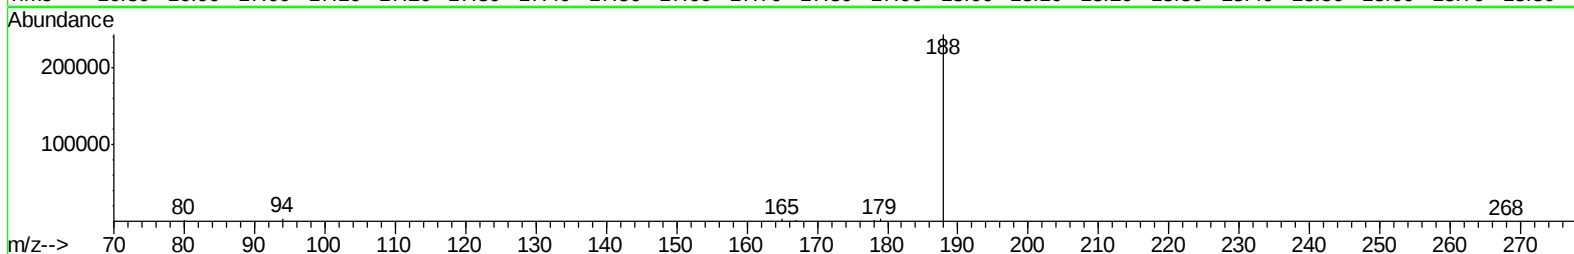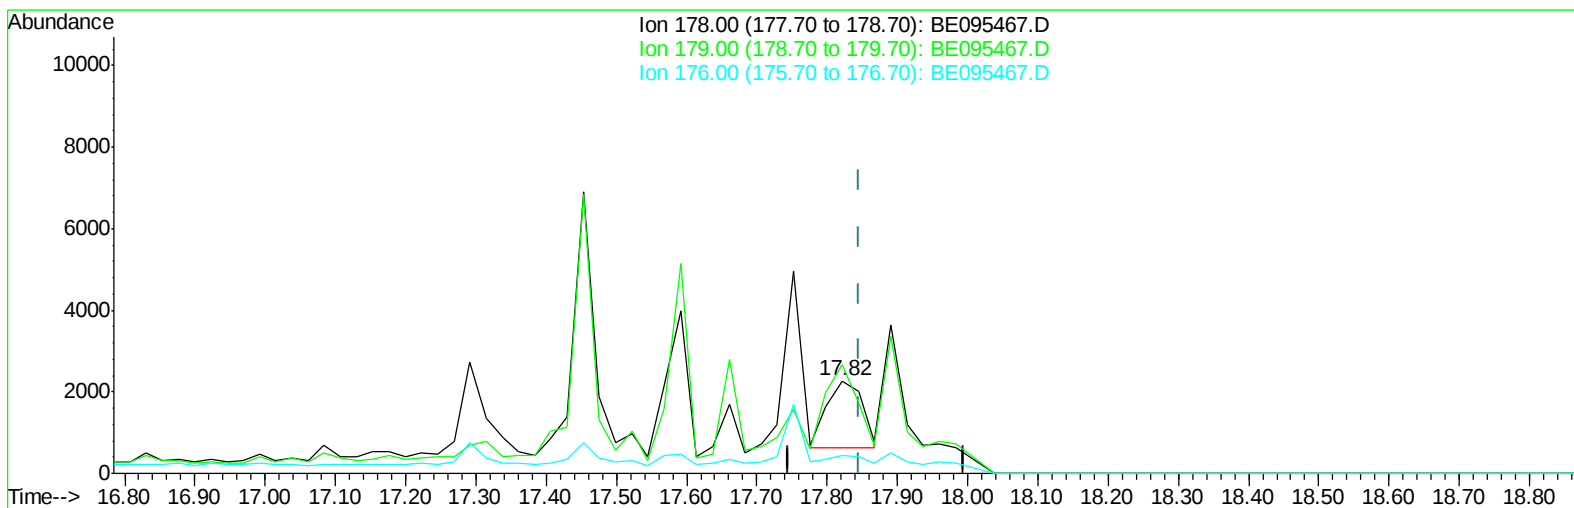

TIC: BE095467.D

(13) Anthracene

17.821min (-0.024) 0.24ng/ul m

response 5728

| Ion    | Exp%  | Act%    |
|--------|-------|---------|
| 178.00 | 100   | 100     |
| 179.00 | 22.60 | 117.93# |
| 176.00 | 18.40 | 19.74   |
| 0.00   | 0.00  | 0.00    |




Data Path : Z:\HPCHEM1\BNA E\DATA\BE020318\  
Data File : BE095467.D  
Acq On : 4 Feb 2018 8:52  
Operator : SJ/JU  
Sample : J1315-19  
Misc :  
ALS Vial : 36 Sample Multiplier: 1

Instrument :  
BNA\_E  
ClientSampleId :  
F6C82

Manual Integrations  
APPROVED

Sohil  
2/5/2018 7:01:01 PM

Quant Time: Feb 05 06:46:21 2018  
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Feb 05 04:46:10 2018  
Response via : Initial Calibration

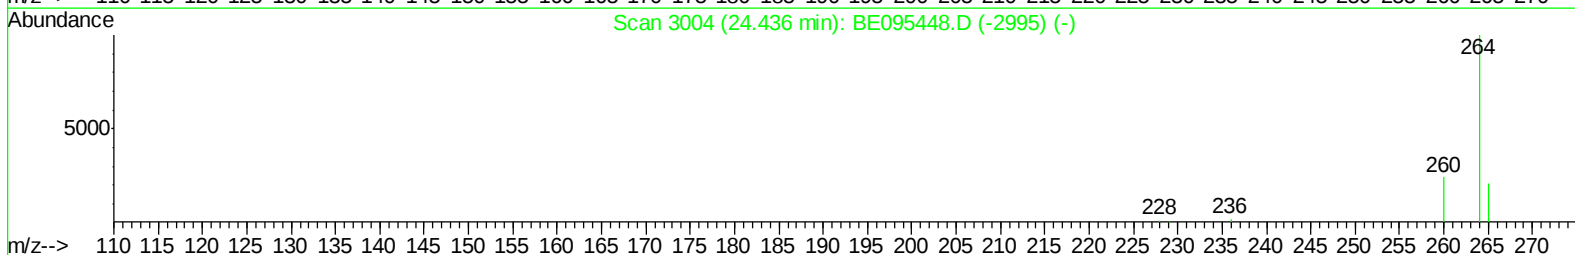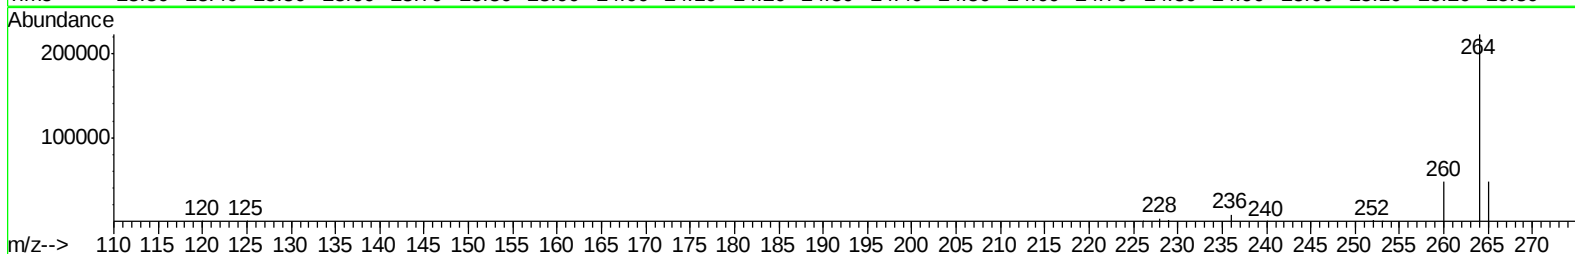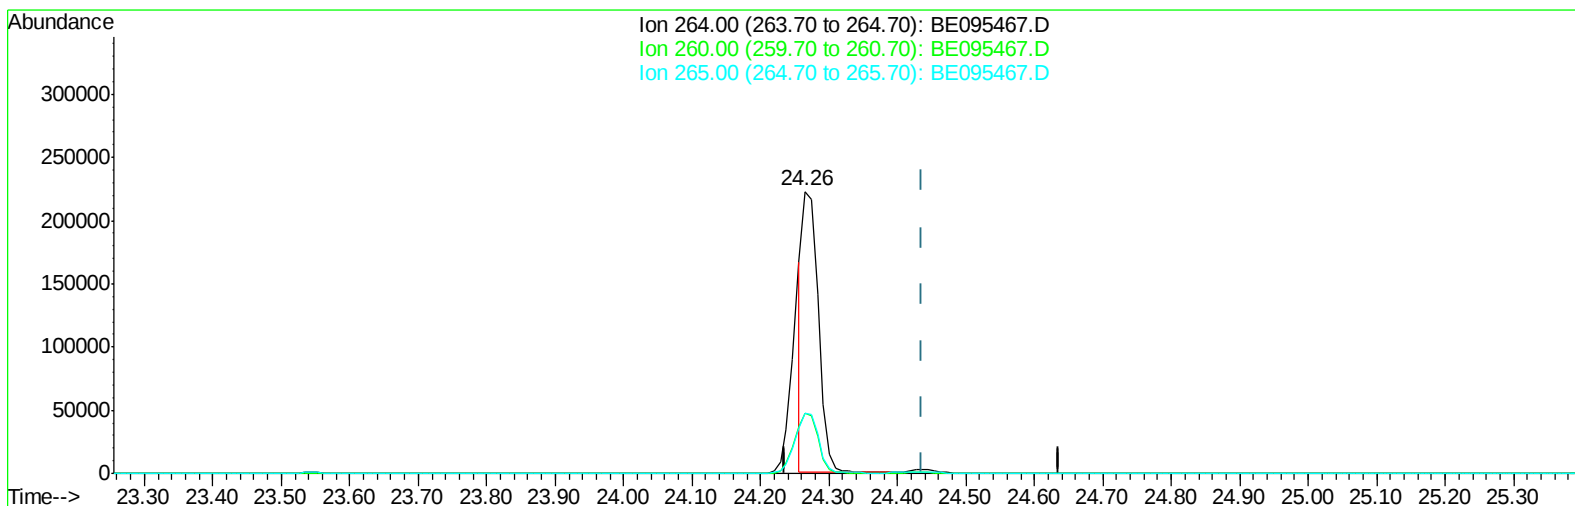

TIC: BE095467.D

(20) Perylene-d12 (I)

24.265min (-0.171) 0.40ng/ul

response 354423

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 264.00 | 100    | 100    |
| 260.00 | 30.10  | 21.35# |
| 265.00 | 103.50 | 21.28# |
| 0.00   | 0.00   | 0.00   |




Data Path : Z:\HPCHEM1\BNA E\DATA\BE020318\  
Data File : BE095467.D  
Acq On : 4 Feb 2018 8:52  
Operator : SJ/JU  
Sample : J1315-19  
Misc :  
ALS Vial : 36 Sample Multiplier: 1

Instrument :  
BNA\_E  
ClientSampleId :  
F6C82

Manual Integrations  
APPROVED

Sohil  
2/5/2018 7:01:01 PM

Quant Time: Feb 05 06:46:21 2018  
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Feb 05 04:46:10 2018  
Response via : Initial Calibration

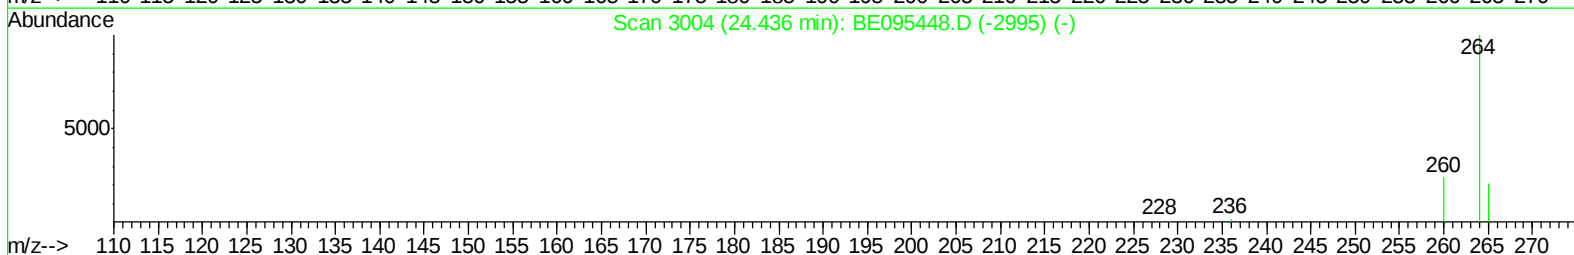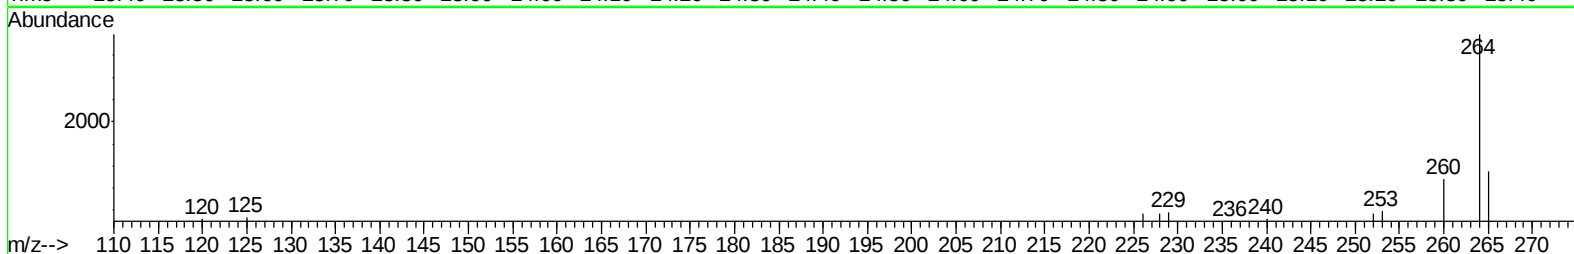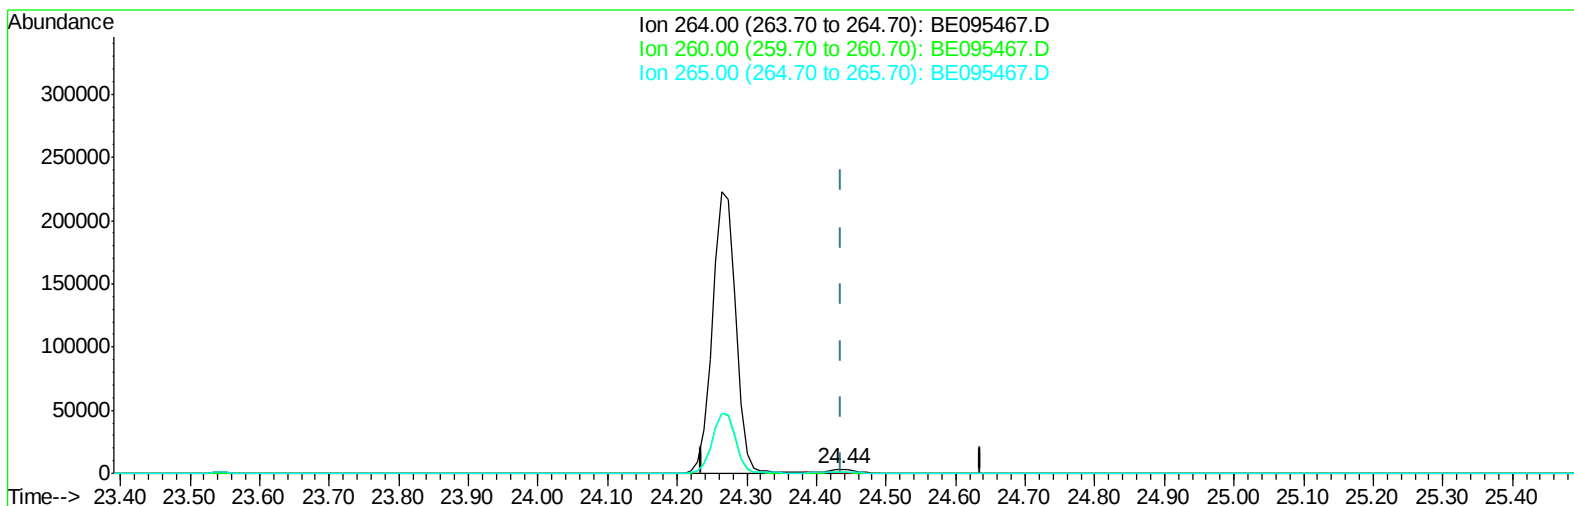

TIC: BE095467.D

(20) Perylene-d12 (I)

24.436min (-0.000) 0.40ng/ul m

response 6850

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 264.00 | 100    | 100    |
| 260.00 | 30.10  | 26.84  |
| 265.00 | 103.50 | 30.95# |
| 0.00   | 0.00   | 0.00   |




Data Path : Z:\HPCHEM1\BNA E\DATA\BE020318\  
Data File : BE095467.D  
Acq On : 4 Feb 2018 8:52  
Operator : SJ/JU  
Sample : J1315-19  
Misc :  
ALS Vial : 36 Sample Multiplier: 1

Instrument :  
BNA\_E  
ClientSampleId :  
F6C82

Manual Integrations  
APPROVED

Sohil  
2/5/2018 7:01:01 PM

Quant Time: Feb 05 06:53:50 2018  
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Feb 05 04:46:10 2018  
Response via : Initial Calibration

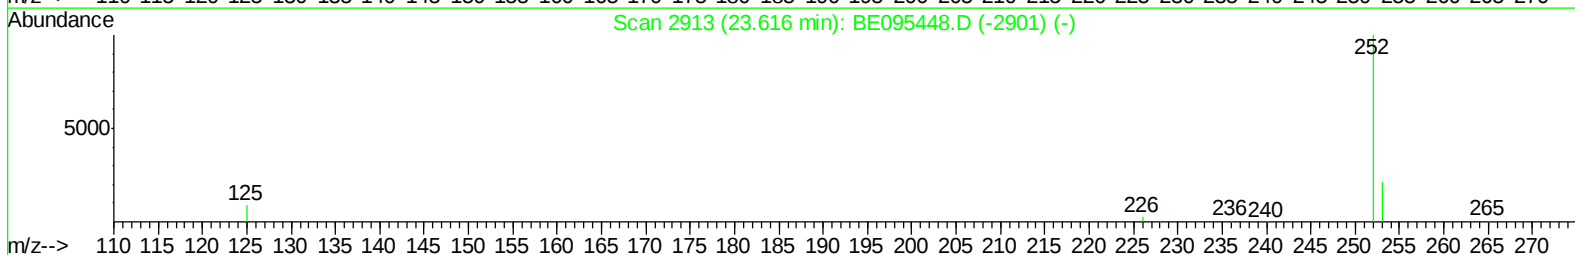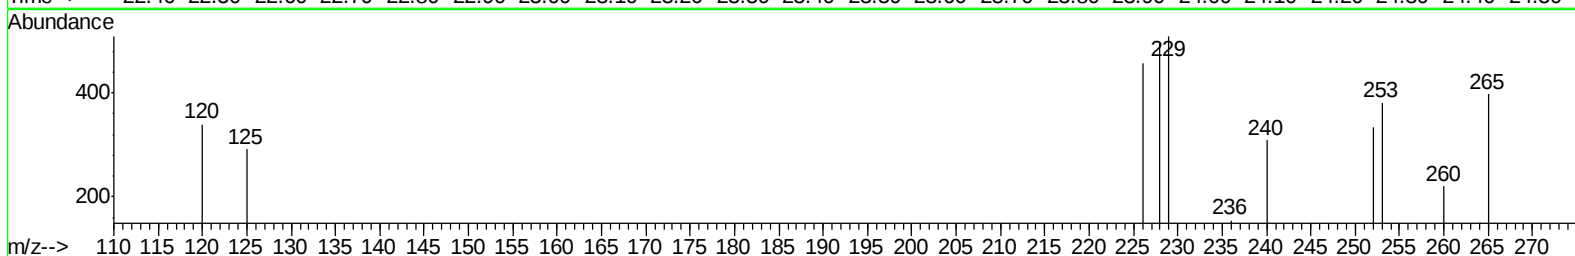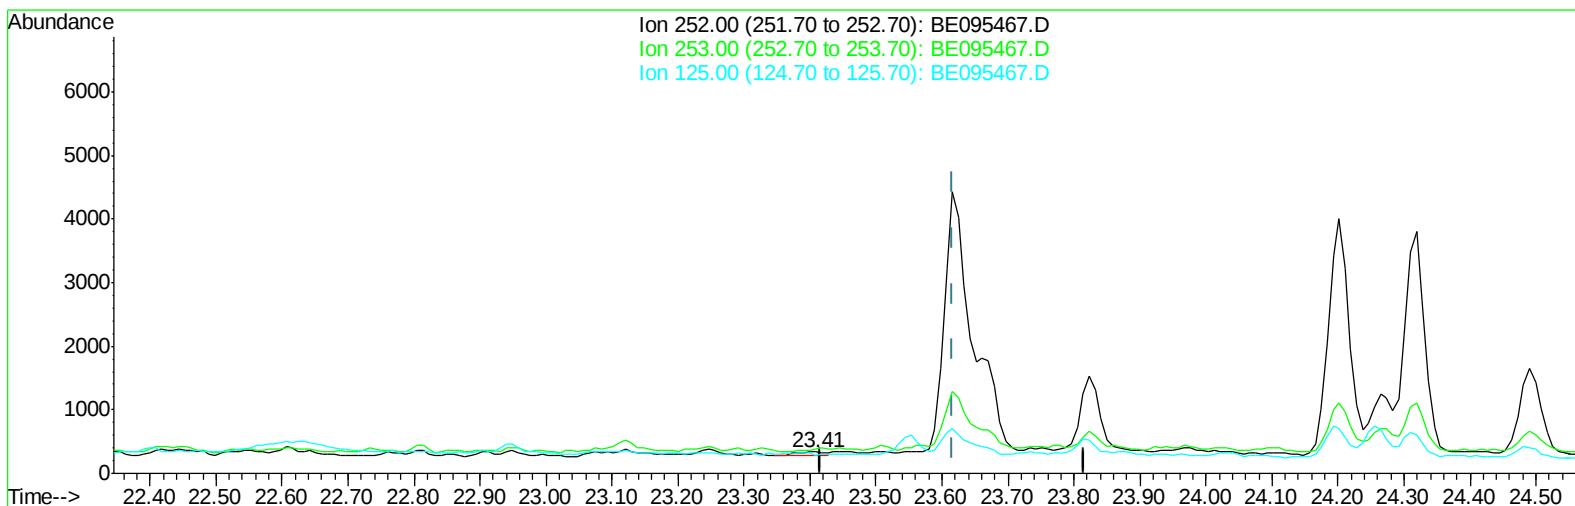

TIC: BE095467.D

(21) Benzo(b)fluoranthene

23.409min (-0.207) 0.01ng/ul

response 181

| Ion    | Exp%  | Act%    |
|--------|-------|---------|
| 252.00 | 100   | 100     |
| 253.00 | 32.10 | 114.03# |
| 125.00 | 17.50 | 86.87#  |
| 0.00   | 0.00  | 0.00    |




Data Path : Z:\HPCHEM1\BNA E\DATA\BE020318\  
Data File : BE095467.D  
Acq On : 4 Feb 2018 8:52  
Operator : SJ/JU  
Sample : J1315-19  
Misc :  
ALS Vial : 36 Sample Multiplier: 1

Instrument :  
BNA\_E  
ClientSampleId :  
F6C82

Manual Integrations  
APPROVED

Sohil  
2/5/2018 7:01:01 PM

Quant Time: Feb 05 06:53:50 2018  
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Feb 05 04:46:10 2018  
Response via : Initial Calibration

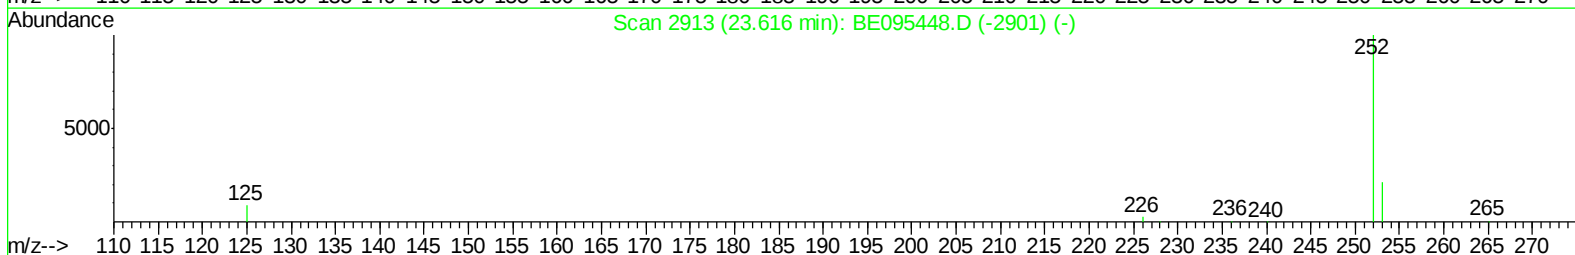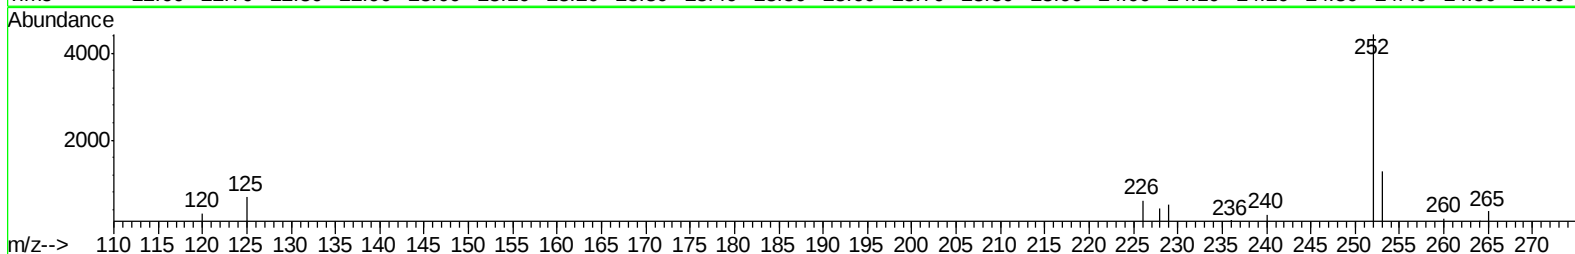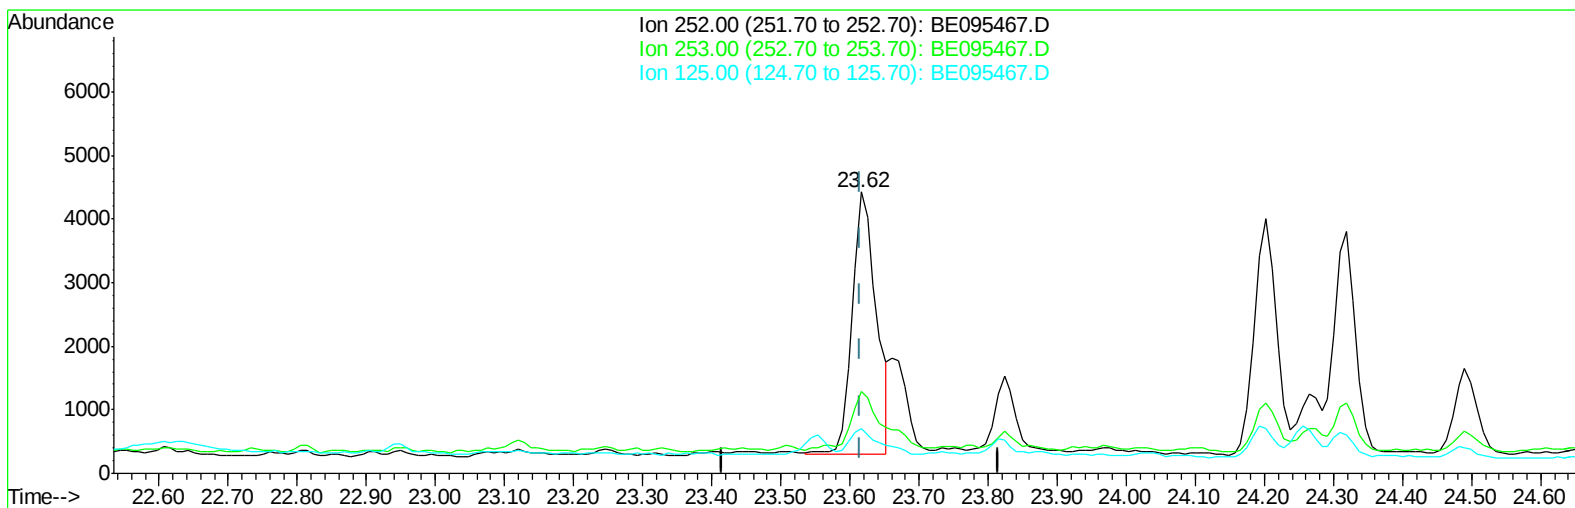

TIC: BE095467.D

(21) Benzo(b)fluoranthene

23.616min (-0.000) 0.42ng/ul m

response 10115

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 252.00 | 100   | 100   |
| 253.00 | 32.10 | 29.06 |
| 125.00 | 17.50 | 15.78 |
| 0.00   | 0.00  | 0.00  |




Data Path : Z:\HPCHEM1\BNA E\DATA\BE020318\  
Data File : BE095467.D  
Acq On : 4 Feb 2018 8:52  
Operator : SJ/JU  
Sample : J1315-19  
Misc :  
ALS Vial : 36 Sample Multiplier: 1

Instrument :  
BNA\_E  
ClientSampleId :  
F6C82

Manual Integrations  
APPROVED

Sohil  
2/5/2018 7:01:01 PM

Quant Time: Feb 05 06:53:50 2018  
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Feb 05 04:46:10 2018  
Response via : Initial Calibration

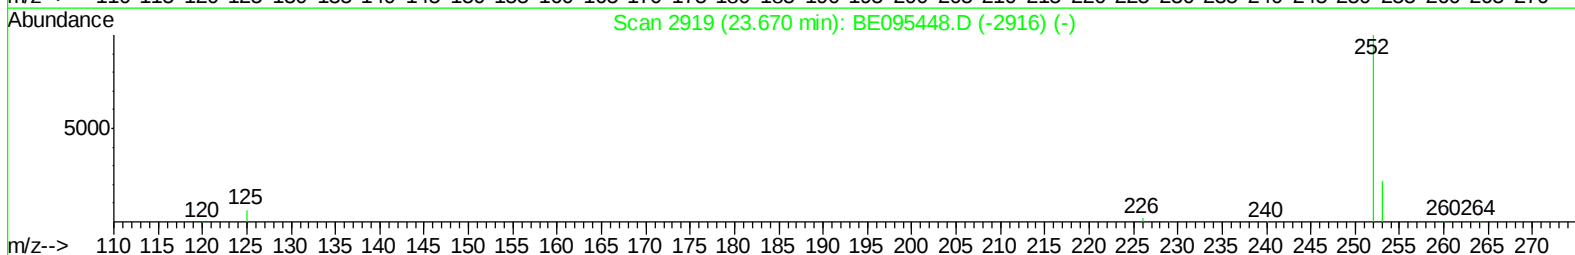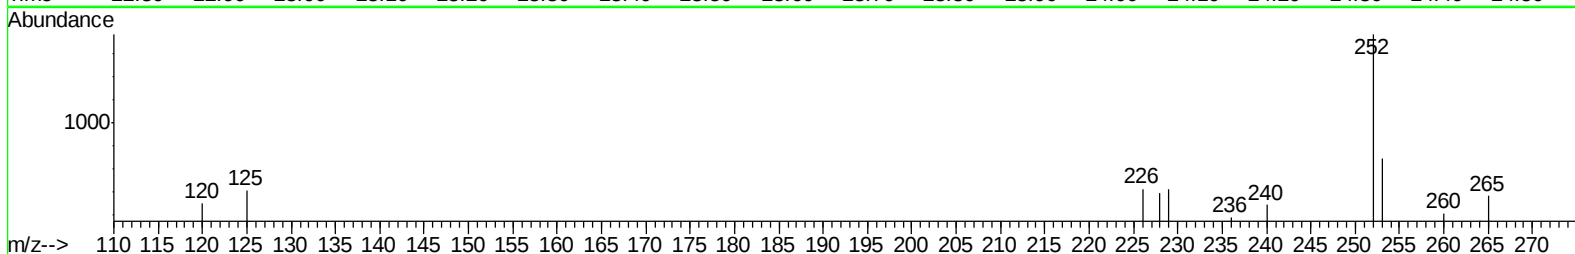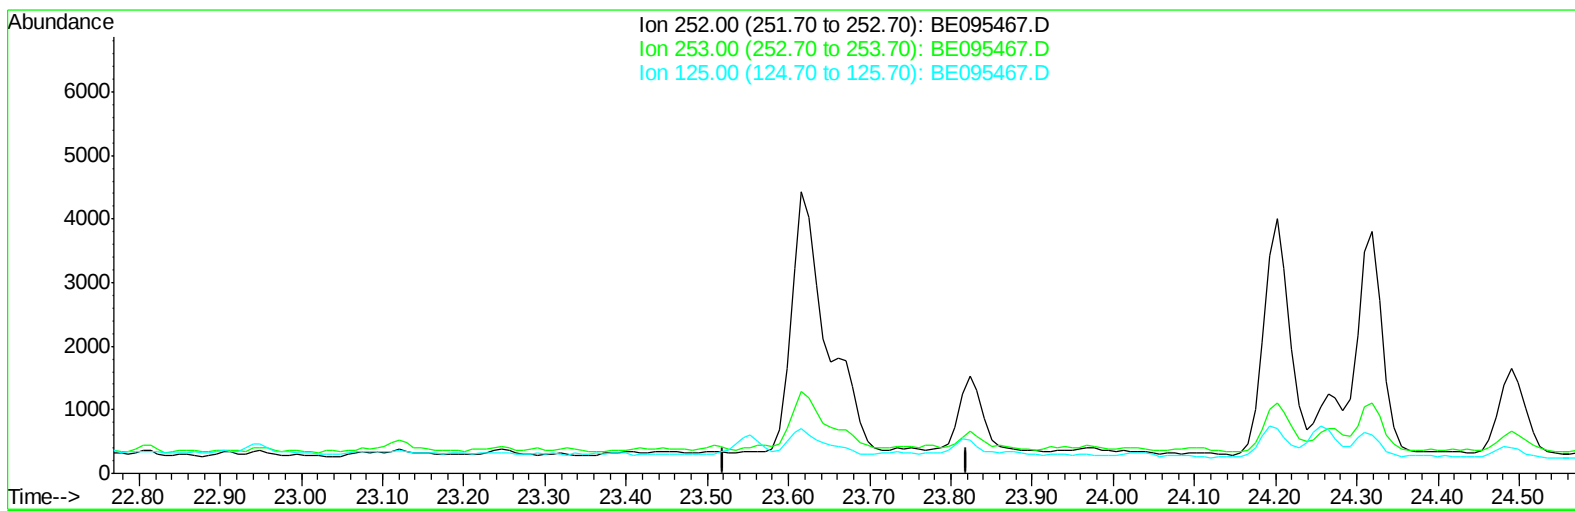

TIC: BE095467.D

(22) Benzo(k)fluoranthene

23.670min (-23.670) 0.00ng/ul

response 0

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 252.00 | 100   | 0.00  |
| 253.00 | 30.60 | 0.00# |
| 125.00 | 17.10 | 0.00# |
| 0.00   | 0.00  | 0.00  |




Data Path : Z:\HPCHEM1\BNA E\DATA\BE020318\  
Data File : BE095467.D  
Acq On : 4 Feb 2018 8:52  
Operator : SJ/JU  
Sample : J1315-19  
Misc :  
ALS Vial : 36 Sample Multiplier: 1

Instrument :  
BNA\_E  
ClientSampleId :  
F6C82

Manual Integrations  
APPROVED

Sohil  
2/5/2018 7:01:01 PM

Quant Time: Feb 05 06:53:50 2018  
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Feb 05 04:46:10 2018  
Response via : Initial Calibration

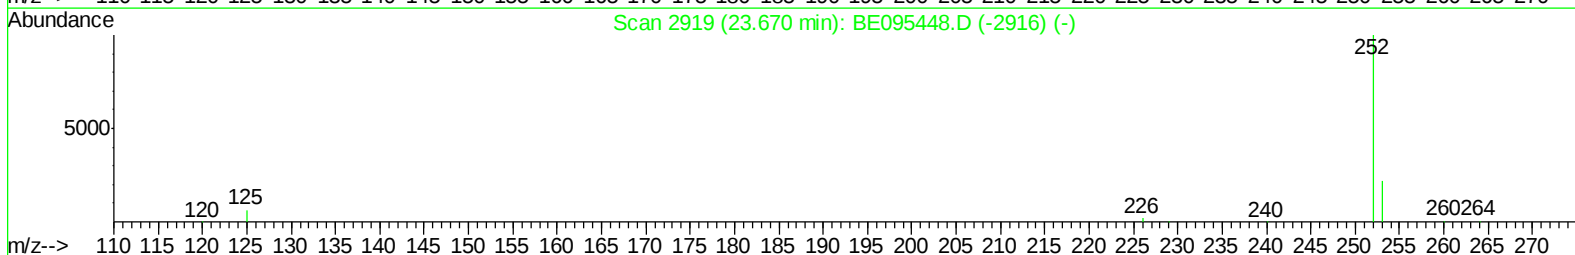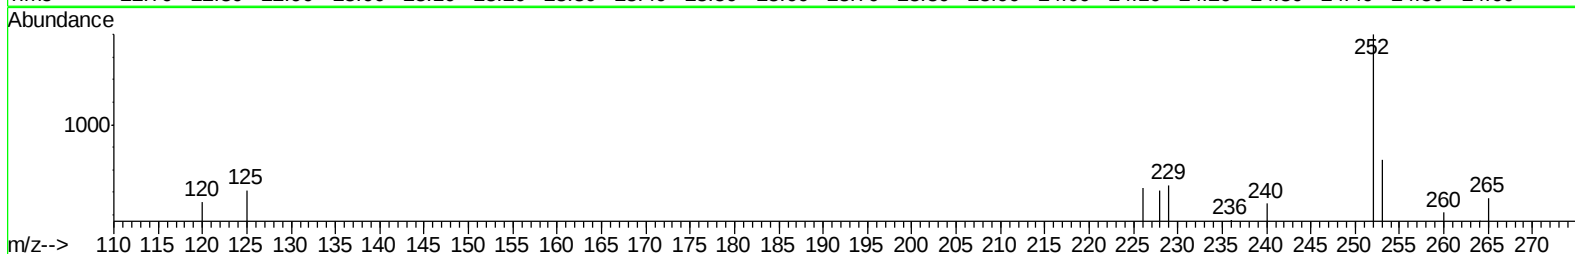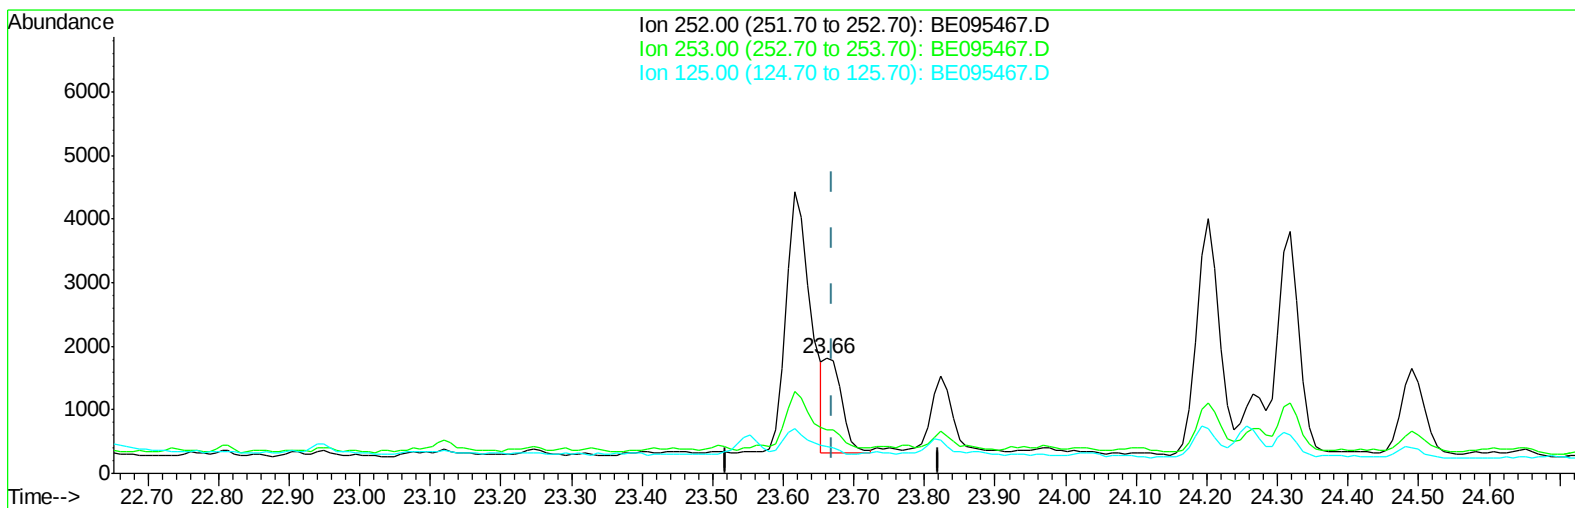

TIC: BE095467.D

(22) Benzo(k)fluoranthene

23.661min (-0.009) 0.12ng/ul m

response 2614

| Ion    | Exp%  | Act%   |
|--------|-------|--------|
| 252.00 | 100   | 100    |
| 253.00 | 30.60 | 37.80# |
| 125.00 | 17.10 | 23.12# |
| 0.00   | 0.00  | 0.00   |




Data Path : Z:\HPCHEM1\BNA E\DATA\BE020318\  
Data File : BE095467.D  
Acq On : 4 Feb 2018 8:52  
Operator : SJ/JU  
Sample : J1315-19  
Misc :  
ALS Vial : 36 Sample Multiplier: 1

Instrument :  
BNA\_E  
ClientSampleId :  
F6C82

Manual Integrations  
APPROVED

Sohil  
2/5/2018 7:01:01 PM

Quant Time: Feb 05 06:53:50 2018  
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Feb 05 04:46:10 2018  
Response via : Initial Calibration

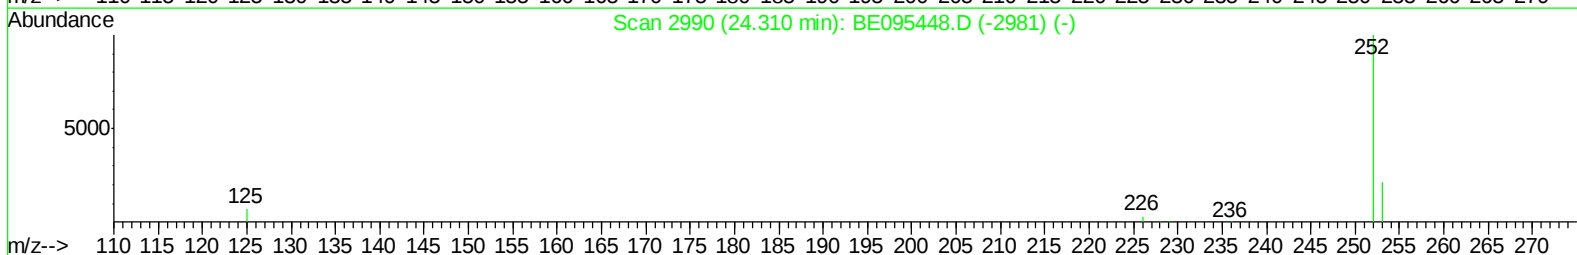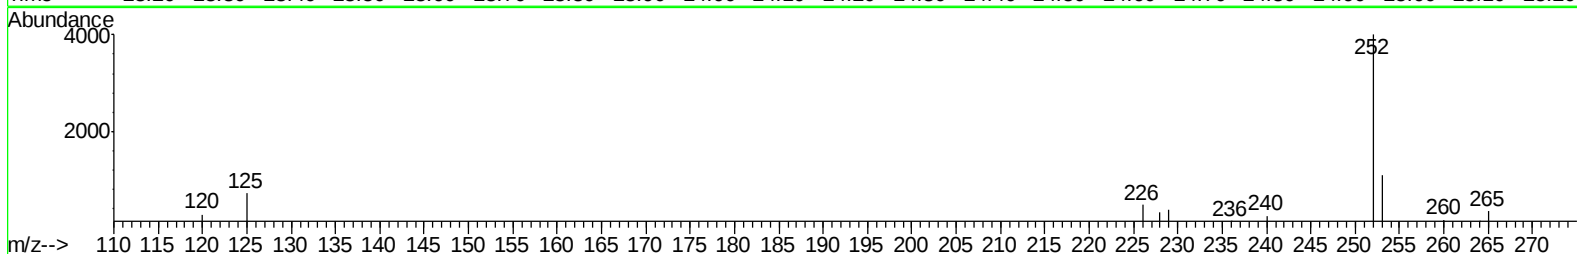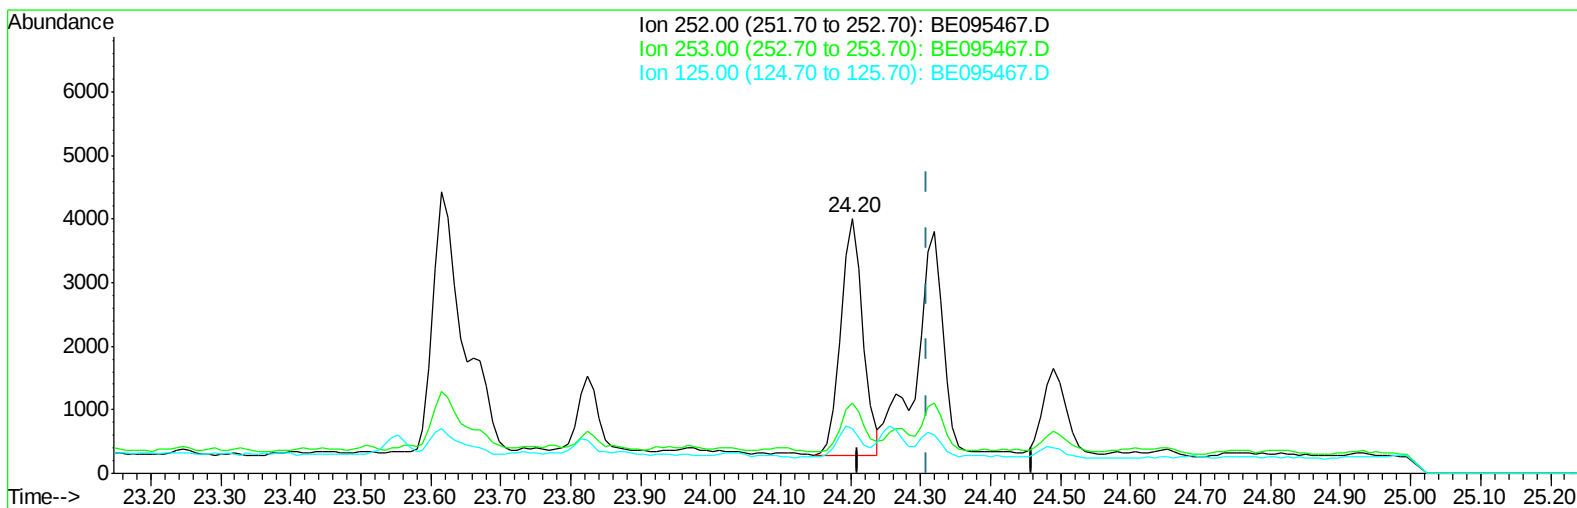

TIC: BE095467.D

(23) Benzo(a)pyrene (C)

24.202min (-0.108) 0.39ng/ul

response 8322

| Ion    | Exp%  | Act%   |
|--------|-------|--------|
| 252.00 | 100   | 100    |
| 253.00 | 35.60 | 27.50# |
| 125.00 | 22.60 | 17.84# |
| 0.00   | 0.00  | 0.00   |




Data Path : Z:\HPCHEM1\BNA E\DATA\BE020318\  
Data File : BE095467.D  
Acq On : 4 Feb 2018 8:52  
Operator : SJ/JU  
Sample : J1315-19  
Misc :  
ALS Vial : 36 Sample Multiplier: 1

Instrument :  
BNA\_E  
ClientSampleId :  
F6C82

Manual Integrations  
APPROVED

Sohil  
2/5/2018 7:01:01 PM

Quant Time: Feb 05 06:53:50 2018  
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Feb 05 04:46:10 2018  
Response via : Initial Calibration

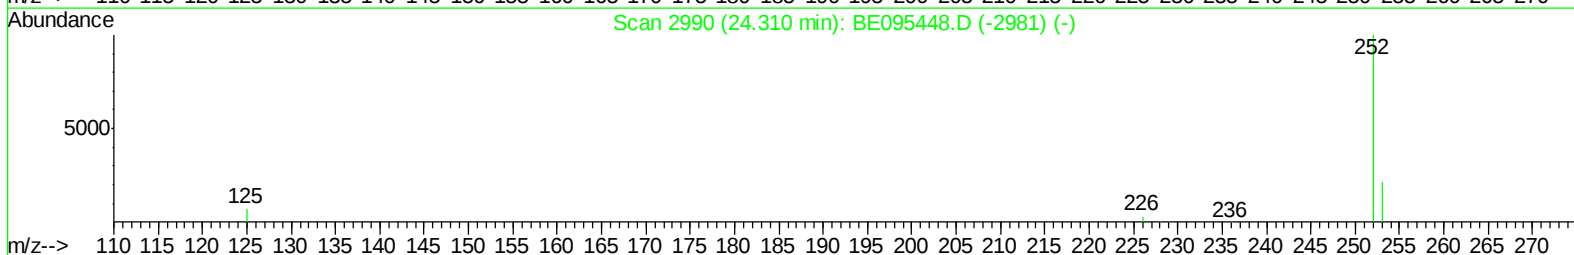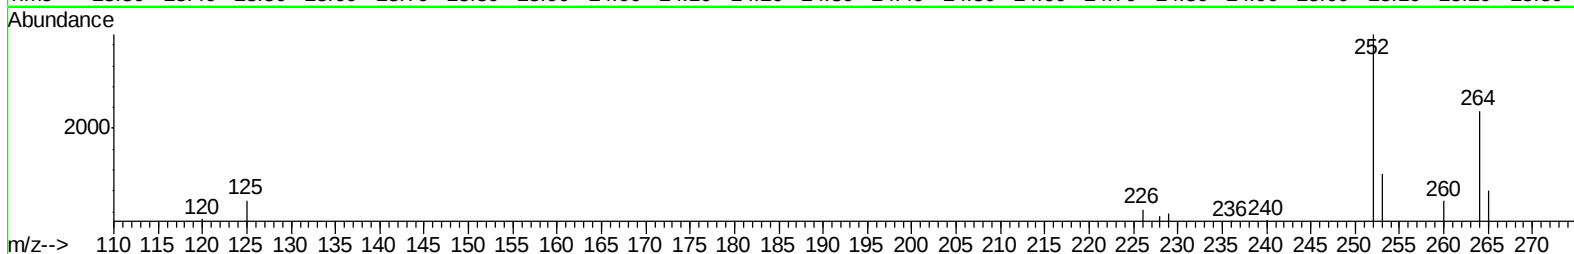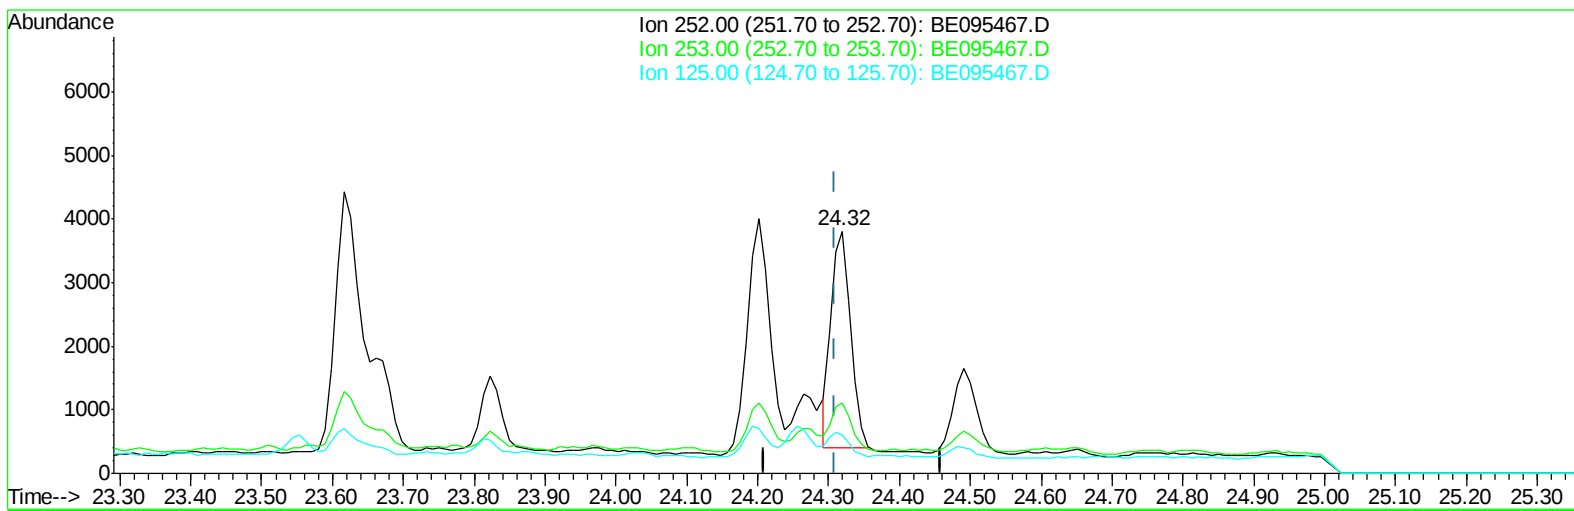

TIC: BE095467.D

(23) Benzo(a)pyrene (C)

24.319min (+0.009) 0.30ng/ul m

response 6445

| Ion    | Exp%  | Act%   |
|--------|-------|--------|
| 252.00 | 100   | 100    |
| 253.00 | 35.60 | 29.32  |
| 125.00 | 22.60 | 16.05# |
| 0.00   | 0.00  | 0.00   |




Data Path : Z:\HPCHEM1\BNA E\DATA\BE020318\  
Data File : BE095467.D  
Acq On : 4 Feb 2018 8:52  
Operator : SJ/JU  
Sample : J1315-19  
Misc :  
ALS Vial : 36 Sample Multiplier: 1

Instrument :  
BNA\_E  
ClientSampleId :  
F6C82

Manual Integrations  
APPROVED

Sohil  
2/5/2018 7:01:01 PM

Quant Time: Feb 05 06:53:50 2018  
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Feb 05 04:46:10 2018  
Response via : Initial Calibration

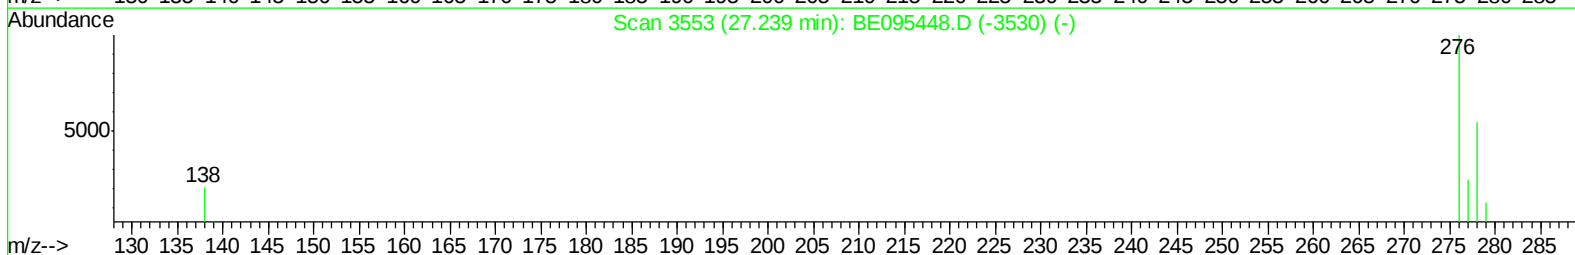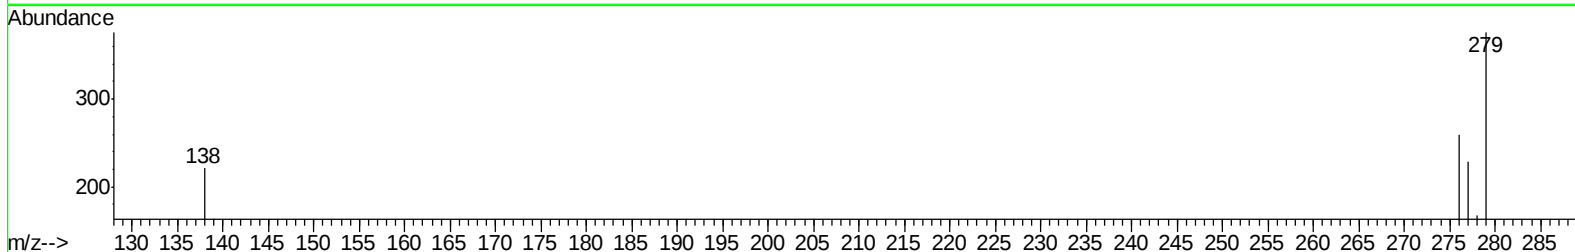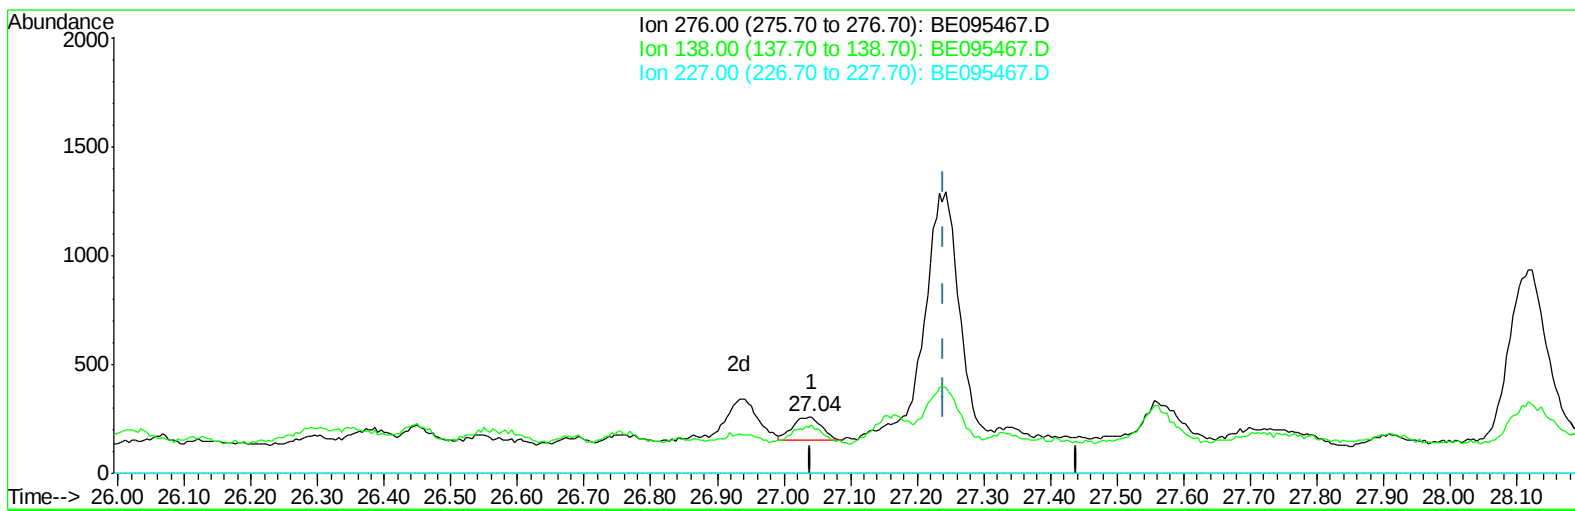

TIC: BE095467.D

(24) Indeno(1,2,3-cd)pyrene

27.042min (-0.197) 0.01ng/ul

response 333

| Ion    | Exp%  | Act%   |
|--------|-------|--------|
| 276.00 | 100   | 100    |
| 138.00 | 35.00 | 78.98# |
| 227.00 | 10.00 | 0.00#  |
| 0.00   | 0.00  | 0.00   |




Data Path : Z:\HPCHEM1\BNA E\DATA\BE020318\  
Data File : BE095467.D  
Acq On : 4 Feb 2018 8:52  
Operator : SJ/JU  
Sample : J1315-19  
Misc :  
ALS Vial : 36 Sample Multiplier: 1

Instrument :  
BNA\_E  
ClientSampleId :  
F6C82

Manual Integrations  
APPROVED

Sohil  
2/5/2018 7:01:01 PM

Quant Time: Feb 05 06:53:50 2018  
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Feb 05 04:46:10 2018  
Response via : Initial Calibration

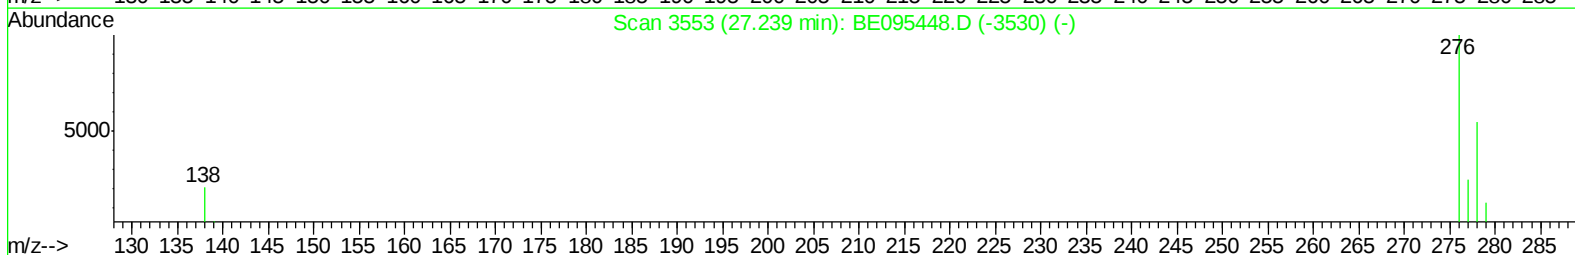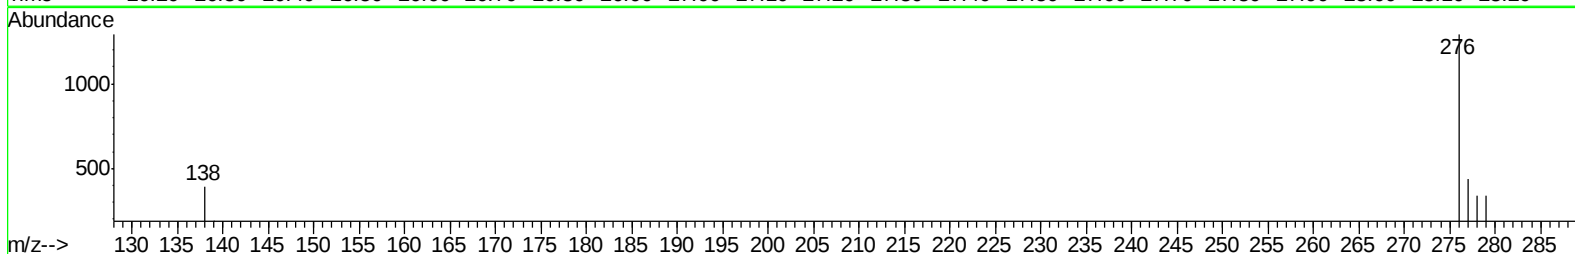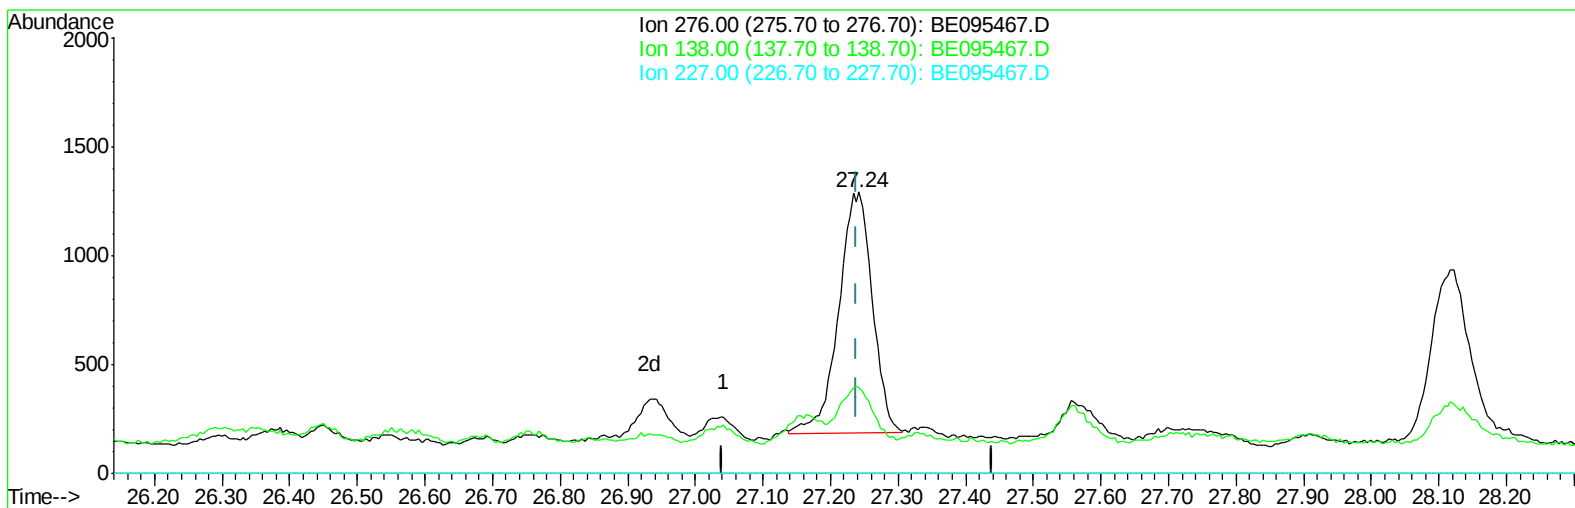

TIC: BE095467.D

(24) Indeno(1,2,3-cd)pyrene

27.242min (+0.003) 0.16ng/ul m

response 3800

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 276.00 | 100   | 100   |
| 138.00 | 35.00 | 6.92# |
| 227.00 | 10.00 | 0.00# |
| 0.00   | 0.00  | 0.00  |




Data Path : Z:\HPCHEM1\BNA E\DATA\BE020318\  
 Data File : BE095467.D  
 Acq On : 4 Feb 2018 8:52  
 Operator : SJ/JU  
 Sample : J1315-19  
 Misc :  
 ALS Vial : 36 Sample Multiplier: 1

Instrument :  
 BNA\_E  
 ClientSampleId :  
 F6C82

Manual Integrations  
 APPROVED

Sohil  
 2/5/2018 7:01:01 PM

Quant Time: Feb 05 06:53:50 2018  
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Mon Feb 05 04:46:10 2018  
 Response via : Initial Calibration

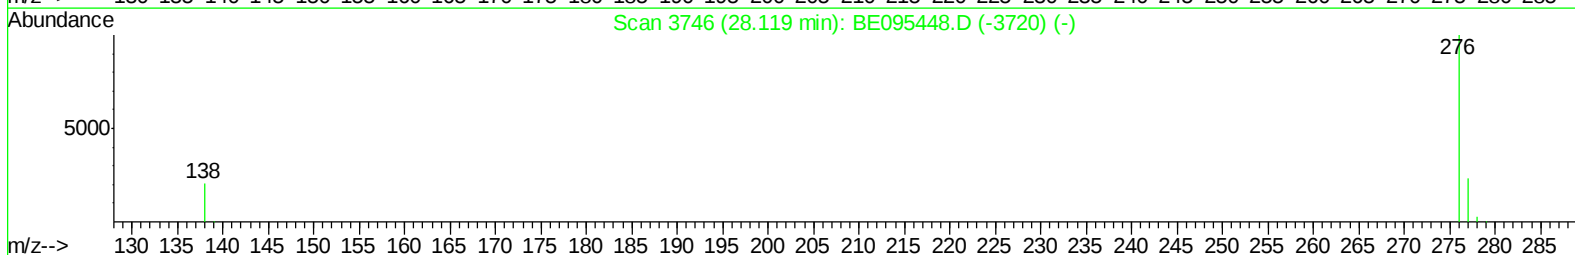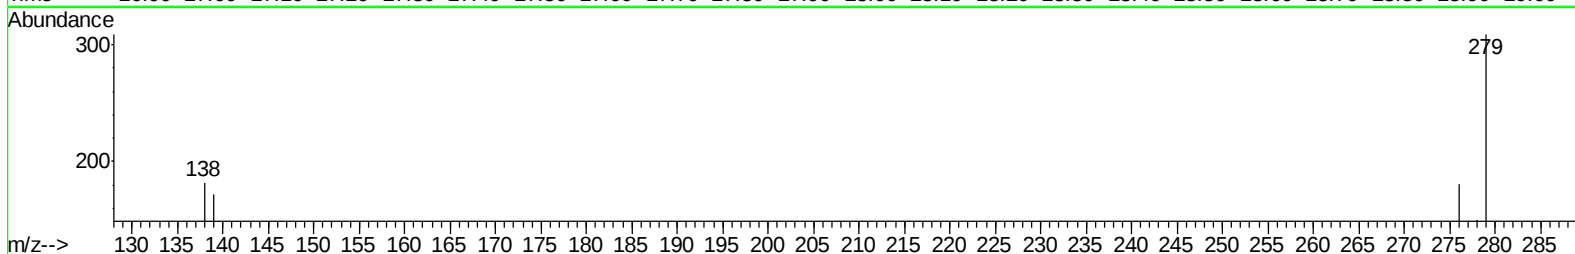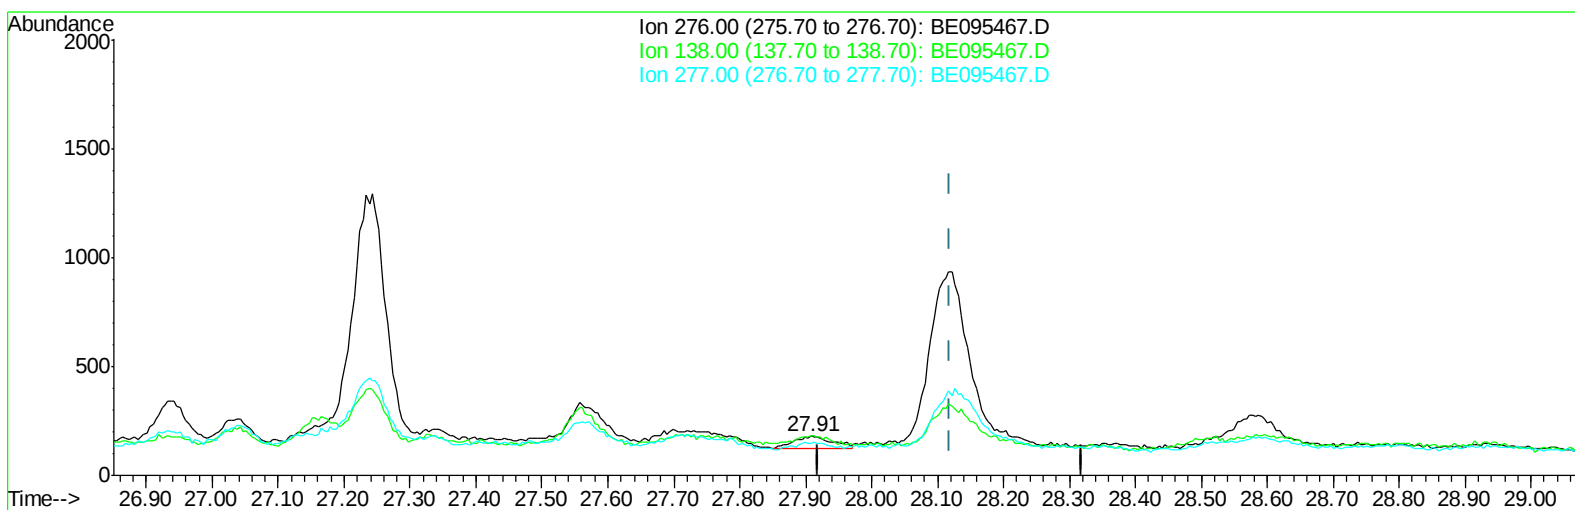

TIC: BE095467.D

(26) Benzo(g,h,i)perylene

27.908min (-0.211) 0.01ng/ul

response 224

| Ion    | Exp%  | Act%    |
|--------|-------|---------|
| 276.00 | 100   | 100     |
| 138.00 | 27.30 | 100.55# |
| 277.00 | 25.60 | 82.32#  |
| 0.00   | 0.00  | 0.00    |




Data Path : Z:\HPCHEM1\BNA E\DATA\BE020318\  
Data File : BE095467.D  
Acq On : 4 Feb 2018 8:52  
Operator : SJ/JU  
Sample : J1315-19  
Misc :  
ALS Vial : 36 Sample Multiplier: 1

Instrument :  
BNA\_E  
ClientSampleId :  
F6C82

Manual Integrations  
APPROVED

Sohil  
2/5/2018 7:01:01 PM

Quant Time: Feb 05 06:53:50 2018  
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Feb 05 04:46:10 2018  
Response via : Initial Calibration

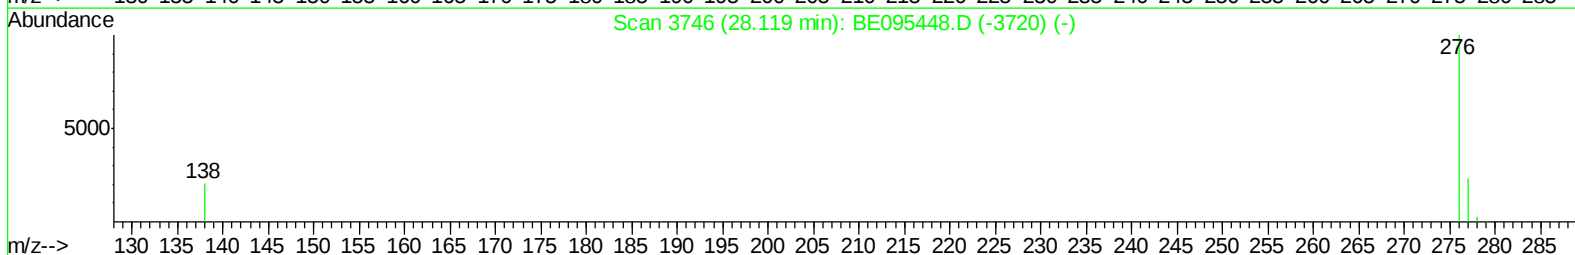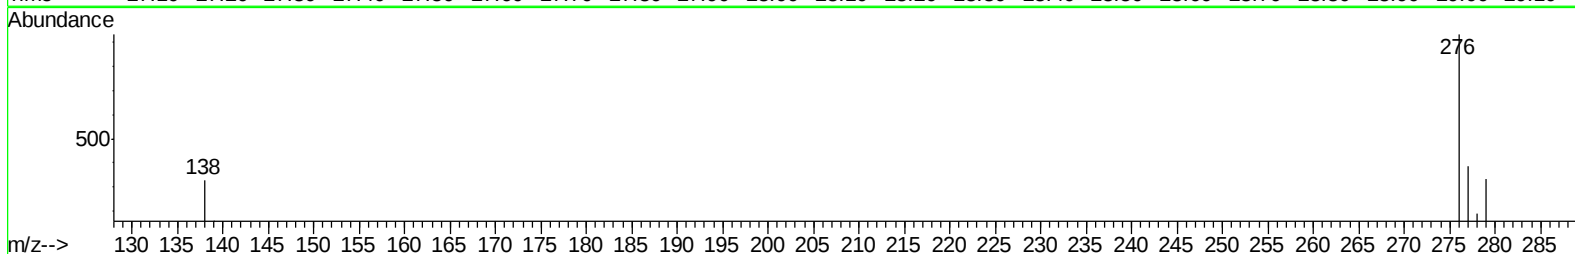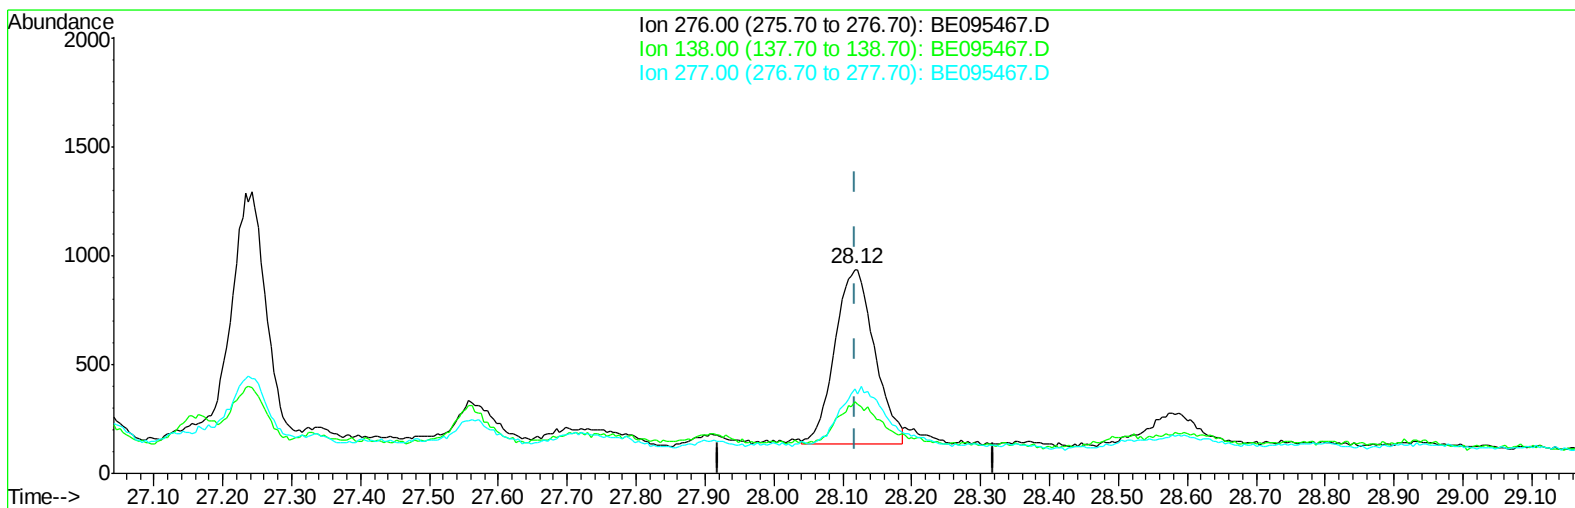

TIC: BE095467.D

(26) Benzo(g,h,i)perylene

28.117min (-0.002) 0.16ng/ul m

response 3210

| Ion    | Exp%  | Act%   |
|--------|-------|--------|
| 276.00 | 100   | 100    |
| 138.00 | 27.30 | 35.33# |
| 277.00 | 25.60 | 41.22# |
| 0.00   | 0.00  | 0.00   |

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020318\  
 Data File : BE095467.D  
 Acq On : 4 Feb 2018 8:52  
 Operator : SJ/JU  
 Sample : J1315-19  
 Misc :  
 ALS Vial : 36 Sample Multiplier: 1

Instrument :  
 BNA\_E  
 ClientSampleId :  
 F6C82

Manual Integrations  
 APPROVED

Sohil  
 2/5/2018 7:01:01 PM

Quant Time: Feb 05 06:55:26 2018  
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Mon Feb 05 04:46:10 2018  
 Response via : Initial Calibration

| Internal Standards          | R.T.  | QIon | Response | Conc   | Units  | Dev(Min) |
|-----------------------------|-------|------|----------|--------|--------|----------|
| 1) 1,4-Dichlorobenzene-d4   | 8.44  | 152  | 1805     | 0.40   | ng/ul  | 0.00     |
| 2) Naphthalene-d8           | 11.26 | 136  | 5392     | 0.40   | ng/ul  | 0.00     |
| 6) Acenaphthene-d10         | 15.01 | 164  | 4100     | 0.40   | ng/ul  | 0.00     |
| 10) Phenanthrene-d10        | 17.71 | 188  | 7916     | 0.40   | ng/ul  | 0.00     |
| 16) Chrysene-d12            | 21.80 | 240  | 7155     | 0.40   | ng/ul  | 0.00     |
| 20) Perylene-d12            | 24.44 | 264  | 6850m    | 0.40   | ng/ul  | 0.00     |
| System Monitoring Compounds |       |      |          |        |        |          |
| 4) 2-Methylnaphthalene-d10  | 12.81 | 152  | 3124     | 0.36   | ng/ul  | 0.00     |
| 14) Fluoranthene-d10        | 19.69 | 212  | 8532     | 0.28   | ng/ul  | 0.00     |
| Target Compounds            |       |      |          | Ovalue |        |          |
| 7) Acenaphthylene           | 14.74 | 152  | 2791     | 0.141  | ng/ul# | 82       |
| 11) Pentachlorophenol       | 17.36 | 266  | 1779     | 1.160  | ng/ul  | 98       |
| 12) Phenanthrene            | 17.75 | 178  | 7771m    | 0.292  | ng/ul  |          |
| 13) Anthracene              | 17.82 | 178  | 5728m    | 0.235  | ng/ul  |          |
| 15) Fluoranthene            | 19.72 | 202  | 6859     | 0.199  | ng/ul  | 77       |
| 17) Pyrene                  | 20.08 | 202  | 16680    | 0.695  | ng/ul# | 84       |
| 18) Benzo(a)anthracene      | 21.79 | 228  | 4776     | 0.213  | ng/ul# | 38       |
| 19) Chrysene                | 21.82 | 228  | 5615     | 0.242  | ng/ul# | 38       |
| 21) Benzo(b)fluoranthene    | 23.62 | 252  | 10115m   | 0.419  | ng/ul  |          |
| 22) Benzo(k)fluoranthene    | 23.66 | 252  | 2614m    | 0.118  | ng/ul  |          |
| 23) Benzo(a)pyrene          | 24.32 | 252  | 6445m    | 0.299  | ng/ul  |          |
| 24) Indeno(1,2,3-cd)pyrene  | 27.24 | 276  | 3800m    | 0.161  | ng/ul  |          |
| 26) Benzo(g,h,i)perylene    | 28.12 | 276  | 3210m    | 0.160  | ng/ul  |          |

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020318\  
Data File : BE095467.D  
Acq On : 4 Feb 2018 8:52  
Operator : SJ/JU  
Sample : J1315-19  
Misc :  
ALS Vial : 36 Sample Multiplier: 1

Instrument :  
BNA\_E  
ClientSampleId :  
F6C82

Manual Integrations  
APPROVED

Sohil  
2/5/2018 7:01:01 PM

Quant Time: Feb 05 06:55:26 2018  
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Feb 05 04:46:10 2018  
Response via : Initial Calibration

