




Data Path : Z:\HPCHEM1\BNA E\DATA\BE020318\
Data File : BE095475.D
Acq On : 4 Feb 2018 13:38
Operator : SJ/JU
Sample : J1315-06
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F6C63

Manual Integrations
APPROVED

Sohil
2/5/2018 7:01:27 PM

Quant Time: Feb 05 06:47:18 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 05 04:46:10 2018
Response via : Initial Calibration

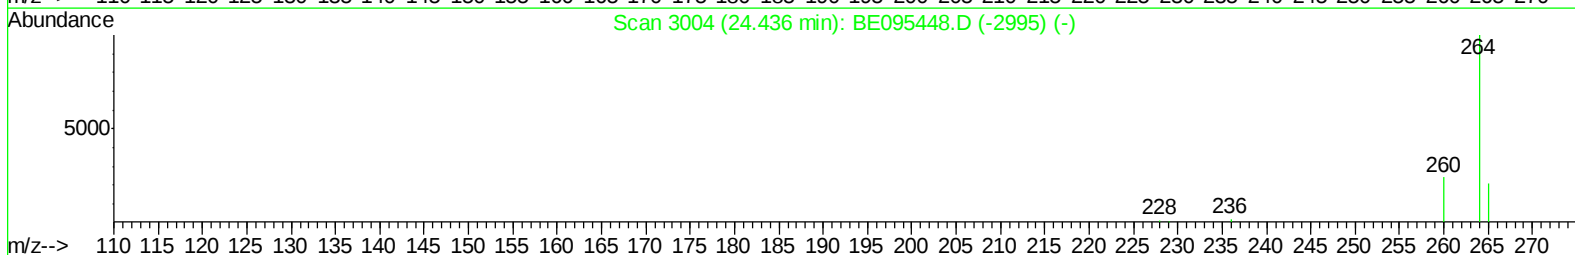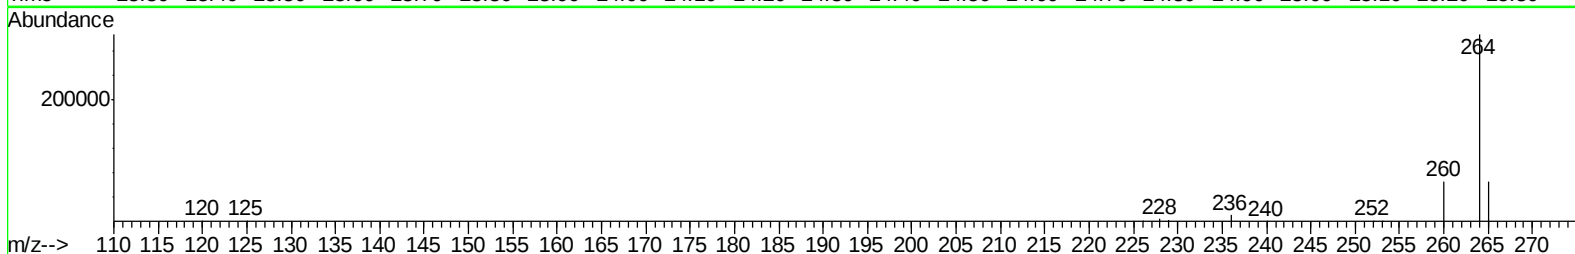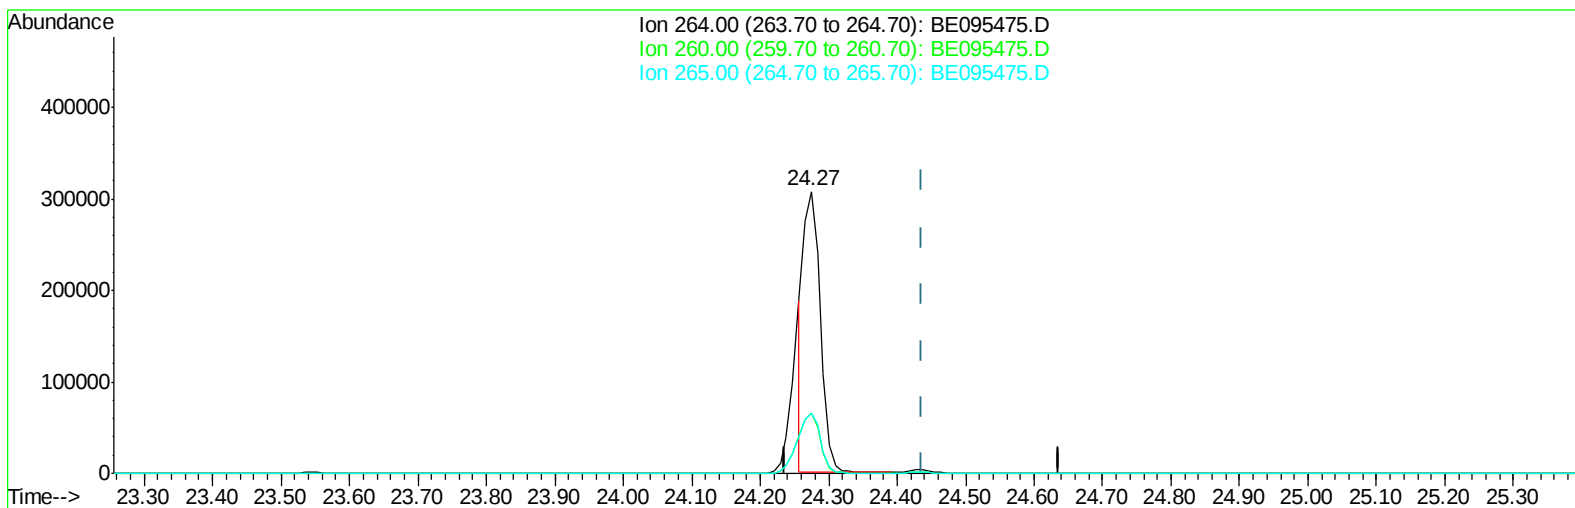

TIC: BE095475.D

(20) Perylene-d12 (I)

24.274min (-0.162) 0.40ng/ul

response 527060

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	21.20#
265.00	103.50	21.37#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA E\DATA\BE020318\
Data File : BE095475.D
Acq On : 4 Feb 2018 13:38
Operator : SJ/JU
Sample : J1315-06
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F6C63

Manual Integrations
APPROVED

Sohil
2/5/2018 7:01:27 PM

Quant Time: Feb 05 06:47:18 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 05 04:46:10 2018
Response via : Initial Calibration

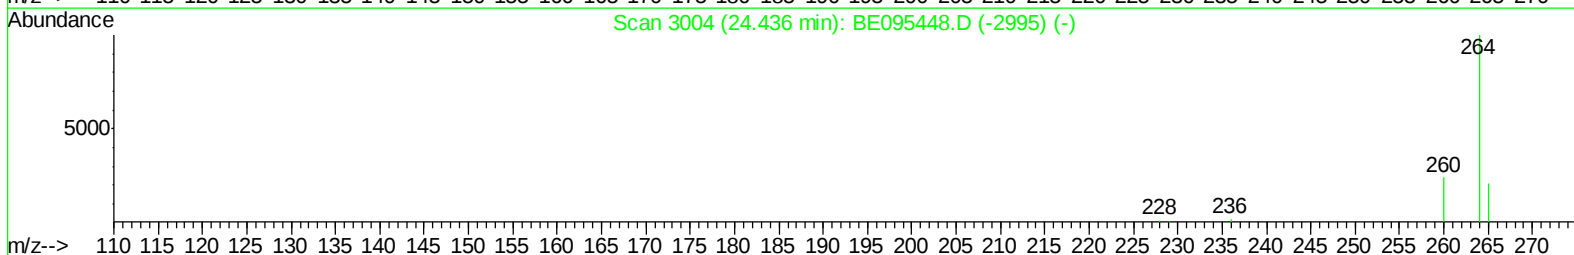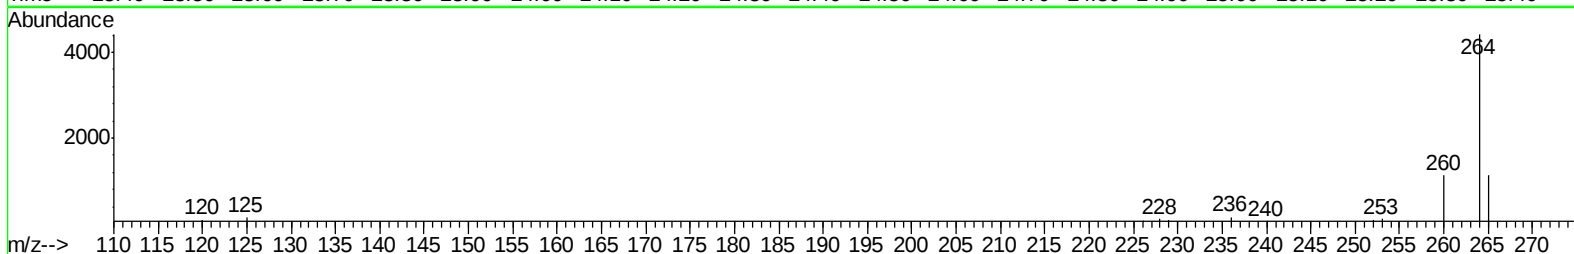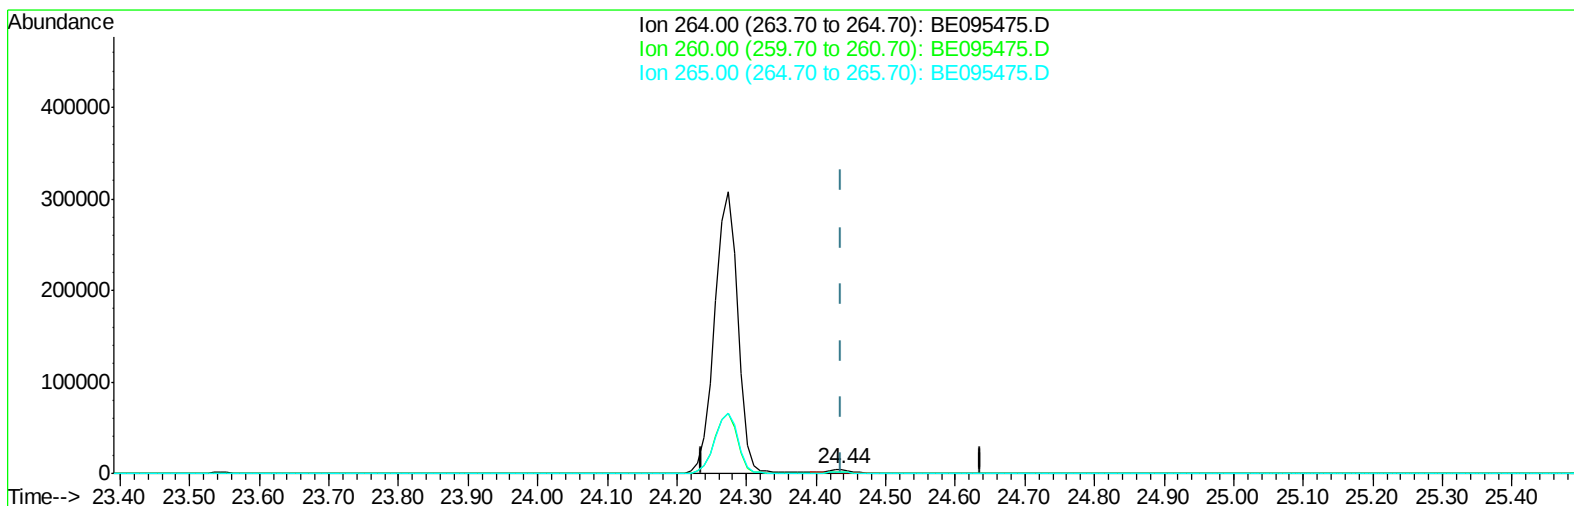

TIC: BE095475.D

(20) Perylene-d12 (I)

24.436min (+0.000) 0.40ng/ul m

response 8233

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	25.59
265.00	103.50	25.89#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020318\
Data File : BE095475.D
Acq On : 4 Feb 2018 13:38
Operator : SJ/JU
Sample : J1315-06
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F6C63

Manual Integrations
APPROVED

Sohil
2/5/2018 7:01:27 PM

Quant Time: Feb 05 07:47:23 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 05 04:46:10 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.44	152	2039	0.40	ng/ul	0.00
2) Naphthalene-d8	11.26	136	6429	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.02	164	4285	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	9127	0.40	ng/ul	0.00
16) Chrysene-d12	21.80	240	8997	0.40	ng/ul	0.00
20) Perylene-d12	24.44	264	8233m	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.81	152	4007	0.38	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	10511	0.30	ng/ul	0.00

Target Compounds	Ovalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020318\
Data File : BE095475.D
Acq On : 4 Feb 2018 13:38
Operator : SJ/JU
Sample : J1315-06
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F6C63

Manual Integrations
APPROVED

Sohil
2/5/2018 7:01:27 PM

Quant Time: Feb 05 07:47:23 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 05 04:46:10 2018
Response via : Initial Calibration

