




Data Path : Z:\HPCHEM1\BNA E\DATA\BE020318\
Data File : BE095480.D
Acq On : 4 Feb 2018 16:37
Operator : SJ/JU
Sample : J1315-11
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F6C68

Manual Integrations
APPROVED

Sohil
2/5/2018 7:01:42 PM

Quant Time: Feb 05 06:47:48 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 05 04:46:10 2018
Response via : Initial Calibration

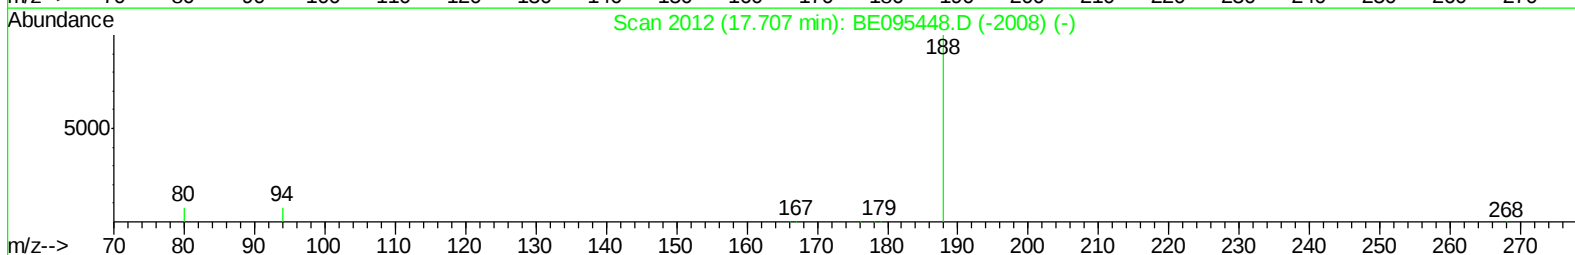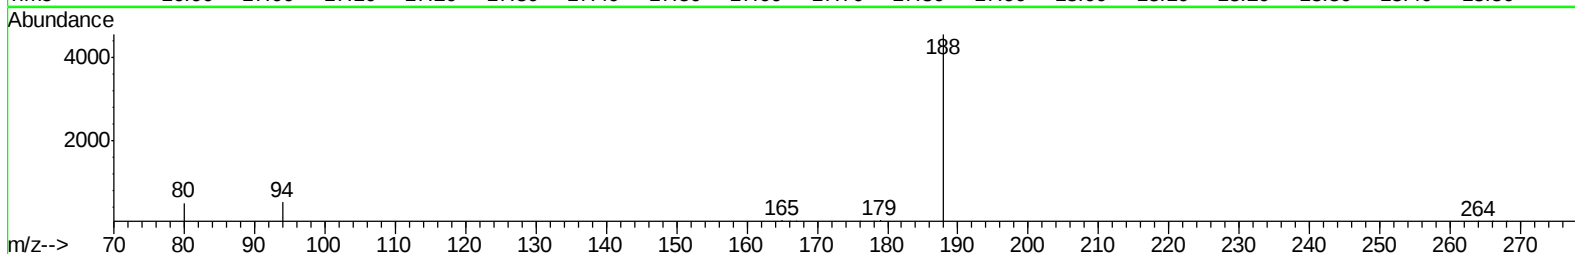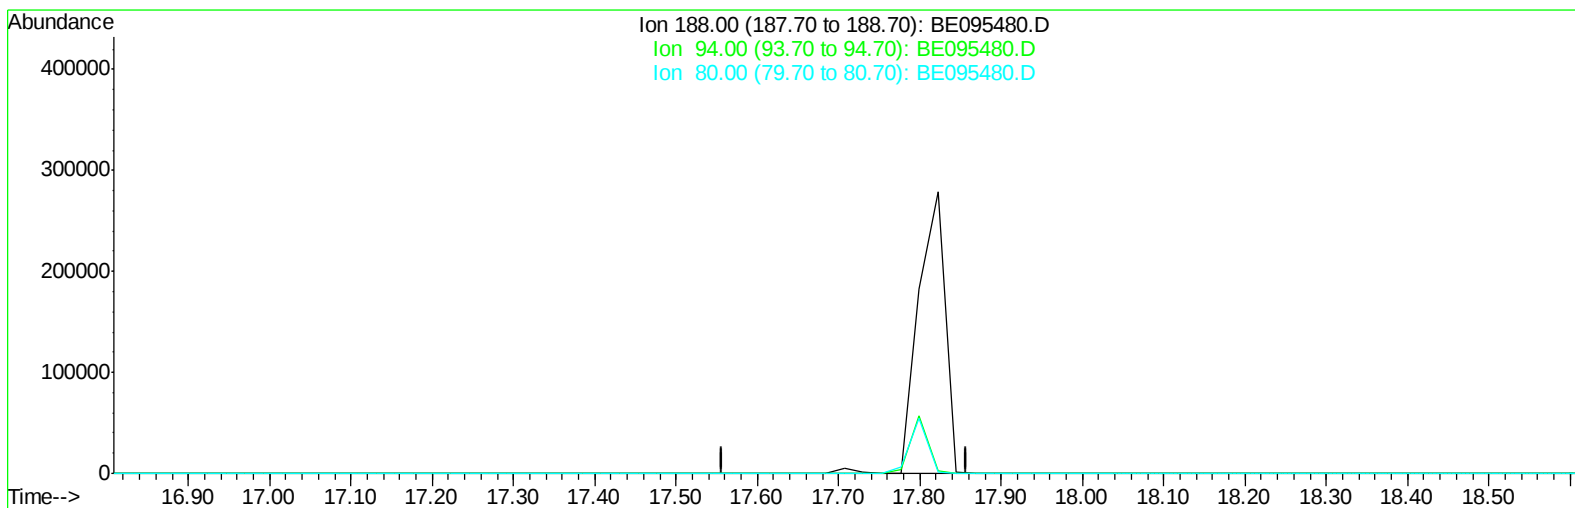

TIC: BE095480.D

(10) Phenanthrene-d10 (I)

17.707min (-17.707) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.00	0.00#
80.00	11.80	0.00#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA E\DATA\BE020318\
Data File : BE095480.D
Acq On : 4 Feb 2018 16:37
Operator : SJ/JU
Sample : J1315-11
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F6C68

Manual Integrations
APPROVED

Sohil
2/5/2018 7:01:42 PM

Quant Time: Feb 05 06:47:48 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 05 04:46:10 2018
Response via : Initial Calibration

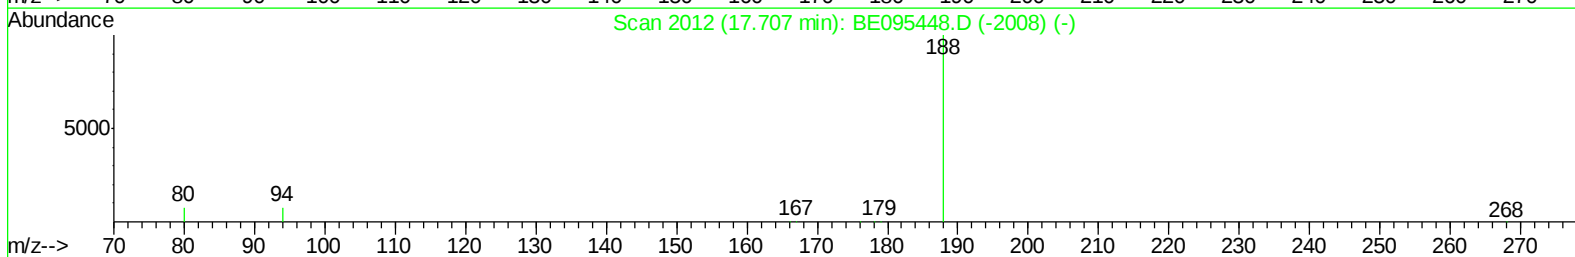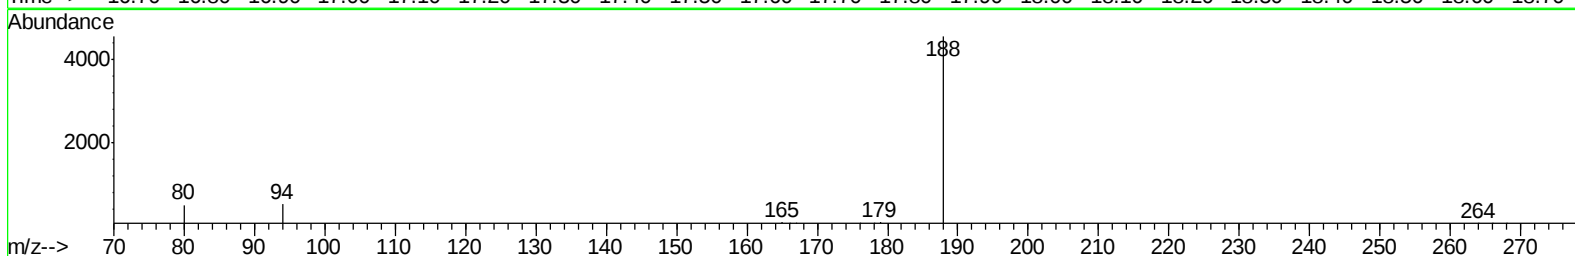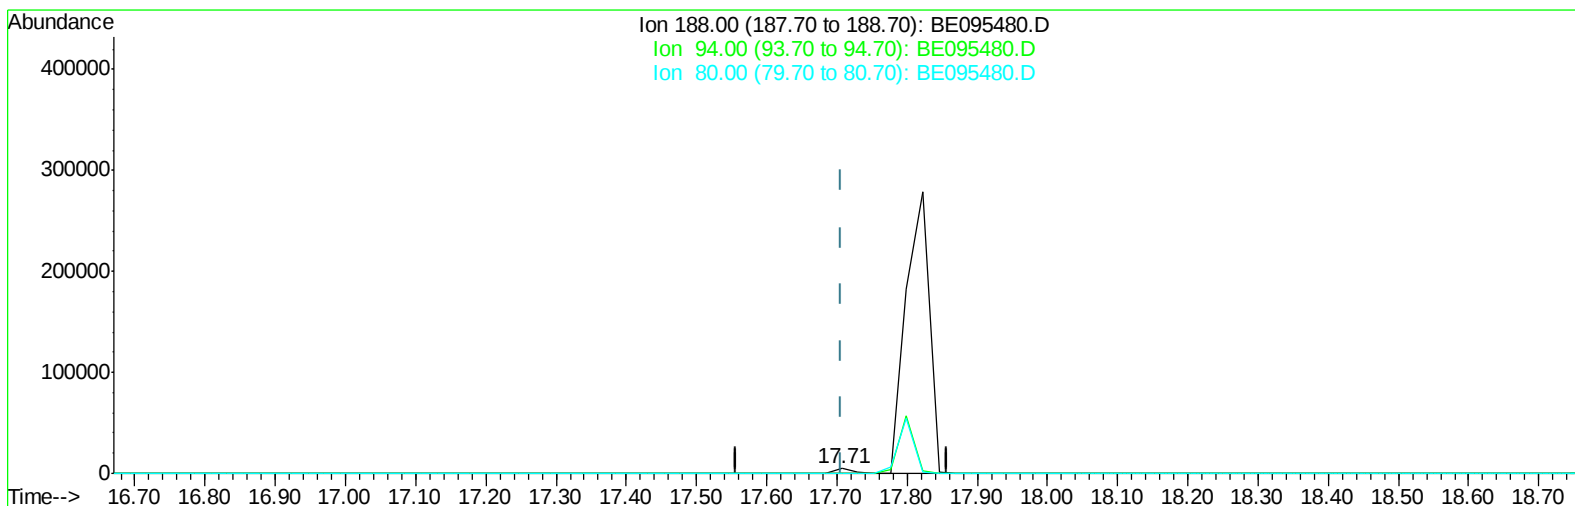

TIC: BE095480.D

(10) Phenanthrene-d10 (I)

17.707min (-0.001) 0.40ng/ul m

response 7836

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	10.95
80.00	11.80	10.77
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA E\DATA\BE020318\
 Data File : BE095480.D
 Acq On : 4 Feb 2018 16:37
 Operator : SJ/JU
 Sample : J1315-11
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 F6C68

Manual Integrations
 APPROVED

Sohil
 2/5/2018 7:01:42 PM

Quant Time: Feb 05 07:54:53 2018
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 05 04:46:10 2018
 Response via : Initial Calibration

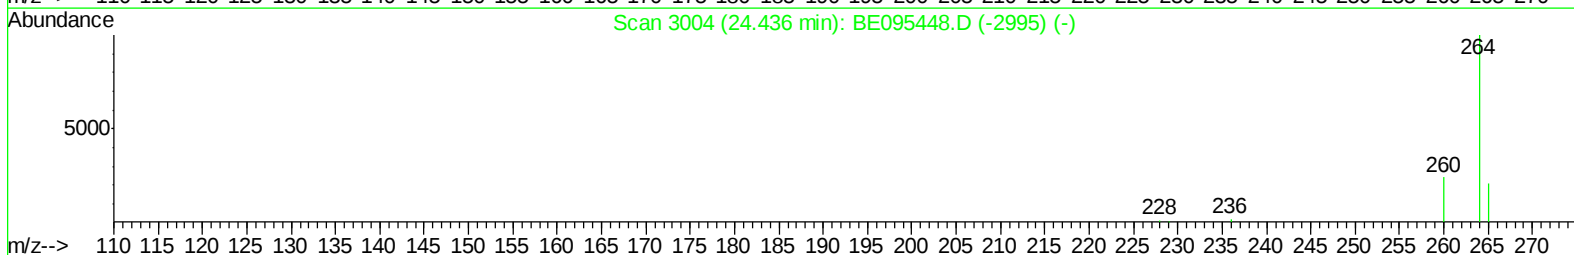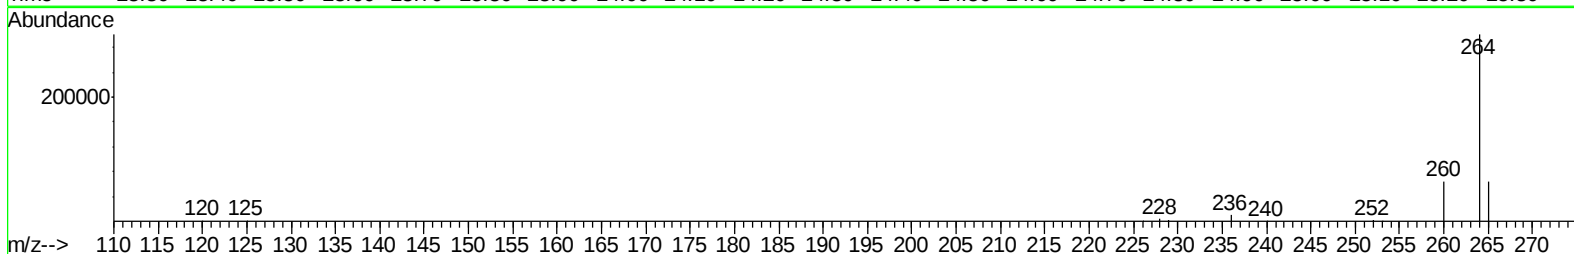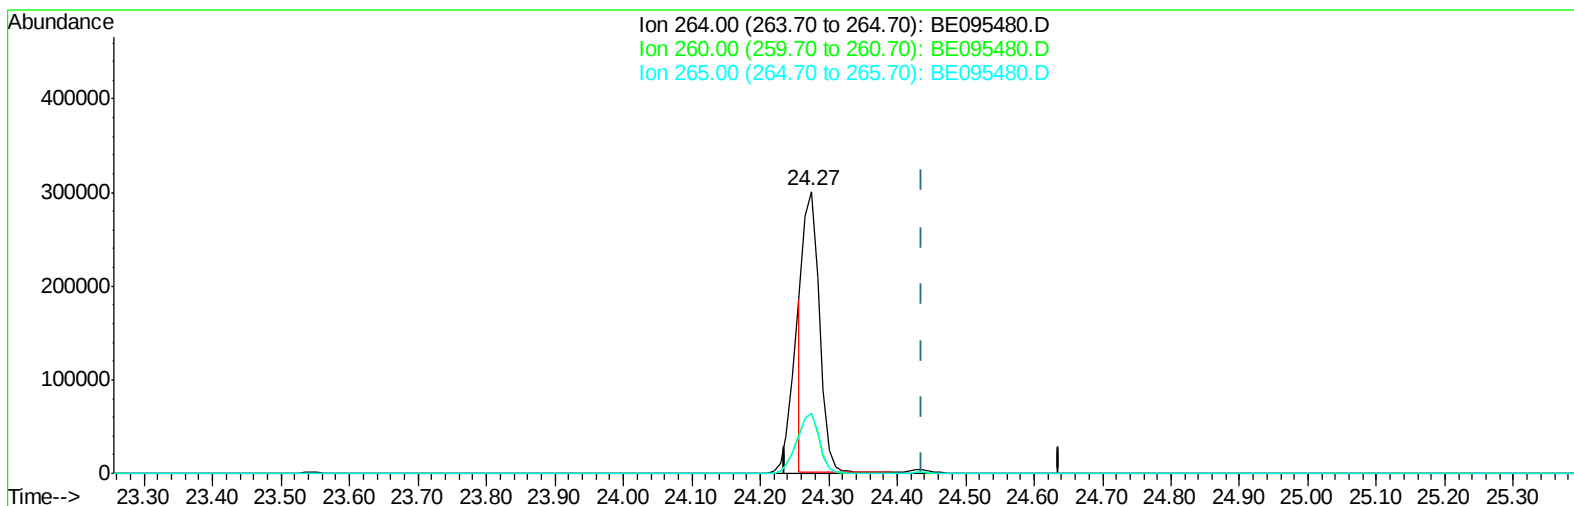

TIC: BE095480.D

(20) Perylene-d12 (I)

24.274min (-0.162) 0.40ng/ul

response 490065

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	21.22#
265.00	103.50	21.41#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA E\DATA\BE020318\
Data File : BE095480.D
Acq On : 4 Feb 2018 16:37
Operator : SJ/JU
Sample : J1315-11
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F6C68

Manual Integrations
APPROVED

Sohil
2/5/2018 7:01:42 PM

Quant Time: Feb 05 07:54:53 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 05 04:46:10 2018
Response via : Initial Calibration

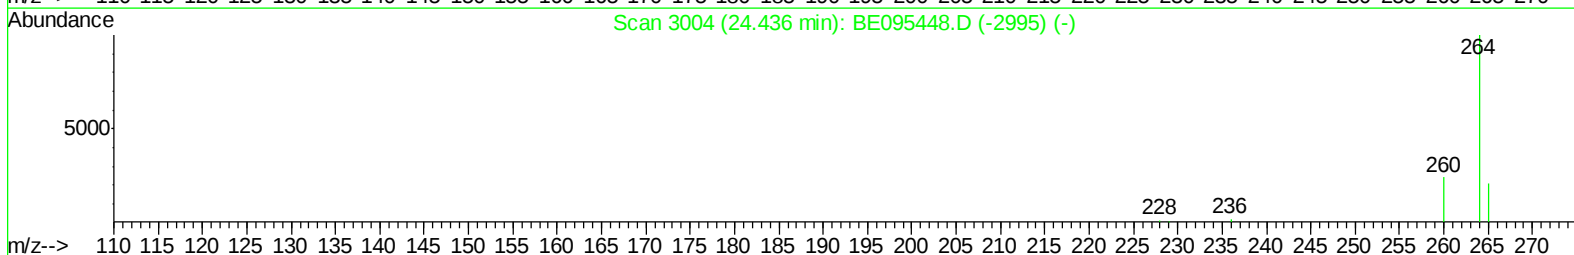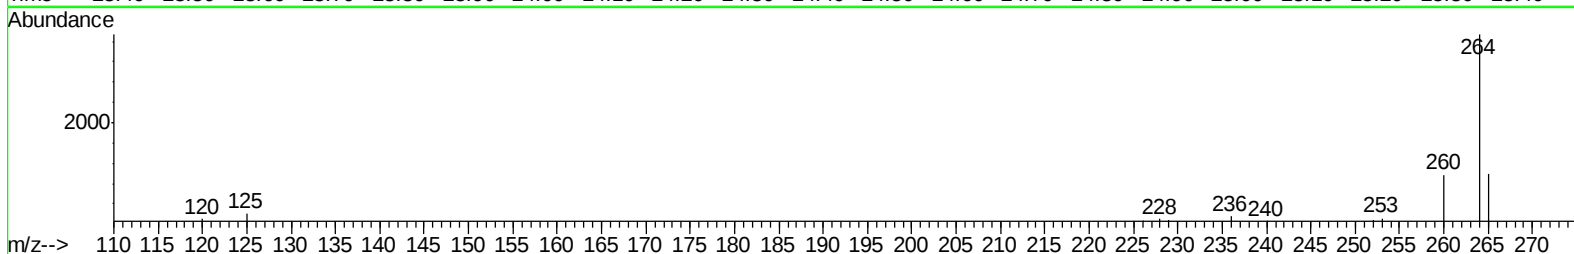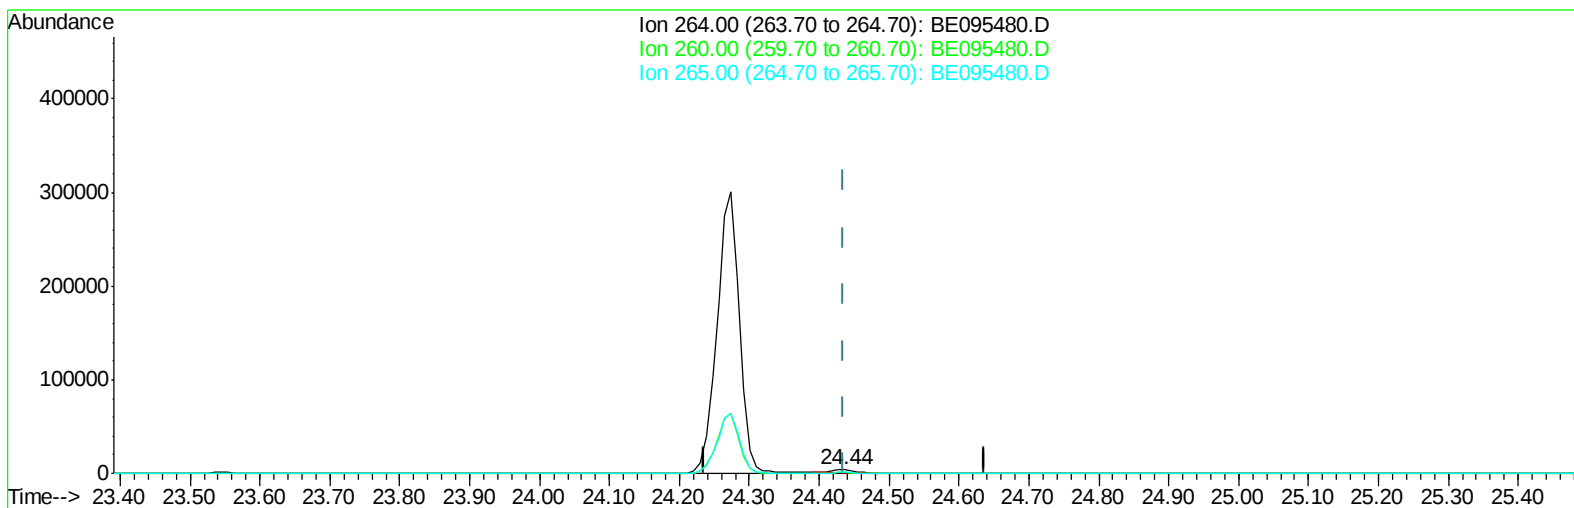

TIC: BE095480.D

(20) Perylene-d12 (I)

24.436min (+0.000) 0.40ng/ul m

response 6738

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	26.08
265.00	103.50	26.69#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020318\
Data File : BE095480.D
Acq On : 4 Feb 2018 16:37
Operator : SJ/JU
Sample : J1315-11
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F6C68

Manual Integrations
APPROVED

Sohil
2/5/2018 7:01:42 PM

Quant Time: Feb 05 07:55:29 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 05 04:46:10 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.44	152	1779	0.40	ng/ul	0.00
2) Naphthalene-d8	11.26	136	5370	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.02	164	3681	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	7836m	0.40	ng/ul	0.00
16) Chrysene-d12	21.80	240	7472	0.40	ng/ul	0.00
20) Perylene-d12	24.44	264	6738m	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.81	152	3940	0.45	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	9847	0.33	ng/ul	0.00

Target Compounds	Ovalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE020318\
Data File : BE095480.D
Acq On : 4 Feb 2018 16:37
Operator : SJ/JU
Sample : J1315-11
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F6C68

Manual Integrations
APPROVED

Sohil
2/5/2018 7:01:42 PM

Quant Time: Feb 05 07:55:29 2018
Quant Method : Z:\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 05 04:46:10 2018
Response via : Initial Calibration

