

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_E\DATA\BE020318\
 Data File : BE095452.D
 Acq On : 3 Feb 2018 23:58
 Operator : SJ/JU
 Sample : J1296-08
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 F6C26

Manual Integrations
 APPROVED

Sohil
 2/5/2018 7:02:32 PM

Quant Time: Feb 05 05:57:54 2018
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 05 04:46:10 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.44	152	1918	0.40	ng/ul	0.00
2) Naphthalene-d8	11.26	136	5805	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.02	164	3761	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	7915	0.40	ng/ul	0.00
16) Chrysene-d12	21.80	240	8068	0.40	ng/ul	0.00
20) Perylene-d12	24.44	264	7493m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	3209	0.34	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	8460	0.28	ng/ul	0.00
Target Compounds						
12) Phenanthrene	17.75	178	535m	0.020	ng/ul	Qvalue
18) Benzo(a)anthracene	21.78	228	544	0.022	ng/ul#	65

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_E\DATA\BE020318\
Data File : BE095452.D
Acq On : 3 Feb 2018 23:58
Operator : SJ/JU
Sample : J1296-08
Misc :
ALS Vial : 21 Sample Multiplier: 1


Instrument :
BNA_E
ClientSampleId :
F6C26

Manual Integrations
APPROVED

Sohil
2/5/2018 7:02:32 PM

Quant Time: Feb 05 05:57:54 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 05 04:46:10 2018
Response via : Initial Calibration

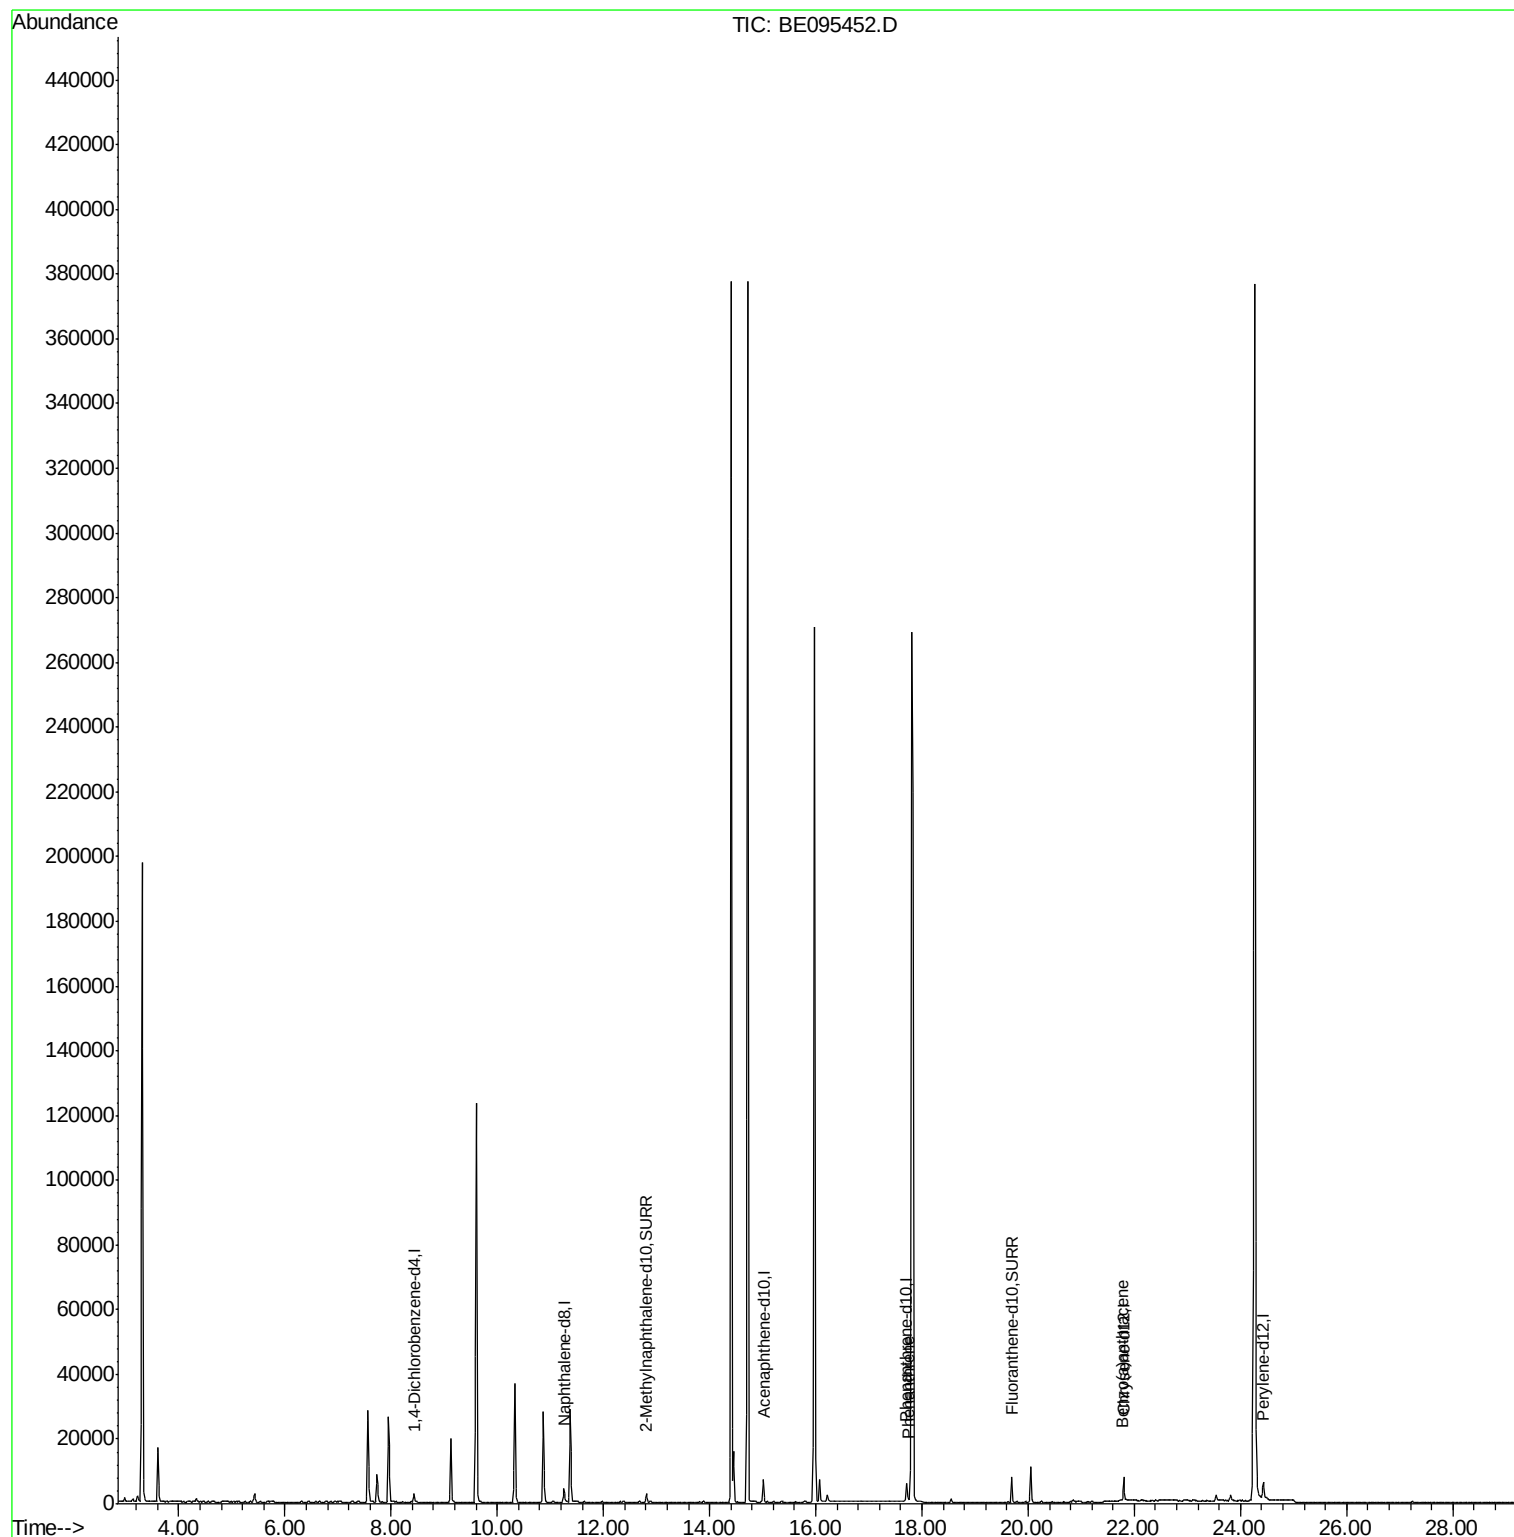

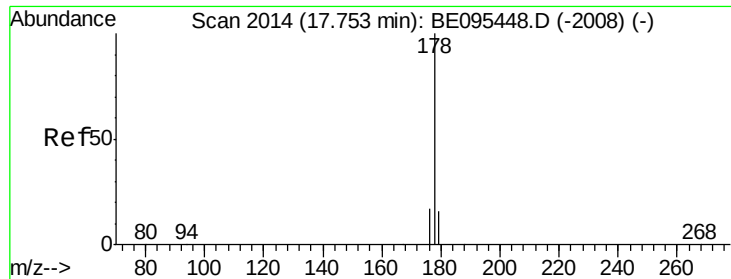

#12

Phenanthrene

Concen: 0.020 ng/ul m

RT: 17.75 min Scan# 2014

Delta R.T. -0.00 min

Lab File: BE095452.D

Acq: 3 Feb 2018 23:58

Instrument :

BNA_E

ClientSampled :





F6C26

Tgt Ion:178 Resp: 535

Ion	Ratio	Lower	Upper
178	100		
179	32.5	18.4	27.6#
176	31.4	13.6	20.4#

Manual Integrations
APPROVED

Sohil
2/5/2018 7:02:32 PM

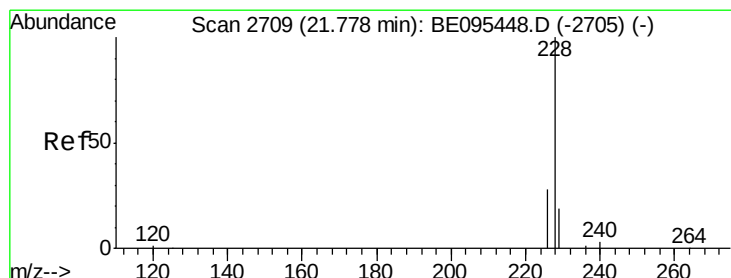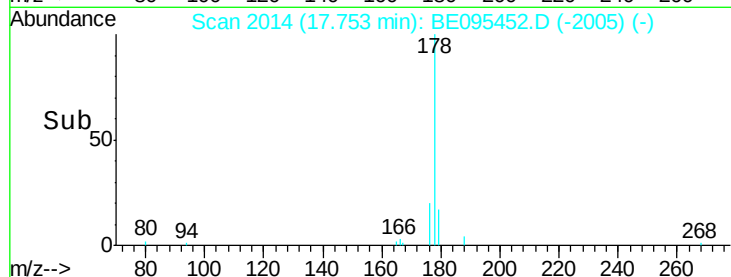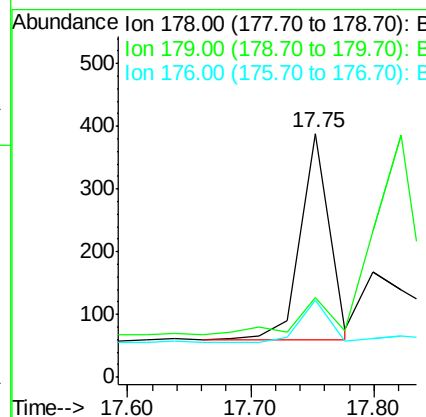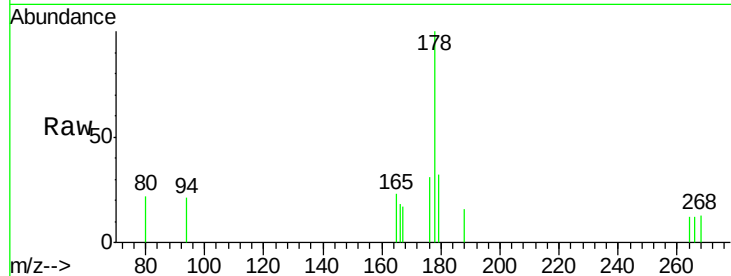

#18

Benzo(a)anthracene

Concen: 0.022 ng/ul

RT: 21.78 min Scan# 2709

Delta R.T. 0.00 min

Lab File: BE095452.D

Acq: 3 Feb 2018 23:58

Tgt Ion:228 Resp: 544

Ion	Ratio	Lower	Upper
228	100		
229	41.3	22.8	34.2#
226	44.6	17.0	25.6#

