

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_E\DATA\BE020318\
 Data File : BE095453.D
 Acq On : 4 Feb 2018 00:33
 Operator : SJ/JU
 Sample : J1296-04
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 F6C22

Manual Integrations
 APPROVED

Sohil
 2/5/2018 7:02:35 PM

Quant Time: Feb 05 06:05:34 2018
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 05 04:46:10 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.43	152	1843	0.40	ng/ul	0.00
2) Naphthalene-d8	11.26	136	5751	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.02	164	3765	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	7932	0.40	ng/ul	0.00
16) Chrysene-d12	21.80	240	7726	0.40	ng/ul	0.00
20) Perylene-d12	24.44	264	6960m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	3635	0.39	ng/ul	0.00
14) Fluoranthene-d10	19.69	212	9143	0.30	ng/ul	0.00
Target Compounds						
3) Naphthalene	11.31	128	3844	0.239	ng/ul#	89
11) Pentachlorophenol	17.36	266	11385	7.411	ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_E\DATA\BE020318\
Data File : BE095453.D
Acq On : 4 Feb 2018 00:33
Operator : SJ/JU
Sample : J1296-04
Misc :
ALS Vial : 22 Sample Multiplier: 1


Instrument :
BNA_E
ClientSampleId :
F6C22

Manual Integrations
APPROVED

Sohil
2/5/2018 7:02:35 PM

Quant Time: Feb 05 06:05:34 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 05 04:46:10 2018
Response via : Initial Calibration

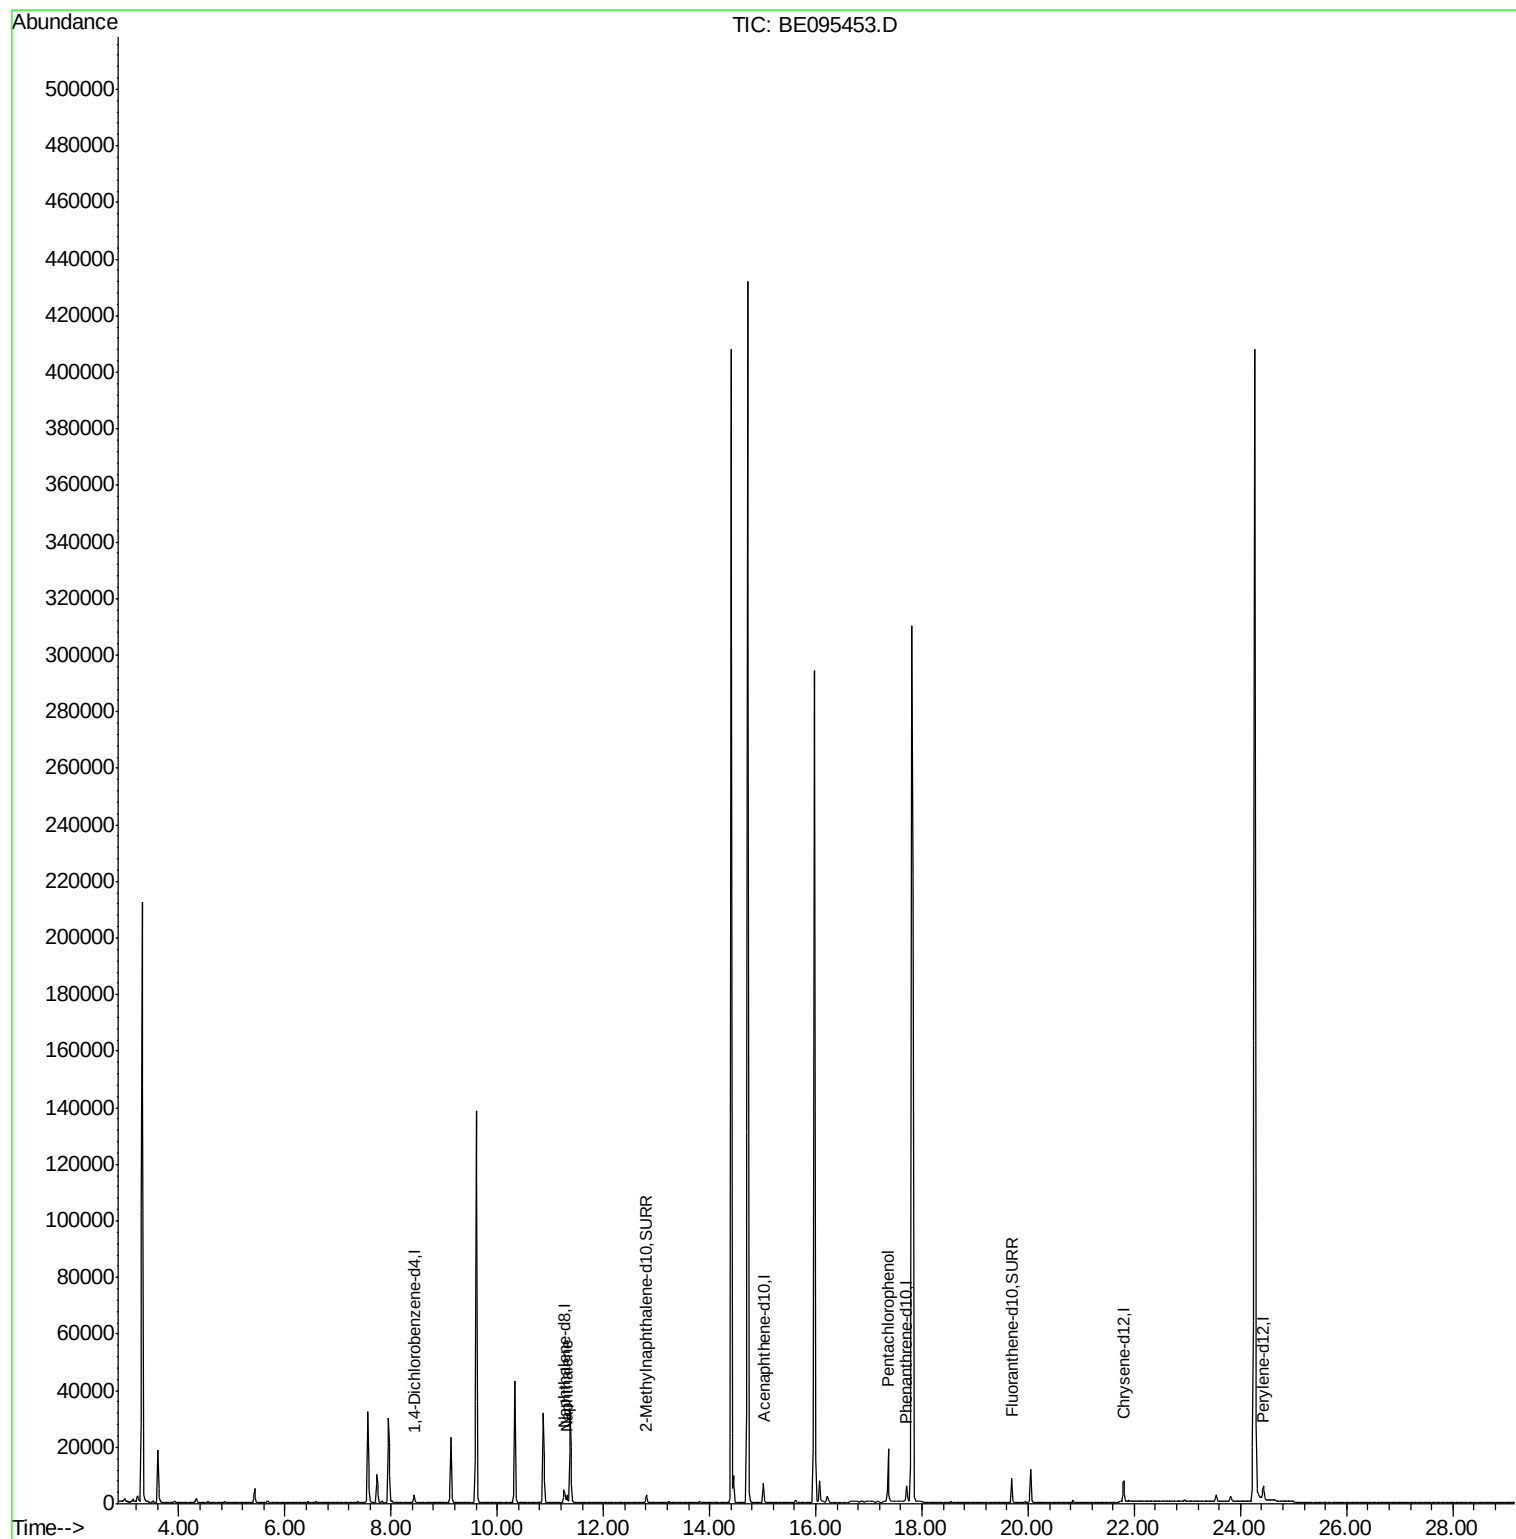

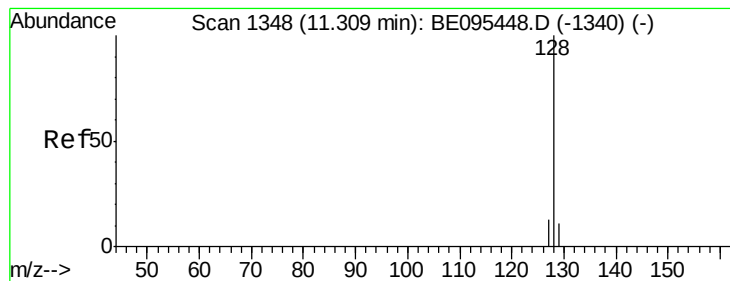

#3

Naphthalene

Concen: 0.239 ng/ul

RT: 11.31 min Scan# 1348

Delta R.T. 0.00 min

Lab File: BE095453.D

Acq: 4 Feb 2018 00:33

Instrument :

BNA_E





ClientSampleId :

F6C22

Tgt Ion:	128	Resp:	3844
Ion Ratio	Lower	Upper	
128	100		
129	12.6	11.3	16.9
127	15.0	4.0	6.0#

Manual Integrations
APPROVED

Sohil
2/5/2018 7:02:35 PM

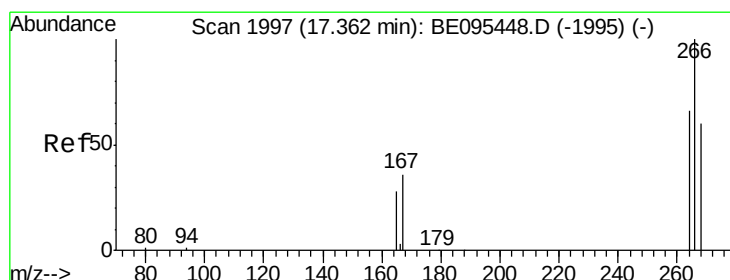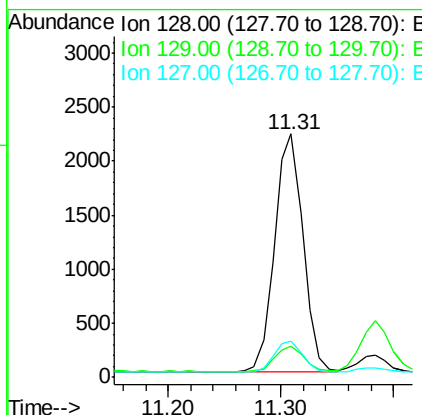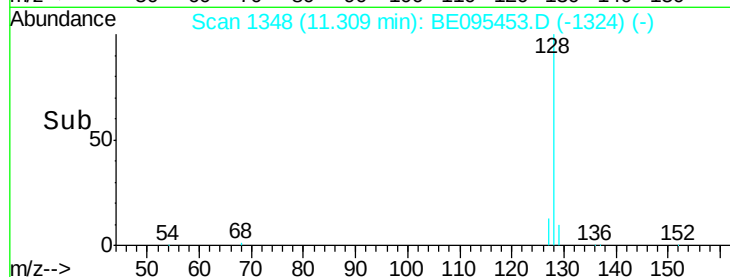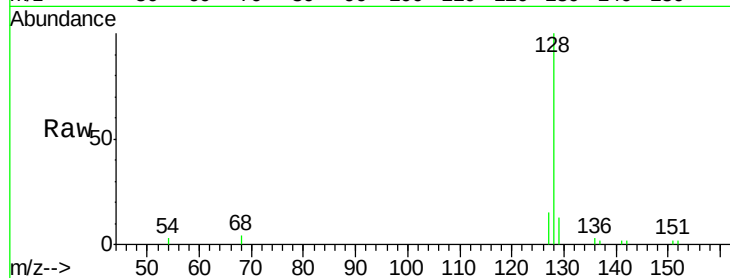

#11

Pentachlorophenol

Concen: 7.411 ng/ul

RT: 17.36 min Scan# 1997

Delta R.T. 0.00 min

Lab File: BE095453.D

Acq: 4 Feb 2018 00:33

Tgt Ion:	266	Resp:	11385
Ion Ratio	Lower	Upper	
266	100		
264	63.1	47.9	71.9
268	62.2	49.8	74.8

