

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_E\DATA\BE020318\
 Data File : BE095457.D
 Acq On : 4 Feb 2018 2:57
 Operator : SJ/JU
 Sample : J1314-08
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 F6C45

Manual Integrations
 APPROVED

Sohil
 2/5/2018 7:02:47 PM

Quant Time: Feb 05 06:19:08 2018
 Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 05 04:46:10 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.43	152	1791	0.40	ng/ul	0.00
2) Naphthalene-d8	11.26	136	5575	0.40	ng/ul	0.00
6) Acenaphthene-d10	15.02	164	3779	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.71	188	7971	0.40	ng/ul	0.00
16) Chrysene-d12	21.80	240	7613	0.40	ng/ul	0.00
20) Perylene-d12	24.44	264	7244m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.81	152	3379	0.37	ng/ul	0.00
14) Fluoranthene-d10	19.70	212	8905	0.29	ng/ul	0.00
Target Compounds						
11) Pentachlorophenol	17.36	266	612	0.396	ng/ul	Qvalue 95

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_E\DATA\BE020318\
Data File : BE095457.D
Acq On : 4 Feb 2018 2:57
Operator : SJ/JU
Sample : J1314-08
Misc :
ALS Vial : 26 Sample Multiplier: 1


Instrument :
BNA_E
ClientSampleId :
F6C45

Manual Integrations
APPROVED

Sohil
2/5/2018 7:02:47 PM

Quant Time: Feb 05 06:19:08 2018
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE012618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 05 04:46:10 2018
Response via : Initial Calibration

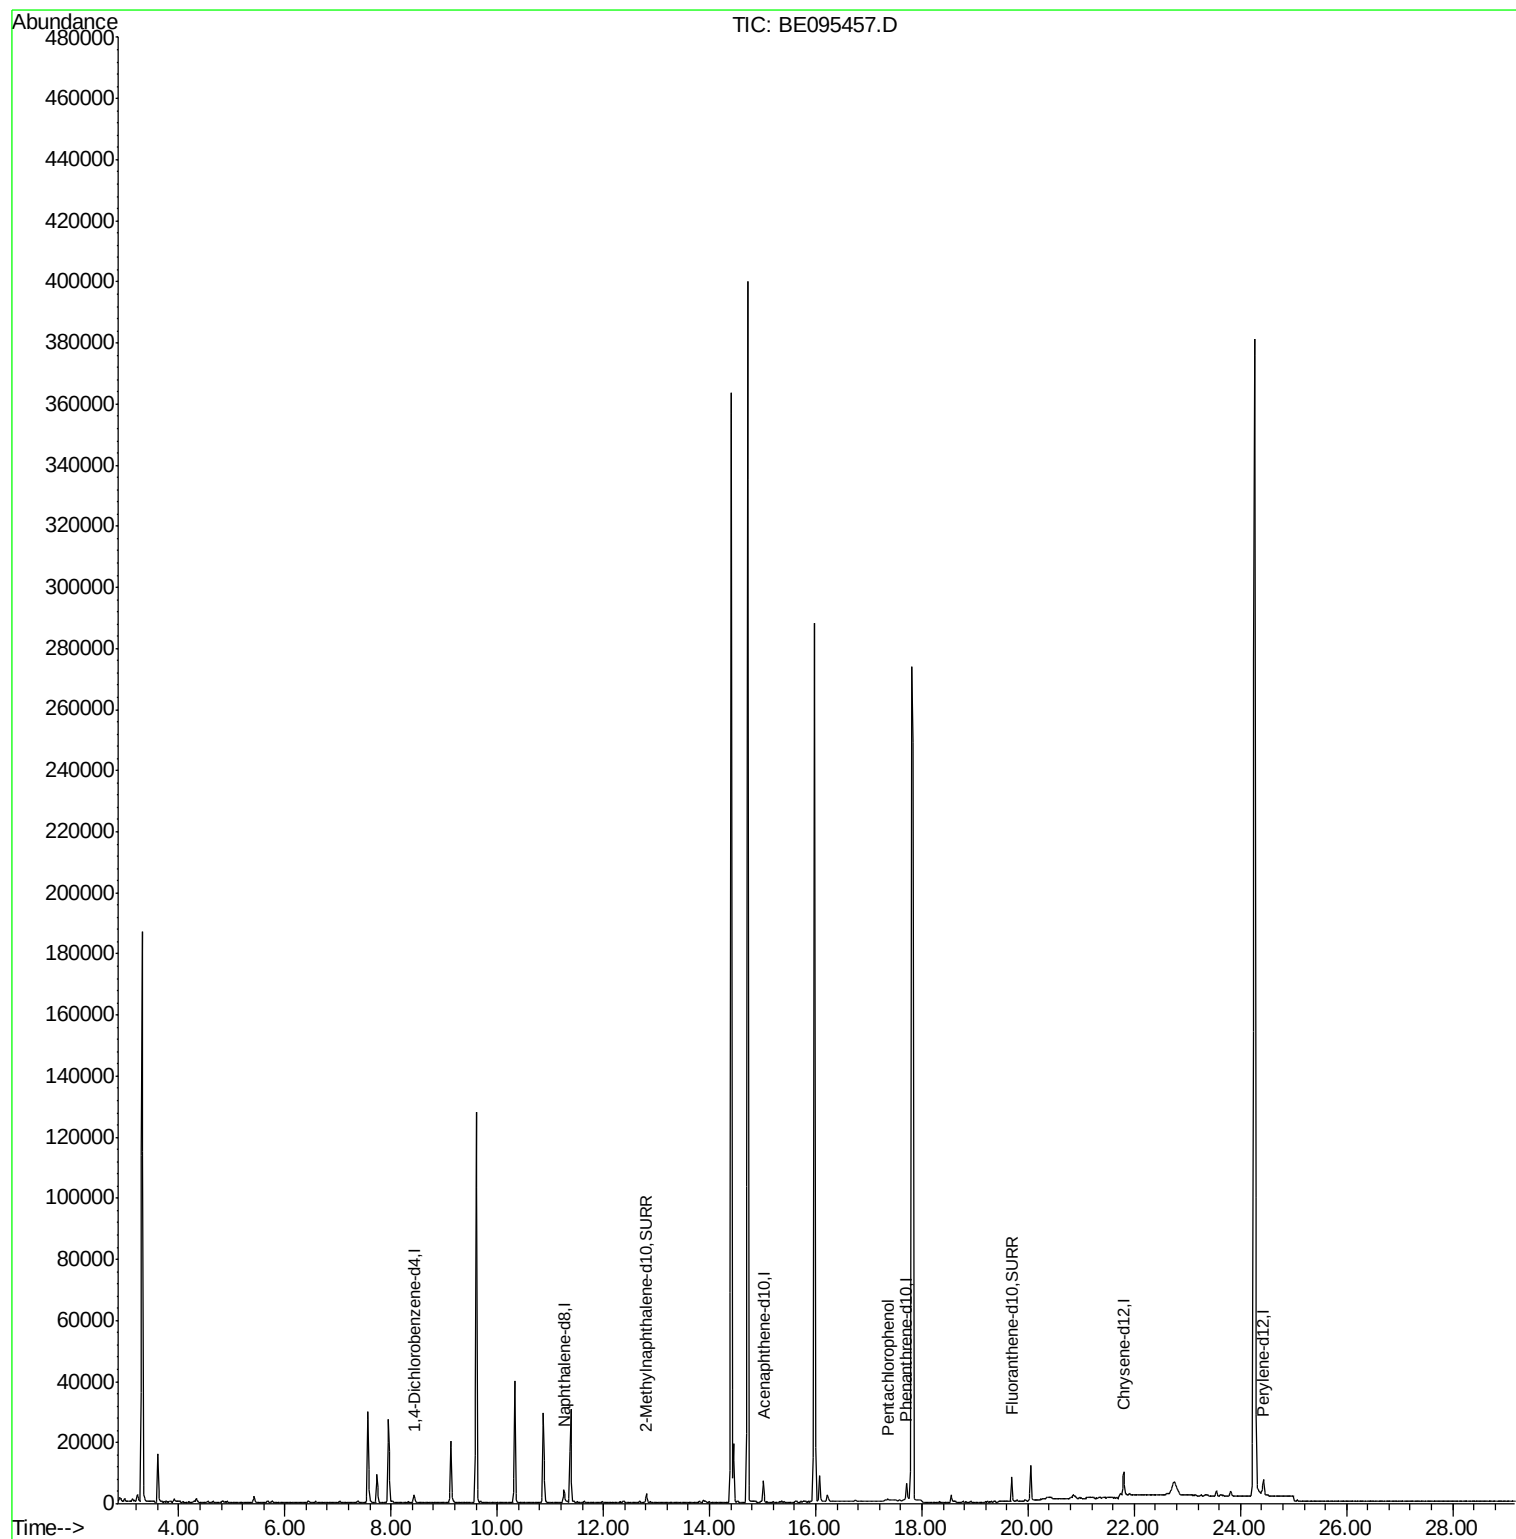

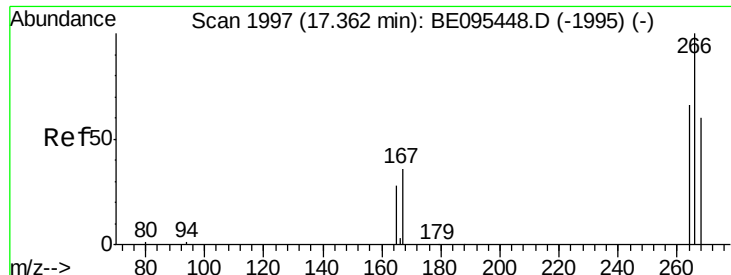


#11
 Pentachlorophenol
 Concen: 0.396 ng/ul
 RT: 17.36 min Scan# 1997
 Delta R.T. 0.00 min
 Lab File: BE095457.D
 Acq: 4 Feb 2018 2:57

Instrument :
 BNA_E
 ClientSampleId :
 F6C45

Tgt Ion:	266	Resp:	612
Ion Ratio	Lower	Upper	
266	100		
264	62.7	47.9	71.9
268	67.2	49.8	74.8

Manual Integrations
 APPROVED

Sohil
 2/5/2018 7:02:47 PM

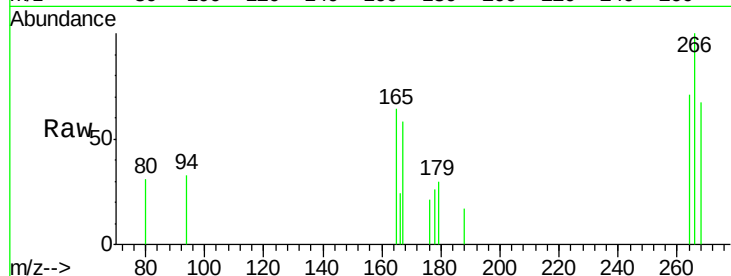

Abundance Ion 266.00 (265.70 to 266.70): E
 Ion 264.00 (263.70 to 264.70): E
 Ion 268.00 (267.70 to 268.70): E

