


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE020415\
Data File : BE089491.D
Acq On : 4 Feb 2015 10:58
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\SIM-BE020315.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Feb 04 00:53:32 2015

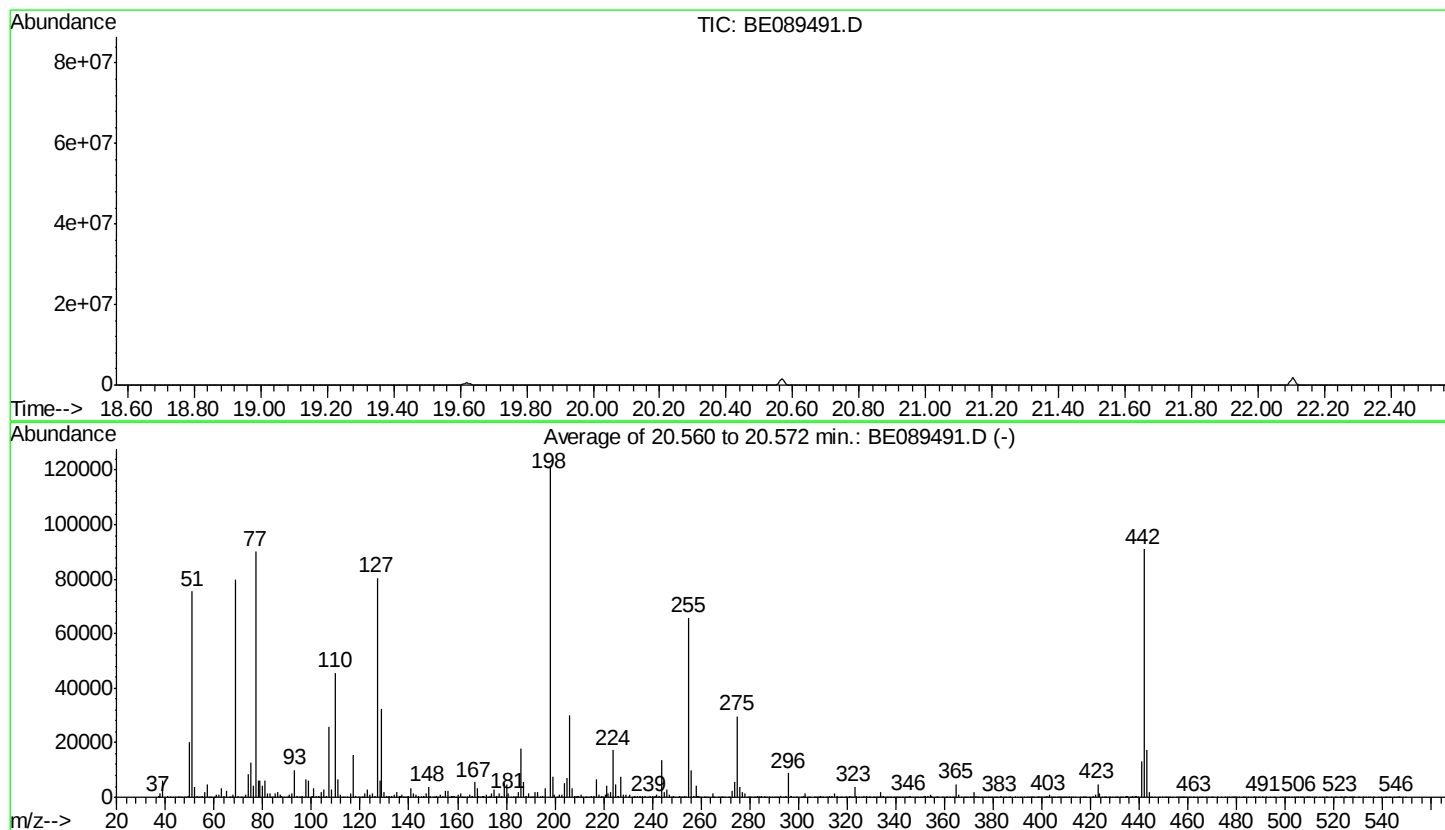

AutoFind: Scans 3263, 3264, 3265; Background Corrected with Scan 3257

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	62.1	75542	PASS
68	69	0.00	2	1.0	806	PASS
69	198	0.00	100	65.7	79944	PASS
70	69	0.00	2	0.4	348	PASS
127	198	10	80	66.2	80464	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	121624	PASS
199	198	5	9	6.3	7674	PASS
275	198	10	60	24.3	29584	PASS
365	198	1	100	3.9	4757	PASS
441	442	0.01	24	14.6	13308	PASS
442	198	50	100	74.8	90922	PASS
443	442	15	24	19.3	17514	PASS